

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120723\
 Data File : PP062285.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2023 23:34
 Operator : YP\AJ
 Sample : 05660-01 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 1705

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/08/2023
 Supervised By :Ankita Jodhani 12/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 00:43:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 28 04:28:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.720	1835700	2088492	1.394	1.161
2) SA Decachlor...	10.238	8.840	1545614	1617085	1.498m	0.783 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120723\
Data File : PP062285.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2023 23:34
Operator : YP\AJ
Sample : 05660-01 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
1705


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/08/2023
Supervised By :Ankita Jodhani 12/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 00:43:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 28 04:28:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

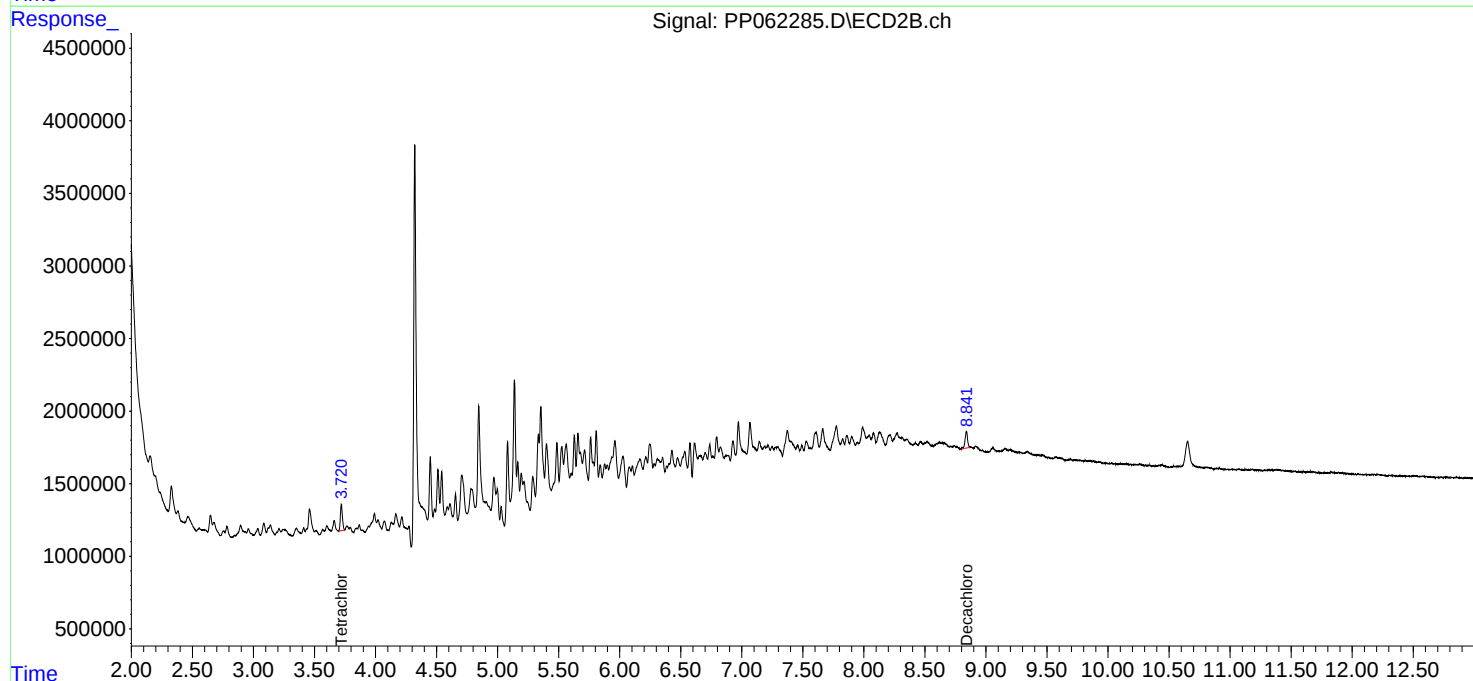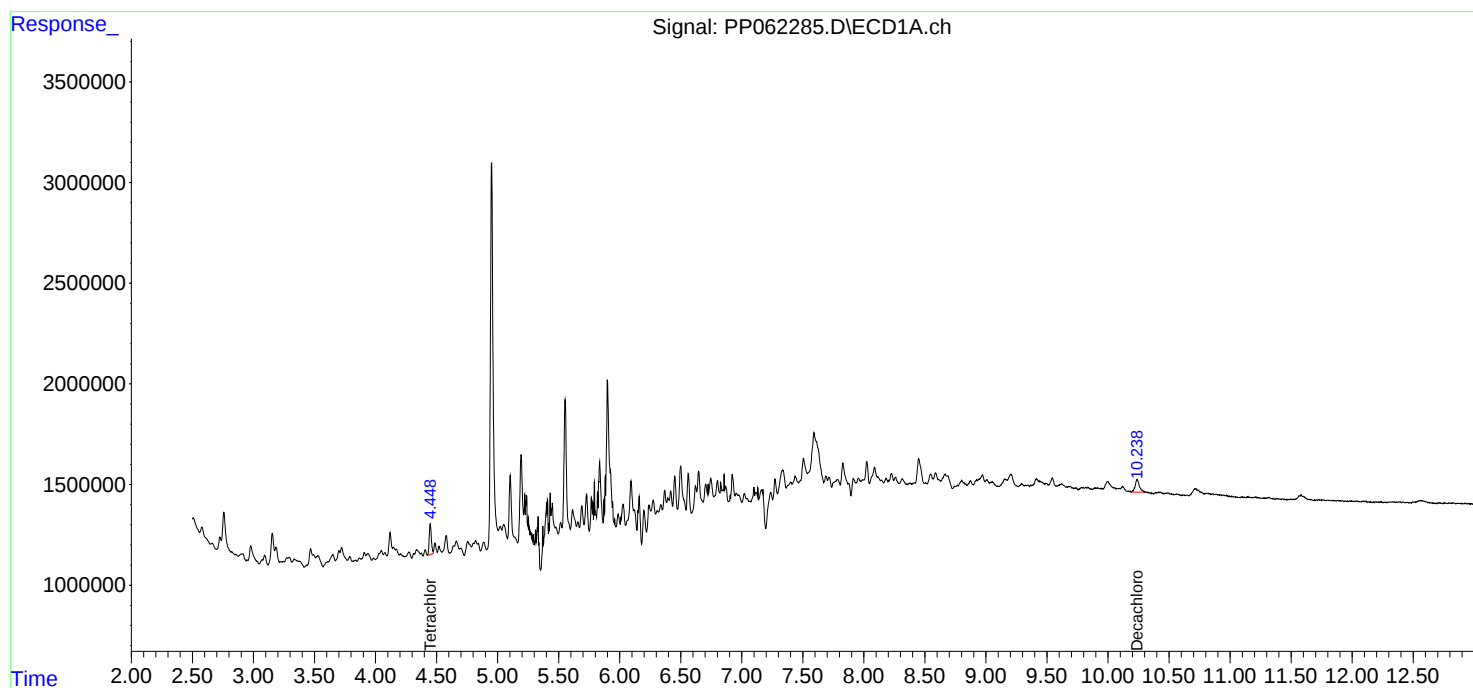

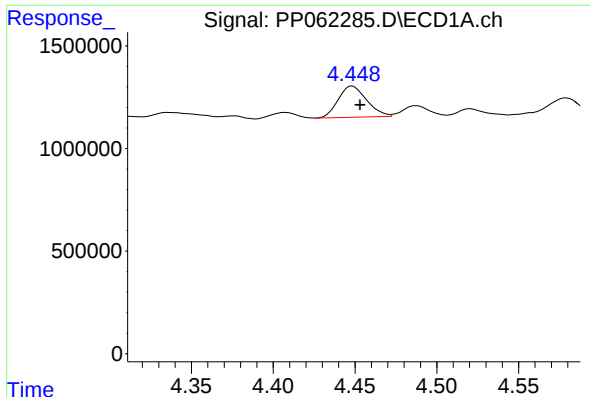


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: -0.005 min
Response: 1835700
Conc: 1.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
1705


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/08/2023
Supervised By :Ankita Jodhani 12/08/2023

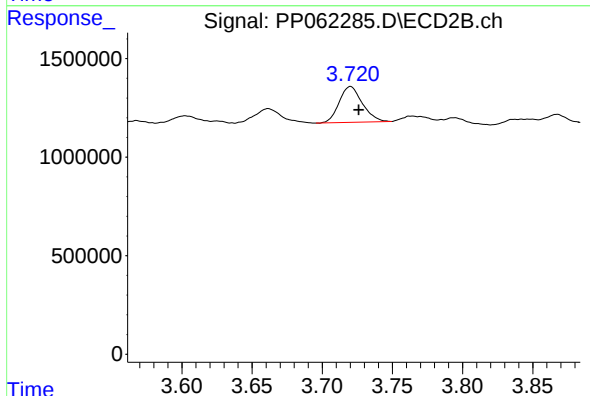


#1 Tetrachloro-m-xylene

R.T.: 3.720 min
Delta R.T.: -0.006 min
Response: 2088492
Conc: 1.16 ng/ml

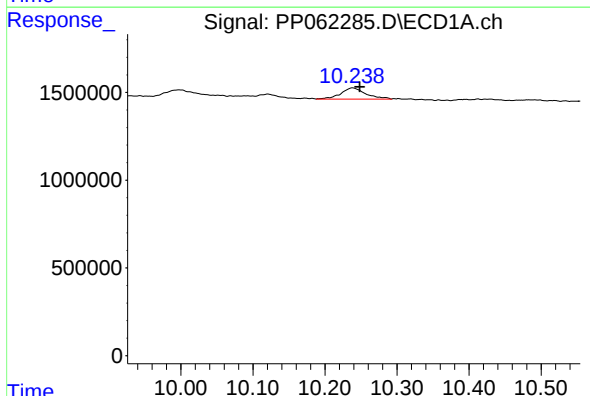

#2 Decachlorobiphenyl

R.T.: 10.238 min
Delta R.T.: -0.011 min
Response: 1545614
Conc: 1.50 ng/ml m

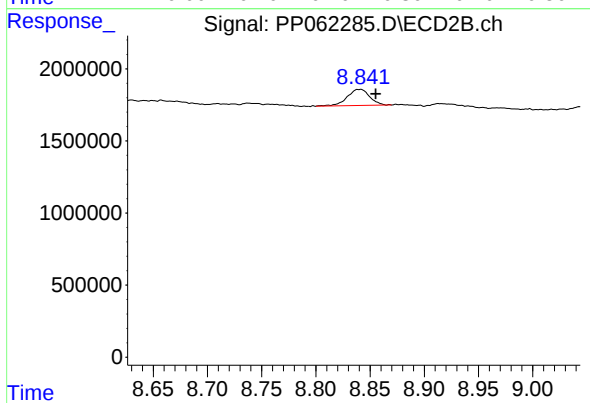

#2 Decachlorobiphenyl

R.T.: 8.840 min
Delta R.T.: -0.015 min
Response: 1617085
Conc: 0.78 ng/ml