

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120723\
 Data File : PP062289.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2023 00:39
 Operator : YP\AJ
 Sample : 05650-04
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 50197

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/08/2023
 Supervised By :Ankita Jodhani 12/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 01:54:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 28 04:28:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.447	3.719	1279898	8558112	0.972	4.756 #
2) SA Decachlor...	10.242	8.837	1784934	1198364	1.730	0.581m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120723\
Data File : PP062289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2023 00:39
Operator : YP\AJ
Sample : 05650-04
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
50197


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/08/2023
Supervised By :Ankita Jodhani 12/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 01:54:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 28 04:28:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

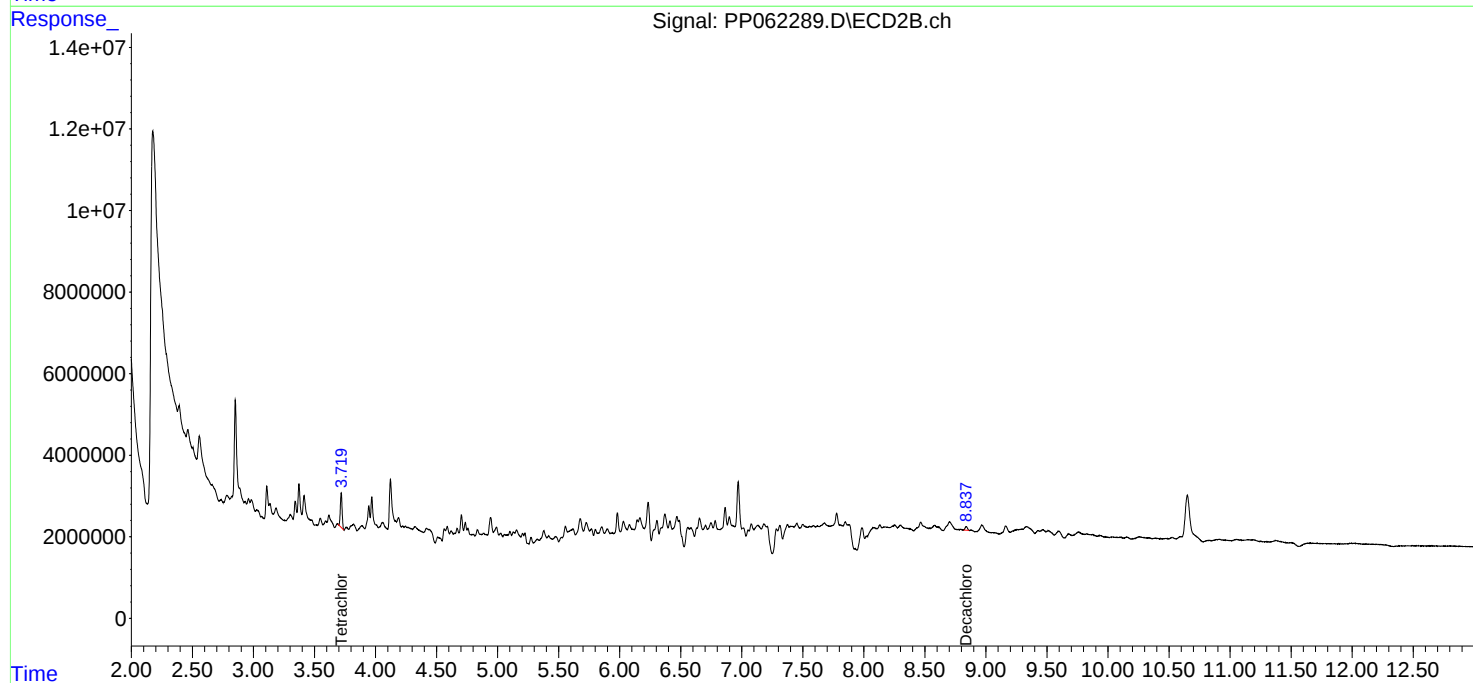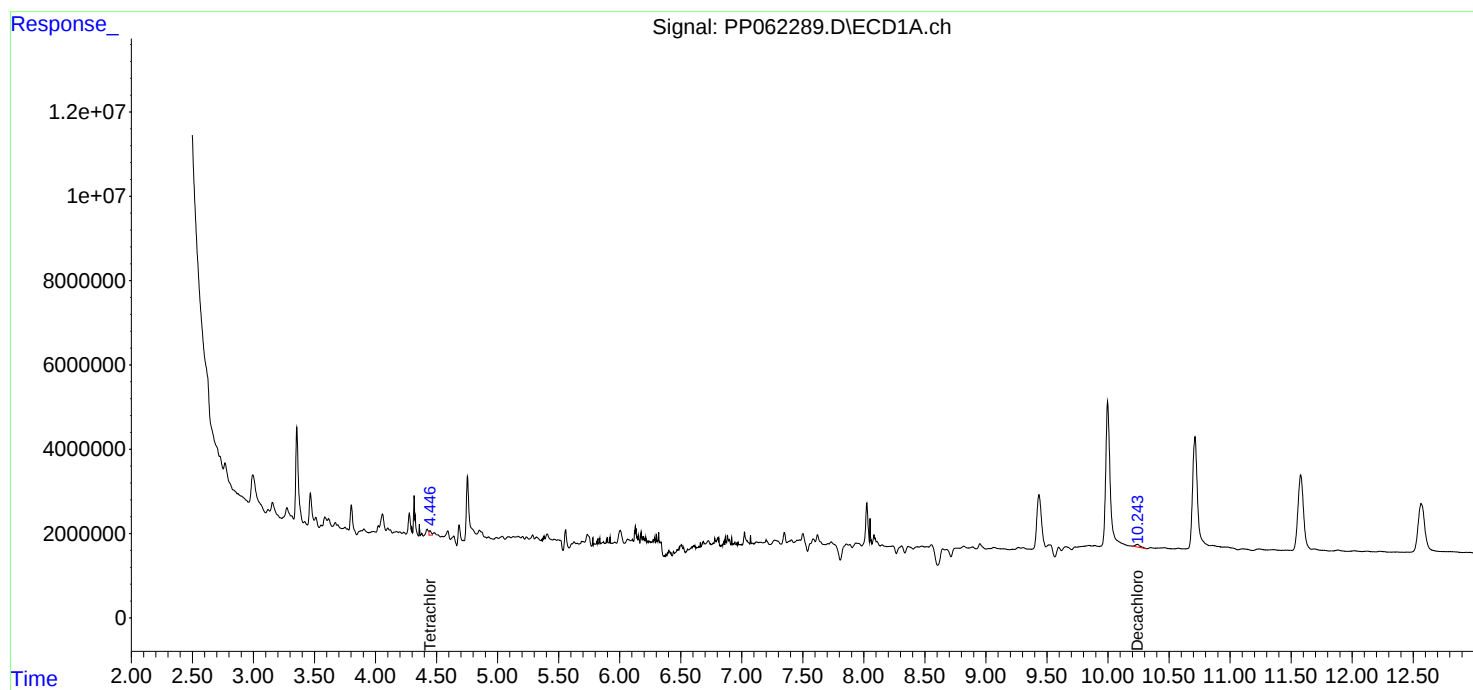

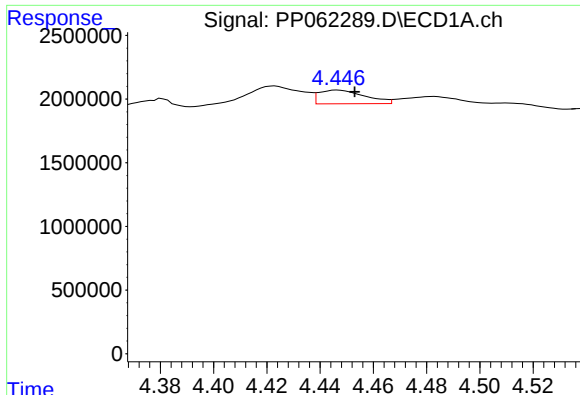


#1 Tetrachloro-m-xylene

R.T.: 4.447 min
Delta R.T.: -0.006 min
Response: 1279898
Conc: 0.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
50197


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/08/2023
Supervised By :Ankita Jodhani 12/08/2023

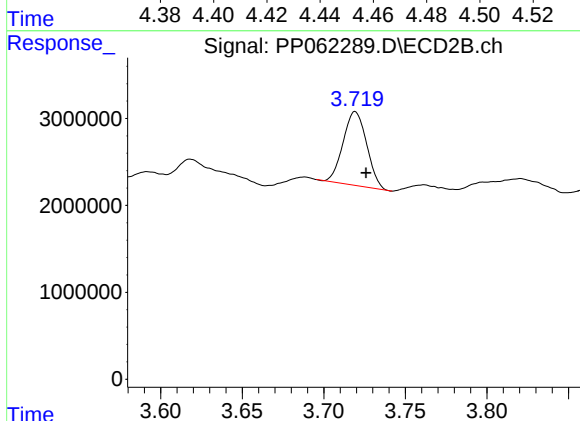


#1 Tetrachloro-m-xylene

R.T.: 3.719 min
Delta R.T.: -0.007 min
Response: 8558112
Conc: 4.76 ng/ml

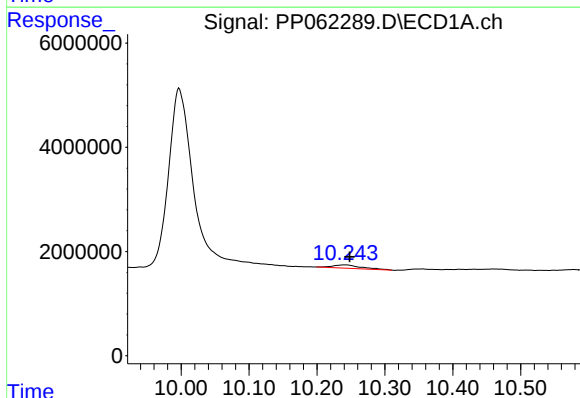

#2 Decachlorobiphenyl

R.T.: 10.242 min
Delta R.T.: -0.007 min
Response: 1784934
Conc: 1.73 ng/ml

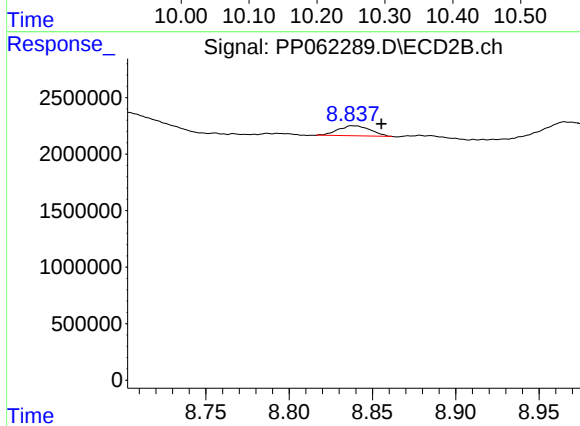

#2 Decachlorobiphenyl

R.T.: 8.837 min
Delta R.T.: -0.019 min
Response: 1198364
Conc: 0.58 ng/ml m