

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120820\
 Data File : PP031908.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Dec 2020 17:49
 Operator : DD\AJ
 Sample : L4965-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CRT002

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 01:03:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.785	4.058	1161209	1026036	23.980	21.412
2)	SA Decachlor...	10.659	9.360	681478	724752	20.065	19.573
Target Compounds							
9)	L2 AR-1221-2	0.000	4.404	0	21508	N.D.	55.757 #
28)	L6 AR-1254-3	0.000	6.764	0	8282	N.D.	2.679 #
29)	L6 AR-1254-4	0.000	7.002	0	8622	N.D.	5.075 #
30)	L6 AR-1254-5	8.350f	7.430	216028	234044	115.559	86.696
31)	L7 AR-1260-1	0.000	6.899	0	26648	N.D.	13.485 #
32)	L7 AR-1260-2	8.031	7.096	81633	30081	39.729	12.352 #
33)	L7 AR-1260-3	0.000	7.251	0	19394	N.D.	8.493 #
34)	L7 AR-1260-4	0.000	7.733	0	18205	N.D.	9.581 #
35)	L7 AR-1260-5	0.000	7.980	0	56375	N.D.	12.423 #
36)	L8 AR-1262-1	0.000	7.469	0	20947	N.D.	7.537 #
37)	L8 AR-1262-2	0.000	7.980	0	56375	N.D.	11.606 #
38)	L8 AR-1262-3	0.000	8.267	0	18434	N.D.	9.372 #
39)	L8 AR-1262-4	0.000	8.330	0	39673	N.D.	10.944 #
40)	L8 AR-1262-5	0.000	8.827	0	38171	N.D.	23.516 #
41)	L9 AR-1268-1	0.000	8.267	0	18434	N.D.	3.332 #
42)	L9 AR-1268-2	0.000	8.330	0	39673	N.D.	7.338 #
44)	L9 AR-1268-4	0.000	8.827	0	38171	N.D.	20.942 #
45)	L9 AR-1268-5	0.000	9.112	0	19205	N.D.	1.387 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120820\
Data File : PP031908.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Dec 2020 17:49
Operator : DD\AJ
Sample : L4965-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
CRT002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 01:03:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

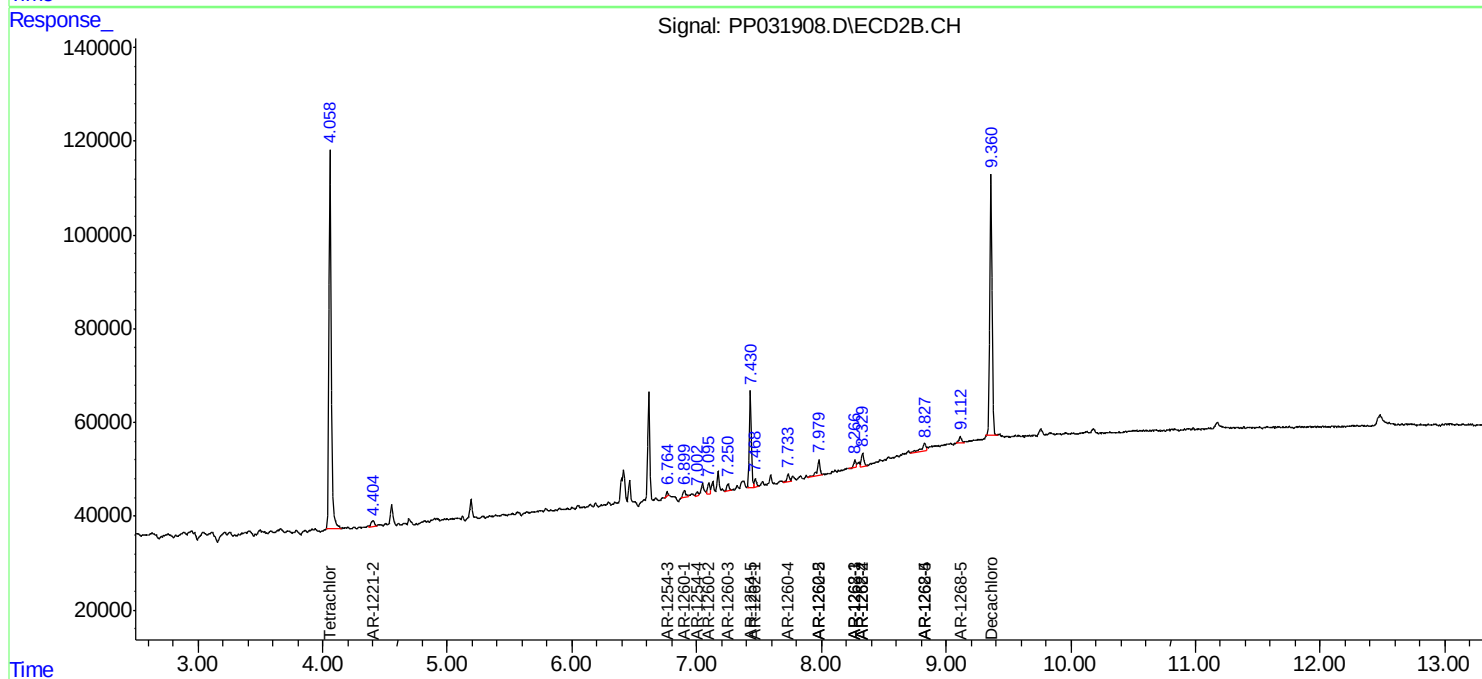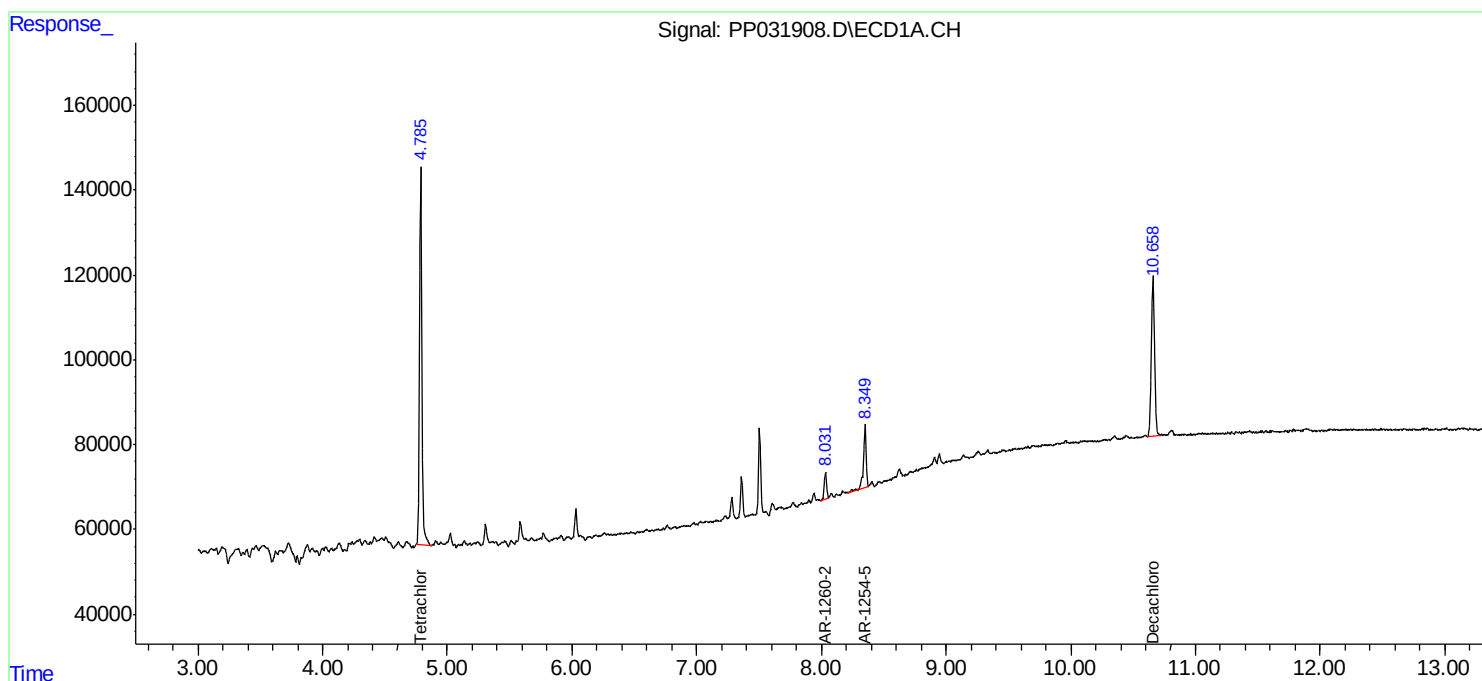


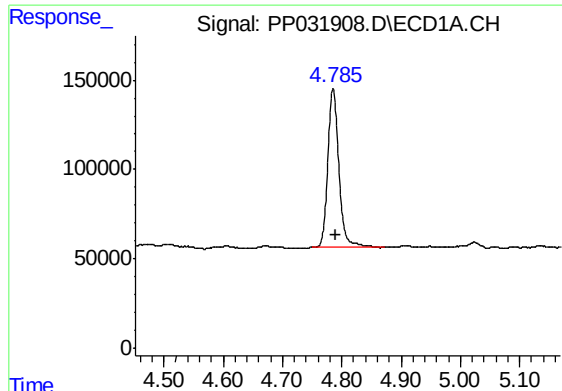

#1 Tetrachloro-m-xylene


R.T.: 4.785 min
Delta R.T.: -0.005 min
Response: 1161209
Conc: 23.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
CRT002

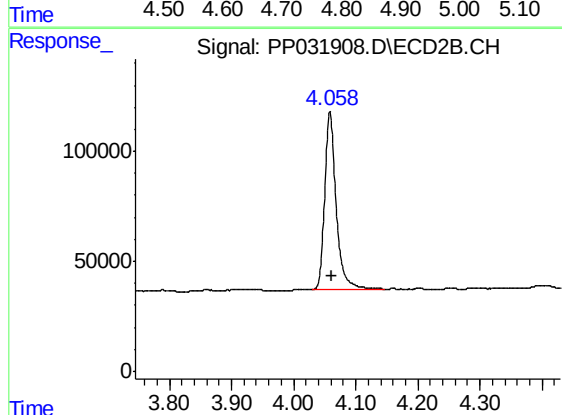


#1 Tetrachloro-m-xylene

R.T.: 4.058 min
Delta R.T.: -0.003 min
Response: 1026036
Conc: 21.41 ng/ml

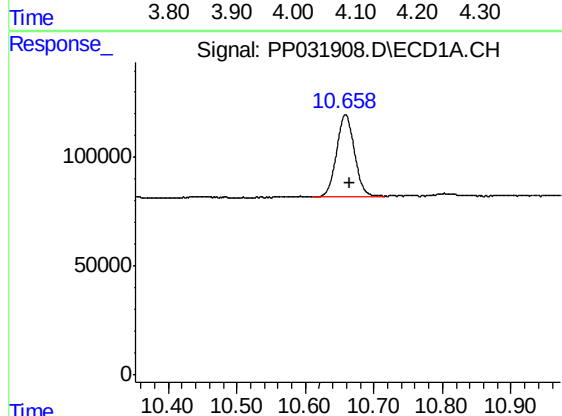


#2 Decachlorobiphenyl

R.T.: 10.659 min
Delta R.T.: -0.006 min
Response: 681478
Conc: 20.06 ng/ml

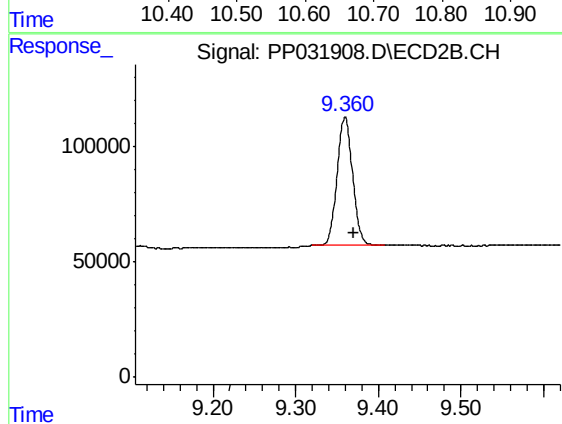

#2 Decachlorobiphenyl


R.T.: 9.360 min
Delta R.T.: -0.011 min
Response: 724752
Conc: 19.57 ng/ml

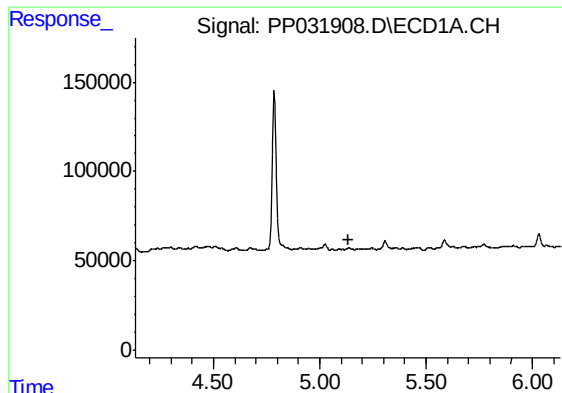

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 5.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT002

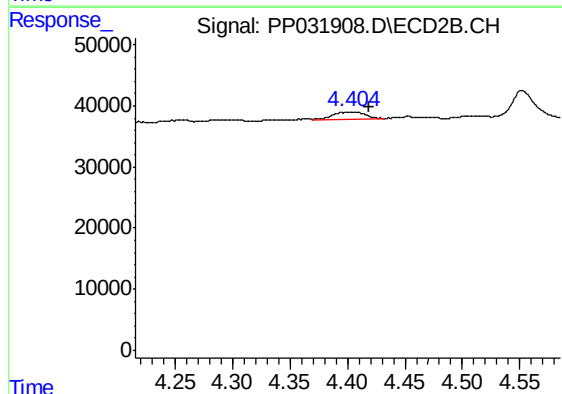


#9 AR-1221-2

R.T.: 4.404 min
Delta R.T.: -0.014 min
Response: 21508
Conc: 55.76 ng/ml

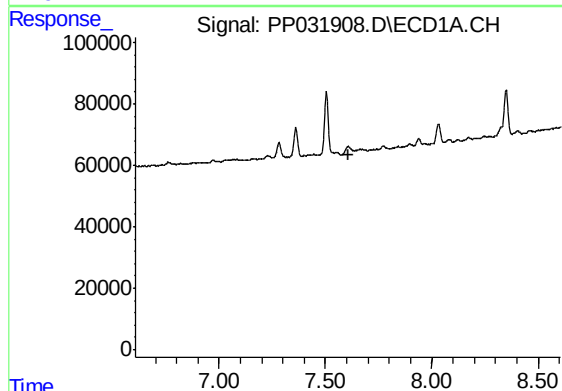


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 7.606 min
Response: 0
Conc: N.D.

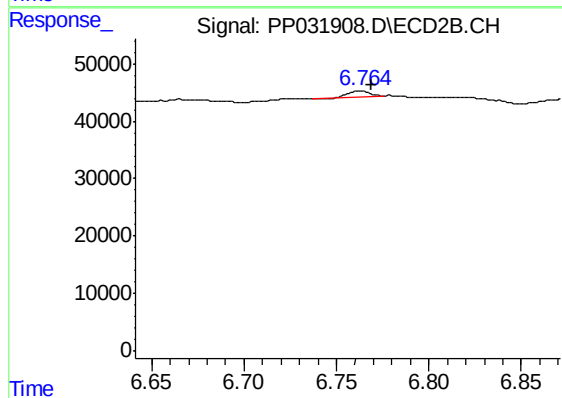

#28 AR-1254-3


R.T.: 6.764 min
Delta R.T.: -0.004 min
Response: 8282
Conc: 2.68 ng/ml

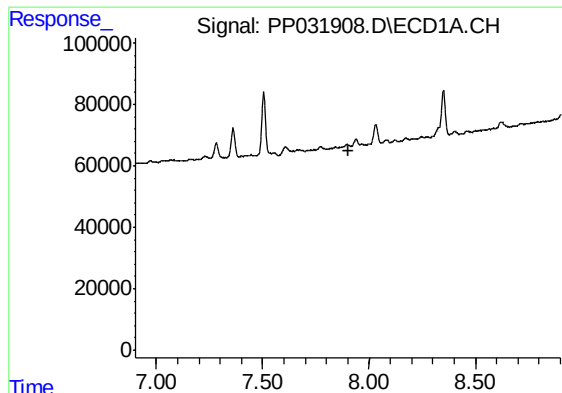

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.901 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT002

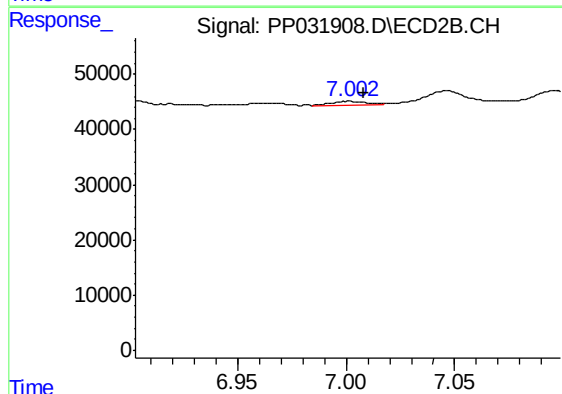


#29 AR-1254-4

R.T.: 7.002 min
Delta R.T.: -0.006 min
Response: 8622
Conc: 5.07 ng/ml

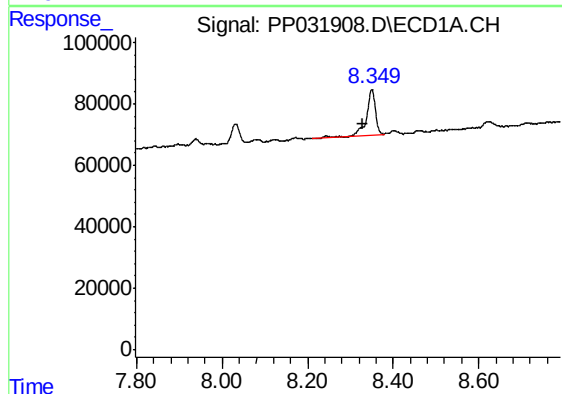


#30 AR-1254-5

R.T.: 8.350 min
Delta R.T.: 0.022 min
Response: 216028
Conc: 115.56 ng/ml

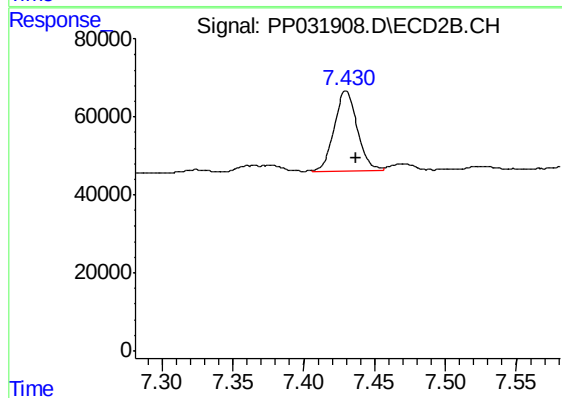

#30 AR-1254-5


R.T.: 7.430 min
Delta R.T.: -0.007 min
Response: 234044
Conc: 86.70 ng/ml

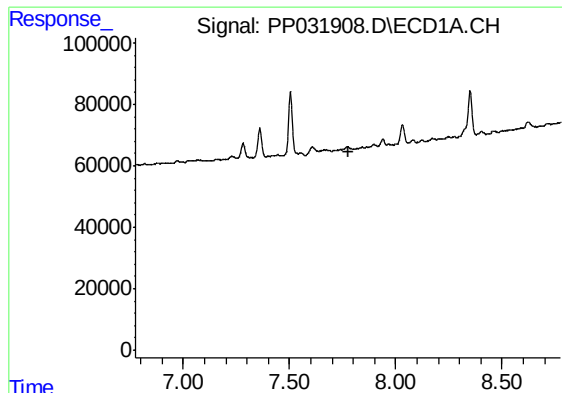

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.775 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT002

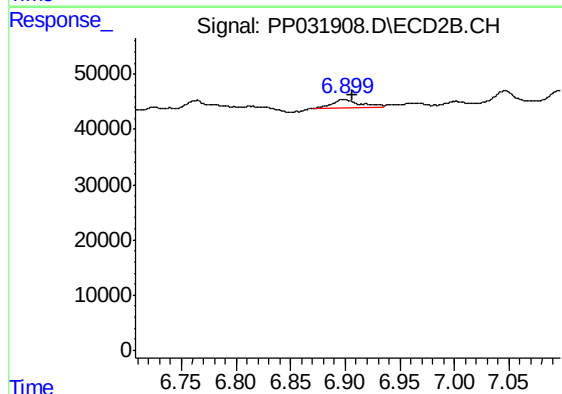


#31 AR-1260-1

R.T.: 6.899 min
Delta R.T.: -0.007 min
Response: 26648
Conc: 13.49 ng/ml

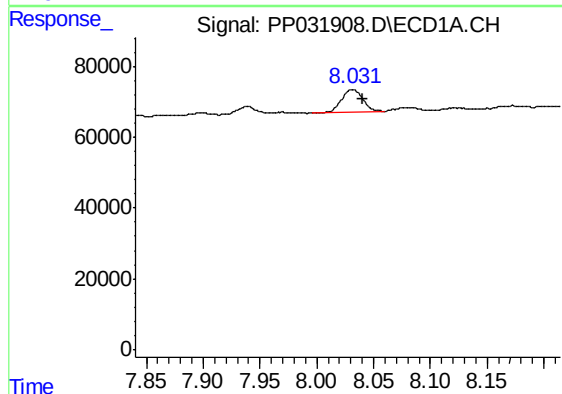


#32 AR-1260-2

R.T.: 8.031 min
Delta R.T.: -0.009 min
Response: 81633
Conc: 39.73 ng/ml

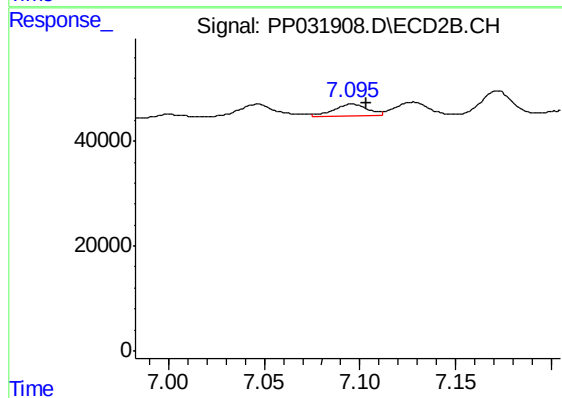

#32 AR-1260-2


R.T.: 7.096 min
Delta R.T.: -0.008 min
Response: 30081
Conc: 12.35 ng/ml

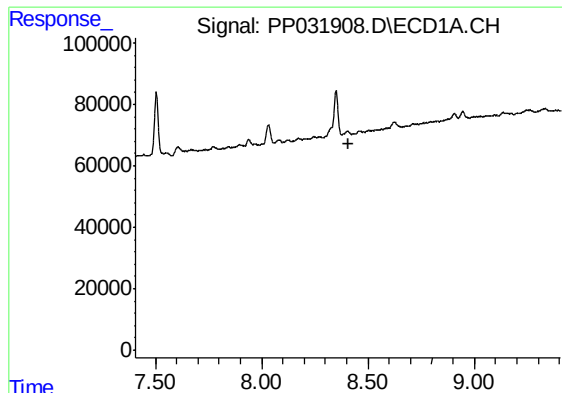

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 8.406 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT002

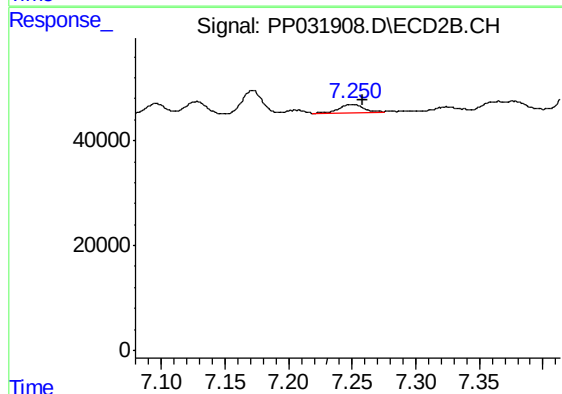


#33 AR-1260-3

R.T.: 7.251 min
Delta R.T.: -0.007 min
Response: 19394
Conc: 8.49 ng/ml

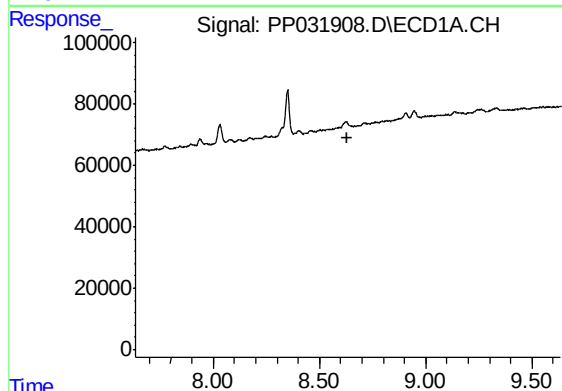


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 8.634 min
Response: 0
Conc: N.D.

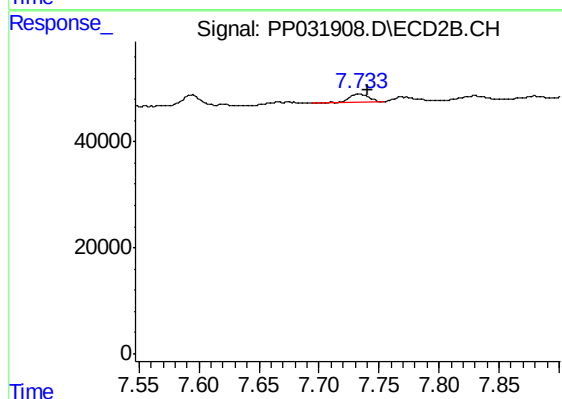

#34 AR-1260-4


R.T.: 7.733 min
Delta R.T.: -0.008 min
Response: 18205
Conc: 9.58 ng/ml

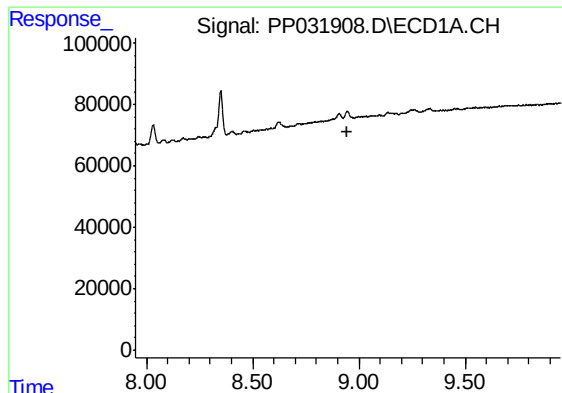

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT002

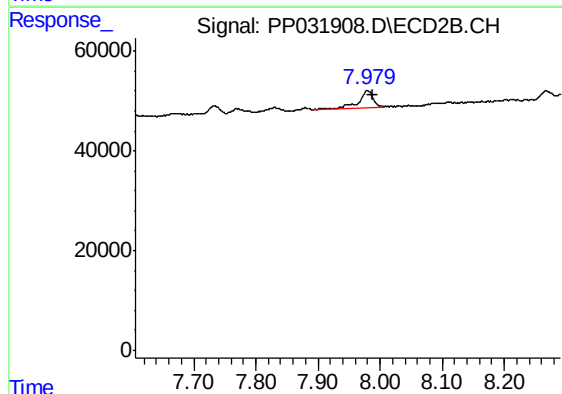


#35 AR-1260-5

R.T.: 7.980 min
Delta R.T.: -0.008 min
Response: 56375
Conc: 12.42 ng/ml

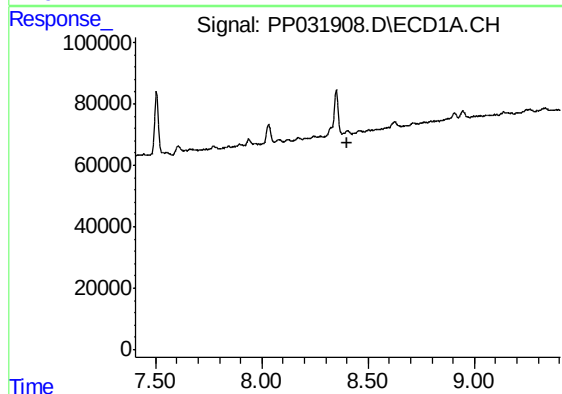


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.405 min
Response: 0
Conc: N.D.

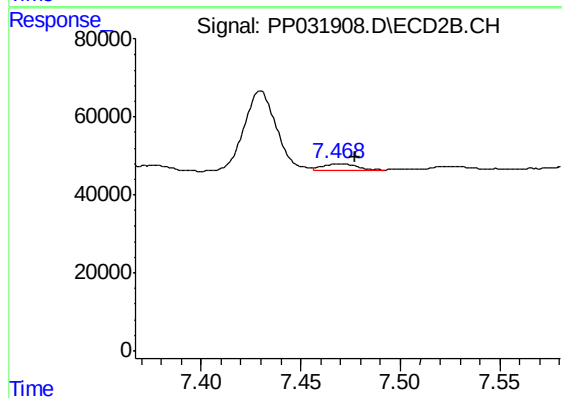

#36 AR-1262-1


R.T.: 7.469 min
Delta R.T.: -0.008 min
Response: 20947
Conc: 7.54 ng/ml

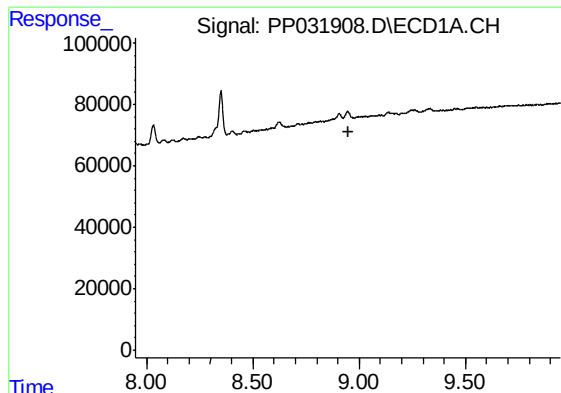

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT002

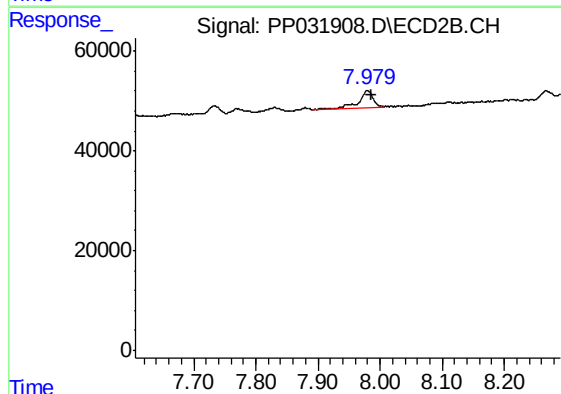


#37 AR-1262-2

R.T.: 7.980 min
Delta R.T.: -0.007 min
Response: 56375
Conc: 11.61 ng/ml

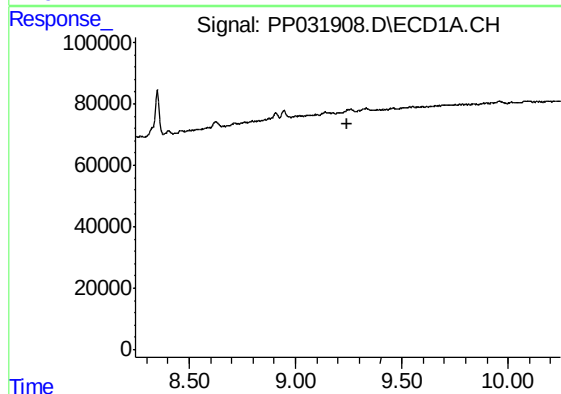


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.246 min
Response: 0
Conc: N.D.

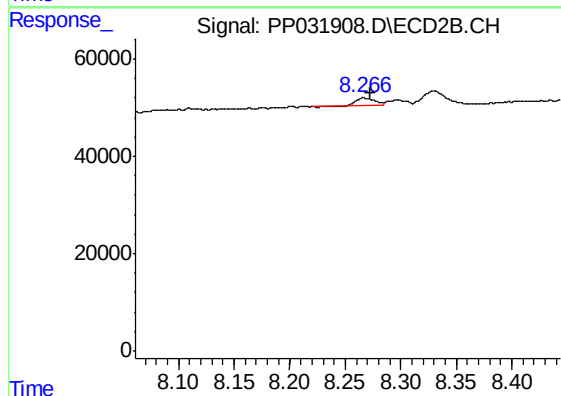

#38 AR-1262-3


R.T.: 8.267 min
Delta R.T.: -0.006 min
Response: 18434
Conc: 9.37 ng/ml

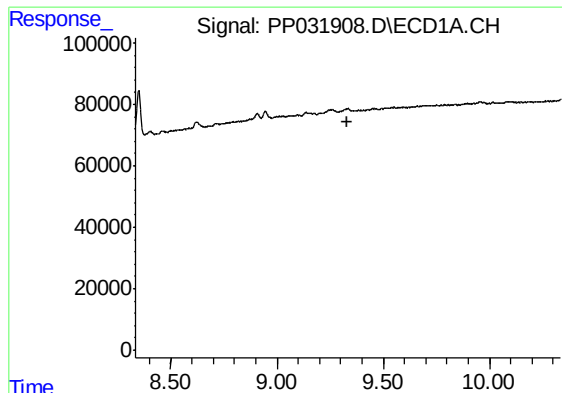

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 9.334 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT002

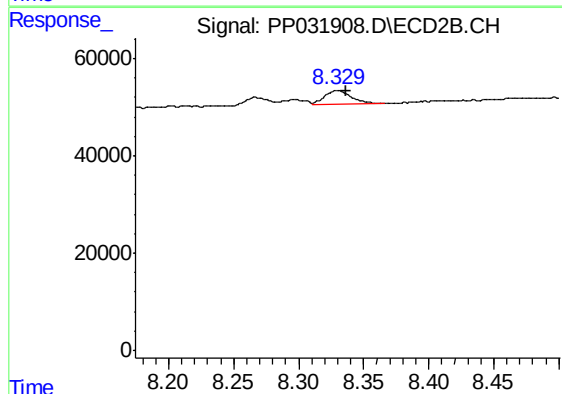


#39 AR-1262-4

R.T.: 8.330 min
Delta R.T.: -0.007 min
Response: 39673
Conc: 10.94 ng/ml

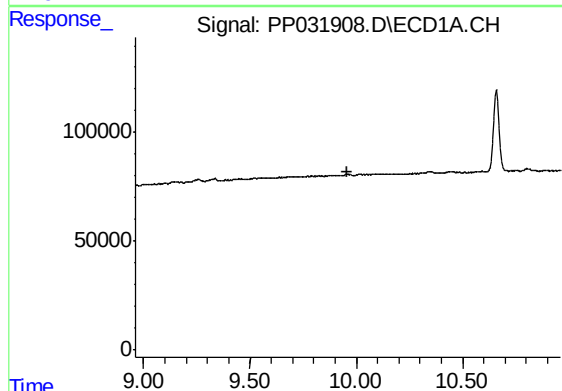


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.961 min
Response: 0
Conc: N.D.

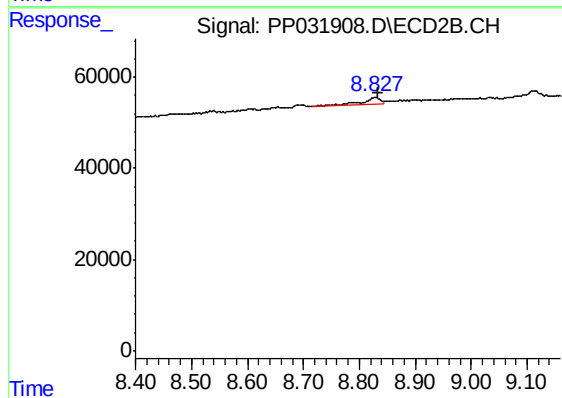

#40 AR-1262-5


R.T.: 8.827 min
Delta R.T.: -0.005 min
Response: 38171
Conc: 23.52 ng/ml

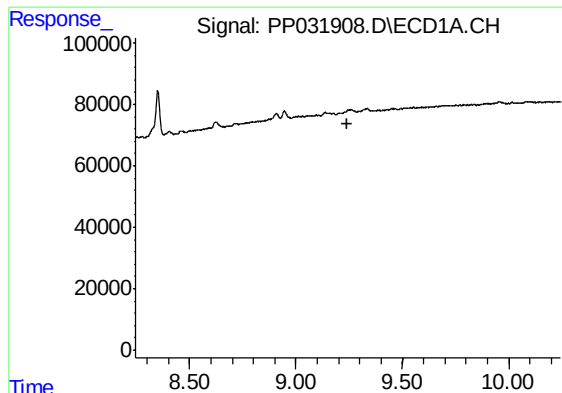

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 9.244 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT002

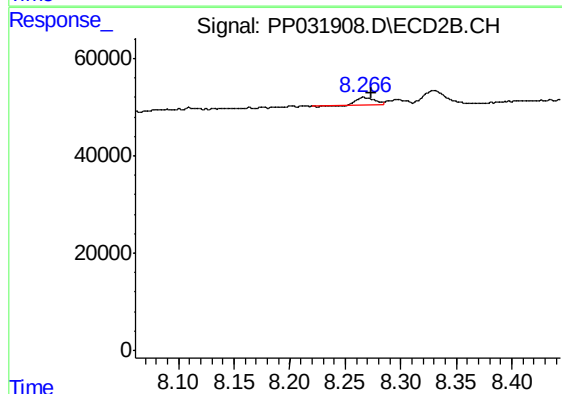


#41 AR-1268-1

R.T.: 8.267 min
Delta R.T.: -0.007 min
Response: 18434
Conc: 3.33 ng/ml

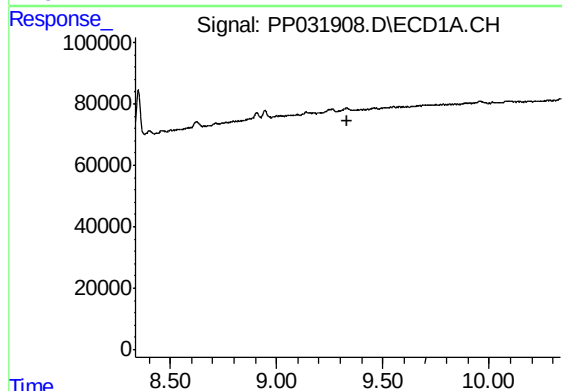


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.336 min
Response: 0
Conc: N.D.

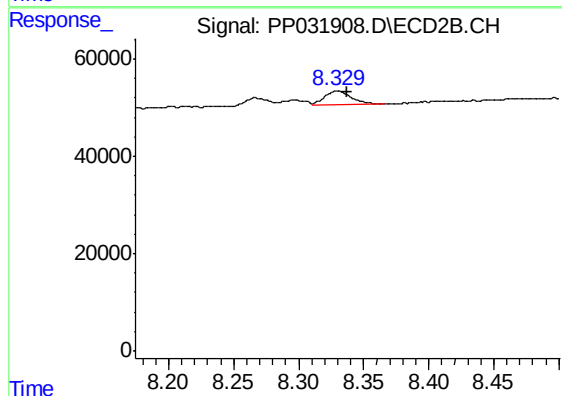

#42 AR-1268-2


R.T.: 8.330 min
Delta R.T.: -0.008 min
Response: 39673
Conc: 7.34 ng/ml

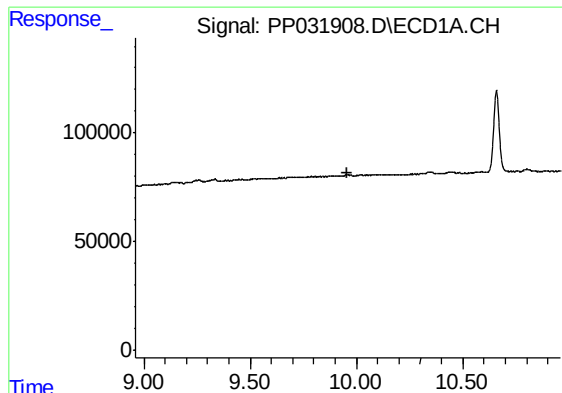

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 9.960 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT002

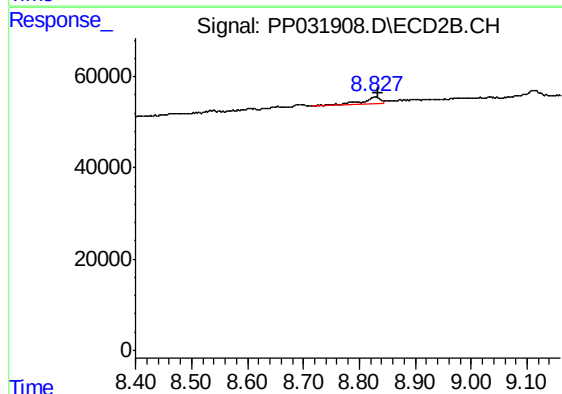


#44 AR-1268-4

R.T.: 8.827 min
Delta R.T.: -0.005 min
Response: 38171
Conc: 20.94 ng/ml

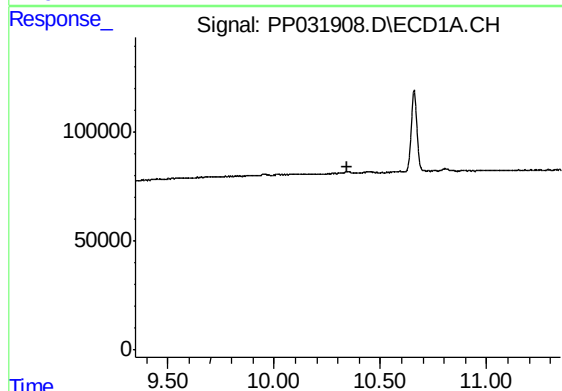

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.347 min
Response: 0
Conc: N.D.

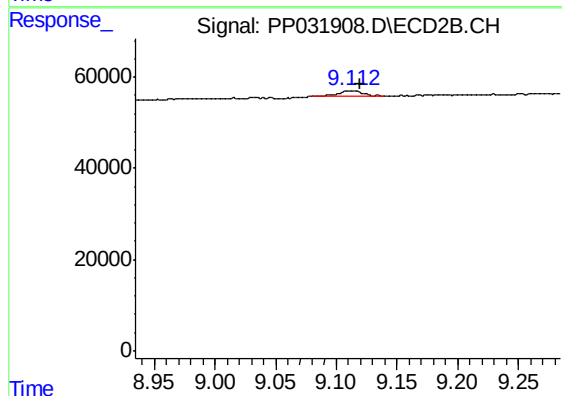

#45 AR-1268-5

R.T.: 9.112 min
Delta R.T.: -0.007 min
Response: 19205
Conc: 1.39 ng/ml