

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120820\
 Data File : PP031909.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Dec 2020 18:06
 Operator : DD\AJ
 Sample : L4965-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CRT014

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 01:03:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.786	4.059	1138012	1026562	23.501	21.423
2)	SA Decachlor...	10.659	9.358	541452	571303	15.942	15.429
Target Compounds							
7)	L1 AR-1016-5	0.000	5.835f	0	3416	N.D.	3.004 #
9)	L2 AR-1221-2	0.000	4.410	0	20323	N.D.	52.683 #
15)	L3 AR-1232-5	0.000	5.835f	0	3416	N.D.	11.789 #
20)	L4 AR-1242-5	0.000	6.190	0	13061	N.D.	12.660 #
24)	L5 AR-1248-4	0.000	5.835f	0	3416	N.D.	2.230 #
26)	L6 AR-1254-1	0.000	6.190	0	13061	N.D.	6.038 #
28)	L6 AR-1254-3	0.000	6.765	0	6505	N.D.	2.104 #
30)	L6 AR-1254-5	8.350f	7.430	318477	342132	170.362	126.735 #
31)	L7 AR-1260-1	0.000	6.897	0	14470	N.D.	7.322 #
32)	L7 AR-1260-2	8.032	7.094	78549	20155	38.228	8.277 #
33)	L7 AR-1260-3	0.000	7.248	0	15564	N.D.	6.815 #
34)	L7 AR-1260-4	8.625	7.733	31929	13305	17.340	7.002 #
35)	L7 AR-1260-5	0.000	7.980	0	41009	N.D.	9.037 #
36)	L8 AR-1262-1	0.000	7.467	0	14440	N.D.	5.196 #
37)	L8 AR-1262-2	0.000	7.980	0	41009	N.D.	8.443 #
38)	L8 AR-1262-3	0.000	8.270	0	11045	N.D.	5.616 #
39)	L8 AR-1262-4	0.000	8.330	0	24278	N.D.	6.697 #
40)	L8 AR-1262-5	0.000	8.830	0	9684	N.D.	5.966 #
41)	L9 AR-1268-1	0.000	8.270	0	11045	N.D.	1.996 #
42)	L9 AR-1268-2	0.000	8.330	0	24278	N.D.	4.490 #
44)	L9 AR-1268-4	0.000	8.830	0	9684	N.D.	5.313 #
45)	L9 AR-1268-5	0.000	9.111	0	15041	N.D.	1.086 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120820\
Data File : PP031909.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Dec 2020 18:06
Operator : DD\AJ
Sample : L4965-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
CRT014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 01:03:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

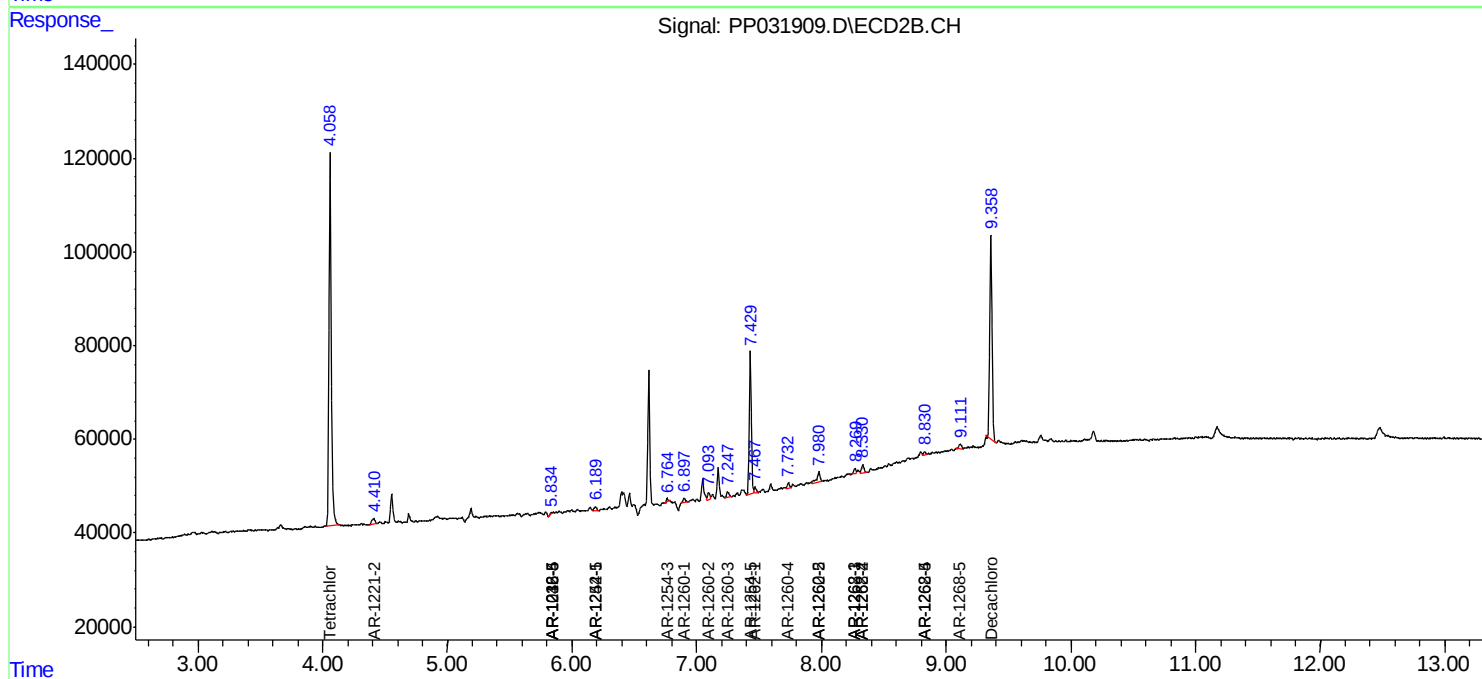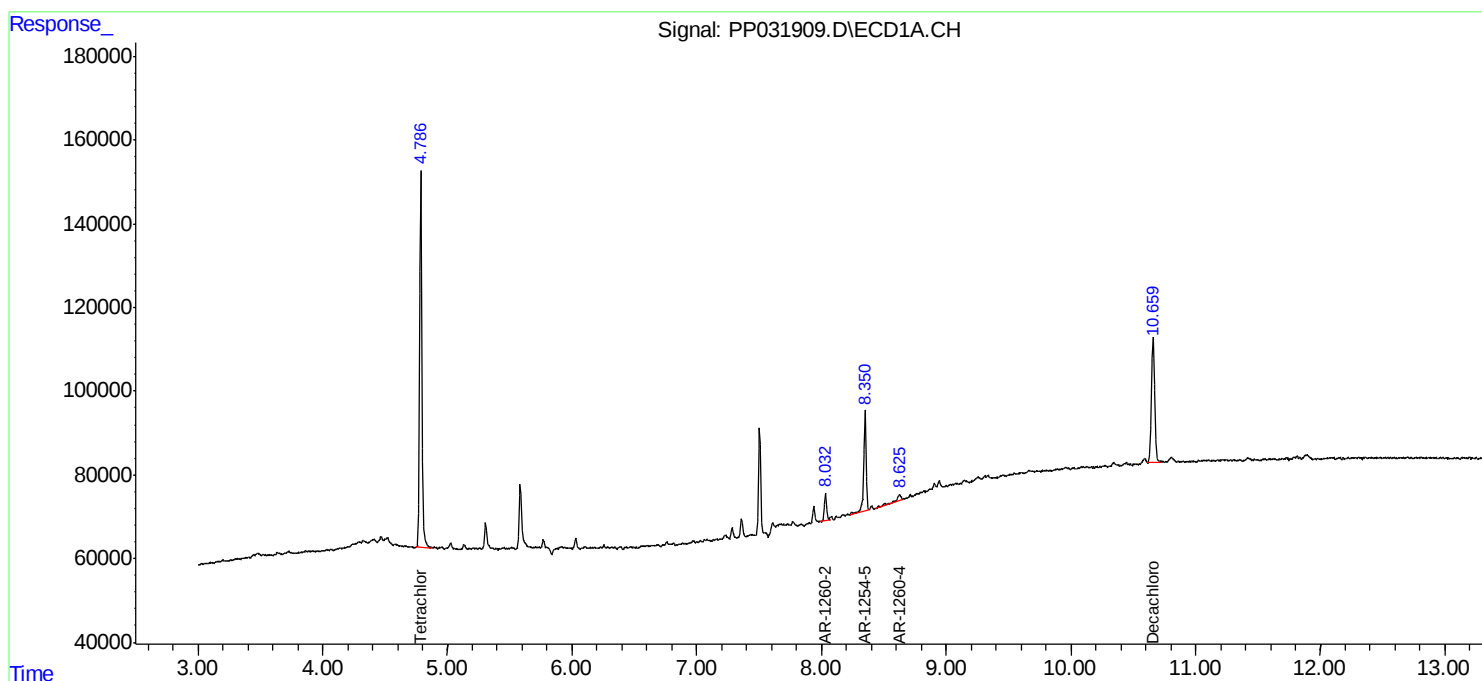


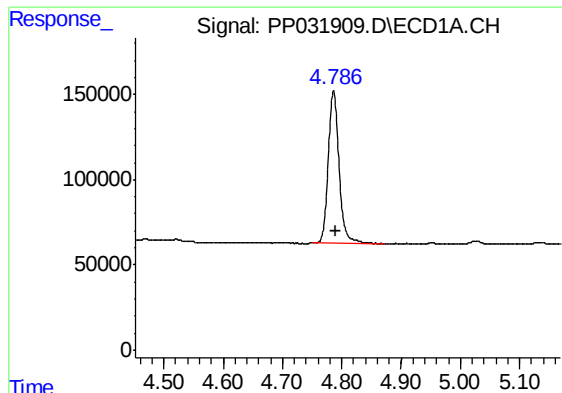

#1 Tetrachloro-m-xylene


R.T.: 4.786 min
Delta R.T.: -0.004 min
Response: 1138012
Conc: 23.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
CRT014

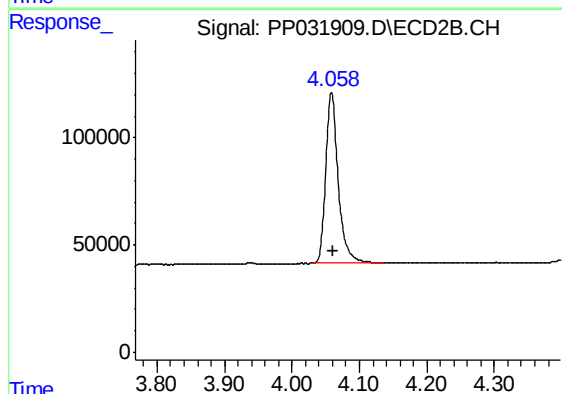


#1 Tetrachloro-m-xylene

R.T.: 4.059 min
Delta R.T.: -0.003 min
Response: 1026562
Conc: 21.42 ng/ml

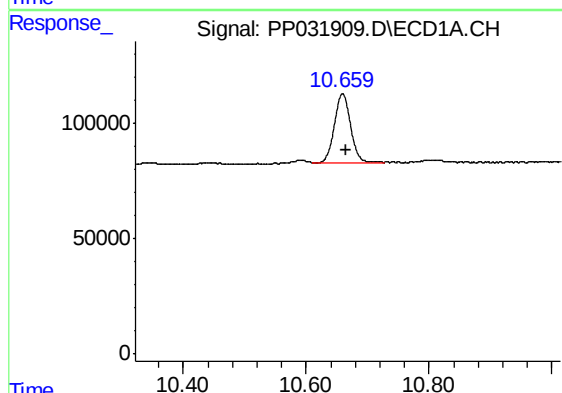


#2 Decachlorobiphenyl

R.T.: 10.659 min
Delta R.T.: -0.006 min
Response: 541452
Conc: 15.94 ng/ml

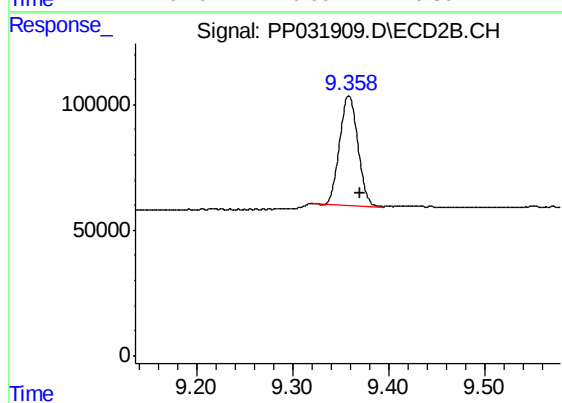

#2 Decachlorobiphenyl


R.T.: 9.358 min
Delta R.T.: -0.012 min
Response: 571303
Conc: 15.43 ng/ml

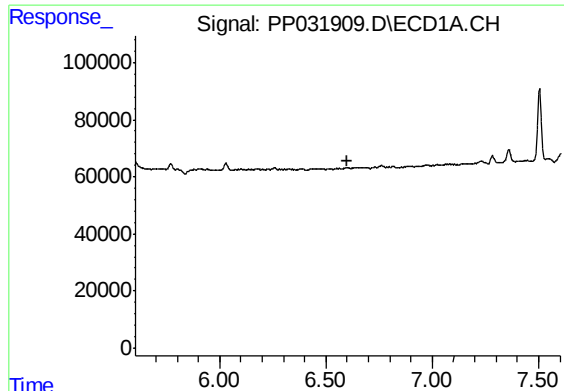

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 6.603 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT014

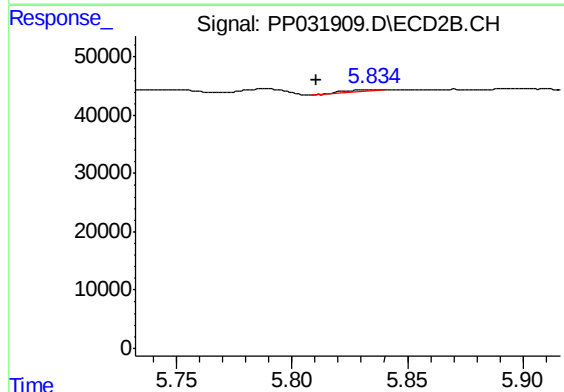


#7 AR-1016-5

R.T.: 5.835 min
Delta R.T.: 0.024 min
Response: 3416
Conc: 3.00 ng/ml

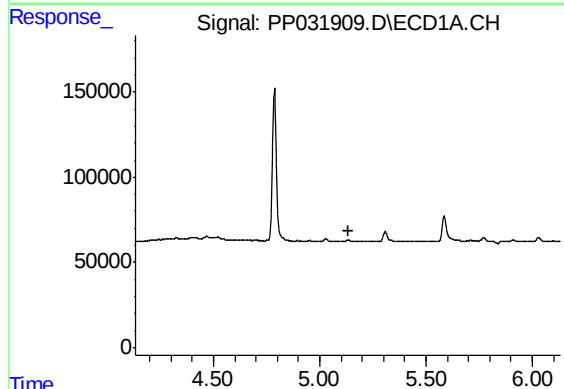


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.133 min
Response: 0
Conc: N.D.

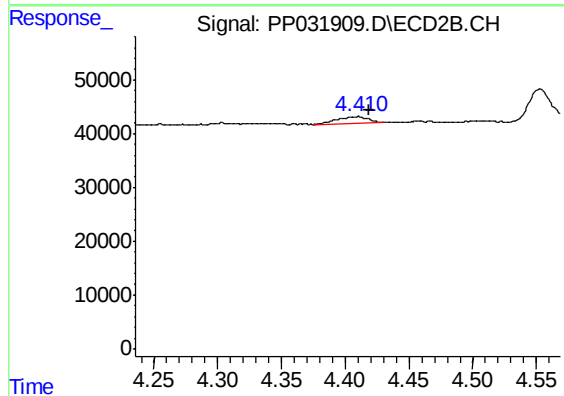

#9 AR-1221-2


R.T.: 4.410 min
Delta R.T.: -0.008 min
Response: 20323
Conc: 52.68 ng/ml

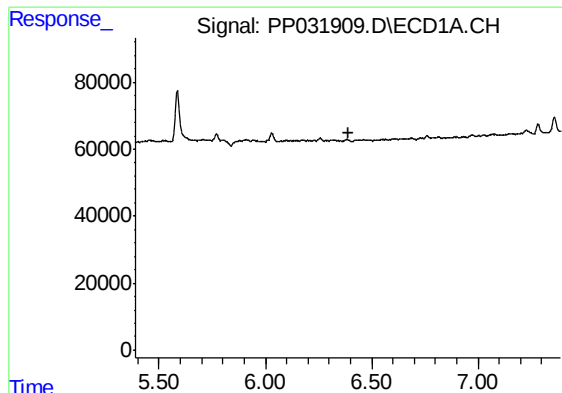

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 6.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT014

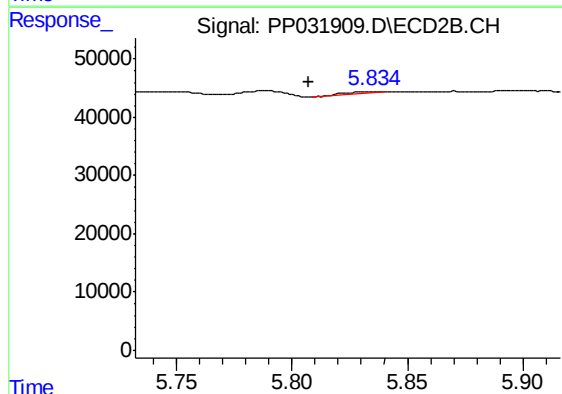


#15 AR-1232-5

R.T.: 5.835 min
Delta R.T.: 0.028 min
Response: 3416
Conc: 11.79 ng/ml

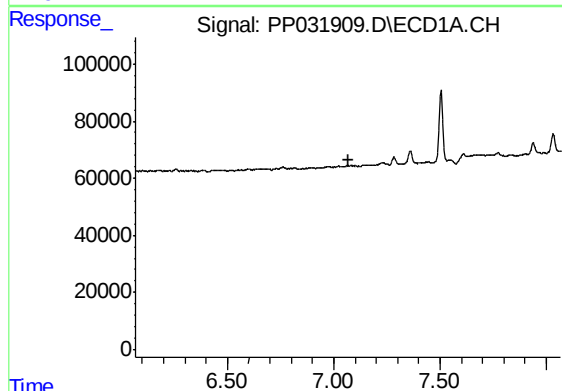


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 7.067 min
Response: 0
Conc: N.D.

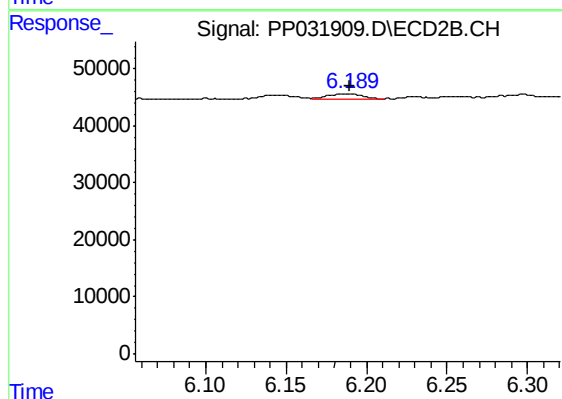

#20 AR-1242-5


R.T.: 6.190 min
Delta R.T.: 0.000 min
Response: 13061
Conc: 12.66 ng/ml

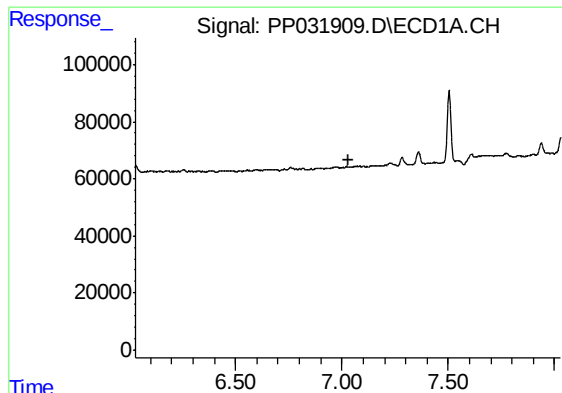

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 7.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT014

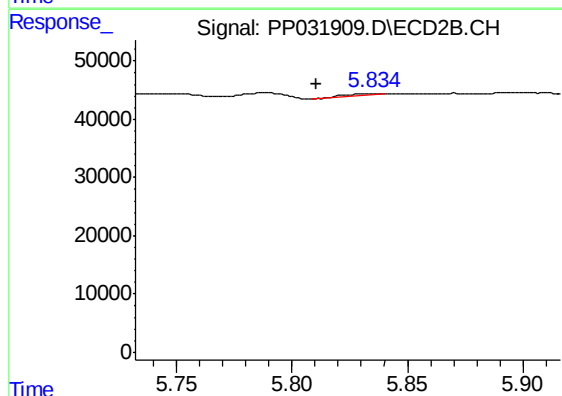


#24 AR-1248-4

R.T.: 5.835 min
Delta R.T.: 0.024 min
Response: 3416
Conc: 2.23 ng/ml

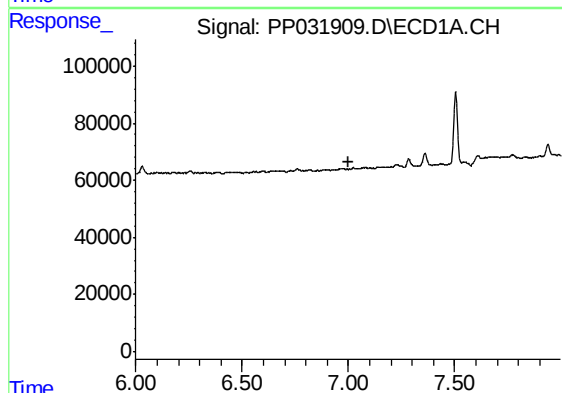


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.998 min
Response: 0
Conc: N.D.

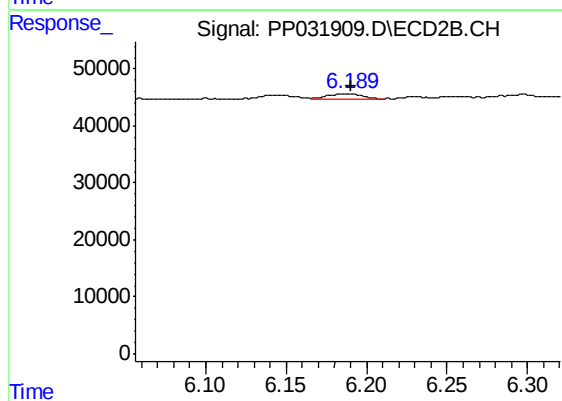

#26 AR-1254-1


R.T.: 6.190 min
Delta R.T.: 0.000 min
Response: 13061
Conc: 6.04 ng/ml

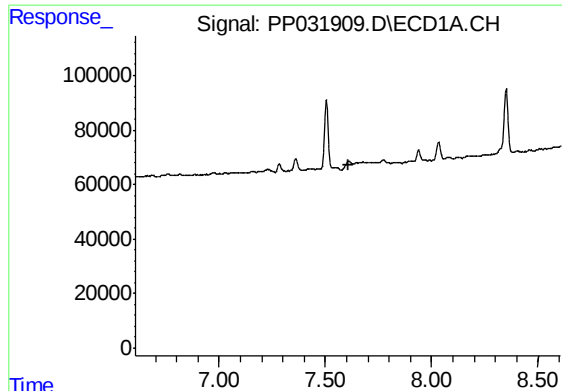

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 7.606 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT014

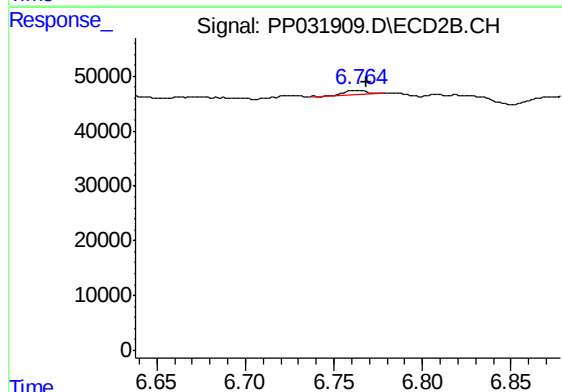


#28 AR-1254-3

R.T.: 6.765 min
Delta R.T.: -0.004 min
Response: 6505
Conc: 2.10 ng/ml

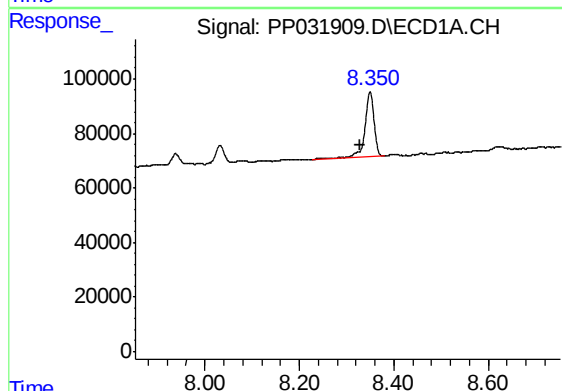


#30 AR-1254-5

R.T.: 8.350 min
Delta R.T.: 0.022 min
Response: 318477
Conc: 170.36 ng/ml

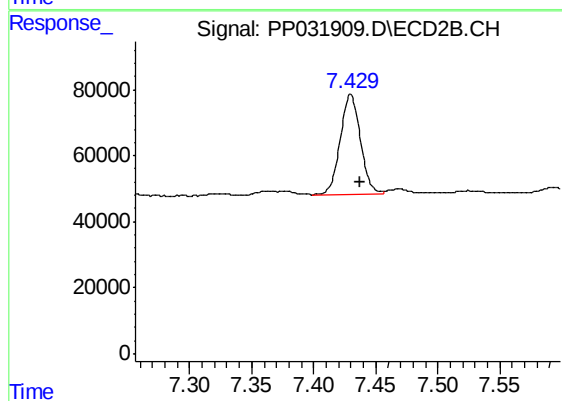

#30 AR-1254-5


R.T.: 7.430 min
Delta R.T.: -0.007 min
Response: 342132
Conc: 126.74 ng/ml

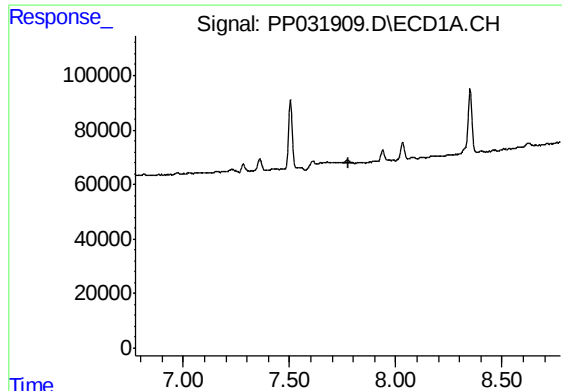

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.775 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT014

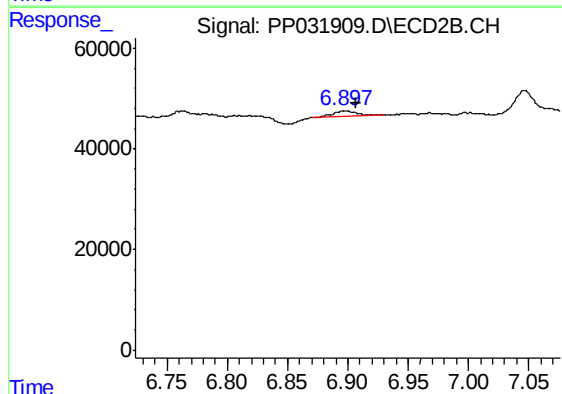


#31 AR-1260-1

R.T.: 6.897 min
Delta R.T.: -0.009 min
Response: 14470
Conc: 7.32 ng/ml

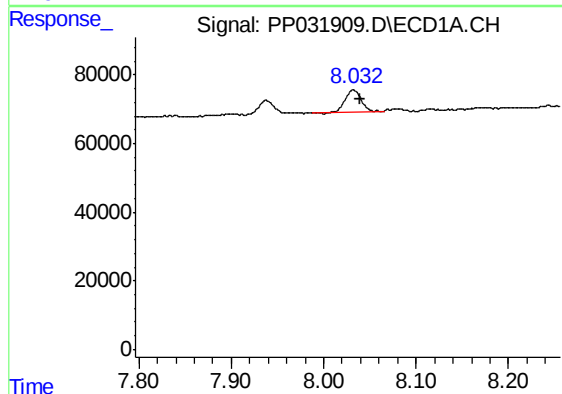


#32 AR-1260-2

R.T.: 8.032 min
Delta R.T.: -0.008 min
Response: 78549
Conc: 38.23 ng/ml

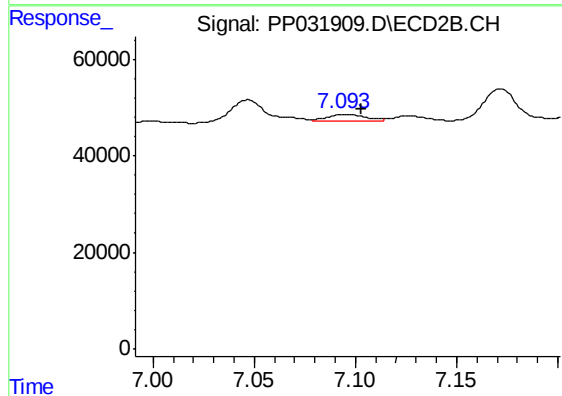

#32 AR-1260-2


R.T.: 7.094 min
Delta R.T.: -0.010 min
Response: 20155
Conc: 8.28 ng/ml

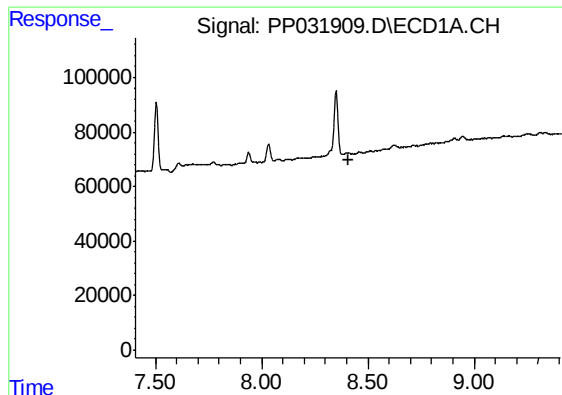

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.406 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT014

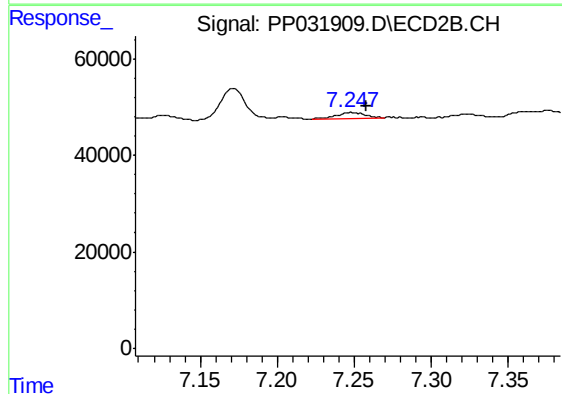


#33 AR-1260-3

R.T.: 7.248 min
Delta R.T.: -0.010 min
Response: 15564
Conc: 6.82 ng/ml

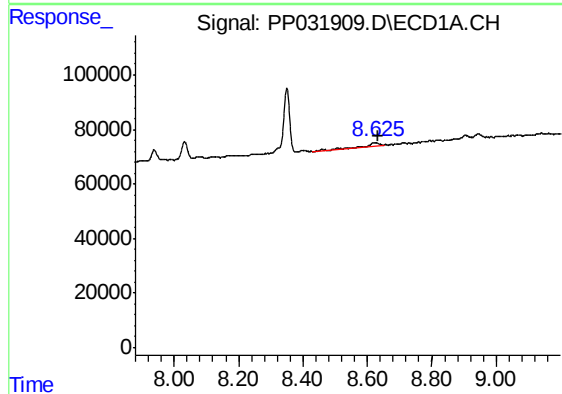


#34 AR-1260-4

R.T.: 8.625 min
Delta R.T.: -0.008 min
Response: 31929
Conc: 17.34 ng/ml

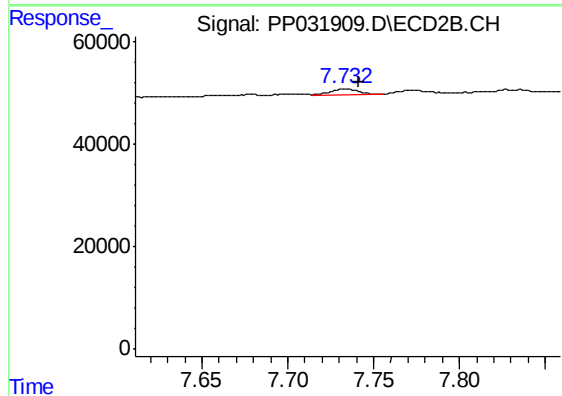

#34 AR-1260-4


R.T.: 7.733 min
Delta R.T.: -0.008 min
Response: 13305
Conc: 7.00 ng/ml

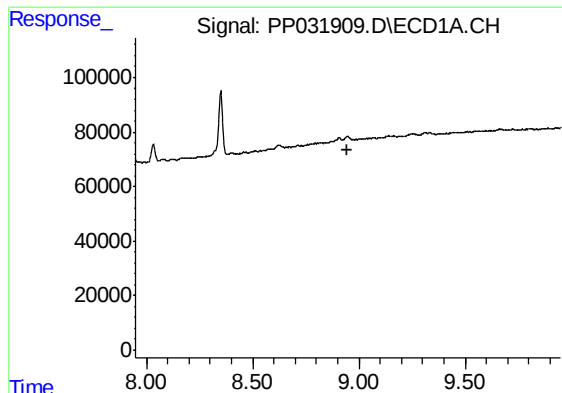

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT014

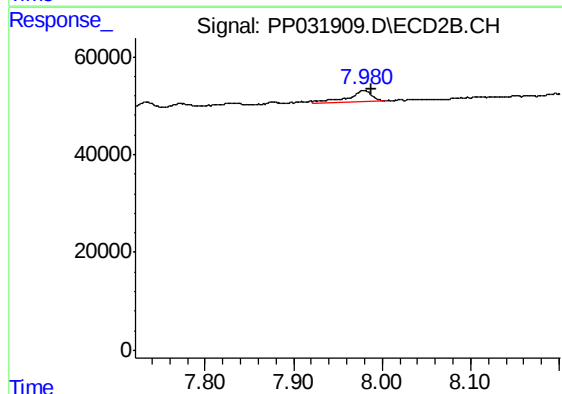


#35 AR-1260-5

R.T.: 7.980 min
Delta R.T.: -0.008 min
Response: 41009
Conc: 9.04 ng/ml

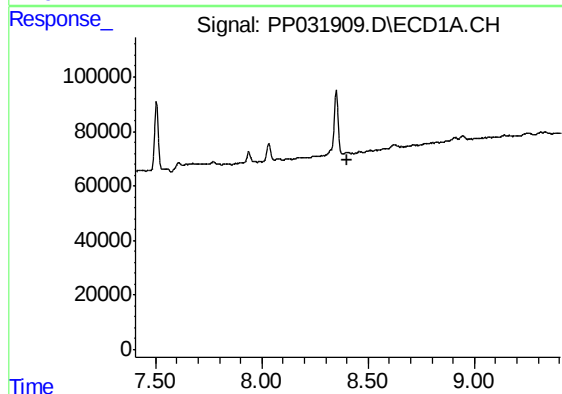


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.405 min
Response: 0
Conc: N.D.

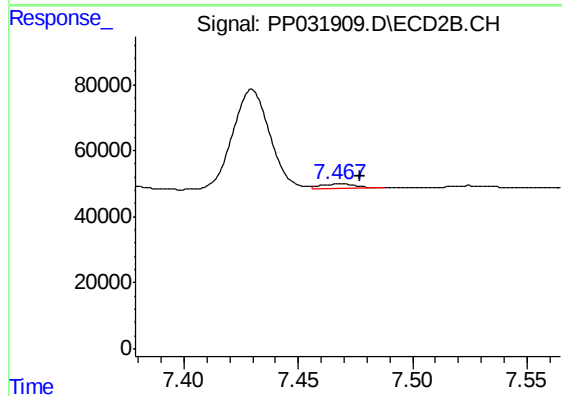

#36 AR-1262-1


R.T.: 7.467 min
Delta R.T.: -0.010 min
Response: 14440
Conc: 5.20 ng/ml

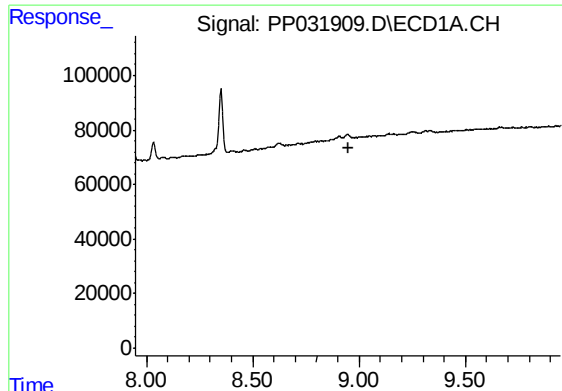

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT014

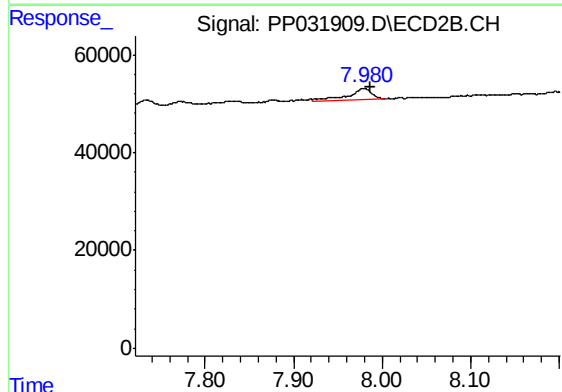


#37 AR-1262-2

R.T.: 7.980 min
Delta R.T.: -0.006 min
Response: 41009
Conc: 8.44 ng/ml

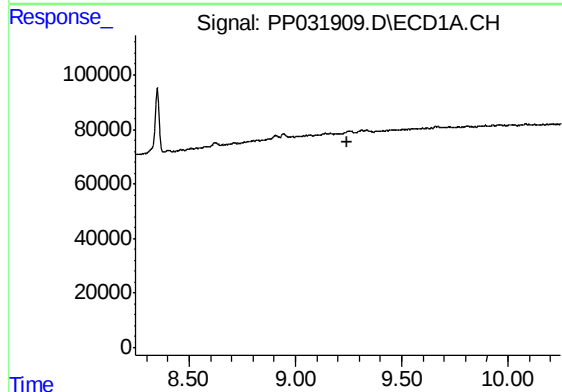


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.246 min
Response: 0
Conc: N.D.

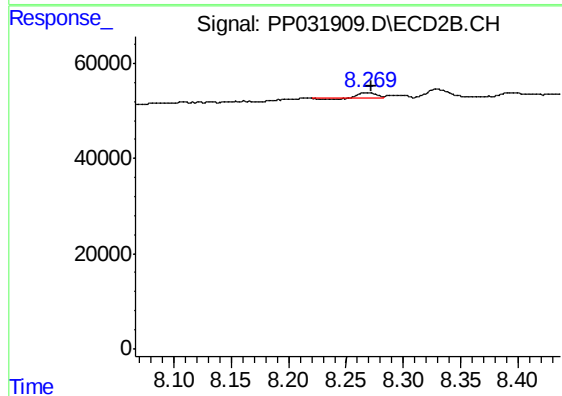

#38 AR-1262-3


R.T.: 8.270 min
Delta R.T.: -0.003 min
Response: 11045
Conc: 5.62 ng/ml

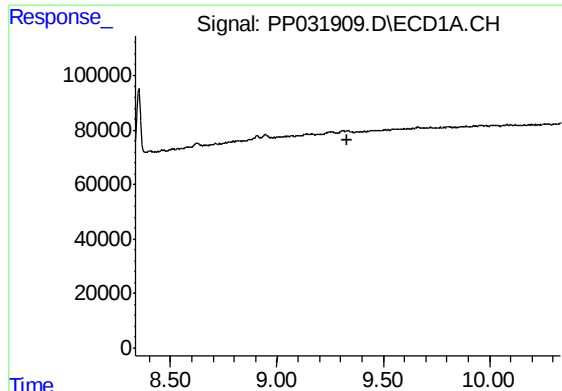

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 9.334 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT014

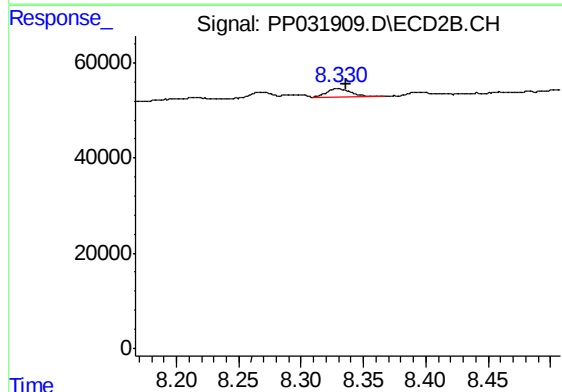


#39 AR-1262-4

R.T.: 8.330 min
Delta R.T.: -0.006 min
Response: 24278
Conc: 6.70 ng/ml

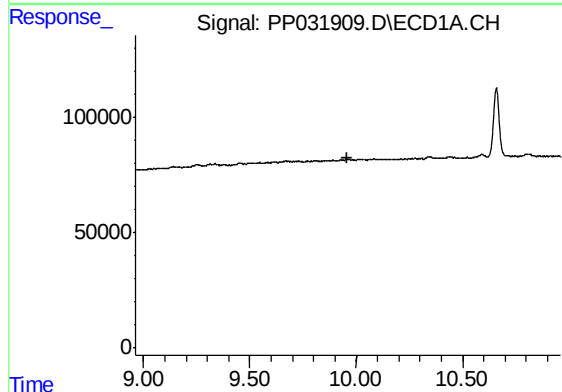


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.961 min
Response: 0
Conc: N.D.

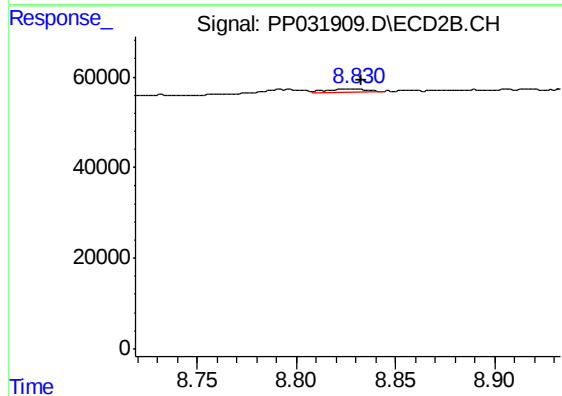

#40 AR-1262-5


R.T.: 8.830 min
Delta R.T.: -0.003 min
Response: 9684
Conc: 5.97 ng/ml

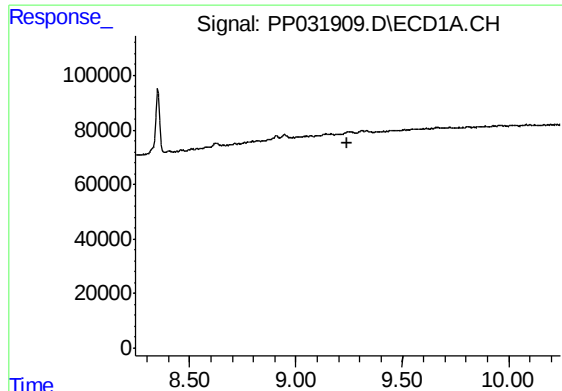

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 9.244 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT014

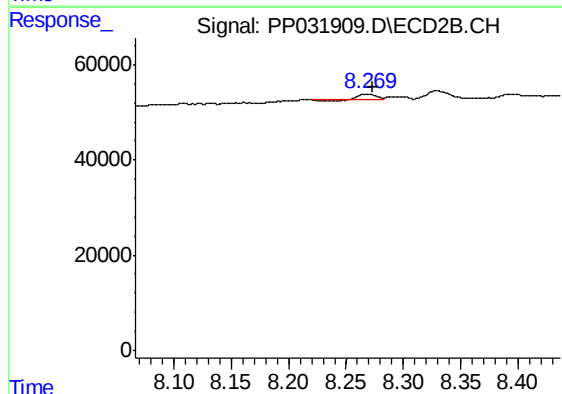


#41 AR-1268-1

R.T.: 8.270 min
Delta R.T.: -0.004 min
Response: 11045
Conc: 2.00 ng/ml

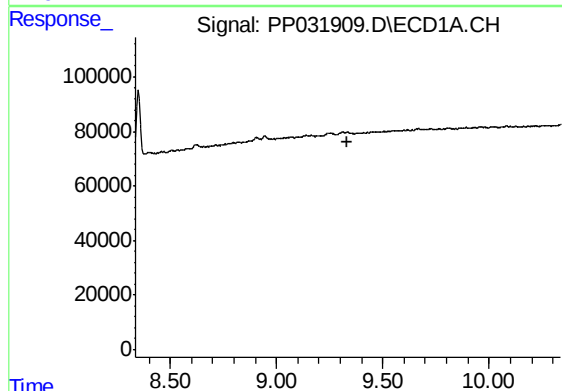


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.336 min
Response: 0
Conc: N.D.

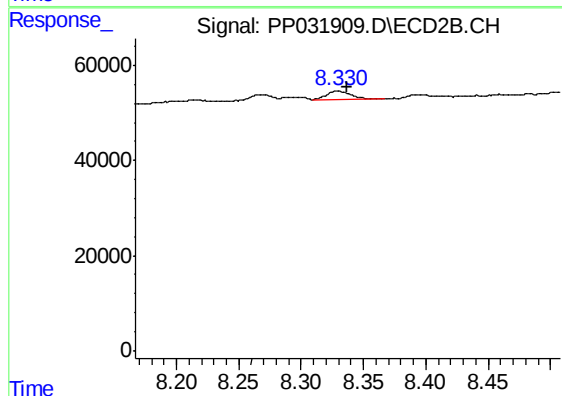

#42 AR-1268-2


R.T.: 8.330 min
Delta R.T.: -0.008 min
Response: 24278
Conc: 4.49 ng/ml

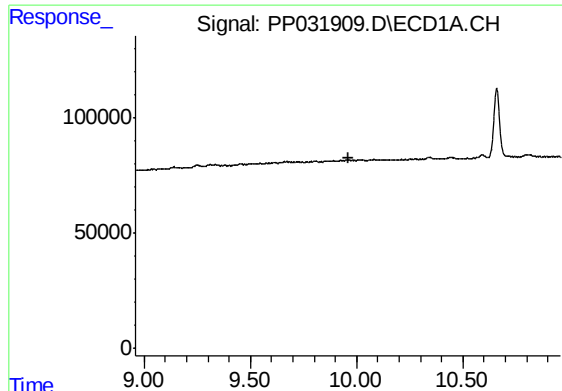

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 9.960 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CRT014

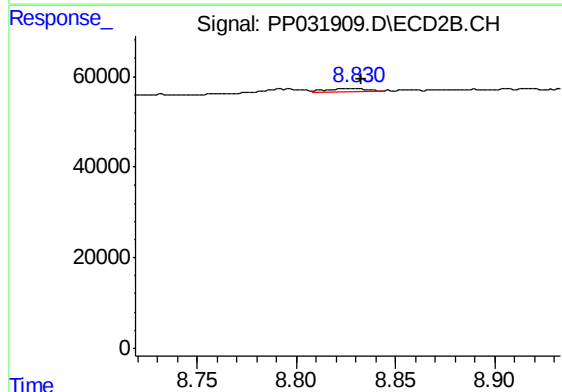


#44 AR-1268-4

R.T.: 8.830 min
Delta R.T.: -0.002 min
Response: 9684
Conc: 5.31 ng/ml

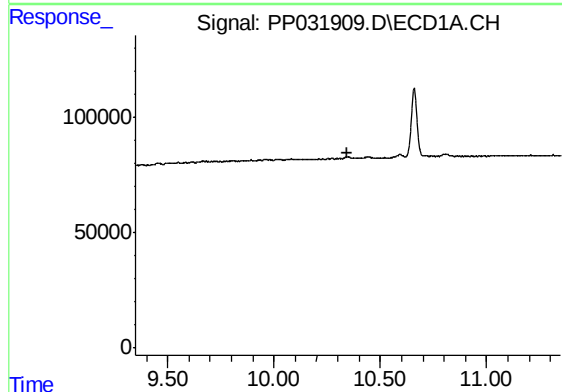

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.347 min
Response: 0
Conc: N.D.

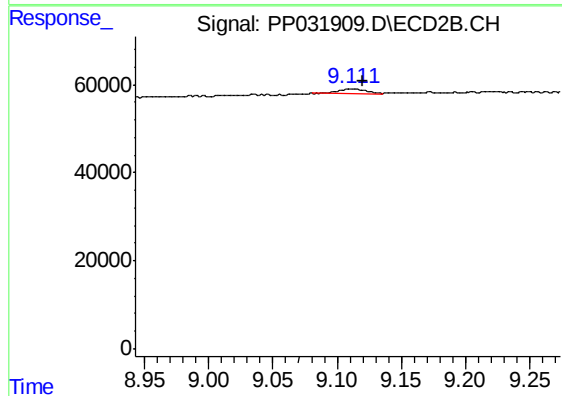

#45 AR-1268-5

R.T.: 9.111 min
Delta R.T.: -0.008 min
Response: 15041
Conc: 1.09 ng/ml