

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120820\
 Data File : PP031909.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Dec 2020 18:06
 Operator : DD\AJ
 Sample : L4965-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CRT014

Manual Integrations
 APPROVED

Ankita
 12/9/2020 10:06:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 01:03:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.786	4.059	1138012	1026562	23.501	21.423
2) SA Decachlor...	10.659	9.358	541452	597763	15.942	16.144m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120820\
Data File : PP031909.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Dec 2020 18:06
Operator : DD\AJ
Sample : L4965-11
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CRT014


Manual Integrations
APPROVED

Ankita
12/9/2020 10:06:55 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 01:03:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

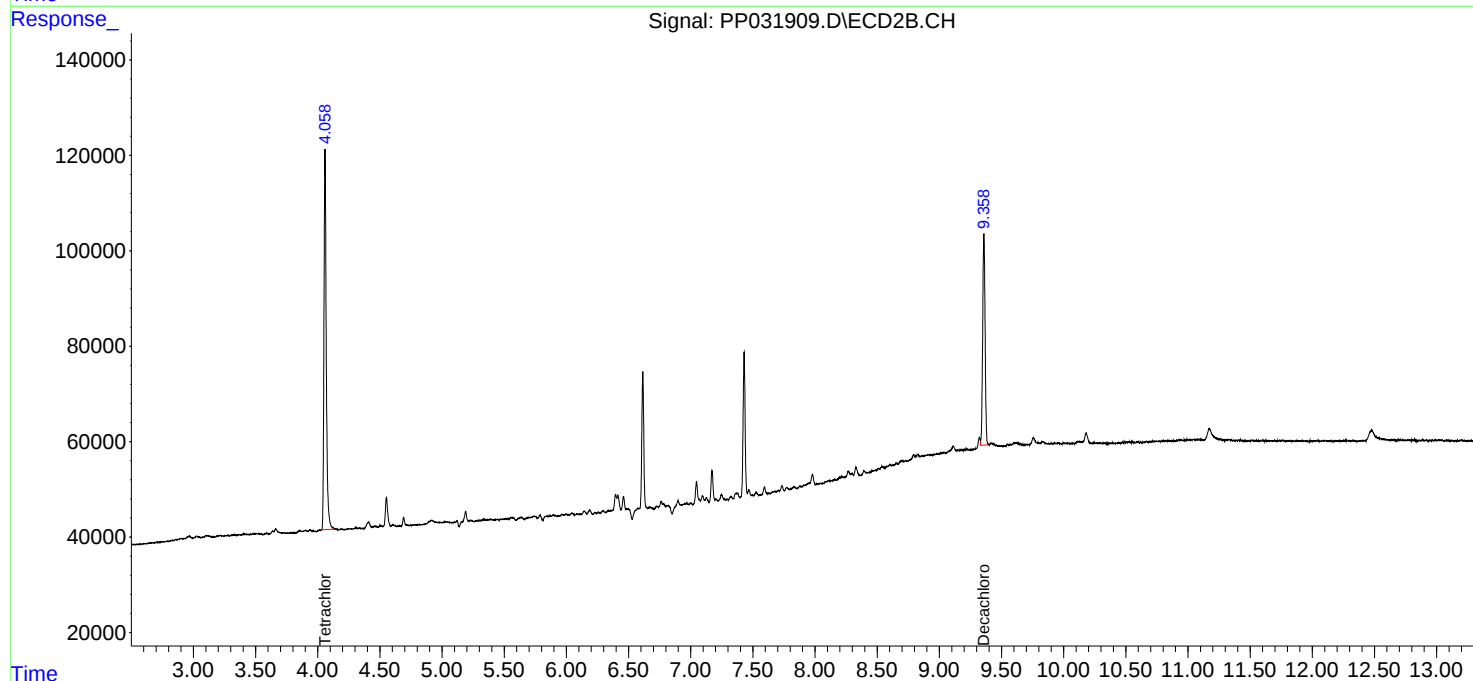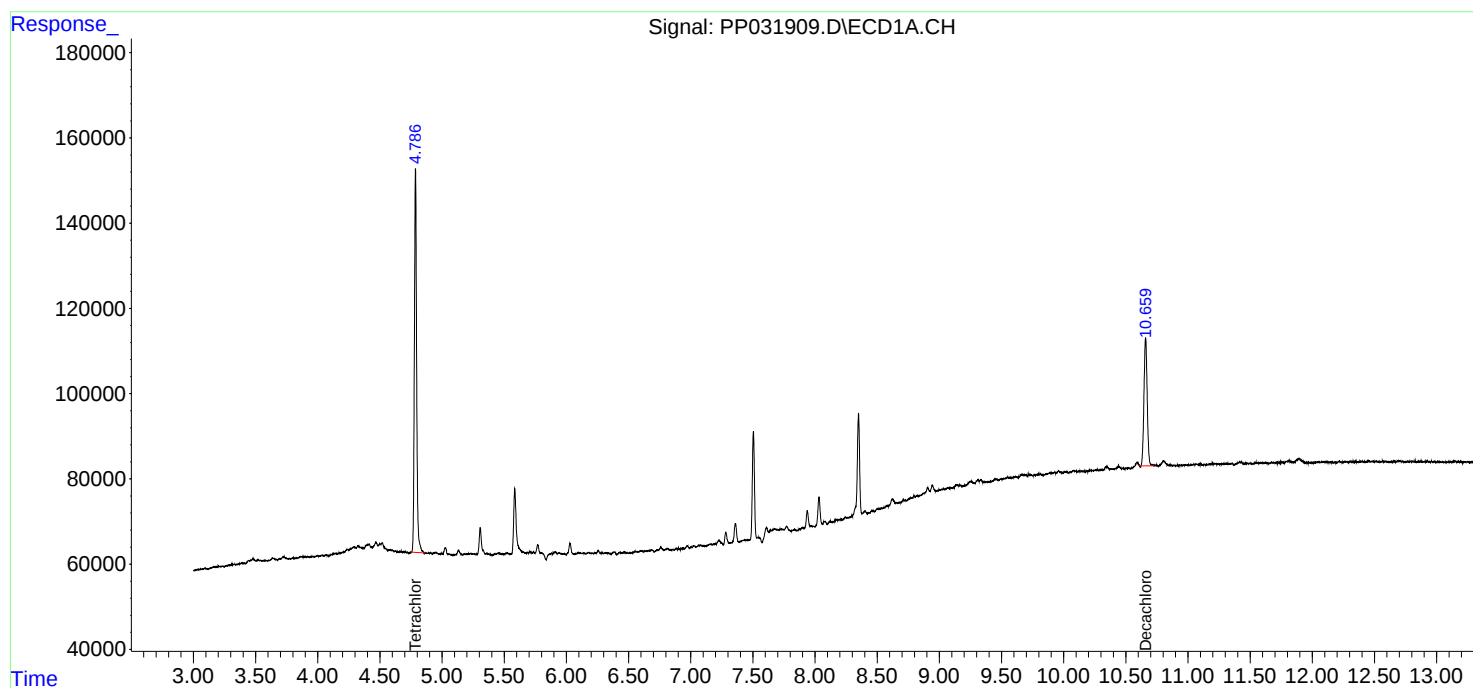

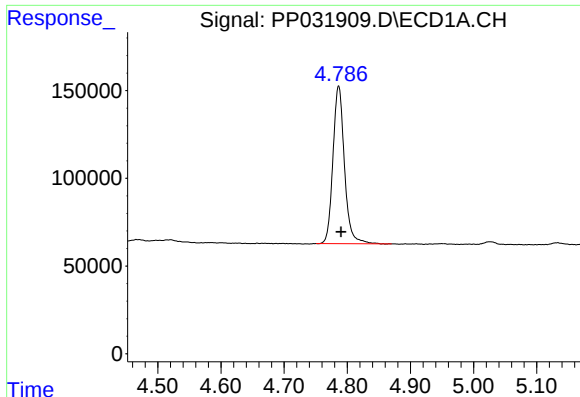


#1 Tetrachloro-m-xylene

R.T.: 4.786 min
Delta R.T.: -0.004 min
Response: 1138012
Conc: 23.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
CRT014


Manual Integrations
APPROVED

Ankita
12/9/2020 10:06:55 AM

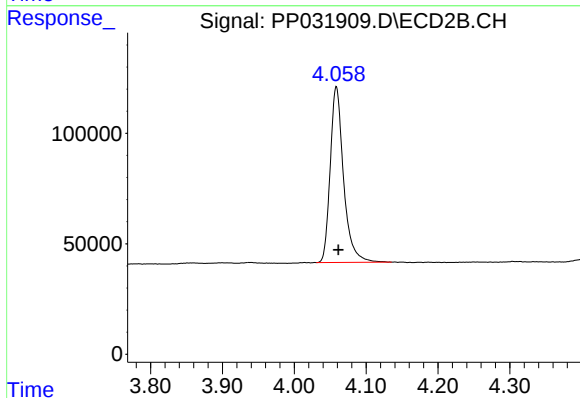


#1 Tetrachloro-m-xylene

R.T.: 4.059 min
Delta R.T.: -0.003 min
Response: 1026562
Conc: 21.42 ng/ml

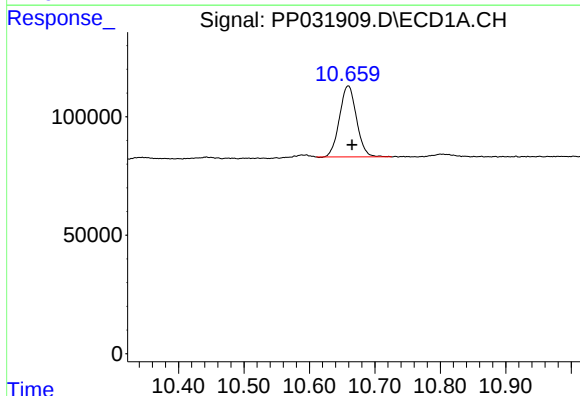

#2 Decachlorobiphenyl

R.T.: 10.659 min
Delta R.T.: -0.006 min
Response: 541452
Conc: 15.94 ng/ml

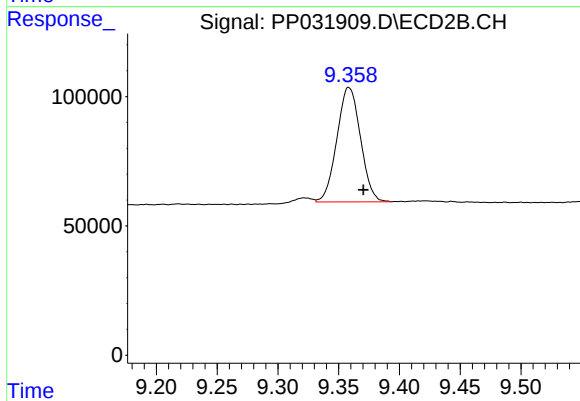

#2 Decachlorobiphenyl

R.T.: 9.358 min
Delta R.T.: -0.013 min
Response: 597763
Conc: 16.14 ng/ml m