

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120820\
 Data File : PP031913.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Dec 2020 19:13
 Operator : DD\AJ
 Sample : L4970-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 4S2-A-D-COMP

Manual Integrations
 APPROVED

Ankita
 12/9/2020 10:06:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 03:57:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.786	4.058	1184008	972863	24.451	20.302
2) SA Decachlor...	10.659	9.358	726149	763000	21.380	20.606
Target Compounds						
31) L7 AR-1260-1	7.775	6.898	43701	39117	24.971m	19.795
32) L7 AR-1260-2	8.033	7.091	39014	136560	18.987	56.076 #
33) L7 AR-1260-3	8.402	7.250	70686	53196	43.338	23.294 #
34) L7 AR-1260-4	8.628	7.733	78763	71044	42.775m	37.389
35) L7 AR-1260-5	8.944	7.979	151205	174297	41.008	38.409

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120820\
Data File : PP031913.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Dec 2020 19:13
Operator : DD\AJ
Sample : L4970-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
4S2-A-D-COMP


Manual Integrations
APPROVED

Ankita
12/9/2020 10:06:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 03:57:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

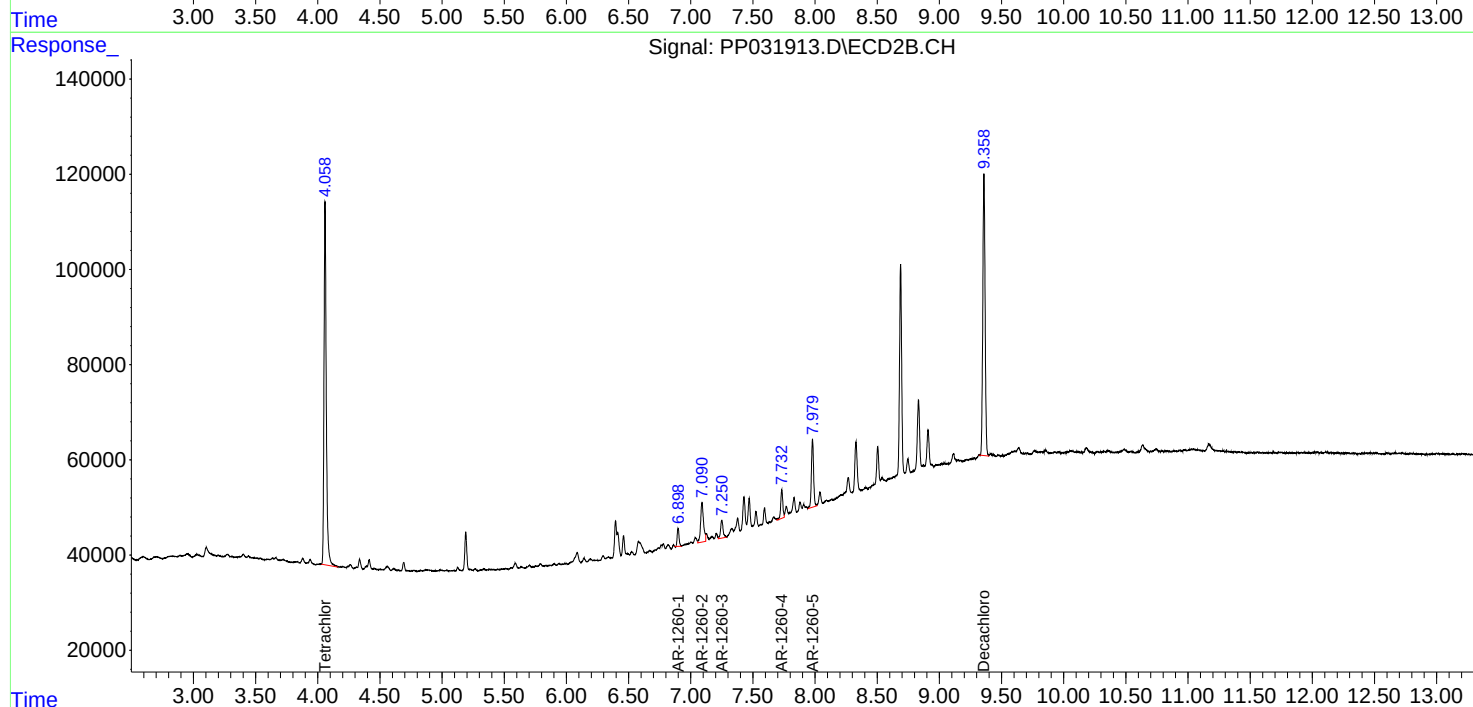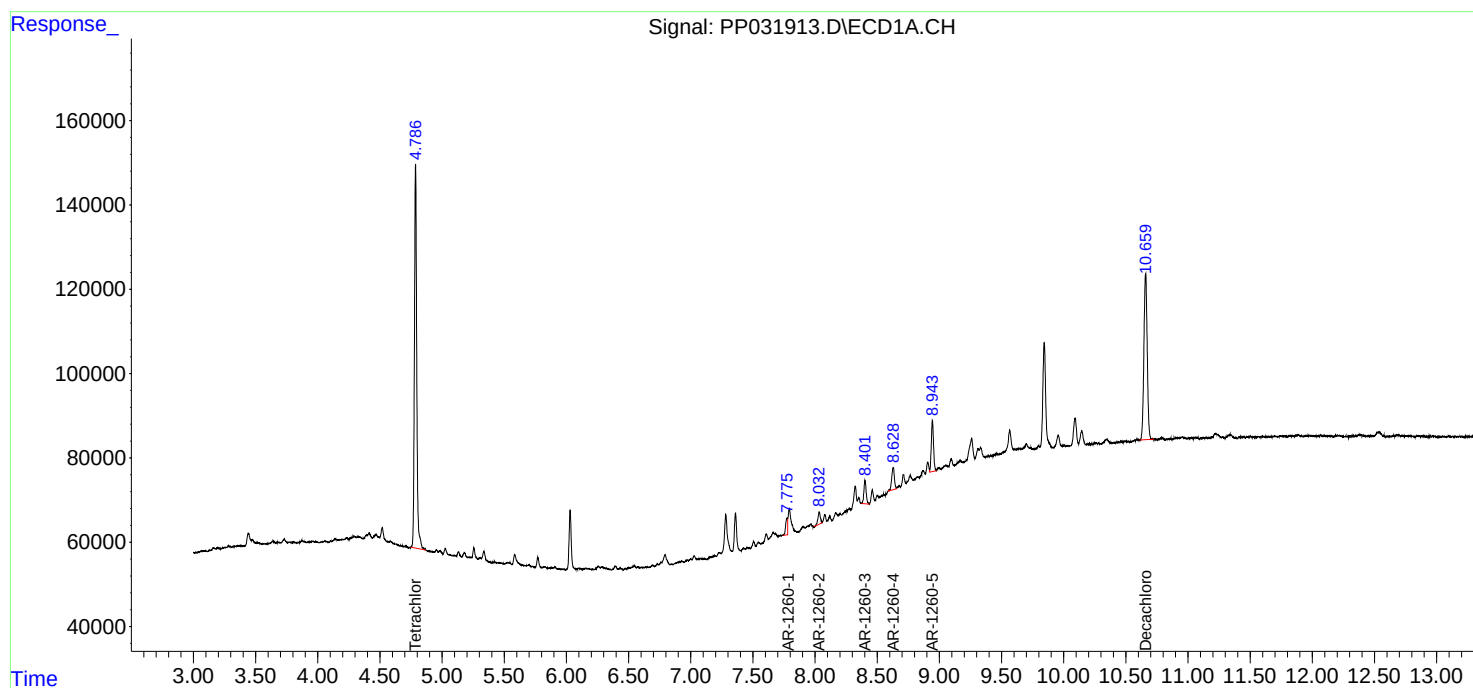

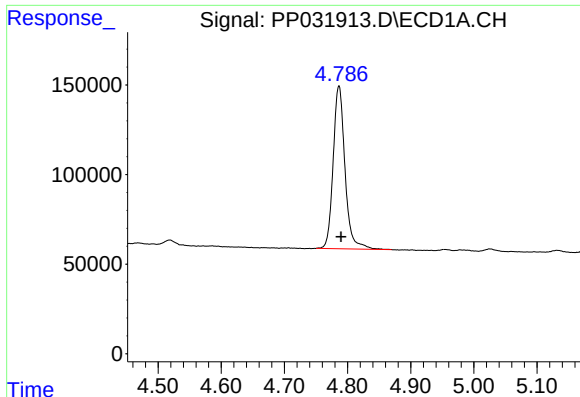


#1 Tetrachloro-m-xylene

R.T.: 4.786 min
Delta R.T.: -0.004 min
Response: 1184008
Conc: 24.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
4S2-A-D-COMP


Manual Integrations
APPROVED

Ankita
12/9/2020 10:06:57 AM

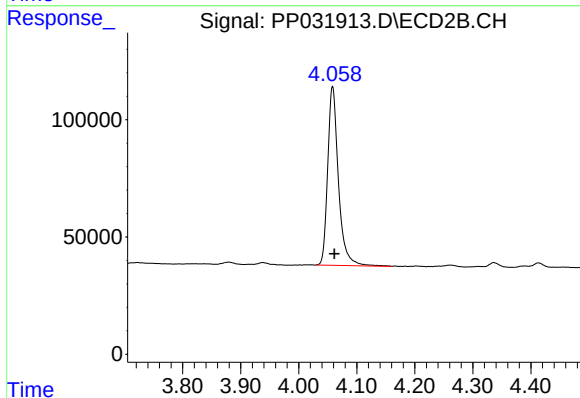


#1 Tetrachloro-m-xylene

R.T.: 4.058 min
Delta R.T.: -0.003 min
Response: 972863
Conc: 20.30 ng/ml

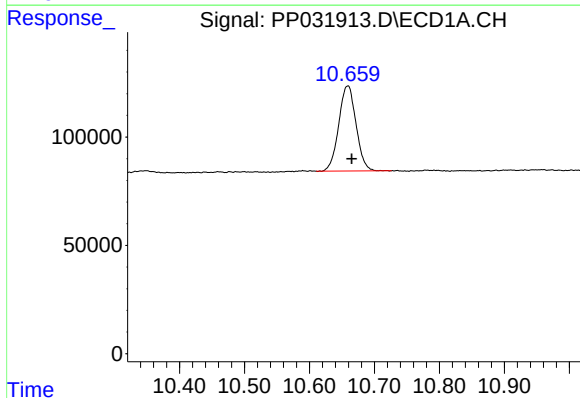


#2 Decachlorobiphenyl

R.T.: 10.659 min
Delta R.T.: -0.006 min
Response: 726149
Conc: 21.38 ng/ml

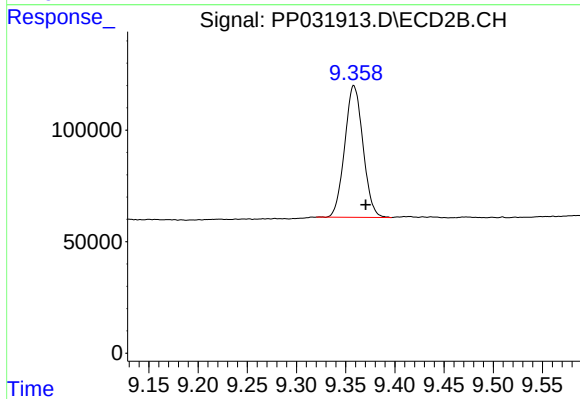

#2 Decachlorobiphenyl

R.T.: 9.358 min
Delta R.T.: -0.012 min
Response: 763000
Conc: 20.61 ng/ml

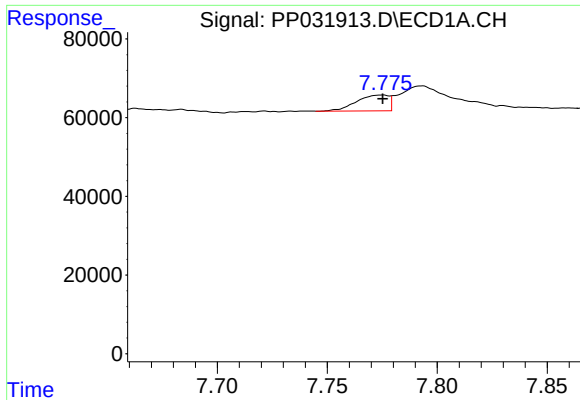


#31 AR-1260-1

R.T.: 7.775 min
Delta R.T.: 0.000 min
Response: 43701
Conc: 24.97 ng/ml m

Instrument :
ECD_P
ClientSampleId :
4S2-A-D-COMP


Manual Integrations
APPROVED

Ankita
12/9/2020 10:06:57 AM

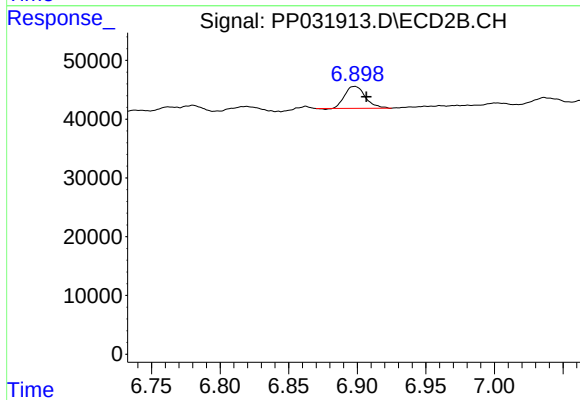


#31 AR-1260-1

R.T.: 6.898 min
Delta R.T.: -0.009 min
Response: 39117
Conc: 19.80 ng/ml

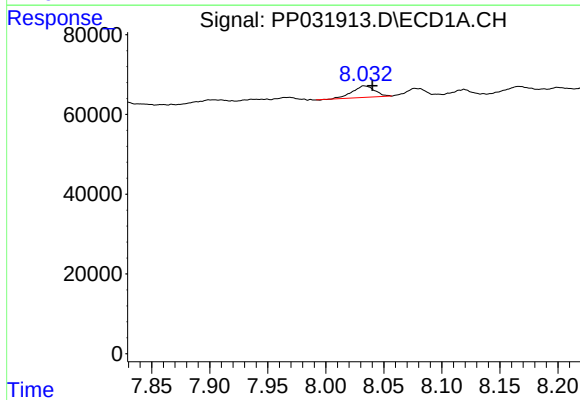


#32 AR-1260-2

R.T.: 8.033 min
Delta R.T.: -0.007 min
Response: 39014
Conc: 18.99 ng/ml

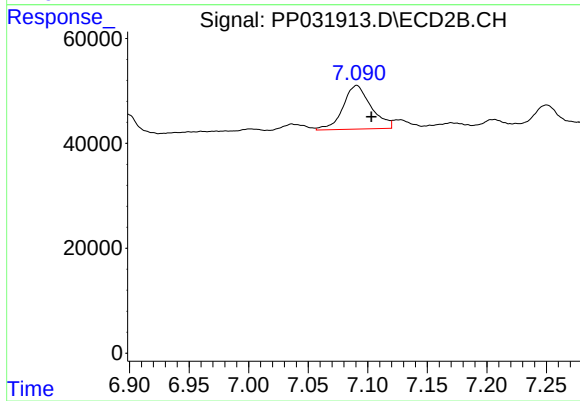

#32 AR-1260-2

R.T.: 7.091 min
Delta R.T.: -0.012 min
Response: 136560
Conc: 56.08 ng/ml

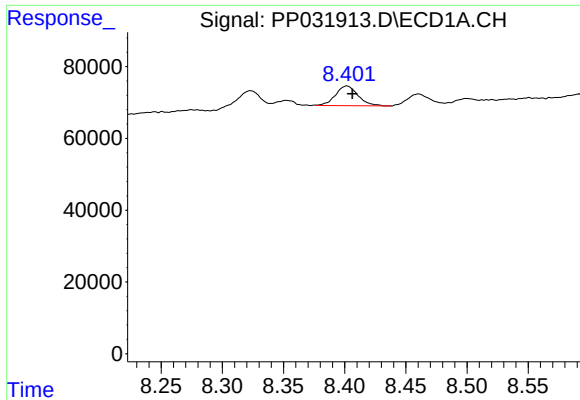


#33 AR-1260-3

R.T.: 8.402 min
Delta R.T.: -0.004 min
Response: 70686
Conc: 43.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
4S2-A-D-COMP


Manual Integrations
APPROVED

Ankita
12/9/2020 10:06:57 AM

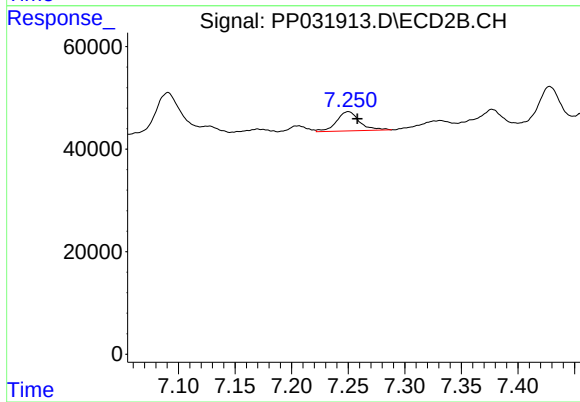


#33 AR-1260-3

R.T.: 7.250 min
Delta R.T.: -0.008 min
Response: 53196
Conc: 23.29 ng/ml

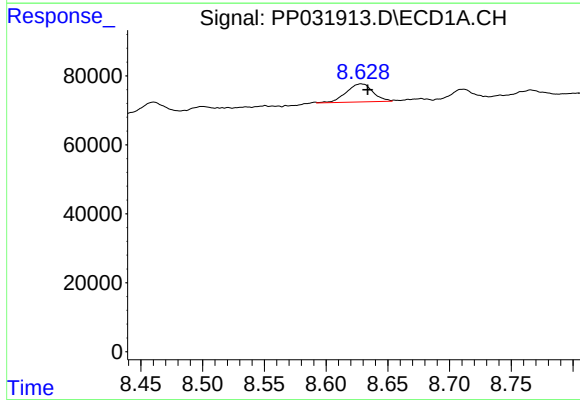


#34 AR-1260-4

R.T.: 8.628 min
Delta R.T.: -0.006 min
Response: 78763
Conc: 42.77 ng/ml m

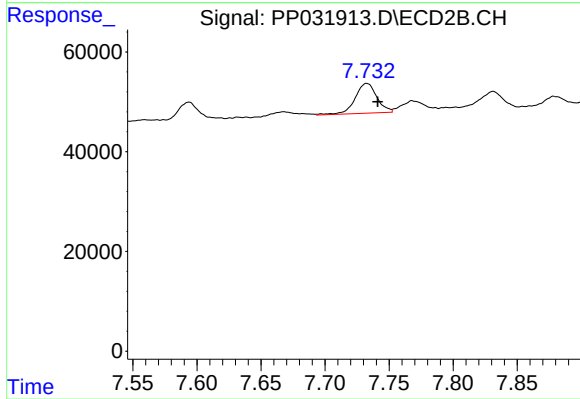

#34 AR-1260-4

R.T.: 7.733 min
Delta R.T.: -0.009 min
Response: 71044
Conc: 37.39 ng/ml

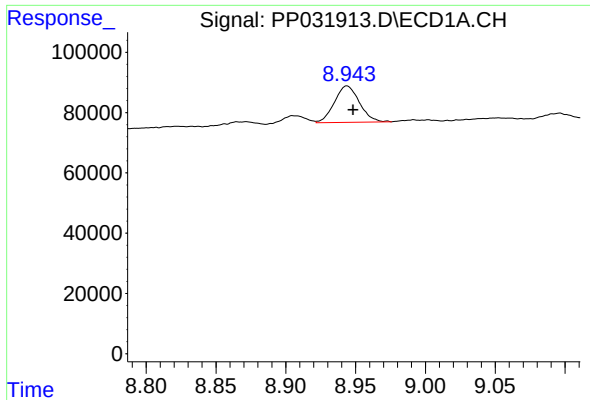


#35 AR-1260-5

R.T.: 8.944 min
Delta R.T.: -0.004 min
Response: 151205
Conc: 41.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
4S2-A-D-COMP

Manual Integrations
APPROVED

Ankita
12/9/2020 10:06:57 AM

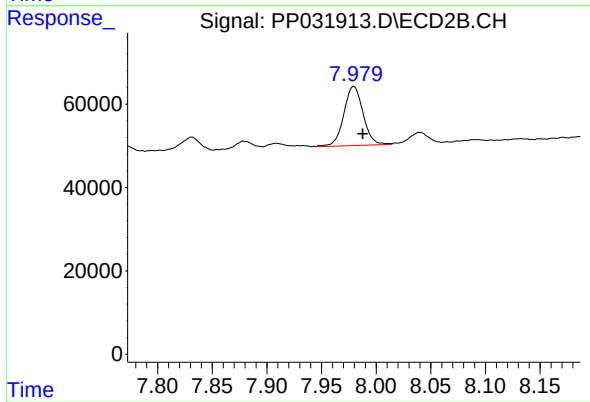

#35 AR-1260-5

R.T.: 7.979 min
Delta R.T.: -0.008 min
Response: 174297
Conc: 38.41 ng/ml