

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120821\
 Data File : PP041750.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Dec 2021 11:16
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 23:54:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.743	3.747	485113	684616	21.513	22.538
2) SA Decachlor...	10.634	9.002	469626	352768	21.810	22.825
Target Compounds						
8) L2 AR-1221-1	4.982f	0.000	13003	0	49.470	N.D. #
9) L2 AR-1221-2	5.094	4.096	7006	12278	37.386	44.601
10) L2 AR-1221-3	0.000	4.188	0	32711	N.D.	37.692 #
11) L3 AR-1232-1	0.000	4.188	0	32711	N.D.	44.159 #
24) L5 AR-1248-4	6.972f	0.000	2377	0	2.838	N.D. #
26) L6 AR-1254-1	6.972	0.000	2377	0	2.801	N.D. #
28) L6 AR-1254-3	7.594	0.000	7692	0	5.400	N.D. #
32) L7 AR-1260-2	8.031f	0.000	2770	0	2.204	N.D. #
33) L7 AR-1260-3	0.000	6.931	0	16123	N.D.	12.054 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120821\
Data File : PP041750.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Dec 2021 11:16
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 23:54:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

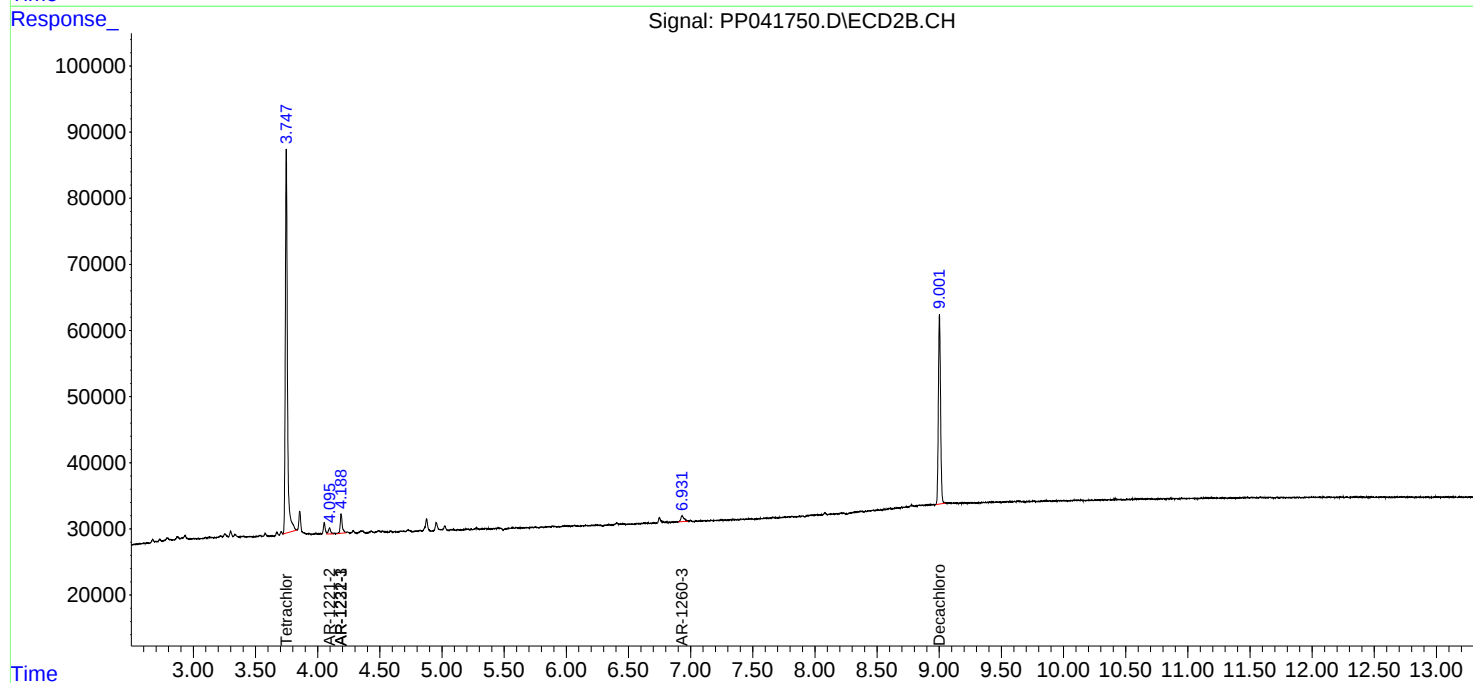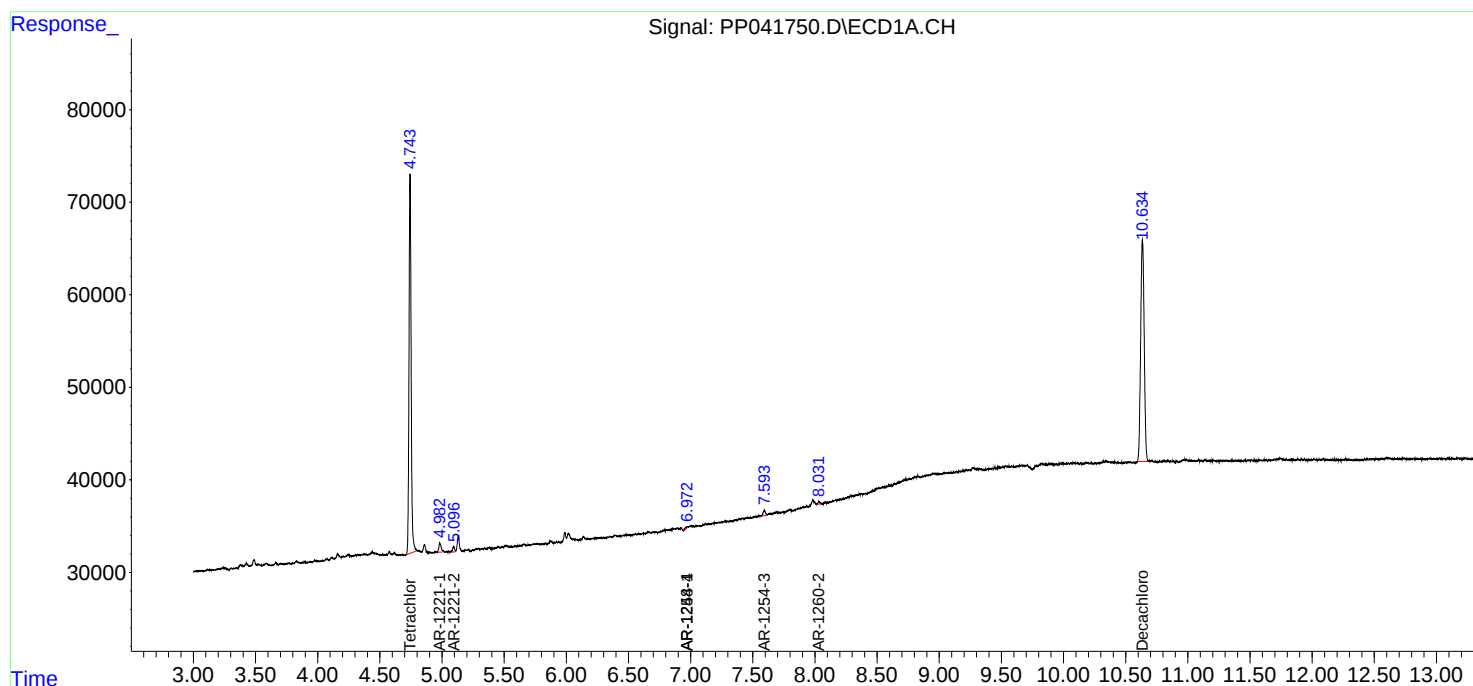


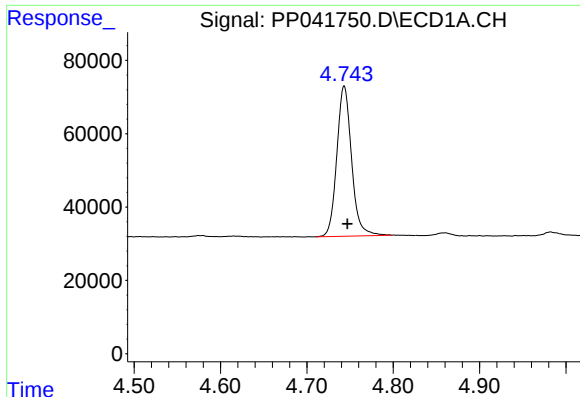

#1 Tetrachloro-m-xylene


R.T.: 4.743 min
Delta R.T.: -0.004 min
Response: 485113
Conc: 21.51 ng/ml

Instrument :
ECD_P
ClientSampleId :

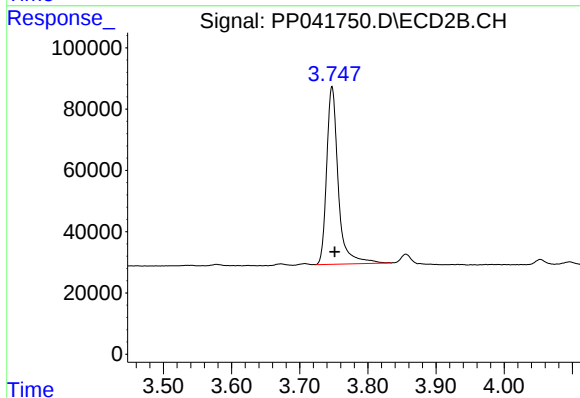


#1 Tetrachloro-m-xylene

R.T.: 3.747 min
Delta R.T.: -0.004 min
Response: 684616
Conc: 22.54 ng/ml

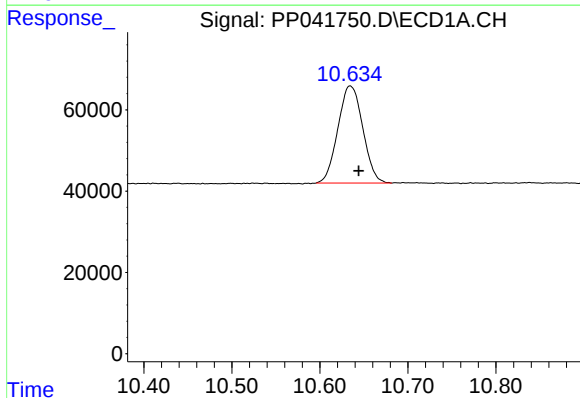


#2 Decachlorobiphenyl

R.T.: 10.634 min
Delta R.T.: -0.010 min
Response: 469626
Conc: 21.81 ng/ml

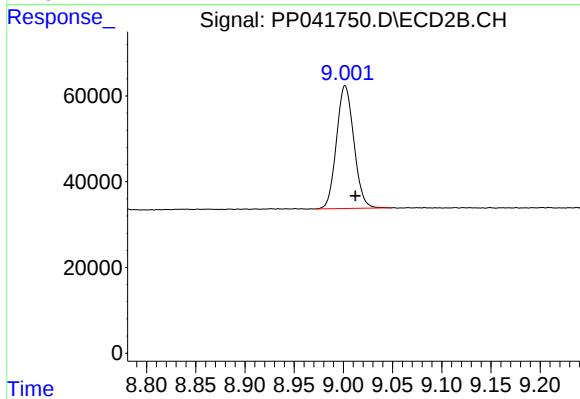

#2 Decachlorobiphenyl


R.T.: 9.002 min
Delta R.T.: -0.011 min
Response: 352768
Conc: 22.83 ng/ml

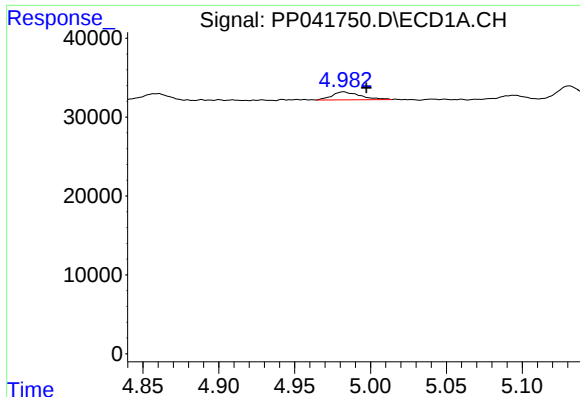

#8 AR-1221-1


R.T.: 4.982 min
Delta R.T.: -0.015 min
Response: 13003
Conc: 49.47 ng/ml

Instrument :
ECD_P
ClientSampleId :

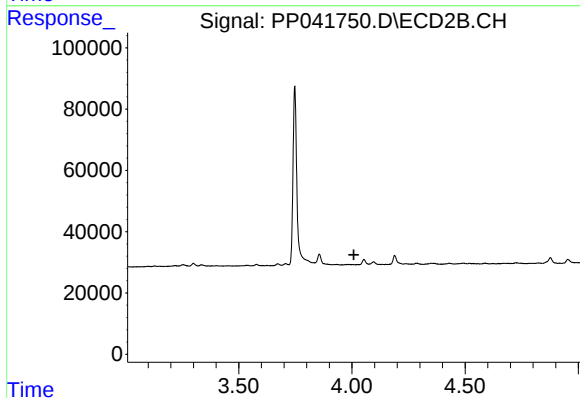


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.008 min
Response: 0
Conc: N.D.

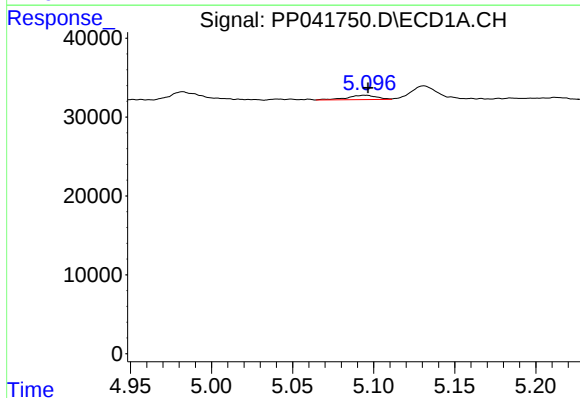


#9 AR-1221-2

R.T.: 5.094 min
Delta R.T.: -0.002 min
Response: 7006
Conc: 37.39 ng/ml

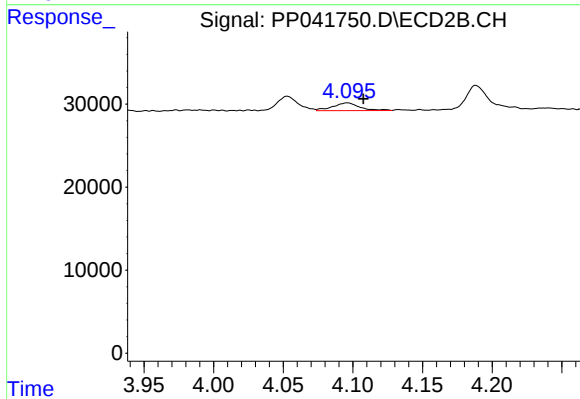

#9 AR-1221-2


R.T.: 4.096 min
Delta R.T.: -0.012 min
Response: 12278
Conc: 44.60 ng/ml

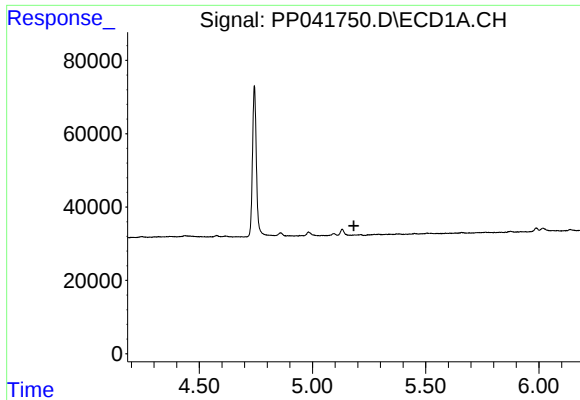

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

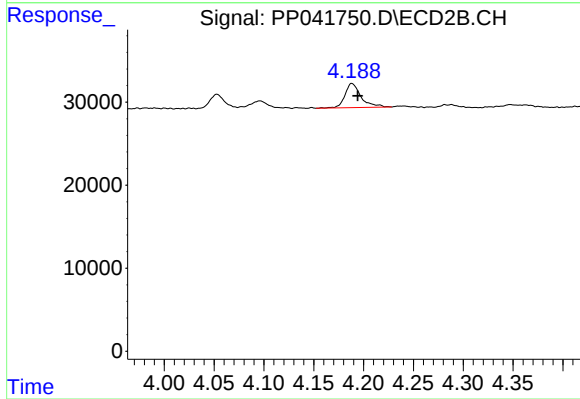


#10 AR-1221-3

R.T.: 4.188 min
Delta R.T.: -0.006 min
Response: 32711
Conc: 37.69 ng/ml

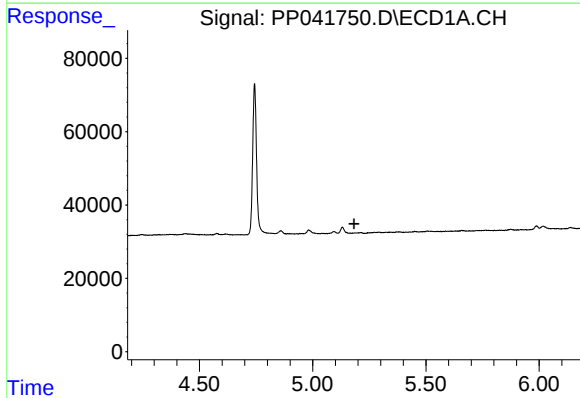


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.182 min
Response: 0
Conc: N.D.

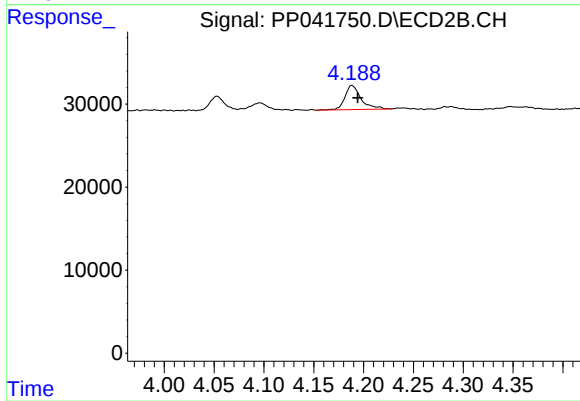

#11 AR-1232-1


R.T.: 4.188 min
Delta R.T.: -0.006 min
Response: 32711
Conc: 44.16 ng/ml

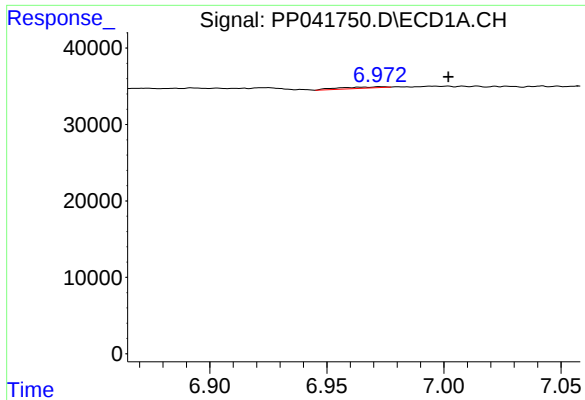

#24 AR-1248-4


R.T.: 6.972 min
Delta R.T.: -0.030 min
Response: 2377
Conc: 2.84 ng/ml

Instrument :
ECD_P
ClientSampleId :

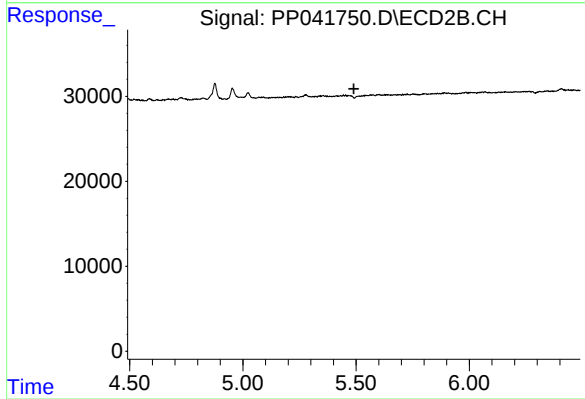


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.491 min
Response: 0
Conc: N.D.

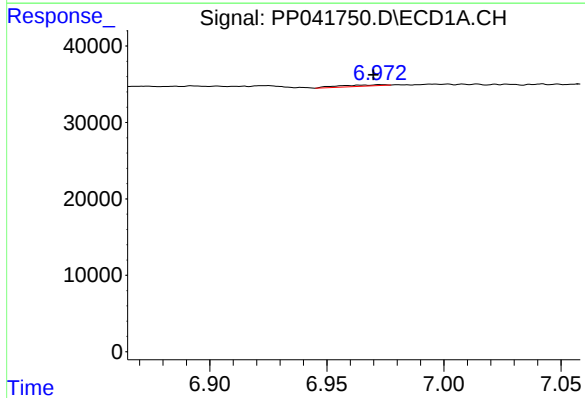


#26 AR-1254-1

R.T.: 6.972 min
Delta R.T.: 0.002 min
Response: 2377
Conc: 2.80 ng/ml

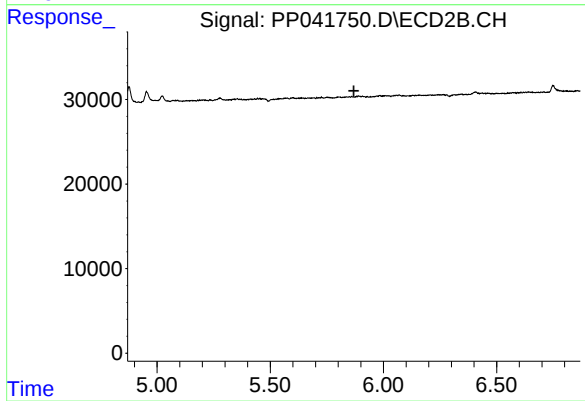

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.869 min
Response: 0
Conc: N.D.

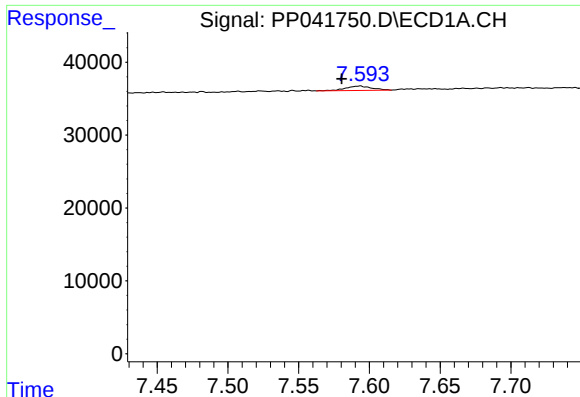

#28 AR-1254-3


R.T.: 7.594 min
Delta R.T.: 0.013 min
Response: 7692
Conc: 5.40 ng/ml

Instrument :
ECD_P
ClientSampleId :

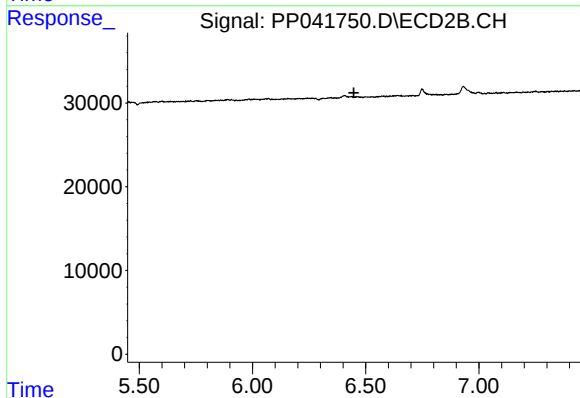


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.448 min
Response: 0
Conc: N.D.

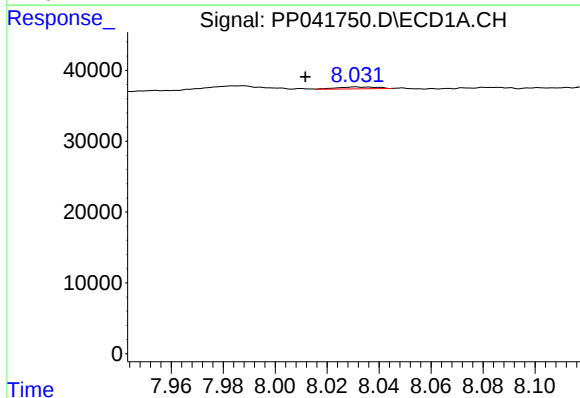


#32 AR-1260-2

R.T.: 8.031 min
Delta R.T.: 0.019 min
Response: 2770
Conc: 2.20 ng/ml

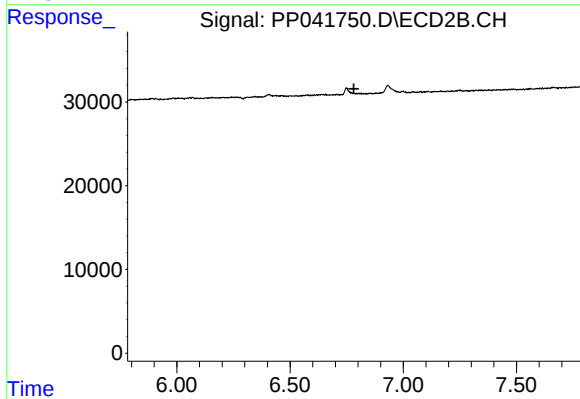

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.782 min
Response: 0
Conc: N.D.

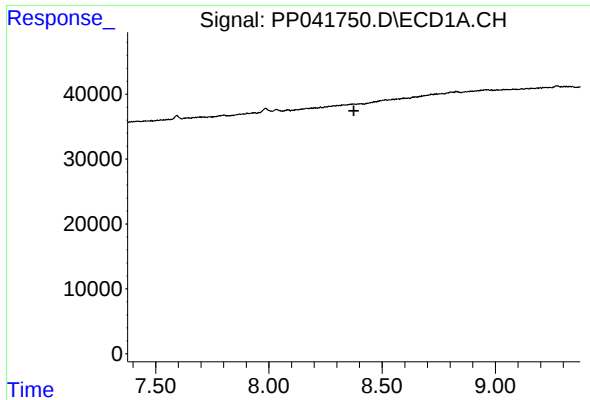

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

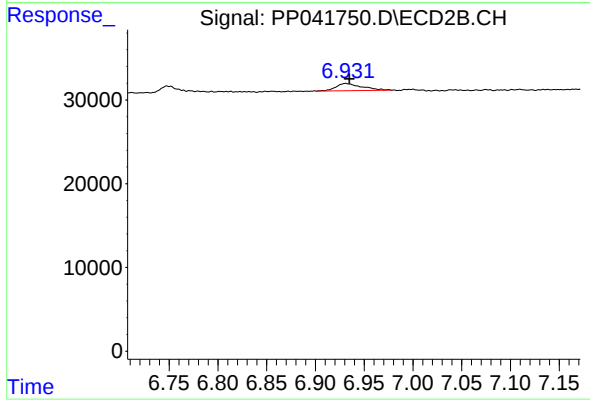

#33 AR-1260-3

R.T.: 6.931 min
Delta R.T.: -0.004 min
Response: 16123
Conc: 12.05 ng/ml