

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120821\
 Data File : PP041778.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Dec 2021 21:33
 Operator : AJ\MA
 Sample : M4965-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RED-CONCRETE-GRAB-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 00:04:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.744	3.747	475698	655256	21.096	21.572
2) SA Decachlor...	10.638	9.002	471916	332557	21.916	21.517

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120821\
Data File : PP041778.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Dec 2021 21:33
Operator : AJ\MA
Sample : M4965-06
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
RED-CONCRETE-GRAB-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 00:04:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

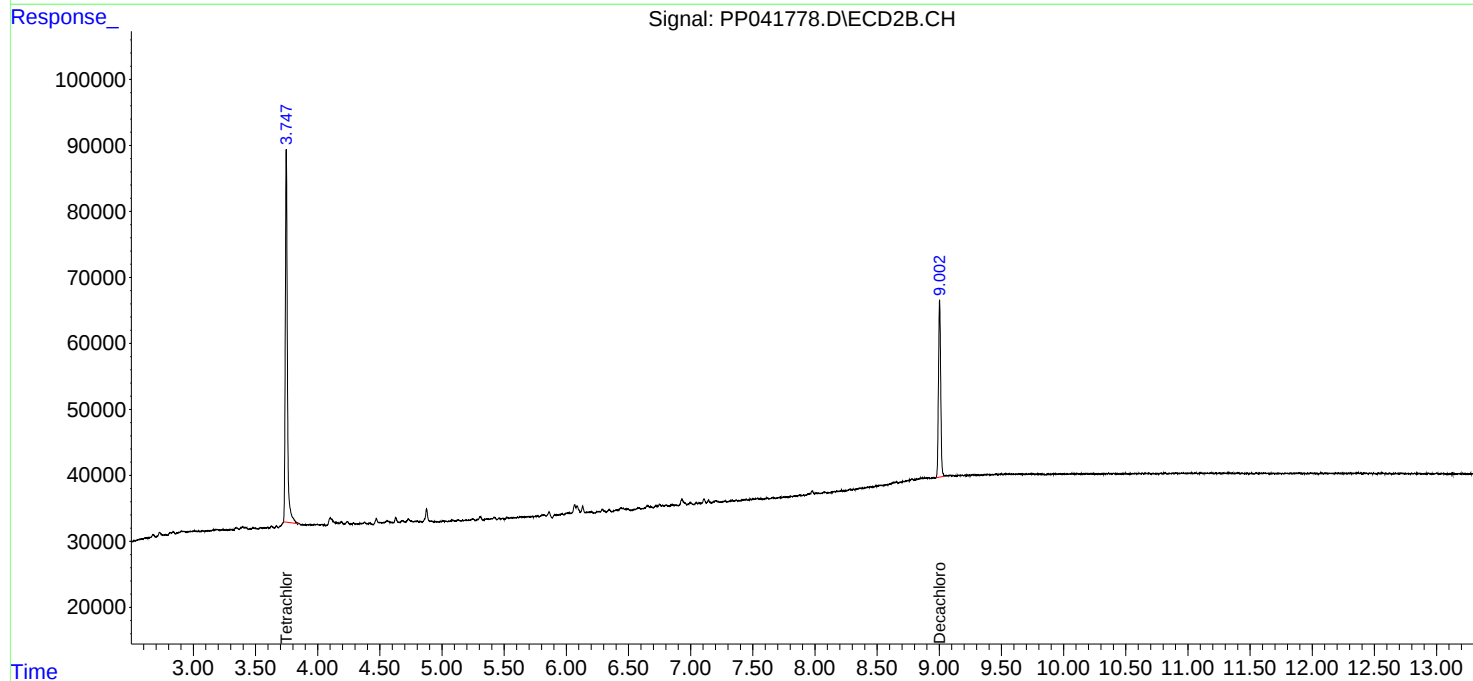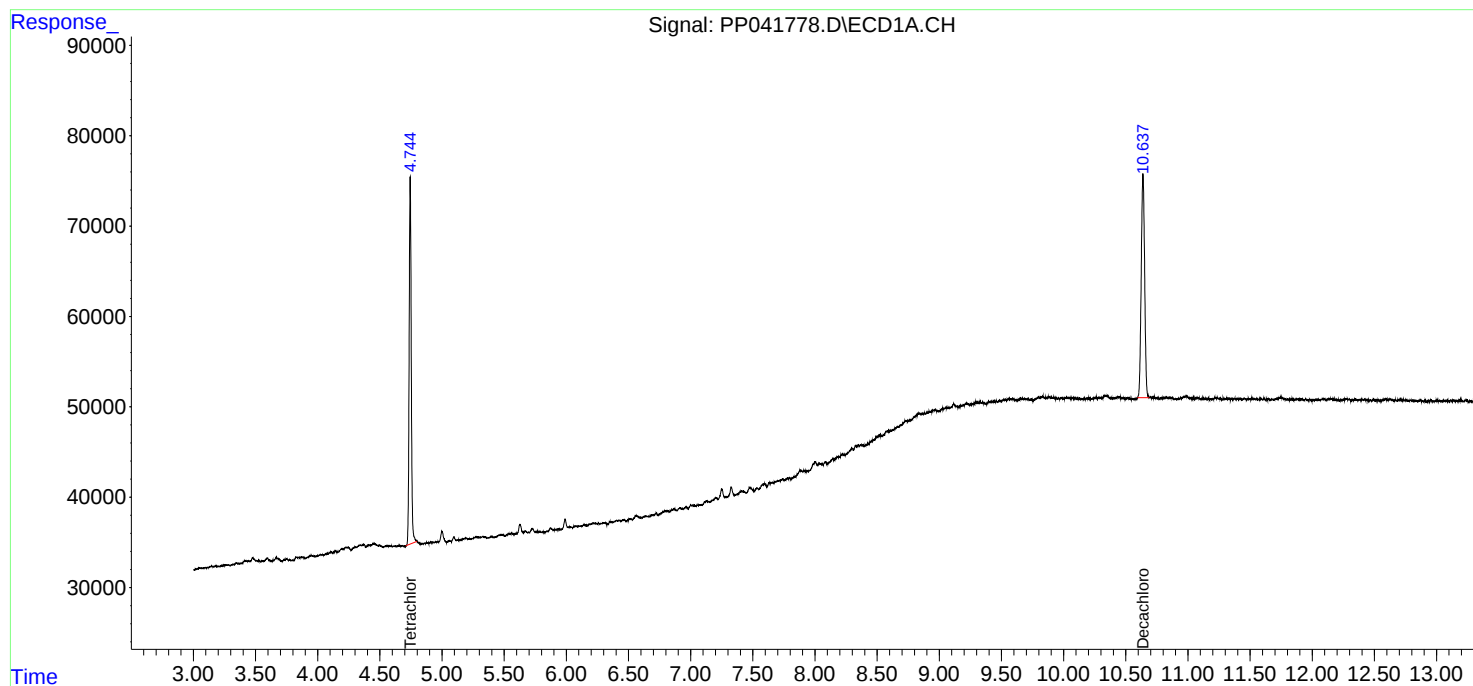


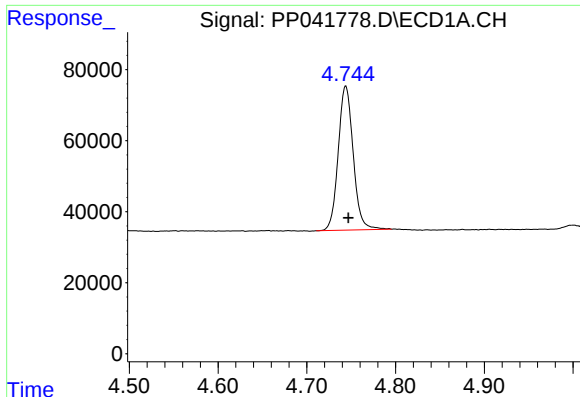

#1 Tetrachloro-m-xylene


R.T.: 4.744 min
Delta R.T.: -0.003 min
Response: 475698
Conc: 21.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
RED-CONCRETE-GRAB-2

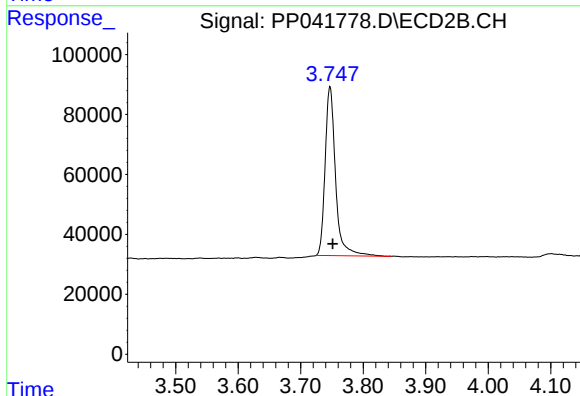


#1 Tetrachloro-m-xylene

R.T.: 3.747 min
Delta R.T.: -0.004 min
Response: 655256
Conc: 21.57 ng/ml

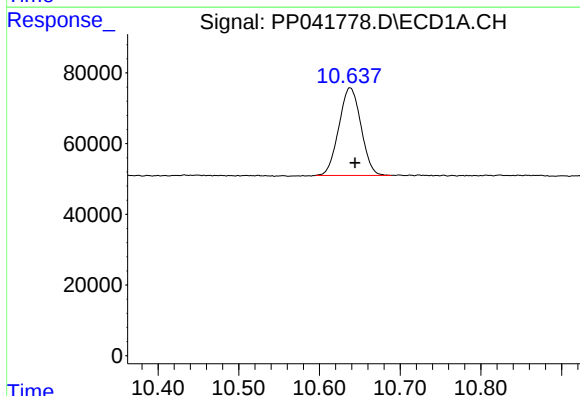

#2 Decachlorobiphenyl

R.T.: 10.638 min
Delta R.T.: -0.006 min
Response: 471916
Conc: 21.92 ng/ml

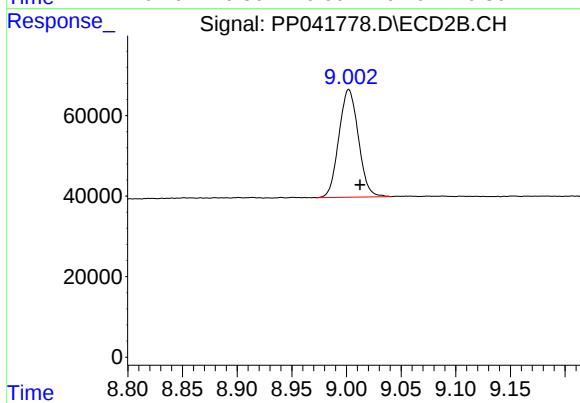

#2 Decachlorobiphenyl

R.T.: 9.002 min
Delta R.T.: -0.010 min
Response: 332557
Conc: 21.52 ng/ml