

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120821\
Data File : PP041784.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Dec 2021 23:13
Operator : AJ\MA
Sample : M4965-18
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BLUE-CONCRETE-GRAB-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 00:06:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.743	3.747	384542	529222	17.053	17.422
2) SA Decachlor...	10.637	9.002	379246	262597	17.613	16.991

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120821\
Data File : PP041784.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Dec 2021 23:13
Operator : AJ\MA
Sample : M4965-18
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BLUE-CONCRETE-GRAB-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 00:06:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

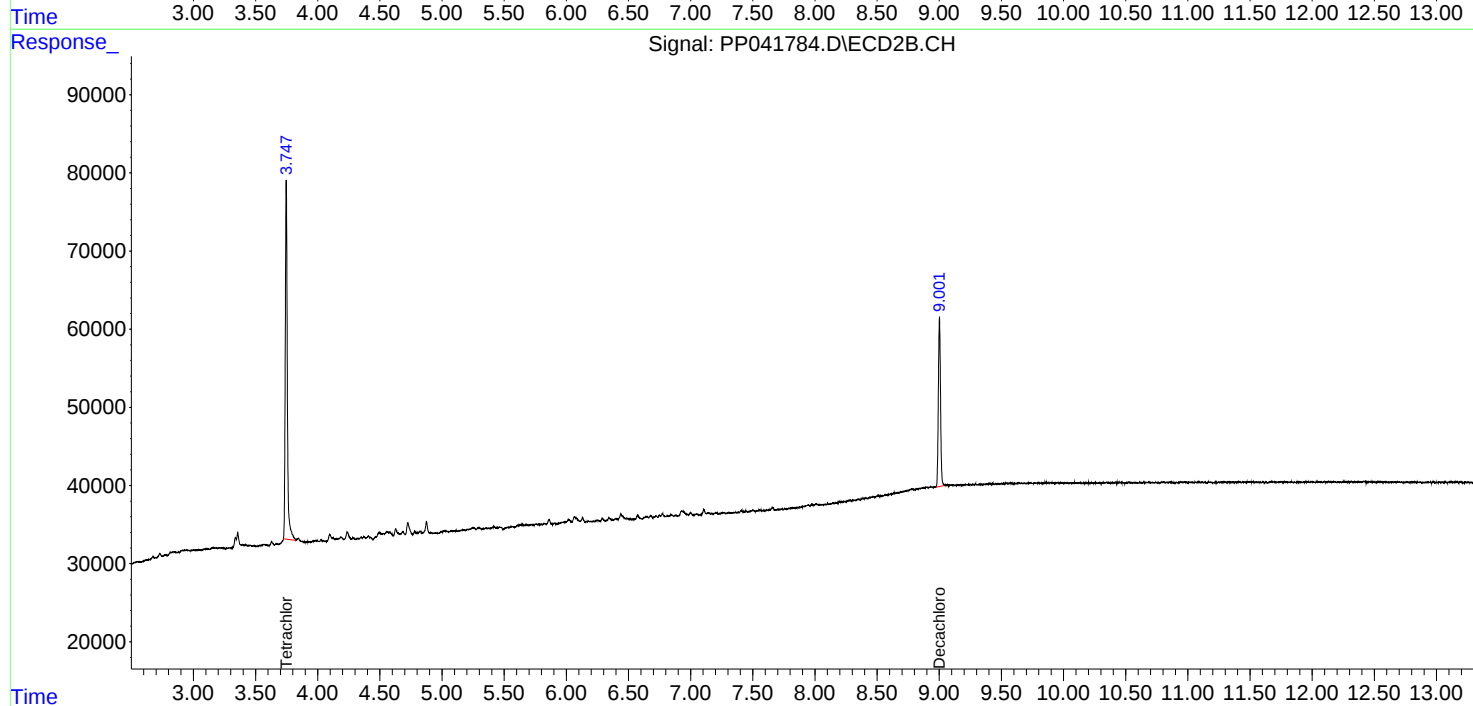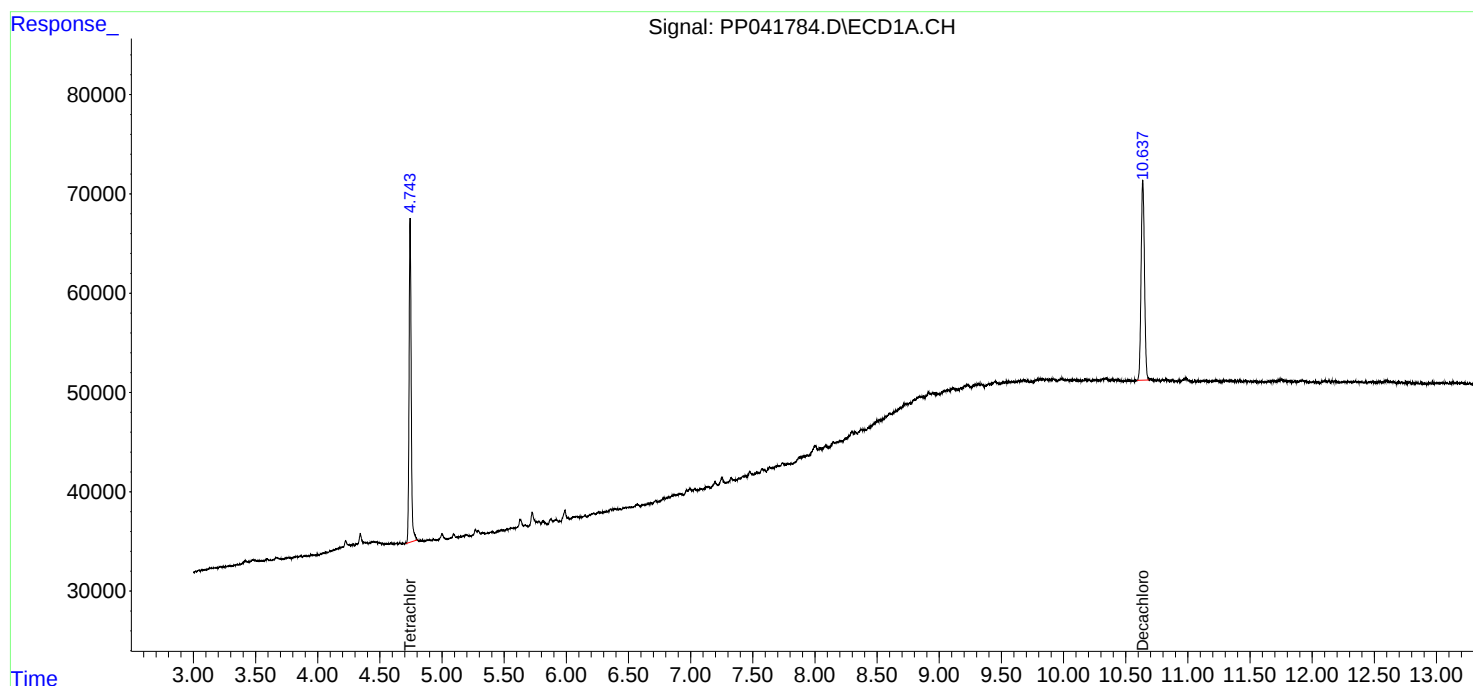

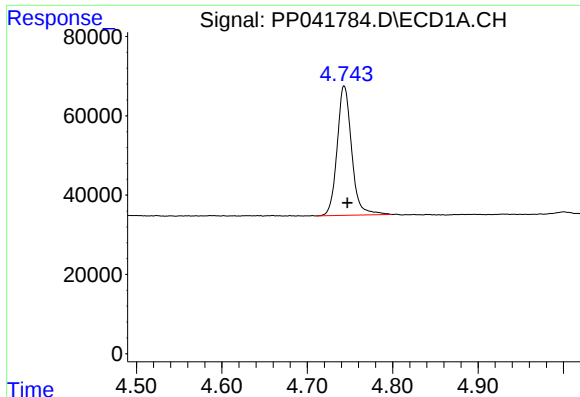

#1 Tetrachloro-m-xylene


R.T.: 4.743 min
Delta R.T.: -0.004 min
Response: 384542
Conc: 17.05 ng/ml

Instrument :

ECD_P


ClientSampleId :

BLUE-CONCRETE-GRAB-2

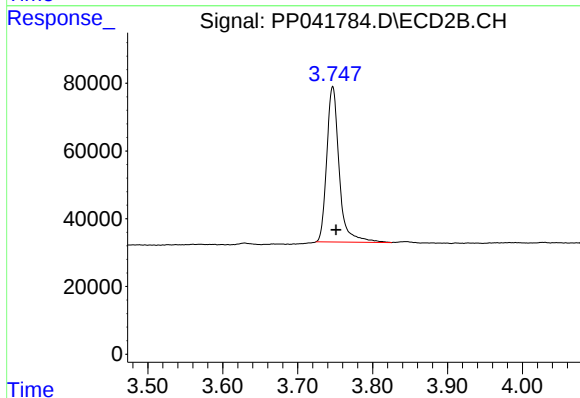


#1 Tetrachloro-m-xylene

R.T.: 3.747 min
Delta R.T.: -0.004 min
Response: 529222
Conc: 17.42 ng/ml

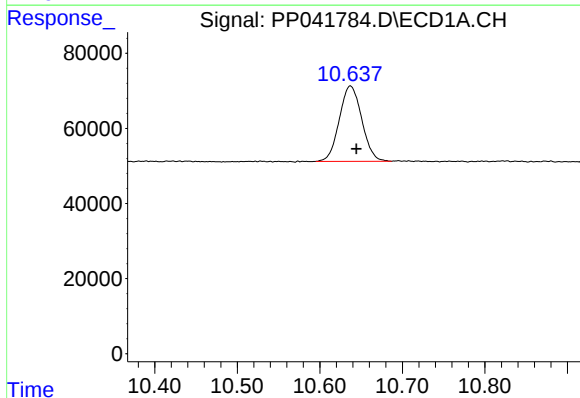

#2 Decachlorobiphenyl

R.T.: 10.637 min
Delta R.T.: -0.007 min
Response: 379246
Conc: 17.61 ng/ml

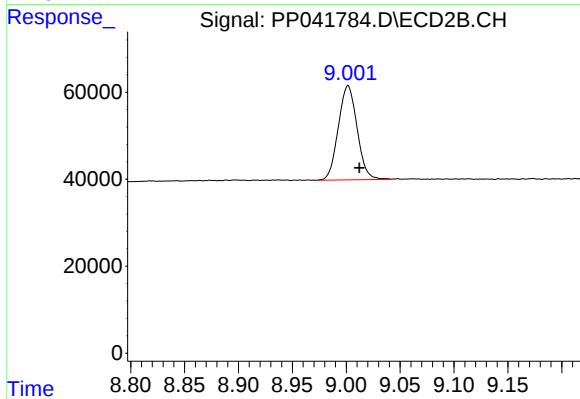

#2 Decachlorobiphenyl

R.T.: 9.002 min
Delta R.T.: -0.011 min
Response: 262597
Conc: 16.99 ng/ml