

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120821\
 Data File : PP041786.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Dec 2021 23:46
 Operator : AJ\MA
 Sample : M4965-23
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RED-WALL-CONCRETE-GRAB-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 00:07:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.743	3.747	461044	635729	20.446	20.929
2) SA Decachlor...	10.636	9.000	447204	308726	20.769	19.975

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120821\
Data File : PP041786.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Dec 2021 23:46
Operator : AJ\MA
Sample : M4965-23
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
RED-WALL-CONCRETE-GRAB-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 00:07:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

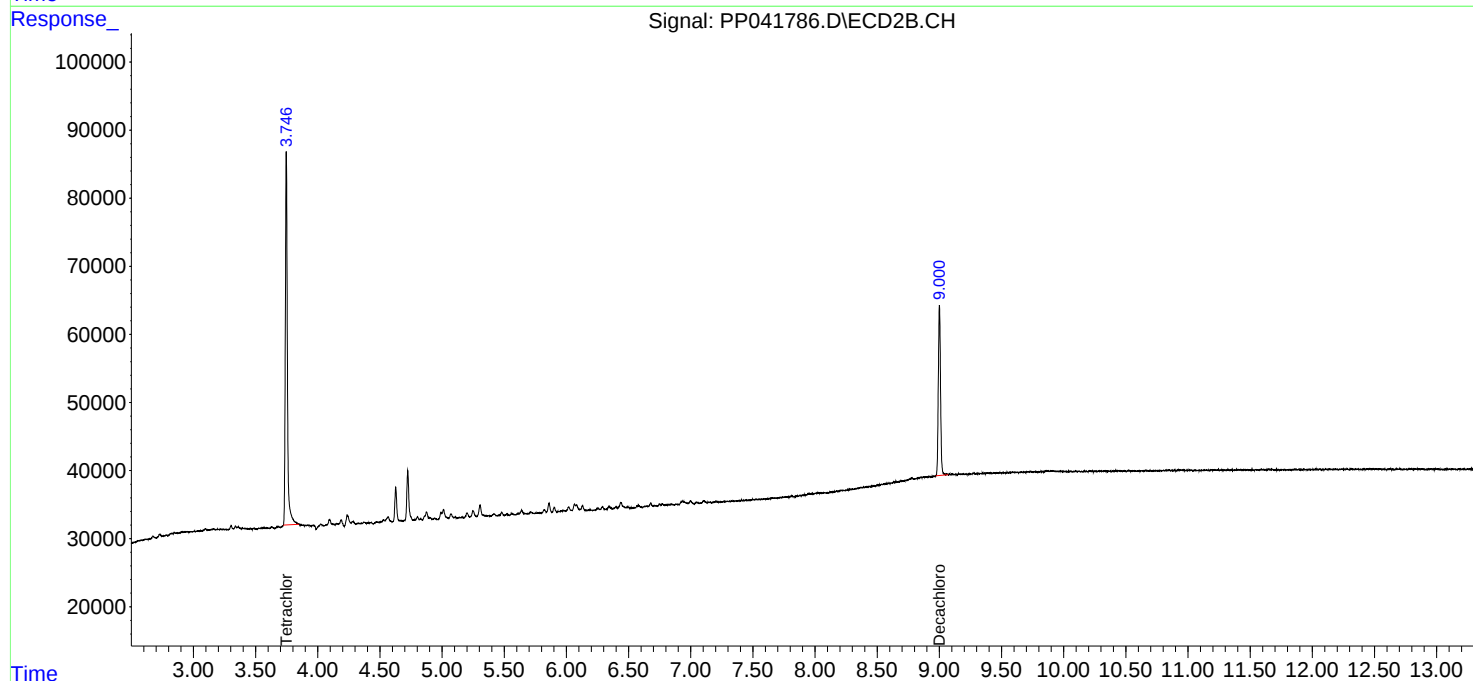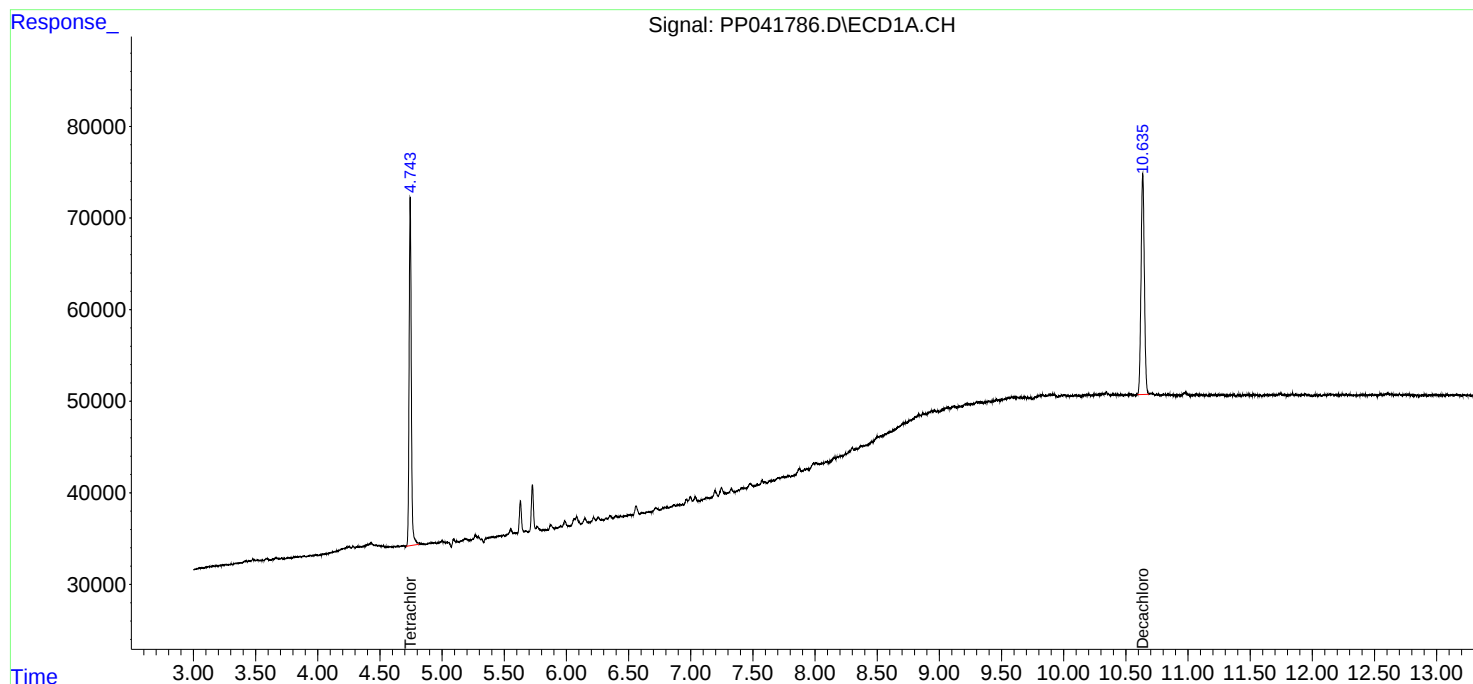


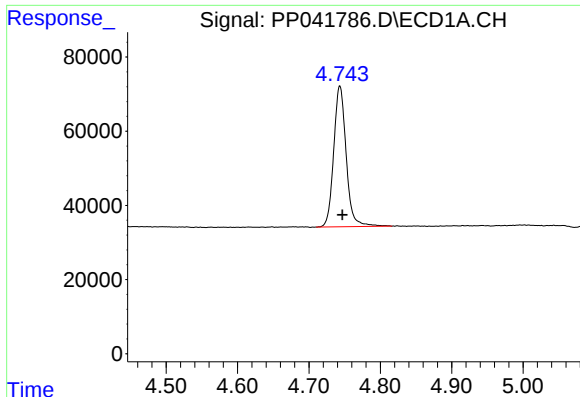

#1 Tetrachloro-m-xylene


R.T.: 4.743 min
Delta R.T.: -0.004 min
Response: 461044
Conc: 20.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
RED-WALL-CONCRETE-GRAB-1

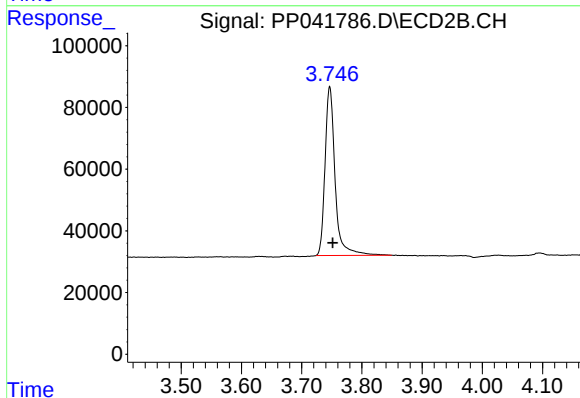


#1 Tetrachloro-m-xylene

R.T.: 3.747 min
Delta R.T.: -0.005 min
Response: 635729
Conc: 20.93 ng/ml

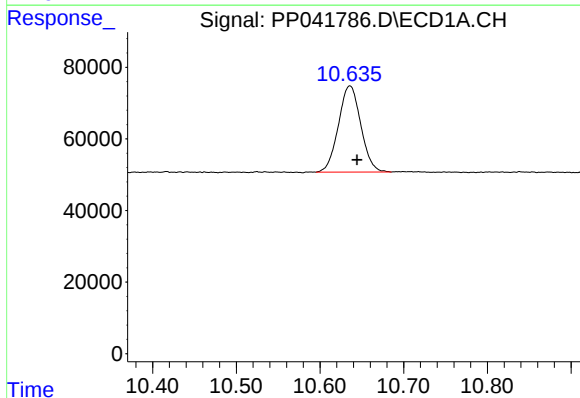

#2 Decachlorobiphenyl

R.T.: 10.636 min
Delta R.T.: -0.008 min
Response: 447204
Conc: 20.77 ng/ml

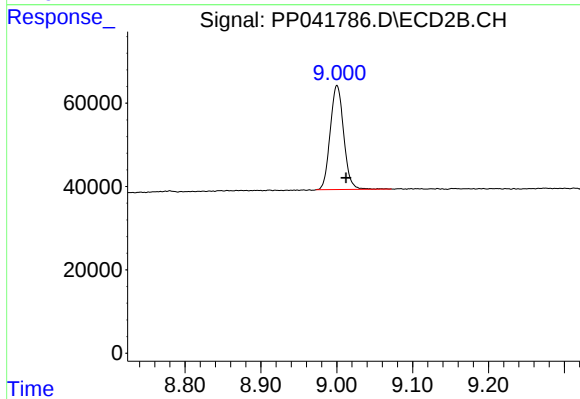

#2 Decachlorobiphenyl

R.T.: 9.000 min
Delta R.T.: -0.012 min
Response: 308726
Conc: 19.98 ng/ml