

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120821\
 Data File : PP041797.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Dec 2021 3:17
 Operator : AJ\MA
 Sample : M4965-34
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FLOORS-GRAB-1

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 12/09/2021
 Supervised By :mohammad ahmed 12/09/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 03:39:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.743	3.745	509208	671873	22.582	22.119
2)	SA Decachlor...	10.633	8.999	486593	345989	22.598	22.386
Target Compounds							
26)	L6 AR-1254-1	6.964	5.858	14359	23709	16.919m	17.032
27)	L6 AR-1254-2	7.194	6.018	27434	17658	20.824	14.786m#
28)	L6 AR-1254-3	7.573	6.436	30956	30755	21.733	17.373m
29)	L6 AR-1254-4	7.869	6.677	22996	15812	22.165	15.341m#
30)	L6 AR-1254-5	8.297	7.104	46237	88469	41.197	60.676 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120821\
Data File : PP041797.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Dec 2021 3:17
Operator : AJ\MA
Sample : M4965-34
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
FLOORS-GRAB-1


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/09/2021
Supervised By :mohammad ahmed 12/09/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 03:39:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

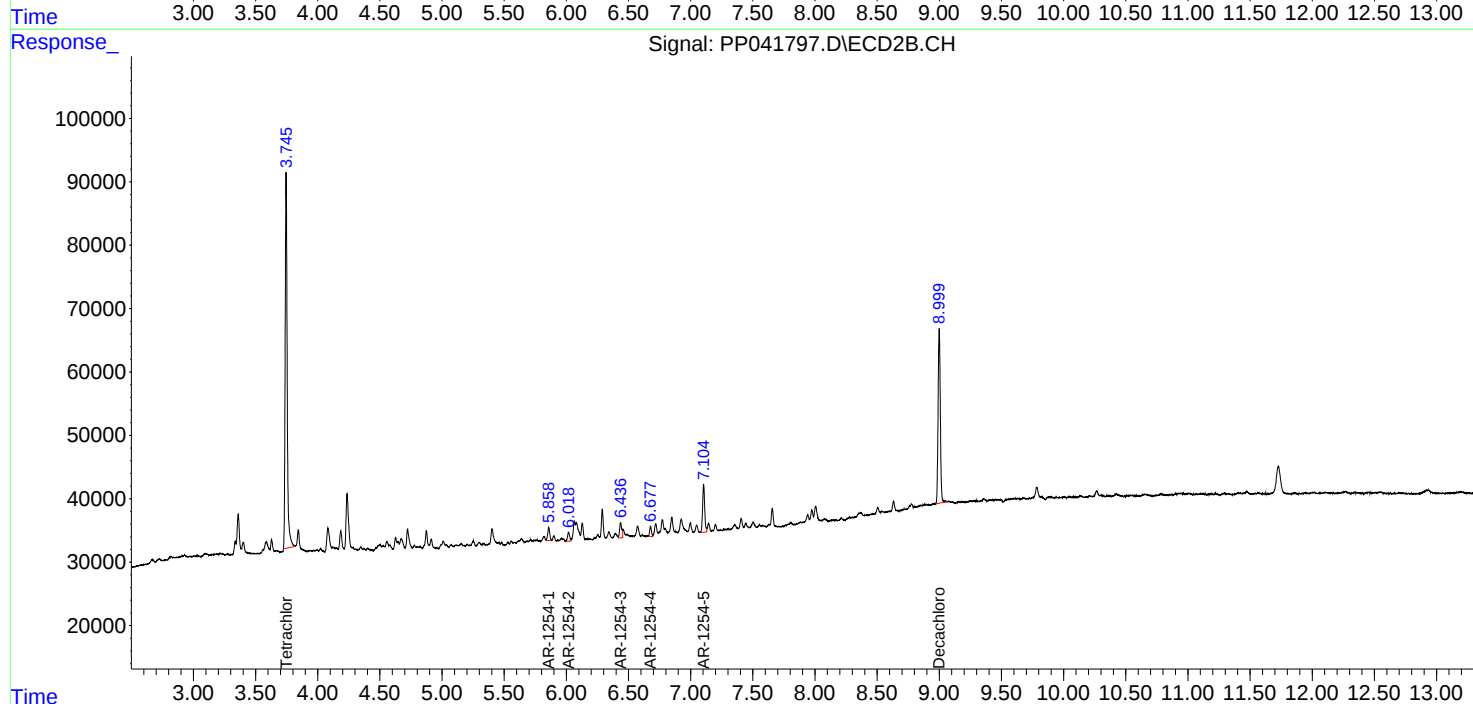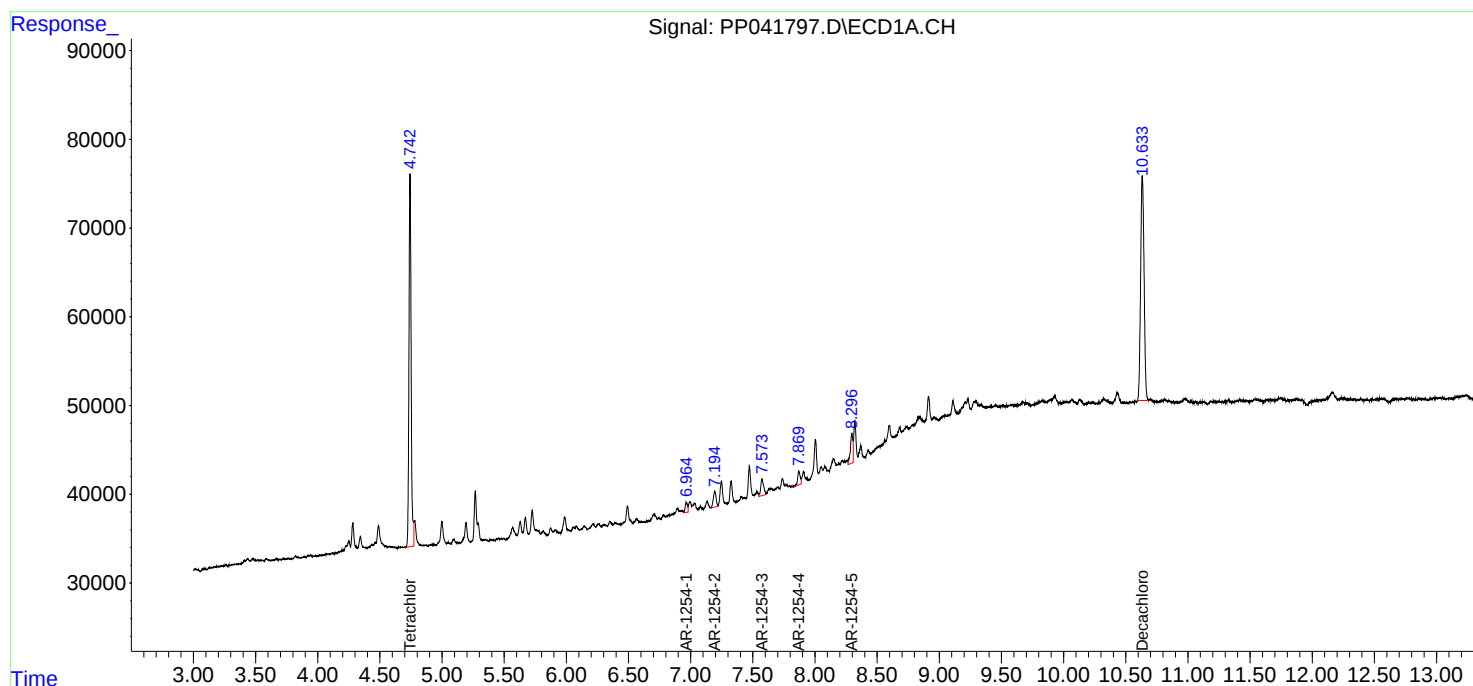

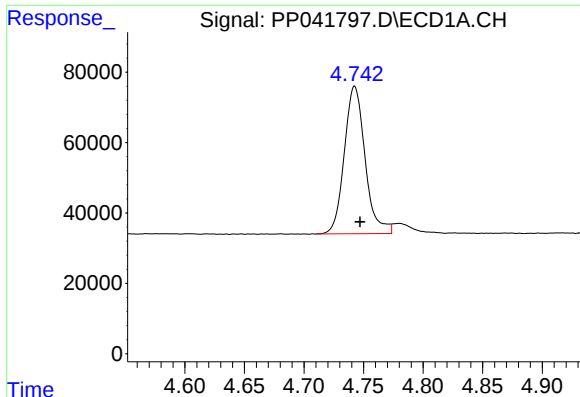


#1 Tetrachloro-m-xylene

R.T.: 4.743 min
Delta R.T.: -0.004 min
Response: 509208
Conc: 22.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
FLOORS-GRAB-1


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/09/2021
Supervised By :mohammad ahmed 12/09/2021

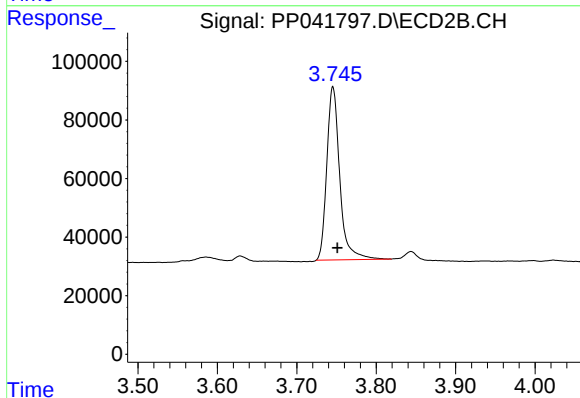


#1 Tetrachloro-m-xylene

R.T.: 3.745 min
Delta R.T.: -0.006 min
Response: 671873
Conc: 22.12 ng/ml

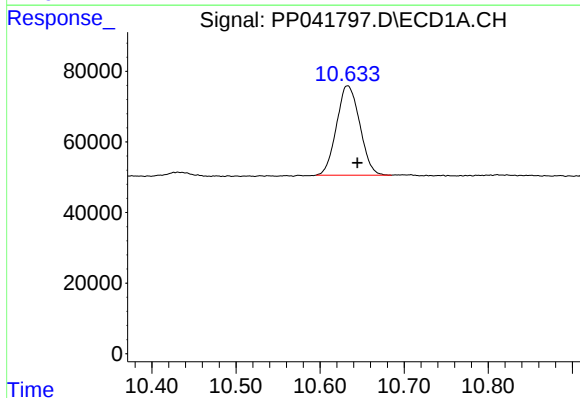


#2 Decachlorobiphenyl

R.T.: 10.633 min
Delta R.T.: -0.011 min
Response: 486593
Conc: 22.60 ng/ml

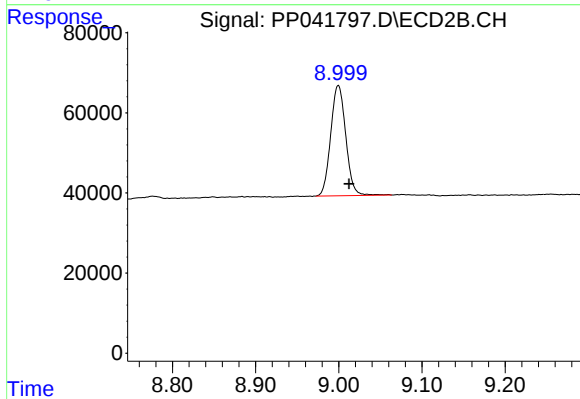

#2 Decachlorobiphenyl

R.T.: 8.999 min
Delta R.T.: -0.013 min
Response: 345989
Conc: 22.39 ng/ml

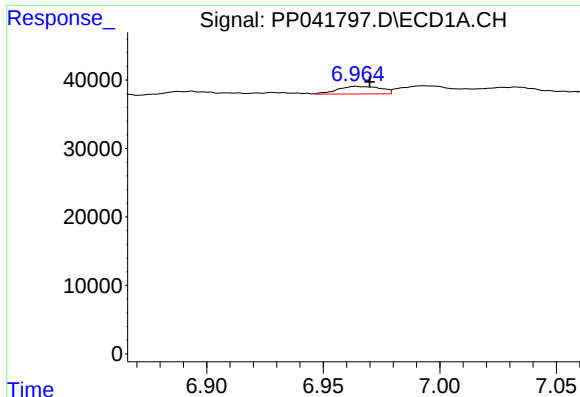


#26 AR-1254-1

R.T.: 6.964 min
Delta R.T.: -0.006 min
Response: 14359
Conc: 16.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
FLOORS-GRAB-1


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/09/2021
Supervised By :mohammad ahmed 12/09/2021

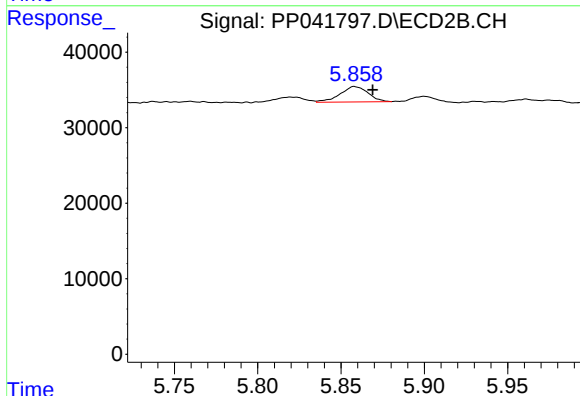


#26 AR-1254-1

R.T.: 5.858 min
Delta R.T.: -0.011 min
Response: 23709
Conc: 17.03 ng/ml

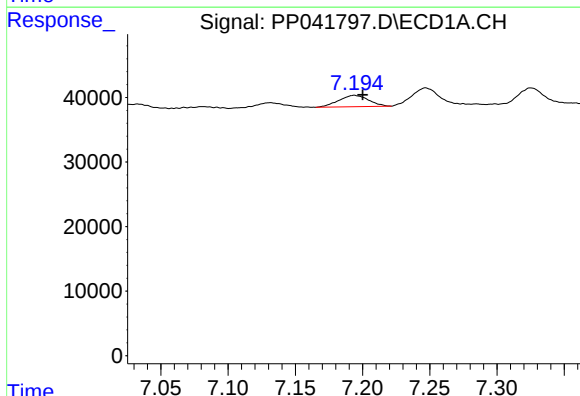


#27 AR-1254-2

R.T.: 7.194 min
Delta R.T.: -0.006 min
Response: 27434
Conc: 20.82 ng/ml

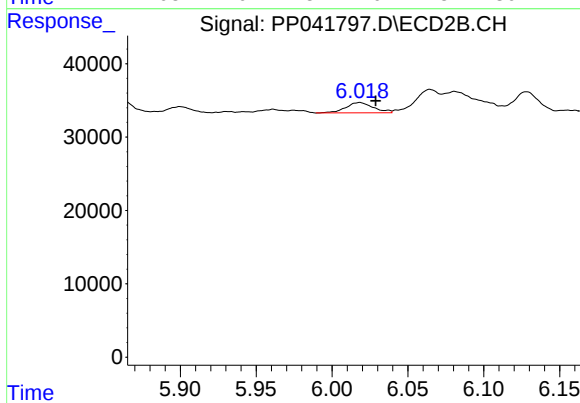

#27 AR-1254-2

R.T.: 6.018 min
Delta R.T.: -0.011 min
Response: 17658
Conc: 14.79 ng/ml m

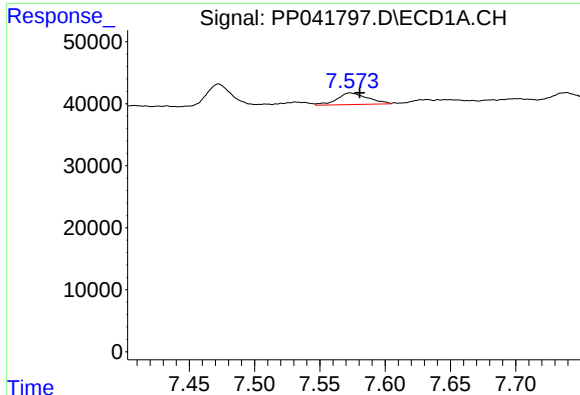


#28 AR-1254-3

R.T.: 7.573 min
Delta R.T.: -0.007 min
Response: 30956
Conc: 21.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
FLOORS-GRAB-1


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/09/2021
Supervised By :mohammad ahmed 12/09/2021

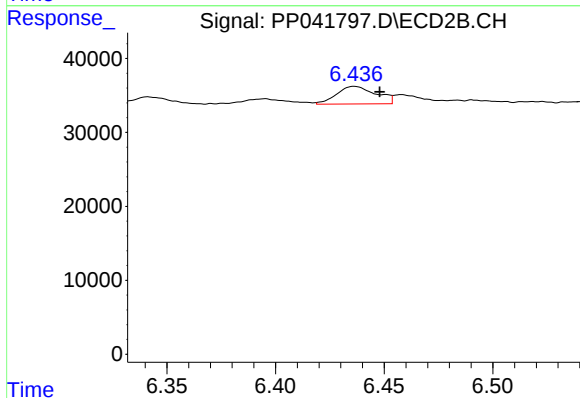


#28 AR-1254-3

R.T.: 6.436 min
Delta R.T.: -0.012 min
Response: 30755
Conc: 17.37 ng/ml m

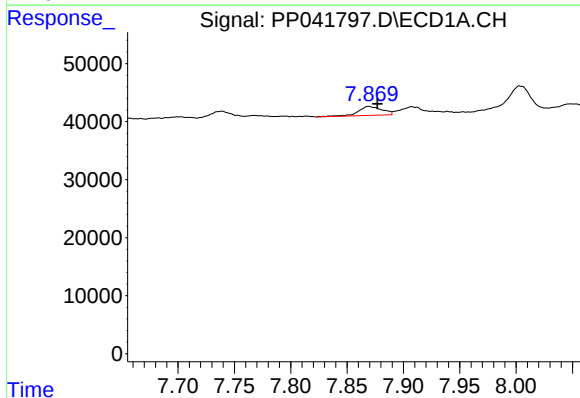


#29 AR-1254-4

R.T.: 7.869 min
Delta R.T.: -0.008 min
Response: 22996
Conc: 22.17 ng/ml

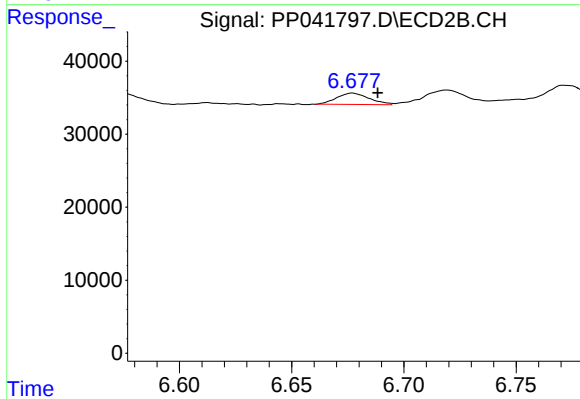

#29 AR-1254-4

R.T.: 6.677 min
Delta R.T.: -0.012 min
Response: 15812
Conc: 15.34 ng/ml m

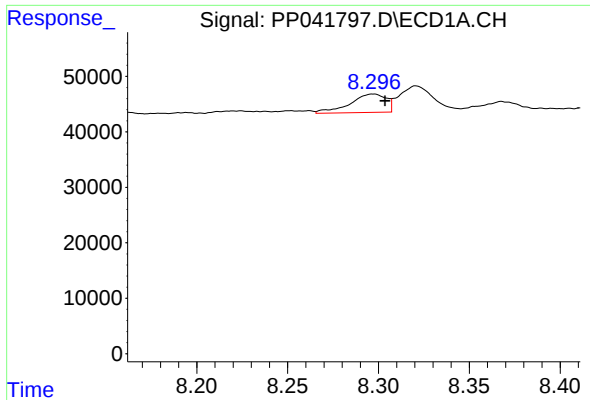


#30 AR-1254-5

R.T.: 8.297 min
Delta R.T.: -0.007 min
Response: 46237
Conc: 41.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
FLOORS-GRAB-1

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/09/2021
Supervised By :mohammad ahmed 12/09/2021

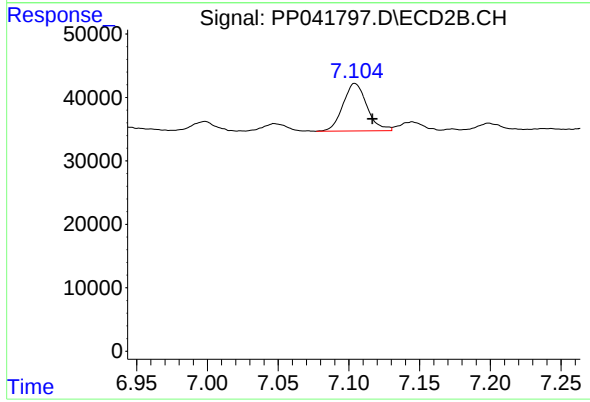

#30 AR-1254-5

R.T.: 7.104 min
Delta R.T.: -0.012 min
Response: 88469
Conc: 60.68 ng/ml