

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120821\
 Data File : PP041801.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Dec 2021 4:23
 Operator : AJ\MA
 Sample : M4965-38
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KEARNY-ST-SIDEWALK-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 06:09:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.743	3.746	458774	610291	20.345	20.091
2)	SA Decachlor...	10.635	9.000	439642	305101	20.418	19.741

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120821\
Data File : PP041801.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Dec 2021 4:23
Operator : AJ\MA
Sample : M4965-38
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
KEARNY-ST-SIDEWALK-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 06:09:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

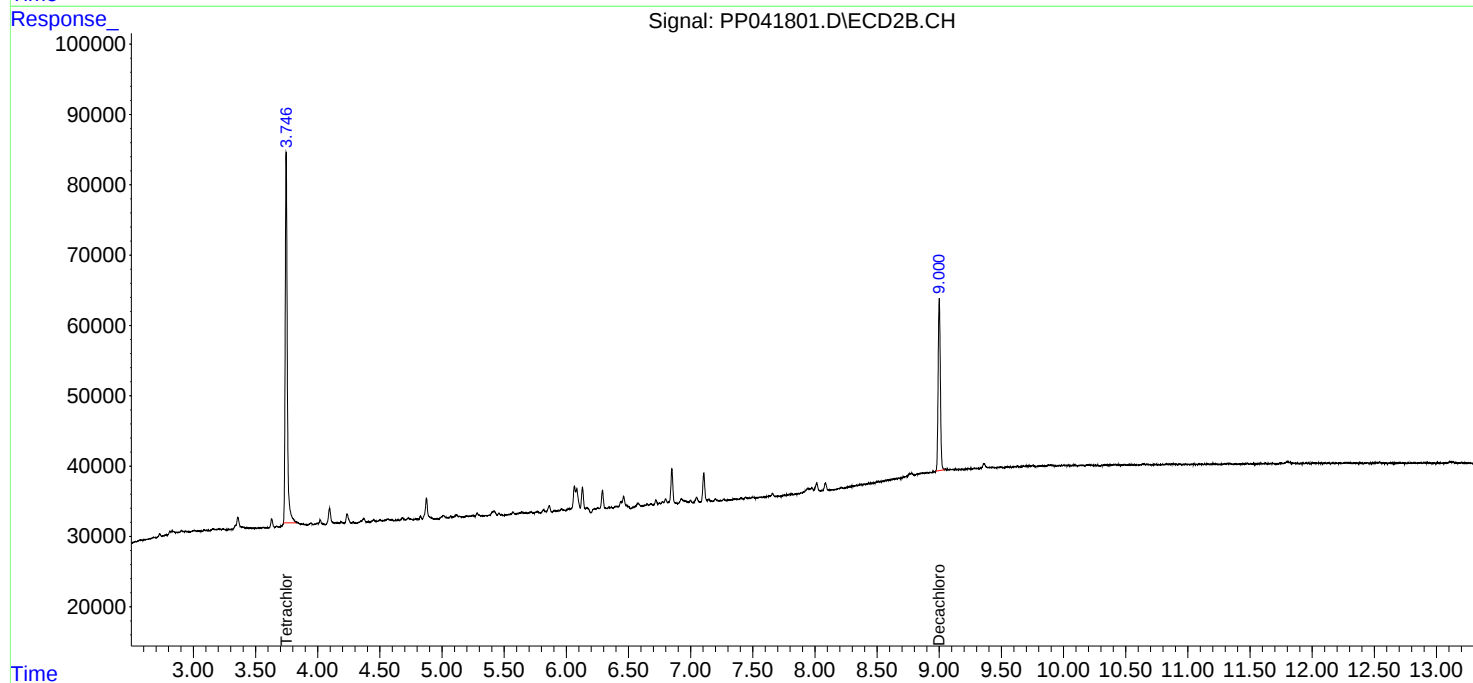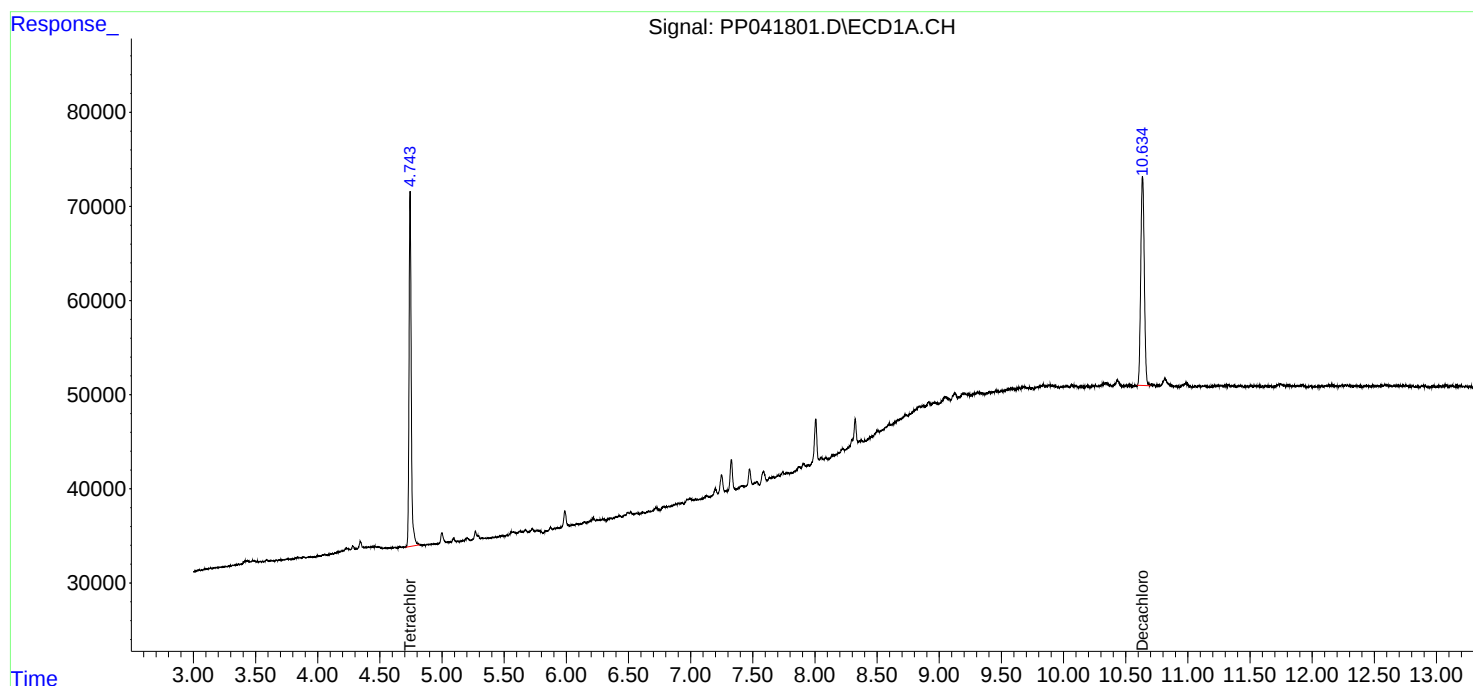


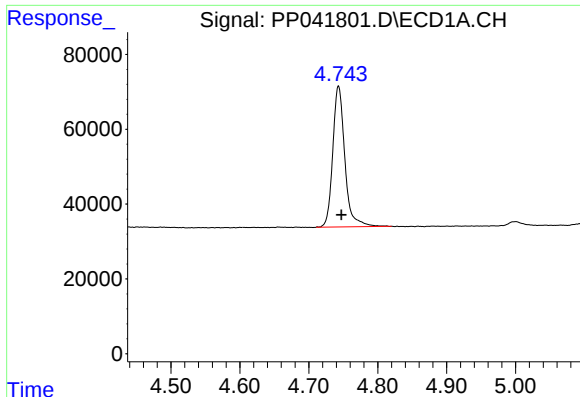

#1 Tetrachloro-m-xylene


R.T.: 4.743 min
Delta R.T.: -0.004 min
Response: 458774
Conc: 20.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
KEARNY-ST-SIDEWALK-1

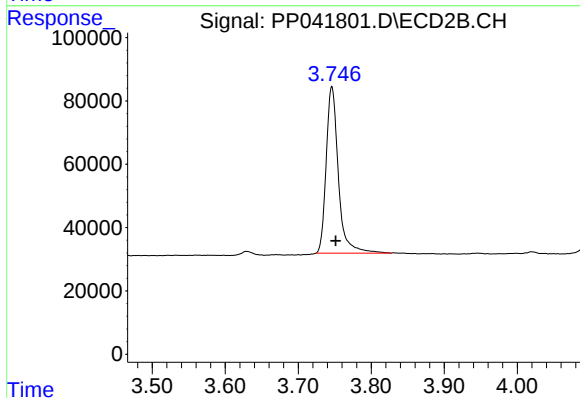


#1 Tetrachloro-m-xylene

R.T.: 3.746 min
Delta R.T.: -0.005 min
Response: 610291
Conc: 20.09 ng/ml

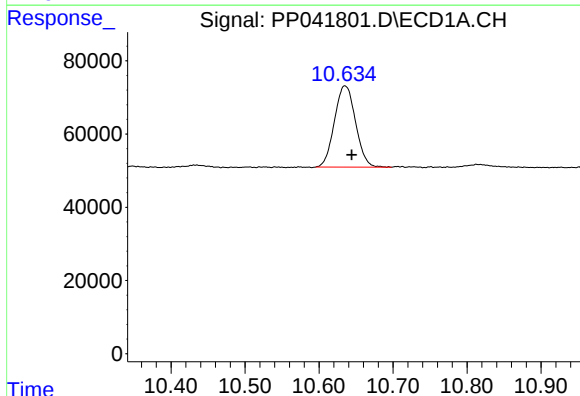

#2 Decachlorobiphenyl

R.T.: 10.635 min
Delta R.T.: -0.009 min
Response: 439642
Conc: 20.42 ng/ml

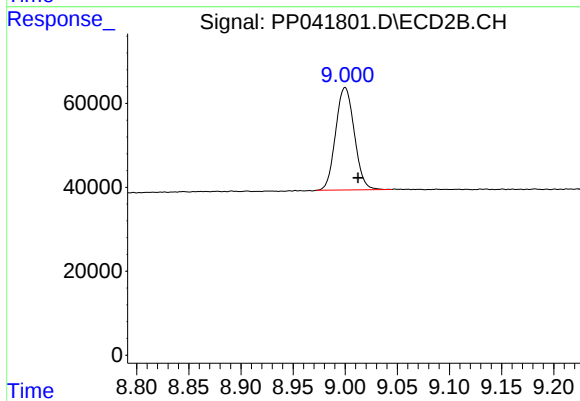

#2 Decachlorobiphenyl

R.T.: 9.000 min
Delta R.T.: -0.012 min
Response: 305101
Conc: 19.74 ng/ml