

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120823\
 Data File : PP062298.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2023 09:04
 Operator : YP\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 16:16:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 28 04:28:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
2)	SA Decachlor...	0.000	8.905f	0	43099	N.D.	0.021 #
Target Compounds							
10)	L2 AR-1221-3	4.800f	0.000	125311	0	3.149	N.D. #
11)	L3 AR-1232-1	4.800f	0.000	125311	0	3.765	N.D. #
20)	L4 AR-1242-5	6.540	0.000	83954	0	2.800	N.D. #
24)	L5 AR-1248-4	6.540f	0.000	83954	0	1.656	N.D. #
25)	L5 AR-1248-5	6.540	0.000	83954	0	1.625	N.D. #
27)	L6 AR-1254-2	6.679f	0.000	79132	0	0.949	N.D. #
34)	L7 AR-1260-4	8.062f	0.000	1702892	0	27.904	N.D. #
39)	L8 AR-1262-4	0.000	7.786f	0	194114	N.D.	1.077 #
42)	L9 AR-1268-2	0.000	7.786f	0	194114	N.D.	0.731 #
45)	L9 AR-1268-5	9.915	0.000	15653681	0	47.759	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120823\
Data File : PP062298.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2023 09:04
Operator : YP\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 16:16:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 28 04:28:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

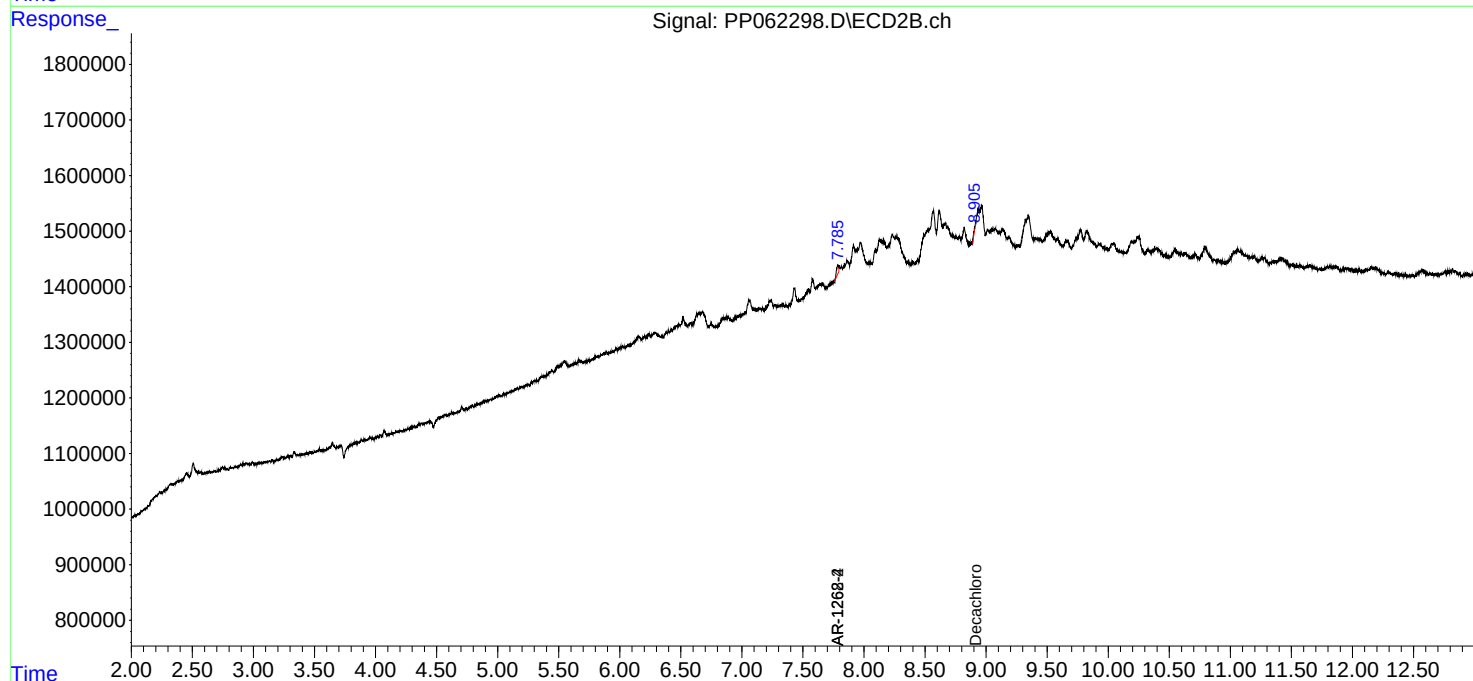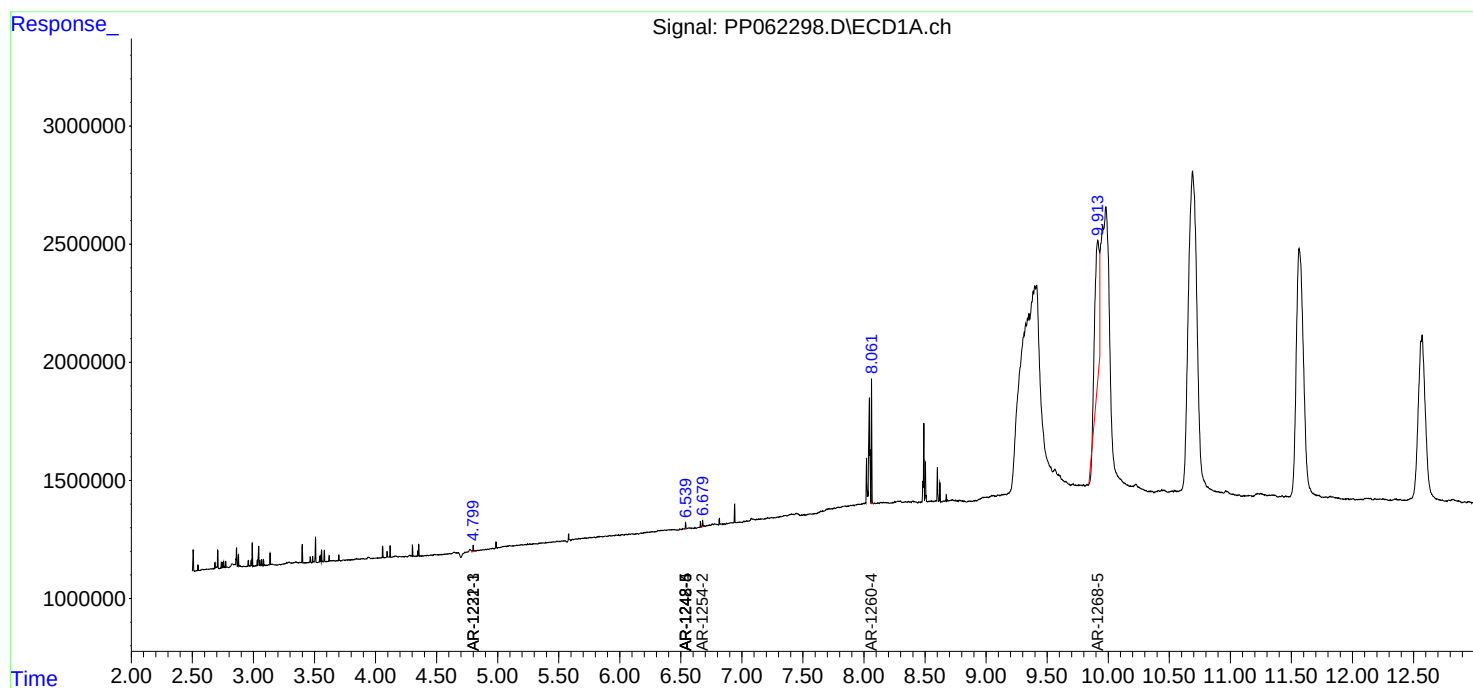


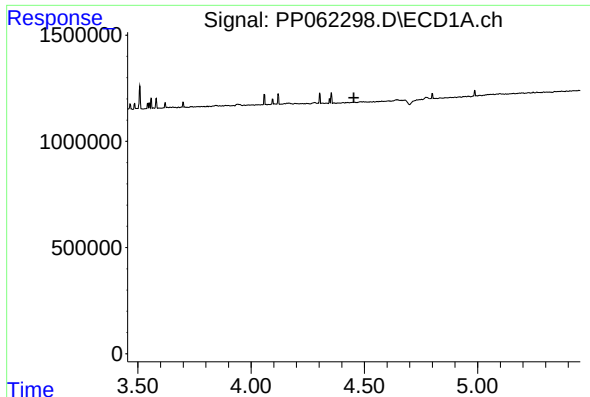

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.453 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

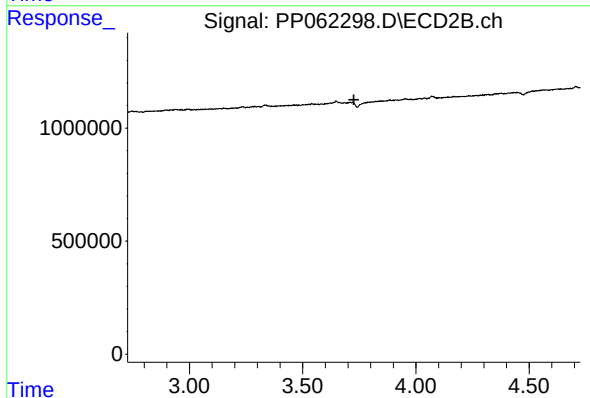


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.726 min
Response: 0
Conc: N.D.

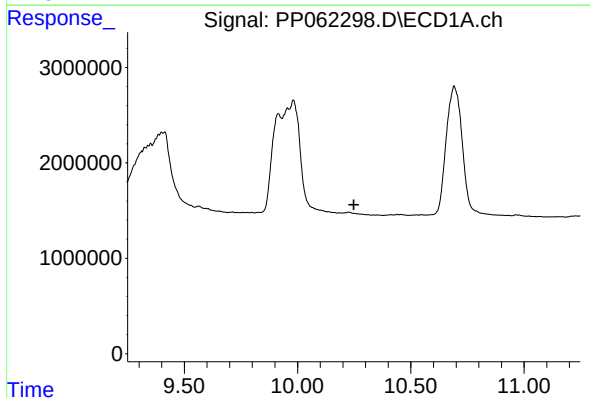


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.248 min
Response: 0
Conc: N.D.

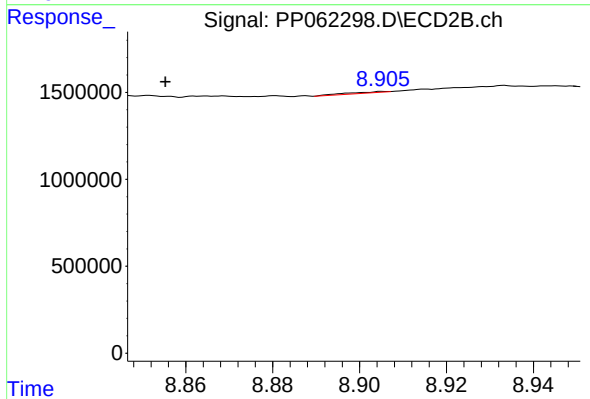

#2 Decachlorobiphenyl


R.T.: 8.905 min
Delta R.T.: 0.050 min
Response: 43099
Conc: 0.02 ng/ml

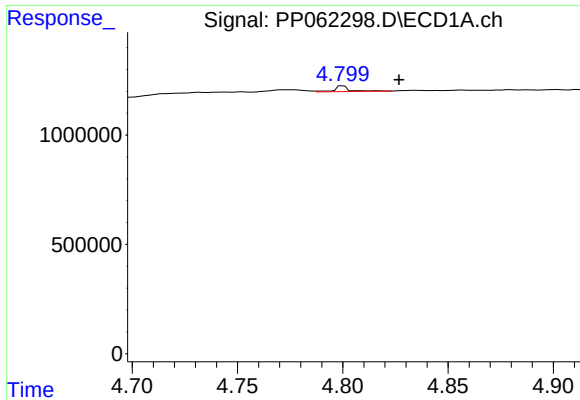

#10 AR-1221-3


R.T.: 4.800 min
Delta R.T.: -0.027 min
Response: 125311
Conc: 3.15 ng/ml

Instrument :
ECD_P
ClientSampleId :

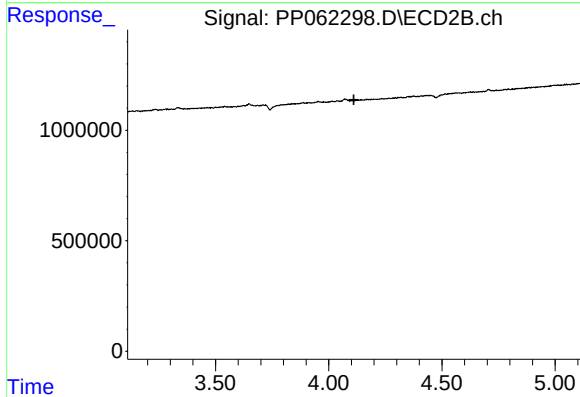


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.111 min
Response: 0
Conc: N.D.

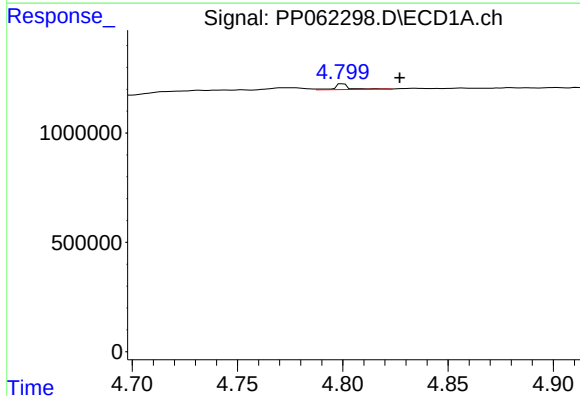


#11 AR-1232-1

R.T.: 4.800 min
Delta R.T.: -0.027 min
Response: 125311
Conc: 3.76 ng/ml

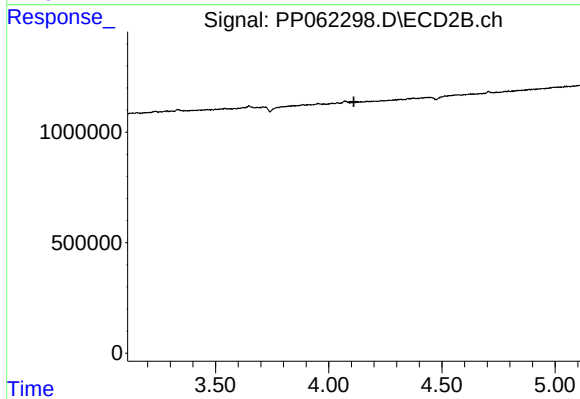

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 4.111 min
Response: 0
Conc: N.D.

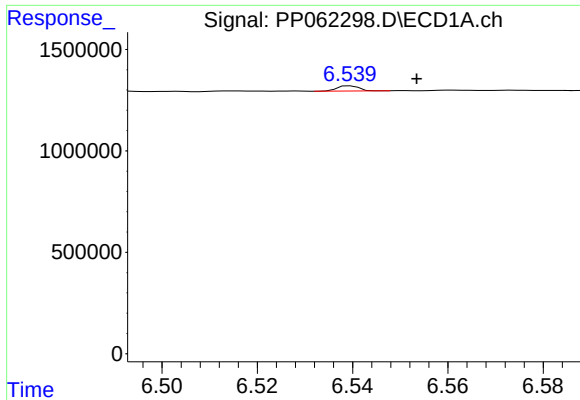

#20 AR-1242-5


R.T.: 6.540 min
Delta R.T.: -0.014 min
Response: 83954
Conc: 2.80 ng/ml

Instrument :
ECD_P
ClientSampleId :

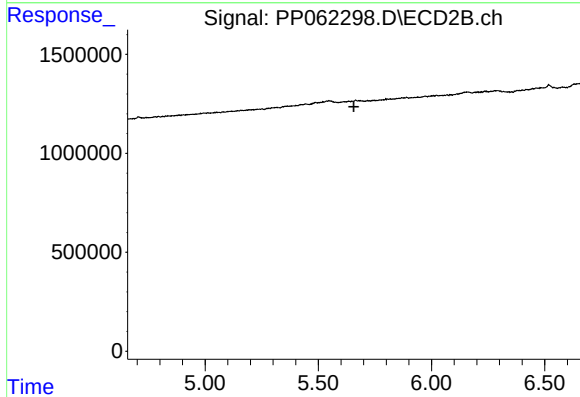


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 5.657 min
Response: 0
Conc: N.D.

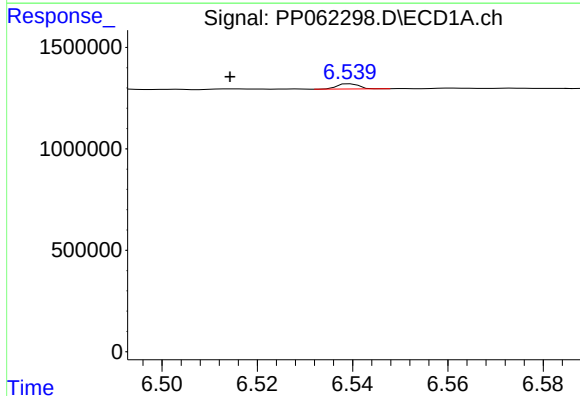


#24 AR-1248-4

R.T.: 6.540 min
Delta R.T.: 0.026 min
Response: 83954
Conc: 1.66 ng/ml

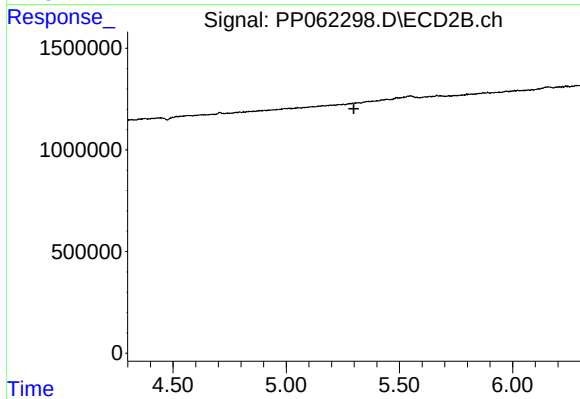

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.299 min
Response: 0
Conc: N.D.

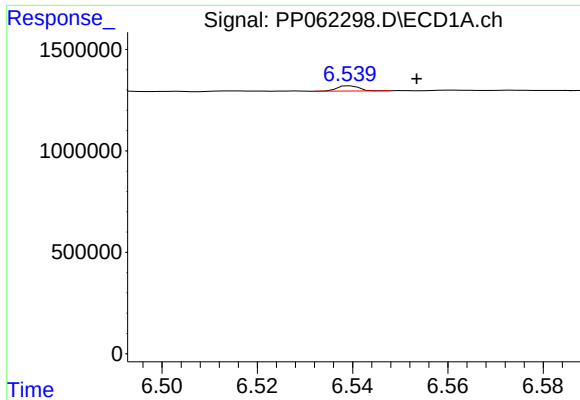

#25 AR-1248-5


R.T.: 6.540 min
Delta R.T.: -0.014 min
Response: 83954
Conc: 1.62 ng/ml

Instrument :
ECD_P
ClientSampleId :

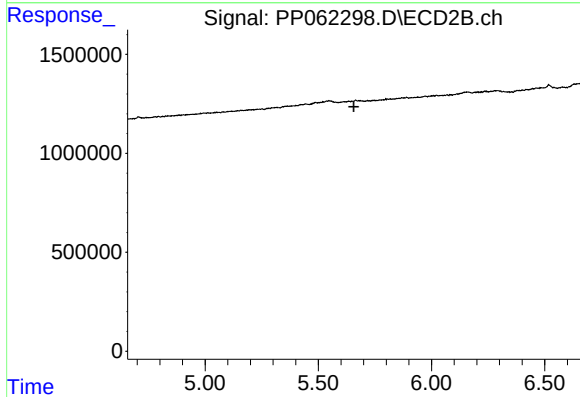


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.657 min
Response: 0
Conc: N.D.

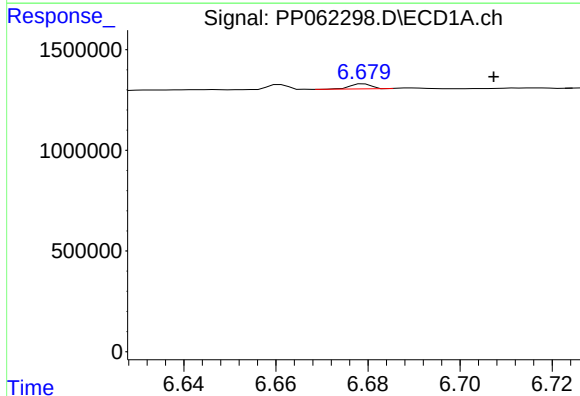


#27 AR-1254-2

R.T.: 6.679 min
Delta R.T.: -0.028 min
Response: 79132
Conc: 0.95 ng/ml

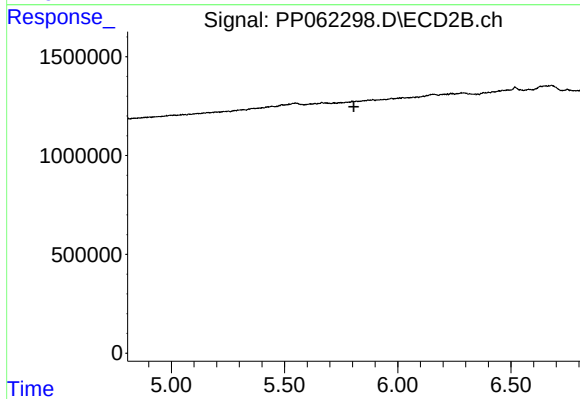

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 5.806 min
Response: 0
Conc: N.D.

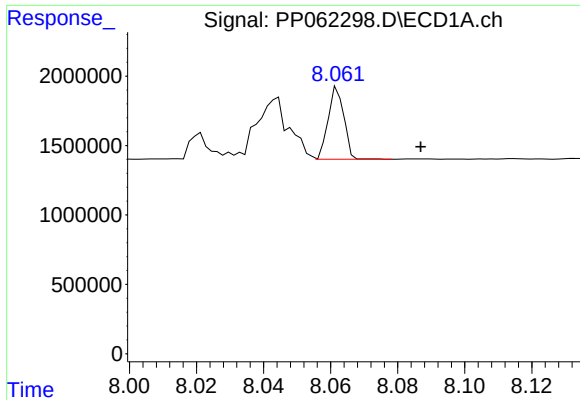

#34 AR-1260-4


R.T.: 8.062 min
Delta R.T.: -0.025 min
Response: 1702892
Conc: 27.90 ng/ml

Instrument :
ECD_P
ClientSampleId :

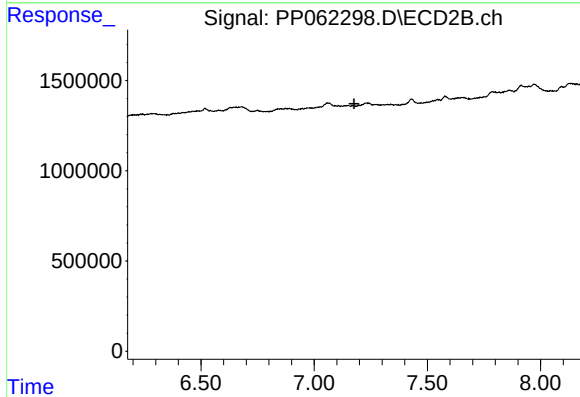


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.176 min
Response: 0
Conc: N.D.

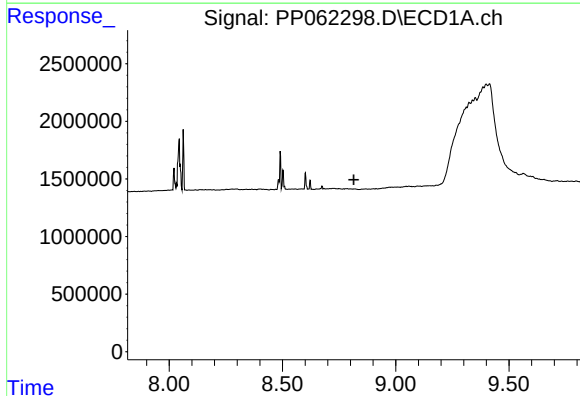


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.815 min
Response: 0
Conc: N.D.

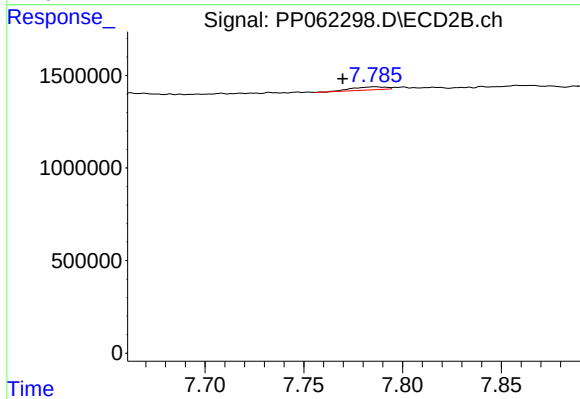

#39 AR-1262-4


R.T.: 7.786 min
Delta R.T.: 0.016 min
Response: 194114
Conc: 1.08 ng/ml

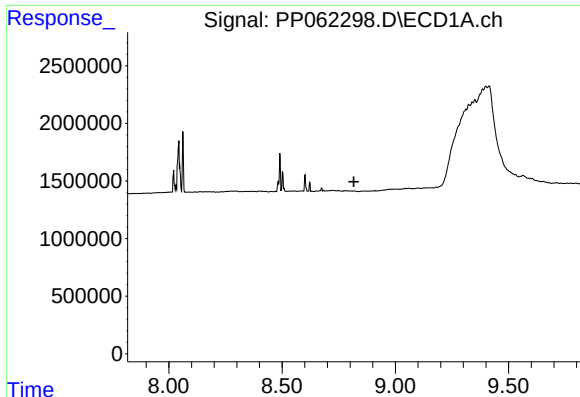

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 8.817 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

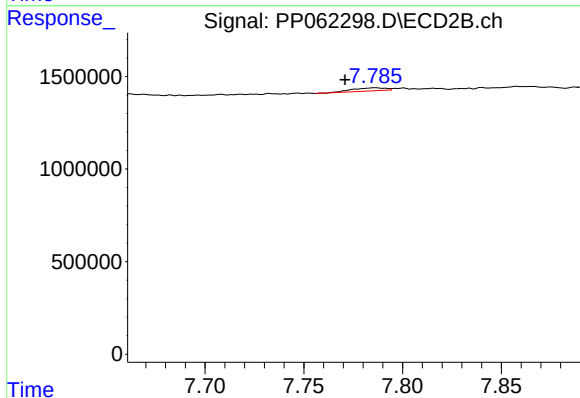


#42 AR-1268-2

R.T.: 7.786 min
Delta R.T.: 0.015 min
Response: 194114
Conc: 0.73 ng/ml

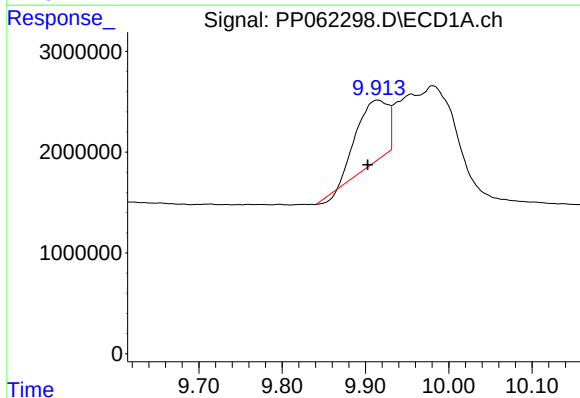

#45 AR-1268-5

R.T.: 9.915 min
Delta R.T.: 0.012 min
Response: 15653681
Conc: 47.76 ng/ml

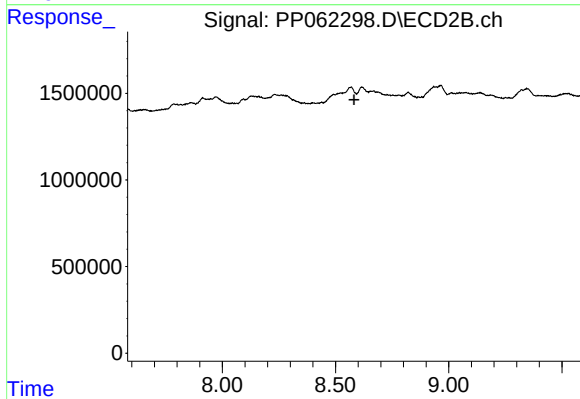

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 8.582 min
Response: 0
Conc: N.D.