

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120823\
 Data File : PP062327.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2023 19:58
 Operator : YP\AJ
 Sample : 05679-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DOUBLE-MANDOOR-CAULK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 22:46:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 28 04:28:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.449	3.719	33501510	38781324	25.448	21.552
2) SA Decachlor...	10.236	8.837	23069331	40282899	22.354m	19.517

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120823\
Data File : PP062327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2023 19:58
Operator : YP\AJ
Sample : 05679-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DOUBLE-MANDOOR-CAULK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 22:46:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 28 04:28:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

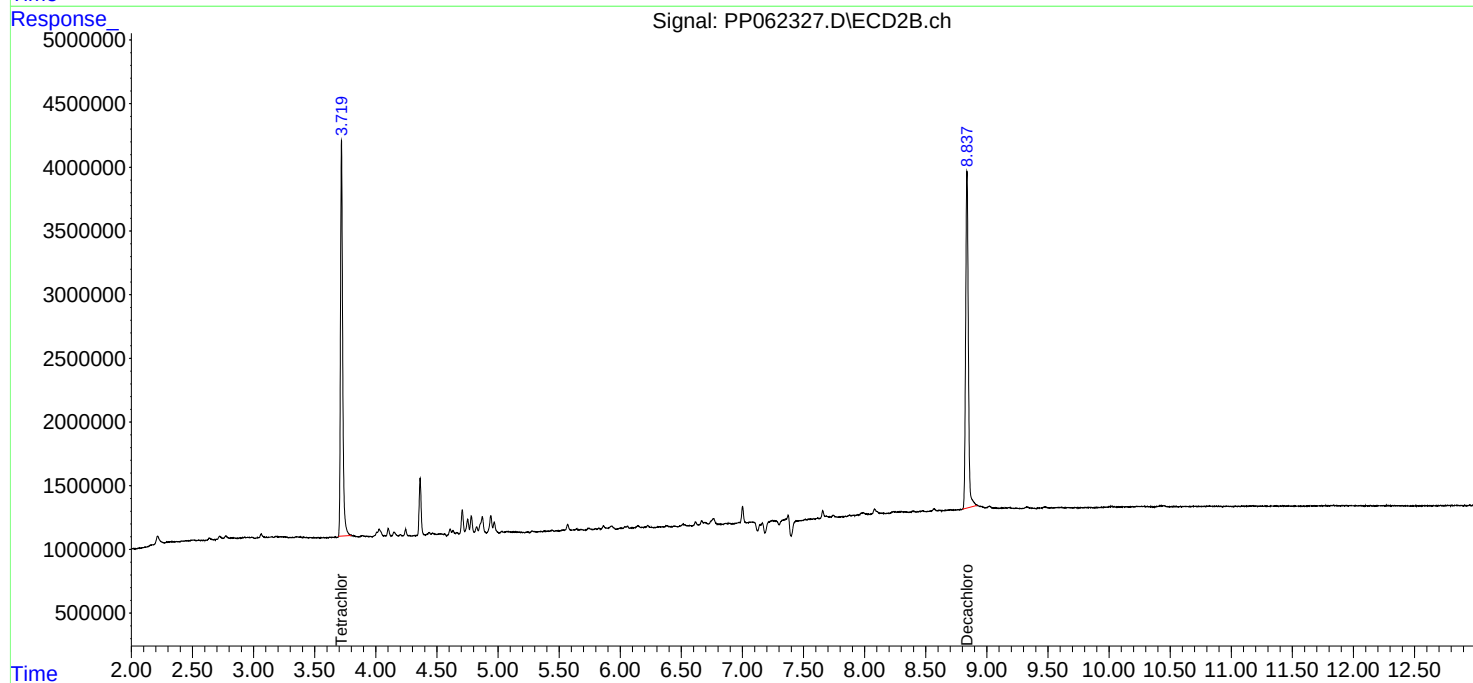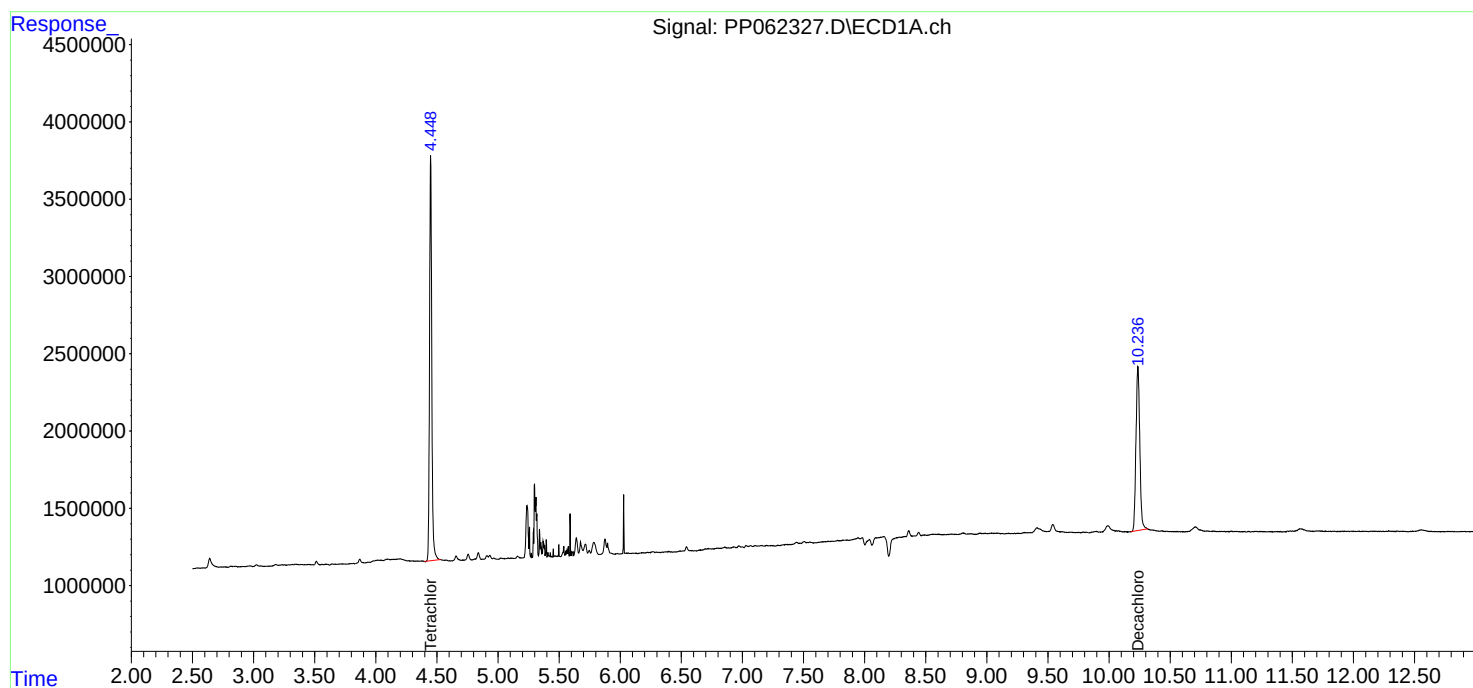


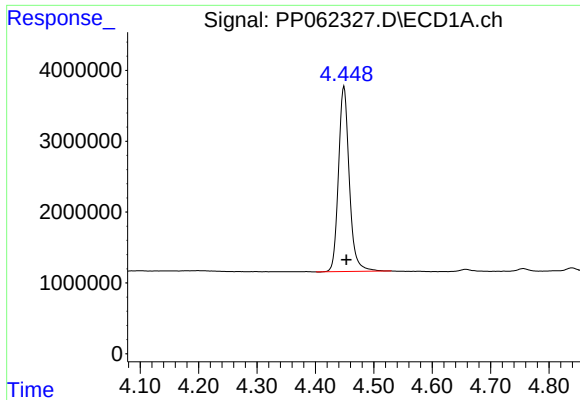

#1 Tetrachloro-m-xylene


R.T.: 4.449 min
Delta R.T.: -0.004 min
Response: 33501510
Conc: 25.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
DOUBLE-MANDOR-CAULK

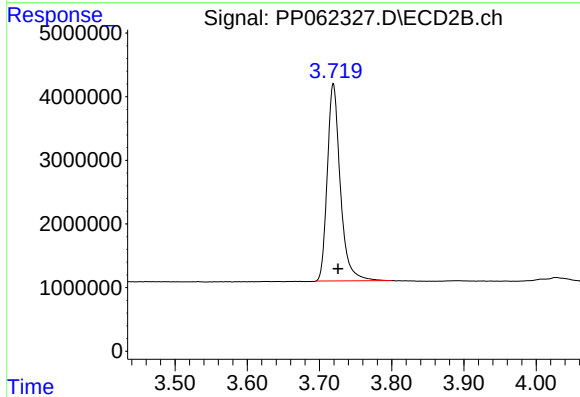


#1 Tetrachloro-m-xylene

R.T.: 3.719 min
Delta R.T.: -0.007 min
Response: 38781324
Conc: 21.55 ng/ml

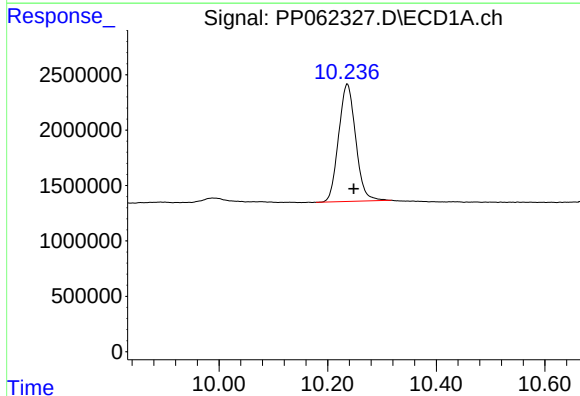

#2 Decachlorobiphenyl

R.T.: 10.236 min
Delta R.T.: -0.013 min
Response: 23069331
Conc: 22.35 ng/ml m

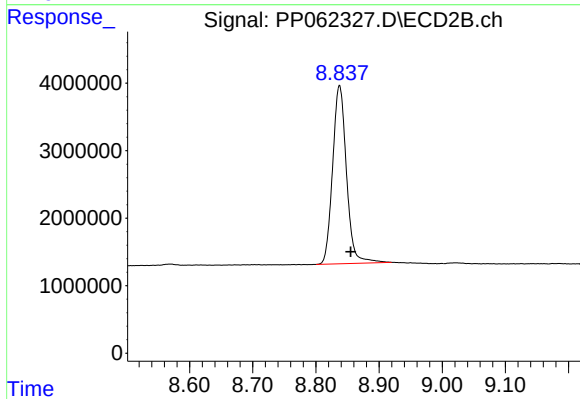

#2 Decachlorobiphenyl

R.T.: 8.837 min
Delta R.T.: -0.018 min
Response: 40282899
Conc: 19.52 ng/ml