

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120823\
 Data File : PP062349.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2023 02:36
 Operator : YP\AJ
 Sample : 05676-01
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-120423-AP01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/11/2023
 Supervised By :Ankita Jodhani 12/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 03:16:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 28 04:28:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.448	3.719	30667434	32704807	23.295	18.175
2)	SA Decachlor...	10.237	8.838	19104448	30891672	18.512m	14.967
Target Compounds							
26)	L6 AR-1254-1	6.482	5.648	1413106	2809064	25.188	25.799
27)	L6 AR-1254-2	6.701	5.797	2995338	3089743	35.924	30.786m
28)	L6 AR-1254-3	7.069	6.208	4160456	6164796	50.290	39.461
29)	L6 AR-1254-4	7.356	6.439	2876775	4170054	54.858	52.466
30)	L6 AR-1254-5	7.775	6.863	3688747	6424393	57.908m	45.522

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120823\
Data File : PP062349.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2023 02:36
Operator : YP\AJ
Sample : 05676-01
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PCB-120423-AP01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/11/2023
Supervised By :Ankita Jodhani 12/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 03:16:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112723.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 28 04:28:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

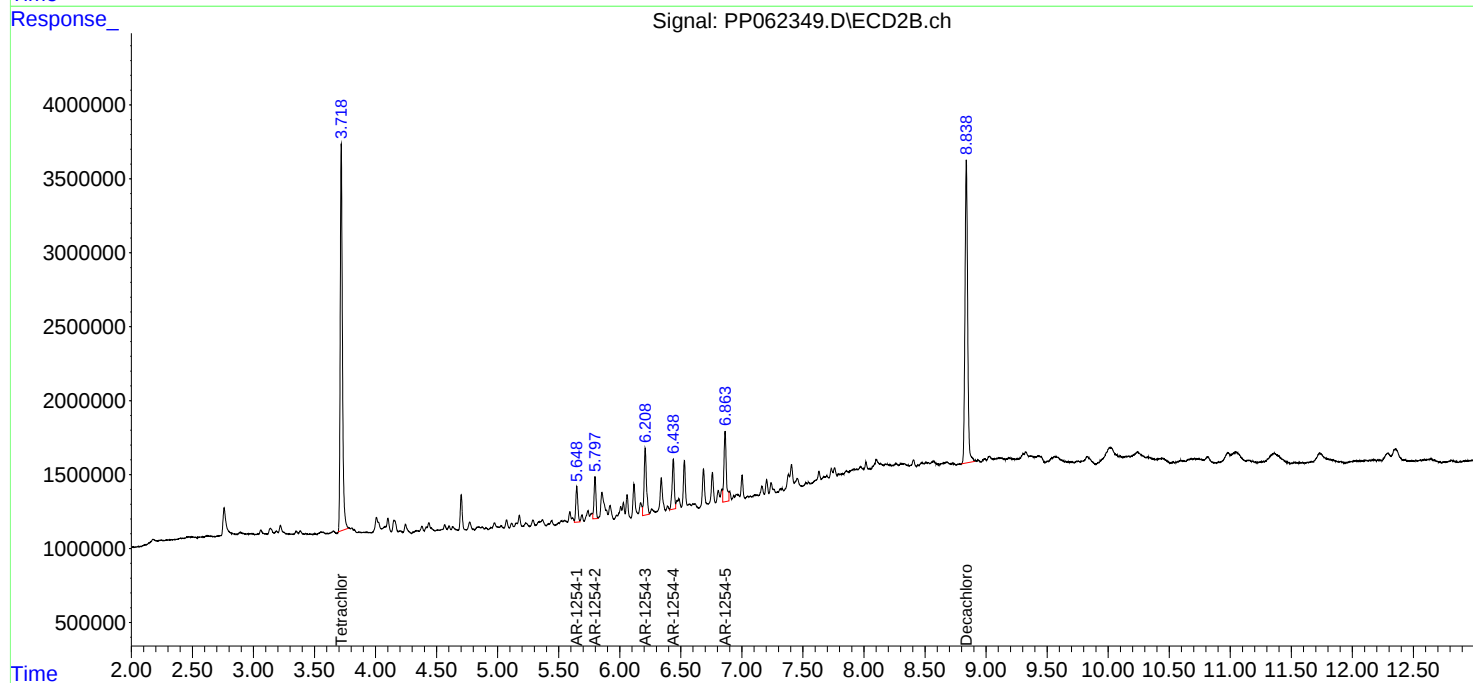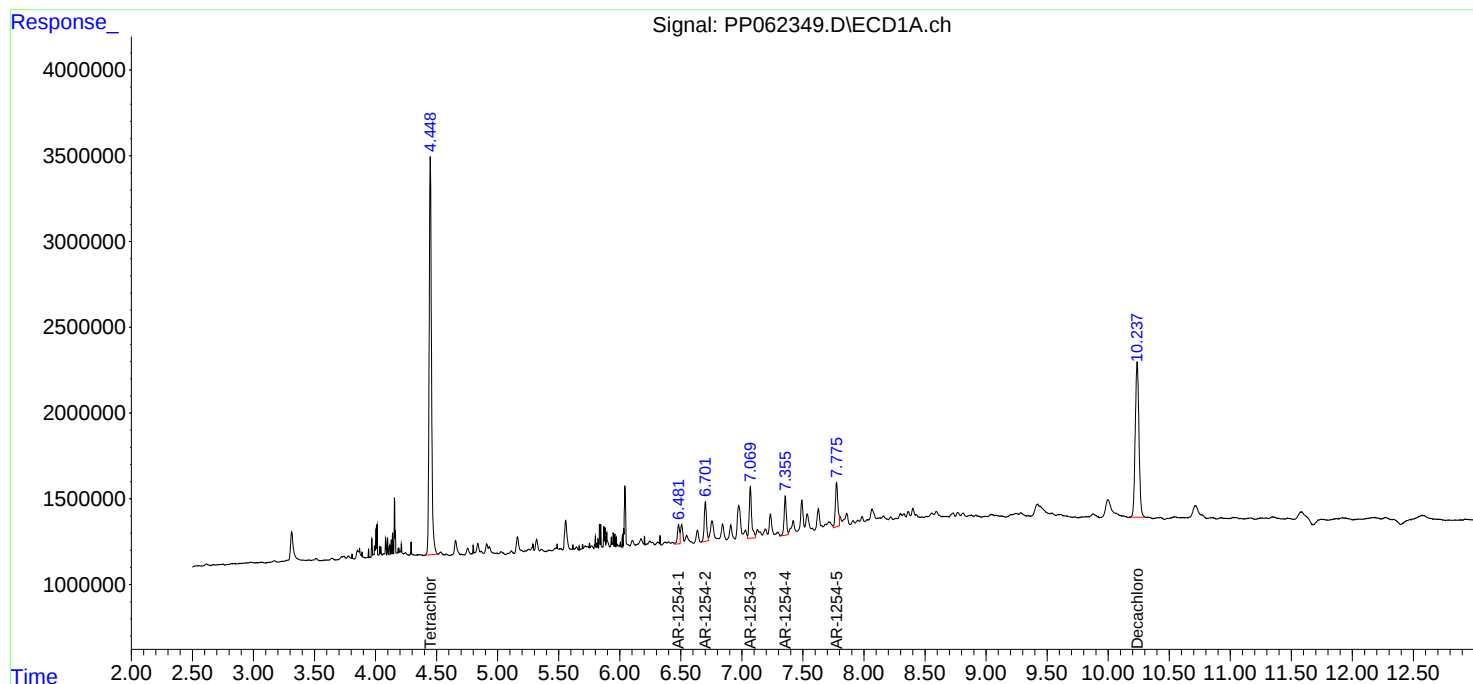

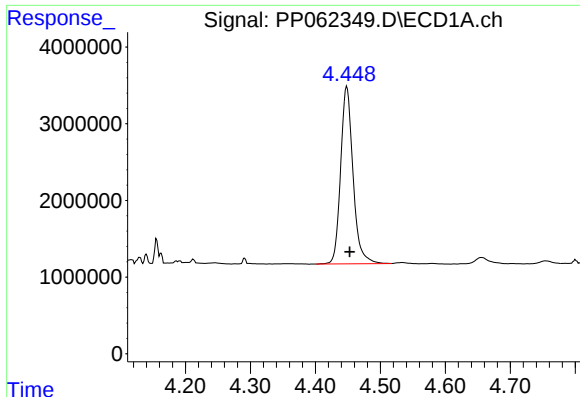


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: -0.005 min
Response: 30667434
Conc: 23.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120423-AP01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/11/2023
Supervised By :Ankita Jodhani 12/11/2023

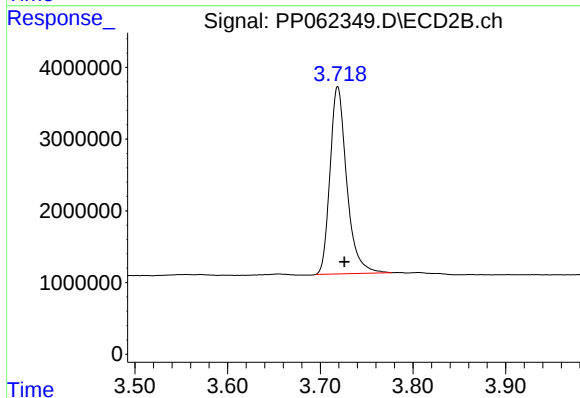


#1 Tetrachloro-m-xylene

R.T.: 3.719 min
Delta R.T.: -0.007 min
Response: 32704807
Conc: 18.18 ng/ml

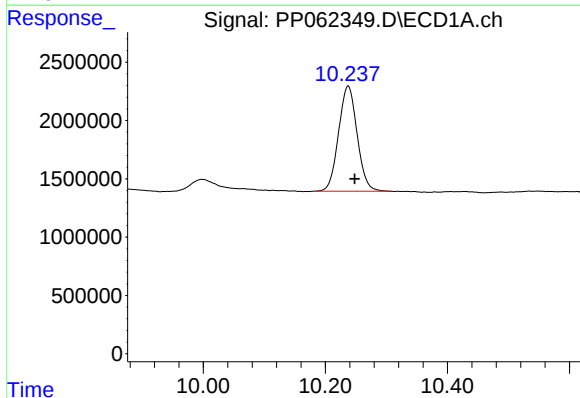


#2 Decachlorobiphenyl

R.T.: 10.237 min
Delta R.T.: -0.012 min
Response: 19104448
Conc: 18.51 ng/ml m

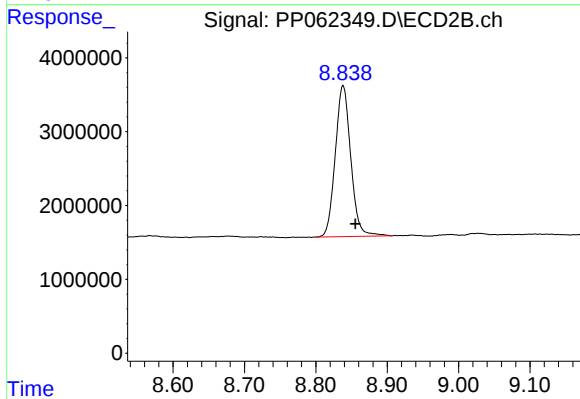

#2 Decachlorobiphenyl

R.T.: 8.838 min
Delta R.T.: -0.017 min
Response: 30891672
Conc: 14.97 ng/ml

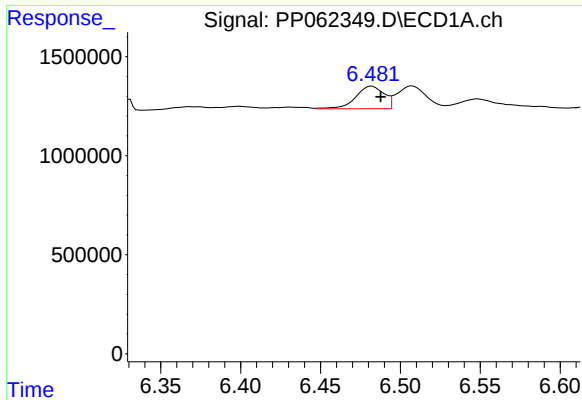


#26 AR-1254-1

R.T.: 6.482 min
Delta R.T.: -0.006 min
Response: 1413106
Conc: 25.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120423-AP01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/11/2023
Supervised By :Ankita Jodhani 12/11/2023

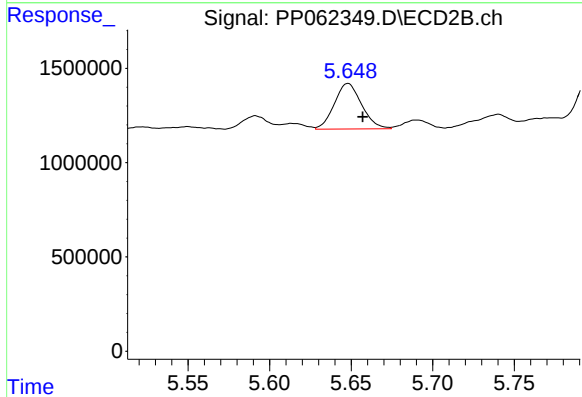


#26 AR-1254-1

R.T.: 5.648 min
Delta R.T.: -0.009 min
Response: 2809064
Conc: 25.80 ng/ml

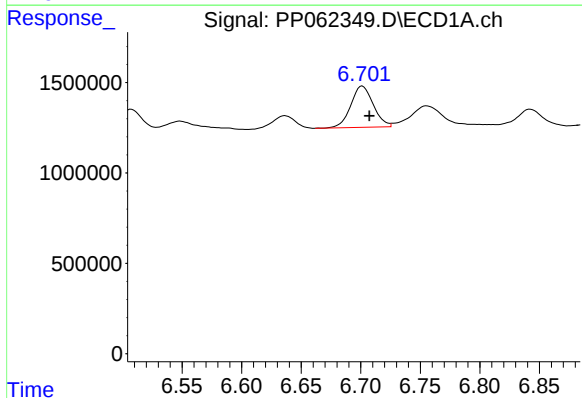


#27 AR-1254-2

R.T.: 6.701 min
Delta R.T.: -0.006 min
Response: 2995338
Conc: 35.92 ng/ml

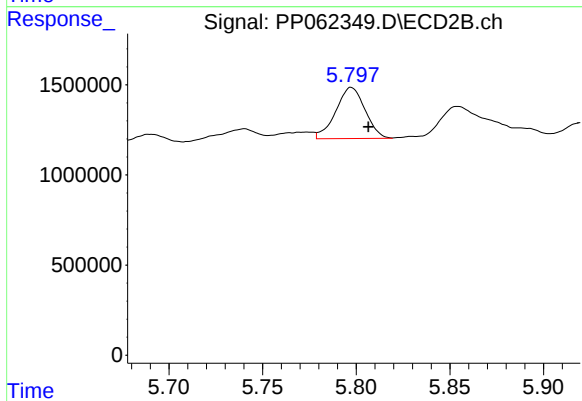

#27 AR-1254-2

R.T.: 5.797 min
Delta R.T.: -0.010 min
Response: 3089743
Conc: 30.79 ng/ml m

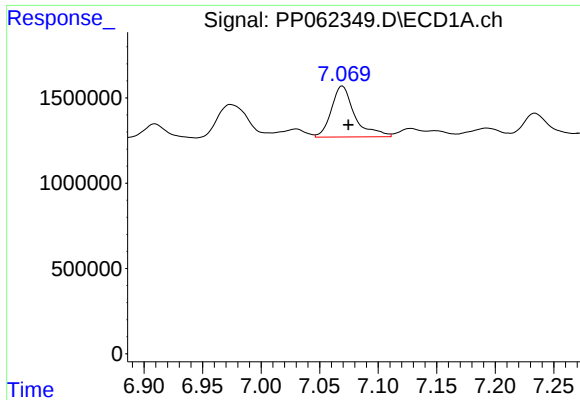


#28 AR-1254-3

R.T.: 7.069 min
Delta R.T.: -0.005 min
Response: 4160456
Conc: 50.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120423-AP01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/11/2023
Supervised By :Ankita Jodhani 12/11/2023

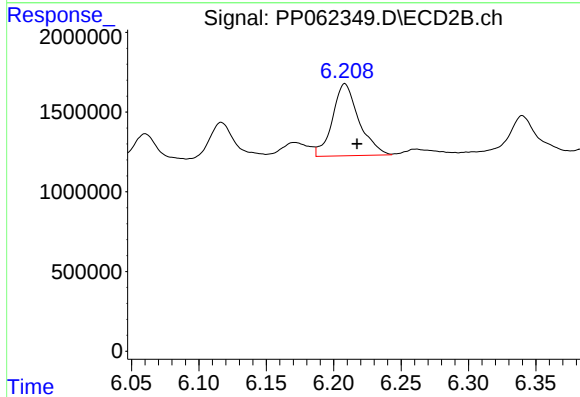


#28 AR-1254-3

R.T.: 6.208 min
Delta R.T.: -0.009 min
Response: 6164796
Conc: 39.46 ng/ml

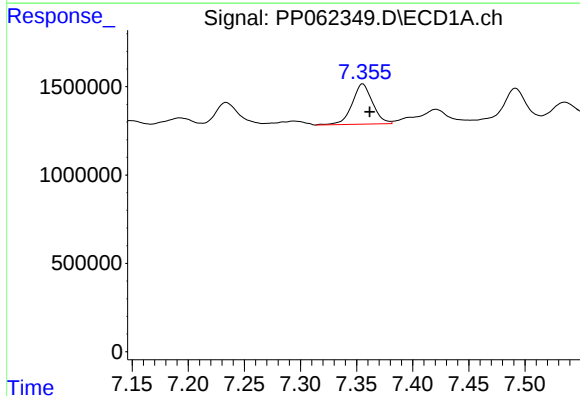


#29 AR-1254-4

R.T.: 7.356 min
Delta R.T.: -0.006 min
Response: 2876775
Conc: 54.86 ng/ml

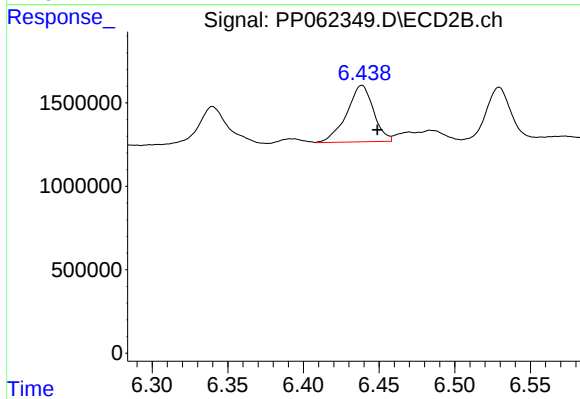

#29 AR-1254-4

R.T.: 6.439 min
Delta R.T.: -0.010 min
Response: 4170054
Conc: 52.47 ng/ml

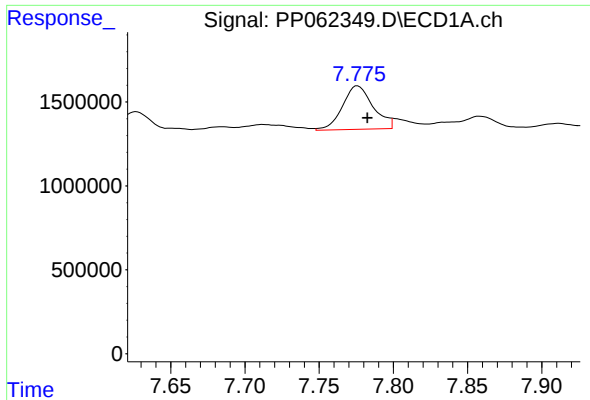


#30 AR-1254-5

R.T.: 7.775 min
Delta R.T.: -0.008 min
Response: 3688747
Conc: 57.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120423-AP01

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/11/2023
Supervised By :Ankita Jodhani 12/11/2023

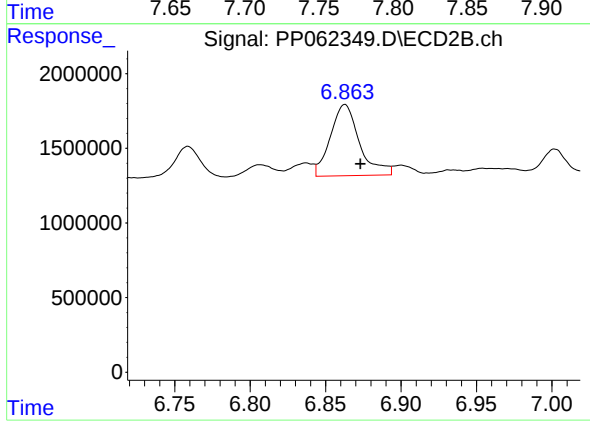

#30 AR-1254-5

R.T.: 6.863 min
Delta R.T.: -0.010 min
Response: 6424393
Conc: 45.52 ng/ml