

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120920\
 Data File : PP031926.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Dec 2020 10:33
 Operator : DD\AJ
 Sample : L4969-03RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 NORTH-BRANFORD-03RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 01:23:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.786	4.057	1684147	1485831	34.780	31.007
2)	SA Decachlor...	10.656	9.358	1216422	1245208	35.815	33.630
Target Compounds							
9)	L2 AR-1221-2	0.000	4.408	0	25973	N.D.	67.332 #
28)	L6 AR-1254-3	7.611	0.000	111036	0	43.952	N.D. #
34)	L7 AR-1260-4	0.000	7.735	0	8253	N.D.	4.343 #
35)	L7 AR-1260-5	0.000	7.968f	0	21268	N.D.	4.687 #
37)	L8 AR-1262-2	0.000	7.968f	0	21268	N.D.	4.378 #
38)	L8 AR-1262-3	0.000	8.270	0	7564	N.D.	3.846 #
41)	L9 AR-1268-1	0.000	8.270	0	7564	N.D.	1.367 #
45)	L9 AR-1268-5	0.000	9.111	0	8261	N.D.	0.597 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120920\
Data File : PP031926.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Dec 2020 10:33
Operator : DD\AJ
Sample : L4969-03RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
NORTH-BRANFORD-03RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 01:23:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

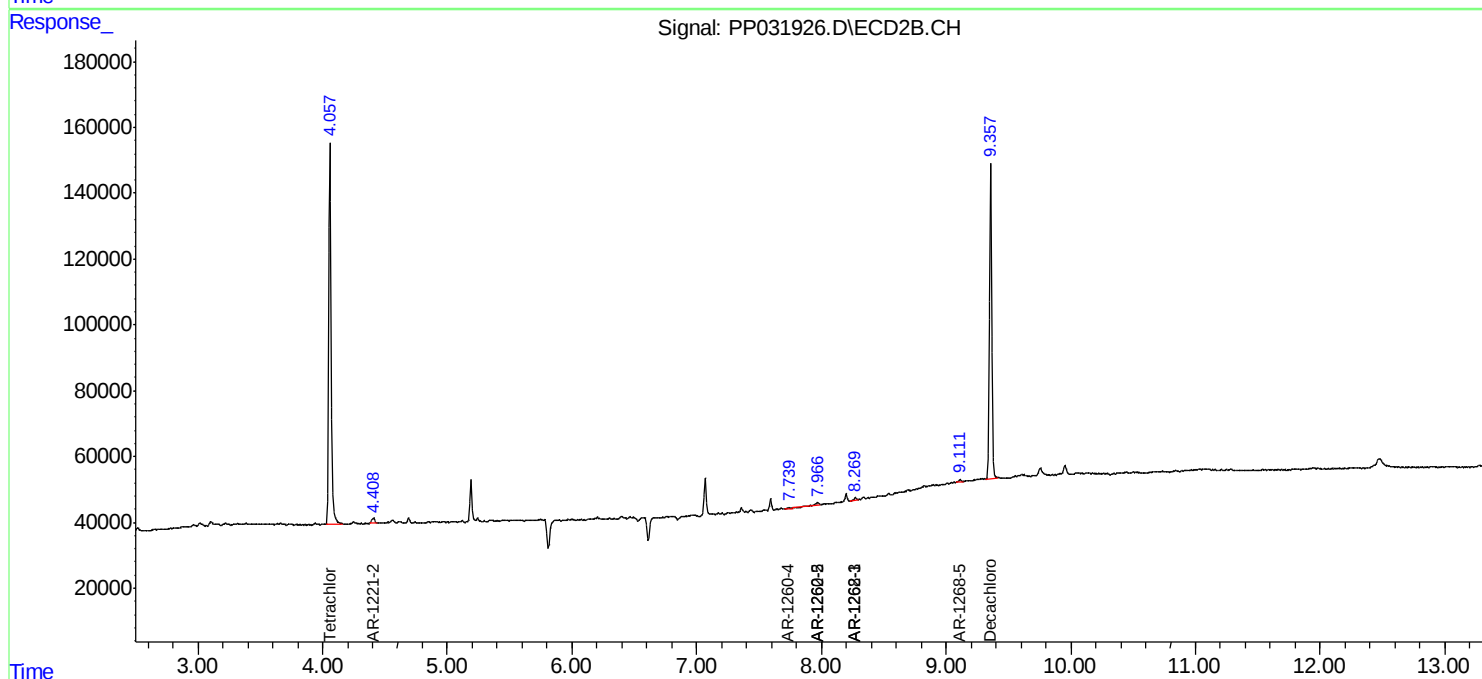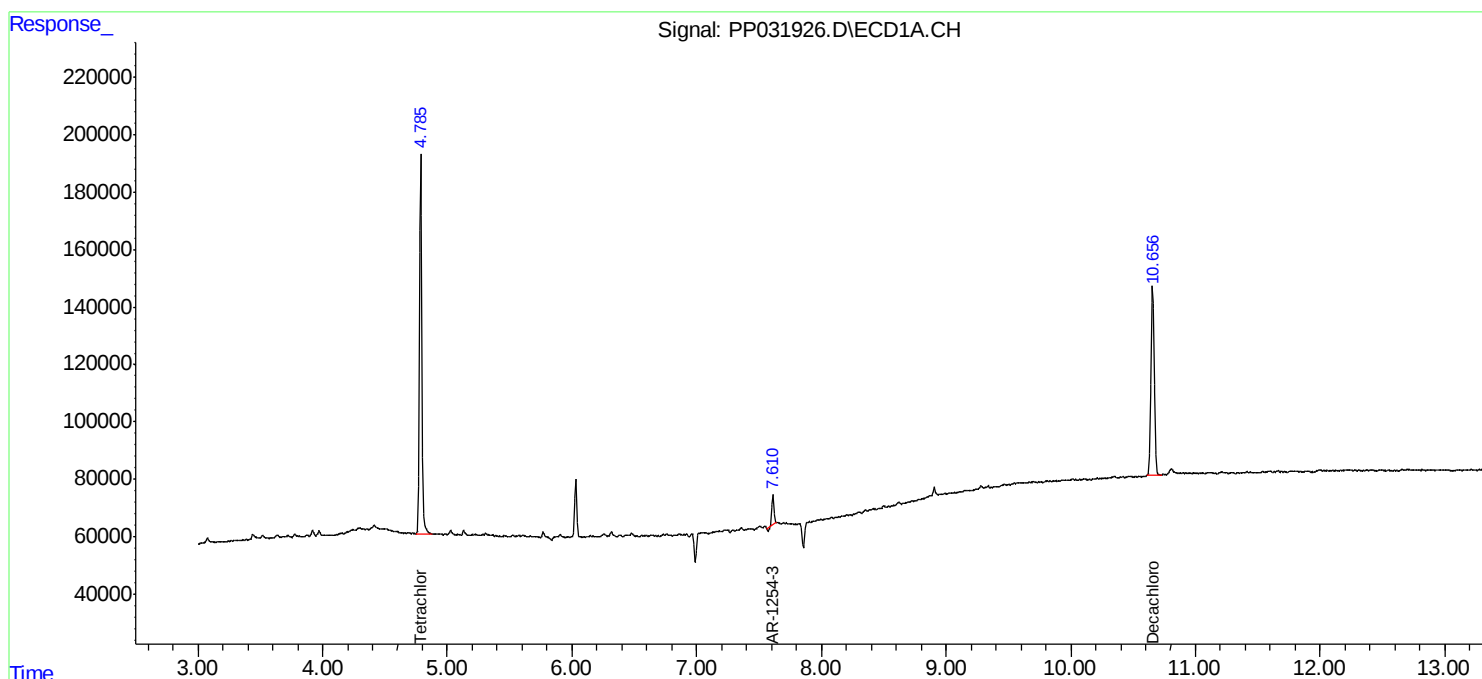


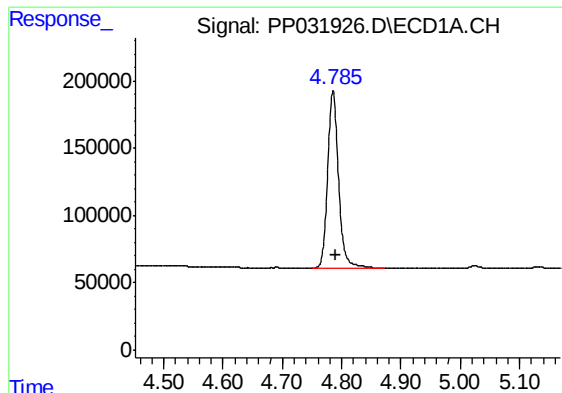

#1 Tetrachloro-m-xylene


R.T.: 4.786 min
Delta R.T.: -0.004 min
Response: 1684147
Conc: 34.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
NORTH-BRANFORD-03RE

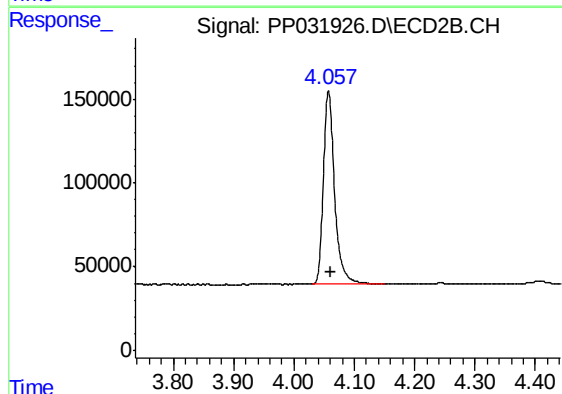


#1 Tetrachloro-m-xylene

R.T.: 4.057 min
Delta R.T.: -0.004 min
Response: 1485831
Conc: 31.01 ng/ml

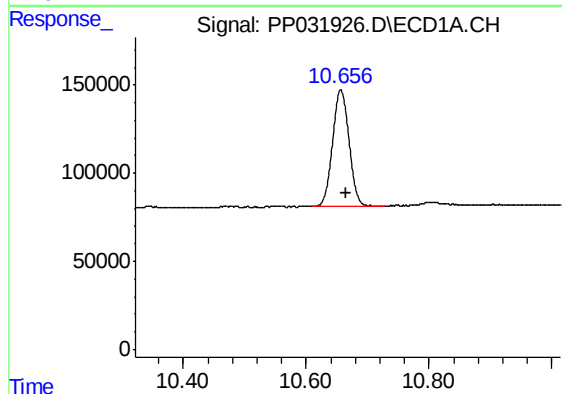


#2 Decachlorobiphenyl

R.T.: 10.656 min
Delta R.T.: -0.009 min
Response: 1216422
Conc: 35.81 ng/ml

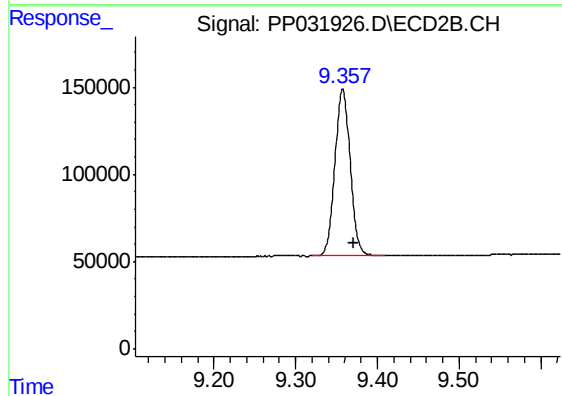

#2 Decachlorobiphenyl


R.T.: 9.358 min
Delta R.T.: -0.013 min
Response: 1245208
Conc: 33.63 ng/ml

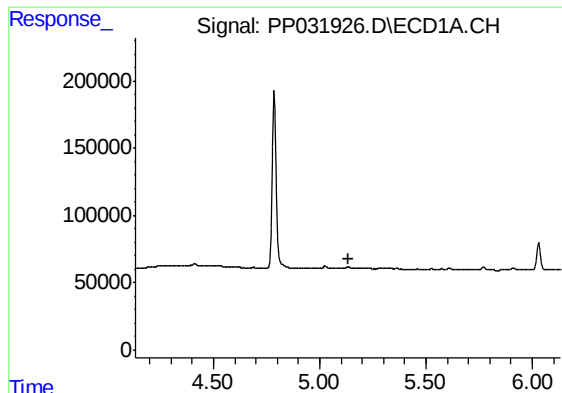

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 5.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
NORTH-BRANFORD-03RE

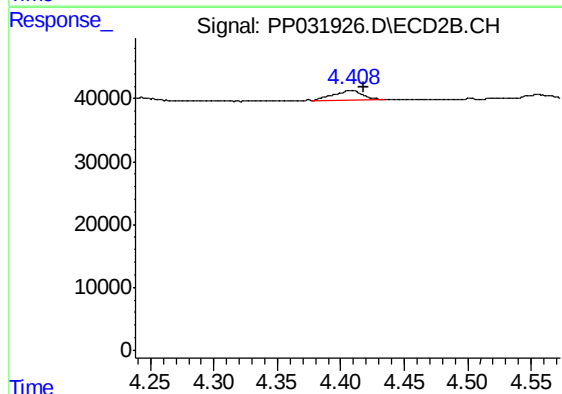


#9 AR-1221-2

R.T.: 4.408 min
Delta R.T.: -0.010 min
Response: 25973
Conc: 67.33 ng/ml

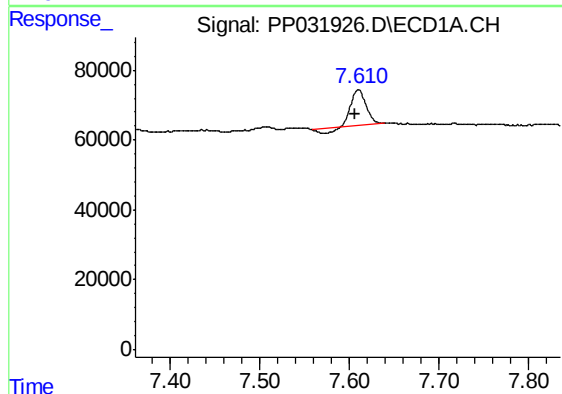


#28 AR-1254-3

R.T.: 7.611 min
Delta R.T.: 0.004 min
Response: 111036
Conc: 43.95 ng/ml

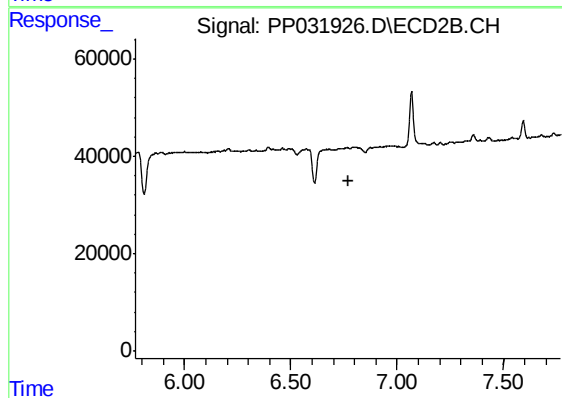

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.769 min
Response: 0
Conc: N.D.

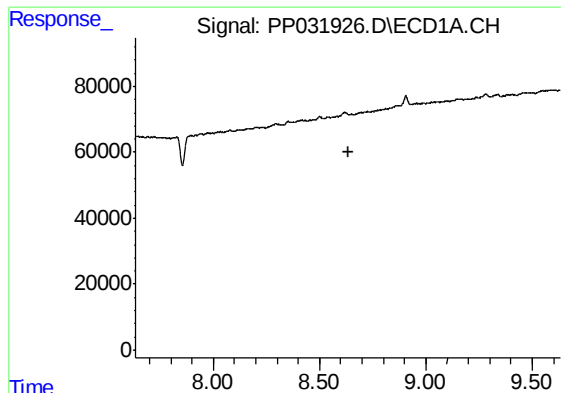

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 8.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
NORTH-BRANFORD-03RE

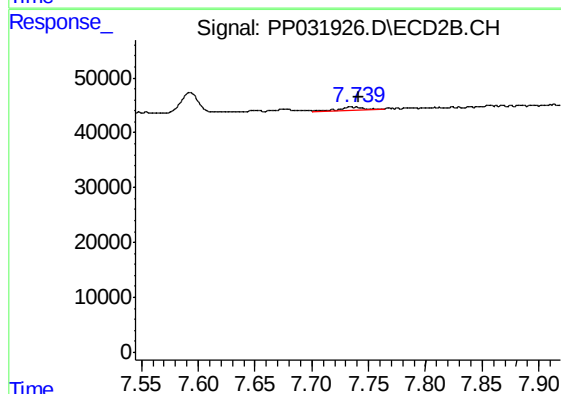


#34 AR-1260-4

R.T.: 7.735 min
Delta R.T.: -0.006 min
Response: 8253
Conc: 4.34 ng/ml

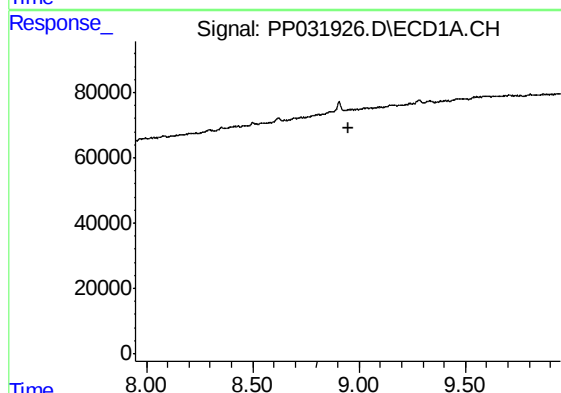


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

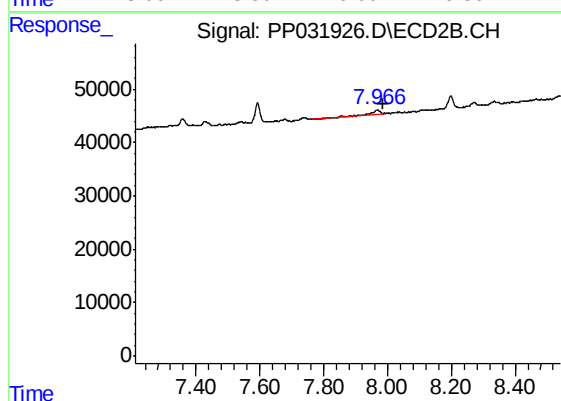

#35 AR-1260-5


R.T.: 7.968 min
Delta R.T.: -0.019 min
Response: 21268
Conc: 4.69 ng/ml

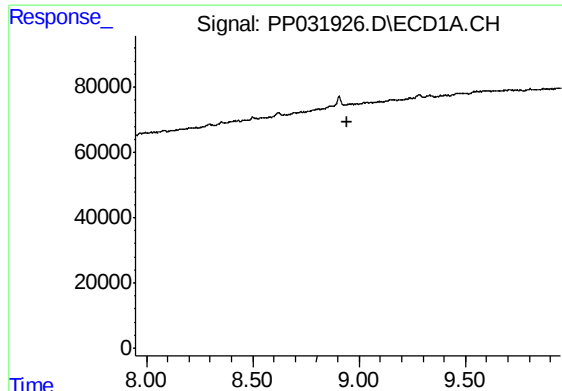

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
NORTH-BRANFORD-03RE

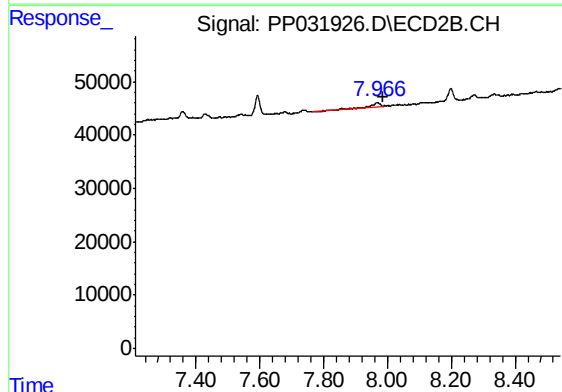


#37 AR-1262-2

R.T.: 7.968 min
Delta R.T.: -0.018 min
Response: 21268
Conc: 4.38 ng/ml

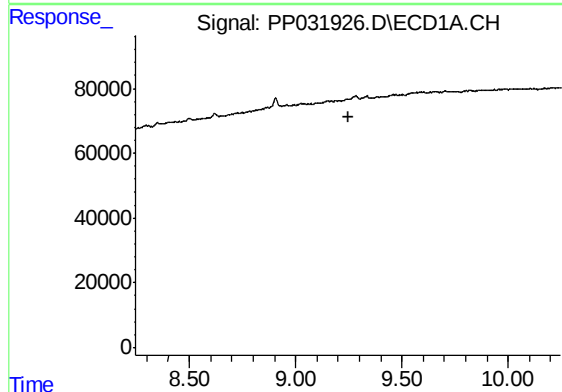


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.246 min
Response: 0
Conc: N.D.

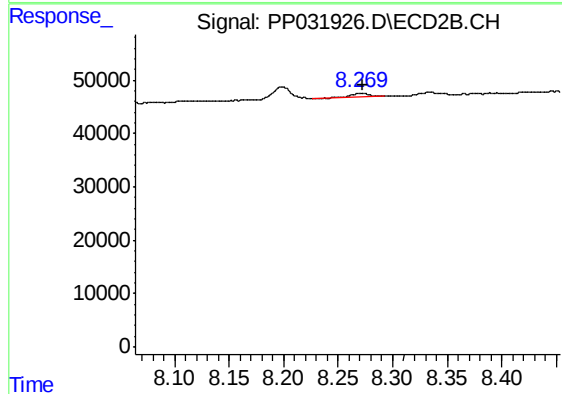

#38 AR-1262-3


R.T.: 8.270 min
Delta R.T.: -0.002 min
Response: 7564
Conc: 3.85 ng/ml

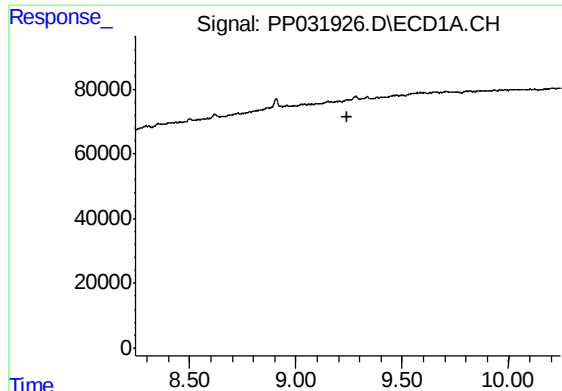

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 9.244 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
NORTH-BRANFORD-03RE

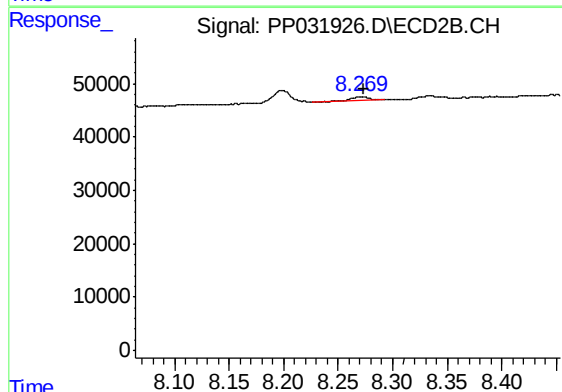


#41 AR-1268-1

R.T.: 8.270 min
Delta R.T.: -0.003 min
Response: 7564
Conc: 1.37 ng/ml

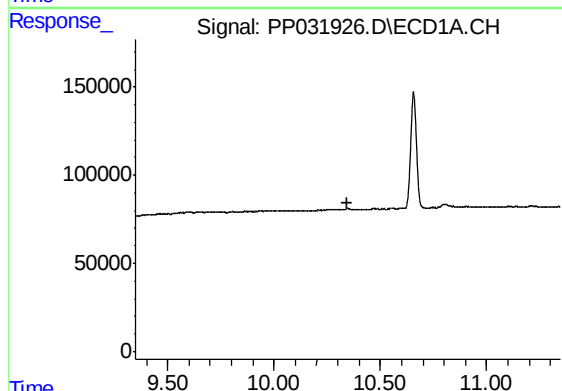

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.347 min
Response: 0
Conc: N.D.

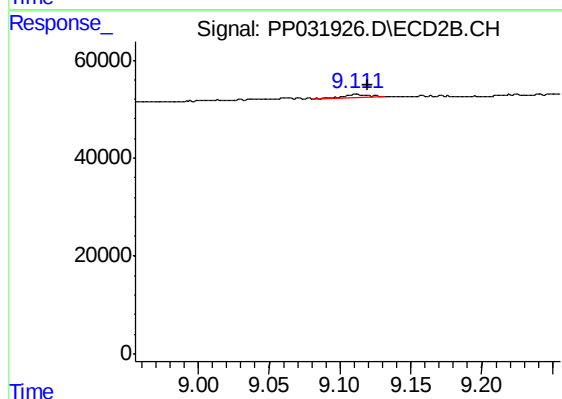

#45 AR-1268-5

R.T.: 9.111 min
Delta R.T.: -0.008 min
Response: 8261
Conc: 0.60 ng/ml