

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120920\
 Data File : PP031946.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Dec 2020 18:05
 Operator : DD\AJ
 Sample : L4983-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TR1-A-D-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 01:36:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.785	4.058	1109877	948331	22.920	19.790
2)	SA Decachlor...	10.658	9.358	743855	802490	21.901	21.673
Target Compounds							
9)	L2 AR-1221-2	0.000	4.410	0	17213	N.D.	44.621 #
28)	L6 AR-1254-3	0.000	6.762	0	8723	N.D.	2.822 #
29)	L6 AR-1254-4	0.000	7.002	0	14071	N.D.	8.282 #
30)	L6 AR-1254-5	0.000	7.430	0	22549	N.D.	8.353 #
31)	L7 AR-1260-1	7.793f	0.000	223777	0	127.869	N.D. #
32)	L7 AR-1260-2	0.000	7.087f	0	221570	N.D.	90.985 #
33)	L7 AR-1260-3	0.000	7.247	0	9345	N.D.	4.092 #
34)	L7 AR-1260-4	8.622	7.733	34750	11669	18.872	6.141 #
35)	L7 AR-1260-5	0.000	7.977	0	33442	N.D.	7.369 #
36)	L8 AR-1262-1	0.000	7.469	0	11629	N.D.	4.184 #
37)	L8 AR-1262-2	0.000	7.977	0	33442	N.D.	6.885 #
38)	L8 AR-1262-3	0.000	8.269	0	19579	N.D.	9.954 #
39)	L8 AR-1262-4	0.000	8.330	0	28792	N.D.	7.942 #
40)	L8 AR-1262-5	0.000	8.831	0	39756	N.D.	24.493 #
41)	L9 AR-1268-1	0.000	8.269	0	19579	N.D.	3.539 #
42)	L9 AR-1268-2	0.000	8.330	0	28792	N.D.	5.325 #
44)	L9 AR-1268-4	0.000	8.831	0	39756	N.D.	21.812 #
45)	L9 AR-1268-5	0.000	9.109	0	12669	N.D.	0.915 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120920\
Data File : PP031946.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Dec 2020 18:05
Operator : DD\AJ
Sample : L4983-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
TR1-A-D-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 01:36:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

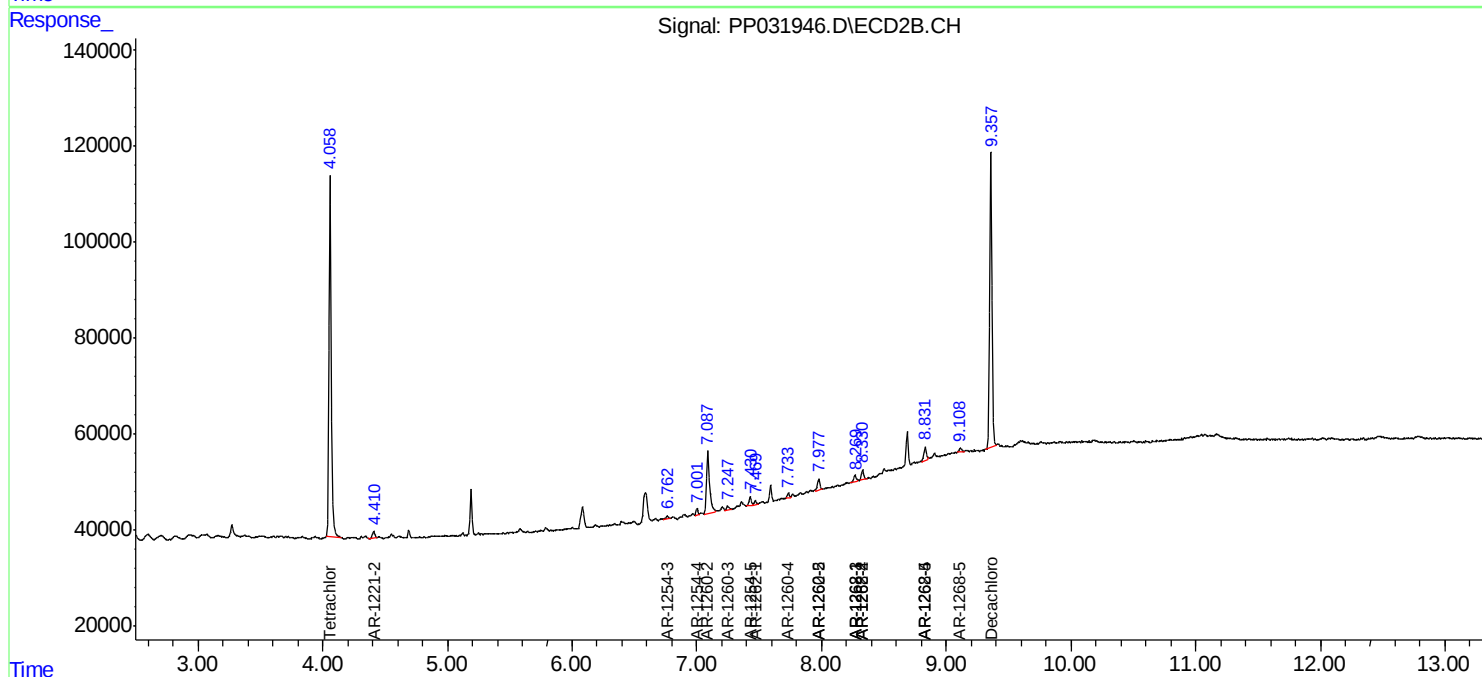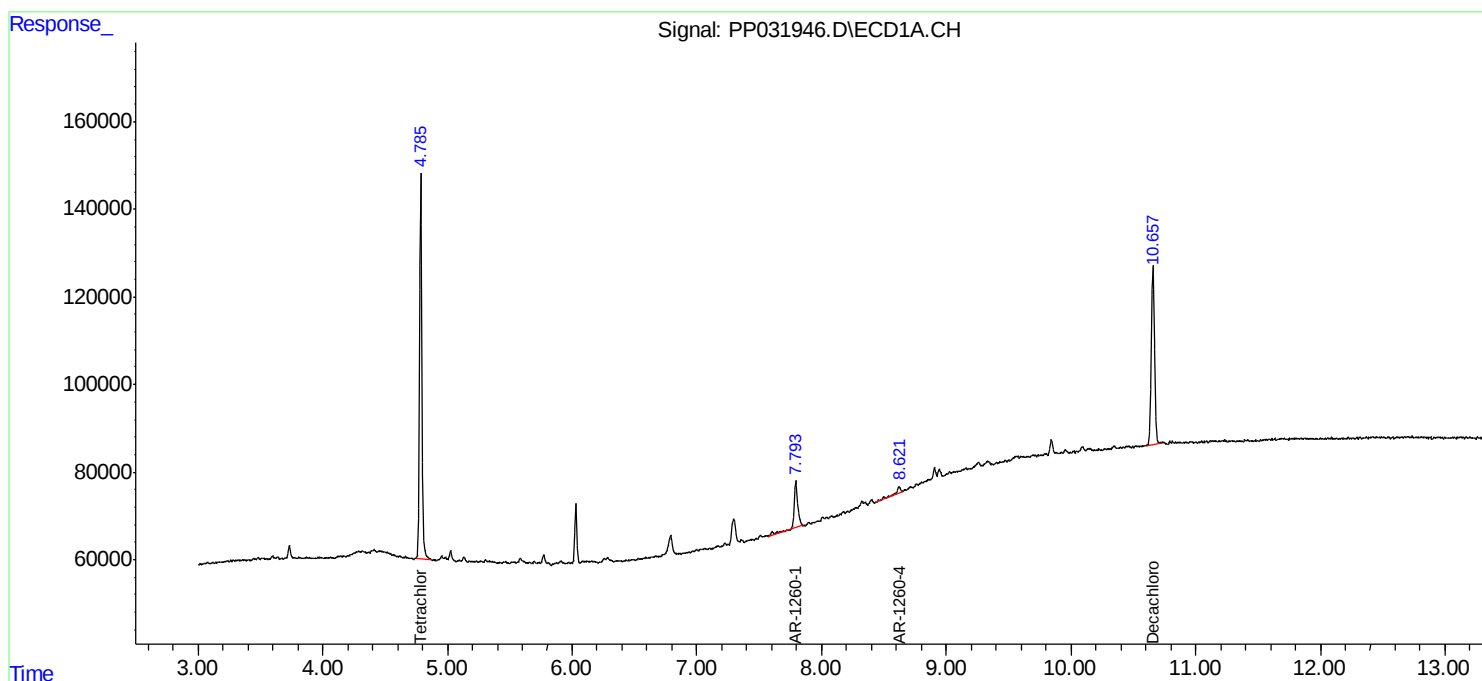


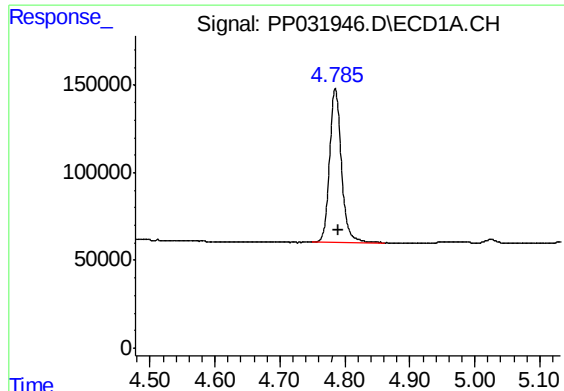

#1 Tetrachloro-m-xylene


R.T.: 4.785 min
Delta R.T.: -0.005 min
Response: 1109877
Conc: 22.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
TR1-A-D-COMP

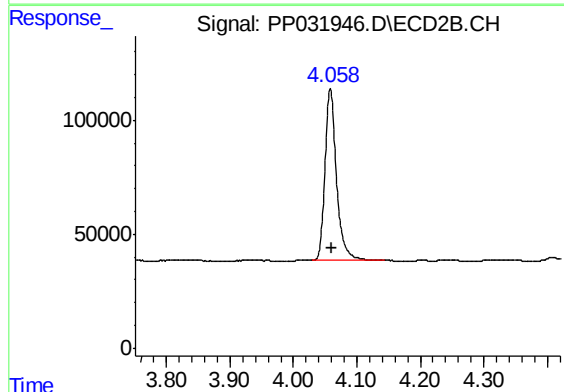


#1 Tetrachloro-m-xylene

R.T.: 4.058 min
Delta R.T.: -0.003 min
Response: 948331
Conc: 19.79 ng/ml

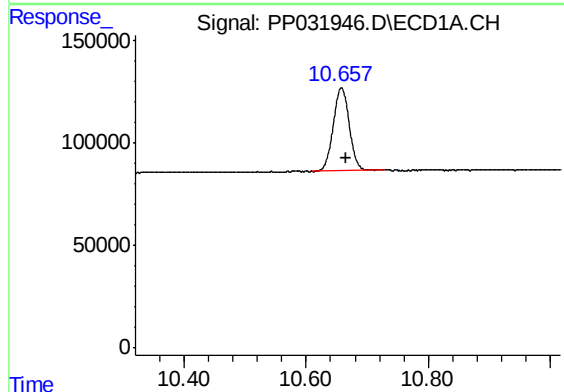


#2 Decachlorobiphenyl

R.T.: 10.658 min
Delta R.T.: -0.007 min
Response: 743855
Conc: 21.90 ng/ml

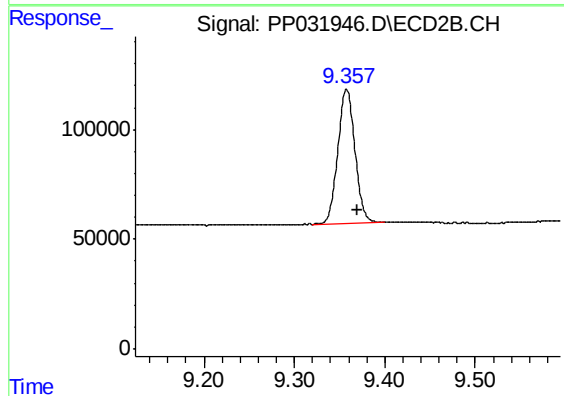

#2 Decachlorobiphenyl


R.T.: 9.358 min
Delta R.T.: -0.013 min
Response: 802490
Conc: 21.67 ng/ml

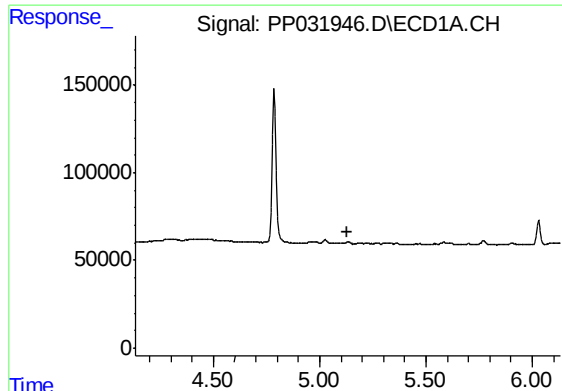

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 5.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR1-A-D-COMP

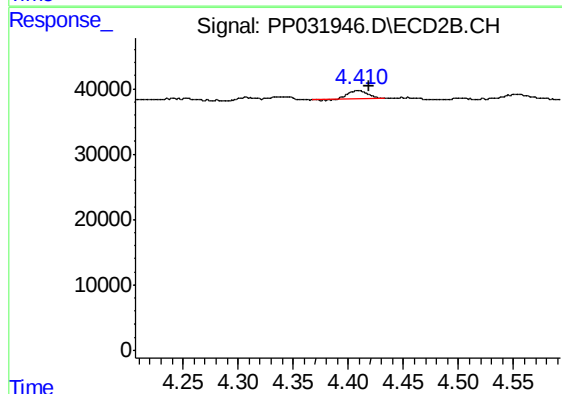


#9 AR-1221-2

R.T.: 4.410 min
Delta R.T.: -0.009 min
Response: 17213
Conc: 44.62 ng/ml

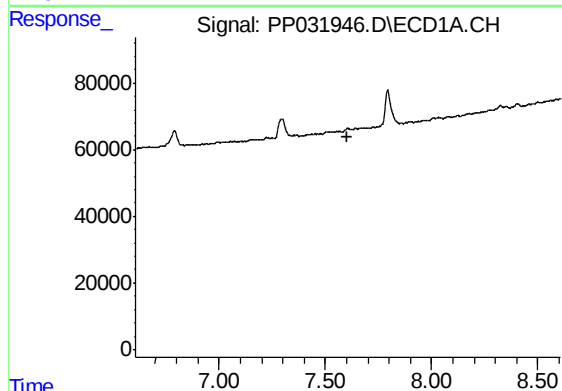


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 7.606 min
Response: 0
Conc: N.D.

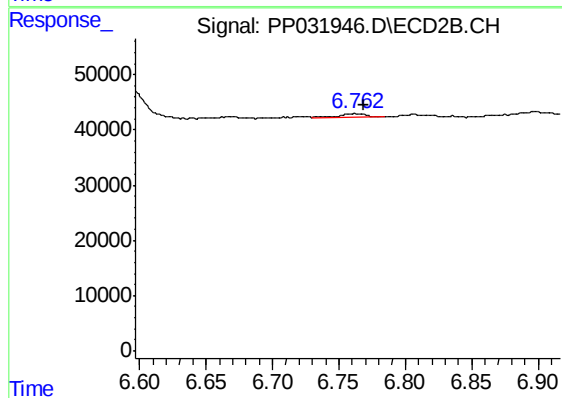

#28 AR-1254-3


R.T.: 6.762 min
Delta R.T.: -0.007 min
Response: 8723
Conc: 2.82 ng/ml

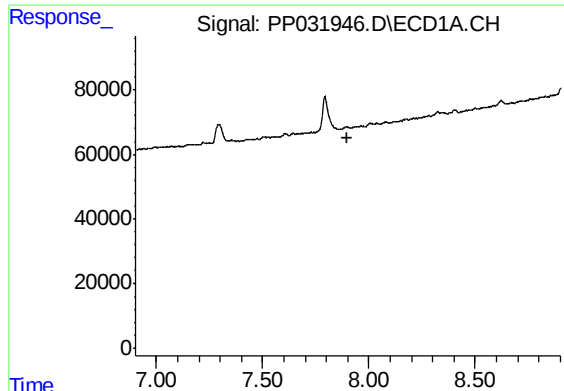

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 7.901 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR1-A-D-COMP

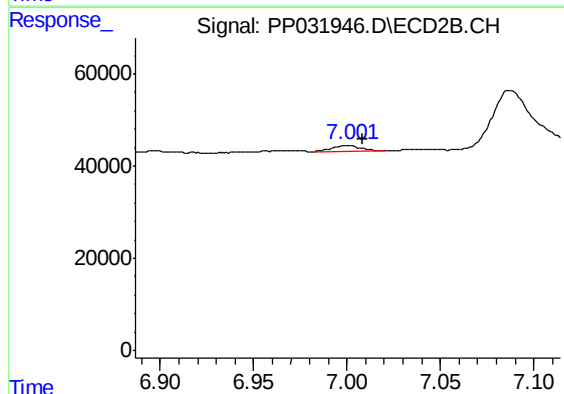


#29 AR-1254-4

R.T.: 7.002 min
Delta R.T.: -0.006 min
Response: 14071
Conc: 8.28 ng/ml

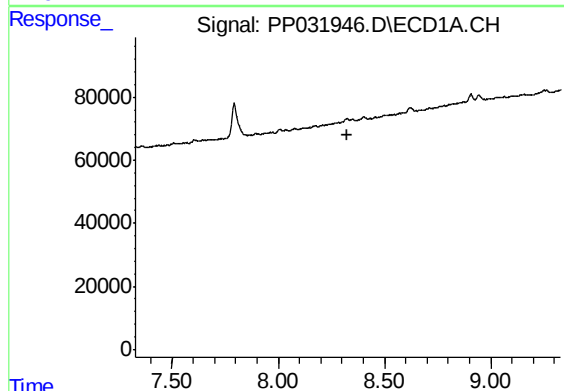


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 8.328 min
Response: 0
Conc: N.D.

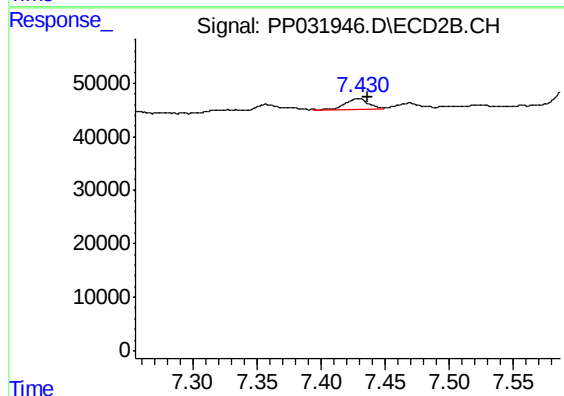

#30 AR-1254-5


R.T.: 7.430 min
Delta R.T.: -0.007 min
Response: 22549
Conc: 8.35 ng/ml

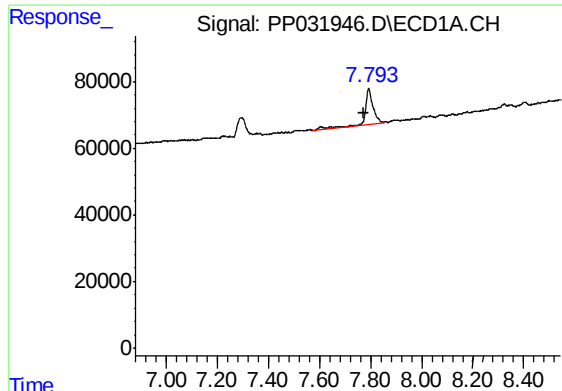

#31 AR-1260-1


R.T.: 7.793 min
Delta R.T.: 0.018 min
Response: 223777
Conc: 127.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
TR1-A-D-COMP

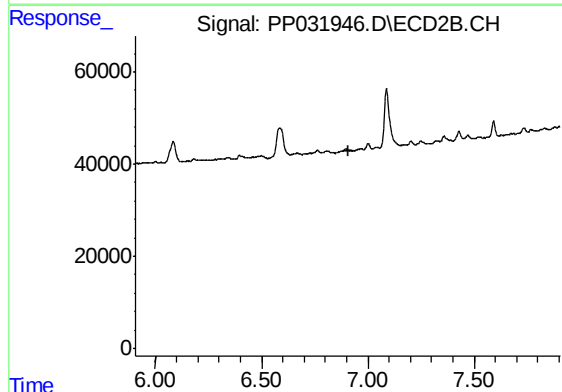


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.907 min
Response: 0
Conc: N.D.

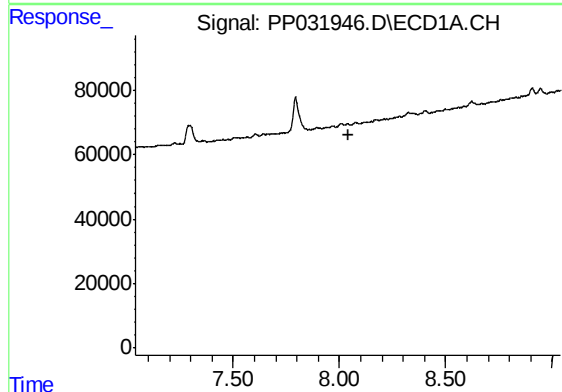


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.040 min
Response: 0
Conc: N.D.

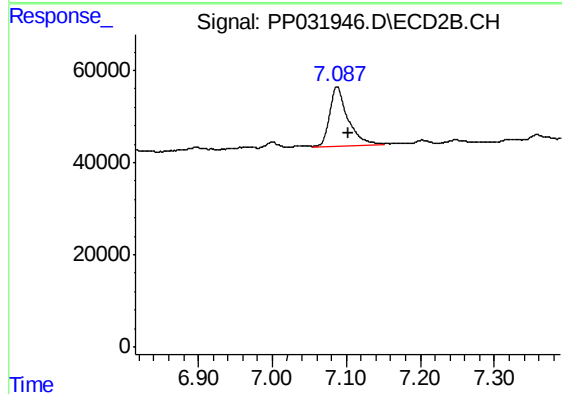

#32 AR-1260-2


R.T.: 7.087 min
Delta R.T.: -0.016 min
Response: 221570
Conc: 90.98 ng/ml

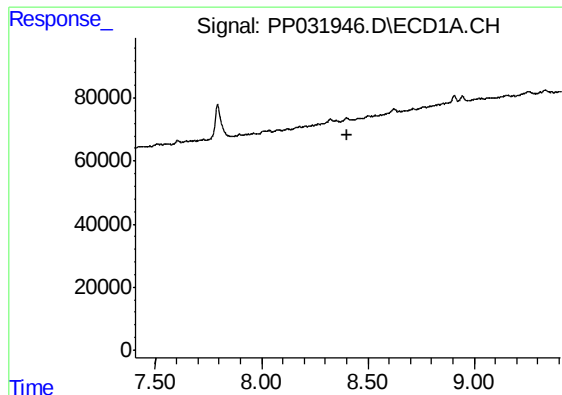

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.406 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR1-A-D-COMP

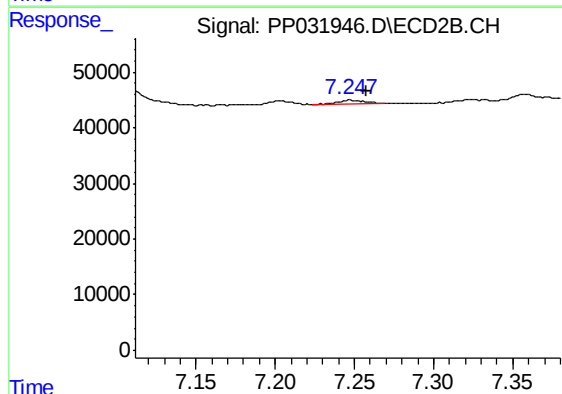


#33 AR-1260-3

R.T.: 7.247 min
Delta R.T.: -0.011 min
Response: 9345
Conc: 4.09 ng/ml

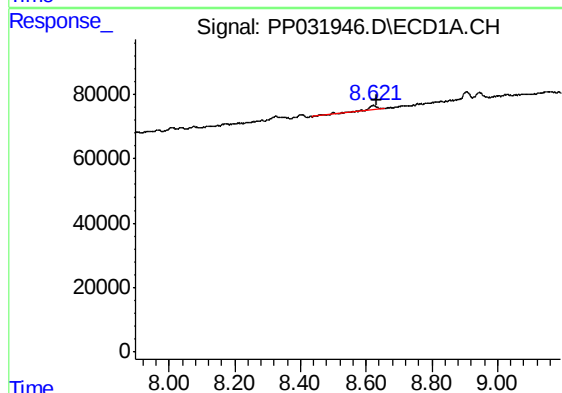


#34 AR-1260-4

R.T.: 8.622 min
Delta R.T.: -0.012 min
Response: 34750
Conc: 18.87 ng/ml

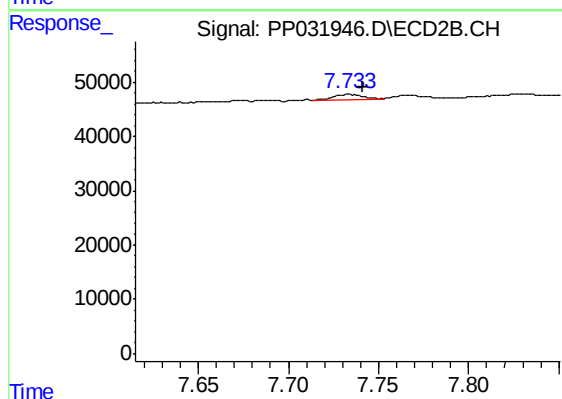

#34 AR-1260-4


R.T.: 7.733 min
Delta R.T.: -0.008 min
Response: 11669
Conc: 6.14 ng/ml

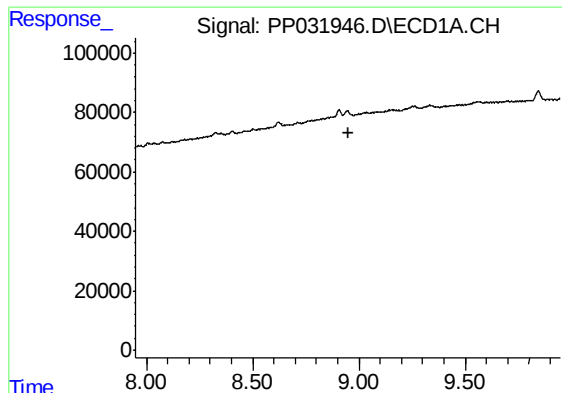

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR1-A-D-COMP

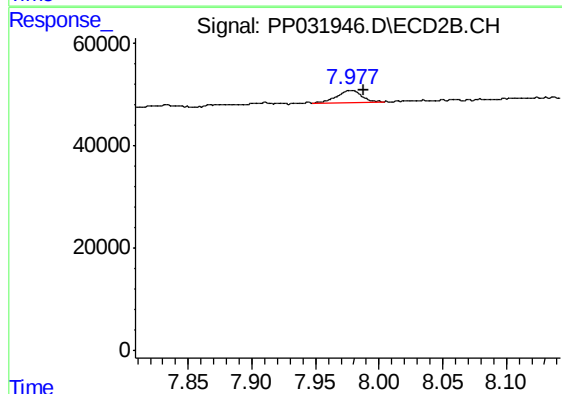


#35 AR-1260-5

R.T.: 7.977 min
Delta R.T.: -0.010 min
Response: 33442
Conc: 7.37 ng/ml

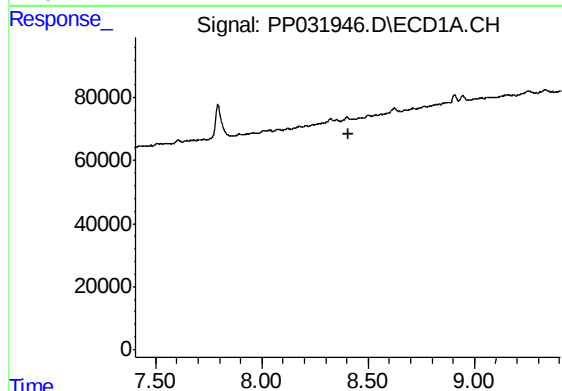


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.405 min
Response: 0
Conc: N.D.

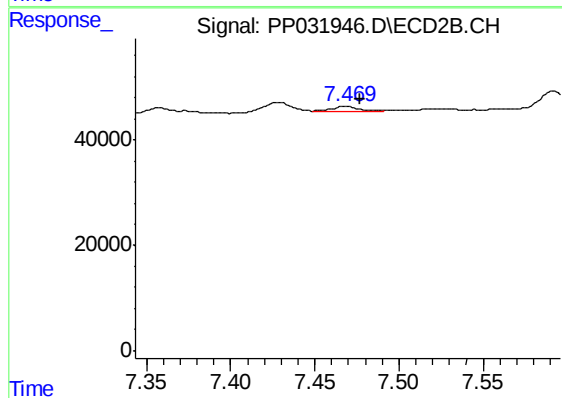

#36 AR-1262-1


R.T.: 7.469 min
Delta R.T.: -0.008 min
Response: 11629
Conc: 4.18 ng/ml

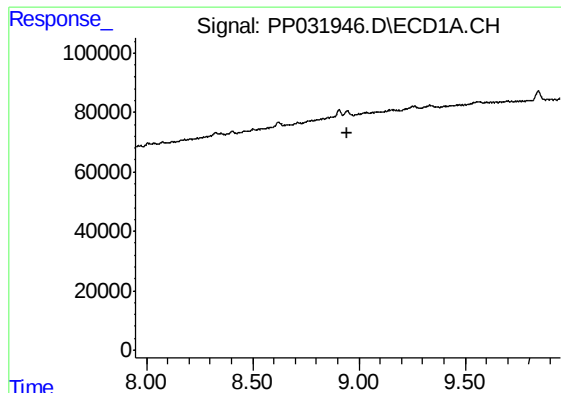

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR1-A-D-COMP

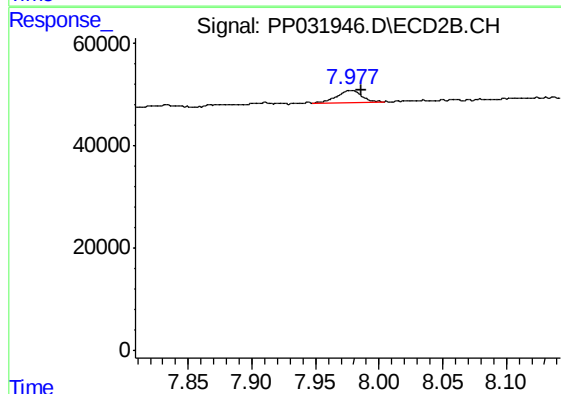


#37 AR-1262-2

R.T.: 7.977 min
Delta R.T.: -0.009 min
Response: 33442
Conc: 6.88 ng/ml

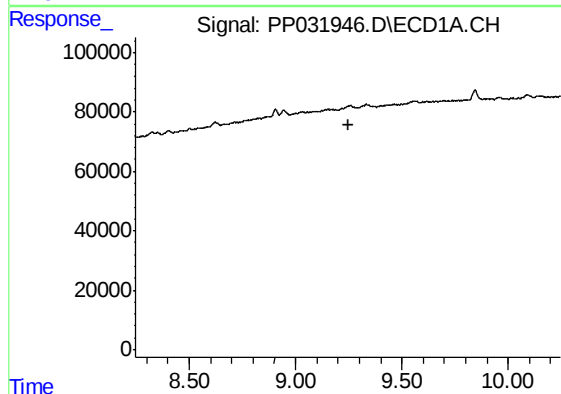


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.246 min
Response: 0
Conc: N.D.

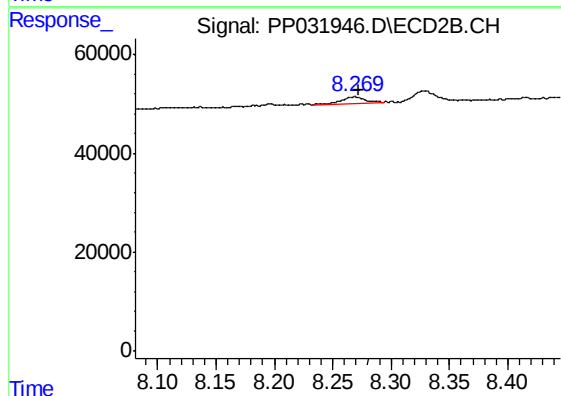

#38 AR-1262-3


R.T.: 8.269 min
Delta R.T.: -0.003 min
Response: 19579
Conc: 9.95 ng/ml

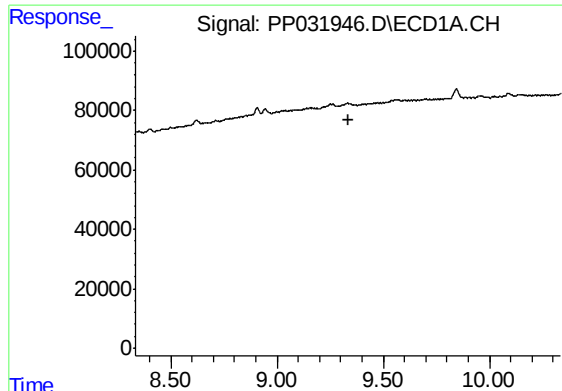

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 9.334 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR1-A-D-COMP

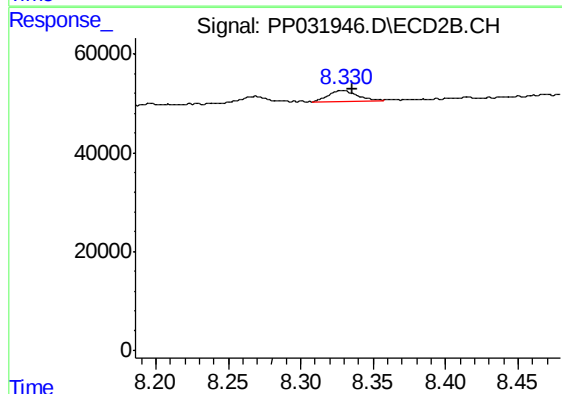


#39 AR-1262-4

R.T.: 8.330 min
Delta R.T.: -0.006 min
Response: 28792
Conc: 7.94 ng/ml

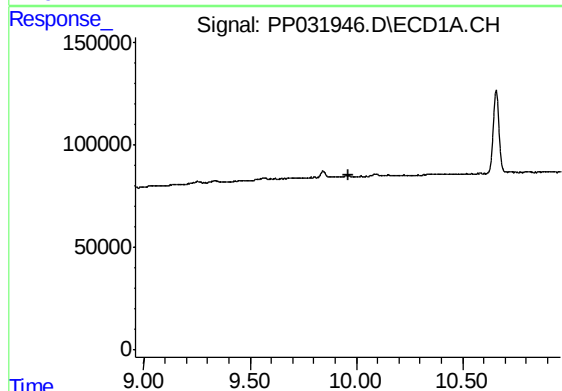


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.961 min
Response: 0
Conc: N.D.

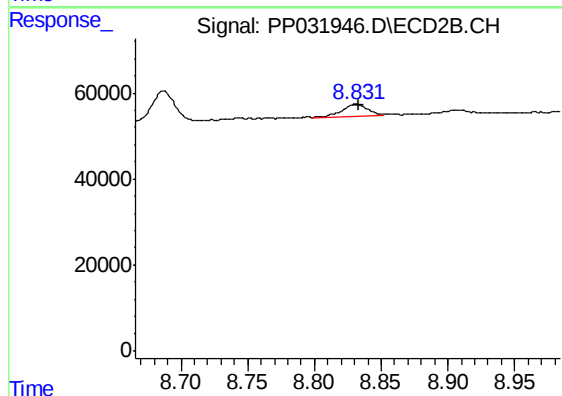

#40 AR-1262-5


R.T.: 8.831 min
Delta R.T.: -0.002 min
Response: 39756
Conc: 24.49 ng/ml

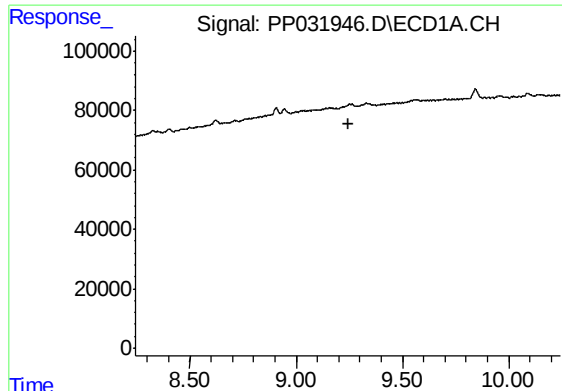

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 9.244 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR1-A-D-COMP

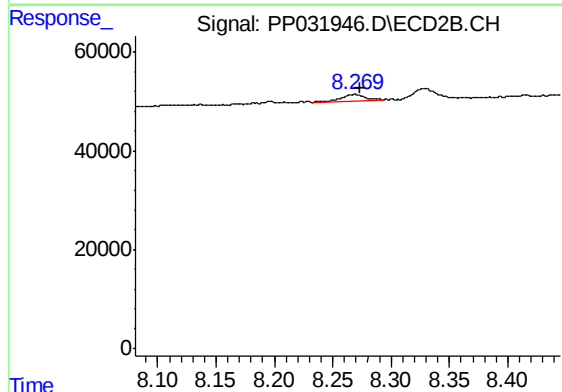


#41 AR-1268-1

R.T.: 8.269 min
Delta R.T.: -0.004 min
Response: 19579
Conc: 3.54 ng/ml

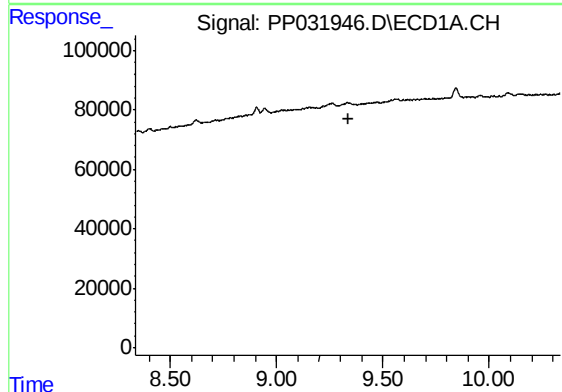


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.336 min
Response: 0
Conc: N.D.

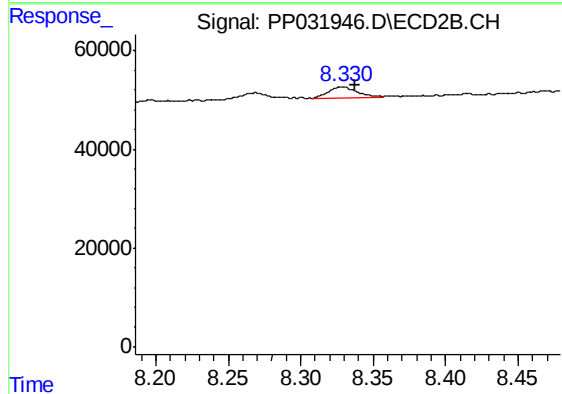

#42 AR-1268-2


R.T.: 8.330 min
Delta R.T.: -0.008 min
Response: 28792
Conc: 5.33 ng/ml

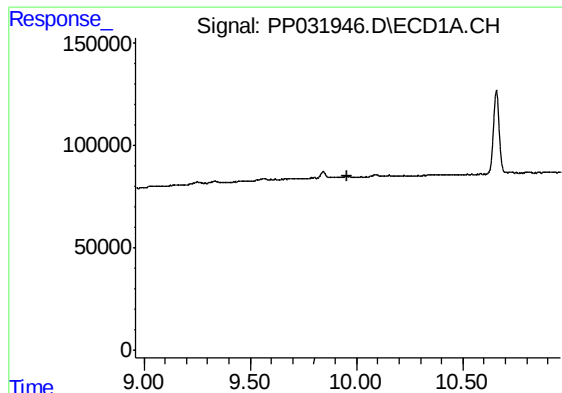

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 9.960 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR1-A-D-COMP

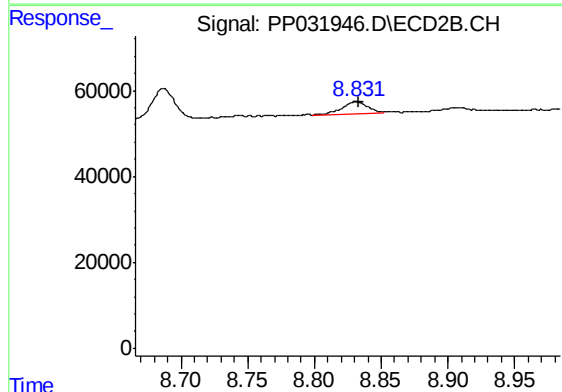


#44 AR-1268-4

R.T.: 8.831 min
Delta R.T.: -0.002 min
Response: 39756
Conc: 21.81 ng/ml

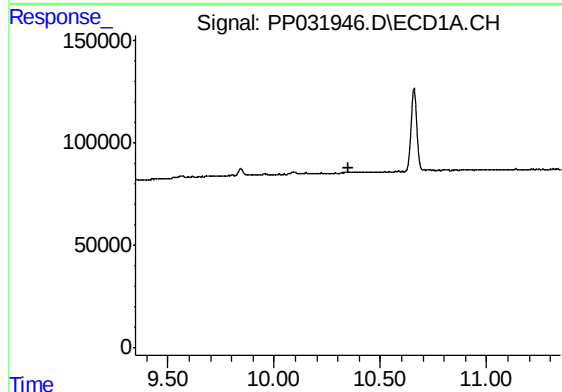

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.347 min
Response: 0
Conc: N.D.

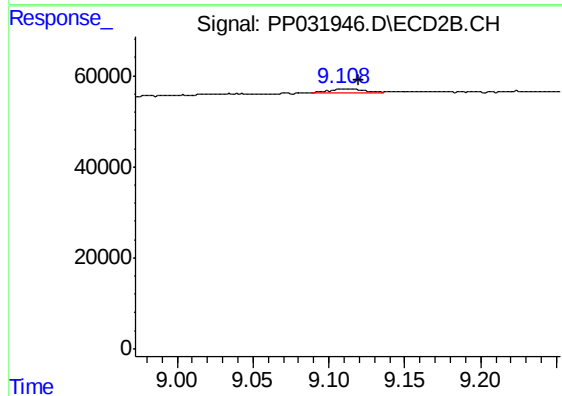

#45 AR-1268-5

R.T.: 9.109 min
Delta R.T.: -0.011 min
Response: 12669
Conc: 0.91 ng/ml