

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120920\
 Data File : PP031948.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Dec 2020 18:39
 Operator : DD\AJ
 Sample : L4984-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TR3-A-D-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 01:37:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.785	4.058	1232375	1093556	25.450	22.821
2)	SA Decachlor...	10.657	9.358	759438	821275	22.360	22.180
Target Compounds							
8)	L2 AR-1221-1	5.025	0.000	47984	0	88.230	N.D. #
9)	L2 AR-1221-2	0.000	4.404	0	31508	N.D.	81.680 #
20)	L4 AR-1242-5	0.000	6.186	0	10499	N.D.	10.176 #
26)	L6 AR-1254-1	0.000	6.186	0	10499	N.D.	4.853 #
27)	L6 AR-1254-2	0.000	6.342	0	12688	N.D.	6.811 #
28)	L6 AR-1254-3	7.603	6.762	31978	44702	12.658	14.461
29)	L6 AR-1254-4	0.000	7.001	0	25101	N.D.	14.775 #
30)	L6 AR-1254-5	8.324	7.429	-4294	81649	N.D.	30.245 #
31)	L7 AR-1260-1	0.000	6.899	0	25866	N.D.	13.090 #
32)	L7 AR-1260-2	0.000	7.094	0	23228	N.D.	9.538 #
33)	L7 AR-1260-3	0.000	7.247	0	26251	N.D.	11.495 #
34)	L7 AR-1260-4	0.000	7.734	0	12800	N.D.	6.736 #
35)	L7 AR-1260-5	0.000	7.975	0	32489	N.D.	7.159 #
36)	L8 AR-1262-1	0.000	7.455f	0	3512	N.D.	1.264 #
37)	L8 AR-1262-2	0.000	7.975	0	32489	N.D.	6.689 #
38)	L8 AR-1262-3	0.000	8.266	0	20698	N.D.	10.523 #
39)	L8 AR-1262-4	0.000	8.330	0	27953	N.D.	7.711 #
40)	L8 AR-1262-5	0.000	8.833	0	73471	N.D.	45.264 #
41)	L9 AR-1268-1	0.000	8.266	0	20698	N.D.	3.741 #
42)	L9 AR-1268-2	0.000	8.330	0	27953	N.D.	5.170 #
44)	L9 AR-1268-4	0.000	8.833	0	73471	N.D.	40.309 #
45)	L9 AR-1268-5	0.000	9.112	0	27782	N.D.	2.006 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120920\
Data File : PP031948.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Dec 2020 18:39
Operator : DD\AJ
Sample : L4984-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TR3-A-D-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 01:37:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

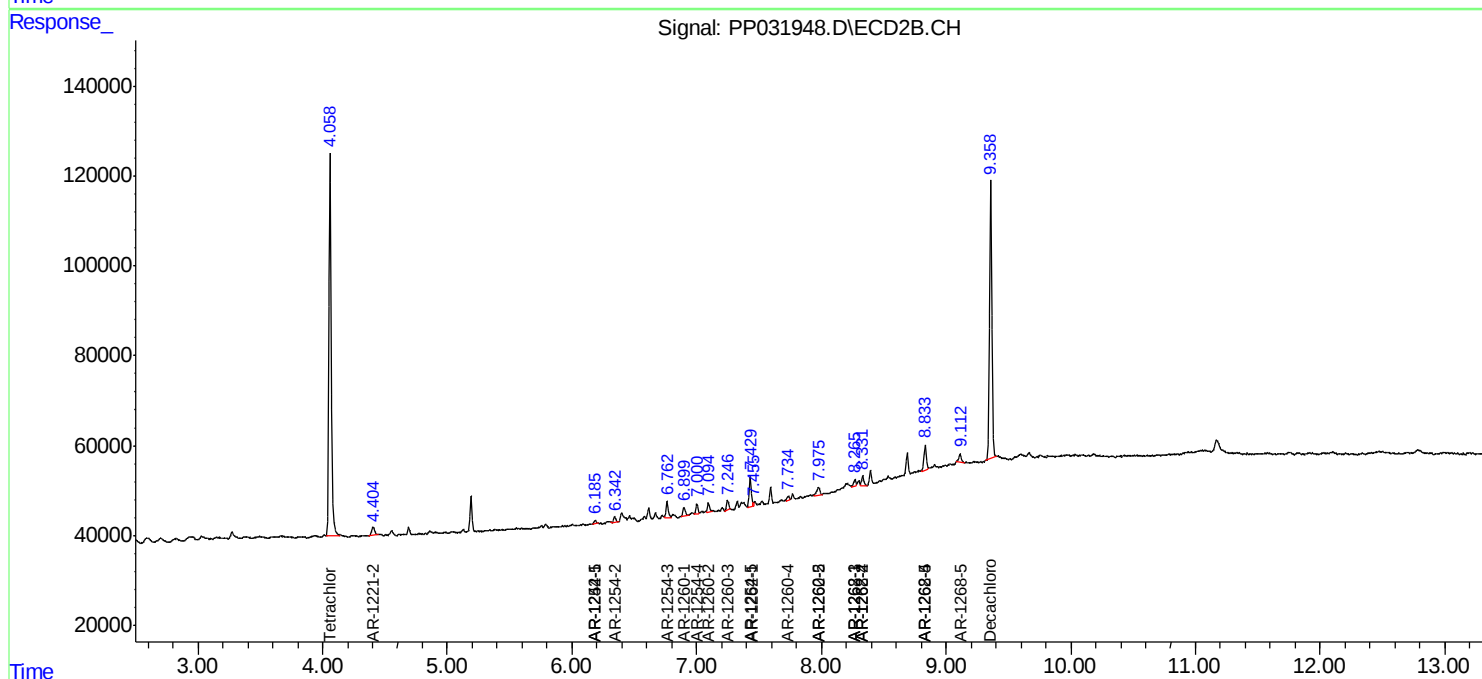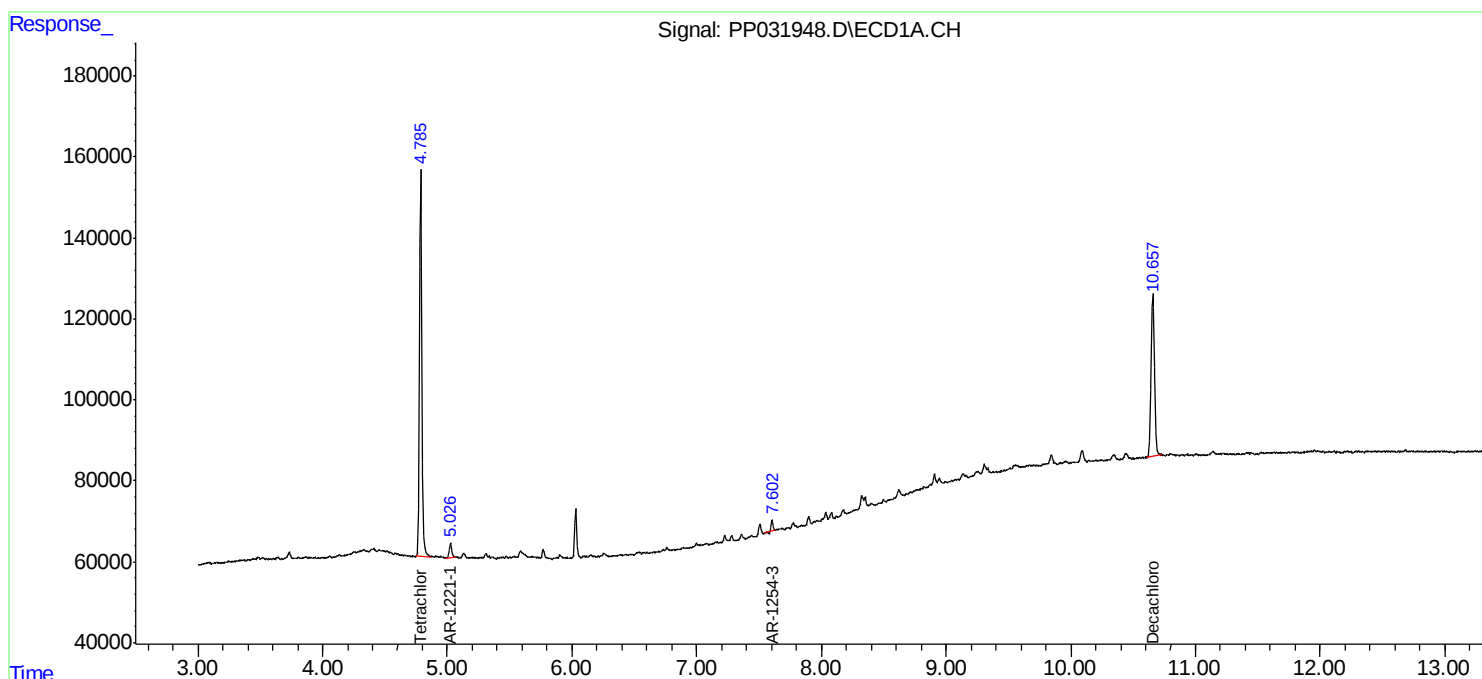


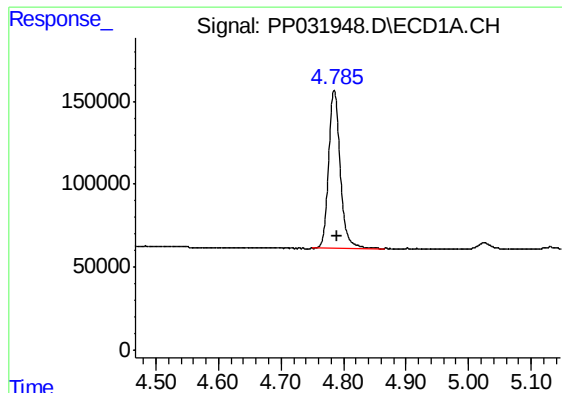

#1 Tetrachloro-m-xylene


R.T.: 4.785 min
Delta R.T.: -0.005 min
Response: 1232375
Conc: 25.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
TR3-A-D-COMP

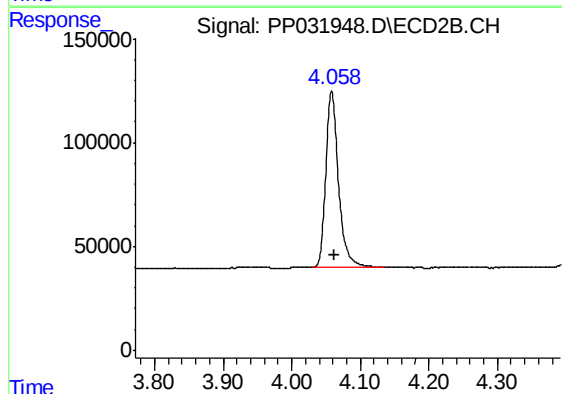


#1 Tetrachloro-m-xylene

R.T.: 4.058 min
Delta R.T.: -0.003 min
Response: 1093556
Conc: 22.82 ng/ml

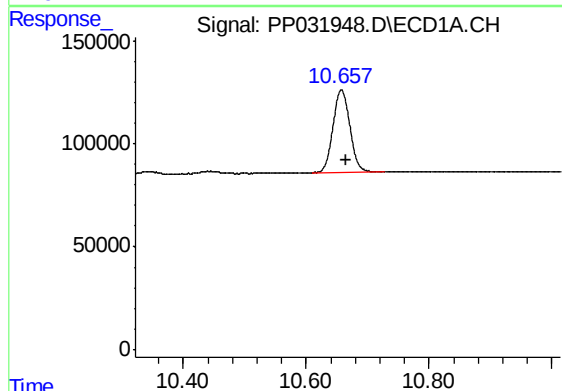


#2 Decachlorobiphenyl

R.T.: 10.657 min
Delta R.T.: -0.008 min
Response: 759438
Conc: 22.36 ng/ml

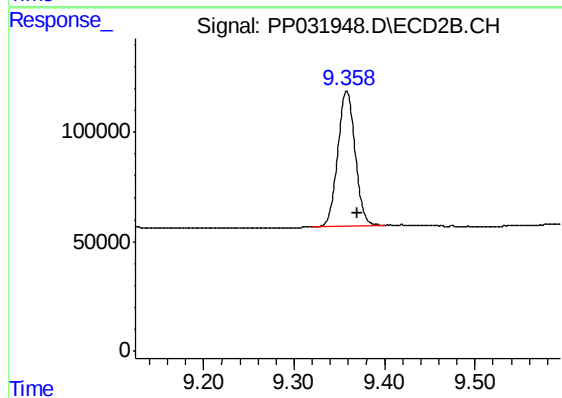

#2 Decachlorobiphenyl


R.T.: 9.358 min
Delta R.T.: -0.012 min
Response: 821275
Conc: 22.18 ng/ml

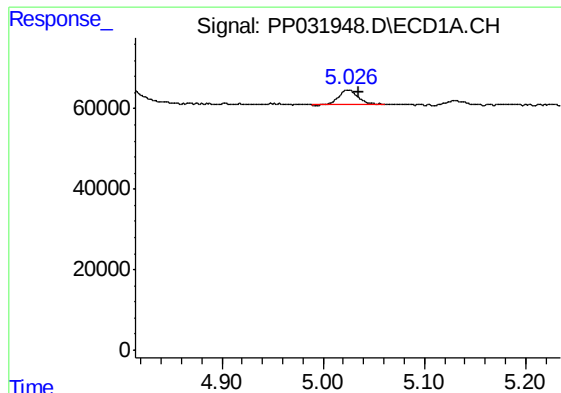

#8 AR-1221-1


R.T.: 5.025 min
Delta R.T.: -0.010 min
Response: 47984
Conc: 88.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
TR3-A-D-COMP

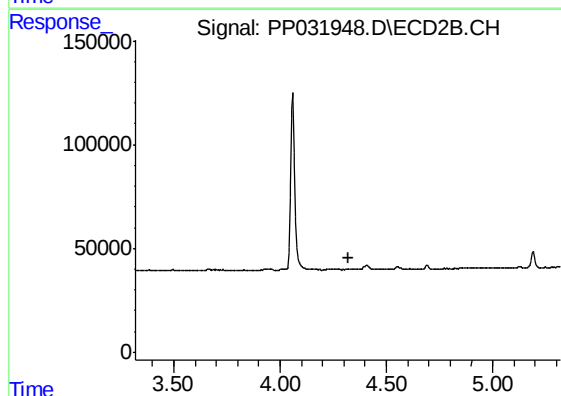


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.319 min
Response: 0
Conc: N.D.

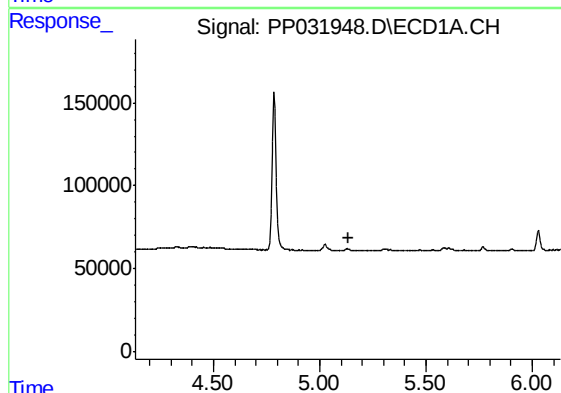


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.133 min
Response: 0
Conc: N.D.

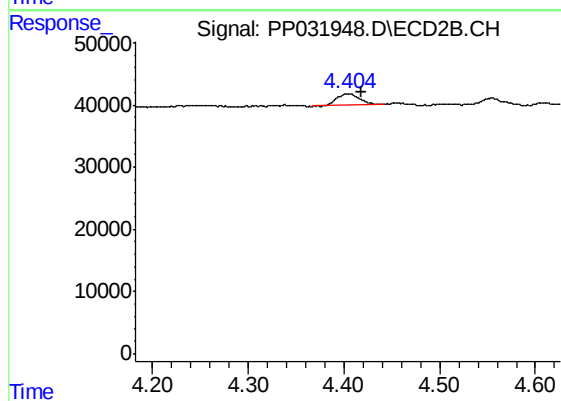

#9 AR-1221-2


R.T.: 4.404 min
Delta R.T.: -0.014 min
Response: 31508
Conc: 81.68 ng/ml

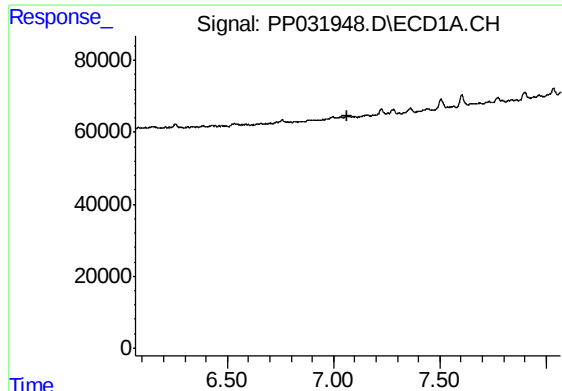

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 7.067 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR3-A-D-COMP

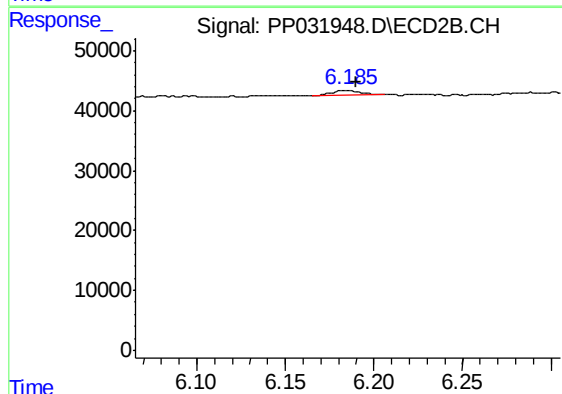


#20 AR-1242-5

R.T.: 6.186 min
Delta R.T.: -0.004 min
Response: 10499
Conc: 10.18 ng/ml

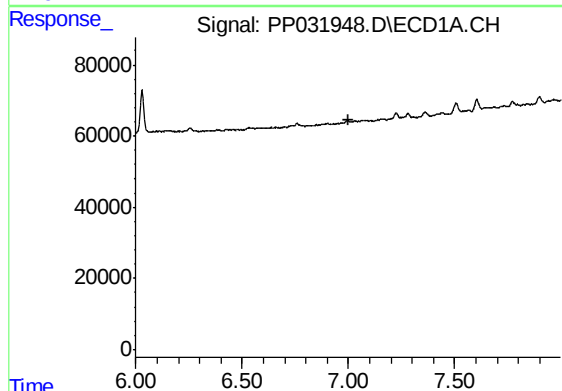


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.998 min
Response: 0
Conc: N.D.

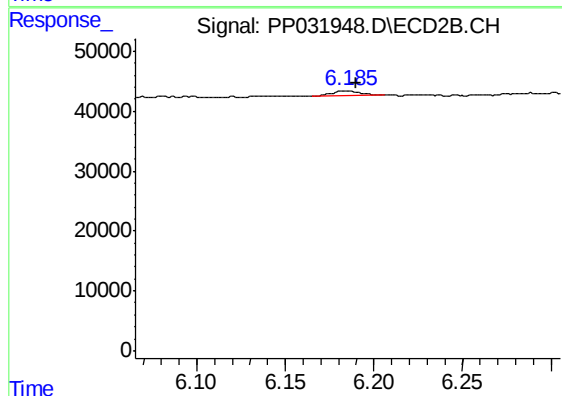

#26 AR-1254-1


R.T.: 6.186 min
Delta R.T.: -0.004 min
Response: 10499
Conc: 4.85 ng/ml

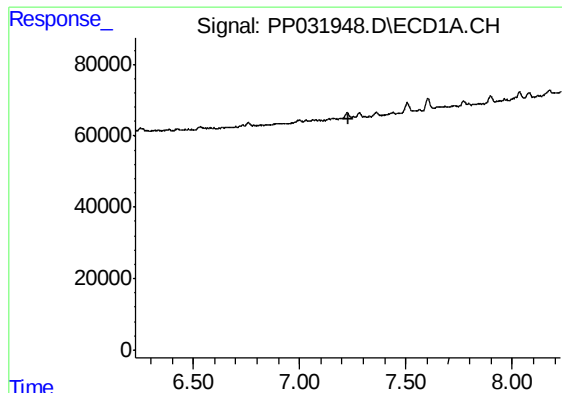

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 7.228 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR3-A-D-COMP

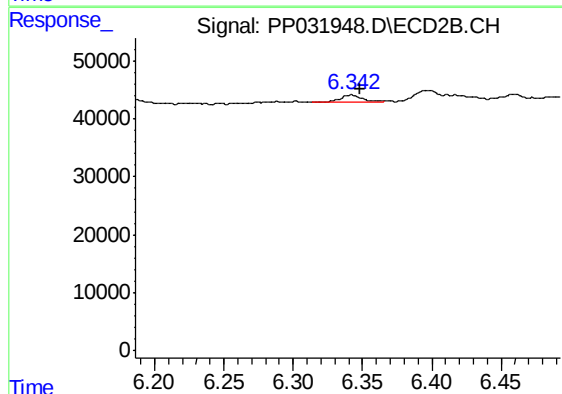


#27 AR-1254-2

R.T.: 6.342 min
Delta R.T.: -0.007 min
Response: 12688
Conc: 6.81 ng/ml

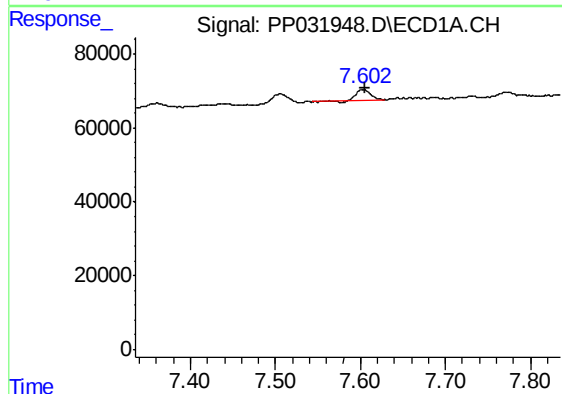


#28 AR-1254-3

R.T.: 7.603 min
Delta R.T.: -0.003 min
Response: 31978
Conc: 12.66 ng/ml

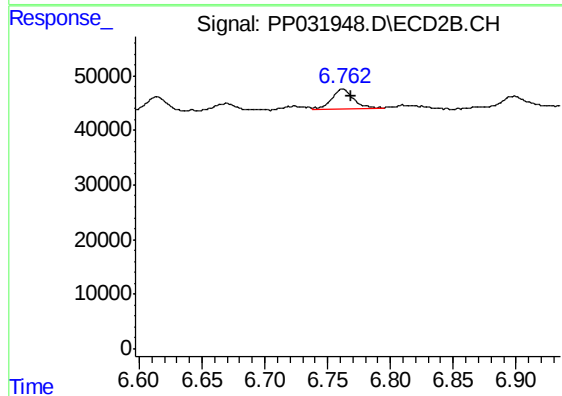

#28 AR-1254-3


R.T.: 6.762 min
Delta R.T.: -0.007 min
Response: 44702
Conc: 14.46 ng/ml

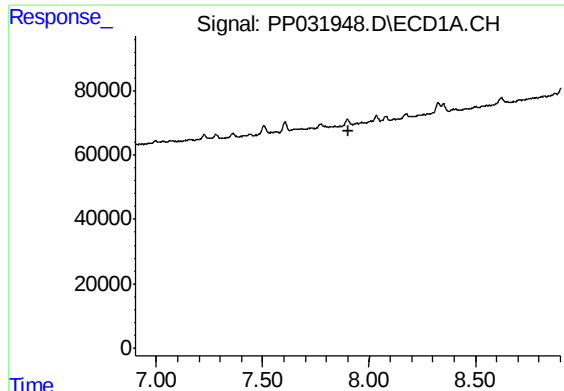

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.901 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR3-A-D-COMP

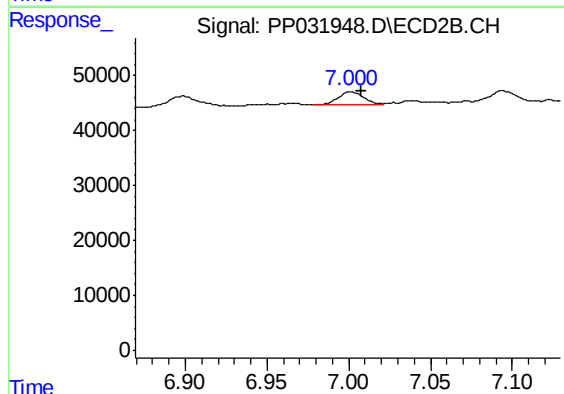


#29 AR-1254-4

R.T.: 7.001 min
Delta R.T.: -0.007 min
Response: 25101
Conc: 14.77 ng/ml

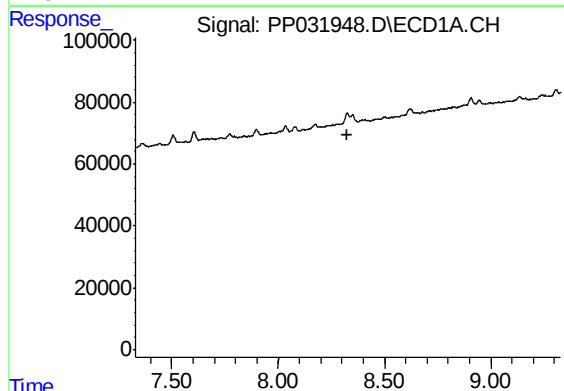


#30 AR-1254-5

R.T.: 8.324 min
Delta R.T.: -0.004 min
Response: -4294
Conc: N.D.

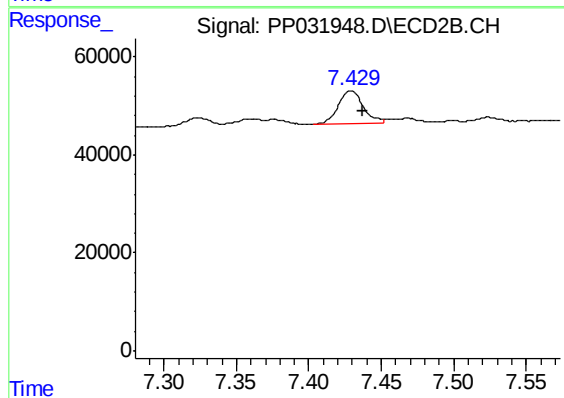

#30 AR-1254-5


R.T.: 7.429 min
Delta R.T.: -0.007 min
Response: 81649
Conc: 30.24 ng/ml

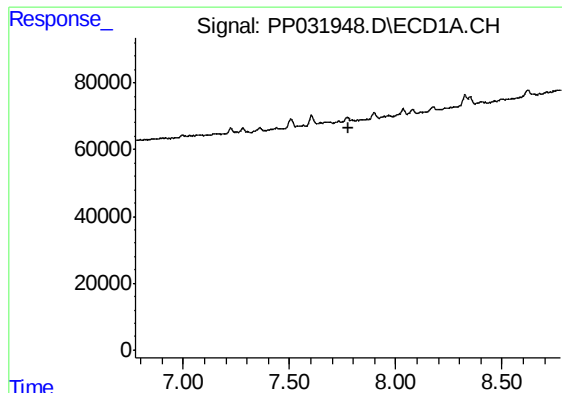

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 7.775 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR3-A-D-COMP

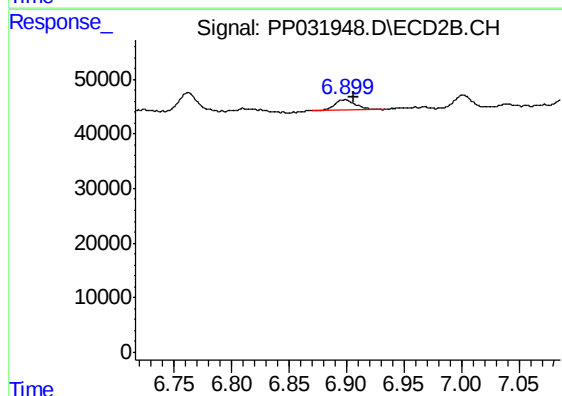


#31 AR-1260-1

R.T.: 6.899 min
Delta R.T.: -0.007 min
Response: 25866
Conc: 13.09 ng/ml

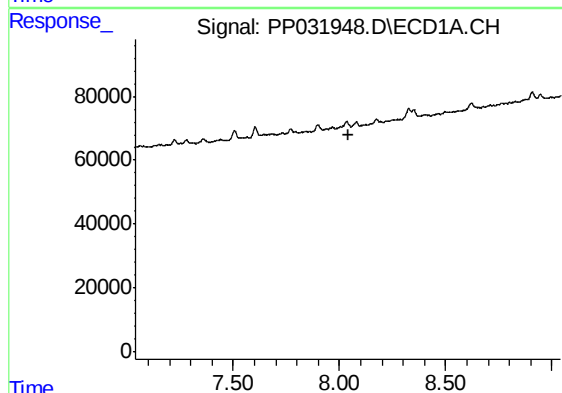


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.040 min
Response: 0
Conc: N.D.

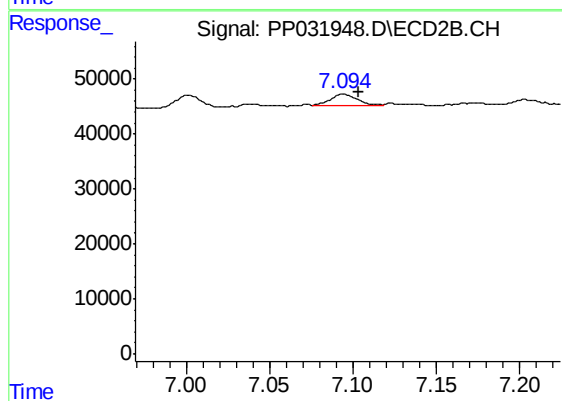

#32 AR-1260-2


R.T.: 7.094 min
Delta R.T.: -0.009 min
Response: 23228
Conc: 9.54 ng/ml

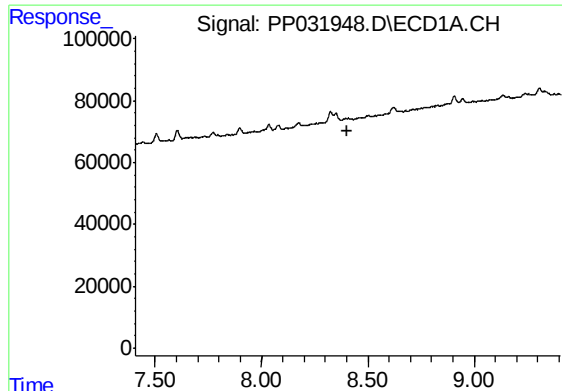

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.406 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR3-A-D-COMP

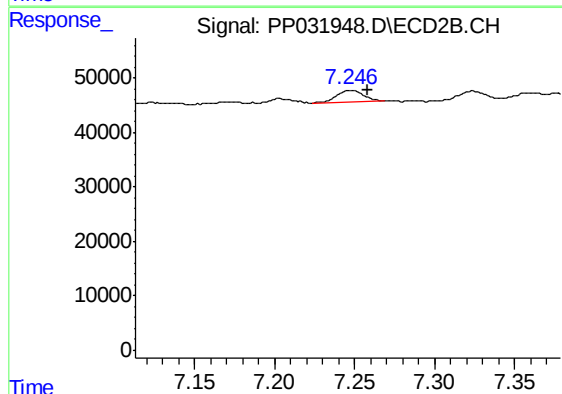


#33 AR-1260-3

R.T.: 7.247 min
Delta R.T.: -0.011 min
Response: 26251
Conc: 11.50 ng/ml

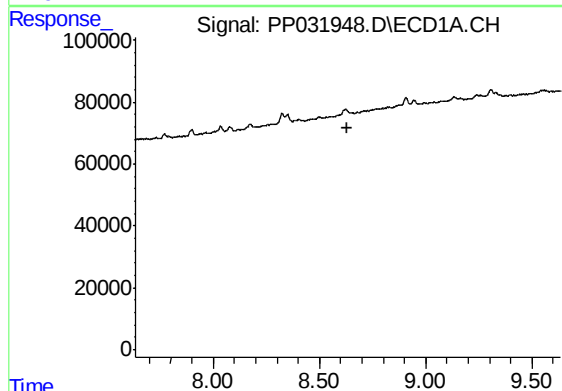


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 8.634 min
Response: 0
Conc: N.D.

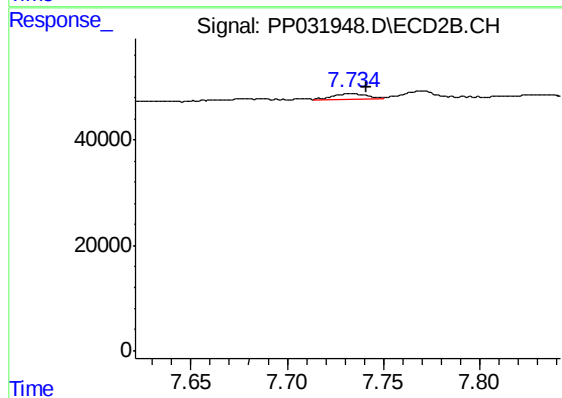

#34 AR-1260-4


R.T.: 7.734 min
Delta R.T.: -0.008 min
Response: 12800
Conc: 6.74 ng/ml

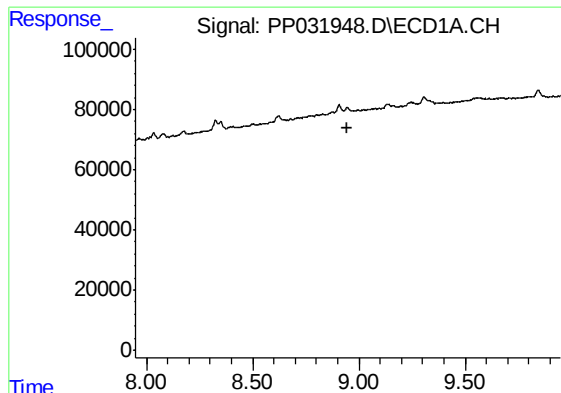

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR3-A-D-COMP

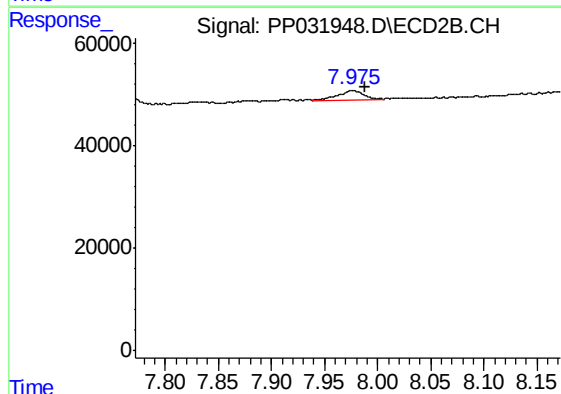


#35 AR-1260-5

R.T.: 7.975 min
Delta R.T.: -0.012 min
Response: 32489
Conc: 7.16 ng/ml

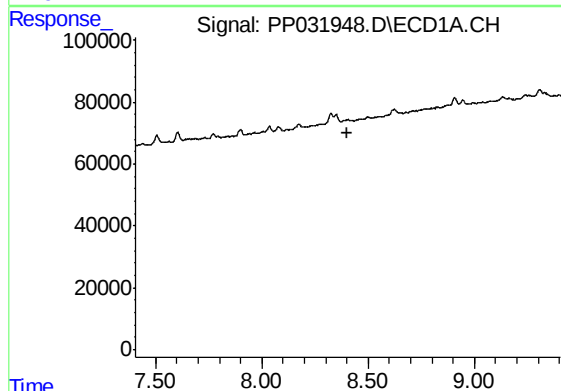


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.405 min
Response: 0
Conc: N.D.

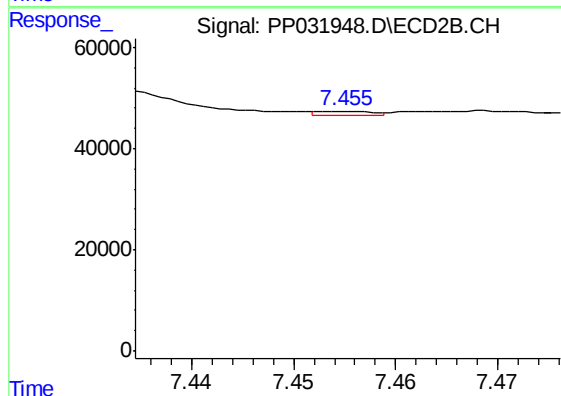

#36 AR-1262-1


R.T.: 7.455 min
Delta R.T.: -0.022 min
Response: 3512
Conc: 1.26 ng/ml

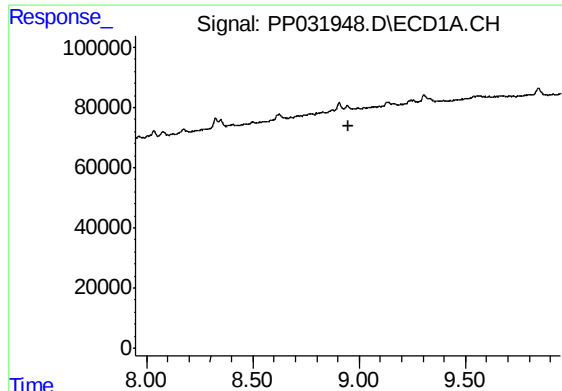

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR3-A-D-COMP

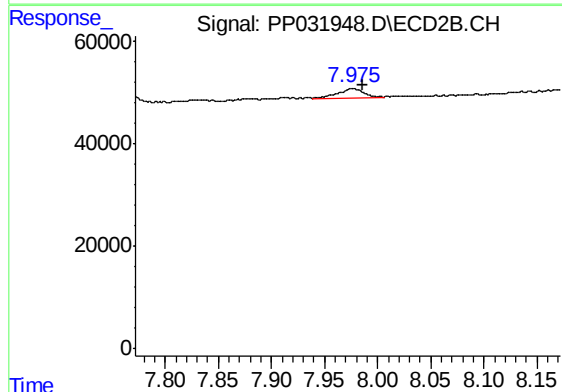


#37 AR-1262-2

R.T.: 7.975 min
Delta R.T.: -0.011 min
Response: 32489
Conc: 6.69 ng/ml

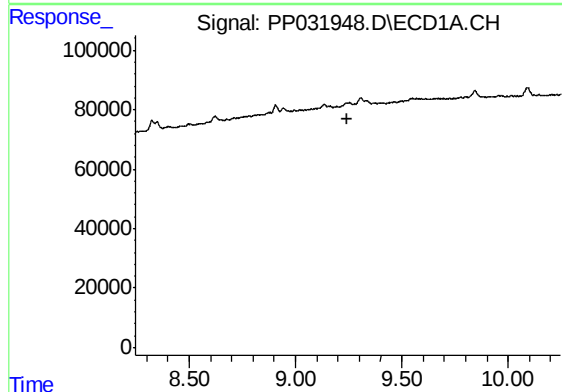


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.246 min
Response: 0
Conc: N.D.

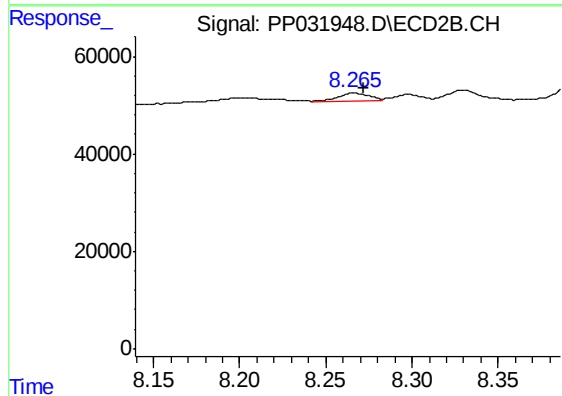

#38 AR-1262-3


R.T.: 8.266 min
Delta R.T.: -0.006 min
Response: 20698
Conc: 10.52 ng/ml

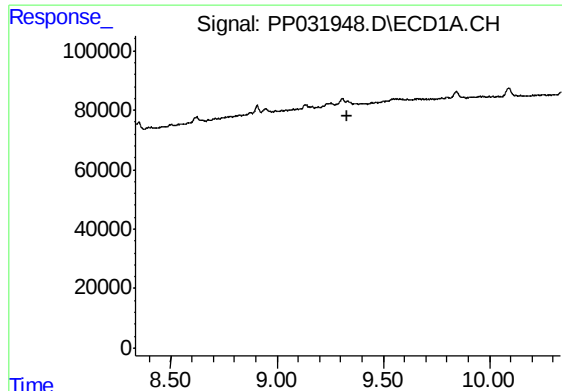

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 9.334 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR3-A-D-COMP

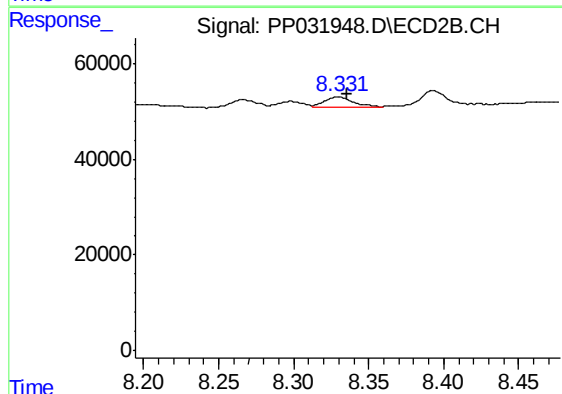


#39 AR-1262-4

R.T.: 8.330 min
Delta R.T.: -0.006 min
Response: 27953
Conc: 7.71 ng/ml

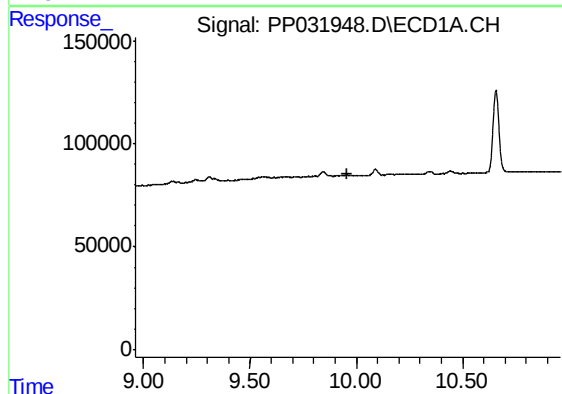


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.961 min
Response: 0
Conc: N.D.

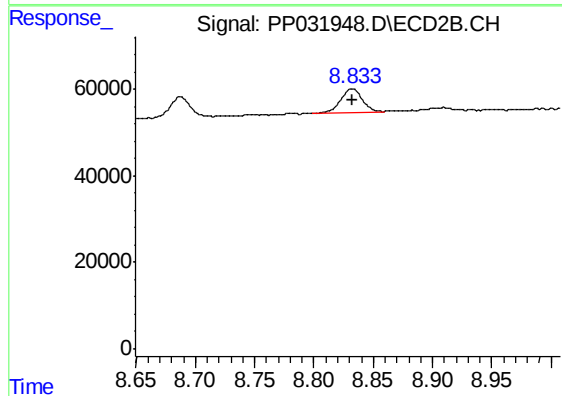

#40 AR-1262-5


R.T.: 8.833 min
Delta R.T.: 0.000 min
Response: 73471
Conc: 45.26 ng/ml

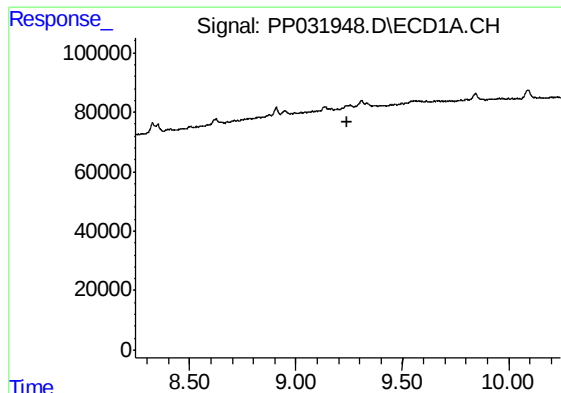

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 9.244 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR3-A-D-COMP

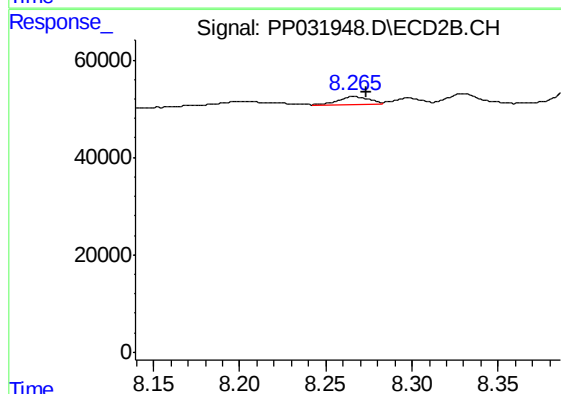


#41 AR-1268-1

R.T.: 8.266 min
Delta R.T.: -0.007 min
Response: 20698
Conc: 3.74 ng/ml

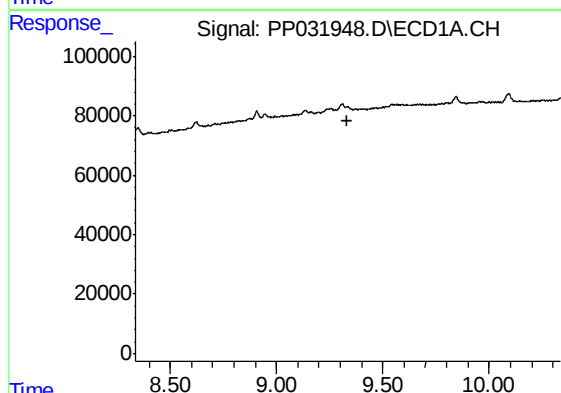


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.336 min
Response: 0
Conc: N.D.

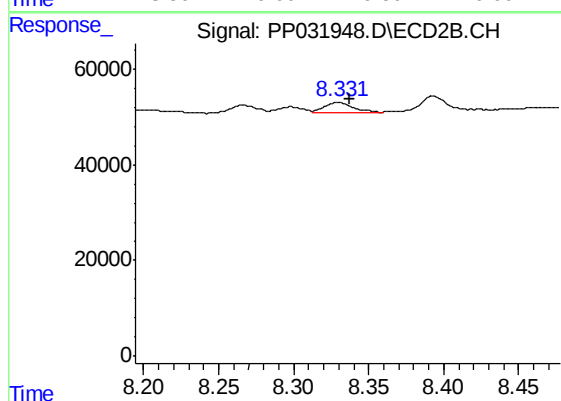

#42 AR-1268-2


R.T.: 8.330 min
Delta R.T.: -0.007 min
Response: 27953
Conc: 5.17 ng/ml

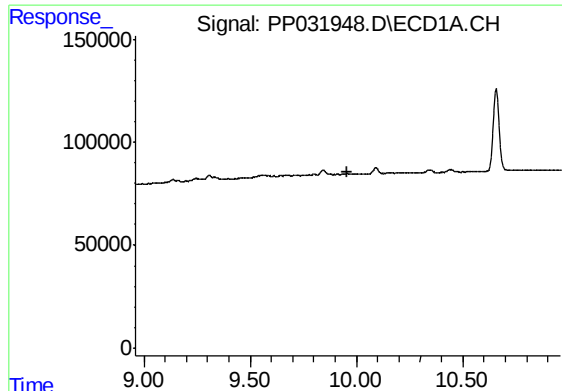

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 9.960 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TR3-A-D-COMP

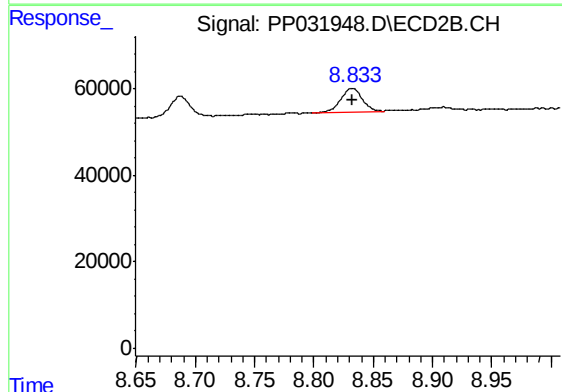


#44 AR-1268-4

R.T.: 8.833 min
Delta R.T.: 0.000 min
Response: 73471
Conc: 40.31 ng/ml

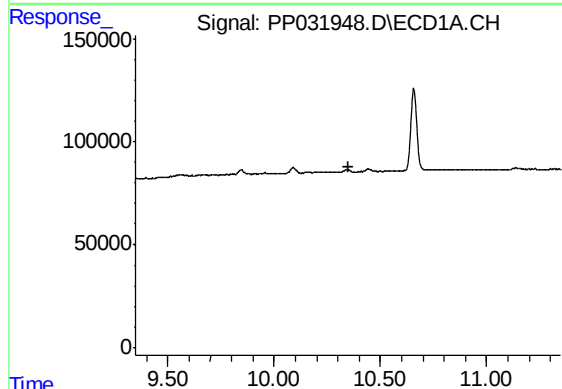

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.347 min
Response: 0
Conc: N.D.

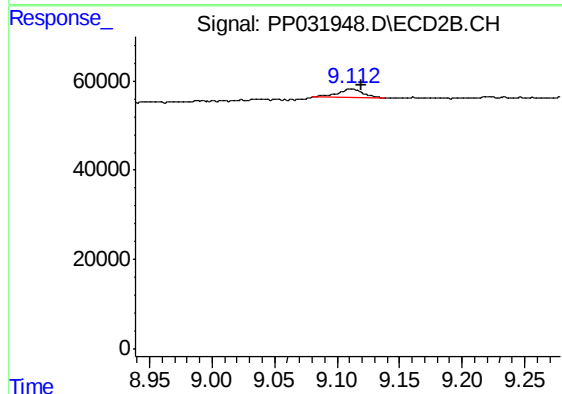

#45 AR-1268-5

R.T.: 9.112 min
Delta R.T.: -0.008 min
Response: 27782
Conc: 2.01 ng/ml