

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120920\
 Data File : PP031926.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Dec 2020 10:33
 Operator : DD\AJ
 Sample : L4969-03RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 NORTH-BRANFORD-03RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 01:23:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.786	4.057	1684147	1485831	34.780	31.007
2) SA Decachlor...	10.656	9.358	1216422	1245208	35.815	33.630

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120920\
Data File : PP031926.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Dec 2020 10:33
Operator : DD\AJ
Sample : L4969-03RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
NORTH-BRANFORD-03RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 01:23:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

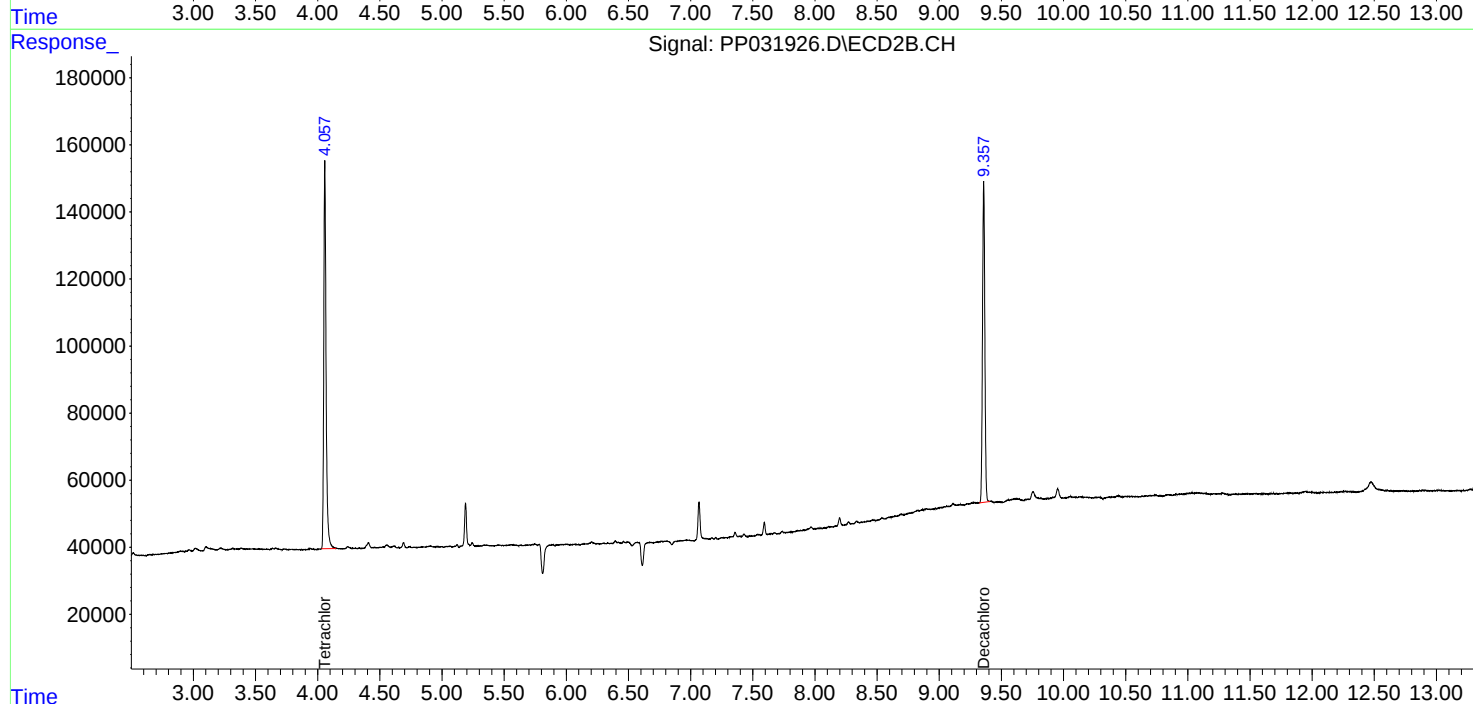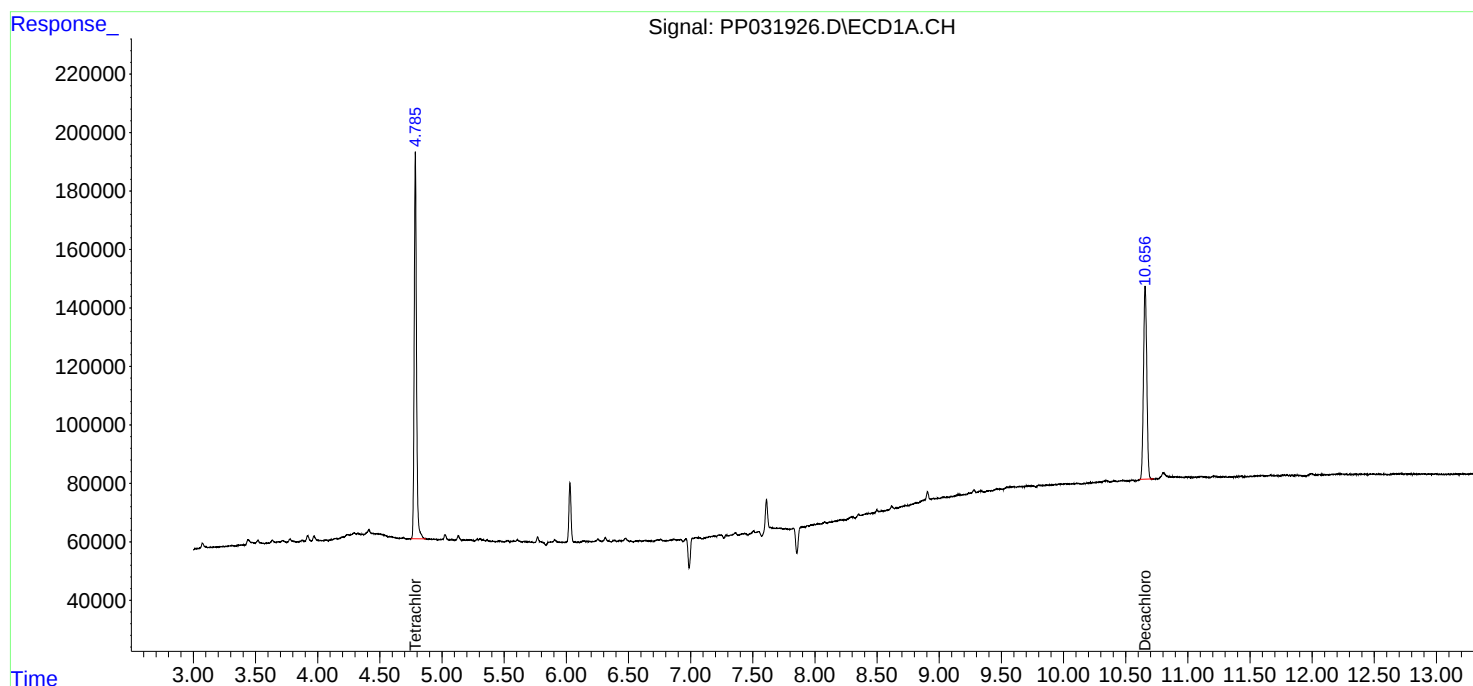


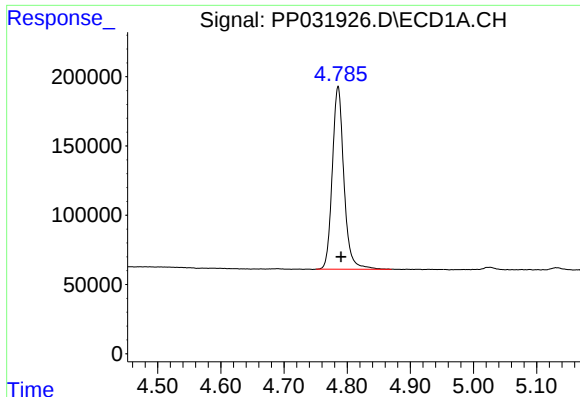

#1 Tetrachloro-m-xylene


R.T.: 4.786 min
Delta R.T.: -0.004 min
Response: 1684147
Conc: 34.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
NORTH-BRANFORD-03RE

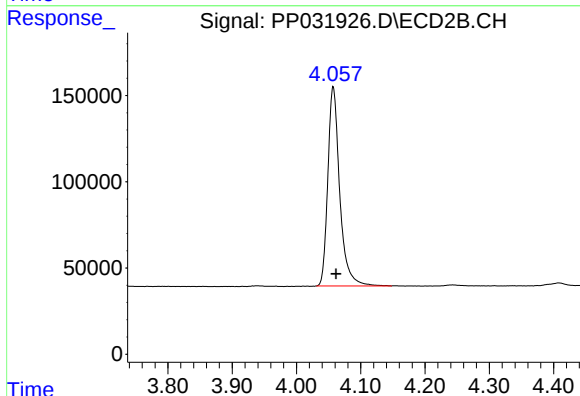


#1 Tetrachloro-m-xylene

R.T.: 4.057 min
Delta R.T.: -0.004 min
Response: 1485831
Conc: 31.01 ng/ml

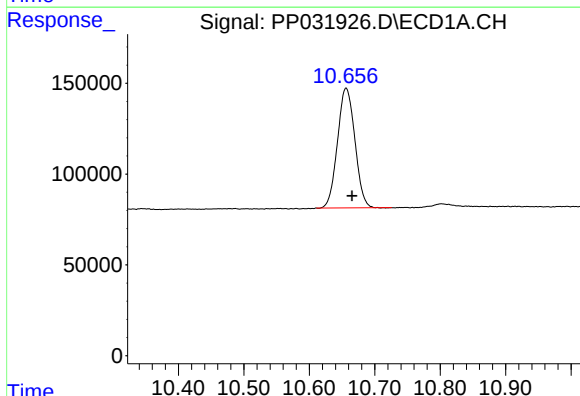

#2 Decachlorobiphenyl

R.T.: 10.656 min
Delta R.T.: -0.009 min
Response: 1216422
Conc: 35.81 ng/ml

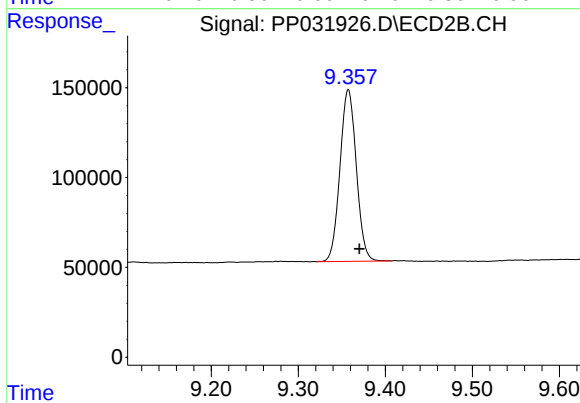

#2 Decachlorobiphenyl

R.T.: 9.358 min
Delta R.T.: -0.013 min
Response: 1245208
Conc: 33.63 ng/ml