

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120920\
 Data File : PP031931.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Dec 2020 13:55
 Operator : DD\AJ
 Sample : L4913-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TEST-PIT-3

Manual Integrations
 APPROVED

Ankita
 12/10/2020 12:04:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 01:26:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.785	4.058	913952	847222	18.874m	17.680m
2) SA Decachlor...	10.657	9.358	579148	657941	17.052	17.769
Target Compounds						
26) L6 AR-1254-1	6.994	6.183	375658	446700	246.517	206.499
27) L6 AR-1254-2	7.225	6.341	1201488	349139	517.339	187.408 #
28) L6 AR-1254-3	7.604	6.762	954868	625853	377.966	202.459 #
29) L6 AR-1254-4	7.897	7.001	357503	307429	210.692	180.958
30) L6 AR-1254-5	8.324	7.429	615272	806823	329.126	298.870

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120920\
Data File : PP031931.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Dec 2020 13:55
Operator : DD\AJ
Sample : L4913-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
TEST-PIT-3


Manual Integrations
APPROVED

Ankita
12/10/2020 12:04:32 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 01:26:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

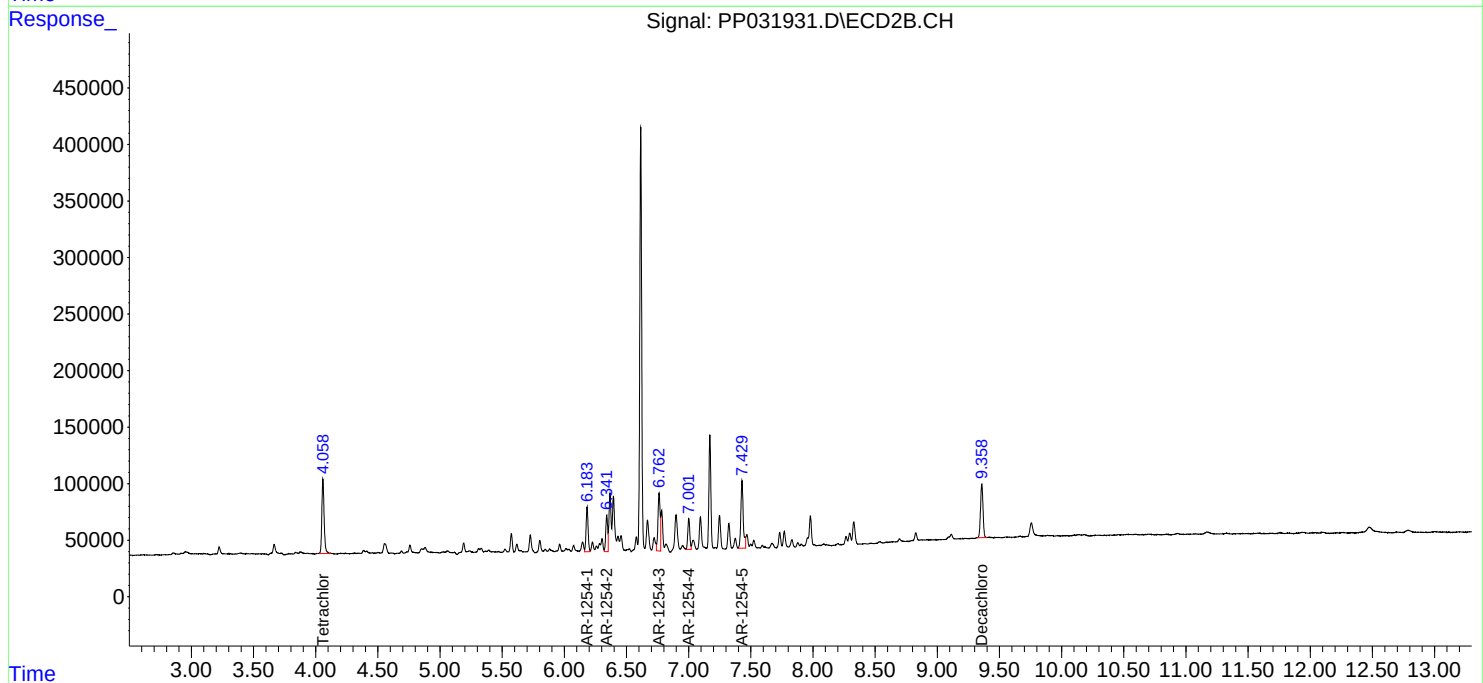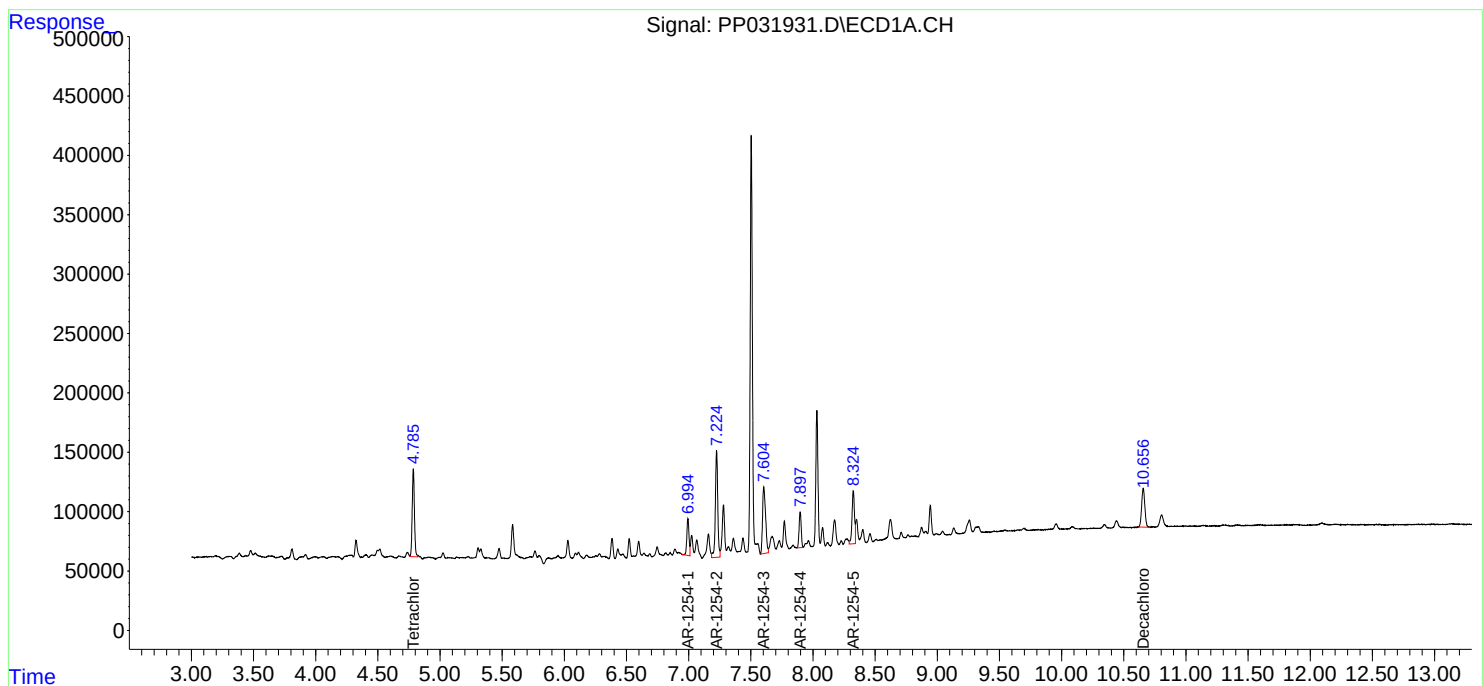

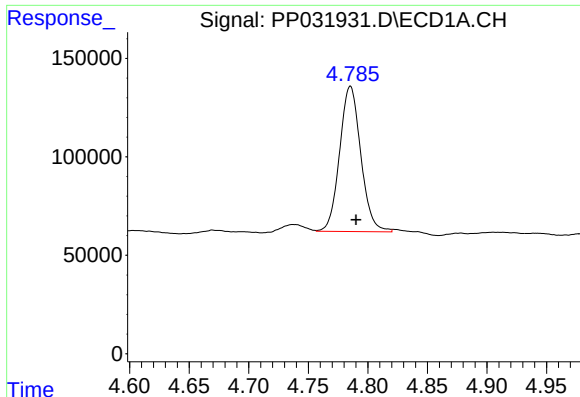


#1 Tetrachloro-m-xylene

R.T.: 4.785 min
Delta R.T.: -0.005 min
Response: 913952
Conc: 18.87 ng/ml m

Instrument :
ECD_P
ClientSampleId :
TEST-PIT-3


Manual Integrations
APPROVED

Ankita
12/10/2020 12:04:32 PM

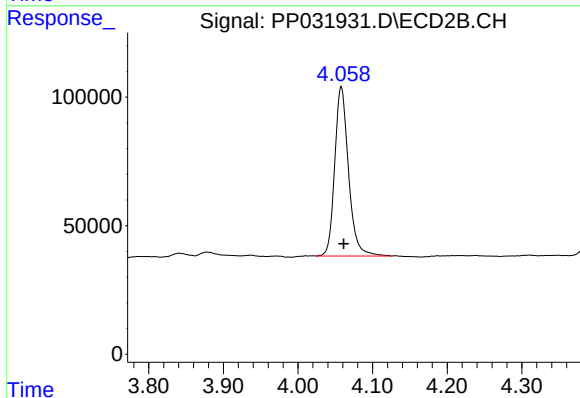


#1 Tetrachloro-m-xylene

R.T.: 4.058 min
Delta R.T.: -0.004 min
Response: 847222
Conc: 17.68 ng/ml m

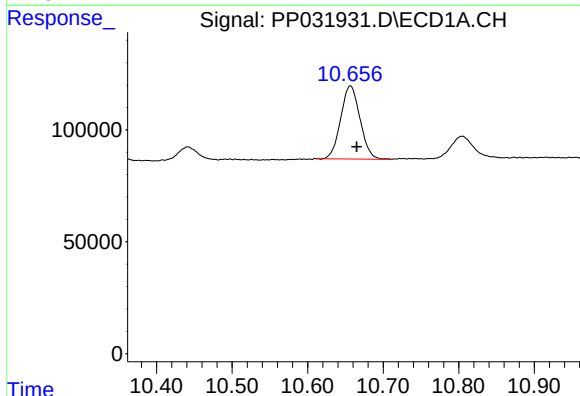


#2 Decachlorobiphenyl

R.T.: 10.657 min
Delta R.T.: -0.008 min
Response: 579148
Conc: 17.05 ng/ml

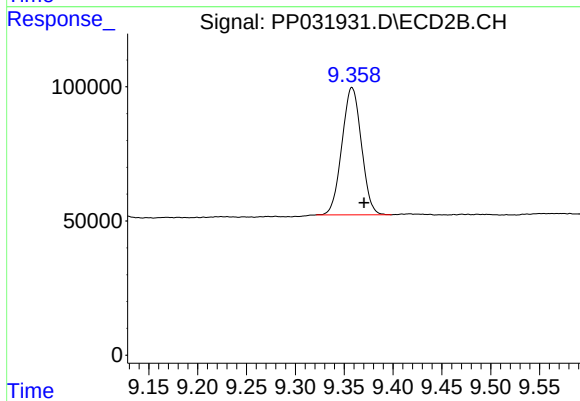

#2 Decachlorobiphenyl

R.T.: 9.358 min
Delta R.T.: -0.012 min
Response: 657941
Conc: 17.77 ng/ml

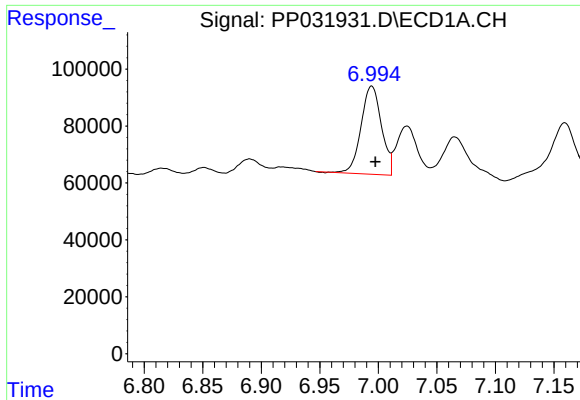


#26 AR-1254-1

R.T.: 6.994 min
Delta R.T.: -0.003 min
Response: 375658
Conc: 246.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
TEST-PIT-3


Manual Integrations
APPROVED

Ankita
12/10/2020 12:04:32 PM

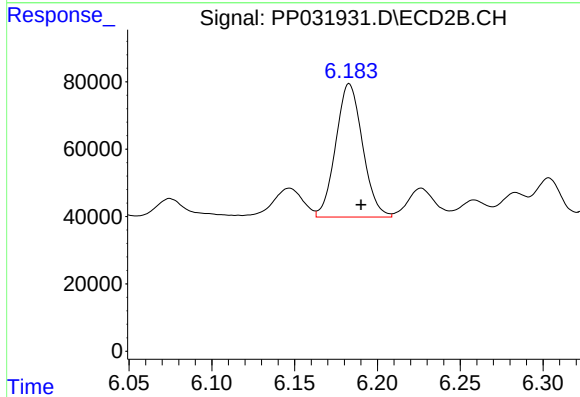


#26 AR-1254-1

R.T.: 6.183 min
Delta R.T.: -0.007 min
Response: 446700
Conc: 206.50 ng/ml

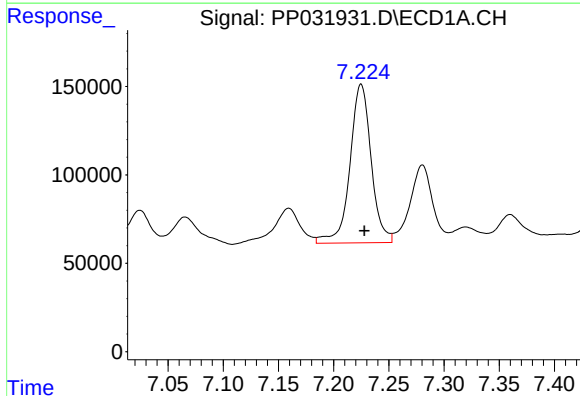


#27 AR-1254-2

R.T.: 7.225 min
Delta R.T.: -0.003 min
Response: 1201488
Conc: 517.34 ng/ml

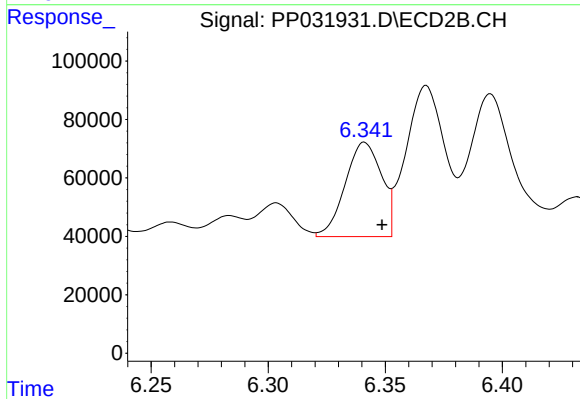

#27 AR-1254-2

R.T.: 6.341 min
Delta R.T.: -0.007 min
Response: 349139
Conc: 187.41 ng/ml

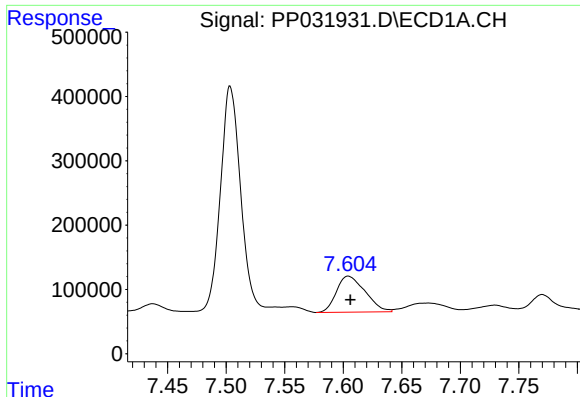


#28 AR-1254-3

R.T.: 7.604 min
Delta R.T.: -0.002 min
Response: 954868
Conc: 377.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
TEST-PIT-3


Manual Integrations
APPROVED

Ankita
12/10/2020 12:04:32 PM

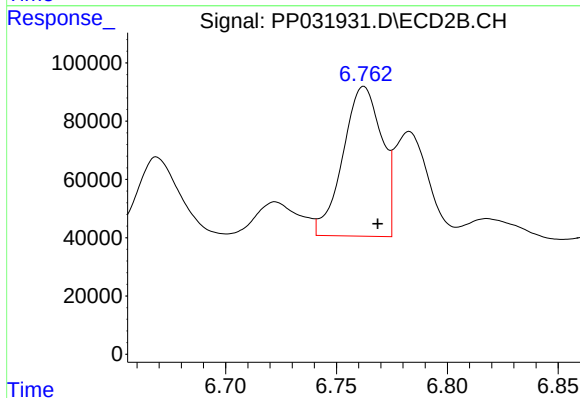


#28 AR-1254-3

R.T.: 6.762 min
Delta R.T.: -0.006 min
Response: 625853
Conc: 202.46 ng/ml

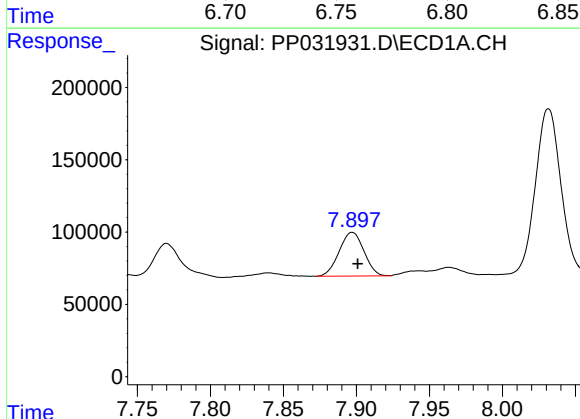


#29 AR-1254-4

R.T.: 7.897 min
Delta R.T.: -0.004 min
Response: 357503
Conc: 210.69 ng/ml

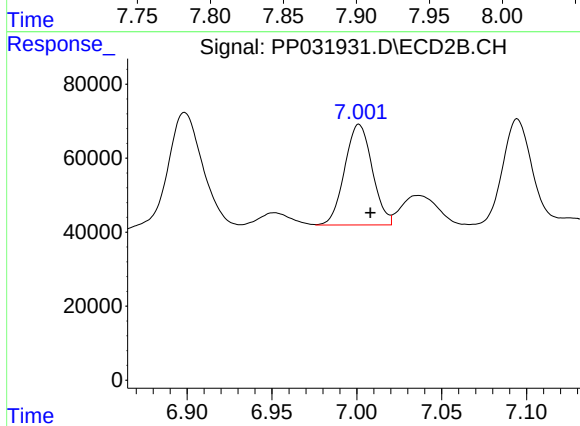

#29 AR-1254-4

R.T.: 7.001 min
Delta R.T.: -0.007 min
Response: 307429
Conc: 180.96 ng/ml

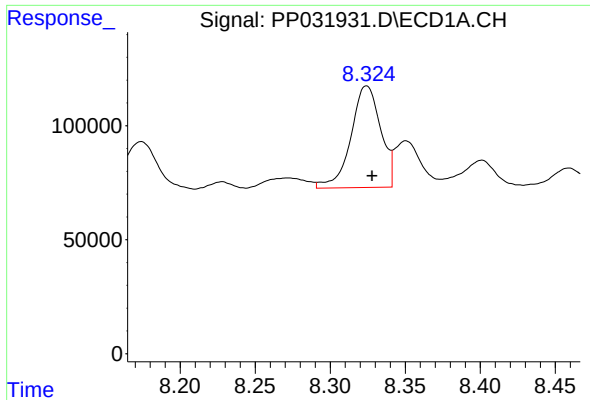


#30 AR-1254-5

R.T.: 8.324 min
Delta R.T.: -0.004 min
Response: 615272
Conc: 329.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
TEST-PIT-3

Manual Integrations
APPROVED

Ankita
12/10/2020 12:04:32 PM

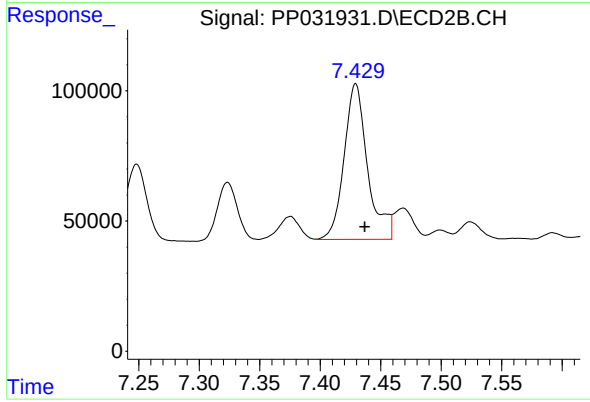

#30 AR-1254-5

R.T.: 7.429 min
Delta R.T.: -0.007 min
Response: 806823
Conc: 298.87 ng/ml