

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120920\
 Data File : PP031953.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Dec 2020 20:19
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 01:40:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.785	4.057	1297051	1170037	26.786	24.417
2) SA Decachlor...	10.657	9.357	869070	932436	25.588	25.182

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120920\
Data File : PP031953.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Dec 2020 20:19
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 01:40:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

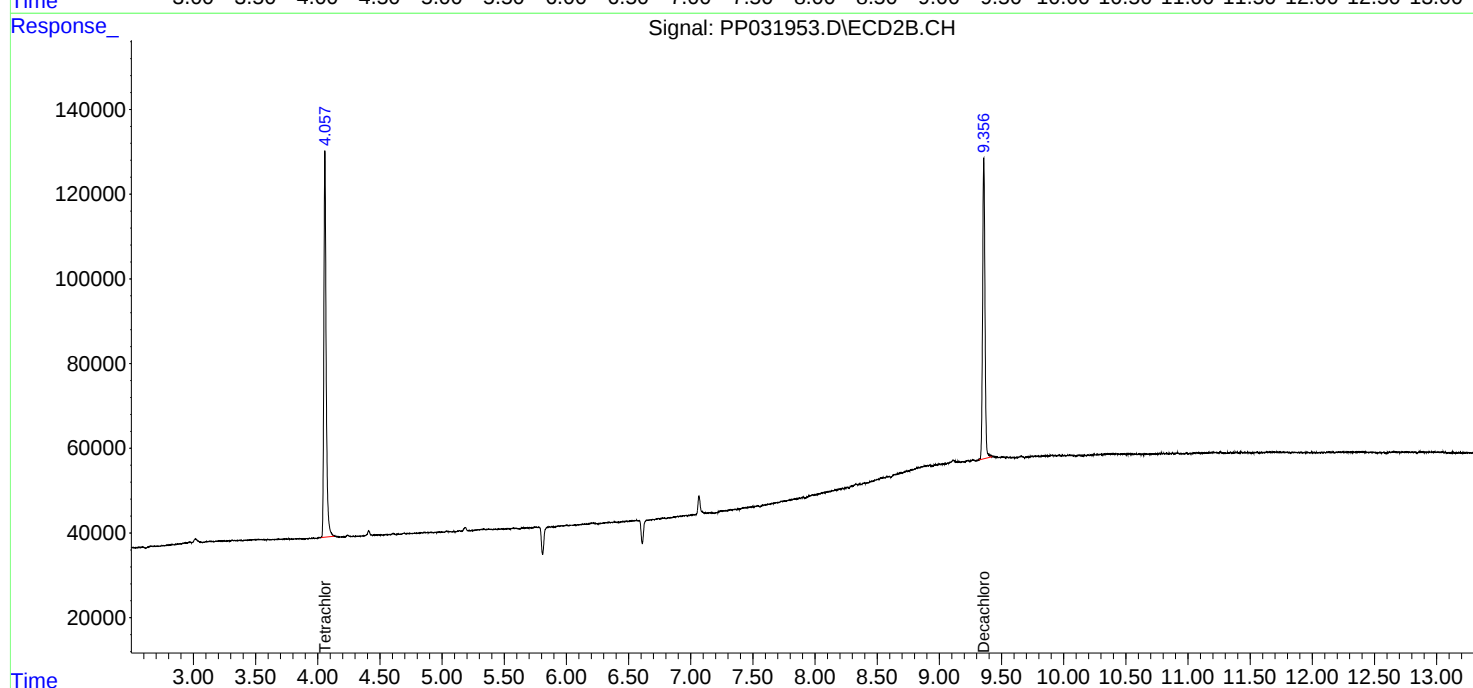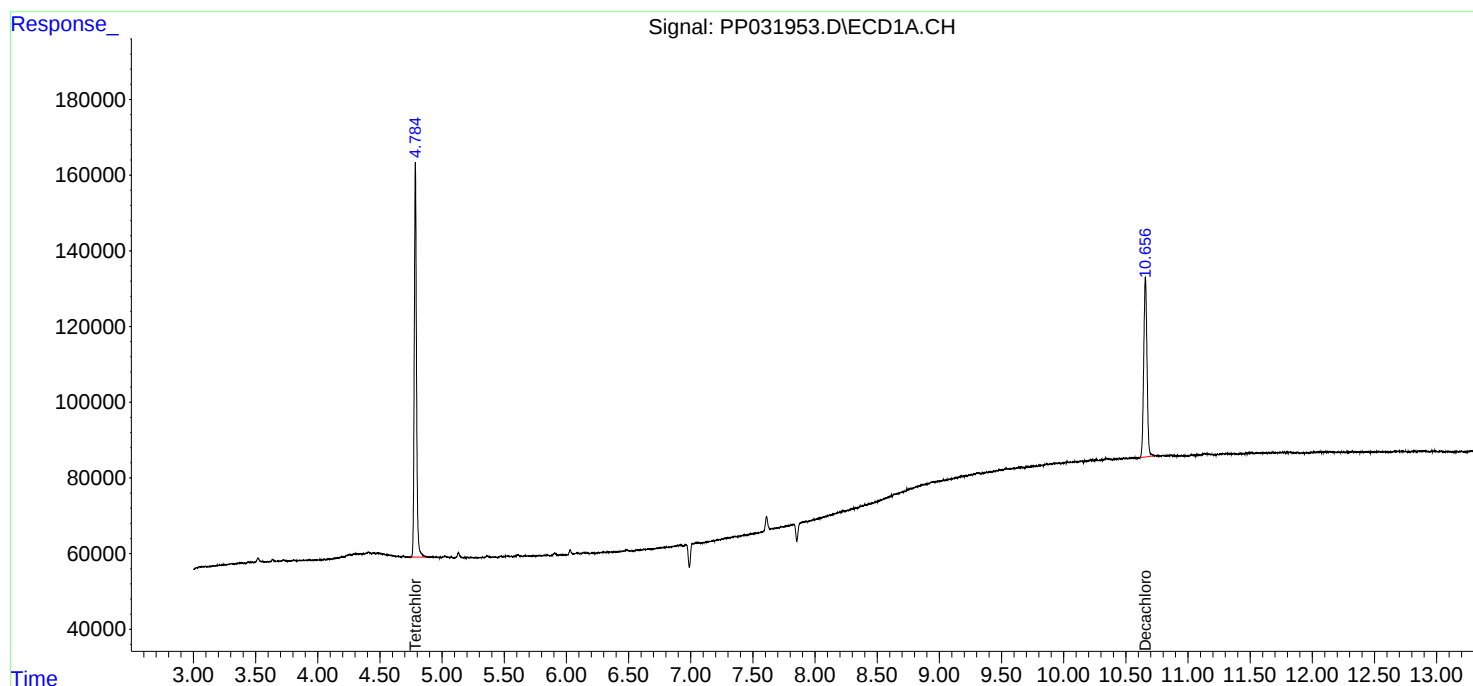


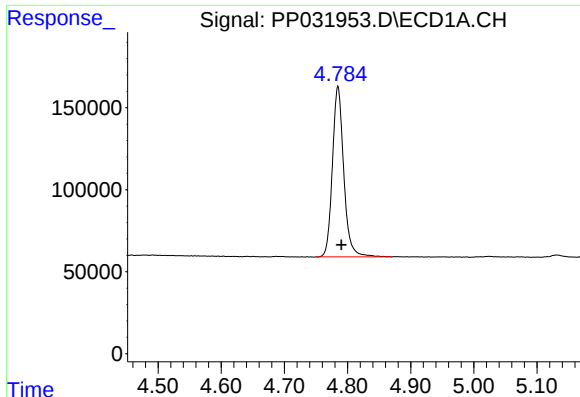

#1 Tetrachloro-m-xylene


R.T.: 4.785 min
Delta R.T.: -0.005 min
Response: 1297051
Conc: 26.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

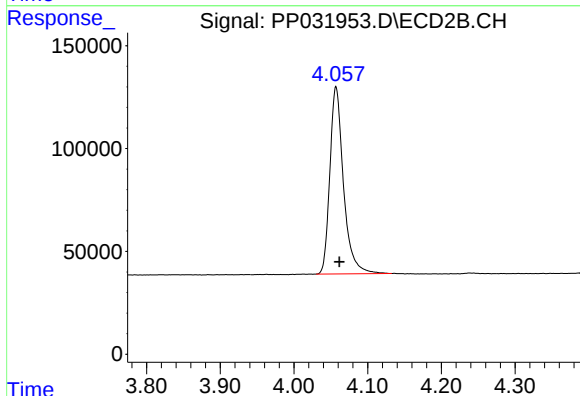


#1 Tetrachloro-m-xylene

R.T.: 4.057 min
Delta R.T.: -0.004 min
Response: 1170037
Conc: 24.42 ng/ml

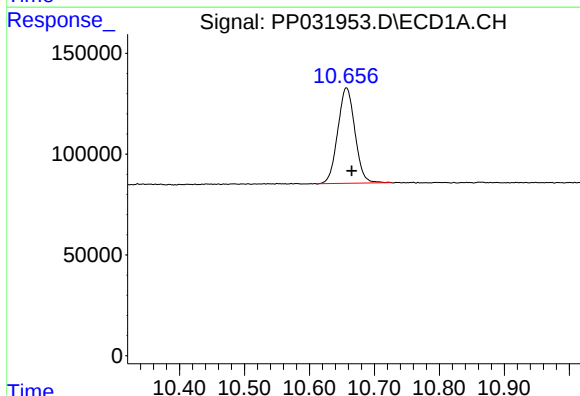

#2 Decachlorobiphenyl

R.T.: 10.657 min
Delta R.T.: -0.008 min
Response: 869070
Conc: 25.59 ng/ml

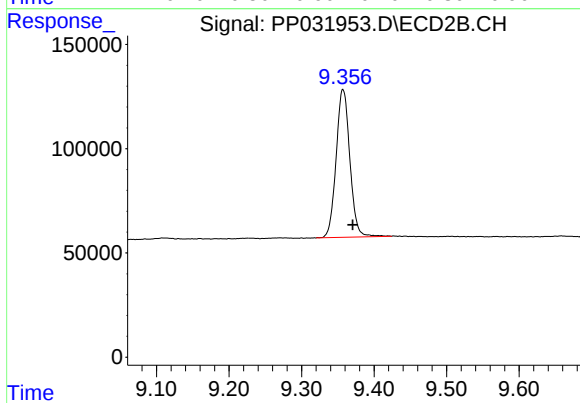

#2 Decachlorobiphenyl

R.T.: 9.357 min
Delta R.T.: -0.013 min
Response: 932436
Conc: 25.18 ng/ml