

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120921\
 Data File : PP041838.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Dec 2021 19:59
 Operator : AJ\MA
 Sample : M4962-07 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 02:06:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.742	3.745	34304	55160	1.521	1.816
2)	SA Decachlor...	10.631	8.996f	41322	30085	1.919	1.947
Target Compounds							
29)	L6 AR-1254-4	7.878	0.000	3081	0	2.969	N.D. #
30)	L6 AR-1254-5	8.299	0.000	1717	0	1.529	N.D. #
32)	L7 AR-1260-2	8.007	0.000	1562	0	1.243	N.D. #
33)	L7 AR-1260-3	8.369	0.000	1149	0	1.269	N.D. #
34)	L7 AR-1260-4	8.617	0.000	1484	0	1.387	N.D. #
36)	L8 AR-1262-1	8.369	0.000	1149	0	0.905	N.D. #
38)	L8 AR-1262-3	0.000	7.922f	0	11181	N.D.	12.546 #
41)	L9 AR-1268-1	0.000	7.922f	0	11181	N.D.	4.662 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120921\
Data File : PP041838.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Dec 2021 19:59
Operator : AJ\MA
Sample : M4962-07 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 02:06:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

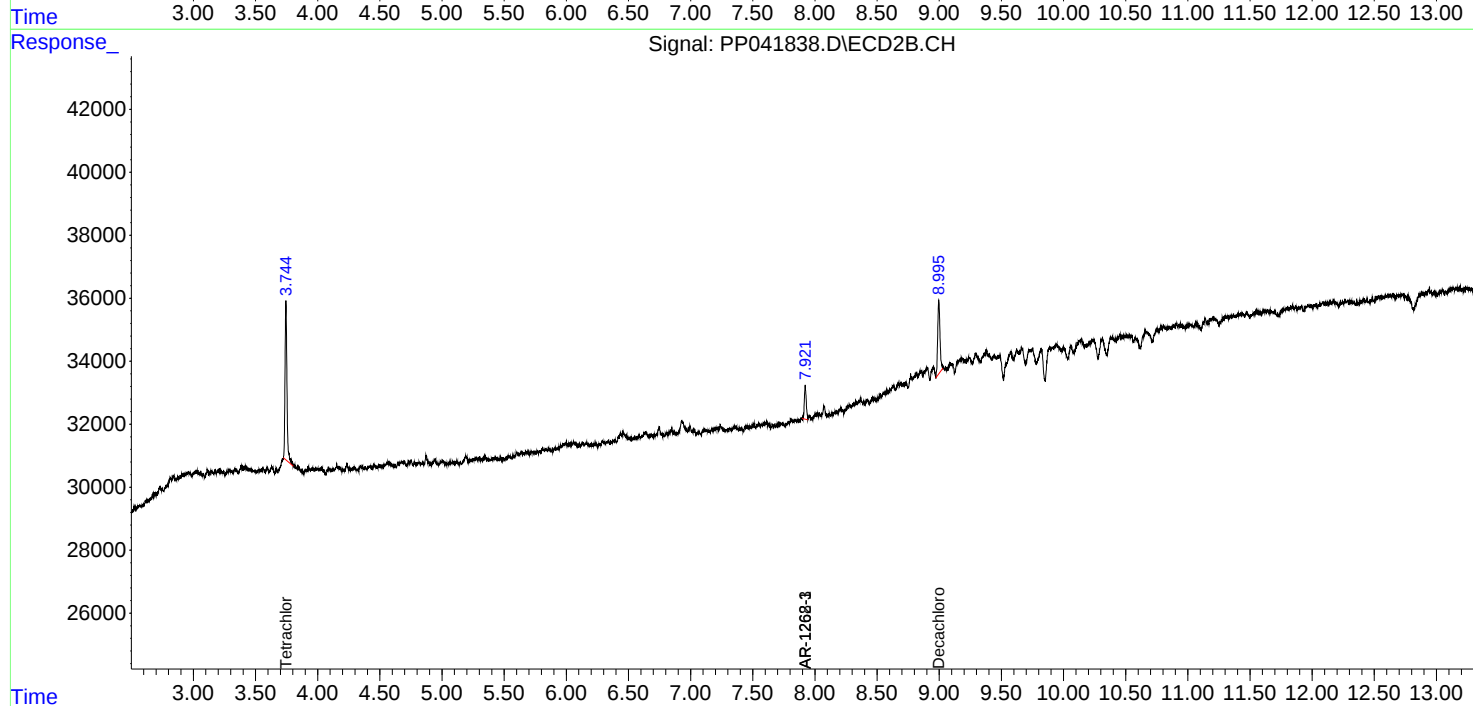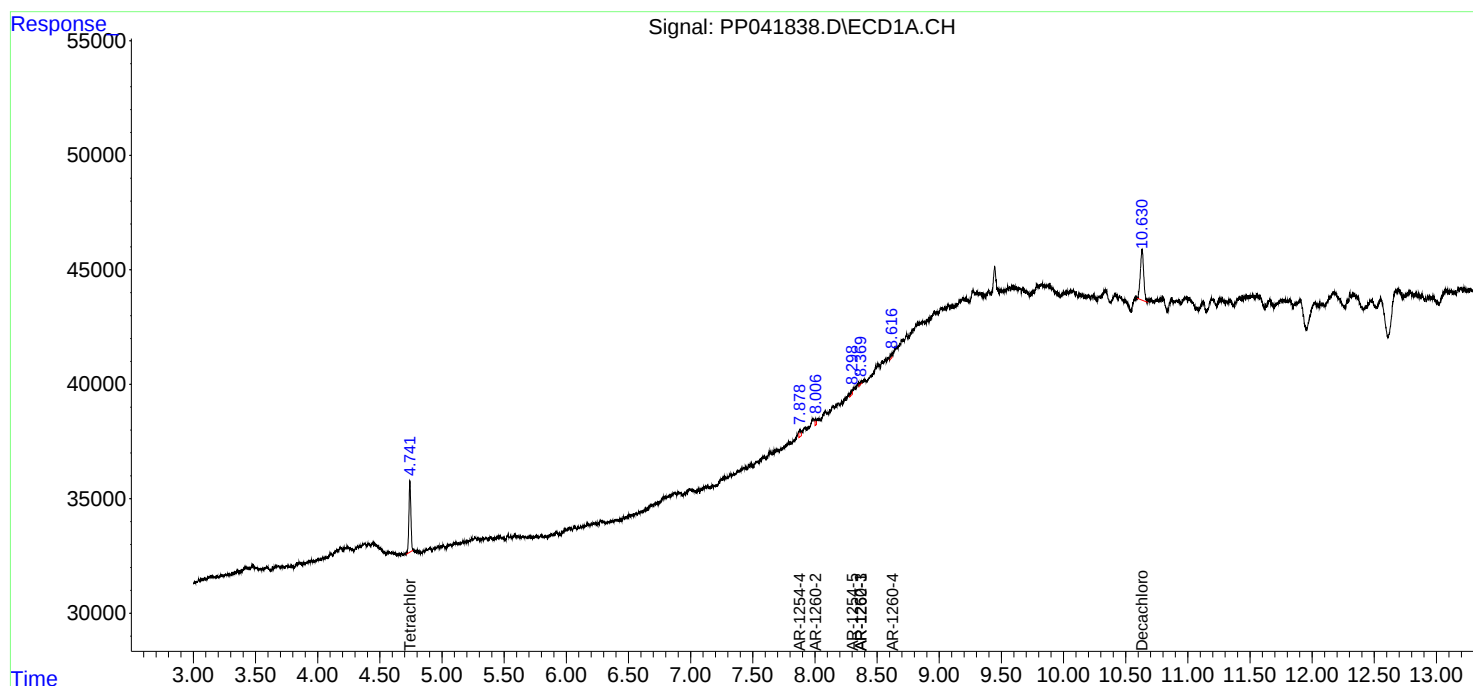


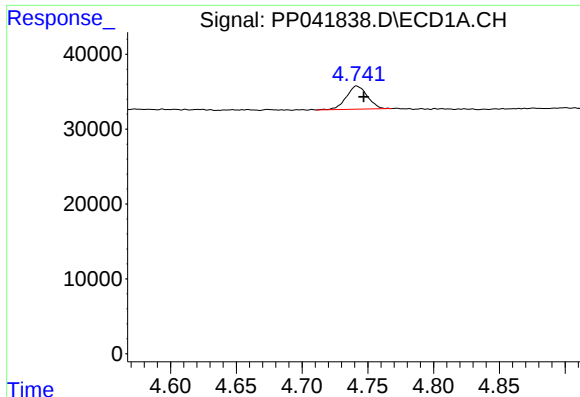

#1 Tetrachloro-m-xylene


R.T.: 4.742 min
Delta R.T.: -0.005 min
Response: 34304
Conc: 1.52 ng/ml

Instrument :
ECD_P
ClientSampleId :

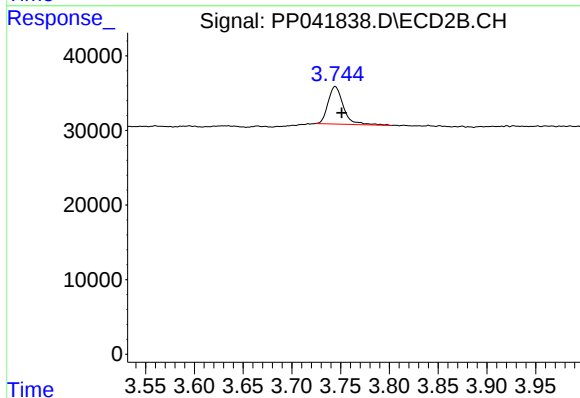


#1 Tetrachloro-m-xylene

R.T.: 3.745 min
Delta R.T.: -0.007 min
Response: 55160
Conc: 1.82 ng/ml

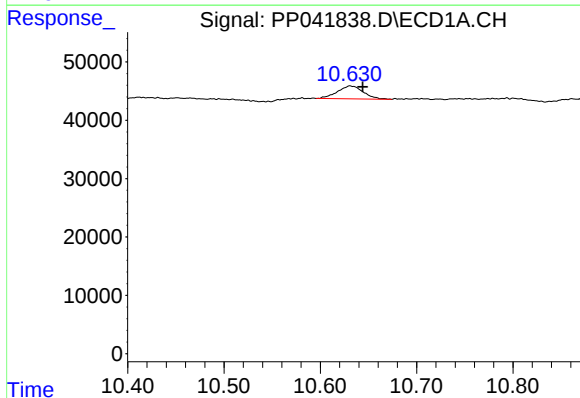


#2 Decachlorobiphenyl

R.T.: 10.631 min
Delta R.T.: -0.013 min
Response: 41322
Conc: 1.92 ng/ml

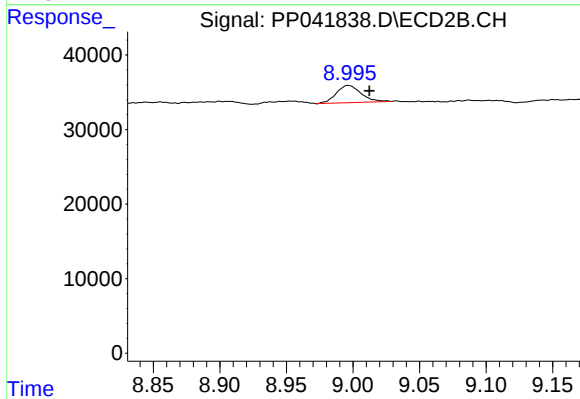

#2 Decachlorobiphenyl


R.T.: 8.996 min
Delta R.T.: -0.016 min
Response: 30085
Conc: 1.95 ng/ml

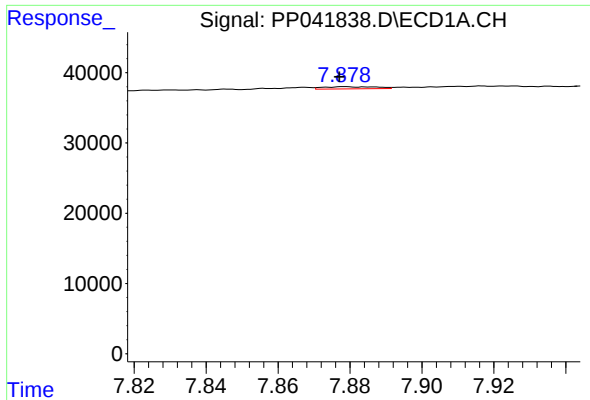

#29 AR-1254-4


R.T.: 7.878 min
Delta R.T.: 0.001 min
Response: 3081
Conc: 2.97 ng/ml

Instrument :
ECD_P
ClientSampleId :

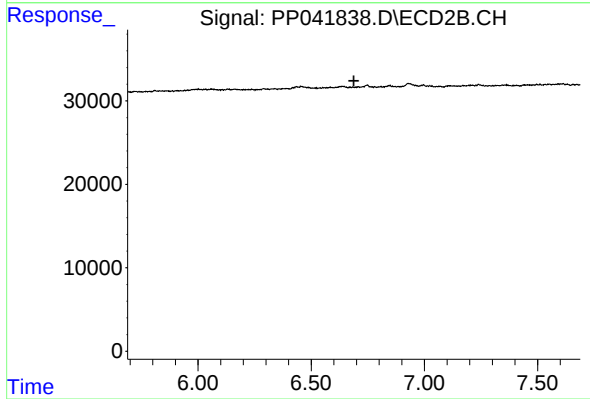


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.688 min
Response: 0
Conc: N.D.

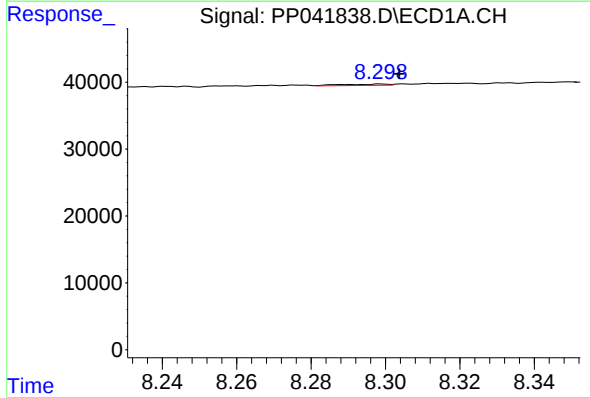


#30 AR-1254-5

R.T.: 8.299 min
Delta R.T.: -0.005 min
Response: 1717
Conc: 1.53 ng/ml

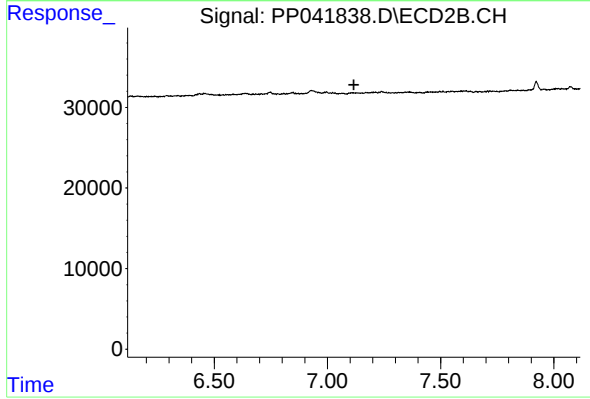

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

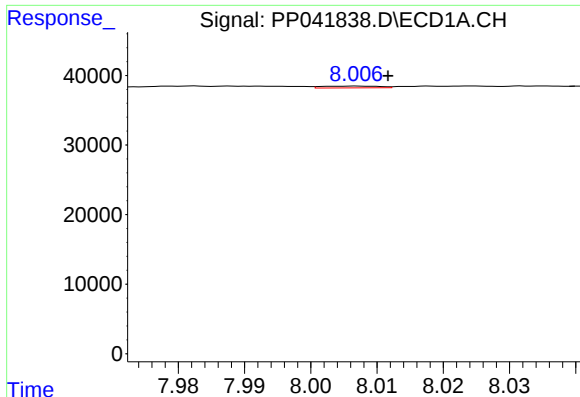

#32 AR-1260-2


R.T.: 8.007 min
Delta R.T.: -0.005 min
Response: 1562
Conc: 1.24 ng/ml

Instrument :
ECD_P
ClientSampleId :

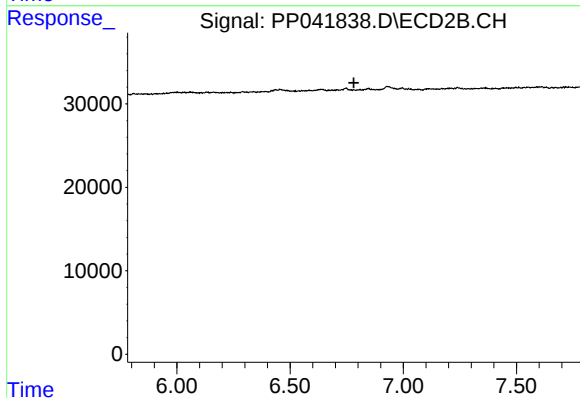


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.782 min
Response: 0
Conc: N.D.

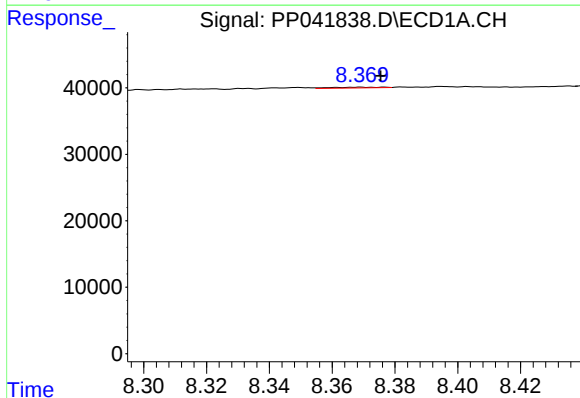


#33 AR-1260-3

R.T.: 8.369 min
Delta R.T.: -0.006 min
Response: 1149
Conc: 1.27 ng/ml

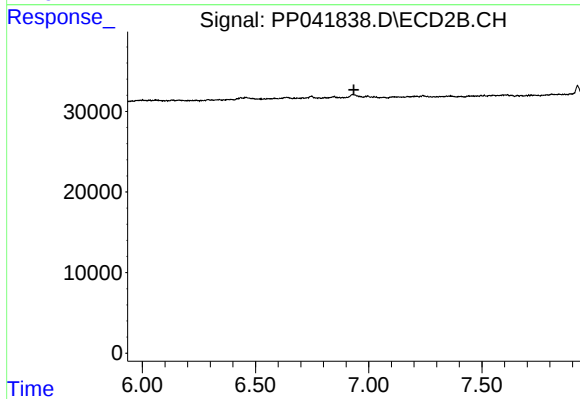

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 6.935 min
Response: 0
Conc: N.D.

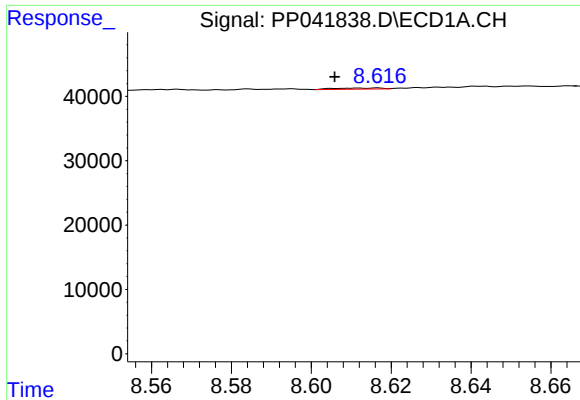

#34 AR-1260-4


R.T.: 8.617 min
Delta R.T.: 0.011 min
Response: 1484
Conc: 1.39 ng/ml

Instrument :
ECD_P
ClientSampleId :

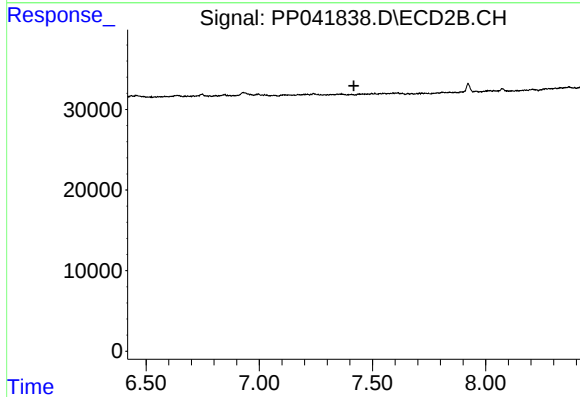


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.418 min
Response: 0
Conc: N.D.

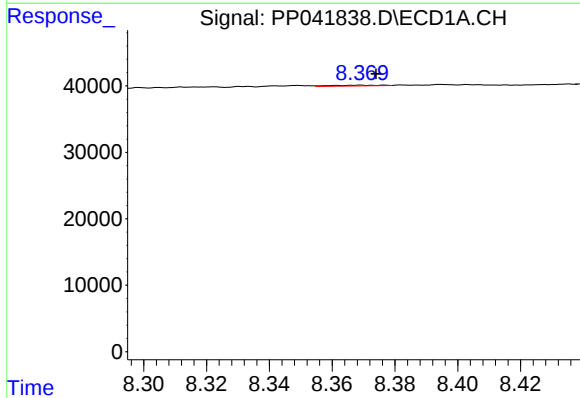


#36 AR-1262-1

R.T.: 8.369 min
Delta R.T.: -0.005 min
Response: 1149
Conc: 0.90 ng/ml

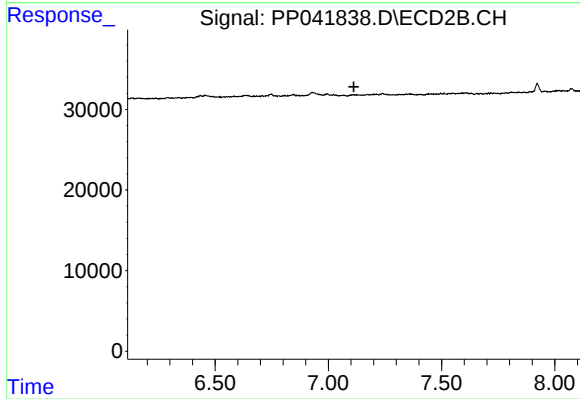

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.113 min
Response: 0
Conc: N.D.

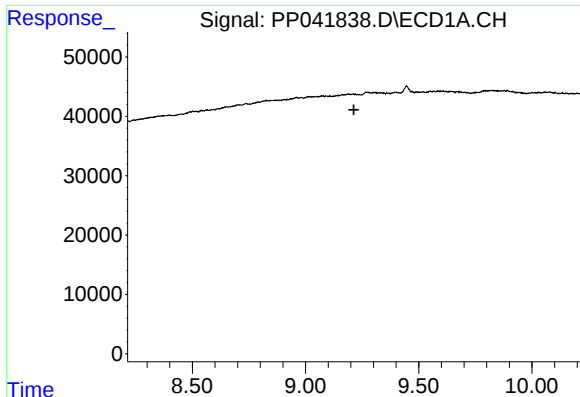

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

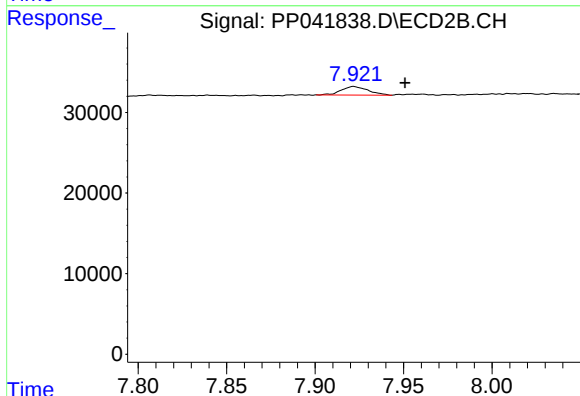


#38 AR-1262-3

R.T.: 7.922 min
Delta R.T.: -0.029 min
Response: 11181
Conc: 12.55 ng/ml

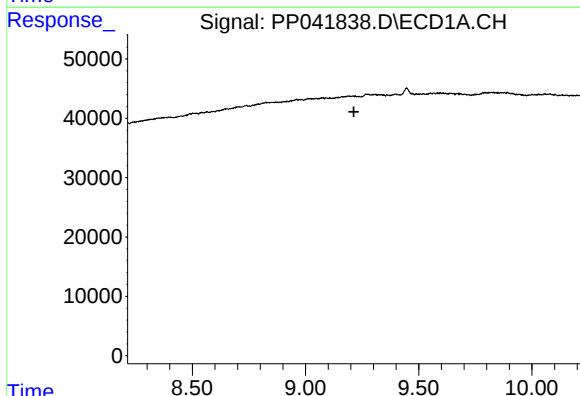

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.214 min
Response: 0
Conc: N.D.

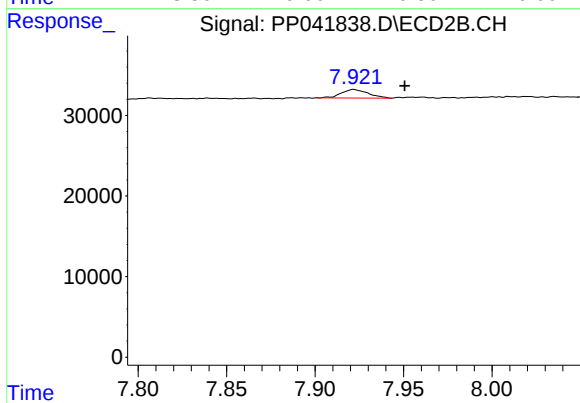

#41 AR-1268-1

R.T.: 7.922 min
Delta R.T.: -0.029 min
Response: 11181
Conc: 4.66 ng/ml