

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120921\
 Data File : PP041852.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Dec 2021 00:20
 Operator : AJ\MA
 Sample : M4962-16 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 02:12:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.741	3.744	31297	49858	1.388	1.641
2)	SA Decachlor...	10.632	8.996f	33143	25109	1.539	1.625
Target Compounds							
30)	L6 AR-1254-5	8.293	0.000	709	0	0.632	N.D. #
32)	L7 AR-1260-2	7.986f	0.000	7657	0	6.094	N.D. #
33)	L7 AR-1260-3	8.391f	0.000	5414	0	5.979	N.D. #
36)	L8 AR-1262-1	8.391f	0.000	5414	0	4.263	N.D. #
39)	L8 AR-1262-4	9.316	0.000	34984	0	51.113	N.D. #
42)	L9 AR-1268-2	9.316	0.000	34984	0	13.359	N.D. #
43)	L9 AR-1268-3	9.543f	0.000	11842	0	5.343	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120921\
Data File : PP041852.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Dec 2021 00:20
Operator : AJ\MA
Sample : M4962-16 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 02:12:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

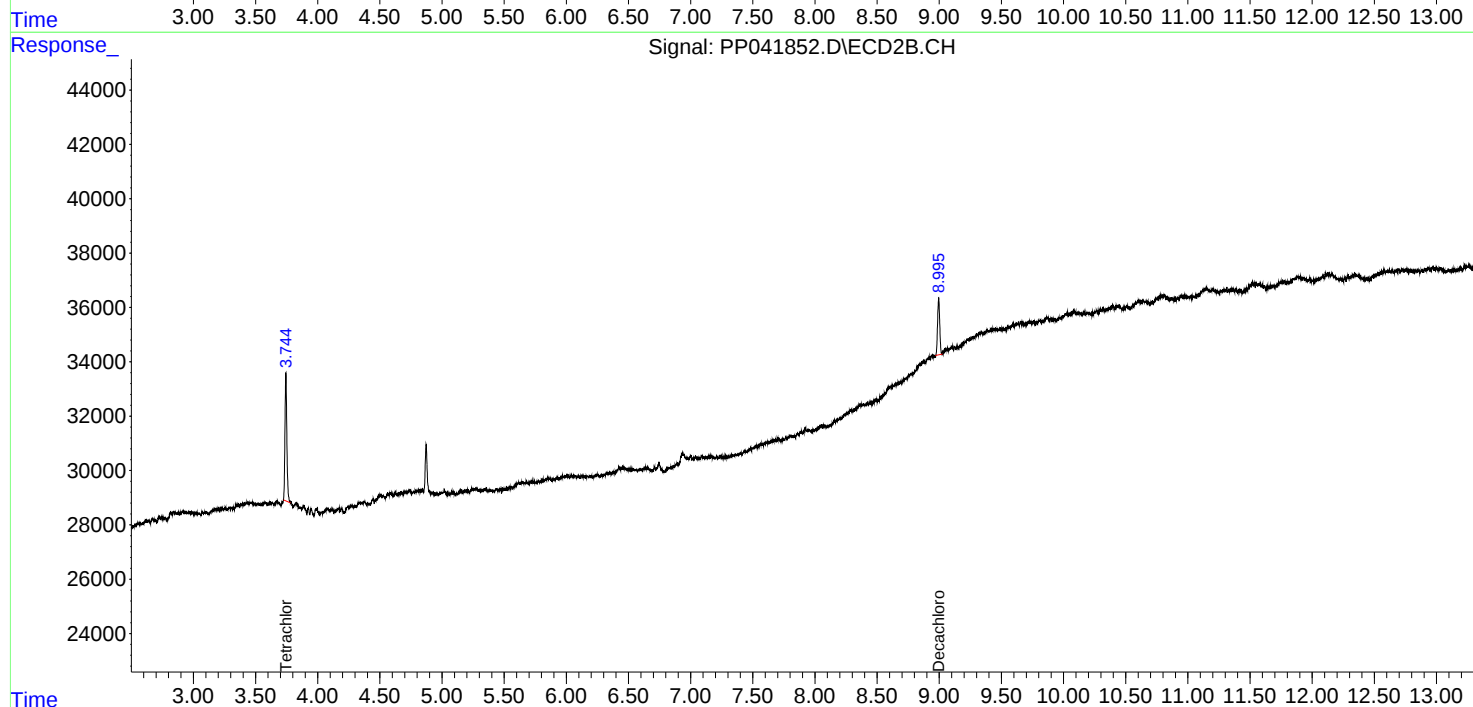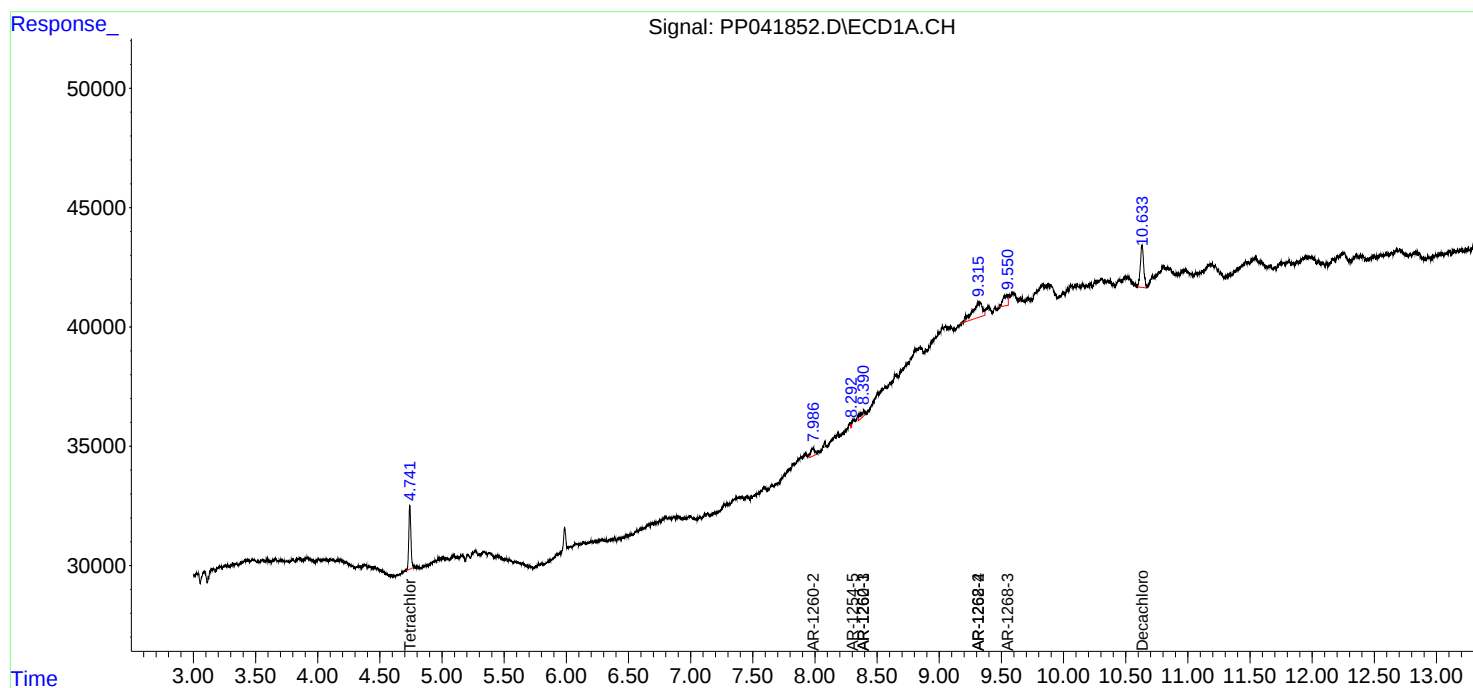


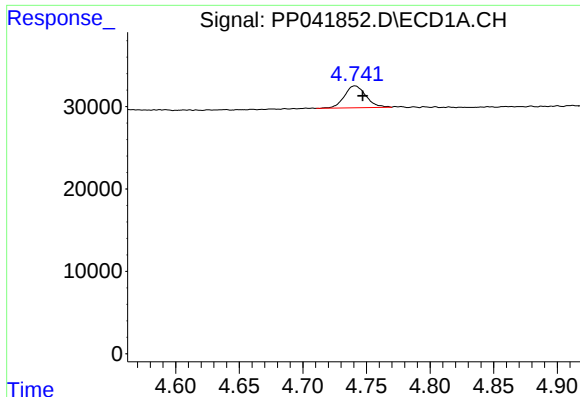

#1 Tetrachloro-m-xylene


R.T.: 4.741 min
Delta R.T.: -0.006 min
Response: 31297
Conc: 1.39 ng/ml

Instrument :
ECD_P
ClientSampleId :

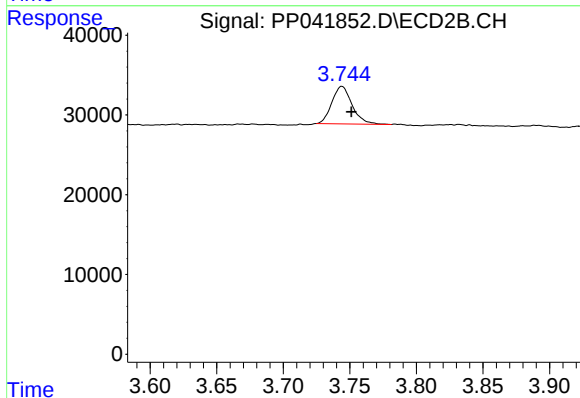


#1 Tetrachloro-m-xylene

R.T.: 3.744 min
Delta R.T.: -0.007 min
Response: 49858
Conc: 1.64 ng/ml

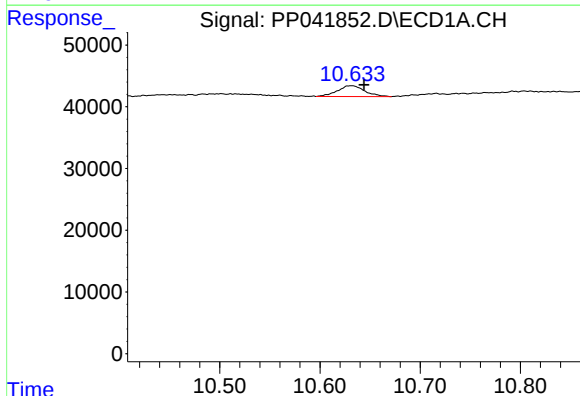


#2 Decachlorobiphenyl

R.T.: 10.632 min
Delta R.T.: -0.012 min
Response: 33143
Conc: 1.54 ng/ml

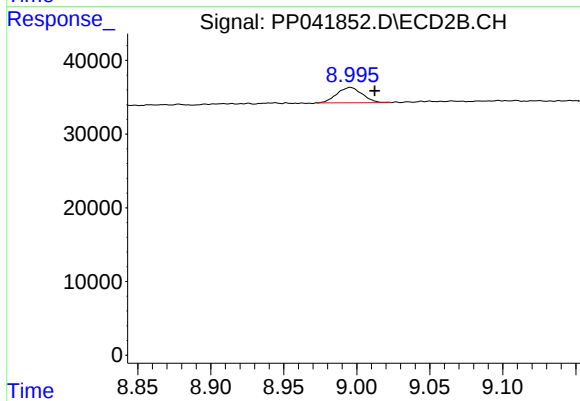

#2 Decachlorobiphenyl


R.T.: 8.996 min
Delta R.T.: -0.017 min
Response: 25109
Conc: 1.62 ng/ml

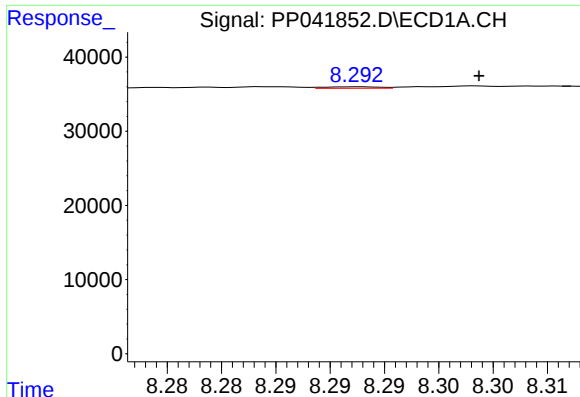

#30 AR-1254-5


R.T.: 8.293 min
Delta R.T.: -0.011 min
Response: 709
Conc: 0.63 ng/ml

Instrument :
ECD_P
ClientSampleId :

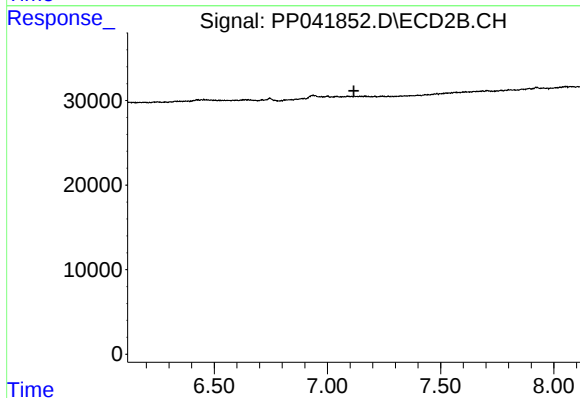


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

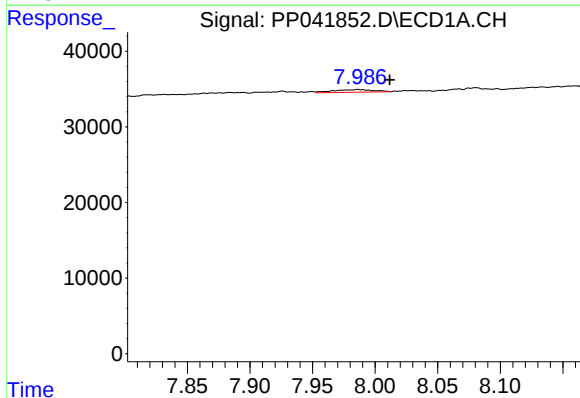


#32 AR-1260-2

R.T.: 7.986 min
Delta R.T.: -0.025 min
Response: 7657
Conc: 6.09 ng/ml

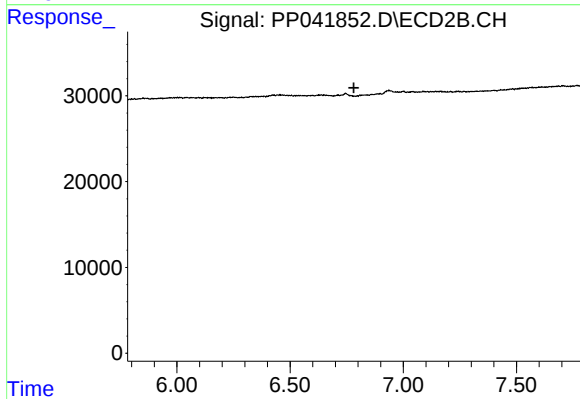

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.782 min
Response: 0
Conc: N.D.

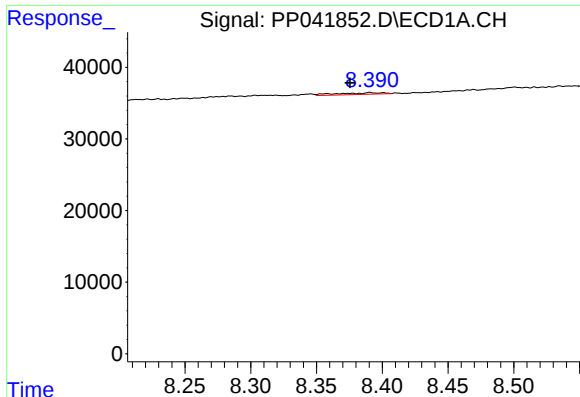

#33 AR-1260-3


R.T.: 8.391 min
Delta R.T.: 0.015 min
Response: 5414
Conc: 5.98 ng/ml

Instrument :
ECD_P
ClientSampleId :

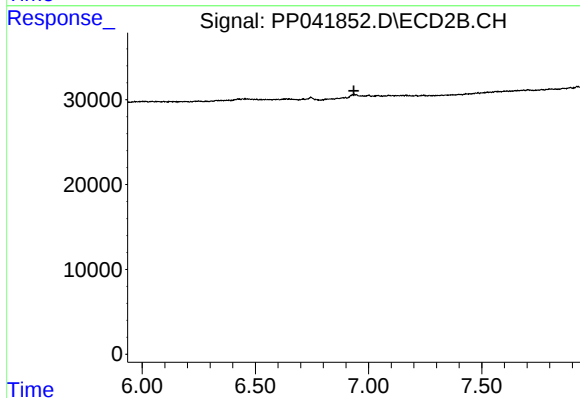


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.935 min
Response: 0
Conc: N.D.

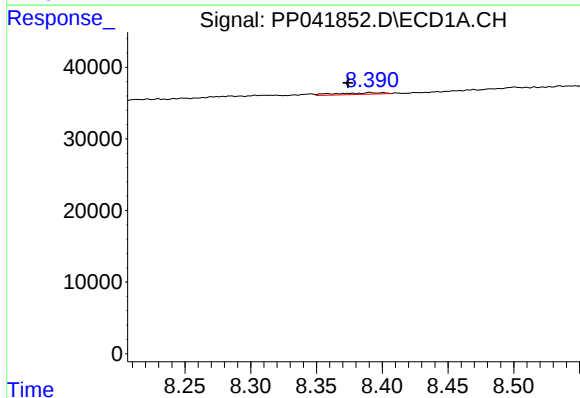


#36 AR-1262-1

R.T.: 8.391 min
Delta R.T.: 0.017 min
Response: 5414
Conc: 4.26 ng/ml

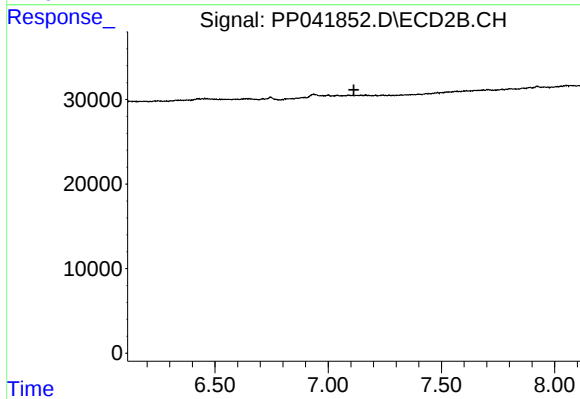

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 7.113 min
Response: 0
Conc: N.D.

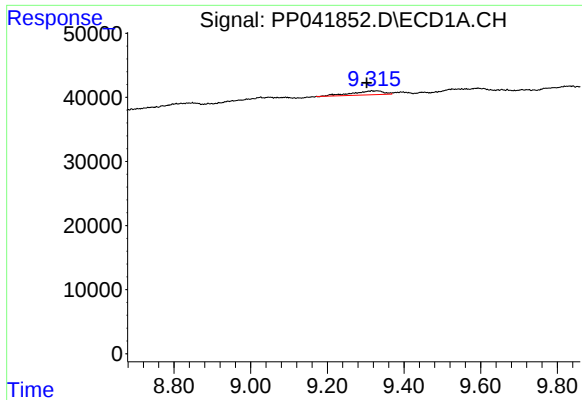

#39 AR-1262-4


R.T.: 9.316 min
Delta R.T.: 0.013 min
Response: 34984
Conc: 51.11 ng/ml

Instrument :
ECD_P
ClientSampleId :

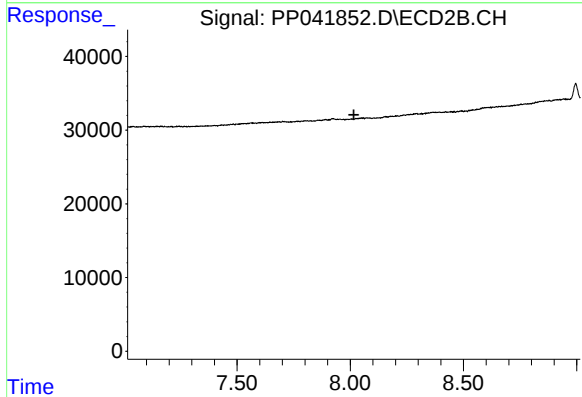


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.016 min
Response: 0
Conc: N.D.

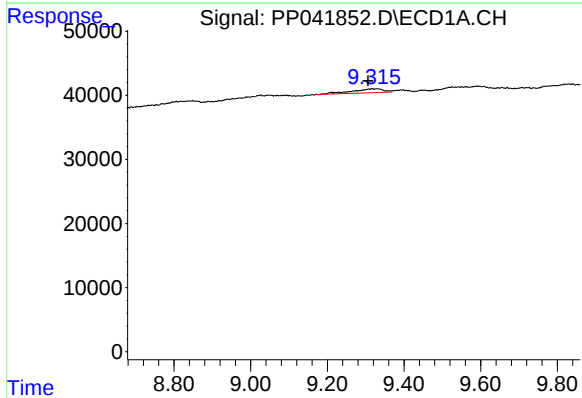


#42 AR-1268-2

R.T.: 9.316 min
Delta R.T.: 0.010 min
Response: 34984
Conc: 13.36 ng/ml

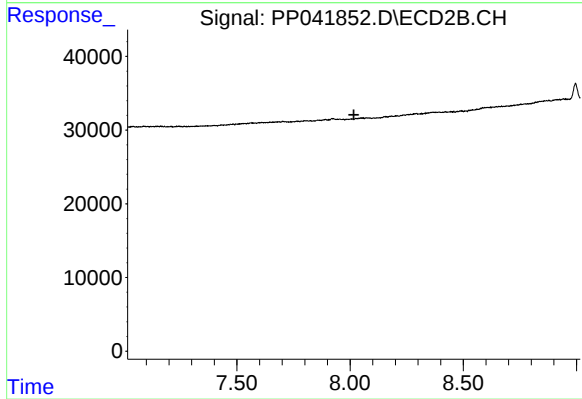

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.017 min
Response: 0
Conc: N.D.

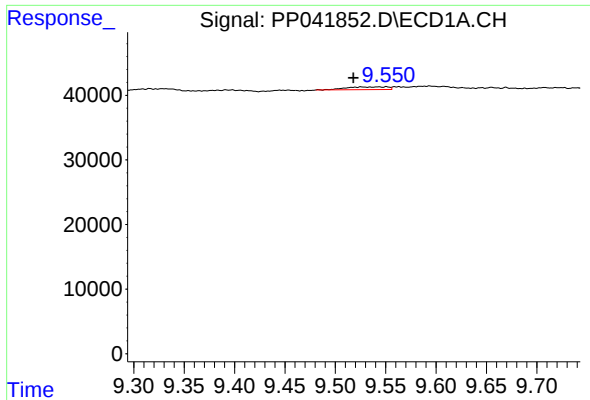

#43 AR-1268-3

R.T.: 9.543 min
Delta R.T.: 0.025 min
Response: 11842
Conc: 5.34 ng/ml

Instrument :
ECD_P
ClientSampleId :

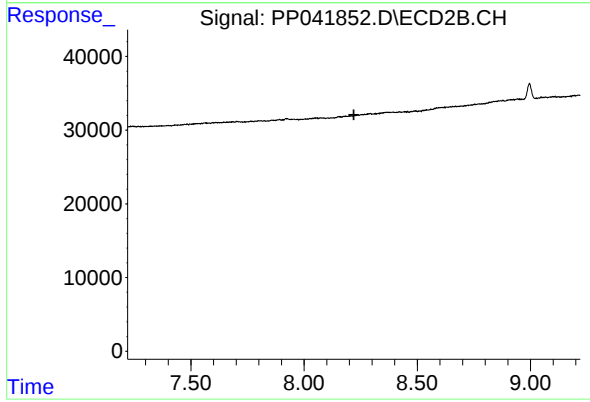

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.220 min
Response: 0
Conc: N.D.