

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120921\
 Data File : PP041817.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Dec 2021 14:09
 Operator : AJ\MA
 Sample : M4962-22 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MOO-2021-35-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 01:57:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.743	3.745	36236	61165	1.607m	2.014 #
2) SA Decachlor...	10.633	9.001	43000	29669	1.997m	1.920m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120921\
Data File : PP041817.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Dec 2021 14:09
Operator : AJ\MA
Sample : M4962-22 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MOO-2021-35-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 01:57:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

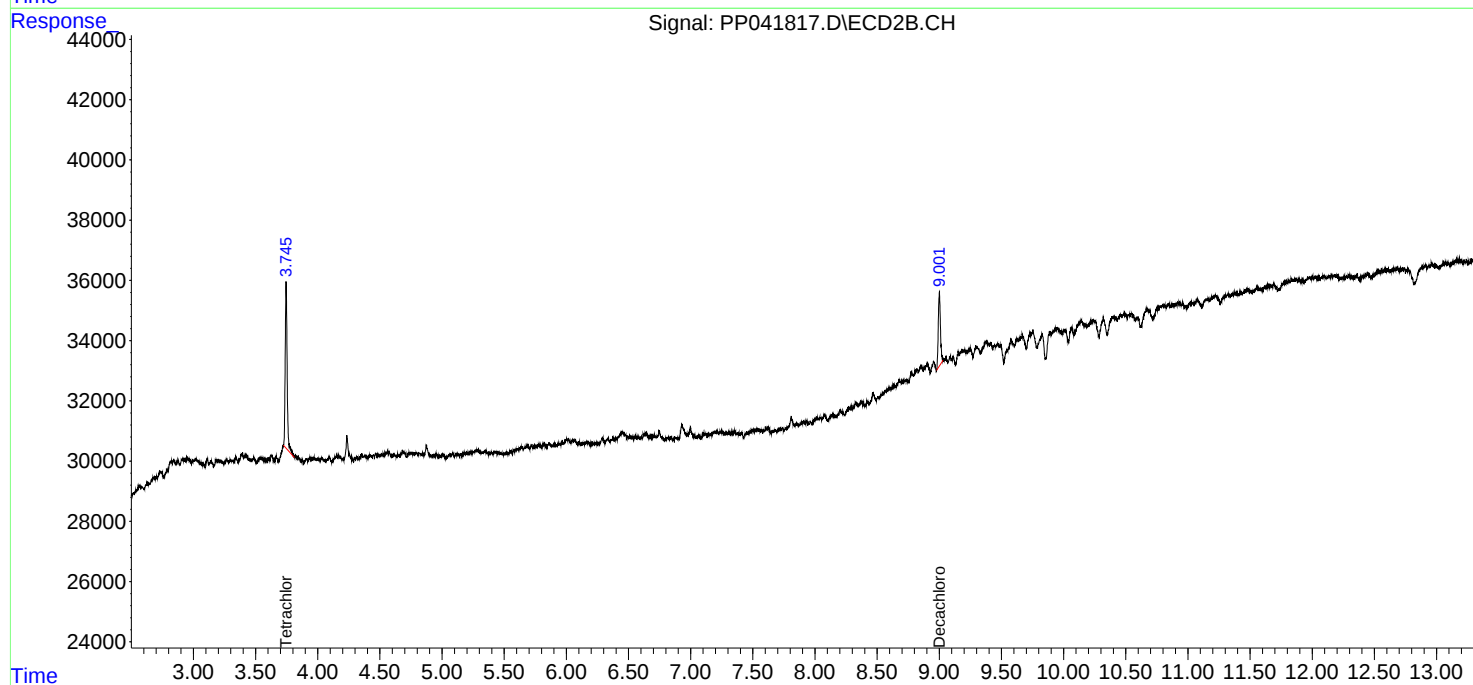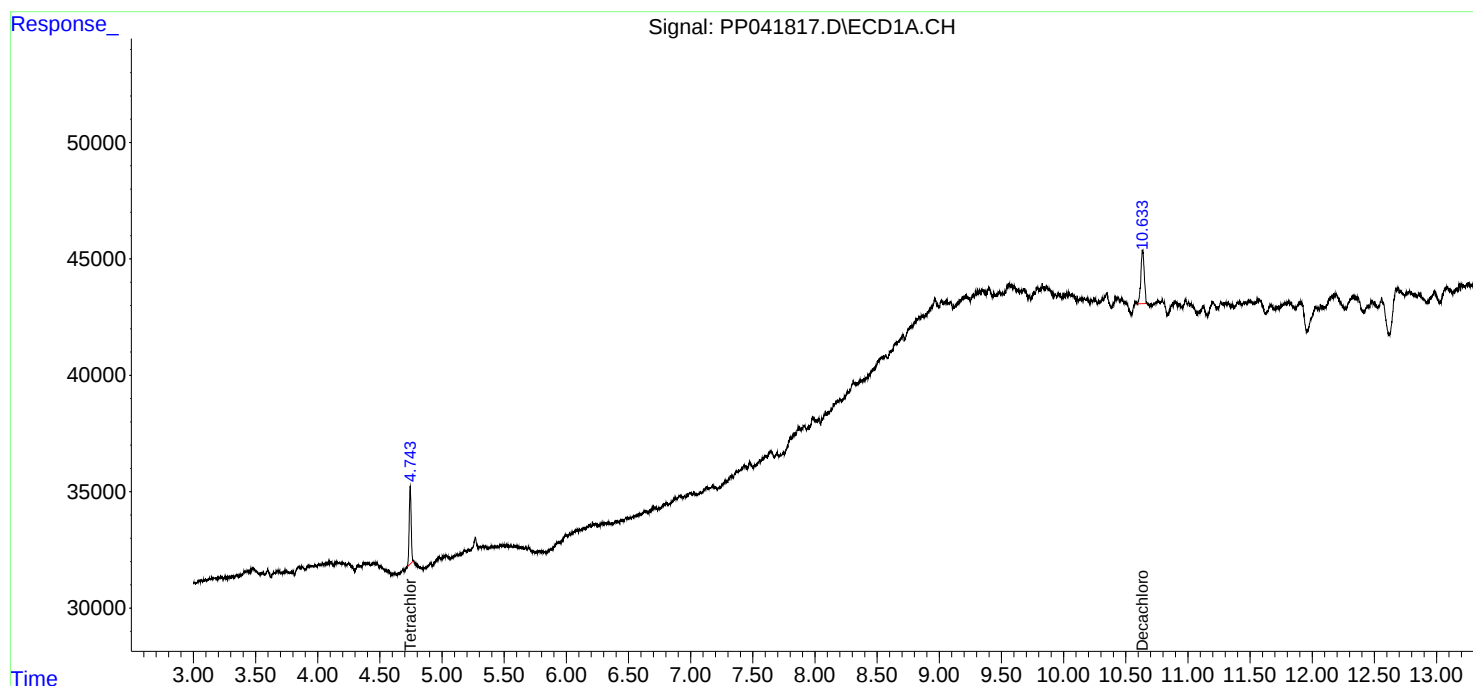


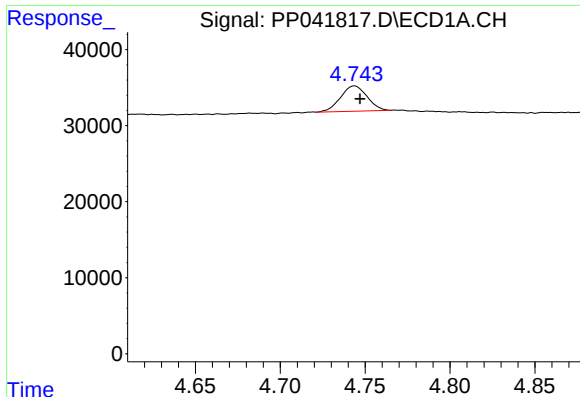

#1 Tetrachloro-m-xylene


R.T.: 4.743 min
Delta R.T.: -0.004 min
Response: 36236
Conc: 1.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2021-35-A

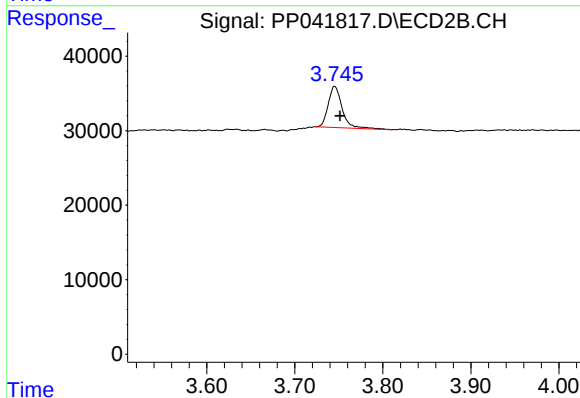


#1 Tetrachloro-m-xylene

R.T.: 3.745 min
Delta R.T.: -0.006 min
Response: 61165
Conc: 2.01 ng/ml

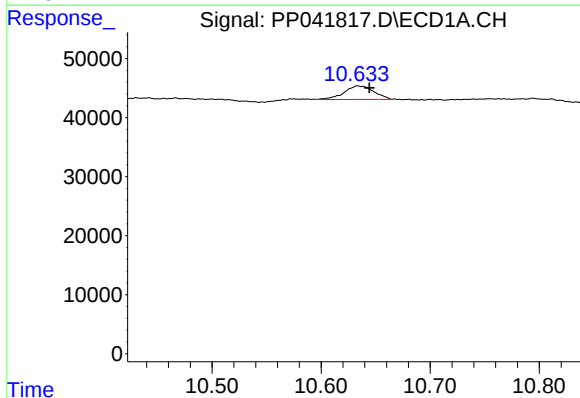

#2 Decachlorobiphenyl

R.T.: 10.633 min
Delta R.T.: -0.011 min
Response: 43000
Conc: 2.00 ng/ml m

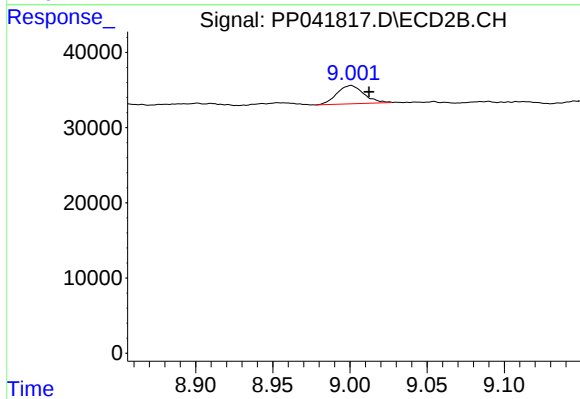

#2 Decachlorobiphenyl

R.T.: 9.001 min
Delta R.T.: -0.012 min
Response: 29669
Conc: 1.92 ng/ml m