

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP120921\  
 Data File : PP041824.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 09 Dec 2021 16:06  
 Operator : AJ\MA  
 Sample : M4962-29 10X  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 MOO-2021-39-B

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Dec 10 02:00:02 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP113021.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Nov 30 23:30:32 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1 | Resp#2 | ng/ml | ng/ml |
|-----------------------------|--------|-------|--------|--------|-------|-------|
| -----                       |        |       |        |        |       |       |
| System Monitoring Compounds |        |       |        |        |       |       |
| 1) SA Tetrachlo...          | 4.742  | 3.745 | 34742  | 55327  | 1.541 | 1.821 |
| 2) SA Decachlor...          | 10.631 | 8.999 | 35465  | 31014  | 1.647 | 2.007 |

Target Compounds

-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP120921\  
Data File : PP041824.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 09 Dec 2021 16:06  
Operator : AJ\MA  
Sample : M4962-29 10X  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
MOO-2021-39-B

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 10 02:00:02 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP113021.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Nov 30 23:30:32 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

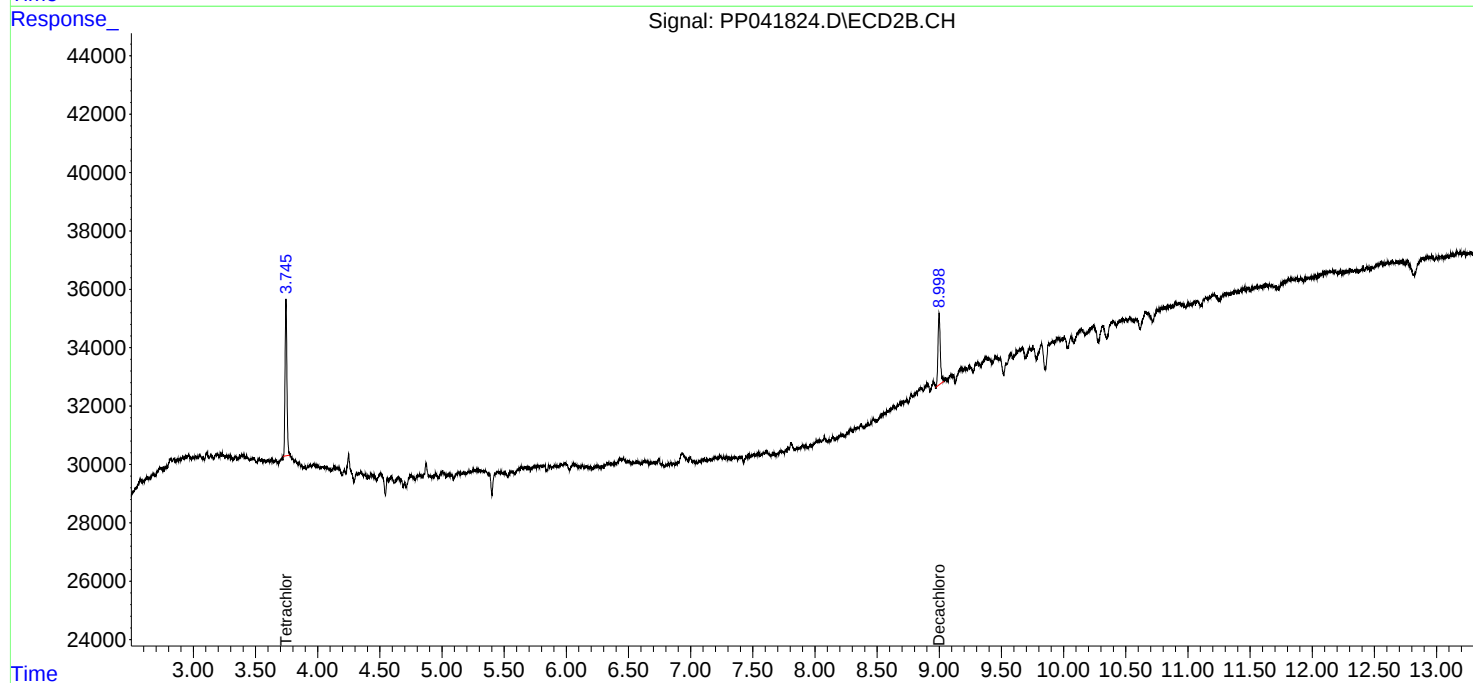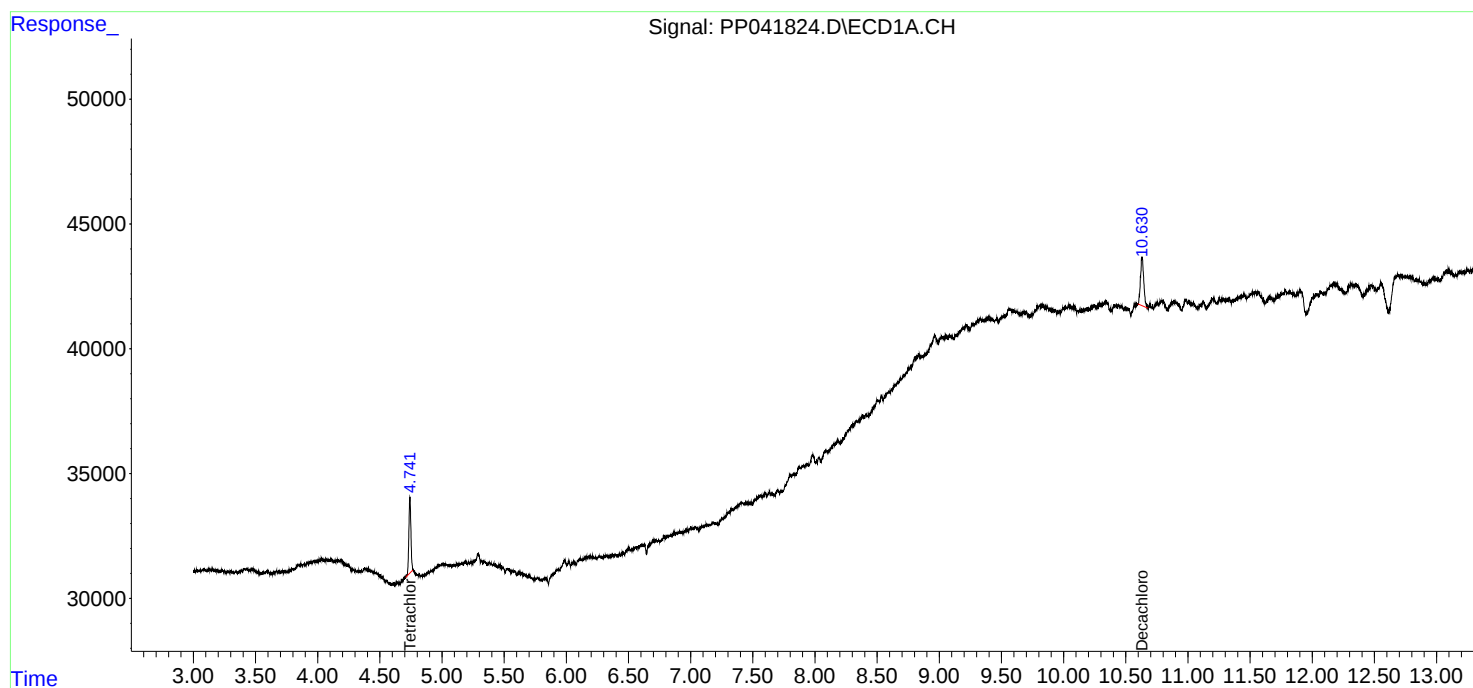


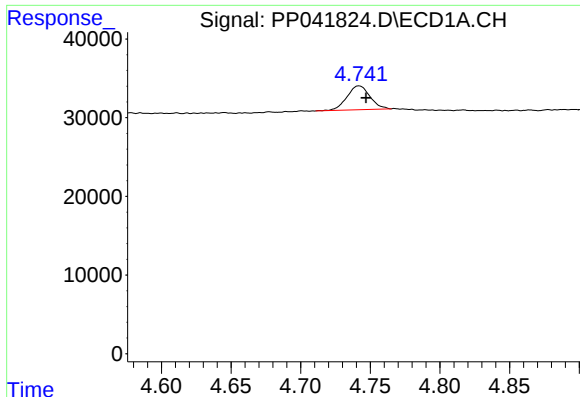

#1 Tetrachloro-m-xylene


R.T.: 4.742 min  
Delta R.T.: -0.005 min  
Response: 34742  
Conc: 1.54 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MOO-2021-39-B

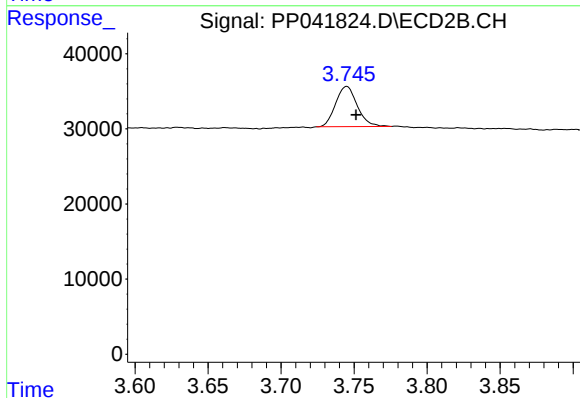


#1 Tetrachloro-m-xylene

R.T.: 3.745 min  
Delta R.T.: -0.006 min  
Response: 55327  
Conc: 1.82 ng/ml

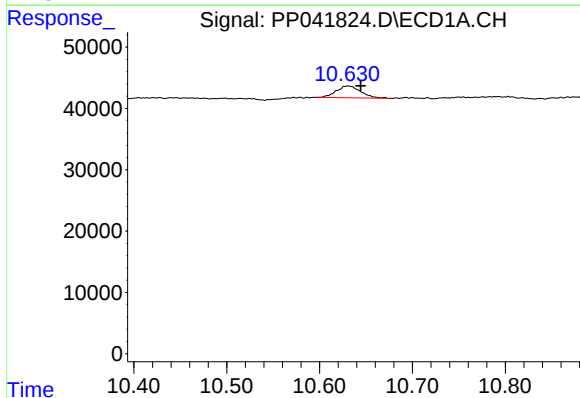

#2 Decachlorobiphenyl

R.T.: 10.631 min  
Delta R.T.: -0.013 min  
Response: 35465  
Conc: 1.65 ng/ml

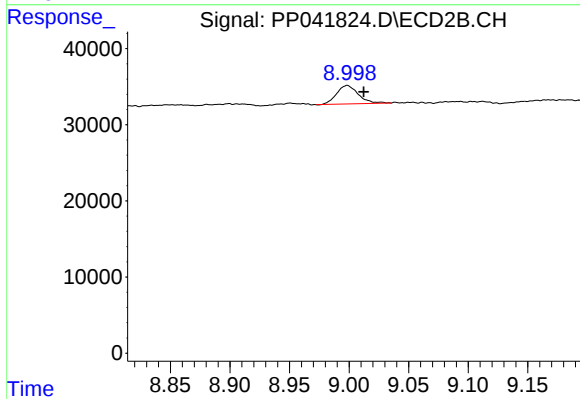

#2 Decachlorobiphenyl

R.T.: 8.999 min  
Delta R.T.: -0.014 min  
Response: 31014  
Conc: 2.01 ng/ml