

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120921\
 Data File : PP041860.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Dec 2021 3:00
 Operator : AJ\MA
 Sample : M4962-19 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MOO-2021-32-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 07:42:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.742	3.744	34932	51867	1.549	1.708
2)	SA Decachlor...	10.632	8.995	43038	29156	1.999	1.886

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP120921\
Data File : PP041860.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Dec 2021 3:00
Operator : AJ\MA
Sample : M4962-19 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MOO-2021-32-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 07:42:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

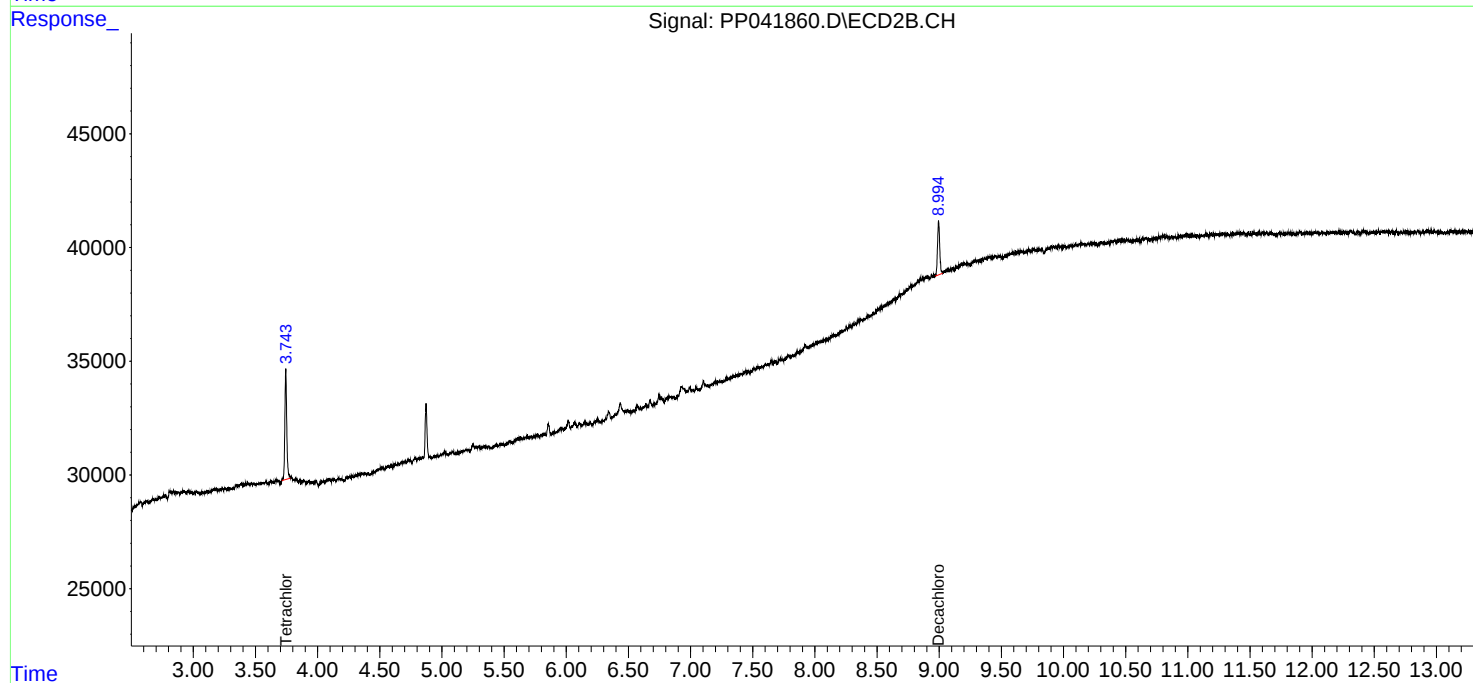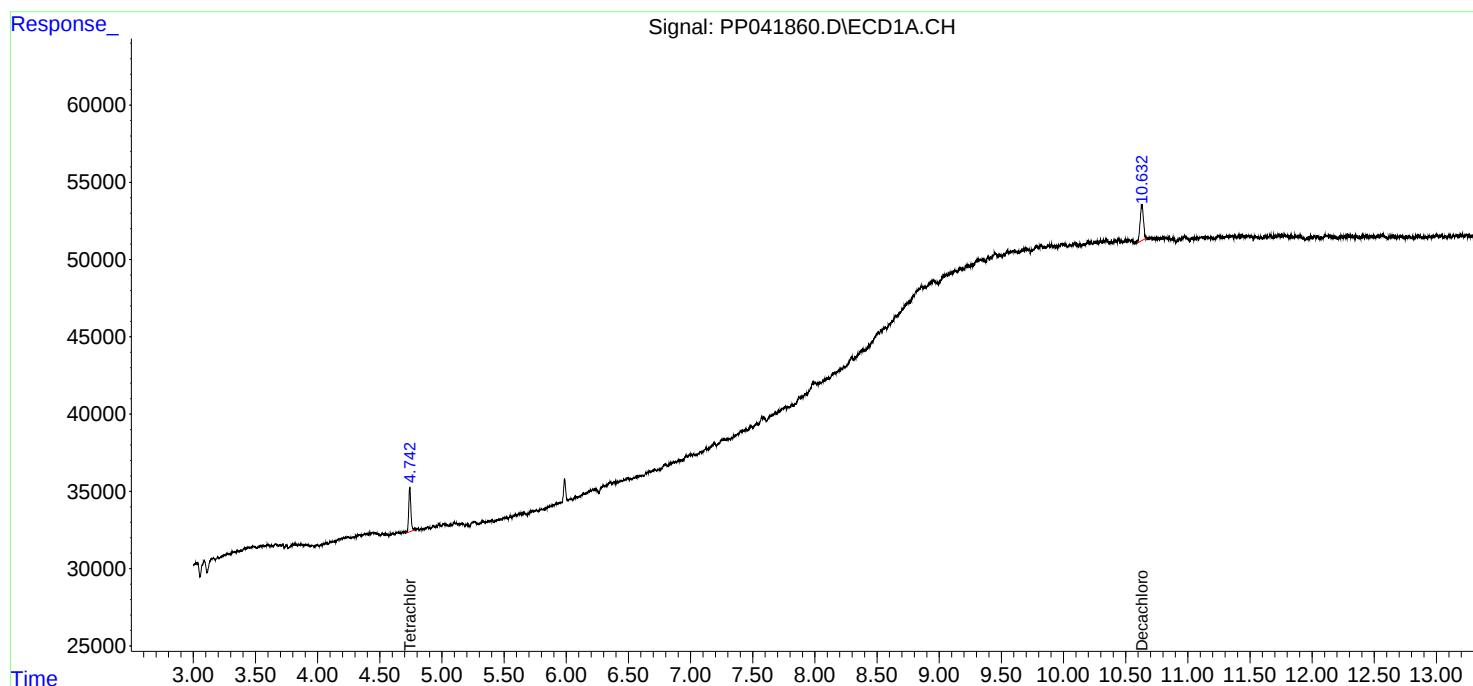


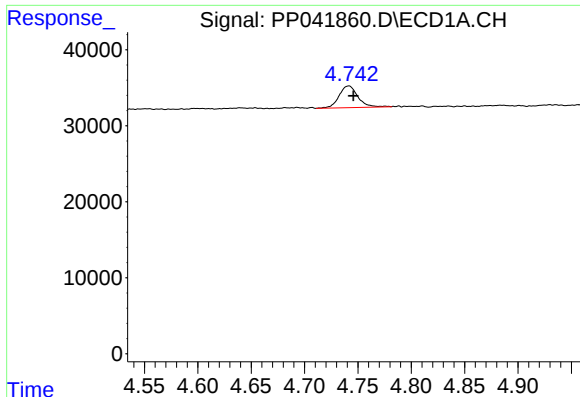

#1 Tetrachloro-m-xylene


R.T.: 4.742 min
Delta R.T.: -0.004 min
Response: 34932
Conc: 1.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2021-32-B

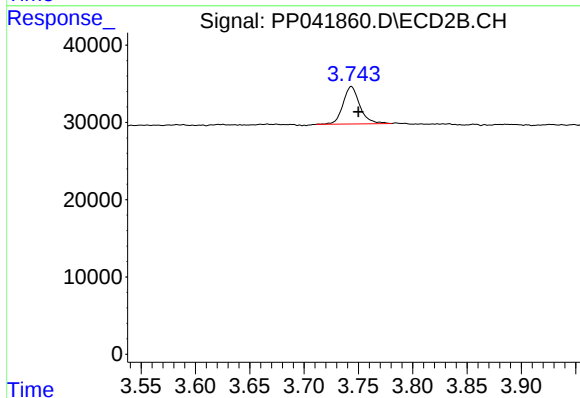


#1 Tetrachloro-m-xylene

R.T.: 3.744 min
Delta R.T.: -0.006 min
Response: 51867
Conc: 1.71 ng/ml

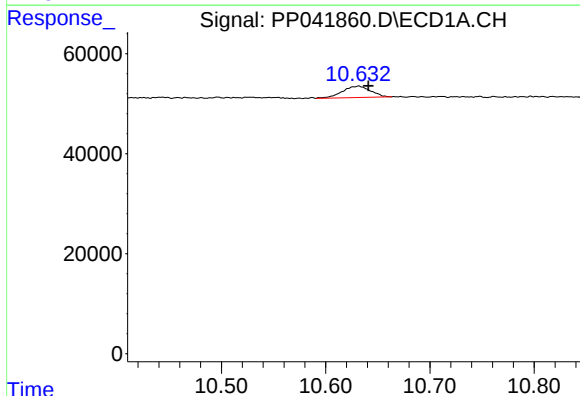

#2 Decachlorobiphenyl

R.T.: 10.632 min
Delta R.T.: -0.009 min
Response: 43038
Conc: 2.00 ng/ml

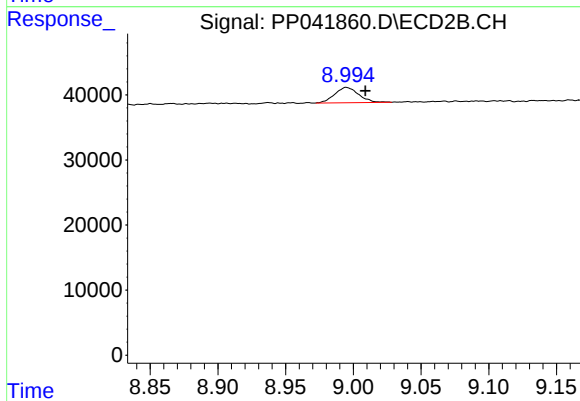

#2 Decachlorobiphenyl

R.T.: 8.995 min
Delta R.T.: -0.014 min
Response: 29156
Conc: 1.89 ng/ml