

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121020\
 Data File : PP031960.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Dec 2020 9:22
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 10:32:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 24 12:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8)	L2	AR-1221-1	0.000	4.307	0	8160 N.D. 16.083 #
20)	L4	AR-1242-5	0.000	6.207f	0	21567 N.D. 20.904 #
25)	L5	AR-1248-5	0.000	6.207f	0	21567 N.D. 14.782 #
26)	L6	AR-1254-1	0.000	6.207f	0	21567 N.D. 9.970 #
28)	L6	AR-1254-3	7.622f	0.000	82490	0 32.652 N.D. #
33)	L7	AR-1260-3	0.000	7.247	0	8340 N.D. 3.652 #
34)	L7	AR-1260-4	8.617f	0.000	144206	0 78.316 N.D. #
35)	L7	AR-1260-5	0.000	7.982	0	11929 N.D. 2.629 #
37)	L8	AR-1262-2	0.000	7.982	0	11929 N.D. 2.456 #
43)	L9	AR-1268-3	0.000	8.574f	0	25260 N.D. 5.507 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121020\
Data File : PP031960.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Dec 2020 9:22
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 10:32:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112220.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 24 12:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

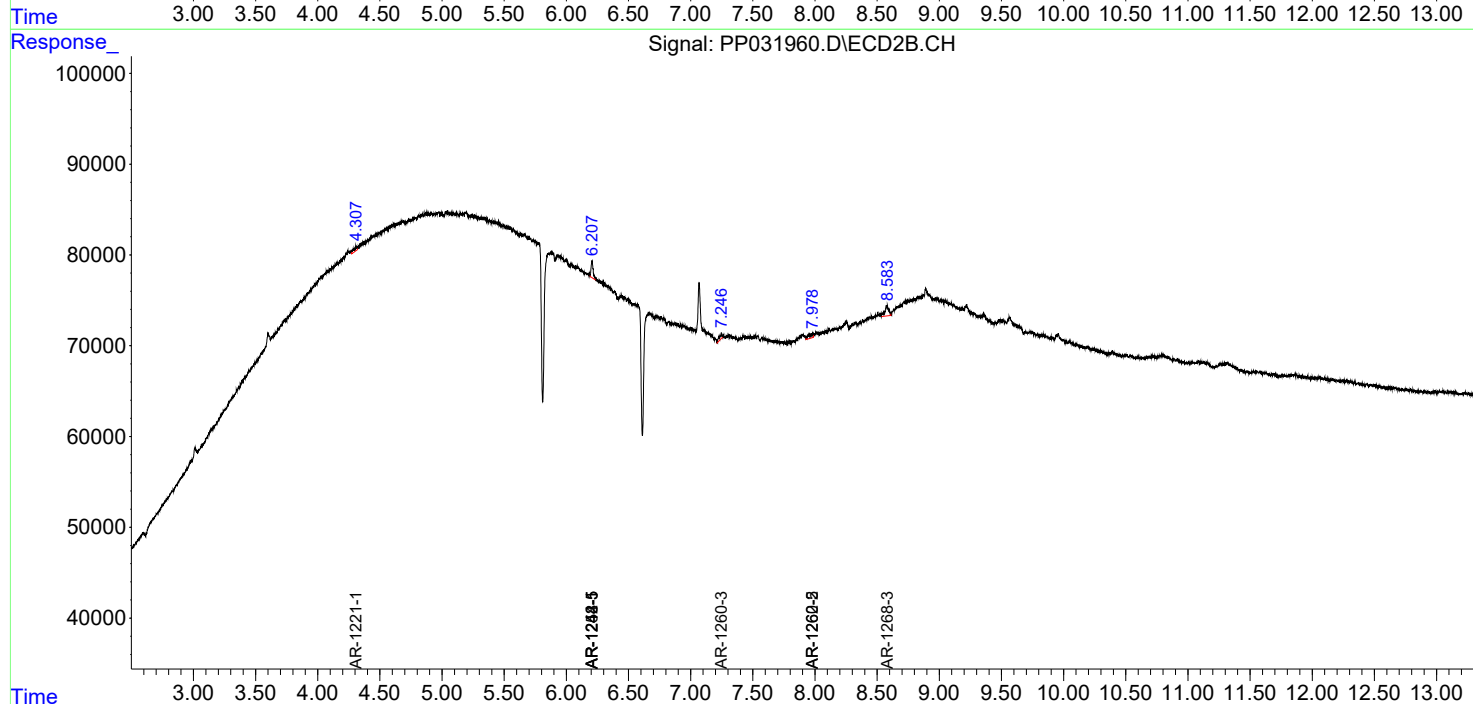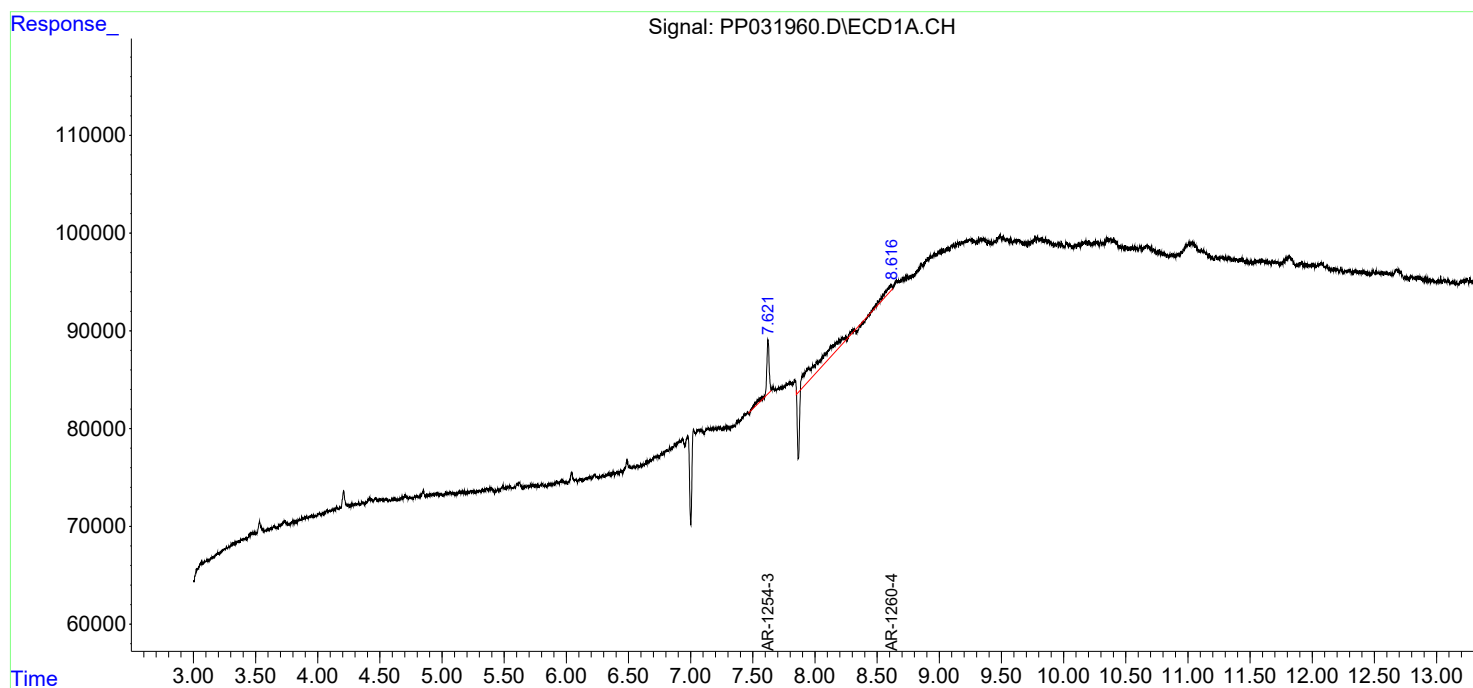


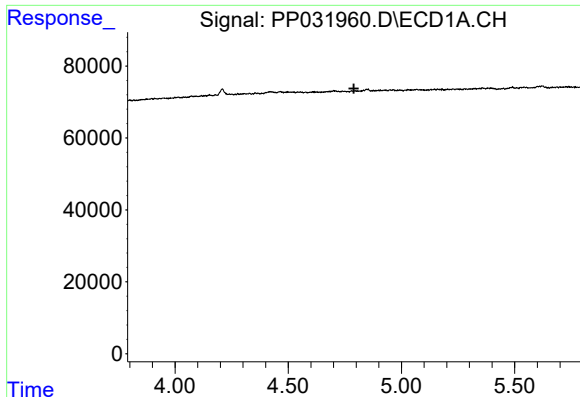

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.790 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

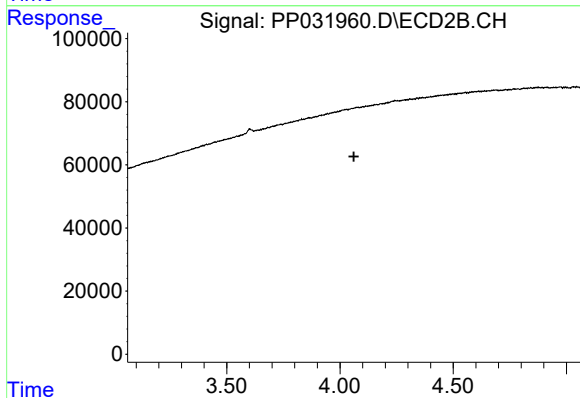


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.062 min
Response: 0
Conc: N.D.

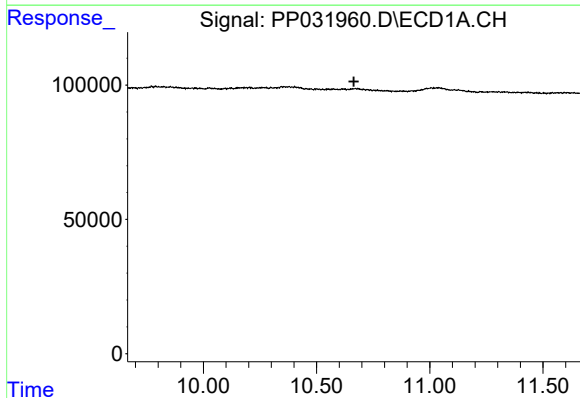


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.665 min
Response: 0
Conc: N.D.

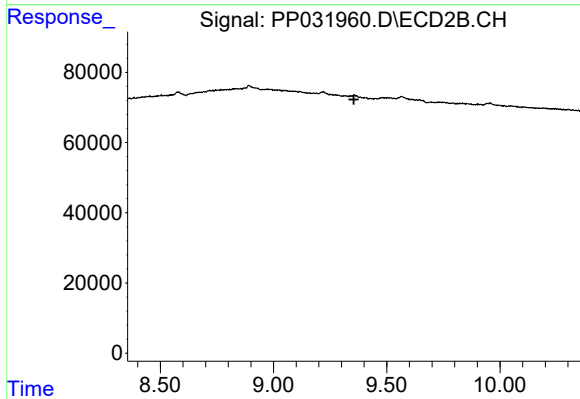

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.355 min
Response: 0
Conc: N.D.

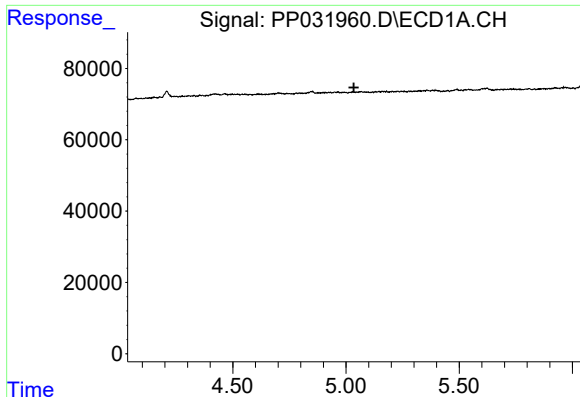

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 5.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

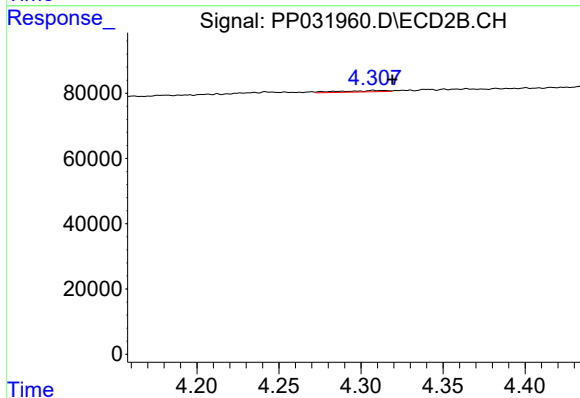


#8 AR-1221-1

R.T.: 4.307 min
Delta R.T.: -0.012 min
Response: 8160
Conc: 16.08 ng/ml

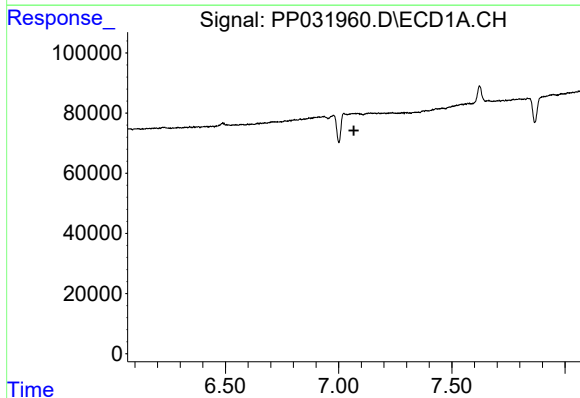


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 7.067 min
Response: 0
Conc: N.D.

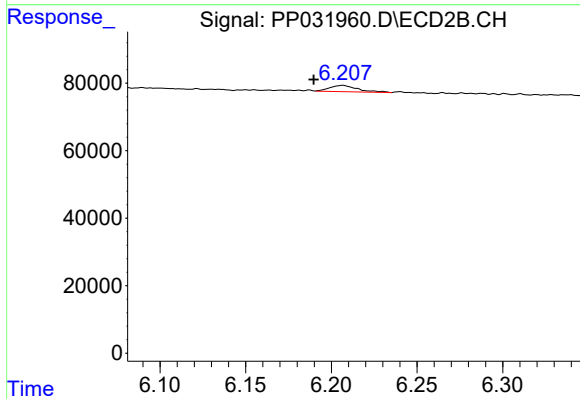

#20 AR-1242-5


R.T.: 6.207 min
Delta R.T.: 0.017 min
Response: 21567
Conc: 20.90 ng/ml

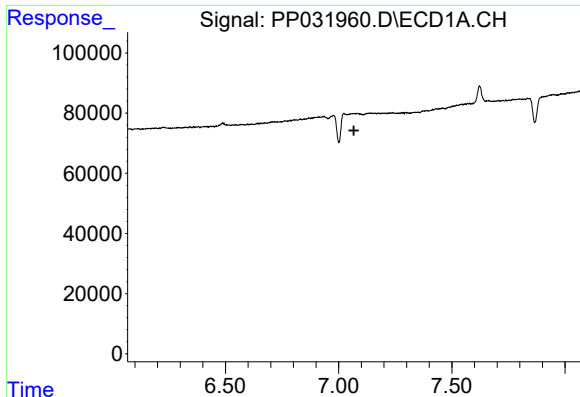

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

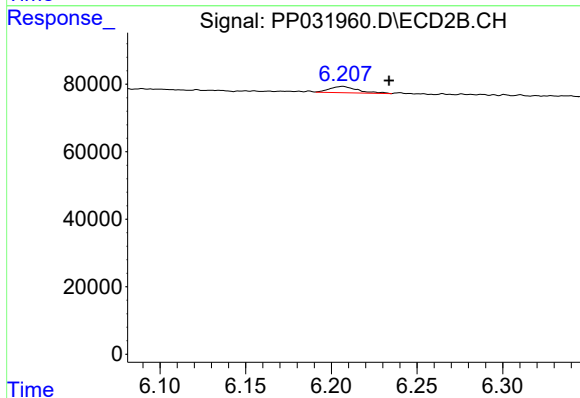


#25 AR-1248-5

R.T.: 6.207 min
Delta R.T.: -0.027 min
Response: 21567
Conc: 14.78 ng/ml

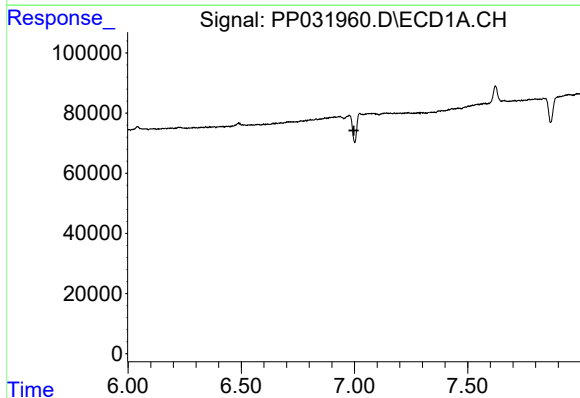


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.998 min
Response: 0
Conc: N.D.

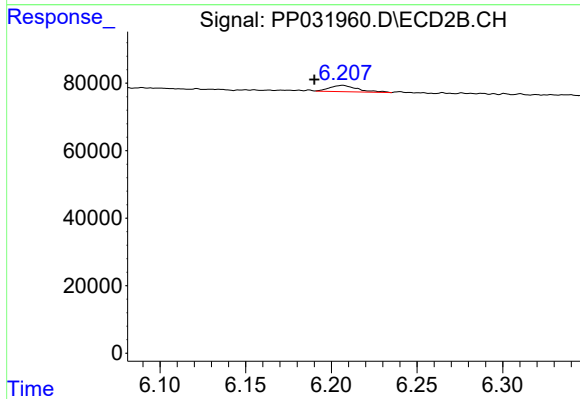

#26 AR-1254-1


R.T.: 6.207 min
Delta R.T.: 0.017 min
Response: 21567
Conc: 9.97 ng/ml

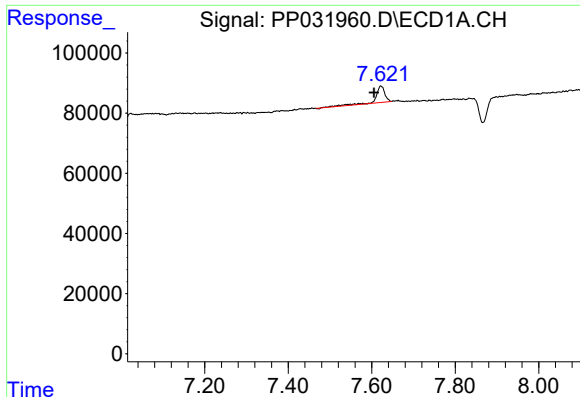

#28 AR-1254-3


R.T.: 7.622 min
Delta R.T.: 0.016 min
Response: 82490
Conc: 32.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

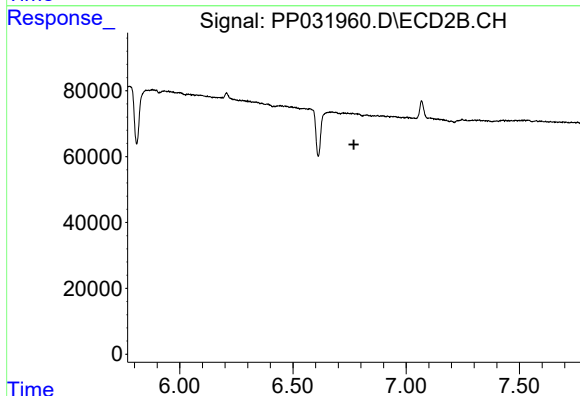


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.769 min
Response: 0
Conc: N.D.

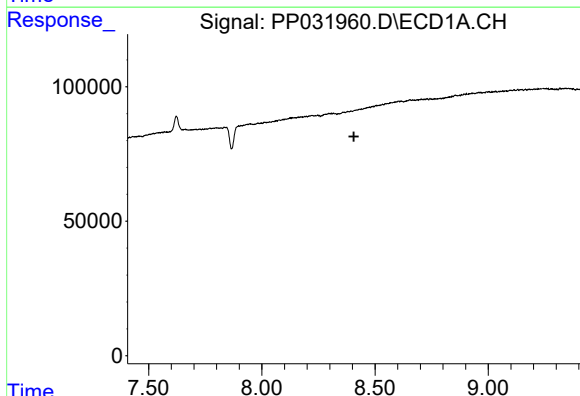


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.406 min
Response: 0
Conc: N.D.

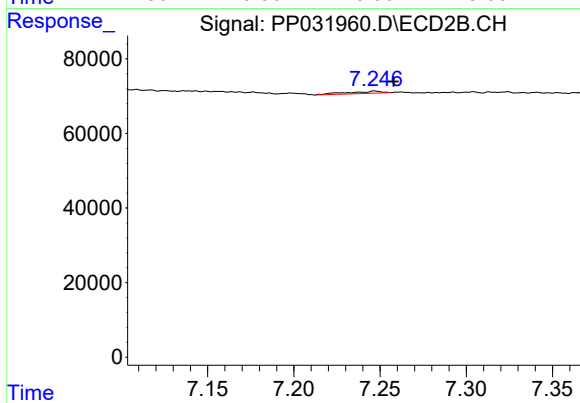

#33 AR-1260-3


R.T.: 7.247 min
Delta R.T.: -0.011 min
Response: 8340
Conc: 3.65 ng/ml

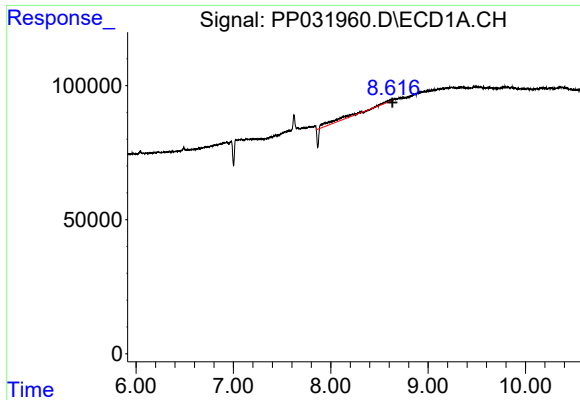

#34 AR-1260-4


R.T.: 8.617 min
Delta R.T.: -0.017 min
Response: 144206
Conc: 78.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

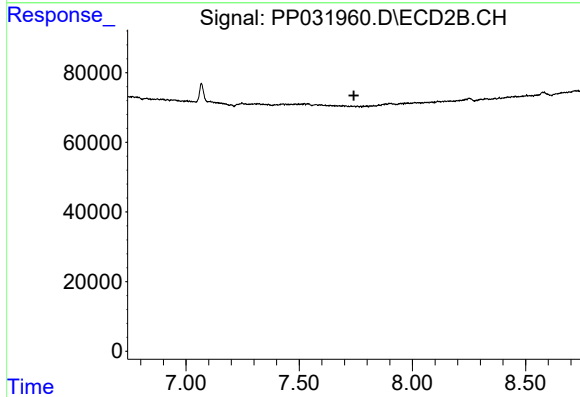


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.741 min
Response: 0
Conc: N.D.

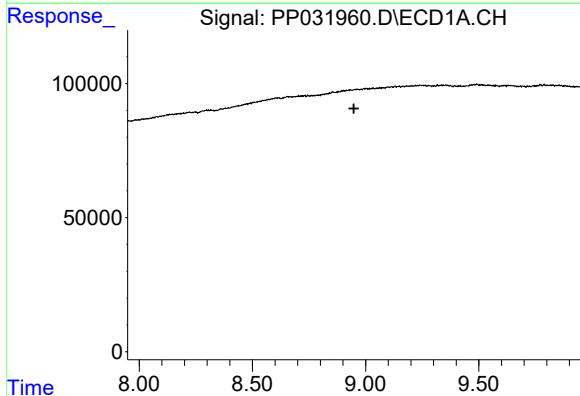


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.948 min
Response: 0
Conc: N.D.

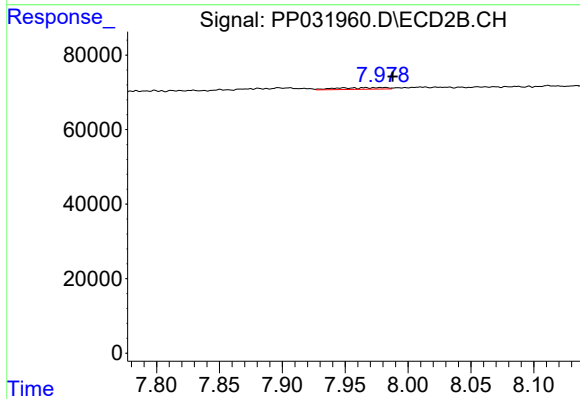

#35 AR-1260-5


R.T.: 7.982 min
Delta R.T.: -0.006 min
Response: 11929
Conc: 2.63 ng/ml

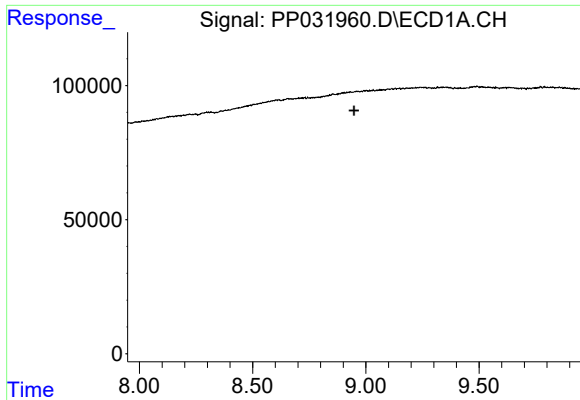

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.948 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

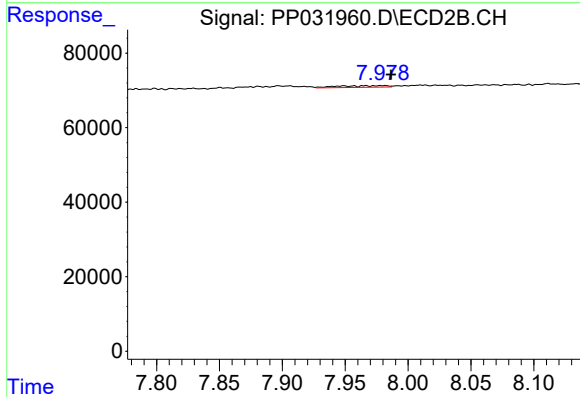


#37 AR-1262-2

R.T.: 7.982 min
Delta R.T.: -0.005 min
Response: 11929
Conc: 2.46 ng/ml

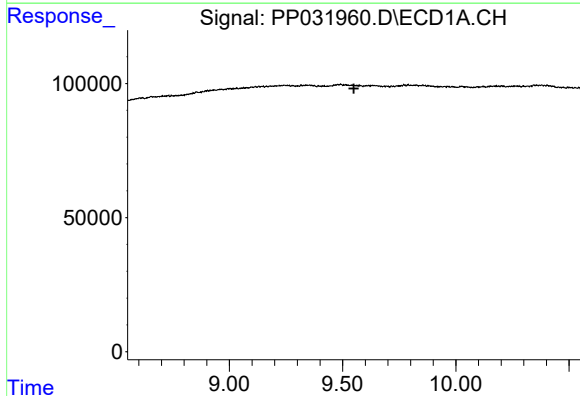

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.550 min
Response: 0
Conc: N.D.

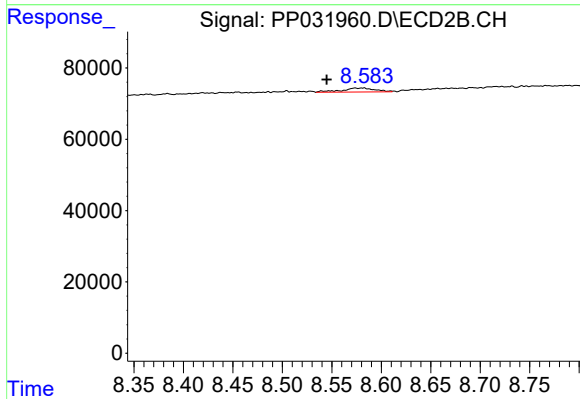

#43 AR-1268-3

R.T.: 8.574 min
Delta R.T.: 0.029 min
Response: 25260
Conc: 5.51 ng/ml