

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121021\
 Data File : PP041902.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Dec 2021 20:16
 Operator : AJ\MA
 Sample : M4962-03RE 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HIA775H-1-1RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 00:05:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 30 23:30:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.741	3.743	62149	88293	2.756	2.907m
2) SA Decachlor...	10.628	8.993	74337	50772	3.452m	3.285

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121021\
Data File : PP041902.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Dec 2021 20:16
Operator : AJ\MA
Sample : M4962-03RE 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HIA775H-1-1RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 00:05:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP113021.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 30 23:30:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

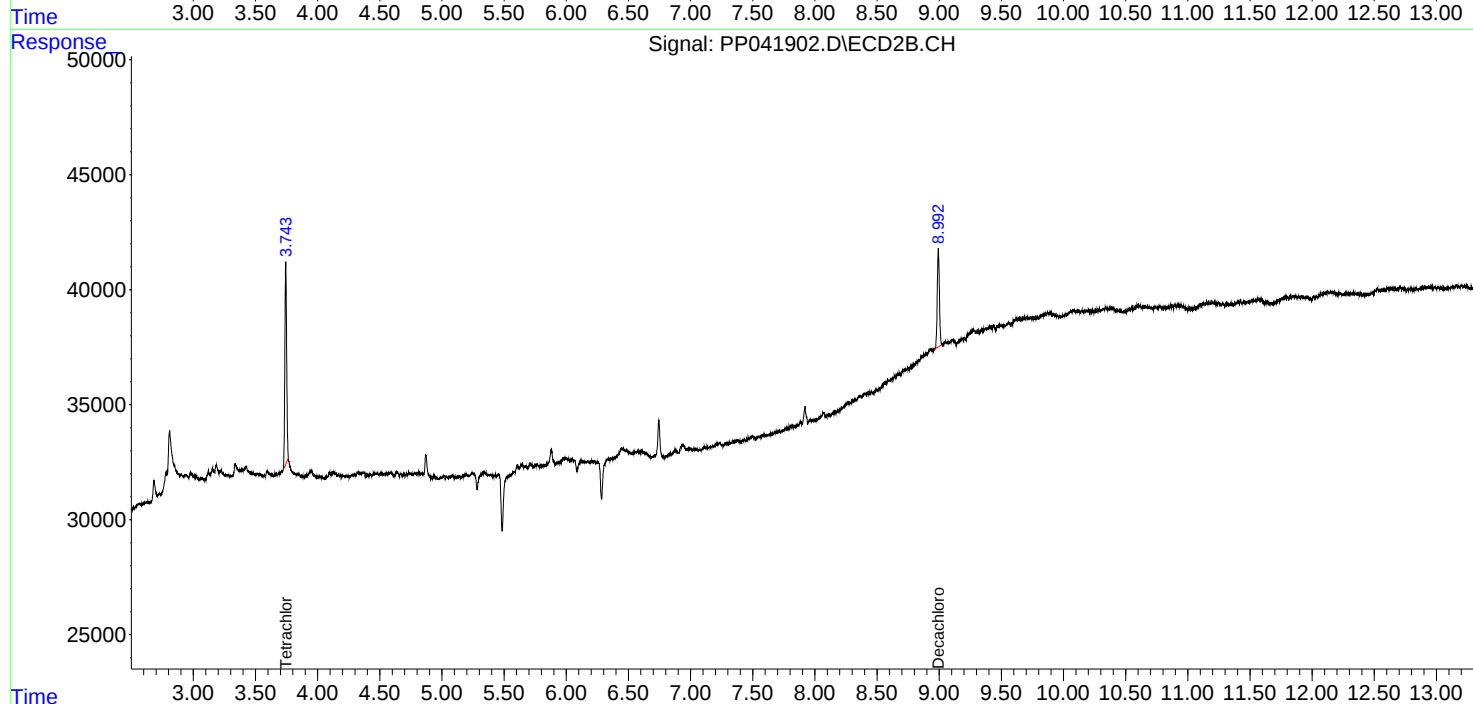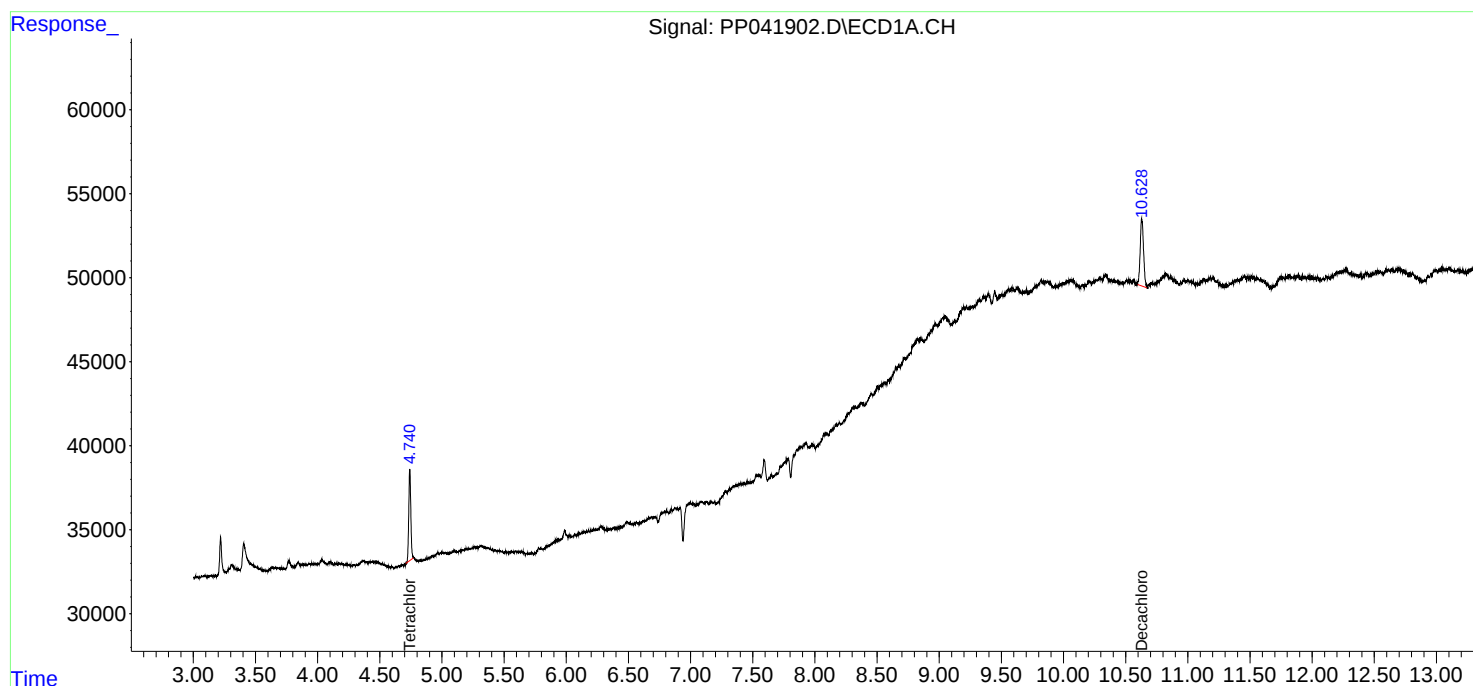


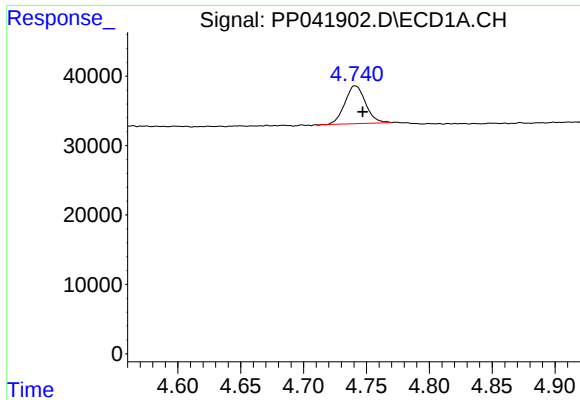

#1 Tetrachloro-m-xylene


R.T.: 4.741 min
Delta R.T.: -0.006 min
Response: 62149
Conc: 2.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
HIA775H-1-1RE

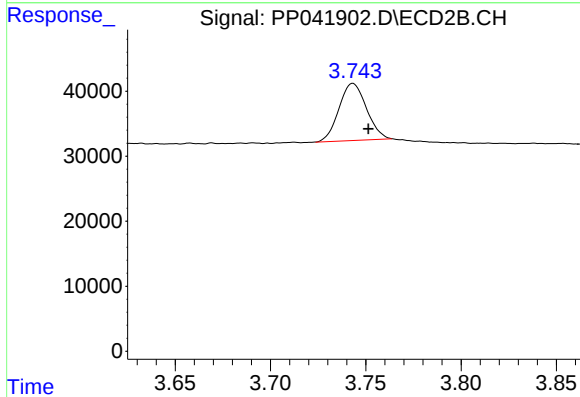


#1 Tetrachloro-m-xylene

R.T.: 3.743 min
Delta R.T.: -0.008 min
Response: 88293
Conc: 2.91 ng/ml m

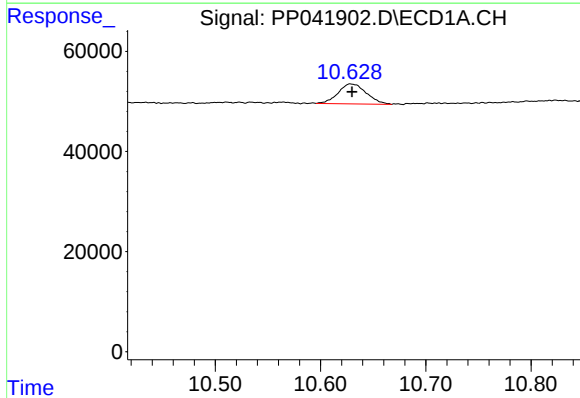

#2 Decachlorobiphenyl

R.T.: 10.628 min
Delta R.T.: -0.002 min
Response: 74337
Conc: 3.45 ng/ml m

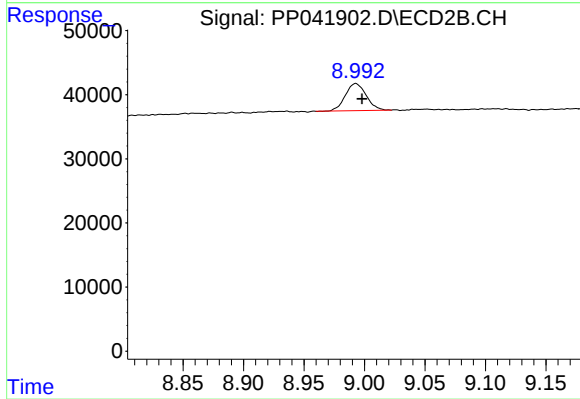

#2 Decachlorobiphenyl

R.T.: 8.993 min
Delta R.T.: -0.005 min
Response: 50772
Conc: 3.29 ng/ml