

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121120\
 Data File : PP032018.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Dec 2020 1:05
 Operator : DD\AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1268ICC050

Manual Integrations
 APPROVED

Ankita
 12/14/2020 3:18:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 04:47:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 04:44:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.780	4.052	274230	236689	5.344	5.013
2) SA Decachlor...	10.643	9.345	273823	302001	4.925	5.129
Target Compounds						
41) L9 AR-1268-1	9.232	8.255	257967	266652	49.020	53.076m
42) L9 AR-1268-2	9.322	8.320	230250	243698	46.593	46.917
43) L9 AR-1268-3	9.536	8.526	212314	228664	48.594	52.669m
44) L9 AR-1268-4	9.944	8.816	60716	70567	41.860	47.344
45) L9 AR-1268-5	10.333	9.100	566802	587179	45.431	44.362m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121120\
Data File : PP032018.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Dec 2020 1:05
Operator : DD\AJ
Sample : AR1268ICC050
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Ankita
12/14/2020 3:18:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 04:47:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 04:44:47 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

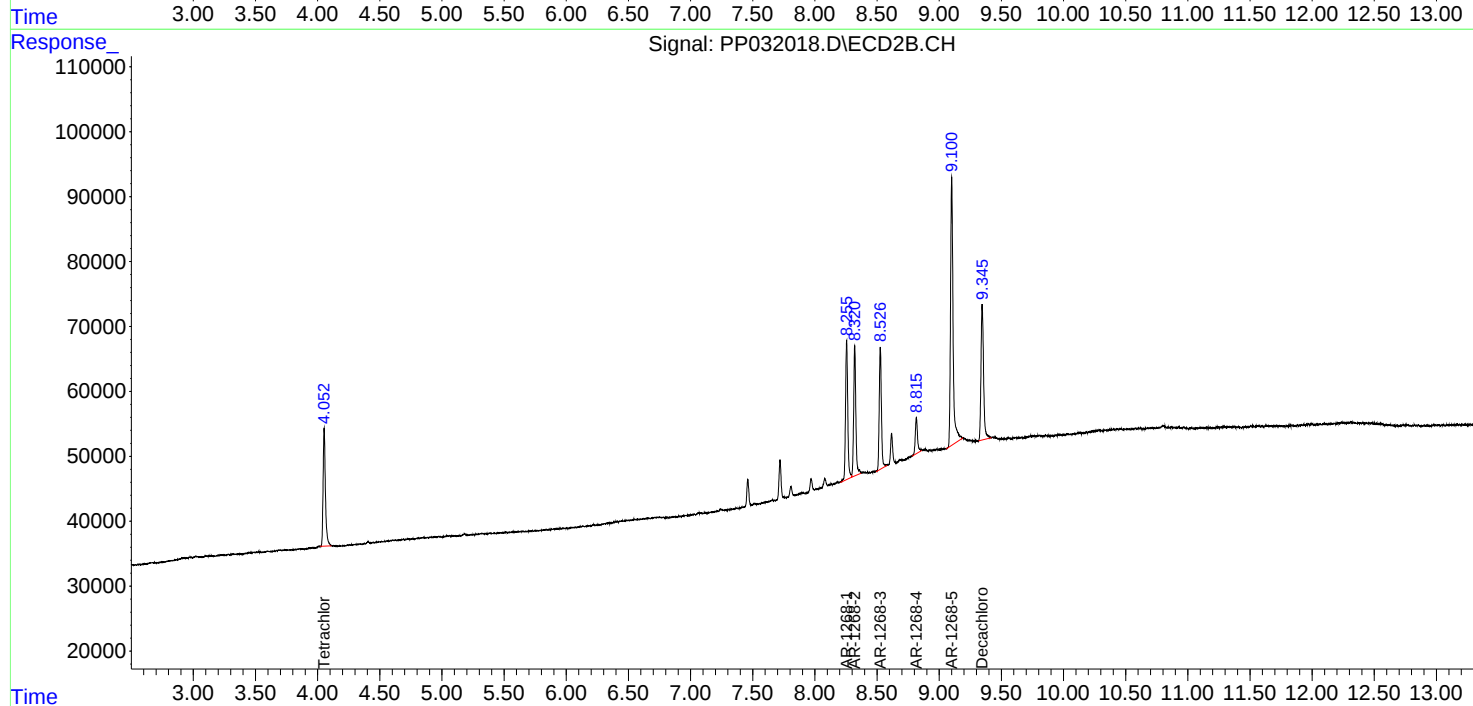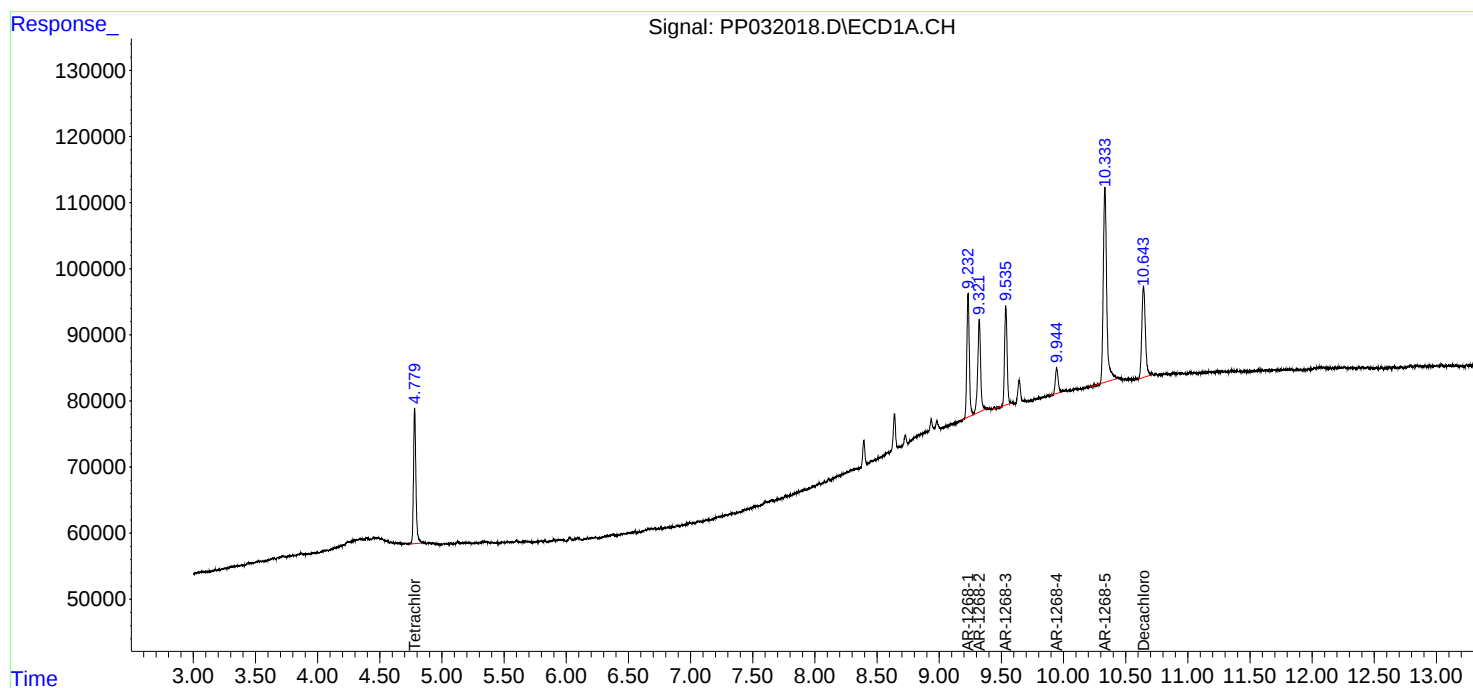

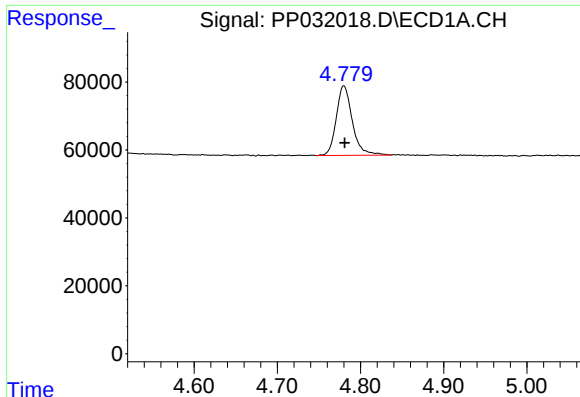


#1 Tetrachloro-m-xylene

R.T.: 4.780 min
Delta R.T.: -0.001 min
Response: 274230
Conc: 5.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Ankita
12/14/2020 3:18:38 PM

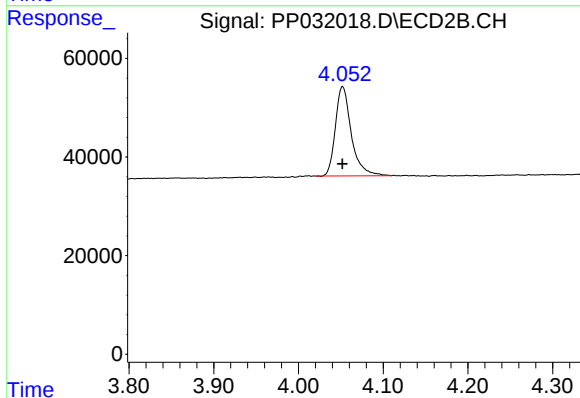


#1 Tetrachloro-m-xylene

R.T.: 4.052 min
Delta R.T.: 0.000 min
Response: 236689
Conc: 5.01 ng/ml

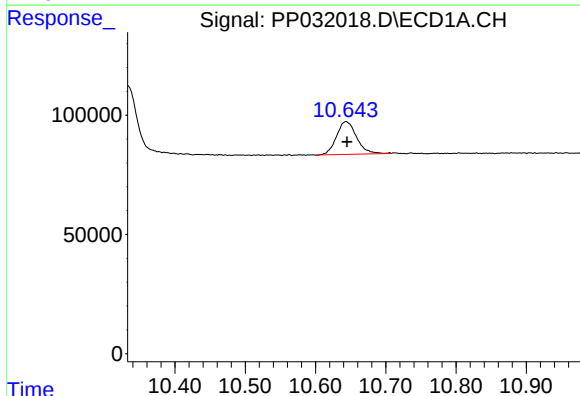


#2 Decachlorobiphenyl

R.T.: 10.643 min
Delta R.T.: -0.001 min
Response: 273823
Conc: 4.92 ng/ml

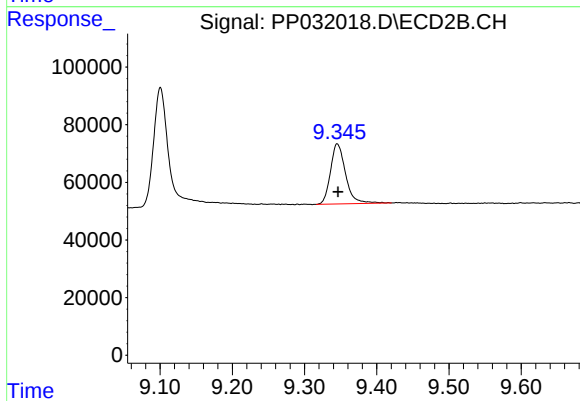

#2 Decachlorobiphenyl

R.T.: 9.345 min
Delta R.T.: -0.001 min
Response: 302001
Conc: 5.13 ng/ml

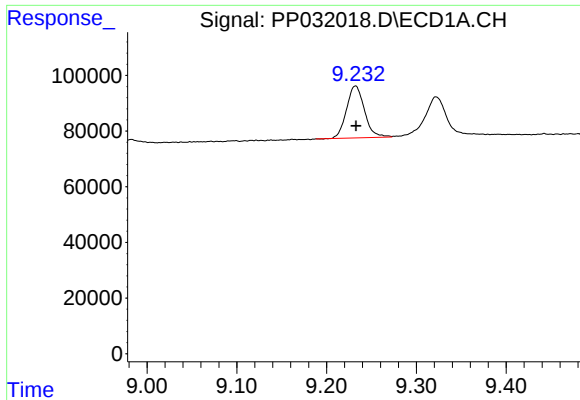


#41 AR-1268-1

R.T.: 9.232 min
Delta R.T.: 0.000 min
Response: 257967
Conc: 49.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Ankita
12/14/2020 3:18:38 PM

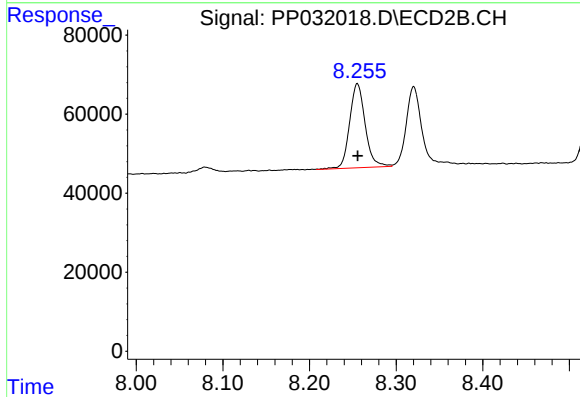


#41 AR-1268-1

R.T.: 8.255 min
Delta R.T.: 0.000 min
Response: 266652
Conc: 53.08 ng/ml m

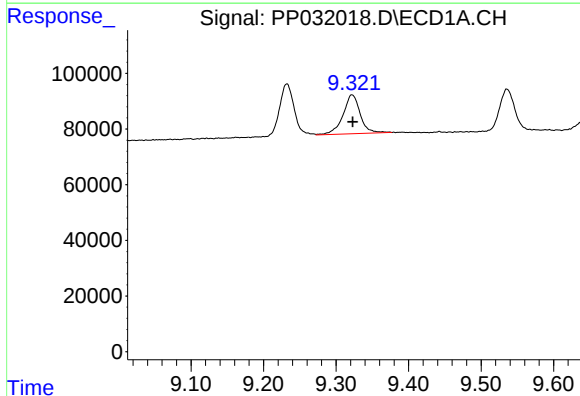


#42 AR-1268-2

R.T.: 9.322 min
Delta R.T.: 0.000 min
Response: 230250
Conc: 46.59 ng/ml

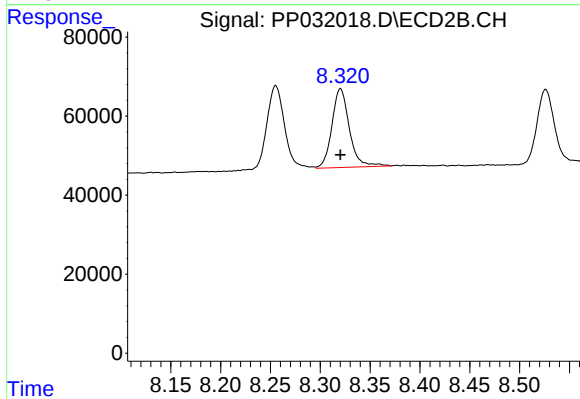

#42 AR-1268-2

R.T.: 8.320 min
Delta R.T.: 0.000 min
Response: 243698
Conc: 46.92 ng/ml

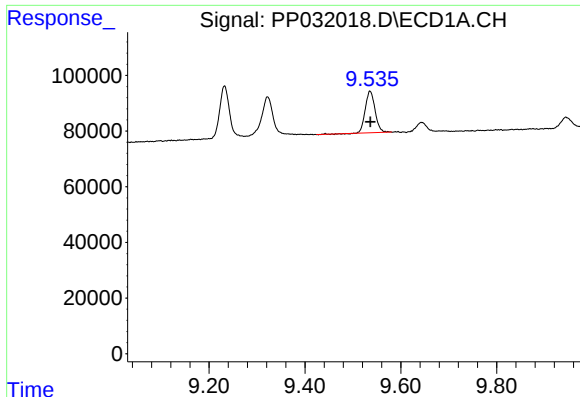


#43 AR-1268-3

R.T.: 9.536 min
Delta R.T.: -0.001 min
Response: 212314
Conc: 48.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050


Manual Integrations
APPROVED

Ankita
12/14/2020 3:18:38 PM

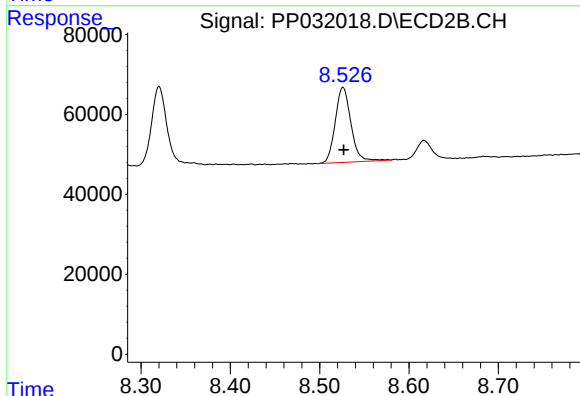


#43 AR-1268-3

R.T.: 8.526 min
Delta R.T.: -0.001 min
Response: 228664
Conc: 52.67 ng/ml m

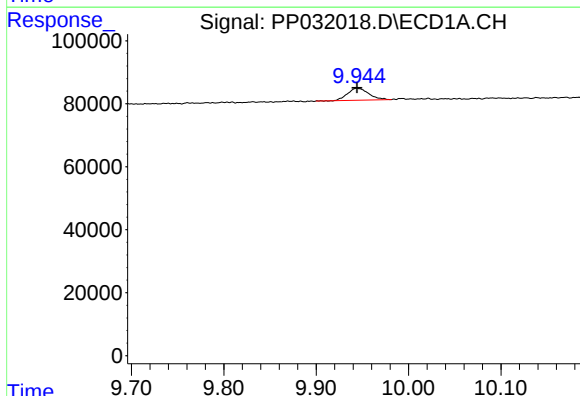


#44 AR-1268-4

R.T.: 9.944 min
Delta R.T.: 0.000 min
Response: 60716
Conc: 41.86 ng/ml

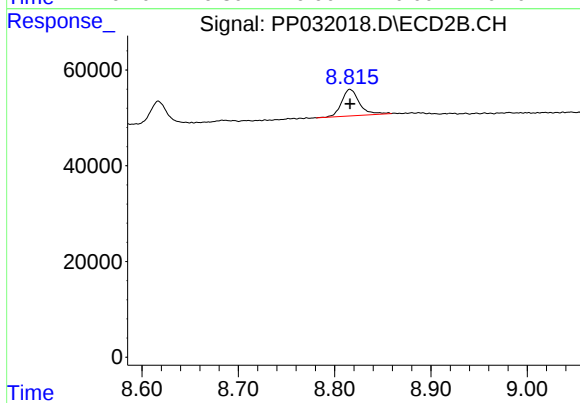

#44 AR-1268-4

R.T.: 8.816 min
Delta R.T.: 0.000 min
Response: 70567
Conc: 47.34 ng/ml

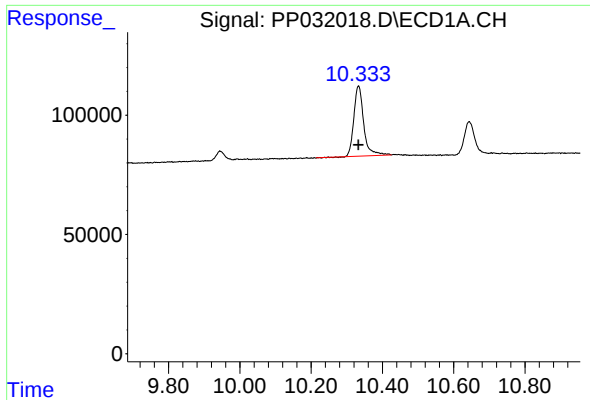


#45 AR-1268-5

R.T.: 10.333 min
Delta R.T.: 0.000 min
Response: 566802
Conc: 45.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1268ICC050

Manual Integrations
APPROVED

Ankita
12/14/2020 3:18:38 PM

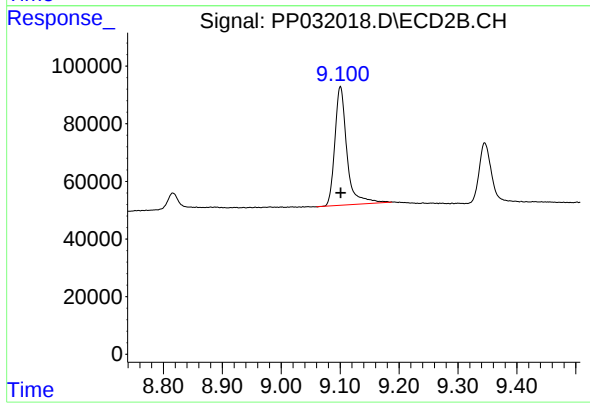

#45 AR-1268-5

R.T.: 9.100 min
Delta R.T.: -0.001 min
Response: 587179
Conc: 44.36 ng/ml m