

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121123\
 Data File : PP062356.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2023 17:12
 Operator : YP\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 05:14:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 12 05:13:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds								
7)	L1	AR-1016-5	0.000	5.288	0	850752	N.D.	10.293 #
15)	L3	AR-1232-5	0.000	5.288	0	850752	N.D.	25.166 #
20)	L4	AR-1242-5	0.000	5.675f	0	760255	N.D.	10.903 #
24)	L5	AR-1248-4	0.000	5.288	0	850752	N.D.	7.810 #
25)	L5	AR-1248-5	0.000	5.675f	0	760255	N.D.	5.481 #
26)	L6	AR-1254-1	0.000	5.675f	0	760255	N.D.	4.767 #
28)	L6	AR-1254-3	7.057	0.000	7041675	0	65.041	N.D. #
32)	L7	AR-1260-2	7.498f	6.514	143259	562884	1.675	3.090 #
33)	L7	AR-1260-3	0.000	6.695	0	618344	N.D.	3.436 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121123\
Data File : PP062356.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2023 17:12
Operator : YP\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 05:14:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 12 05:13:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

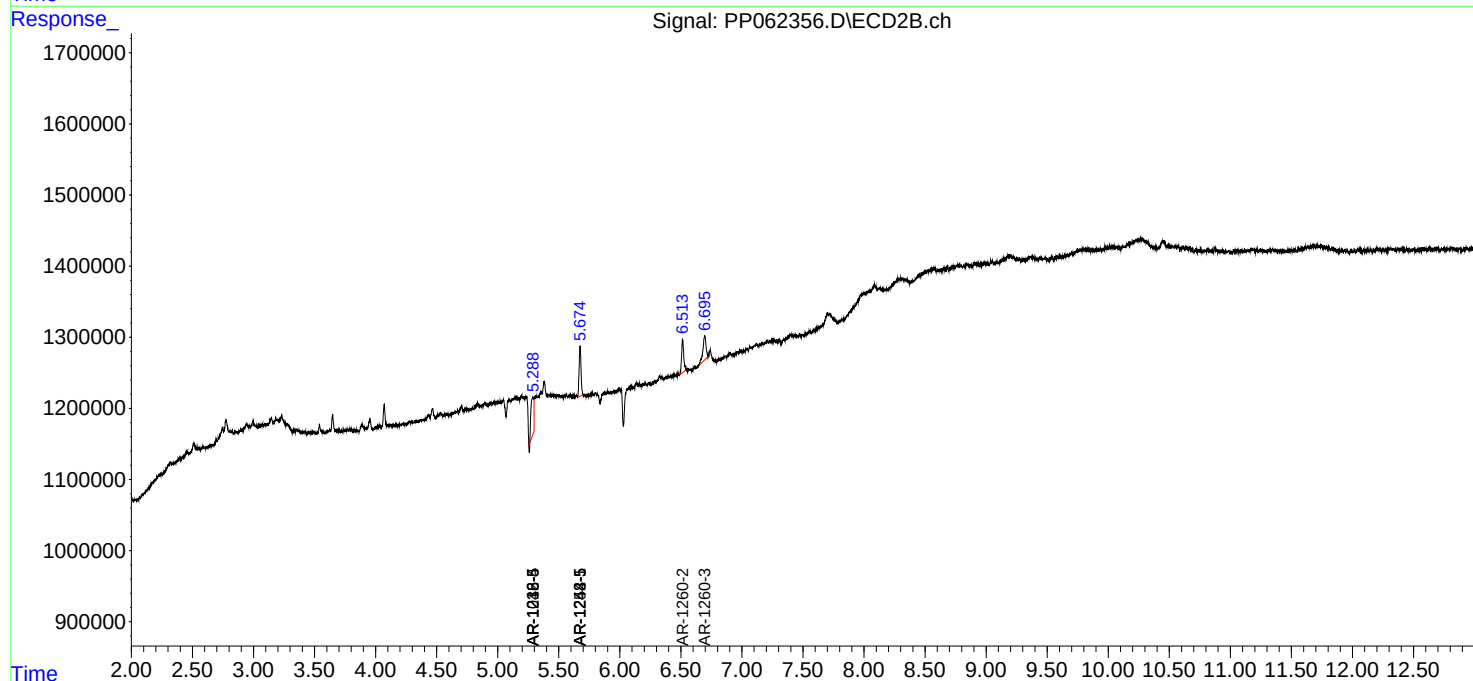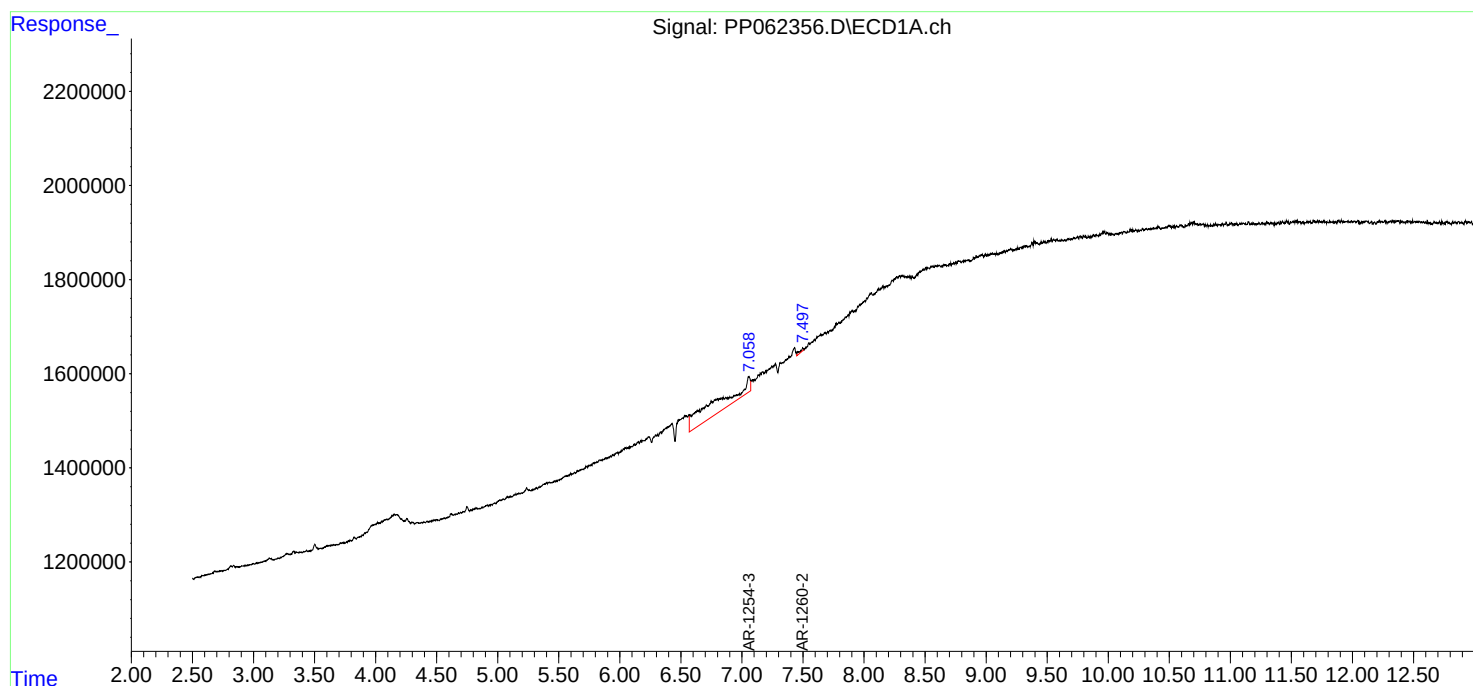

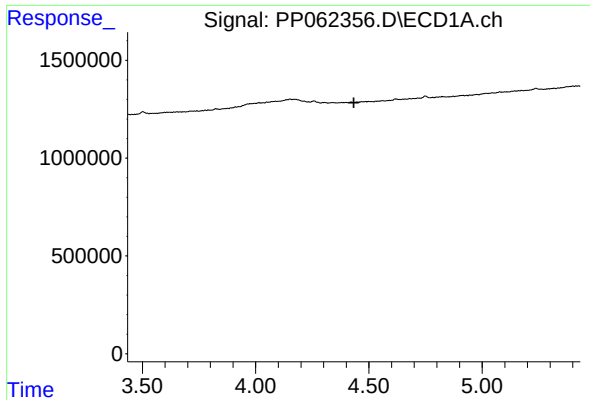

#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.720 min
Response: 0
Conc: N.D.

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.212 min
Response: 0
Conc: N.D.

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.838 min
Response: 0
Conc: N.D.

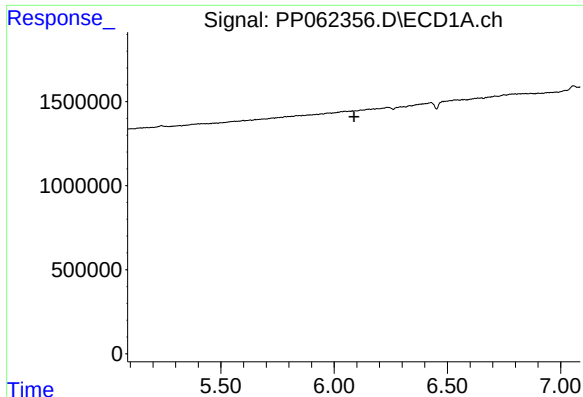

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

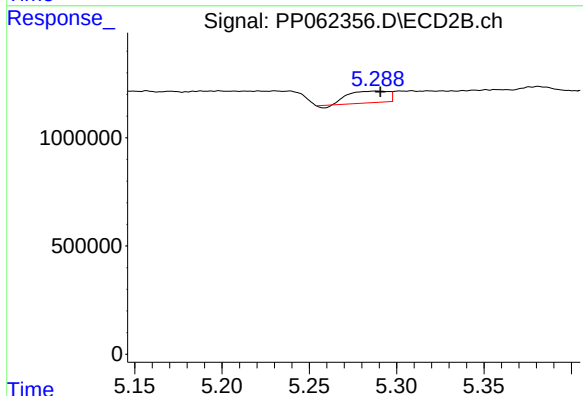


#7 AR-1016-5

R.T.: 5.288 min
Delta R.T.: -0.003 min
Response: 850752
Conc: 10.29 ng/ml

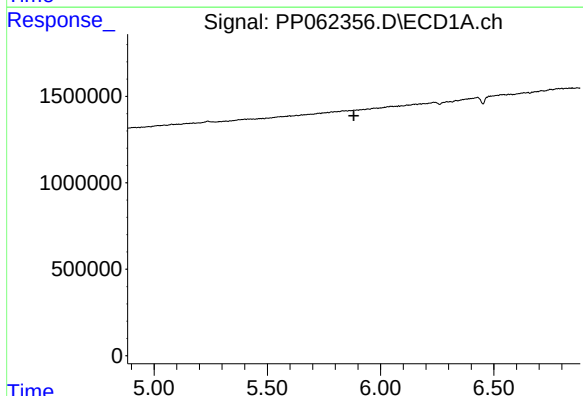


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.882 min
Response: 0
Conc: N.D.

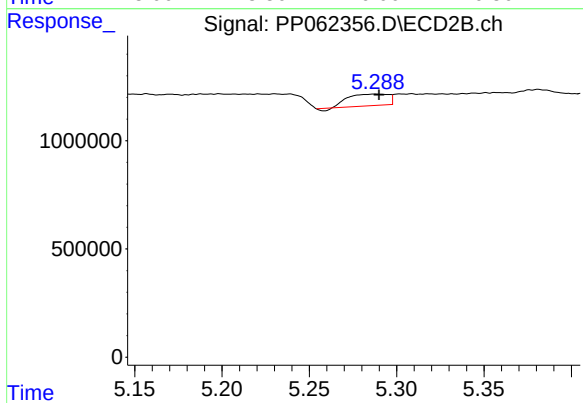

#15 AR-1232-5


R.T.: 5.288 min
Delta R.T.: -0.002 min
Response: 850752
Conc: 25.17 ng/ml

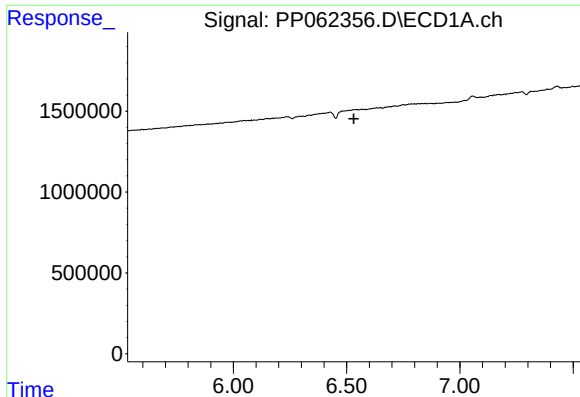

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.532 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

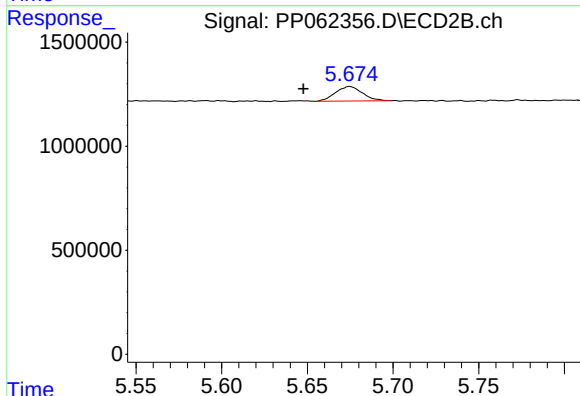


#20 AR-1242-5

R.T.: 5.675 min
Delta R.T.: 0.027 min
Response: 760255
Conc: 10.90 ng/ml

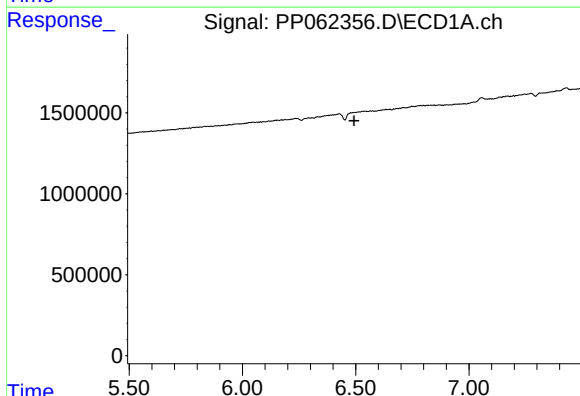


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.493 min
Response: 0
Conc: N.D.

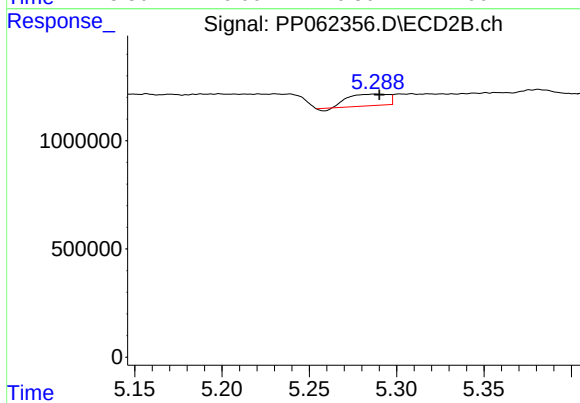

#24 AR-1248-4


R.T.: 5.288 min
Delta R.T.: -0.002 min
Response: 850752
Conc: 7.81 ng/ml

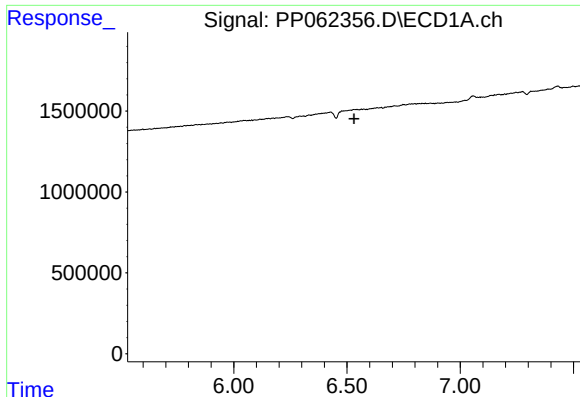

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.531 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

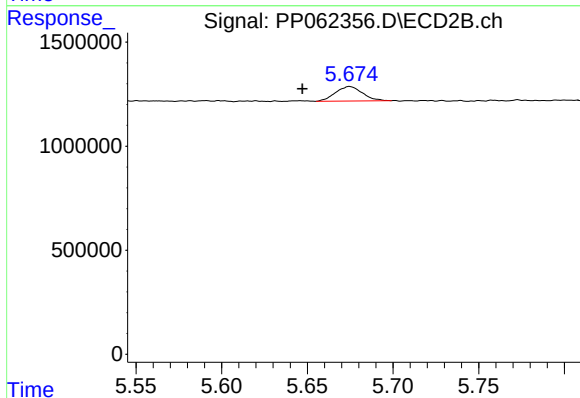


#25 AR-1248-5

R.T.: 5.675 min
Delta R.T.: 0.028 min
Response: 760255
Conc: 5.48 ng/ml

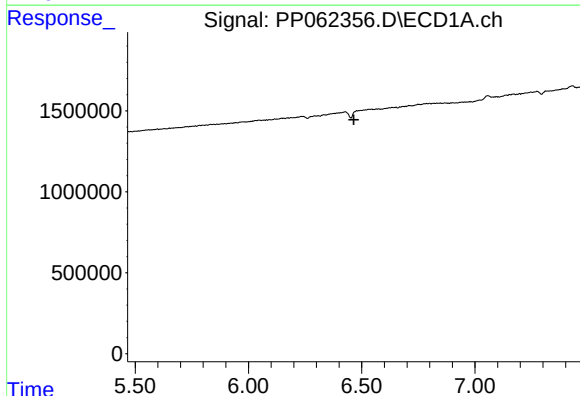


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.466 min
Response: 0
Conc: N.D.

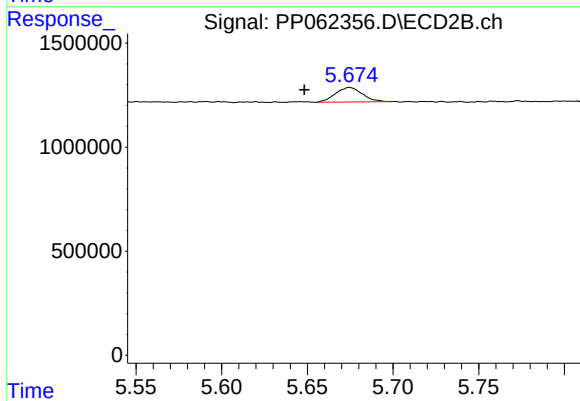

#26 AR-1254-1


R.T.: 5.675 min
Delta R.T.: 0.026 min
Response: 760255
Conc: 4.77 ng/ml

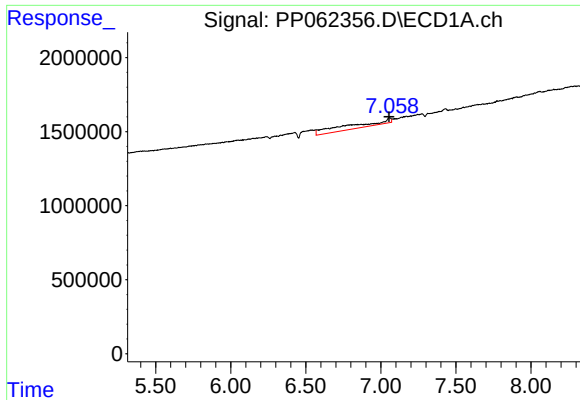

#28 AR-1254-3


R.T.: 7.057 min
Delta R.T.: 0.003 min
Response: 7041675
Conc: 65.04 ng/ml

Instrument :
ECD_P
ClientSampleId :

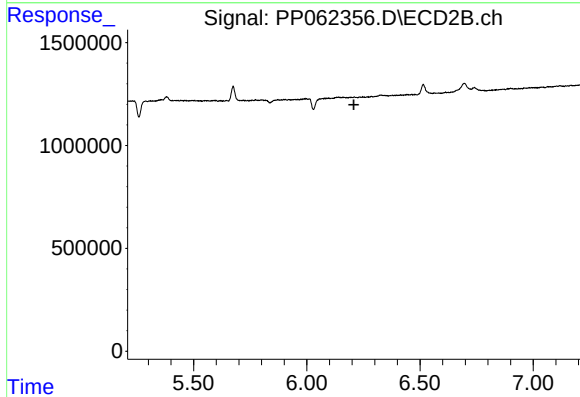


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.208 min
Response: 0
Conc: N.D.

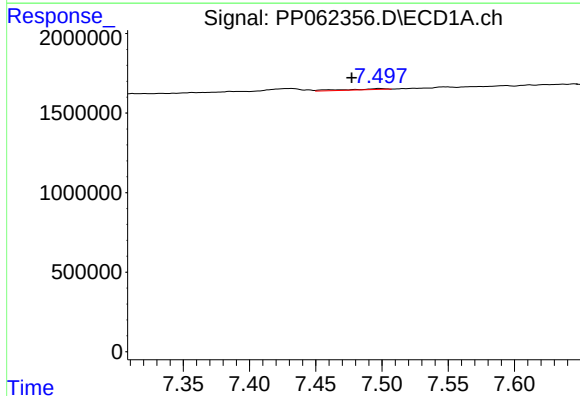


#32 AR-1260-2

R.T.: 7.498 min
Delta R.T.: 0.021 min
Response: 143259
Conc: 1.67 ng/ml

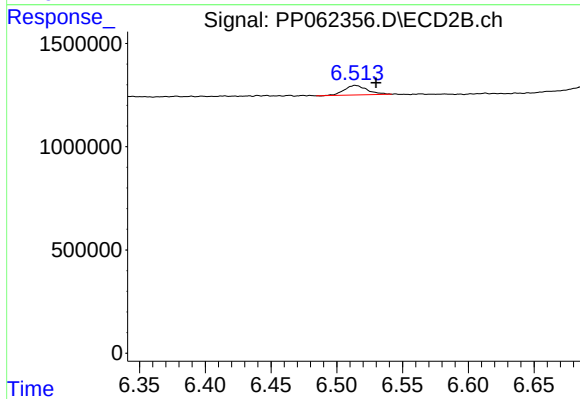

#32 AR-1260-2


R.T.: 6.514 min
Delta R.T.: -0.016 min
Response: 562884
Conc: 3.09 ng/ml

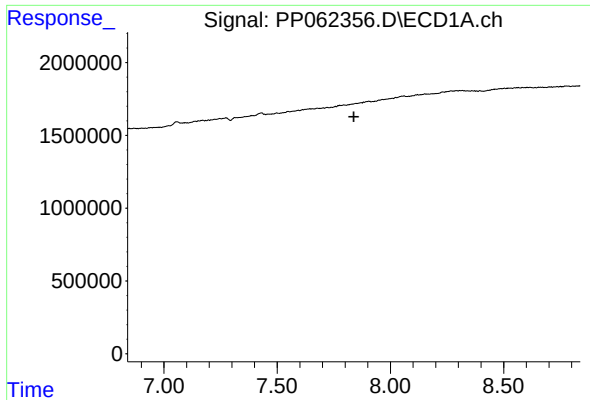

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 7.838 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

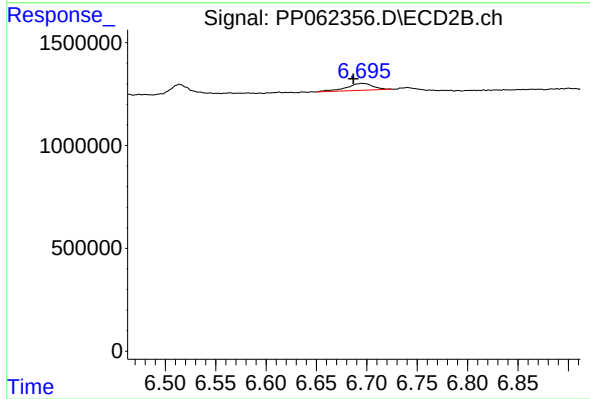

#33 AR-1260-3

R.T.: 6.695 min
Delta R.T.: 0.008 min
Response: 618344
Conc: 3.44 ng/ml