

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121220\
 Data File : PP032049.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Dec 2020 14:37
 Operator : DD\AJ
 Sample : L5013-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 12-10-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 04:54:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.780	4.052	1075659	950209	20.881	20.091
2)	SA Decachlor...	10.646	9.347	825352	844572	26.319	25.184
Target Compounds							
8)	L2 AR-1221-1	5.020	0.000	976124	0	1875.582	N.D. #
9)	L2 AR-1221-2	0.000	4.378f	0	776038	N.D.	2156.486 #
10)	L2 AR-1221-3	0.000	4.496	0	25164	N.D.	22.500 #
11)	L3 AR-1232-1	0.000	4.496	0	25164	N.D.	27.161 #
14)	L3 AR-1232-4	0.000	5.603	0	50511	N.D.	128.746 #
19)	L4 AR-1242-4	0.000	5.603	0	50511	N.D.	62.274 #
23)	L5 AR-1248-3	0.000	5.603	0	50511	N.D.	41.351 #
30)	L6 AR-1254-5	0.000	7.417	0	202058	N.D.	84.934 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121220\
Data File : PP032049.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Dec 2020 14:37
Operator : DD\AJ
Sample : L5013-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
12-10-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 04:54:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

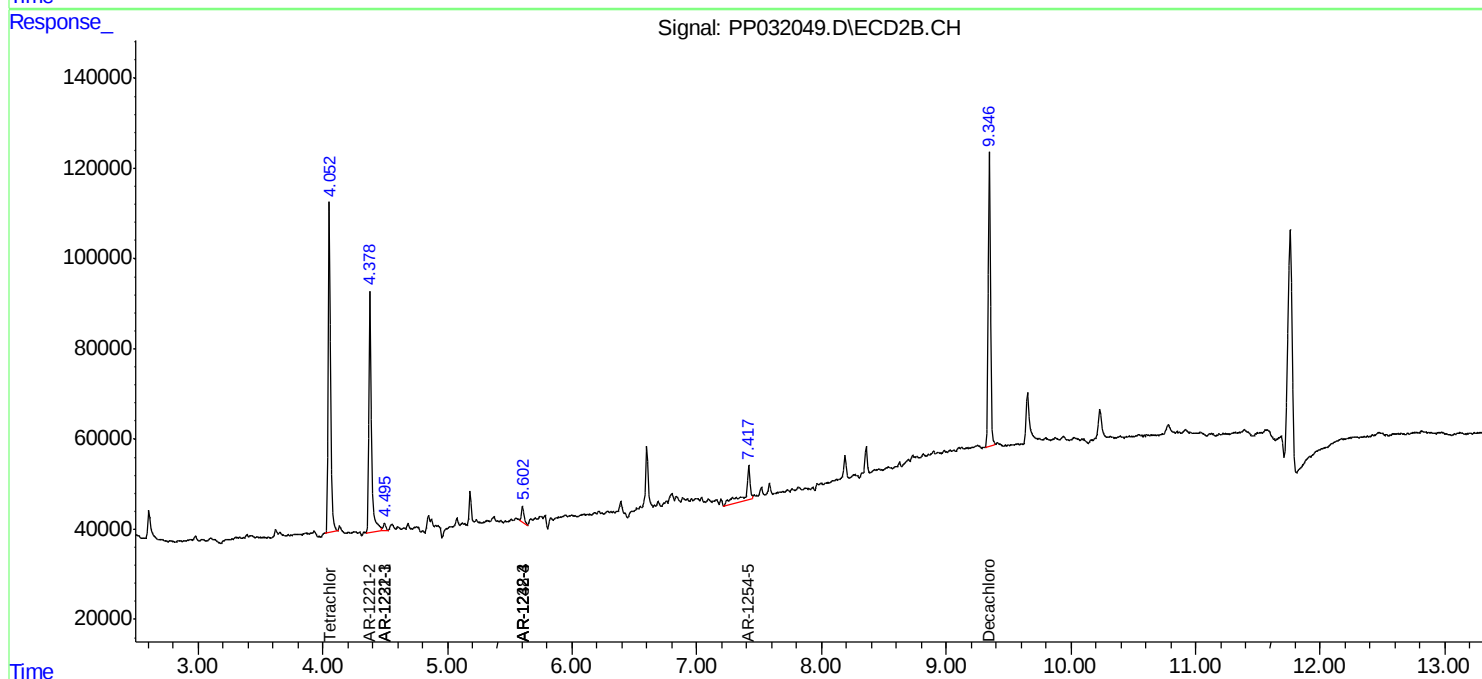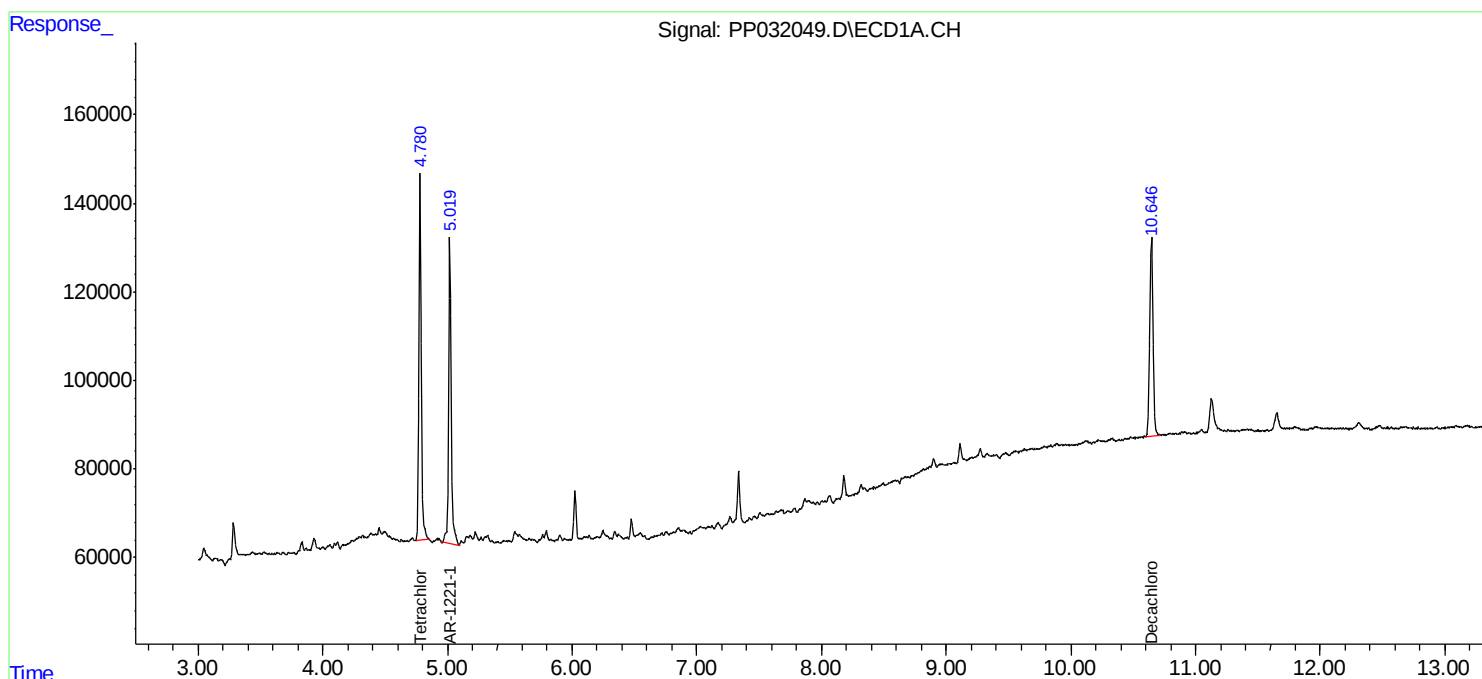


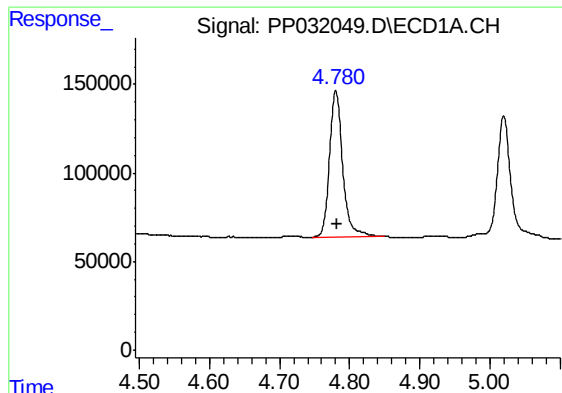

#1 Tetrachloro-m-xylene


R.T.: 4.780 min
Delta R.T.: -0.002 min
Response: 1075659
Conc: 20.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
12-10-A

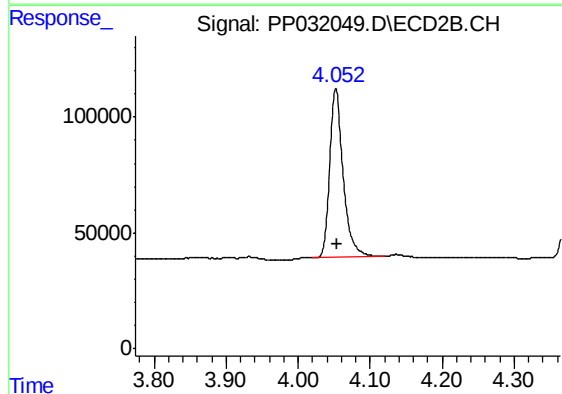


#1 Tetrachloro-m-xylene

R.T.: 4.052 min
Delta R.T.: -0.002 min
Response: 950209
Conc: 20.09 ng/ml

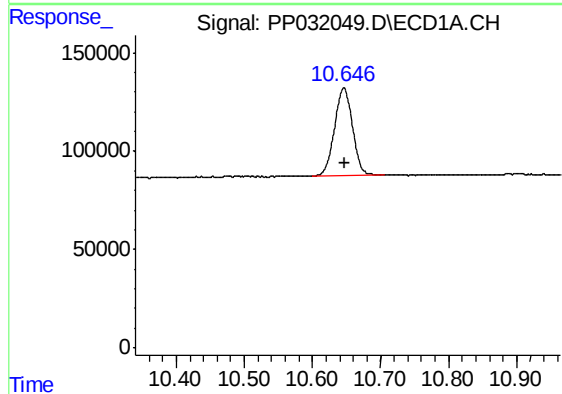


#2 Decachlorobiphenyl

R.T.: 10.646 min
Delta R.T.: 0.000 min
Response: 825352
Conc: 26.32 ng/ml

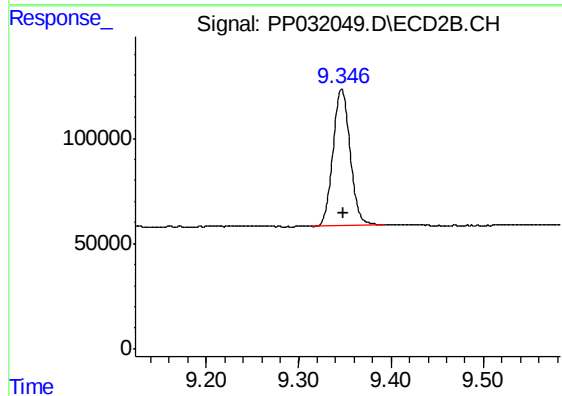

#2 Decachlorobiphenyl


R.T.: 9.347 min
Delta R.T.: -0.001 min
Response: 844572
Conc: 25.18 ng/ml

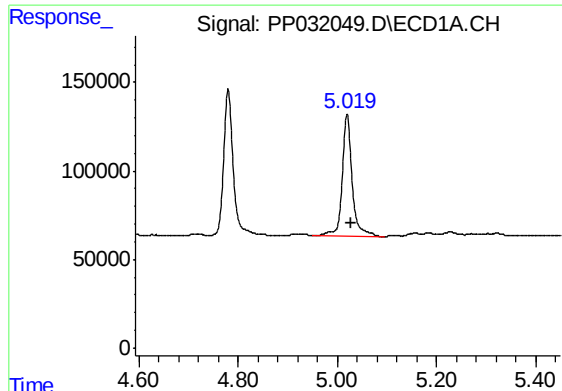

#8 AR-1221-1


R.T.: 5.020 min
Delta R.T.: -0.007 min
Response: 976124
Conc: 1875.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
12-10-A

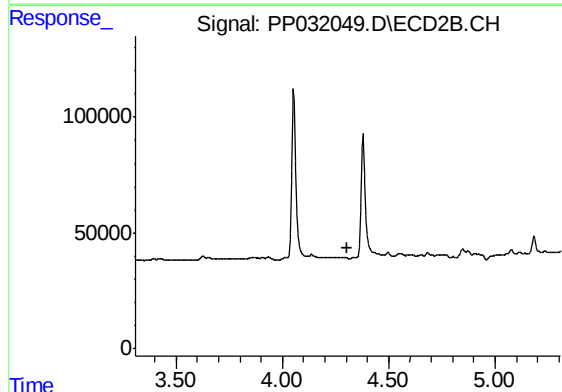


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.308 min
Response: 0
Conc: N.D.

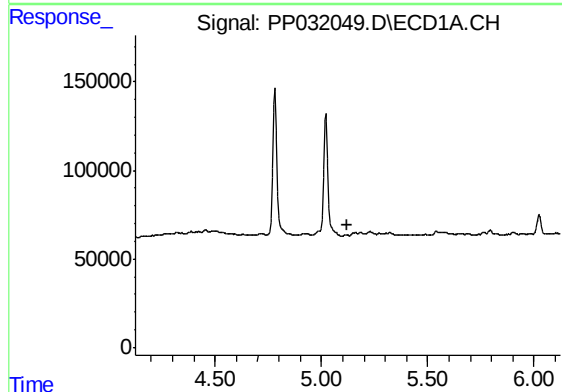


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.124 min
Response: 0
Conc: N.D.

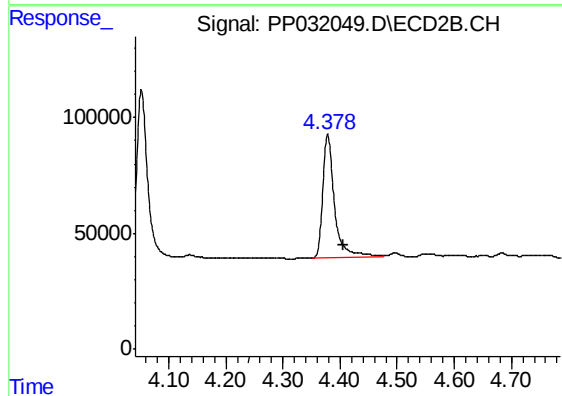

#9 AR-1221-2


R.T.: 4.378 min
Delta R.T.: -0.028 min
Response: 776038
Conc: 2156.49 ng/ml

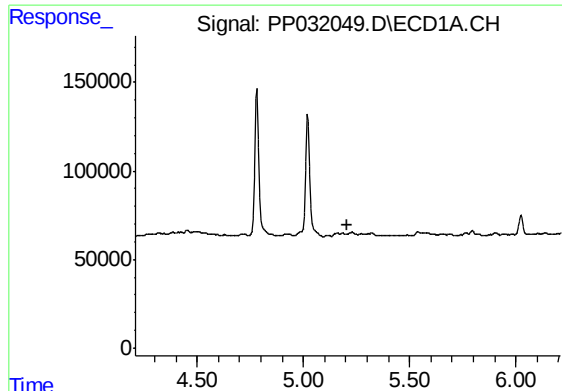

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 5.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
12-10-A

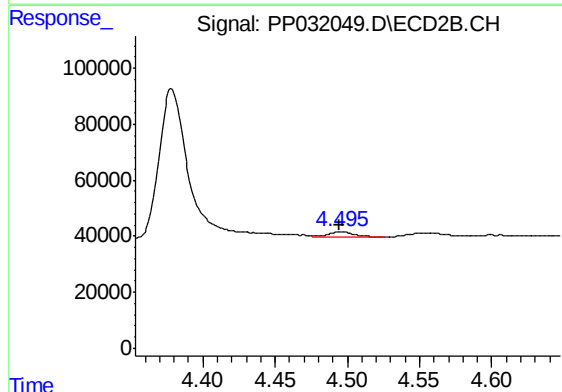


#10 AR-1221-3

R.T.: 4.496 min
Delta R.T.: 0.000 min
Response: 25164
Conc: 22.50 ng/ml

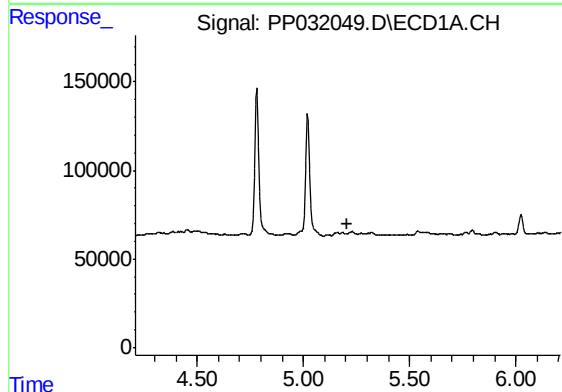


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 5.210 min
Response: 0
Conc: N.D.

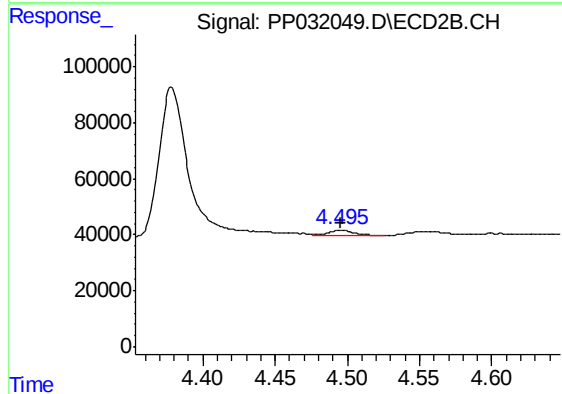

#11 AR-1232-1


R.T.: 4.496 min
Delta R.T.: 0.000 min
Response: 25164
Conc: 27.16 ng/ml

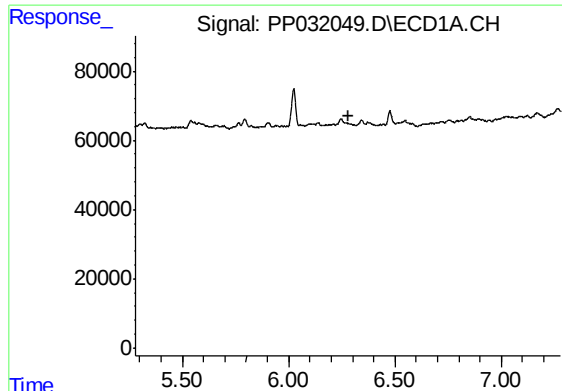

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 6.279 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
12-10-A

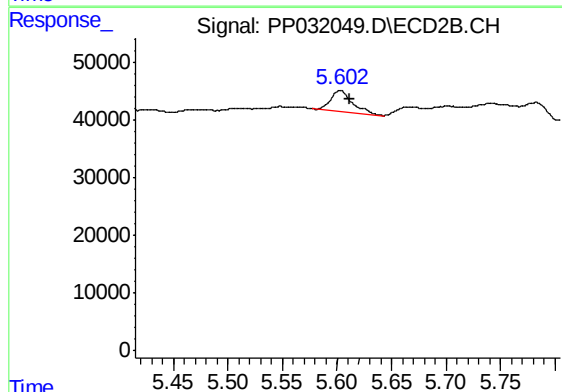


#14 AR-1232-4

R.T.: 5.603 min
Delta R.T.: -0.009 min
Response: 50511
Conc: 128.75 ng/ml

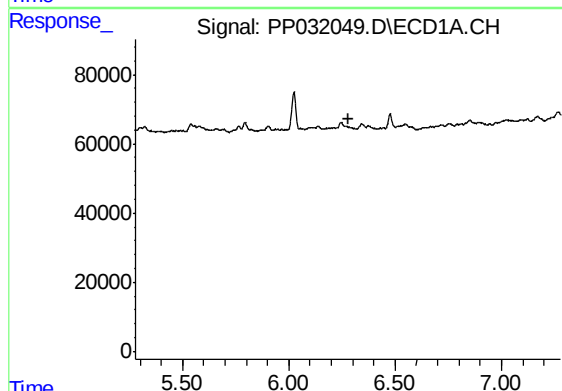


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 6.278 min
Response: 0
Conc: N.D.

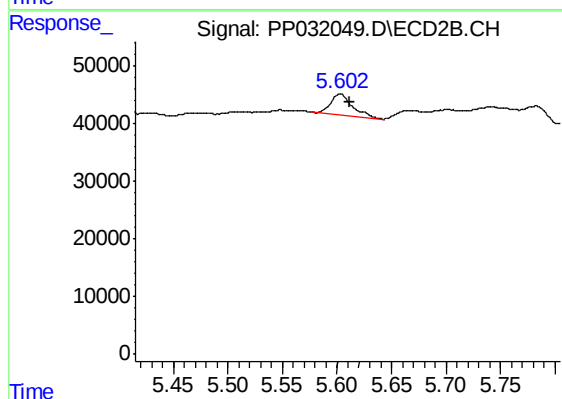

#19 AR-1242-4


R.T.: 5.603 min
Delta R.T.: -0.009 min
Response: 50511
Conc: 62.27 ng/ml

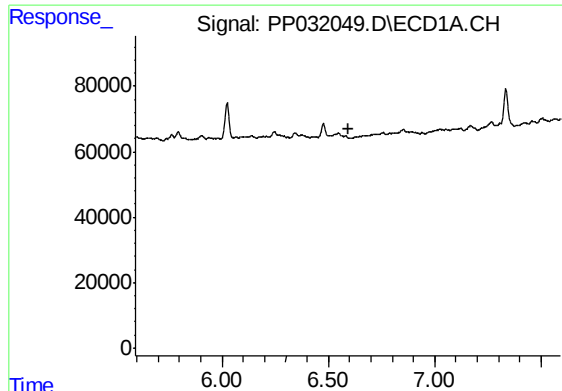

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T. : 6.592 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
12-10-A

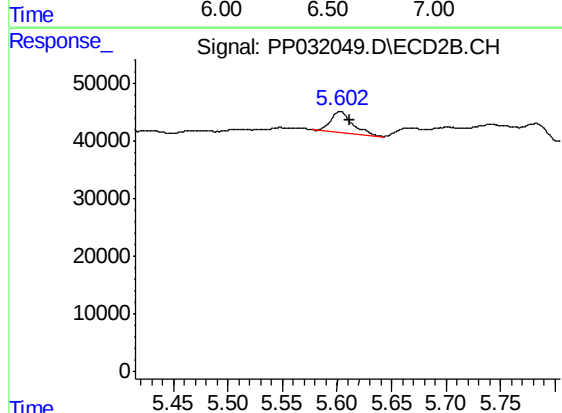


#23 AR-1248-3

R.T.: 5.603 min
Delta R.T.: -0.009 min
Response: 50511
Conc: 41.35 ng/ml

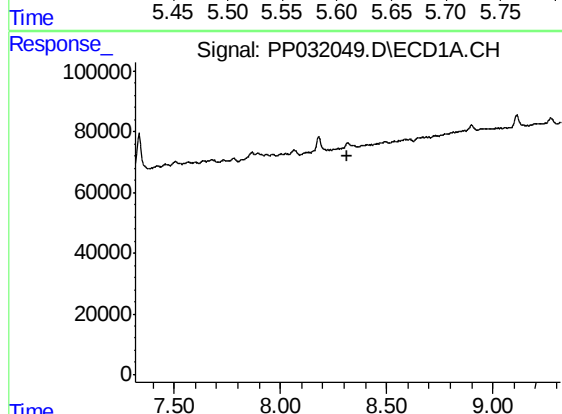

#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 8.318 min
Response: 0
Conc: N.D.

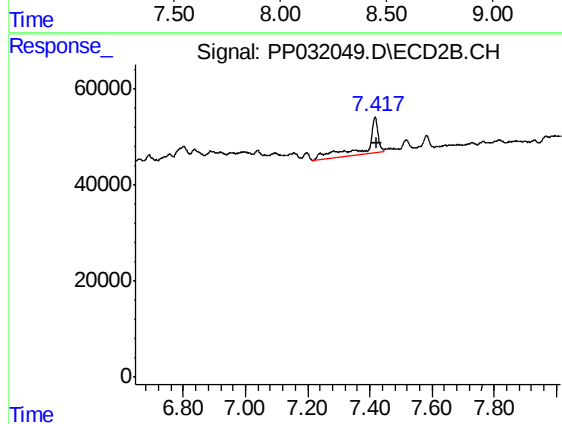

#30 AR-1254-5

R.T.: 7.417 min
Delta R.T.: -0.003 min
Response: 202058
Conc: 84.93 ng/ml