

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121220\
 Data File : PP032035.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Dec 2020 10:41
 Operator : DD\AJ
 Sample : L4987-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 32834

Manual Integrations
 APPROVED

Ankita
 12/14/2020 3:22:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 04:44:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.780	4.053	614732	605543	11.933	12.803
2)	SA Decachlor...	10.643	9.345	257595	254240	8.214	7.581
Target Compounds							
16)	L4 AR-1242-1	6.083	5.304	55693	37371	48.607	36.080 #
17)	L4 AR-1242-2	6.108	5.323	76344	65105	43.344	42.120
18)	L4 AR-1242-3	6.172	5.515	51228	52204	46.162	62.002m#
19)	L4 AR-1242-4	6.277	5.611	27765	52448	30.510m	64.662m#
20)	L4 AR-1242-5	7.049	6.175	94159	46328	108.555	52.093 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121220\
Data File : PP032035.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Dec 2020 10:41
Operator : DD\AJ
Sample : L4987-05
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
32834


Manual Integrations
APPROVED

Ankita
12/14/2020 3:22:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 04:44:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

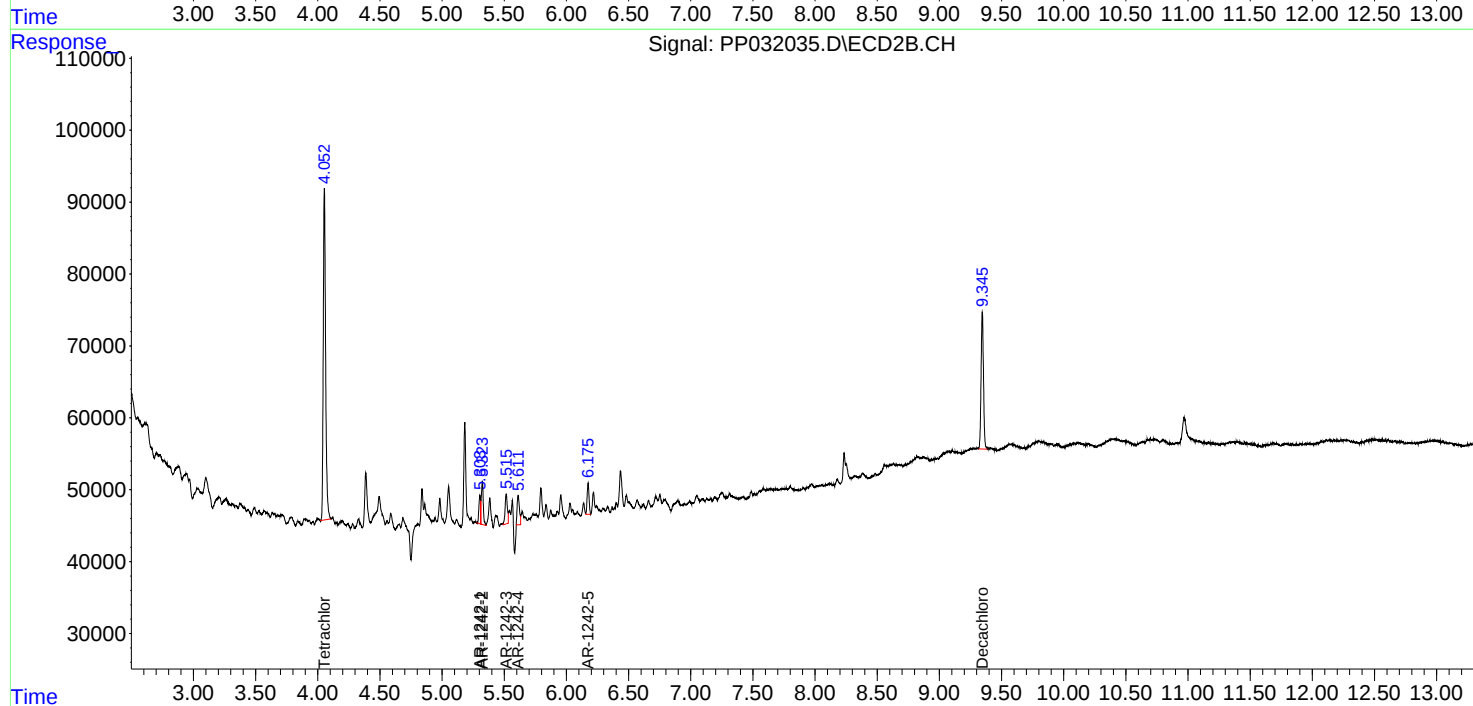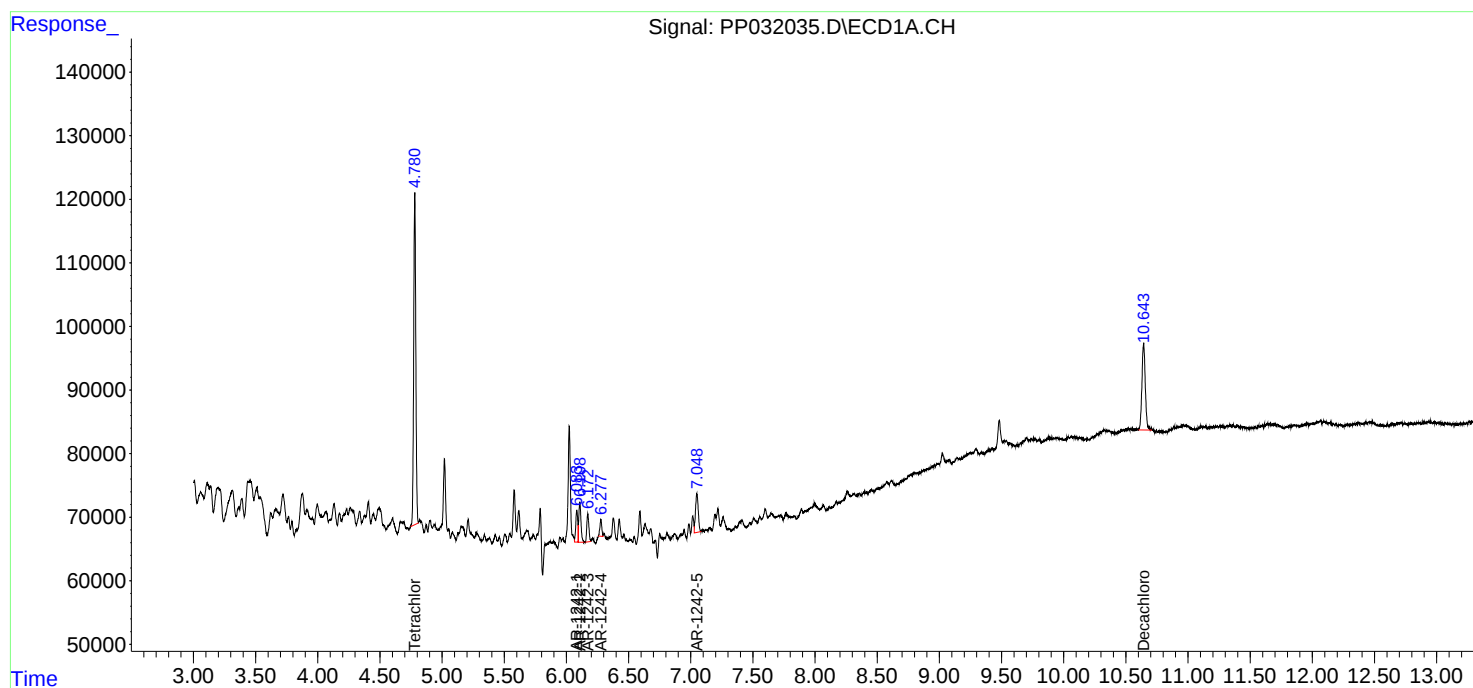

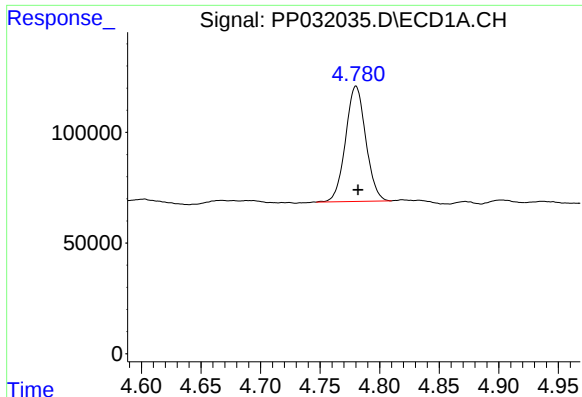


#1 Tetrachloro-m-xylene

R.T.: 4.780 min
Delta R.T.: -0.002 min
Response: 614732
Conc: 11.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
32834


Manual Integrations
APPROVED

Ankita
12/14/2020 3:22:59 PM

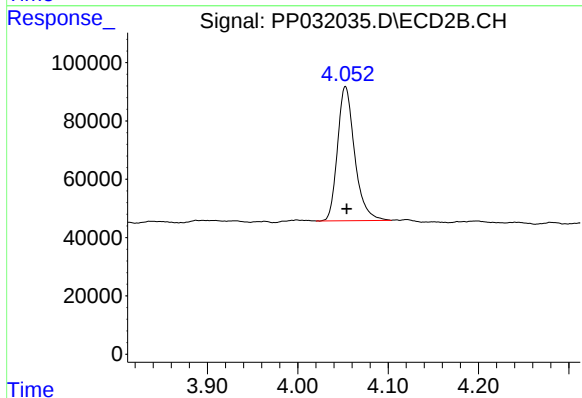


#1 Tetrachloro-m-xylene

R.T.: 4.053 min
Delta R.T.: -0.001 min
Response: 605543
Conc: 12.80 ng/ml

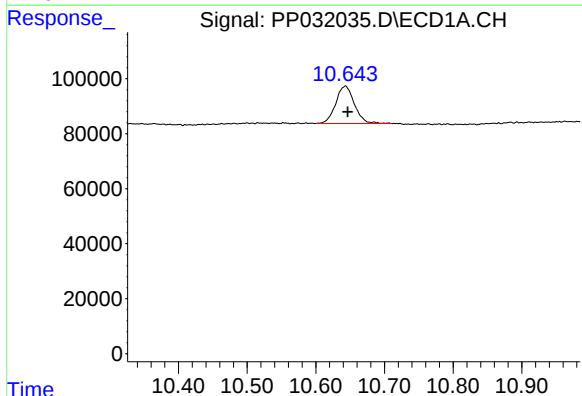


#2 Decachlorobiphenyl

R.T.: 10.643 min
Delta R.T.: -0.003 min
Response: 257595
Conc: 8.21 ng/ml

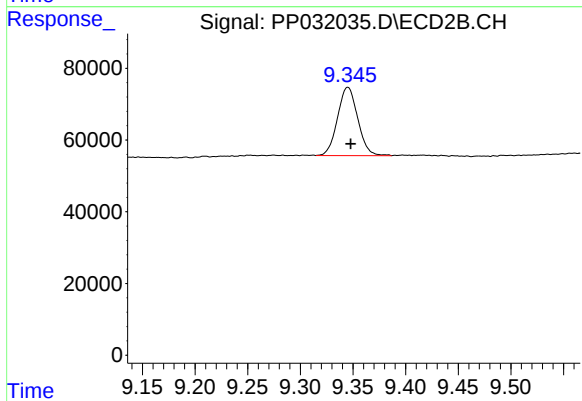

#2 Decachlorobiphenyl

R.T.: 9.345 min
Delta R.T.: -0.003 min
Response: 254240
Conc: 7.58 ng/ml

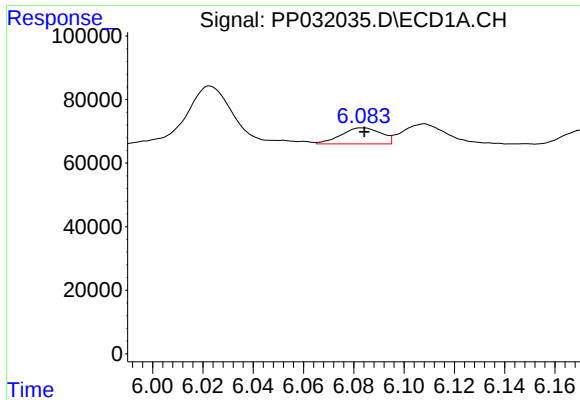


#16 AR-1242-1

R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 55693
Conc: 48.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
32834


Manual Integrations
APPROVED

Ankita
12/14/2020 3:22:59 PM

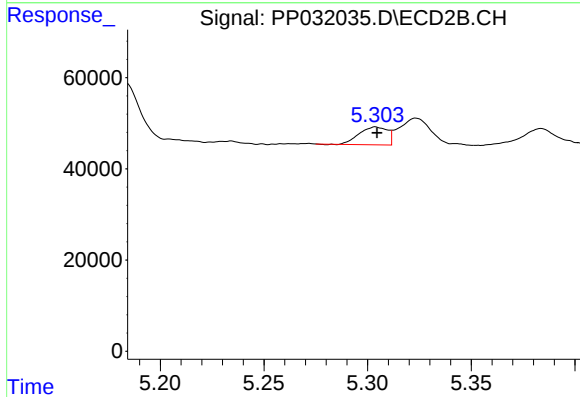


#16 AR-1242-1

R.T.: 5.304 min
Delta R.T.: 0.000 min
Response: 37371
Conc: 36.08 ng/ml

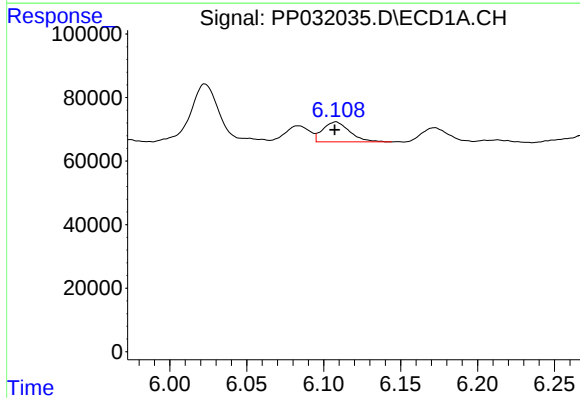


#17 AR-1242-2

R.T.: 6.108 min
Delta R.T.: 0.000 min
Response: 76344
Conc: 43.34 ng/ml

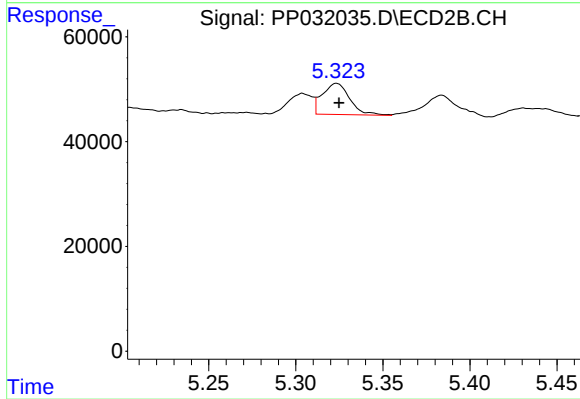

#17 AR-1242-2

R.T.: 5.323 min
Delta R.T.: -0.001 min
Response: 65105
Conc: 42.12 ng/ml

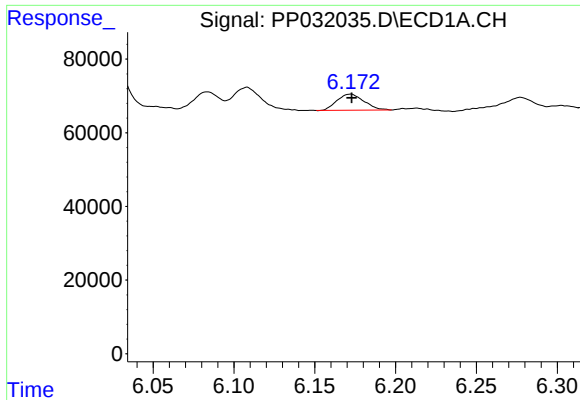


#18 AR-1242-3

R.T.: 6.172 min
Delta R.T.: 0.000 min
Response: 51228
Conc: 46.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
32834


Manual Integrations
APPROVED

Ankita
12/14/2020 3:22:59 PM

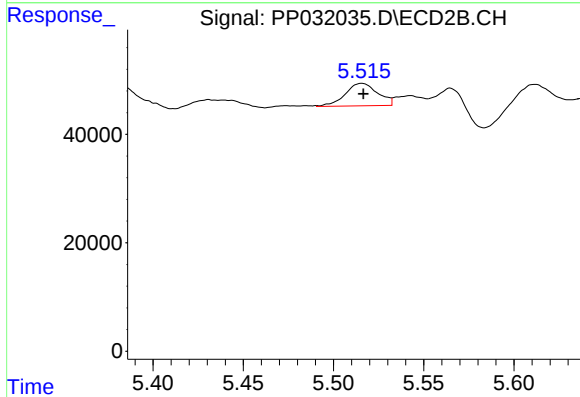


#18 AR-1242-3

R.T.: 5.515 min
Delta R.T.: -0.001 min
Response: 52204
Conc: 62.00 ng/ml m

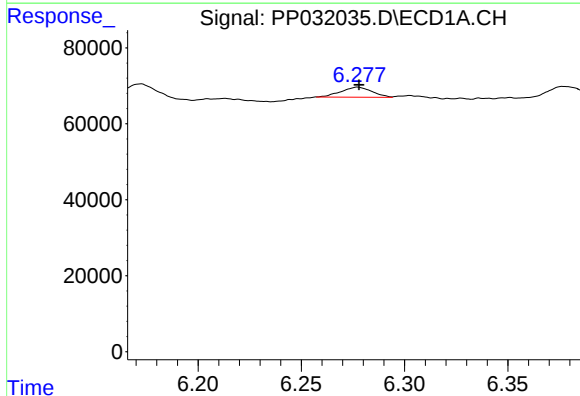


#19 AR-1242-4

R.T.: 6.277 min
Delta R.T.: -0.001 min
Response: 27765
Conc: 30.51 ng/ml m

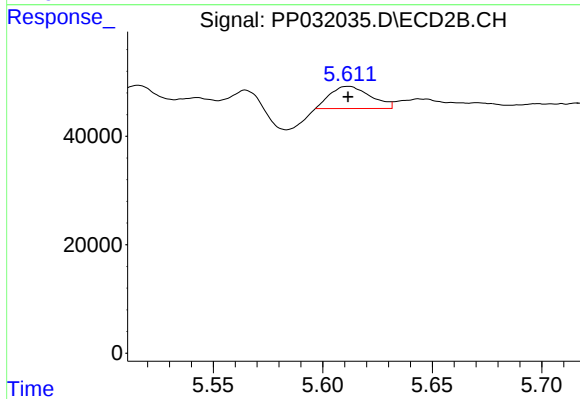

#19 AR-1242-4

R.T.: 5.611 min
Delta R.T.: 0.000 min
Response: 52448
Conc: 64.66 ng/ml m

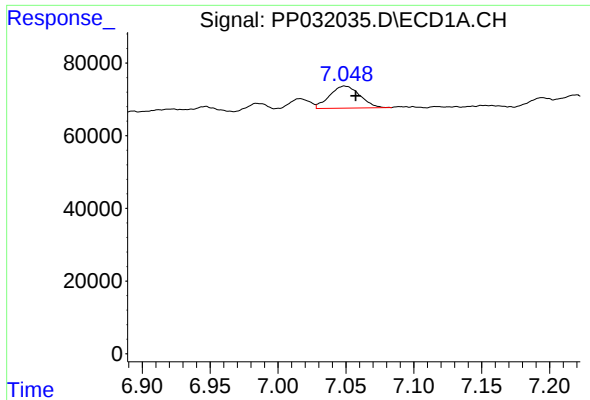


#20 AR-1242-5

R.T.: 7.049 min
Delta R.T.: -0.008 min
Response: 94159
Conc: 108.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
32834

Manual Integrations
APPROVED

Ankita
12/14/2020 3:22:59 PM

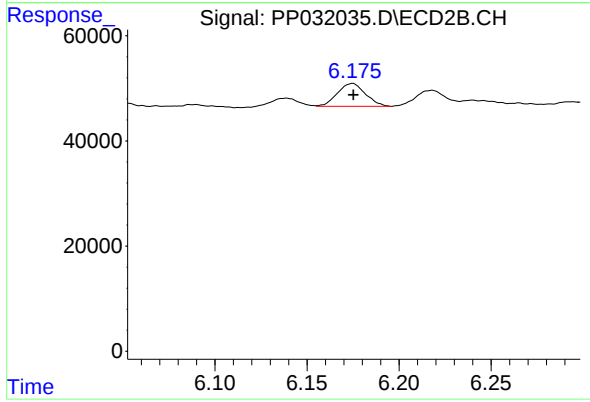

#20 AR-1242-5

R.T.: 6.175 min
Delta R.T.: 0.000 min
Response: 46328
Conc: 52.09 ng/ml