

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121220\
 Data File : PP032070.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Dec 2020 20:44
 Operator : DD\AJ
 Sample : L5038-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JBD-GW-SB-02

Manual Integrations
 APPROVED

Ankita
 12/14/2020 3:23:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 05:04:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.781	4.055	958466	858400	18.606	18.149
2) SA Decachlor...	10.644	9.345	434117	450548	13.843	13.435m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121220\
Data File : PP032070.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Dec 2020 20:44
Operator : DD\AJ
Sample : L5038-01
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
JBD-GW-SB-02


Manual Integrations
APPROVED

Ankita
12/14/2020 3:23:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 05:04:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

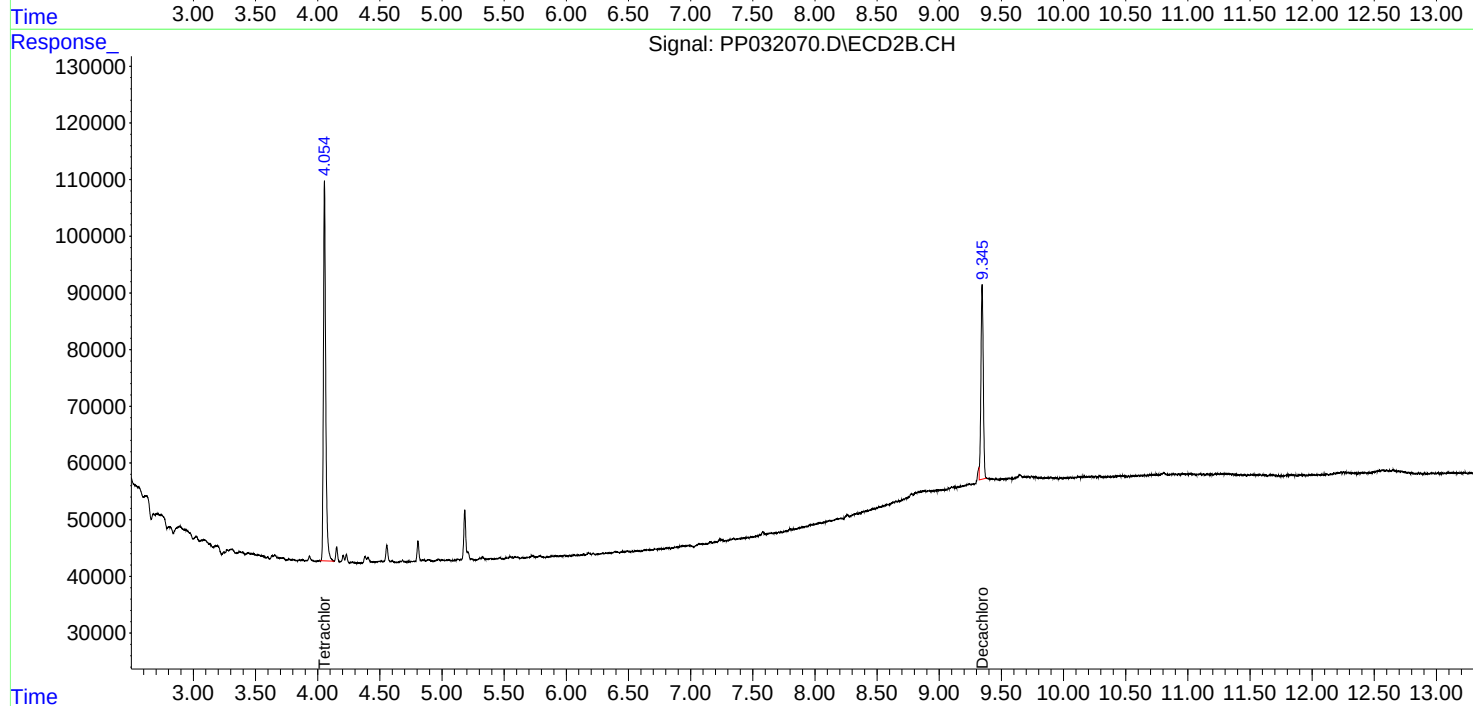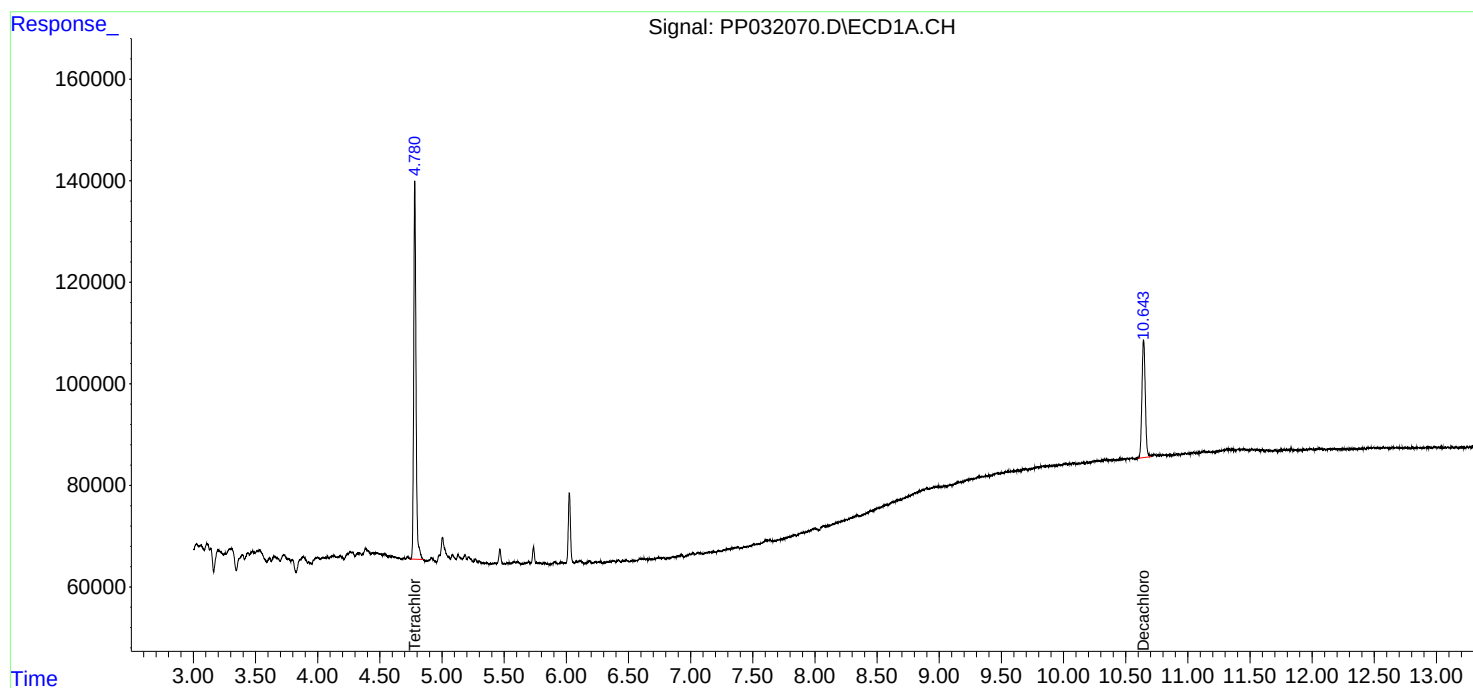

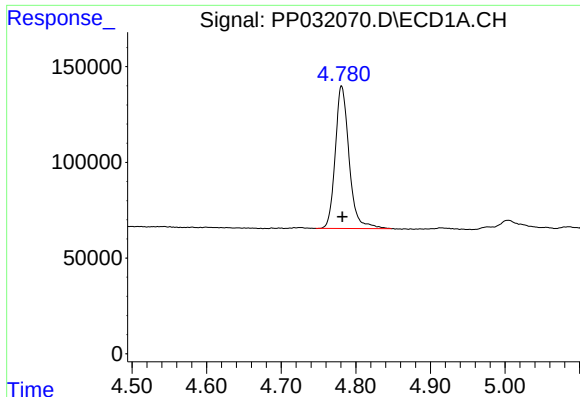


#1 Tetrachloro-m-xylene

R.T.: 4.781 min
Delta R.T.: 0.000 min
Response: 958466
Conc: 18.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
JBD-GW-SB-02


Manual Integrations
APPROVED

Ankita
12/14/2020 3:23:07 PM

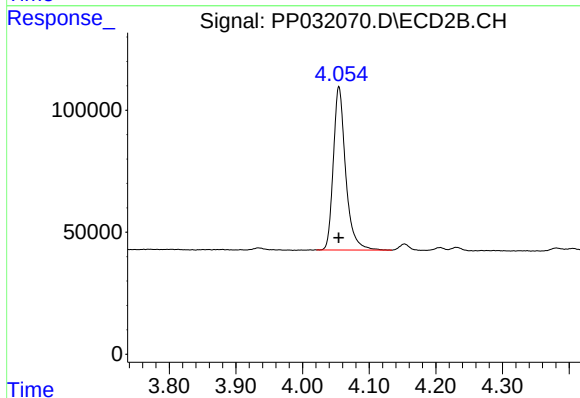


#1 Tetrachloro-m-xylene

R.T.: 4.055 min
Delta R.T.: 0.000 min
Response: 858400
Conc: 18.15 ng/ml

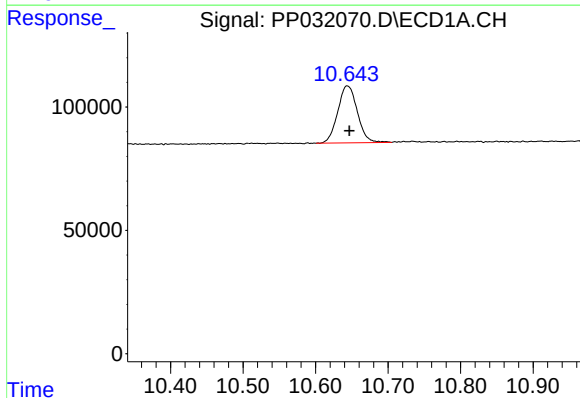

#2 Decachlorobiphenyl

R.T.: 10.644 min
Delta R.T.: -0.003 min
Response: 434117
Conc: 13.84 ng/ml

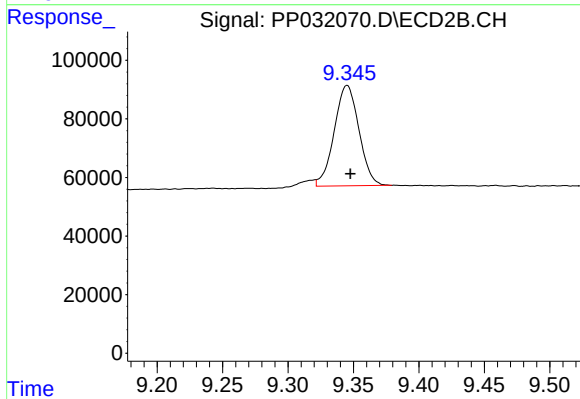

#2 Decachlorobiphenyl

R.T.: 9.345 min
Delta R.T.: -0.003 min
Response: 450548
Conc: 13.43 ng/ml m