

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121223\
 Data File : PP062409.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2023 15:12
 Operator : YP\AJ
 Sample : 05764-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-120623-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 23:28:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 12 05:13:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.432	3.718	32919198	51343805	19.624	16.731
2) SA Decachlor...	10.194	8.832	38492768	31445988	36.835	13.654 #
Target Compounds						
3) L1 AR-1016-1	5.608	4.832	4286292	-2490028	86.595	N.D. #
4) L1 AR-1016-2	5.630	4.859	3705181	777629	48.172	5.897 #
5) L1 AR-1016-3	5.693	0.000	2636701	0	53.450	N.D. #
6) L1 AR-1016-4	5.793	5.070	6097515	118.3E6	155.148	1875.111 #
7) L1 AR-1016-5	6.085	0.000	4815077	0	116.117	N.D. #
8) L2 AR-1221-1	0.000	3.914f	0	918971	N.D.	24.829 #
9) L2 AR-1221-2	4.727	4.029	196796	11266766	17.222	395.701 #
10) L2 AR-1221-3	4.803	0.000	516132	0	11.772	N.D. #
11) L3 AR-1232-1	4.803	0.000	516132	0	14.343	N.D. #
12) L3 AR-1232-2	5.336	4.859	721596	777629	34.612	13.431 #
13) L3 AR-1232-3	5.630	0.000	3705181	0	109.267	N.D. #
14) L3 AR-1232-4	5.793	0.000	6097515	0	336.703	N.D. #
15) L3 AR-1232-5	5.881	0.000	14214460	0	949.181	N.D. #
16) L4 AR-1242-1	5.608	4.832	4286292	-2490028	104.017	N.D. #
17) L4 AR-1242-2	5.630	4.859	3705181	777629	59.564	7.283 #
18) L4 AR-1242-3	5.693	0.000	2636701	0	65.046	N.D. #
19) L4 AR-1242-4	5.793	0.000	6097515	0	180.747	N.D. #
20) L4 AR-1242-5	6.529	5.646	20391247	27255501	573.229	390.888 #
21) L5 AR-1248-1	5.608	4.832	4286292	-2490028	138.513	N.D. #
22) L5 AR-1248-2	5.881	5.070	14214460	118.3E6	269.979	1329.485 #
23) L5 AR-1248-3	6.085	0.000	4815077	0	84.679	N.D. #
24) L5 AR-1248-4	6.490	0.000	11653693	0	199.307	N.D. #
25) L5 AR-1248-5	6.529	5.646	20391247	27255501	339.638	196.507 #
26) L6 AR-1254-1	6.464	5.646	23325649	27255501	344.028	170.902 #
27) L6 AR-1254-2	6.684	5.796	13981530	24880021	132.640	175.847 #
28) L6 AR-1254-3	0.000	6.205	0	23882763	N.D.	107.749 #
29) L6 AR-1254-4	7.319f	6.415f	31566413	92904540	491.643	842.717 #
30) L6 AR-1254-5	7.788f	6.861	71539221	6055940	975.836	32.635 #
31) L7 AR-1260-1	7.216	0.000	13081011	0	165.538	N.D. #
32) L7 AR-1260-2	7.472	6.526	8689208	7250840	101.571	39.800 #
33) L7 AR-1260-3	0.000	6.684	0	16130778	N.D.	89.626 #
34) L7 AR-1260-4	0.000	7.167	0	336610	N.D.	2.304 #
35) L7 AR-1260-5	0.000	7.407	0	911493	N.D.	3.151 #
36) L8 AR-1262-1	7.874f	6.955	40769532	990031	1012.963	11.261 #
37) L8 AR-1262-2	0.000	7.167	0	336610	N.D.	1.862 #
38) L8 AR-1262-3	8.696	7.685	143.2E6	177224	1633.743	1.415 #
39) L8 AR-1262-4	0.000	7.745	0	42179787	N.D.	179.078 #
40) L8 AR-1262-5	9.430f	0.000	16933935	0	415.972	N.D. #
41) L9 AR-1268-1	8.696	7.685	143.2E6	177224	865.901	0.451 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121223\
 Data File : PP062409.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2023 15:12
 Operator : YP\AJ
 Sample : 05764-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-120623-03

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 23:28:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 12 05:13:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.745	0	42179787	N.D.	118.543 #
43) L9	AR-1268-3	0.000	7.974	0	1050542	N.D.	3.150 #
44) L9	AR-1268-4	9.430f	0.000	16933935	0	368.016	N.D. #
45) L9	AR-1268-5	0.000	8.567	0	210575	N.D.	0.245 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121223\
Data File : PP062409.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2023 15:12
Operator : YP\AJ
Sample : 05764-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 23:28:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 12 05:13:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

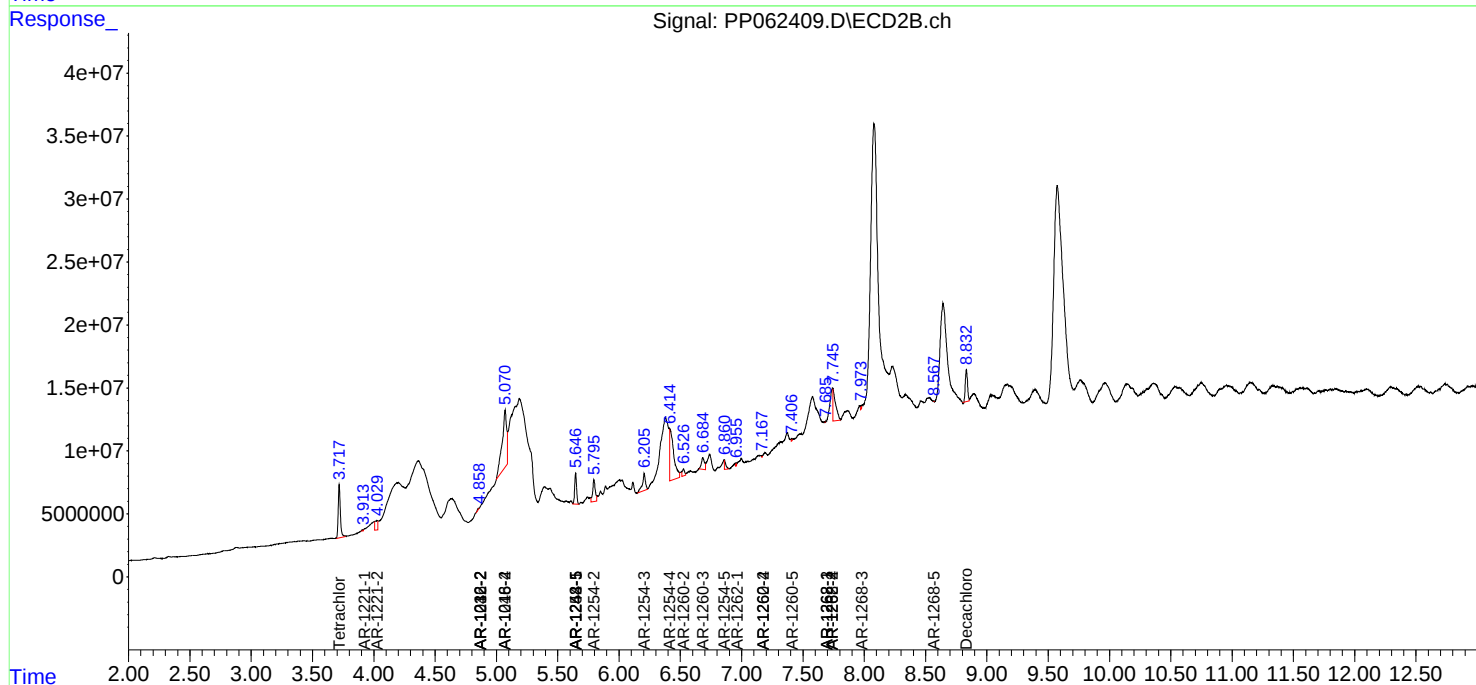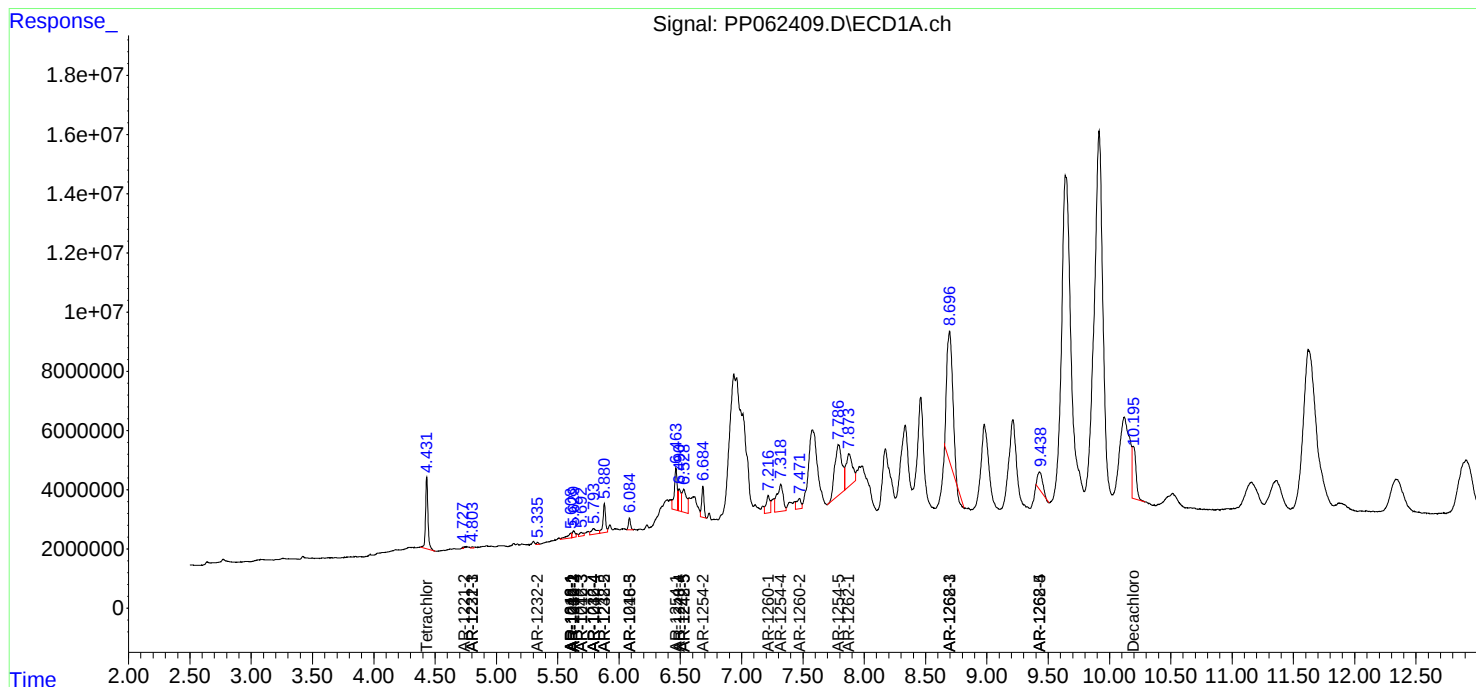


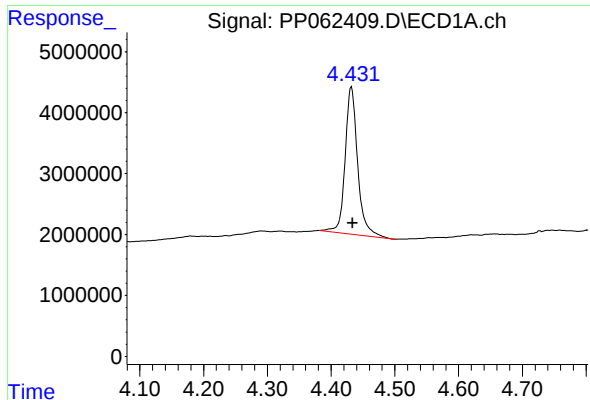

#1 Tetrachloro-m-xylene


R.T.: 4.432 min
Delta R.T.: -0.002 min
Response: 32919198
Conc: 19.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

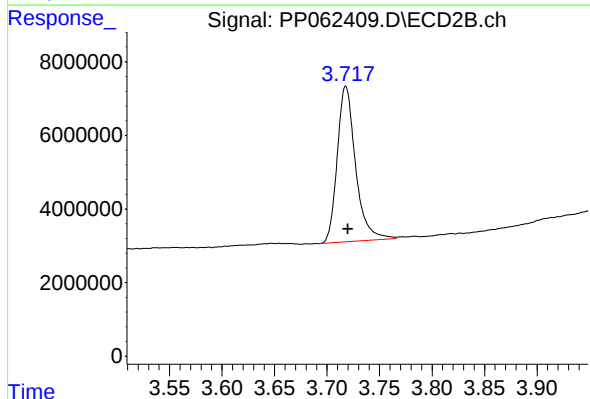


#1 Tetrachloro-m-xylene

R.T.: 3.718 min
Delta R.T.: -0.002 min
Response: 51343805
Conc: 16.73 ng/ml

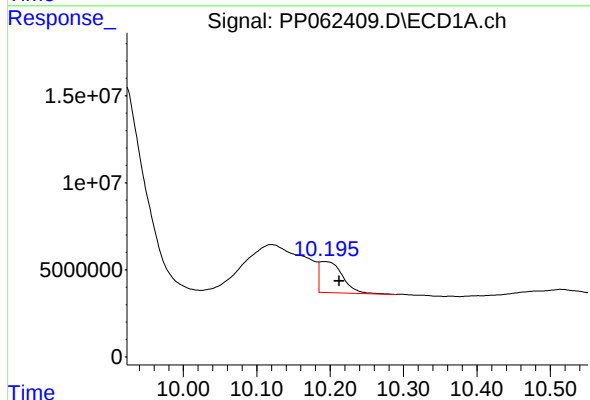


#2 Decachlorobiphenyl

R.T.: 10.194 min
Delta R.T.: -0.018 min
Response: 38492768
Conc: 36.84 ng/ml

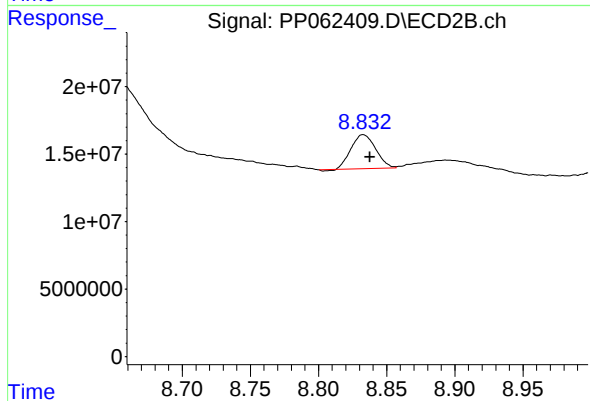

#2 Decachlorobiphenyl


R.T.: 8.832 min
Delta R.T.: -0.005 min
Response: 31445988
Conc: 13.65 ng/ml

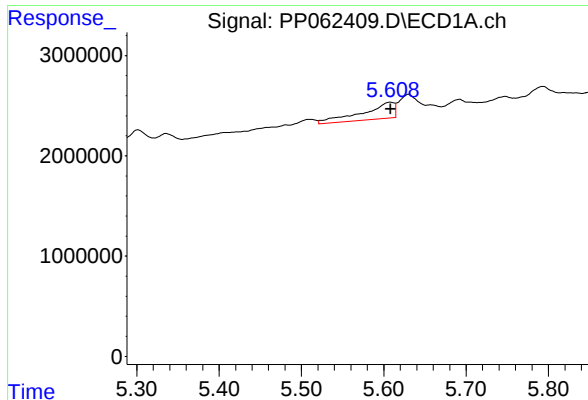

#3 AR-1016-1


R.T.: 5.608 min
Delta R.T.: 0.000 min
Response: 4286292
Conc: 86.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

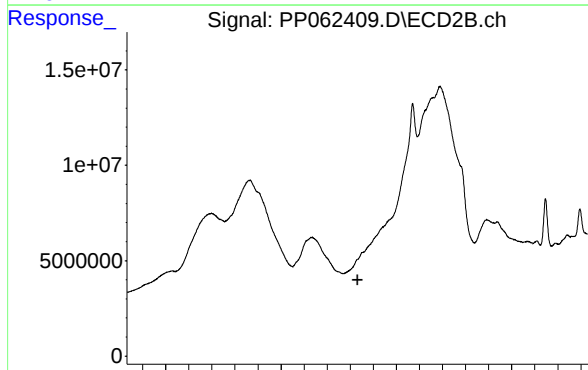


#3 AR-1016-1

R.T.: 4.832 min
Delta R.T.: 0.000 min
Response: -2490028
Conc: N.D.

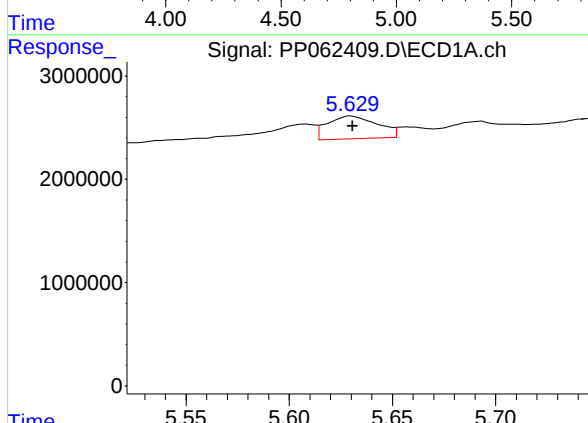


#4 AR-1016-2

R.T.: 5.630 min
Delta R.T.: 0.000 min
Response: 3705181
Conc: 48.17 ng/ml

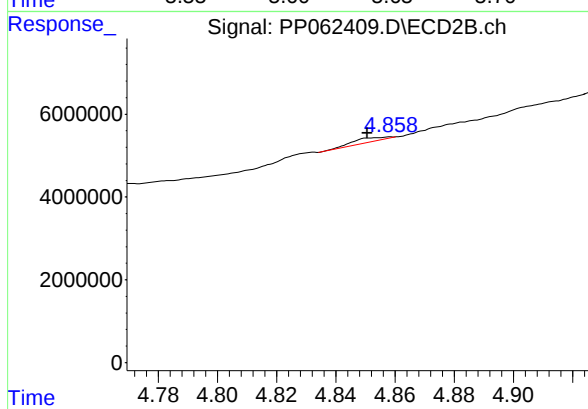

#4 AR-1016-2


R.T.: 4.859 min
Delta R.T.: 0.008 min
Response: 777629
Conc: 5.90 ng/ml

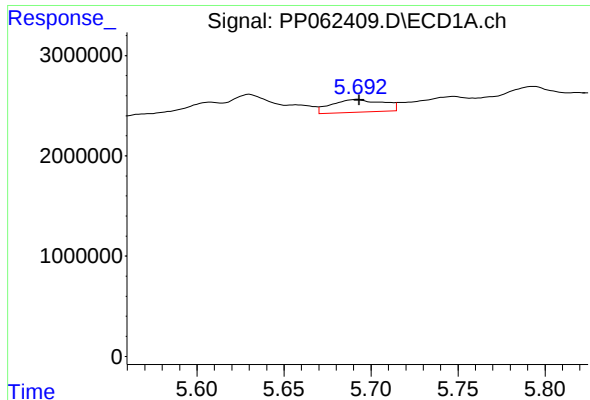

#5 AR-1016-3


R.T.: 5.693 min
Delta R.T.: 0.000 min
Response: 2636701
Conc: 53.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

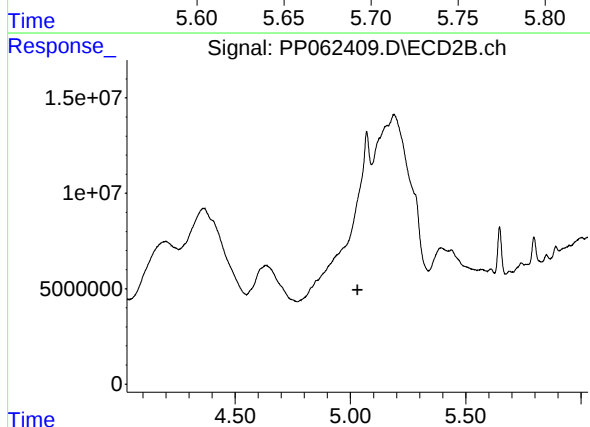


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T.: 5.031 min
Response: 0
Conc: N.D.

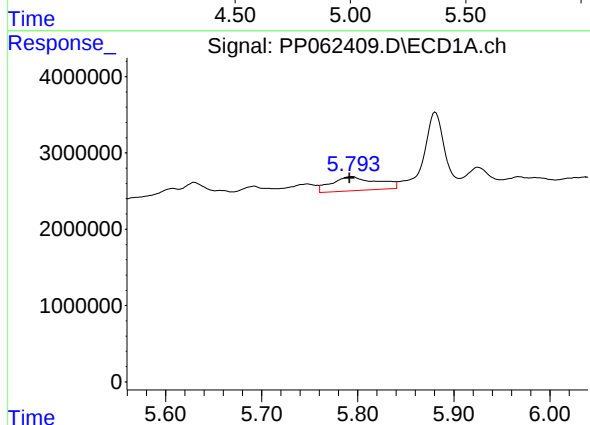


#6 AR-1016-4

R.T.: 5.793 min
Delta R.T.: 0.002 min
Response: 6097515
Conc: 155.15 ng/ml

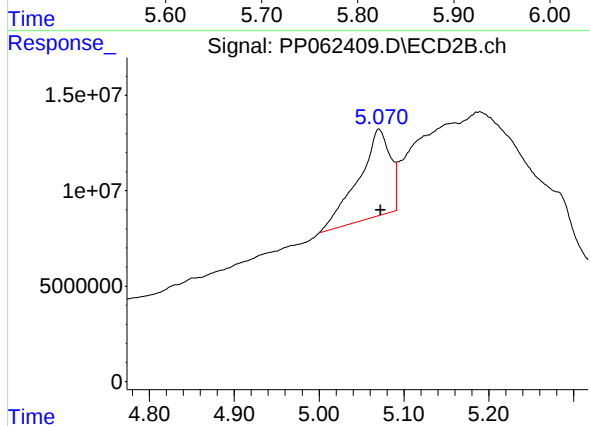

#6 AR-1016-4


R.T.: 5.070 min
Delta R.T.: -0.002 min
Response: 118276494
Conc: 1875.11 ng/ml

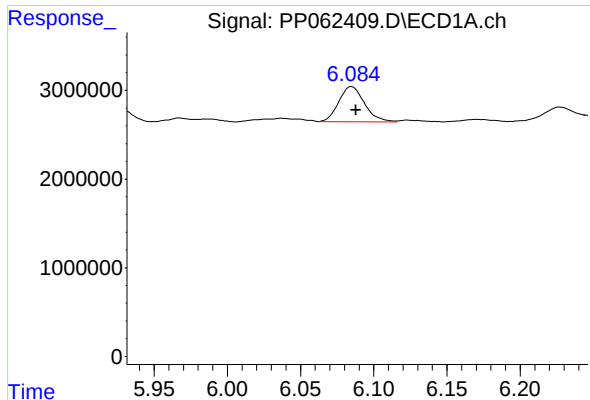

#7 AR-1016-5


R.T.: 6.085 min
Delta R.T.: -0.003 min
Response: 4815077
Conc: 116.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

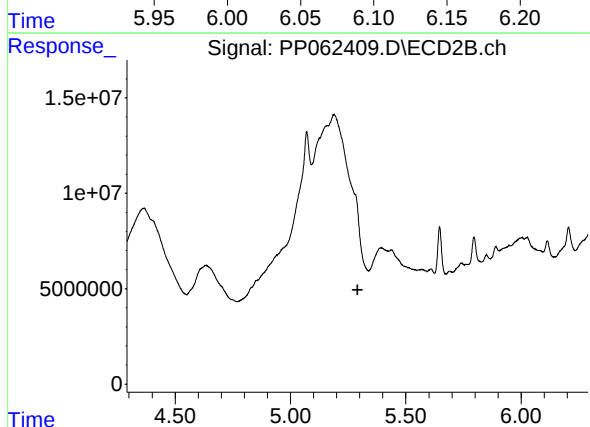


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T.: 5.291 min
Response: 0
Conc: N.D.

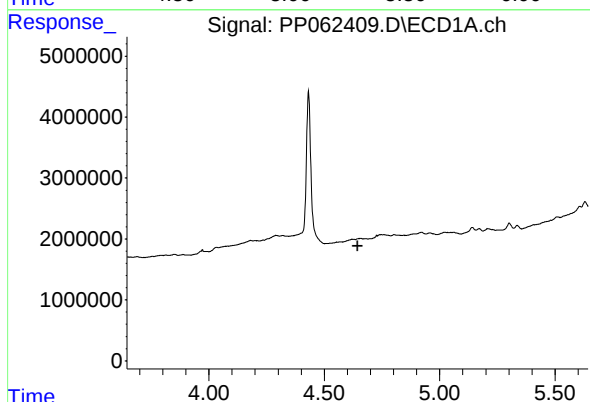


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T.: 4.644 min
Response: 0
Conc: N.D.

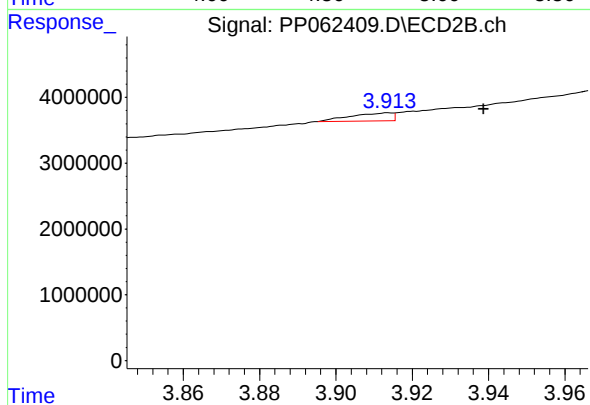

#8 AR-1221-1


R.T.: 3.914 min
Delta R.T.: -0.025 min
Response: 918971
Conc: 24.83 ng/ml

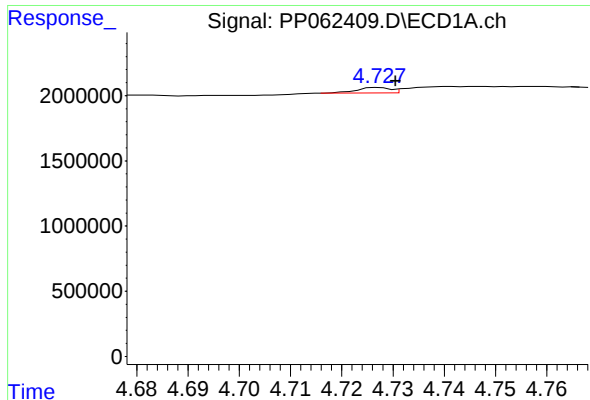

#9 AR-1221-2


R.T.: 4.727 min
Delta R.T.: -0.003 min
Response: 196796
Conc: 17.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

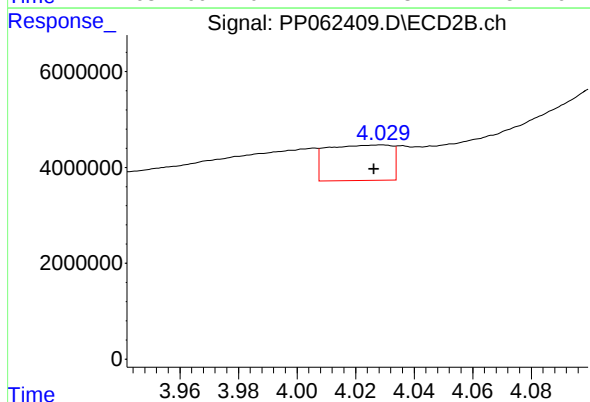


#9 AR-1221-2

R.T.: 4.029 min
Delta R.T.: 0.003 min
Response: 11266766
Conc: 395.70 ng/ml

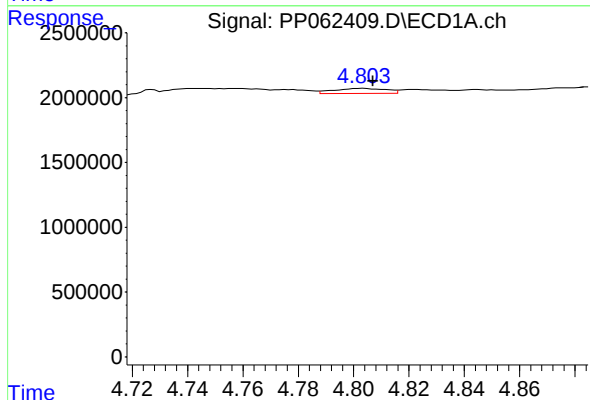


#10 AR-1221-3

R.T.: 4.803 min
Delta R.T.: -0.004 min
Response: 516132
Conc: 11.77 ng/ml

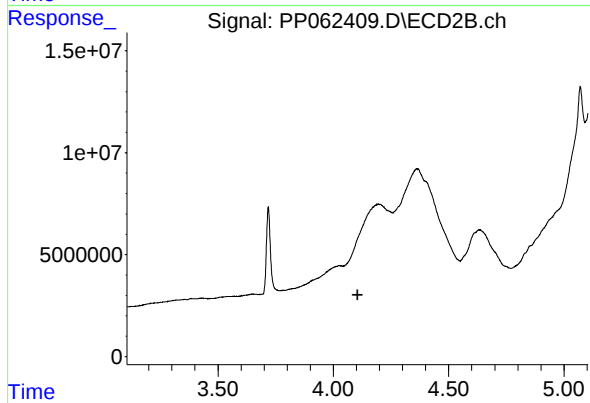

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 4.105 min
Response: 0
Conc: N.D.

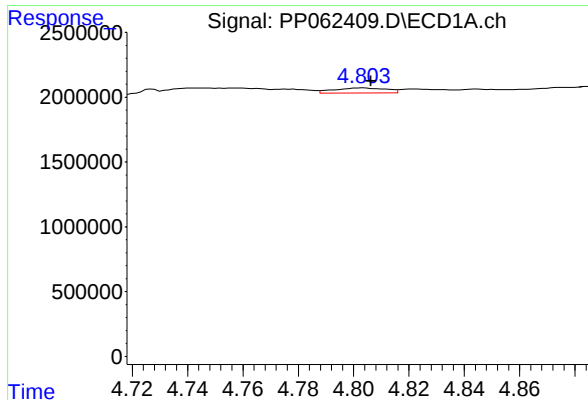

#11 AR-1232-1


R.T.: 4.803 min
Delta R.T.: -0.003 min
Response: 516132
Conc: 14.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

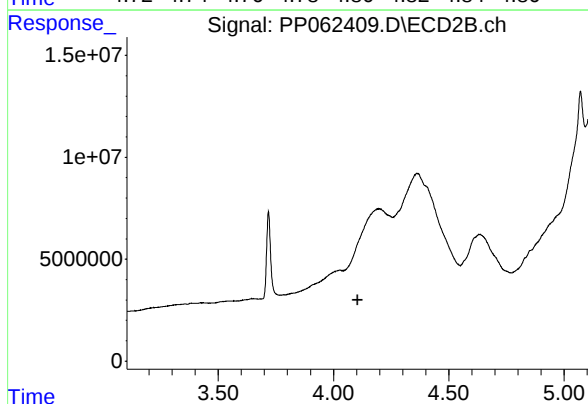


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.104 min
Response: 0
Conc: N.D.

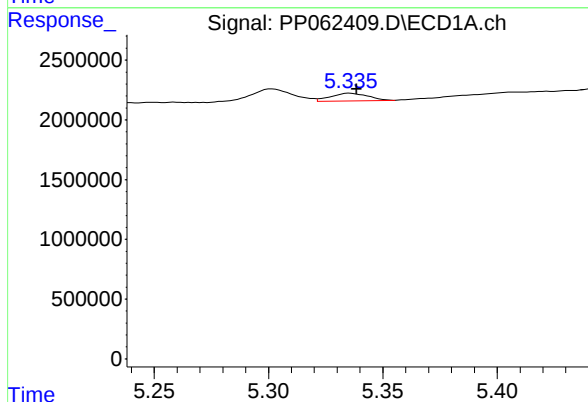


#12 AR-1232-2

R.T.: 5.336 min
Delta R.T.: -0.003 min
Response: 721596
Conc: 34.61 ng/ml

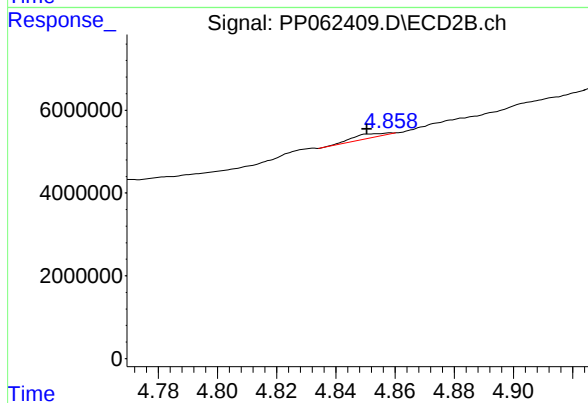

#12 AR-1232-2


R.T.: 4.859 min
Delta R.T.: 0.008 min
Response: 777629
Conc: 13.43 ng/ml

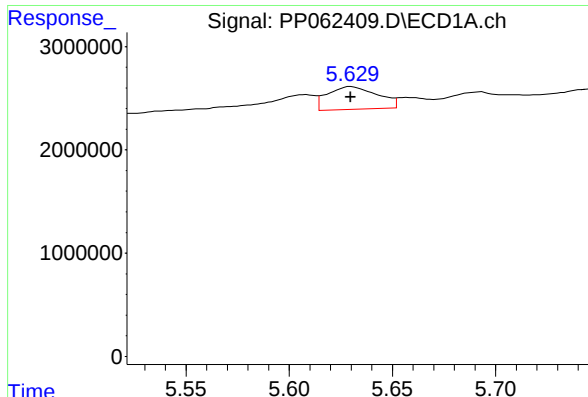

#13 AR-1232-3


R.T.: 5.630 min
Delta R.T.: 0.000 min
Response: 3705181
Conc: 109.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

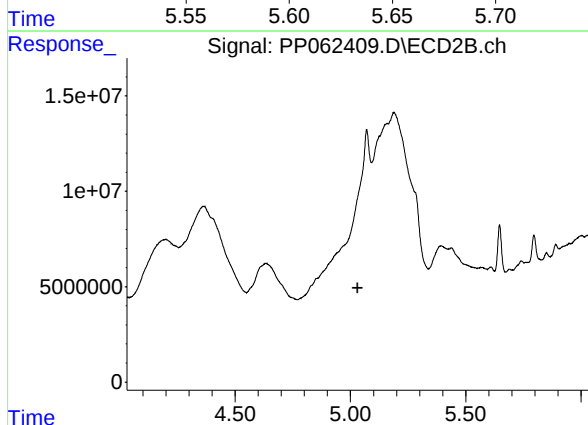


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 5.030 min
Response: 0
Conc: N.D.

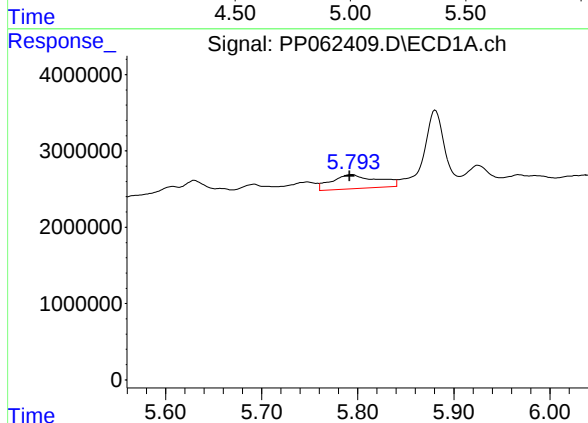


#14 AR-1232-4

R.T.: 5.793 min
Delta R.T.: 0.002 min
Response: 6097515
Conc: 336.70 ng/ml

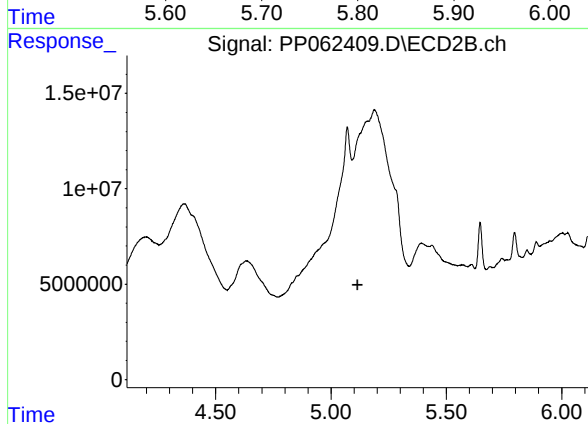

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.115 min
Response: 0
Conc: N.D.

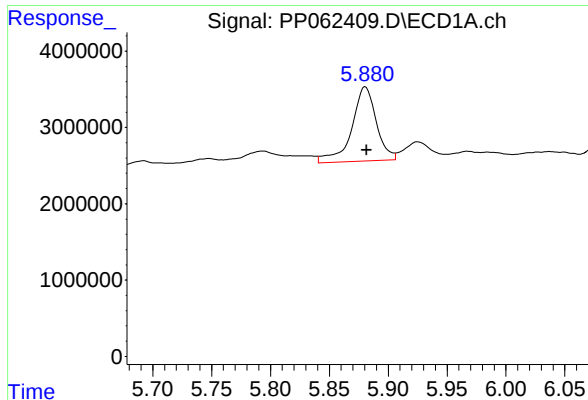

#15 AR-1232-5


R.T.: 5.881 min
Delta R.T.: -0.001 min
Response: 14214460
Conc: 949.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

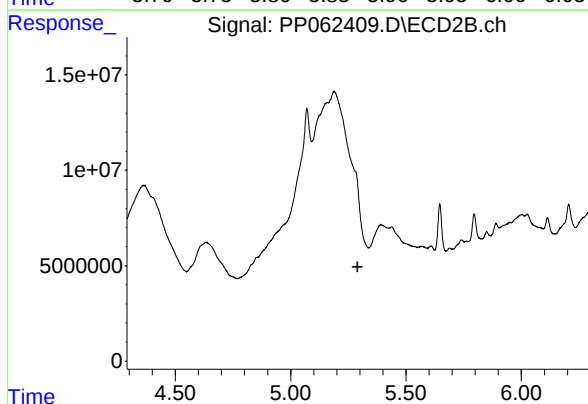


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

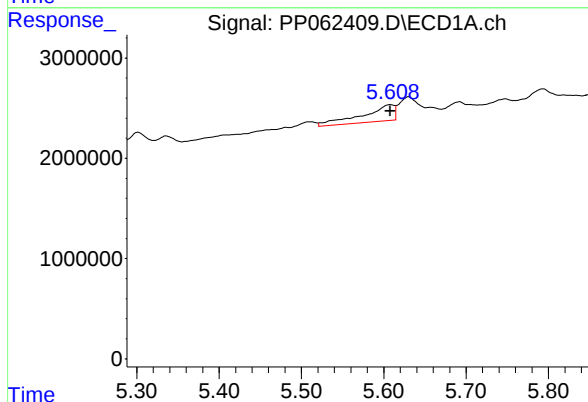


#16 AR-1242-1

R.T.: 5.608 min
Delta R.T.: 0.000 min
Response: 4286292
Conc: 104.02 ng/ml

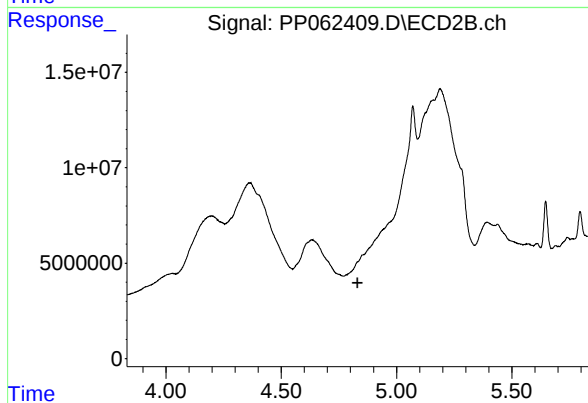

#16 AR-1242-1


R.T.: 4.832 min
Delta R.T.: 0.001 min
Response: -2490028
Conc: N.D.

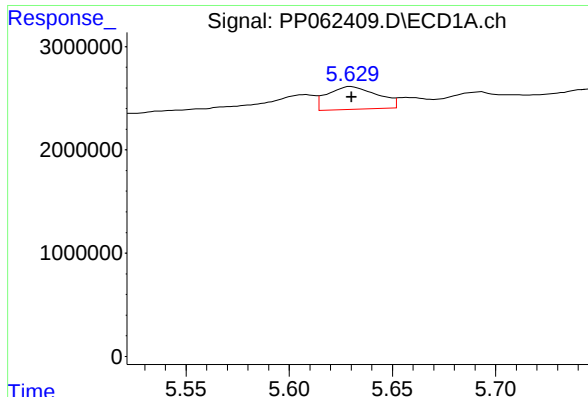

#17 AR-1242-2


R.T.: 5.630 min
Delta R.T.: 0.000 min
Response: 3705181
Conc: 59.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

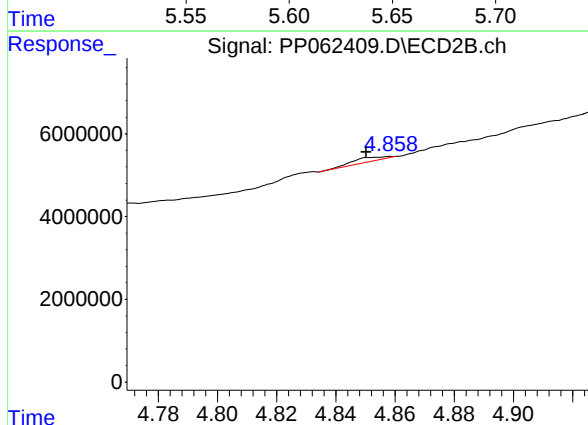


#17 AR-1242-2

R.T.: 4.859 min
Delta R.T.: 0.008 min
Response: 777629
Conc: 7.28 ng/ml

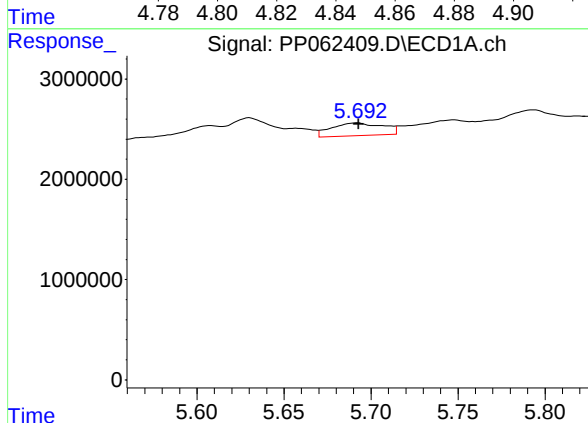


#18 AR-1242-3

R.T.: 5.693 min
Delta R.T.: 0.000 min
Response: 2636701
Conc: 65.05 ng/ml

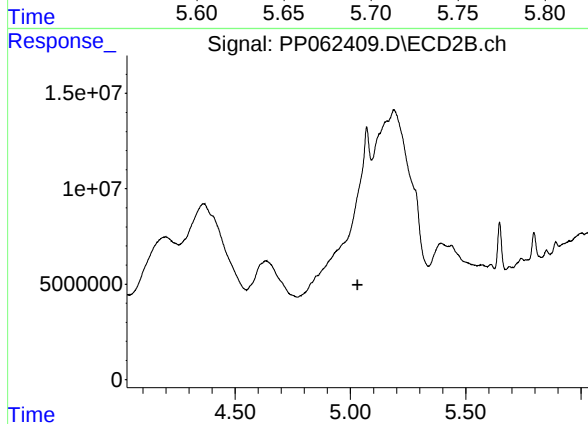

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 5.030 min
Response: 0
Conc: N.D.

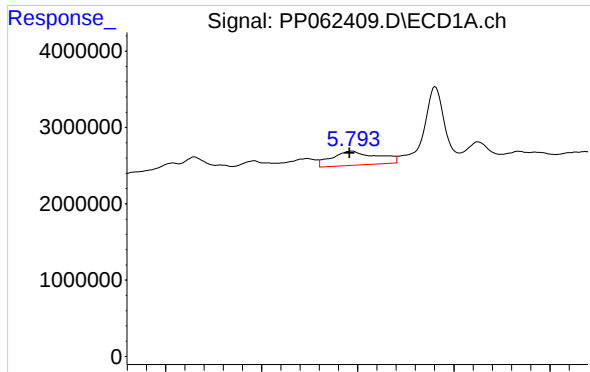

#19 AR-1242-4


R.T.: 5.793 min
Delta R.T.: 0.002 min
Response: 6097515
Conc: 180.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

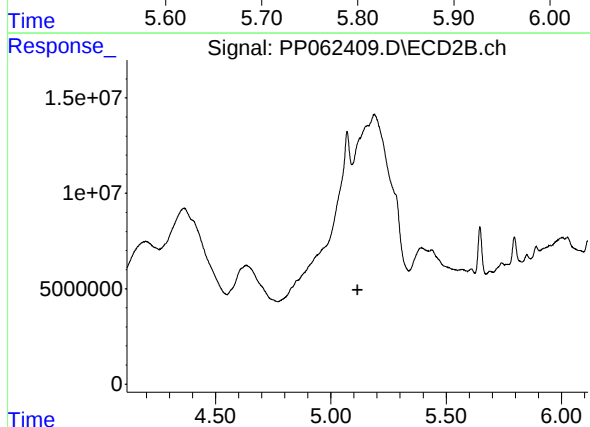


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T.: 5.116 min
Response: 0
Conc: N.D.

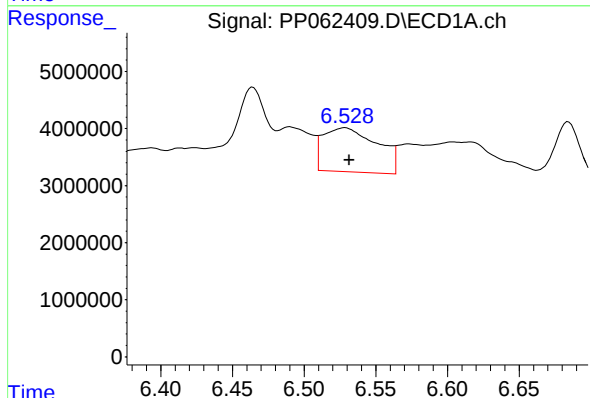


#20 AR-1242-5

R.T.: 6.529 min
Delta R.T.: -0.003 min
Response: 20391247
Conc: 573.23 ng/ml

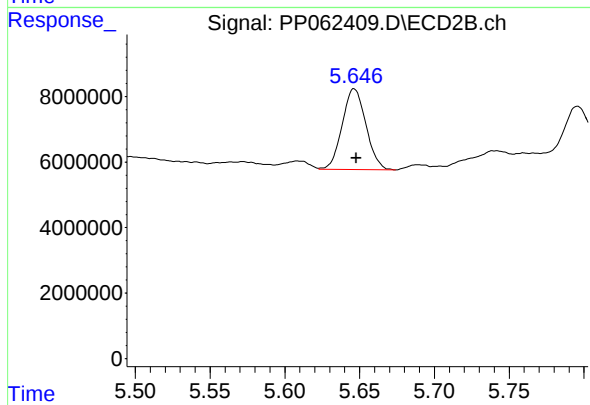

#20 AR-1242-5


R.T.: 5.646 min
Delta R.T.: -0.002 min
Response: 27255501
Conc: 390.89 ng/ml

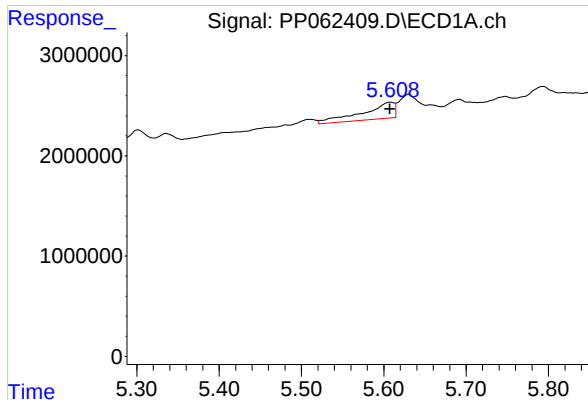

#21 AR-1248-1


R.T.: 5.608 min
Delta R.T.: 0.000 min
Response: 4286292
Conc: 138.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

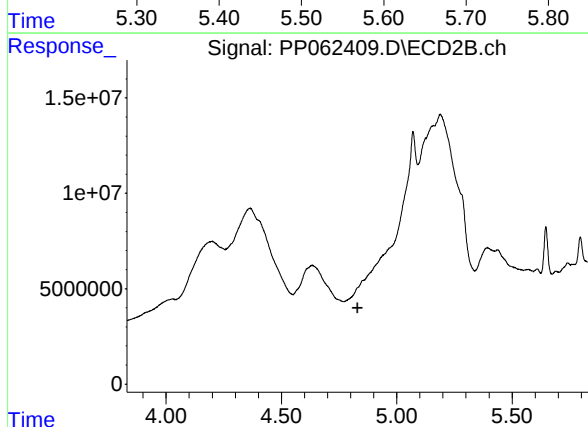


#21 AR-1248-1

R.T.: 4.832 min
Delta R.T.: 0.002 min
Response: -2490028
Conc: N.D.

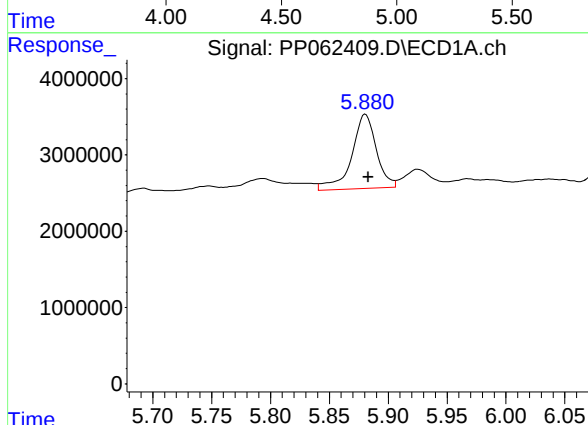


#22 AR-1248-2

R.T.: 5.881 min
Delta R.T.: -0.002 min
Response: 14214460
Conc: 269.98 ng/ml

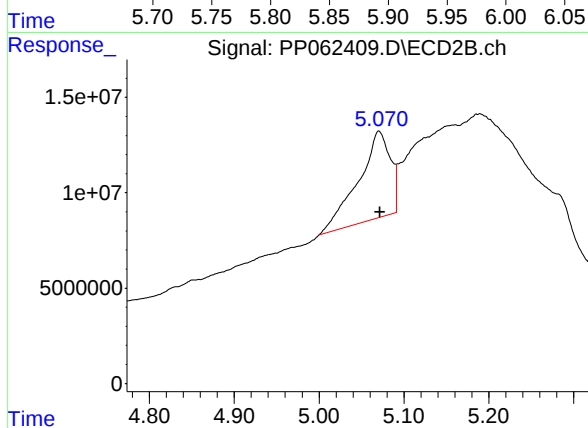

#22 AR-1248-2


R.T.: 5.070 min
Delta R.T.: 0.000 min
Response: 118276494
Conc: 1329.48 ng/ml

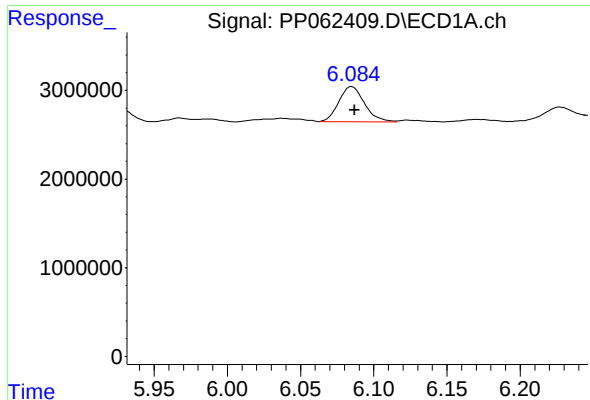

#23 AR-1248-3


R.T.: 6.085 min
Delta R.T.: -0.002 min
Response: 4815077
Conc: 84.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

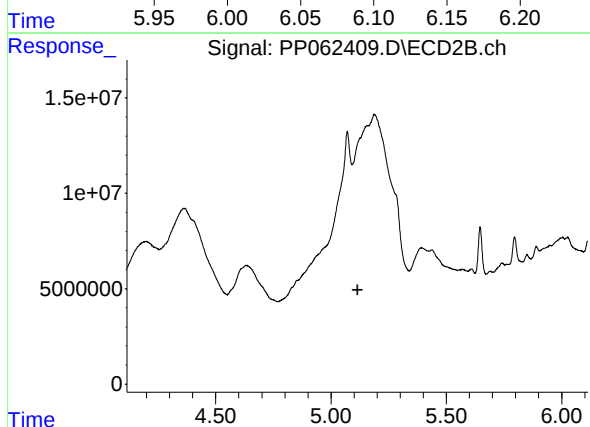


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T.: 5.115 min
Response: 0
Conc: N.D.

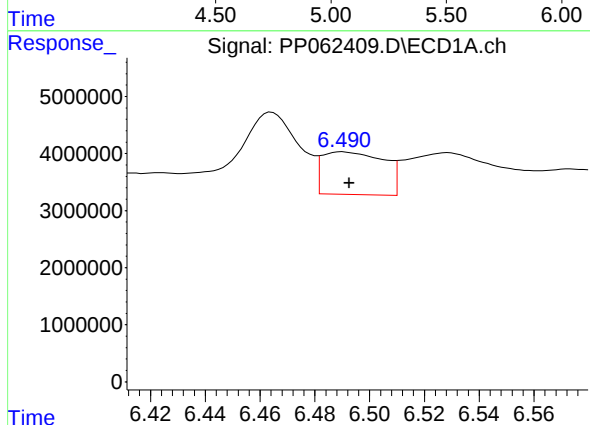


#24 AR-1248-4

R.T.: 6.490 min
Delta R.T.: -0.003 min
Response: 11653693
Conc: 199.31 ng/ml

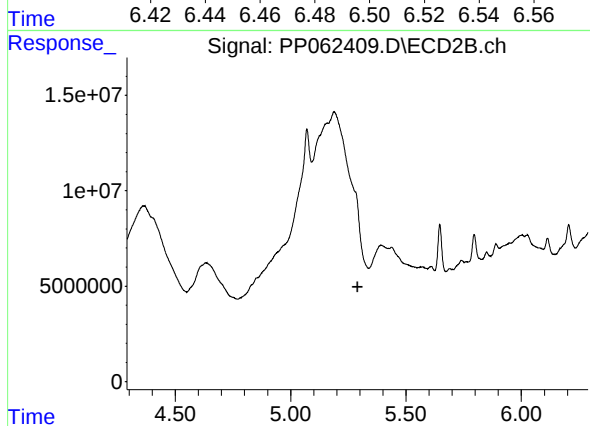

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

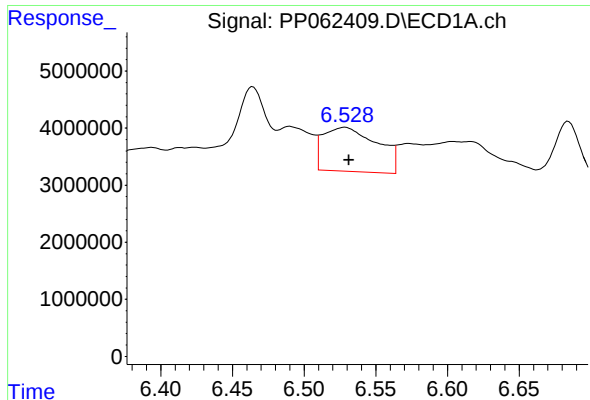

#25 AR-1248-5


R.T.: 6.529 min
Delta R.T.: -0.003 min
Response: 20391247
Conc: 339.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

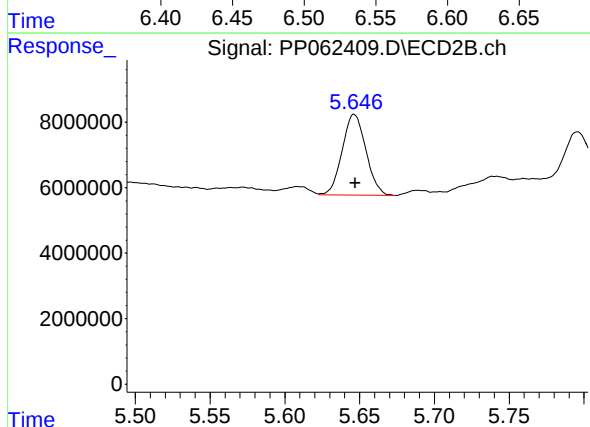


#25 AR-1248-5

R.T.: 5.646 min
Delta R.T.: 0.000 min
Response: 27255501
Conc: 196.51 ng/ml

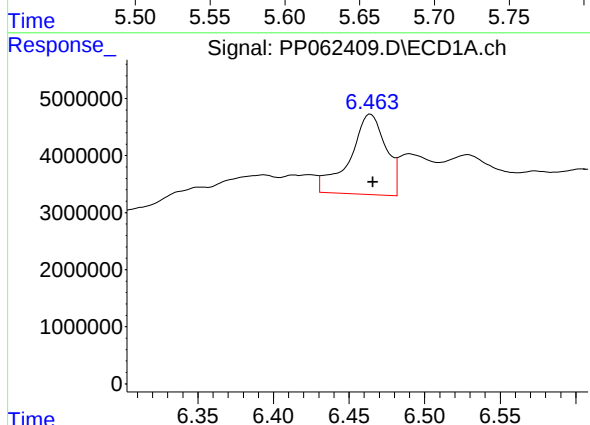


#26 AR-1254-1

R.T.: 6.464 min
Delta R.T.: -0.002 min
Response: 23325649
Conc: 344.03 ng/ml

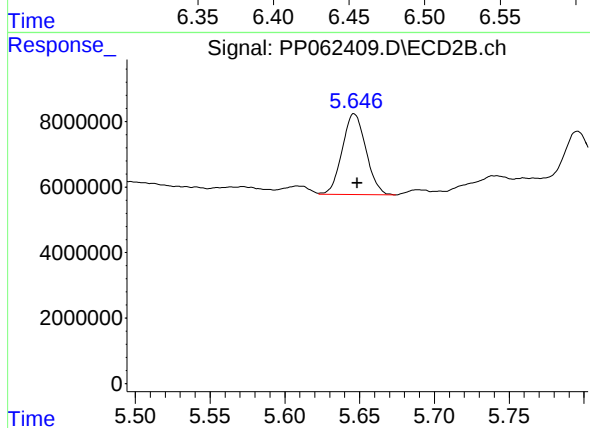

#26 AR-1254-1


R.T.: 5.646 min
Delta R.T.: -0.002 min
Response: 27255501
Conc: 170.90 ng/ml

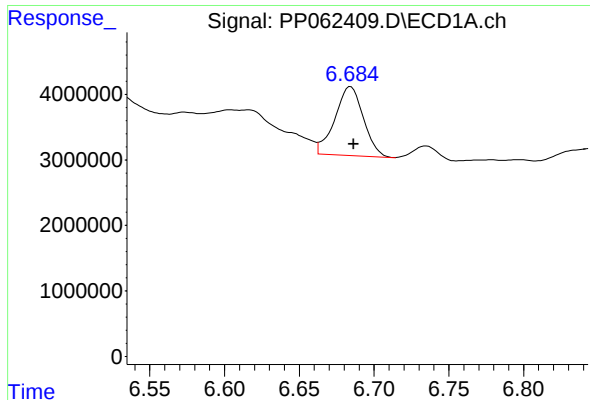

#27 AR-1254-2


R.T.: 6.684 min
Delta R.T.: -0.002 min
Response: 13981530
Conc: 132.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

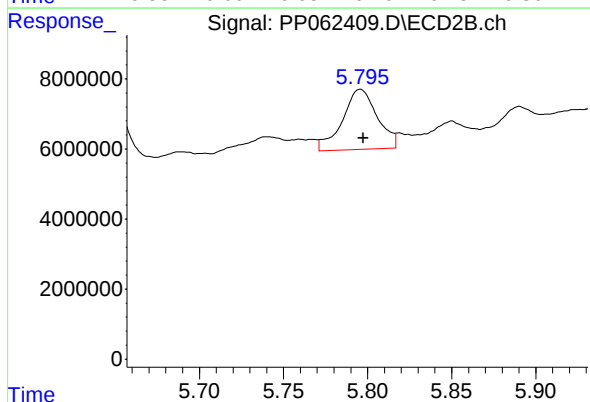


#27 AR-1254-2

R.T.: 5.796 min
Delta R.T.: -0.002 min
Response: 24880021
Conc: 175.85 ng/ml

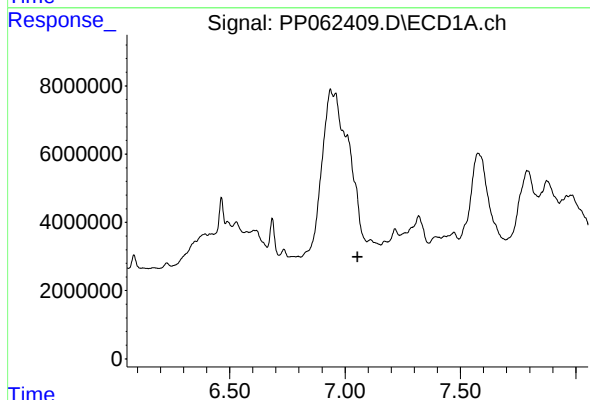


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 7.054 min
Response: 0
Conc: N.D.

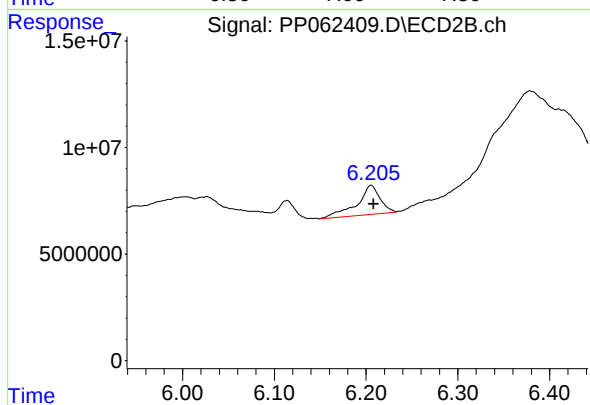

#28 AR-1254-3


R.T.: 6.205 min
Delta R.T.: -0.003 min
Response: 23882763
Conc: 107.75 ng/ml

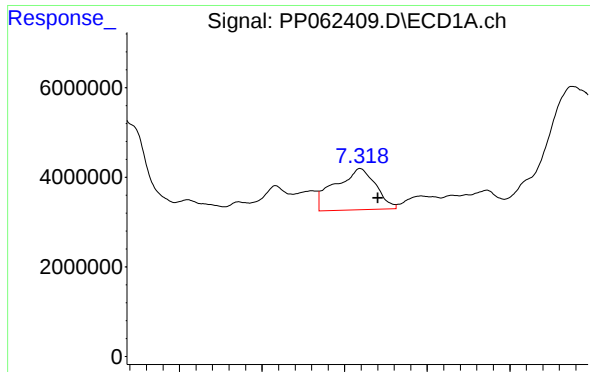

#29 AR-1254-4


R.T.: 7.319 min
Delta R.T.: -0.021 min
Response: 31566413
Conc: 491.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

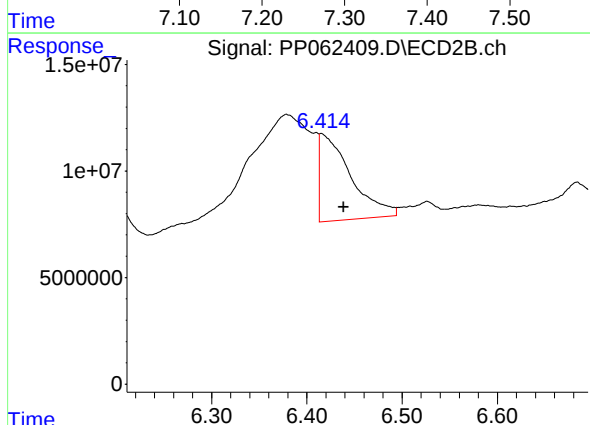


#29 AR-1254-4

R.T.: 6.415 min
Delta R.T.: -0.023 min
Response: 92904540
Conc: 842.72 ng/ml

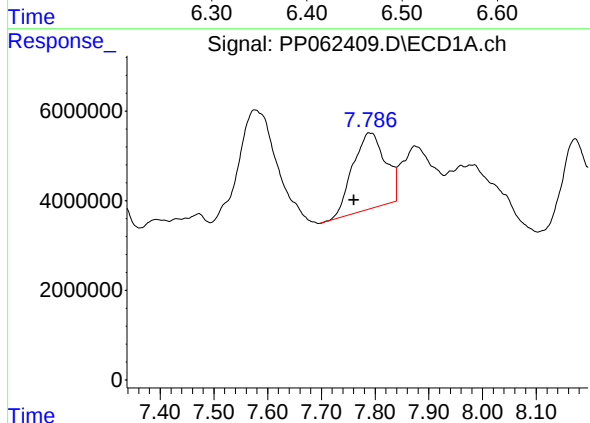


#30 AR-1254-5

R.T.: 7.788 min
Delta R.T.: 0.028 min
Response: 71539221
Conc: 975.84 ng/ml

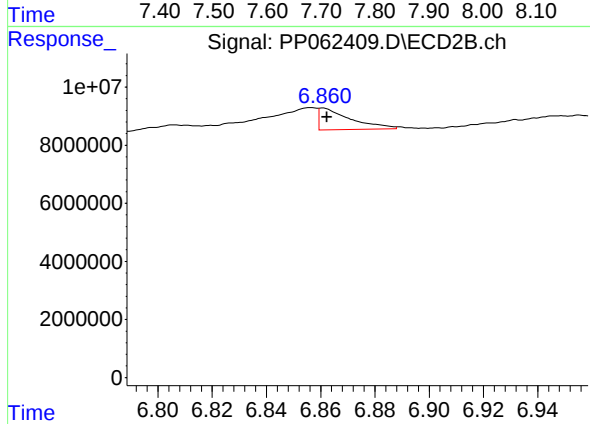

#30 AR-1254-5


R.T.: 6.861 min
Delta R.T.: -0.001 min
Response: 6055940
Conc: 32.64 ng/ml

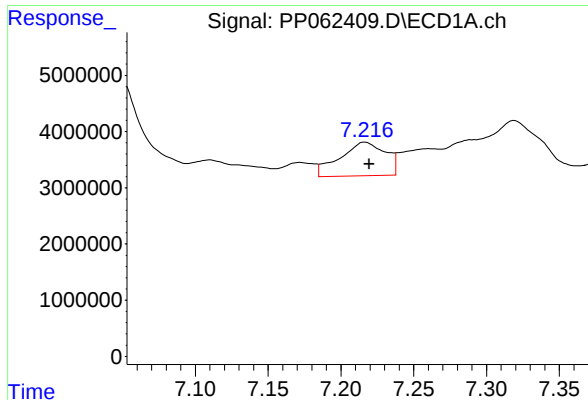

#31 AR-1260-1


R.T.: 7.216 min
Delta R.T.: -0.003 min
Response: 13081011
Conc: 165.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

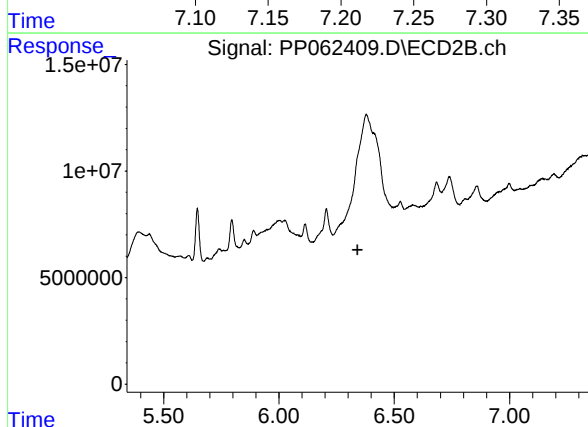


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T.: 6.341 min
Response: 0
Conc: N.D.

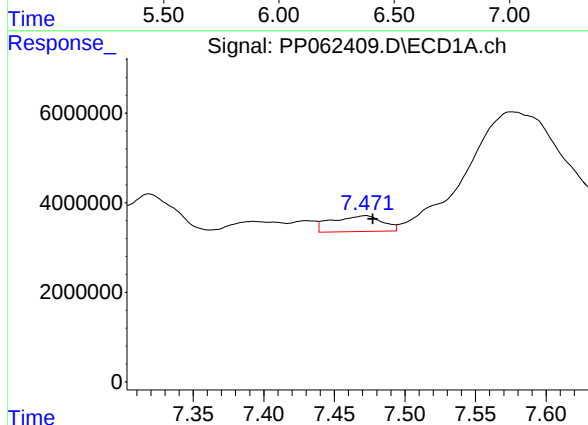


#32 AR-1260-2

R.T.: 7.472 min
Delta R.T.: -0.005 min
Response: 8689208
Conc: 101.57 ng/ml

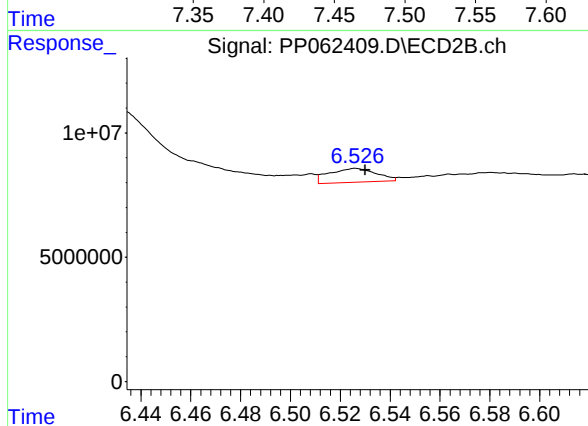

#32 AR-1260-2


R.T.: 6.526 min
Delta R.T.: -0.004 min
Response: 7250840
Conc: 39.80 ng/ml

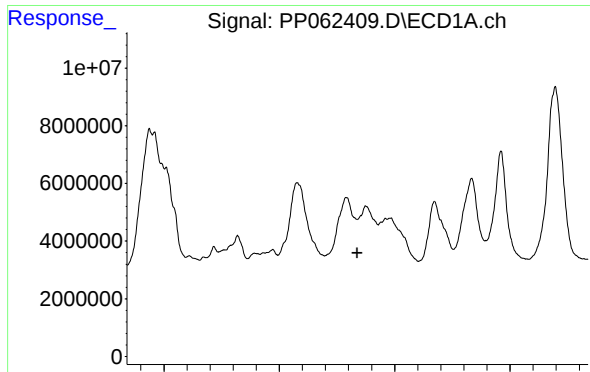

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.838 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

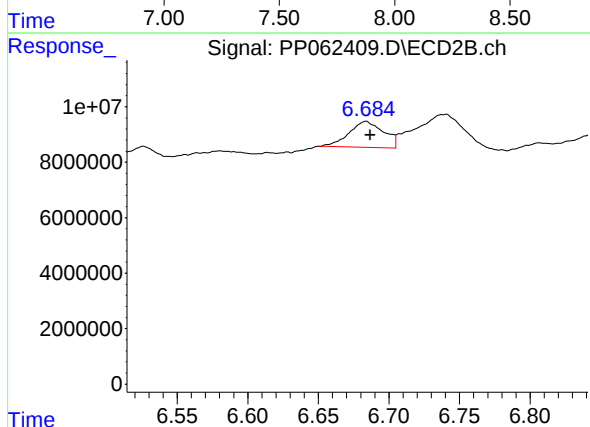


#33 AR-1260-3

R.T.: 6.684 min
Delta R.T.: -0.003 min
Response: 16130778
Conc: 89.63 ng/ml

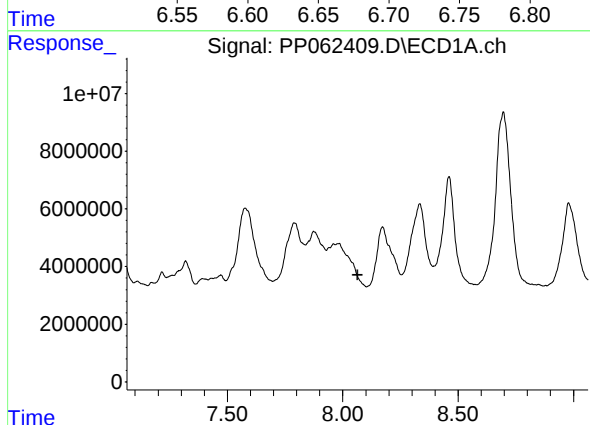


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 8.064 min
Response: 0
Conc: N.D.

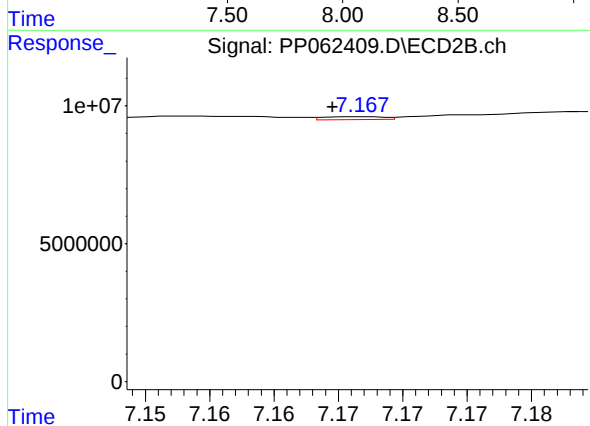

#34 AR-1260-4


R.T.: 7.167 min
Delta R.T.: 0.002 min
Response: 336610
Conc: 2.30 ng/ml

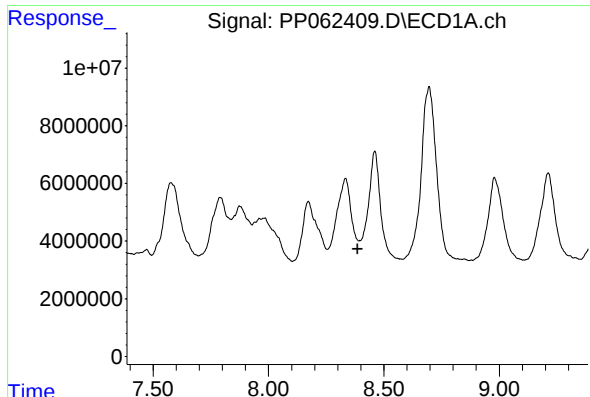

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.386 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

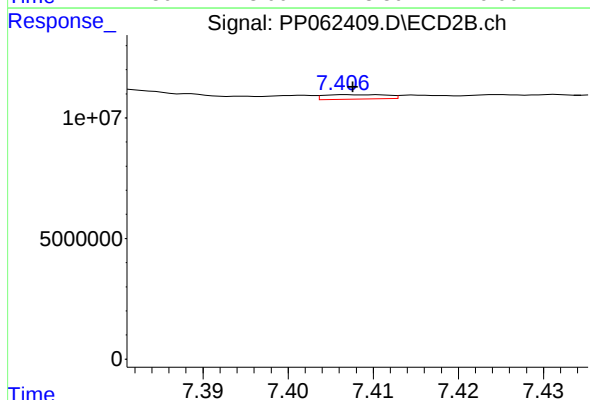


#35 AR-1260-5

R.T.: 7.407 min
Delta R.T.: 0.000 min
Response: 911493
Conc: 3.15 ng/ml

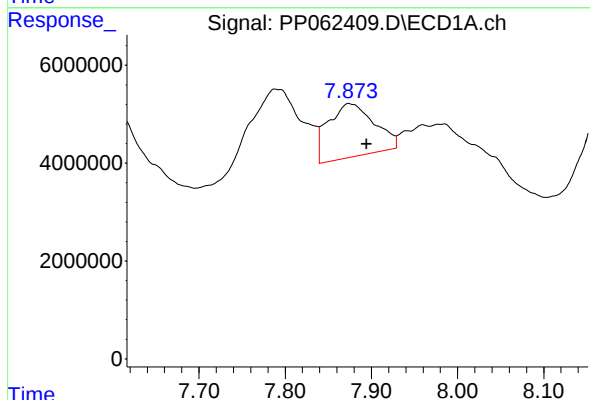


#36 AR-1262-1

R.T.: 7.874 min
Delta R.T.: -0.021 min
Response: 40769532
Conc: 1012.96 ng/ml

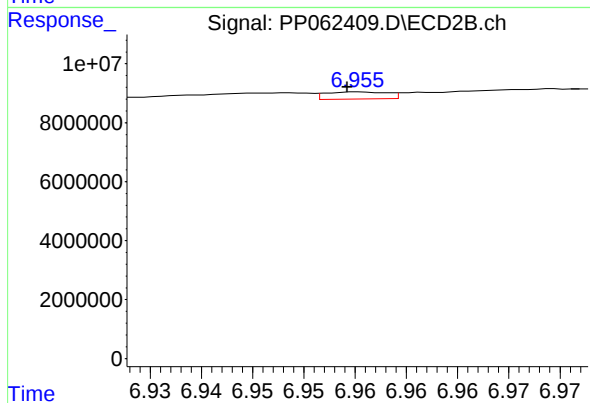

#36 AR-1262-1


R.T.: 6.955 min
Delta R.T.: 0.001 min
Response: 990031
Conc: 11.26 ng/ml

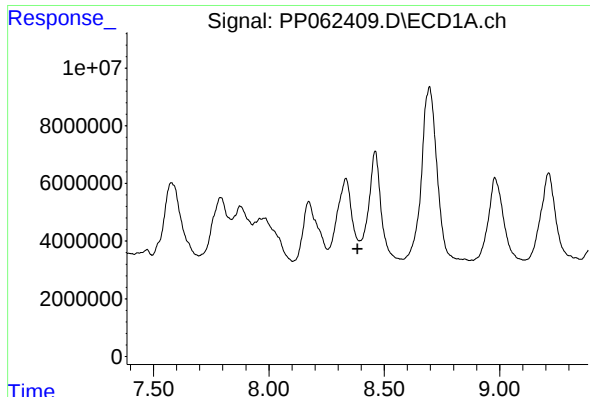

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.384 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

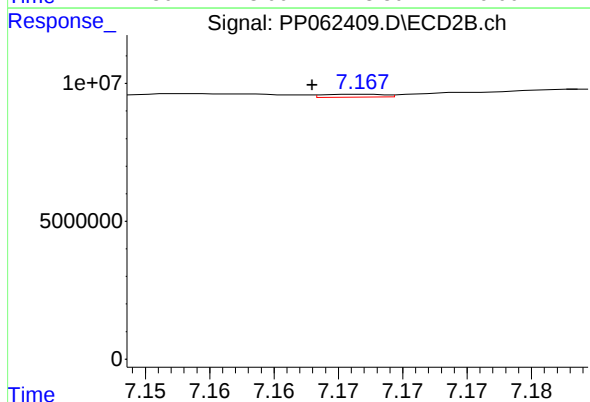


#37 AR-1262-2

R.T.: 7.167 min
Delta R.T.: 0.004 min
Response: 336610
Conc: 1.86 ng/ml

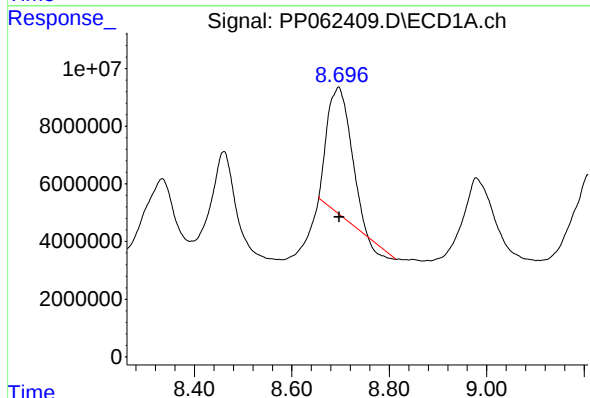


#38 AR-1262-3

R.T.: 8.696 min
Delta R.T.: -0.001 min
Response: 143197602
Conc: 1633.74 ng/ml

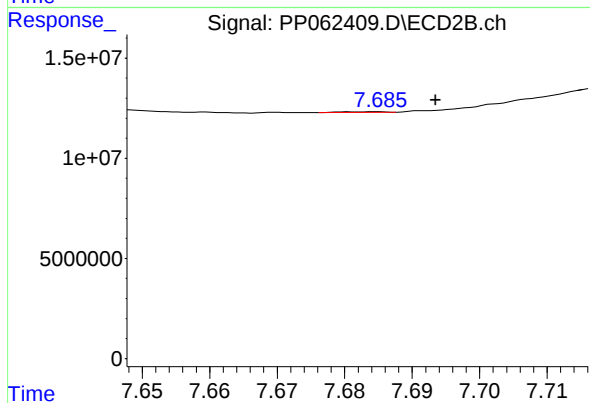

#38 AR-1262-3


R.T.: 7.685 min
Delta R.T.: -0.008 min
Response: 177224
Conc: 1.41 ng/ml

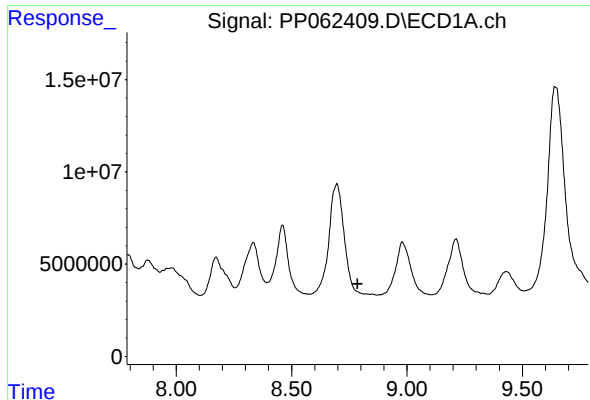

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.786 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

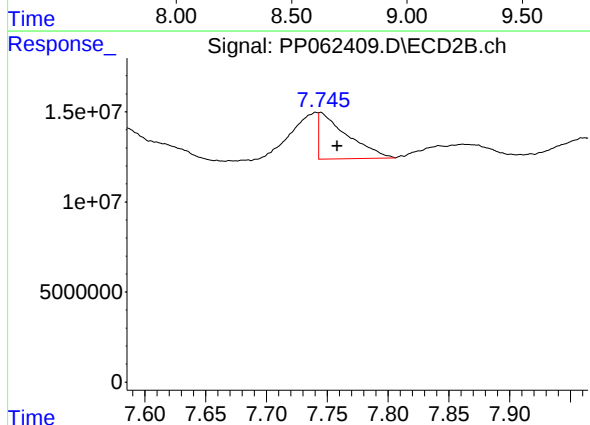


#39 AR-1262-4

R.T.: 7.745 min
Delta R.T.: -0.013 min
Response: 42179787
Conc: 179.08 ng/ml

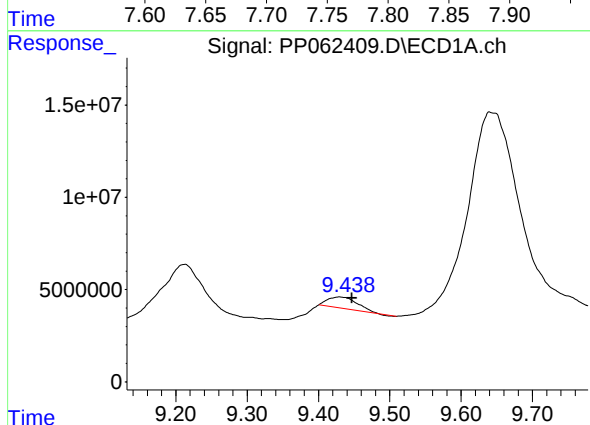


#40 AR-1262-5

R.T.: 9.430 min
Delta R.T.: -0.017 min
Response: 16933935
Conc: 415.97 ng/ml

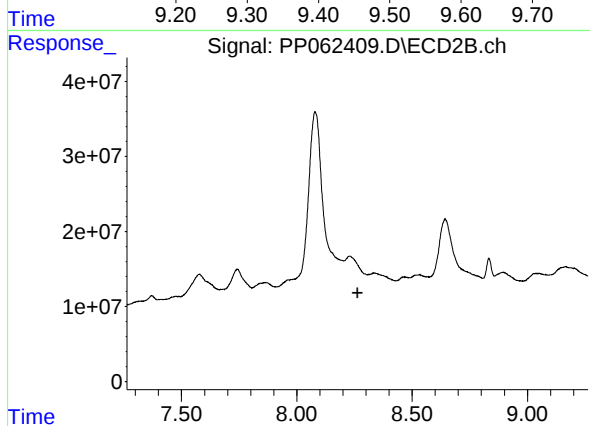

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 8.263 min
Response: 0
Conc: N.D.

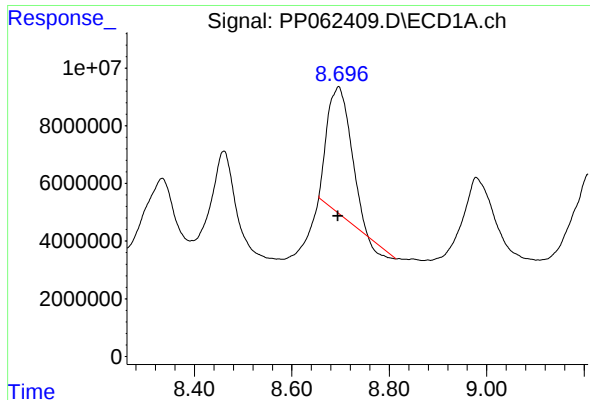

#41 AR-1268-1


R.T.: 8.696 min
Delta R.T.: 0.001 min
Response: 143197602
Conc: 865.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

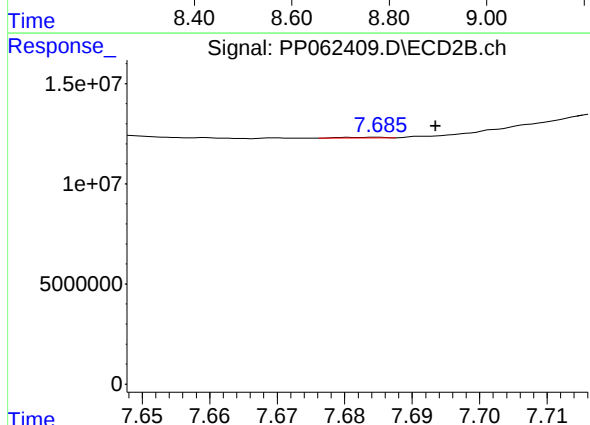


#41 AR-1268-1

R.T.: 7.685 min
Delta R.T.: -0.008 min
Response: 177224
Conc: 0.45 ng/ml

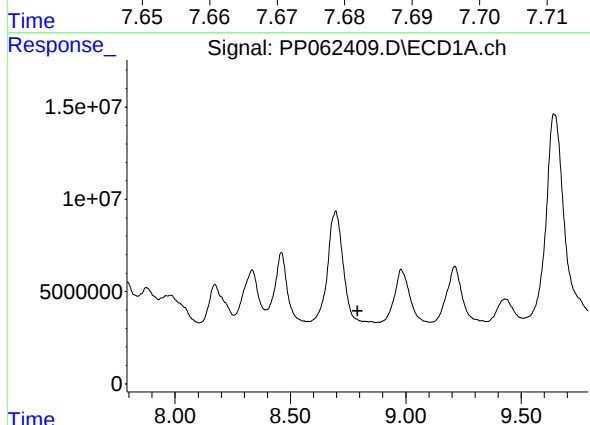


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.790 min
Response: 0
Conc: N.D.

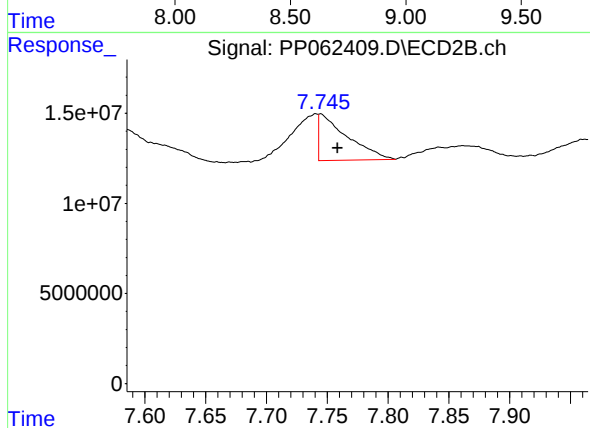

#42 AR-1268-2


R.T.: 7.745 min
Delta R.T.: -0.014 min
Response: 42179787
Conc: 118.54 ng/ml

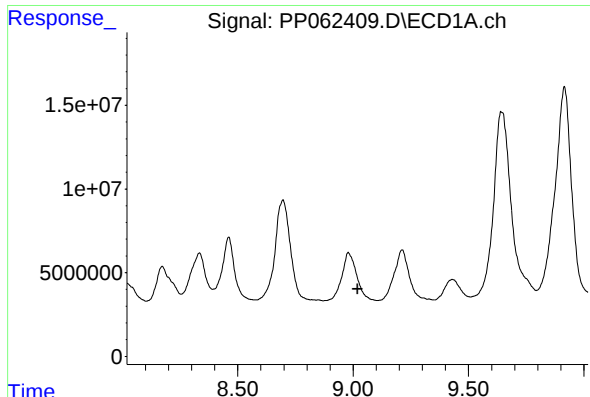

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.019 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

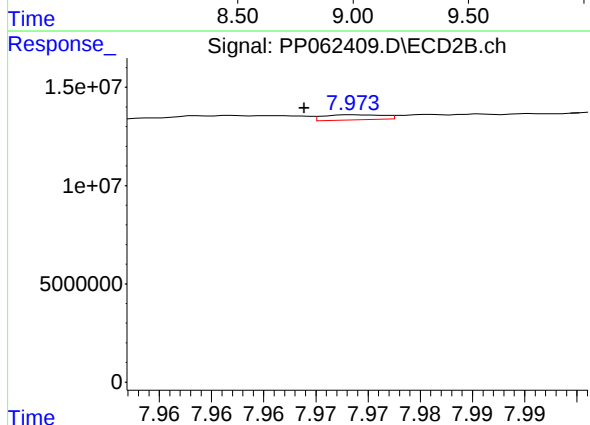


#43 AR-1268-3

R.T.: 7.974 min
Delta R.T.: 0.005 min
Response: 1050542
Conc: 3.15 ng/ml

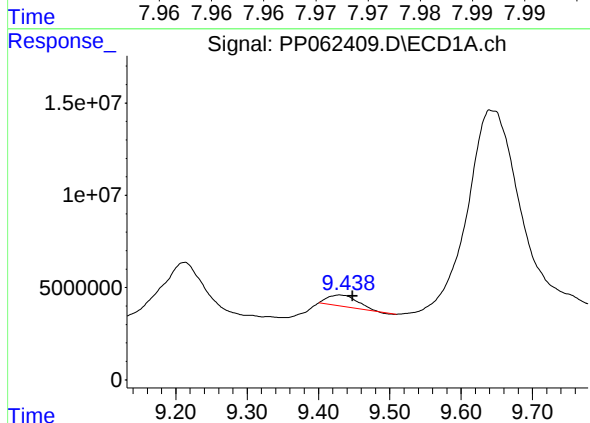


#44 AR-1268-4

R.T.: 9.430 min
Delta R.T.: -0.018 min
Response: 16933935
Conc: 368.02 ng/ml

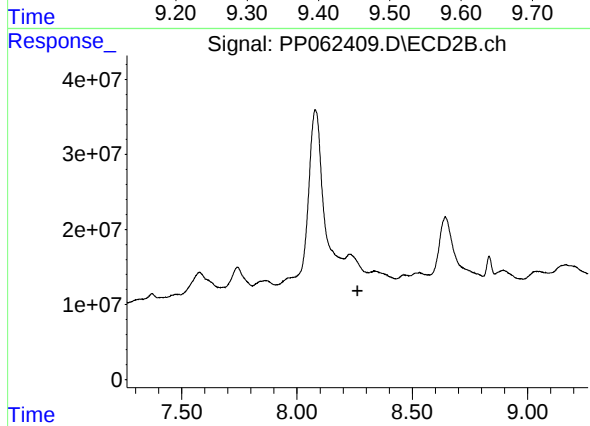

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 8.262 min
Response: 0
Conc: N.D.

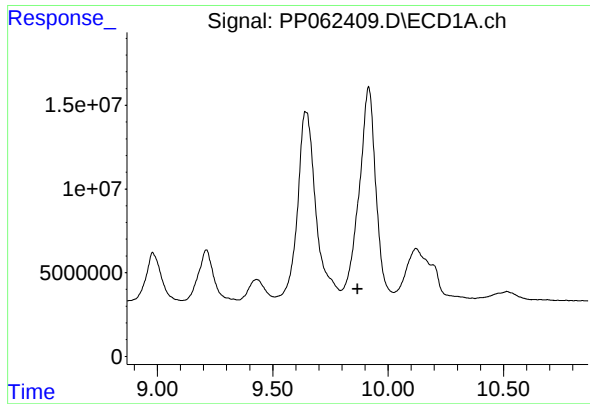

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-120623-03

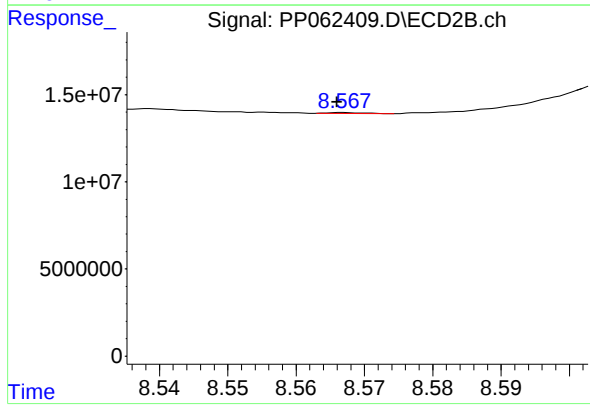

#45 AR-1268-5

R.T.: 8.567 min
Delta R.T.: 0.000 min
Response: 210575
Conc: 0.24 ng/ml