

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121223\
 Data File : PP062408.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2023 14:56
 Operator : YP\AJ
 Sample : 05764-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-120623-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 23:28:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 12 05:13:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.432	3.718	38580484	62533800	22.999	20.377
2)	SA Decachlor...	10.200	8.830	86981327	134.6E6	83.236	58.451 #
Target Compounds							
3)	L1 AR-1016-1	5.606	4.830	3980.2E6	5669.9E6	80411.781	61575.059
4)	L1 AR-1016-2	5.629	4.849	5421.0E6	6511.5E6	70478.941	49379.154 #
5)	L1 AR-1016-3	5.691	5.030	3135.5E6	4965.6E6	63560.794	69394.806
6)	L1 AR-1016-4	5.790	5.079	3353.3E6	38633.1E6	85323.786	612474.555 #
7)	L1 AR-1016-5	6.085	5.292	22465.8E6	33143.5E6	541767.983	400983.267 #
8)	L2 AR-1221-1	4.635	3.931	4085941	4210182	203.228	113.754 #
9)	L2 AR-1221-2	4.726	4.024	6480973	30734129	567.179	1079.417 #
10)	L2 AR-1221-3	4.804	4.102	108.0E6	195.9E6	2462.309	2397.439
11)	L3 AR-1232-1	4.804	4.102	108.0E6	195.9E6	3000.156	3064.060
12)	L3 AR-1232-2	5.337	4.849	1428.4E6	6511.5E6	68514.604	112465.830 #
13)	L3 AR-1232-3	5.629	5.030	5421.0E6	4965.6E6	159866.236	157603.967
14)	L3 AR-1232-4	5.790	5.115	3353.3E6	19687.8E6	185170.414	625382.530 #
15)	L3 AR-1232-5	5.882	5.292	30468.3E6	33143.5E6	2034543.228	980431.000 #
16)	L4 AR-1242-1	5.606	4.830	3980.2E6	5669.9E6	96589.819	75551.654
17)	L4 AR-1242-2	5.629	4.849	5421.0E6	6511.5E6	87146.080	60988.744 #
18)	L4 AR-1242-3	5.691	5.030	3135.5E6	4965.6E6	77349.713	85239.447
19)	L4 AR-1242-4	5.790	5.115	3353.3E6	19687.8E6	99402.057	309018.826 #
20)	L4 AR-1242-5	6.539	5.666f	31976.1E6	52627.0E6	898897.838	754754.917
21)	L5 AR-1248-1	5.606	4.830	3980.2E6	5669.9E6	128622.018	102161.406
22)	L5 AR-1248-2	5.882	5.079	30468.3E6	38633.1E6	578692.023	434254.678
23)	L5 AR-1248-3	6.085	5.115	22465.8E6	19687.8E6	395086.813	211892.684 #
24)	L5 AR-1248-4	0.000	5.292	0	33143.5E6	N.D.	304277.739 #
25)	L5 AR-1248-5	6.539	5.666f	31976.1E6	52627.0E6	532595.676	379430.509 #
26)	L6 AR-1254-1	6.459	5.666f	66912.1E6	52627.0E6	986881.342	329990.060 #
27)	L6 AR-1254-2	6.679	5.817f	55282.0E6	53406.7E6	524450.161	377468.774 #
28)	L6 AR-1254-3	7.075f	6.231f	56367.9E6	104674.3E6	520651.073	472247.783
29)	L6 AR-1254-4	7.337	0.000	56991.0E6	0	887626.165	N.D. #
30)	L6 AR-1254-5	7.761	0.000	101550.3E6	0	1385203.307	N.D. #
31)	L7 AR-1260-1	0.000	6.359f	0	68834.3E6	N.D.	425401.469 #
32)	L7 AR-1260-2	7.476	6.542	61276.2E6	50048.8E6	716275.722	274719.761 #
33)	L7 AR-1260-3	0.000	6.696	0	49312.1E6	N.D.	273989.696 #
34)	L7 AR-1260-4	8.046f	7.165	44035.6E6	27489.7E6	599202.510	188125.897 #
35)	L7 AR-1260-5	8.386	7.409	22814.1E6	91051.1E6	193910.669	314773.065 #
36)	L8 AR-1262-1	7.895	6.938f	16287.1E6	43603.2E6	404670.489	495970.047
37)	L8 AR-1262-2	8.386	7.165	22814.1E6	27489.7E6	174772.747	152096.474
38)	L8 AR-1262-3	8.712	7.695	25589.4E6	10634.4E6	291949.540	84892.078 #
39)	L8 AR-1262-4	8.762f	7.759	20535.5E6	41802.0E6	303000.654	177473.848 #
40)	L8 AR-1262-5	9.446	8.262	9842.9E6	13503.8E6	241784.376	146070.911 #
41)	L9 AR-1268-1	8.712f	7.695	25589.4E6	10634.4E6	154736.293	27076.656 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121223\
 Data File : PP062408.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2023 14:56
 Operator : YP\AJ
 Sample : 05764-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-120623-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 23:28:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 12 05:13:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.762f	7.759	20535.5E6	41802.0E6	144198.809	117480.768
43) L9	AR-1268-3	9.017	7.966	252.4E6	674.6E6	1936.358	2022.700
44) L9	AR-1268-4	9.446	8.262	9842.9E6	13503.8E6	213909.784	122455.477 #
45) L9	AR-1268-5	9.861	8.564	1605.9E6	3232.8E6	4109.610	3758.086



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121223\
Data File : PP062408.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2023 14:56
Operator : YP\AJ
Sample : 05764-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 23:28:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 12 05:13:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

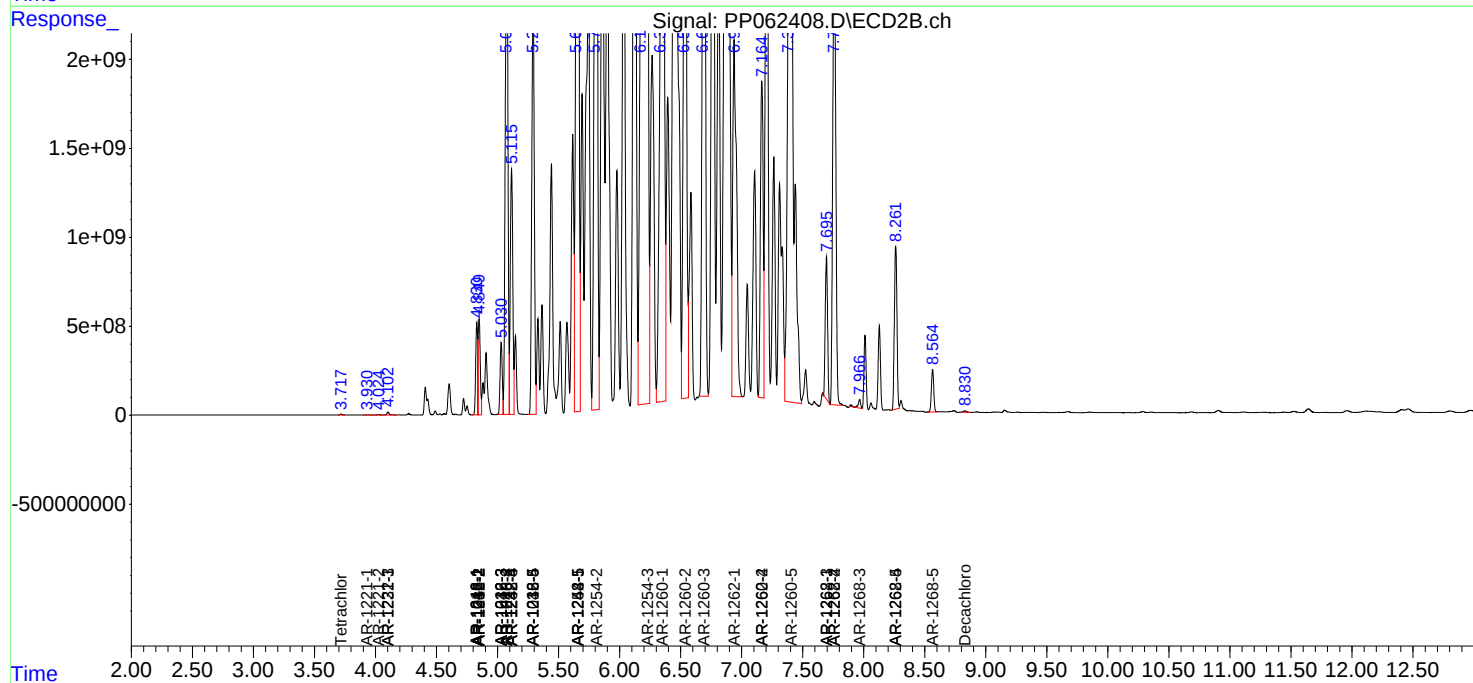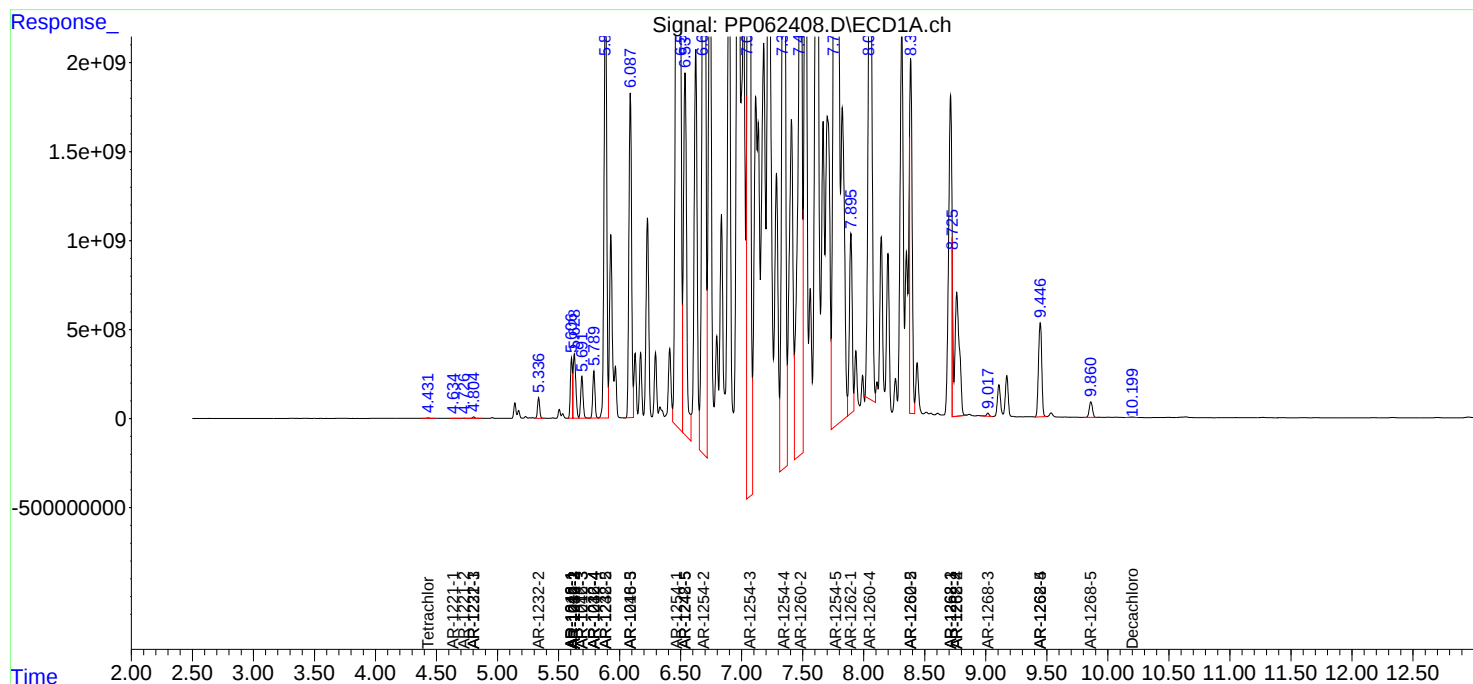


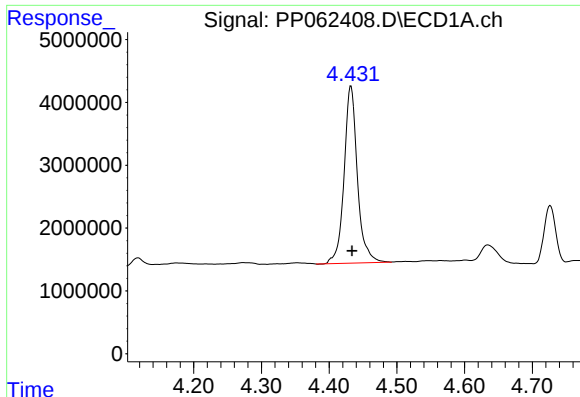

#1 Tetrachloro-m-xylene


R.T.: 4.432 min
Delta R.T.: -0.002 min
Response: 38580484
Conc: 23.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

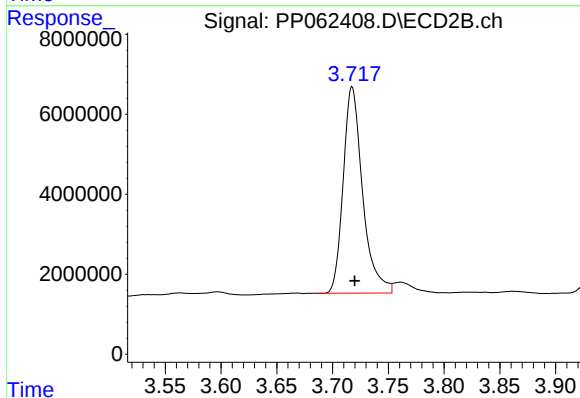


#1 Tetrachloro-m-xylene

R.T.: 3.718 min
Delta R.T.: -0.002 min
Response: 62533800
Conc: 20.38 ng/ml

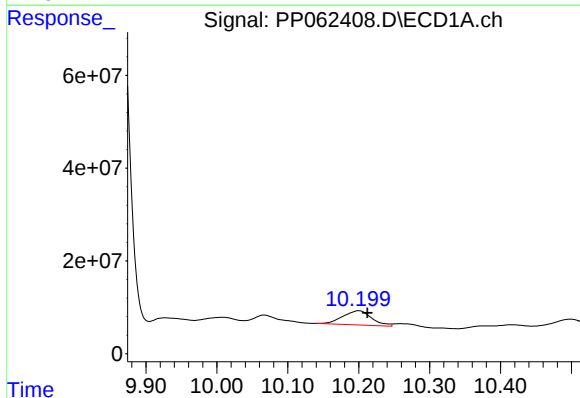


#2 Decachlorobiphenyl

R.T.: 10.200 min
Delta R.T.: -0.013 min
Response: 86981327
Conc: 83.24 ng/ml

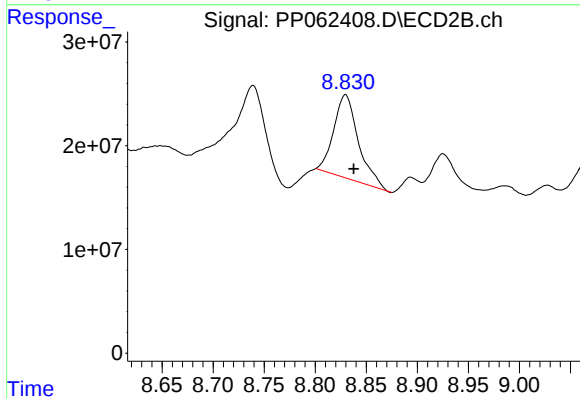

#2 Decachlorobiphenyl


R.T.: 8.830 min
Delta R.T.: -0.008 min
Response: 134612545
Conc: 58.45 ng/ml

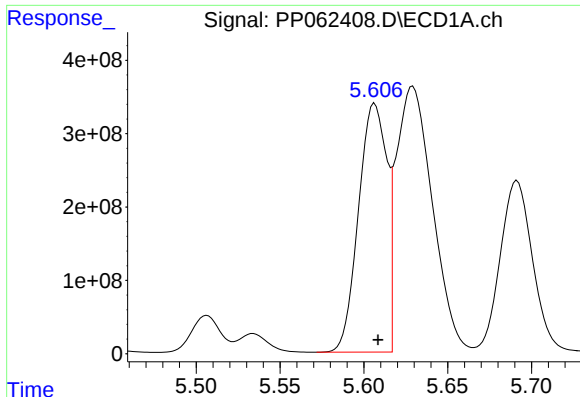

#3 AR-1016-1


R.T.: 5.606 min
Delta R.T.: -0.002 min
Response: 3980226777
Conc: 80411.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

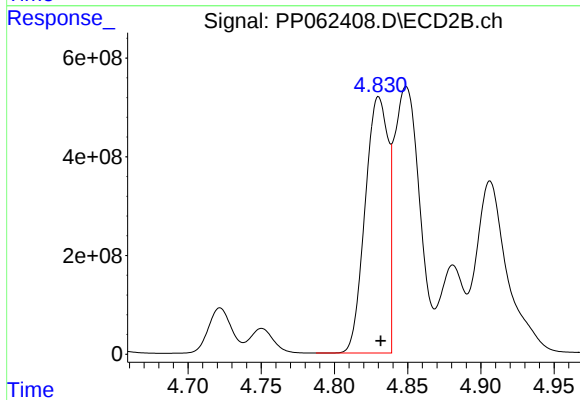


#3 AR-1016-1

R.T.: 4.830 min
Delta R.T.: -0.001 min
Response: 5669918168
Conc: 61575.06 ng/ml

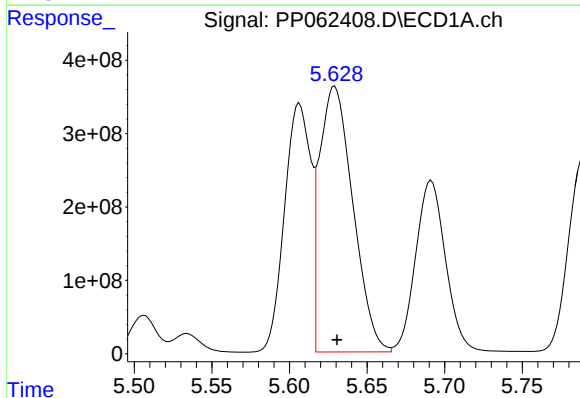


#4 AR-1016-2

R.T.: 5.629 min
Delta R.T.: -0.001 min
Response: 5420958340
Conc: 70478.94 ng/ml

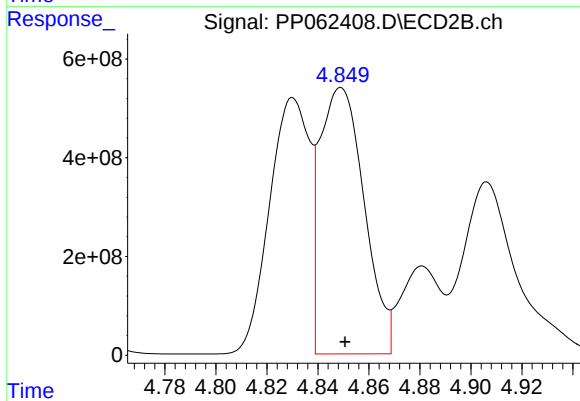

#4 AR-1016-2


R.T.: 4.849 min
Delta R.T.: -0.002 min
Response: 6511516569
Conc: 49379.15 ng/ml

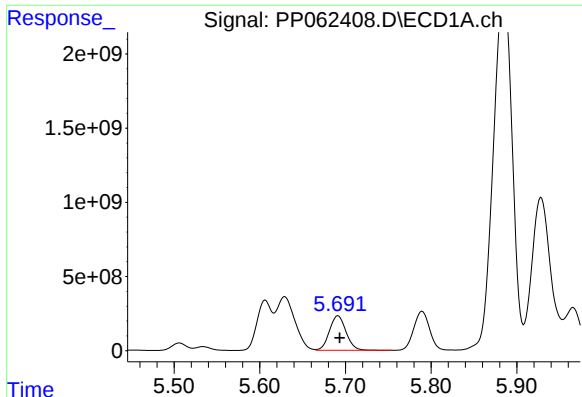

#5 AR-1016-3


R.T.: 5.691 min
Delta R.T.: -0.002 min
Response: 3135460171
Conc: 63560.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

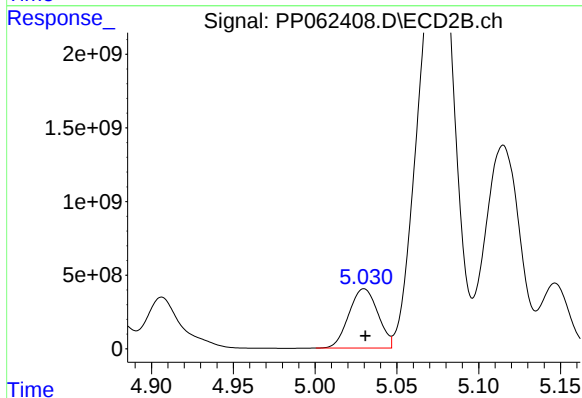


#5 AR-1016-3

R.T.: 5.030 min
Delta R.T.: 0.000 min
Response: 4965619138
Conc: 69394.81 ng/ml

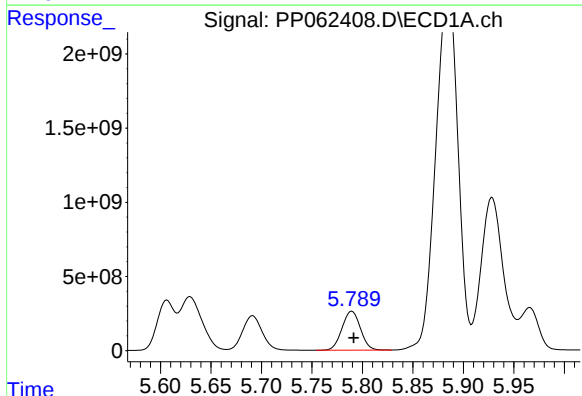


#6 AR-1016-4

R.T.: 5.790 min
Delta R.T.: -0.002 min
Response: 3353334328
Conc: 85323.79 ng/ml

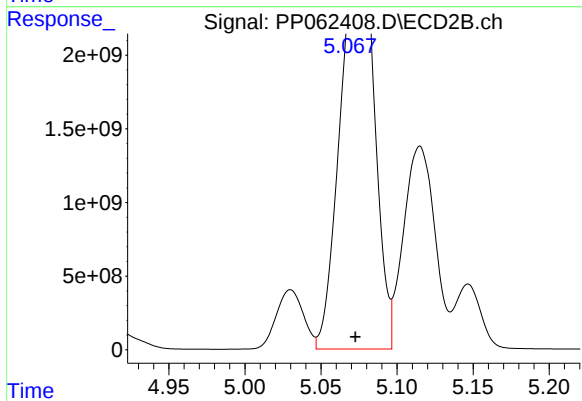

#6 AR-1016-4


R.T.: 5.079 min
Delta R.T.: 0.007 min
Response: 38633103931
Conc: 612474.56 ng/ml

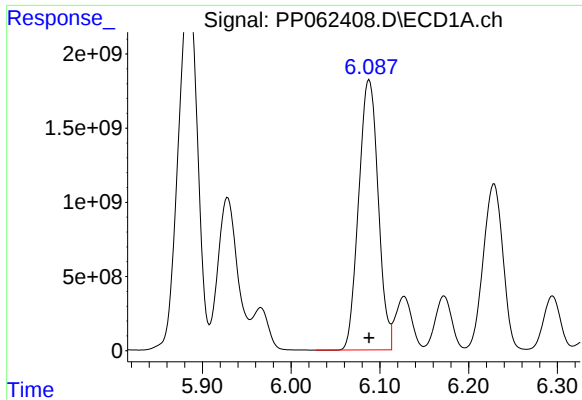

#7 AR-1016-5


R.T.: 6.085 min
Delta R.T.: -0.002 min
Response: 22465802572
Conc: 541767.98 ng

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

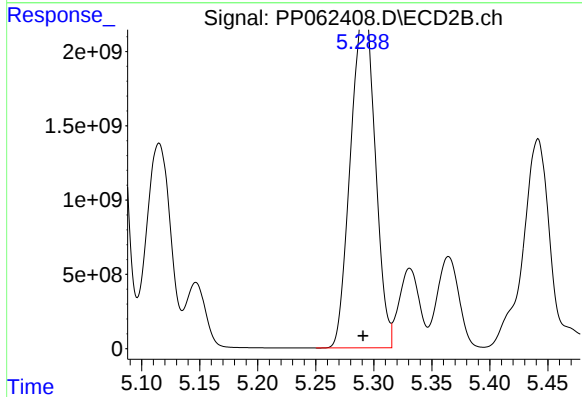


#7 AR-1016-5

R.T.: 5.292 min
Delta R.T.: 0.002 min
Response: 33143544764
Conc: 400983.27 ng/ml

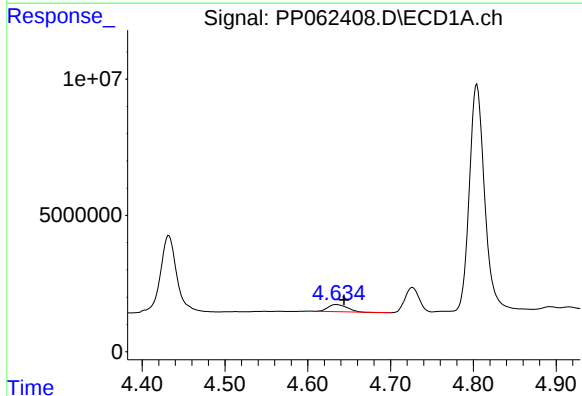


#8 AR-1221-1

R.T.: 4.635 min
Delta R.T.: -0.009 min
Response: 4085941
Conc: 203.23 ng/ml

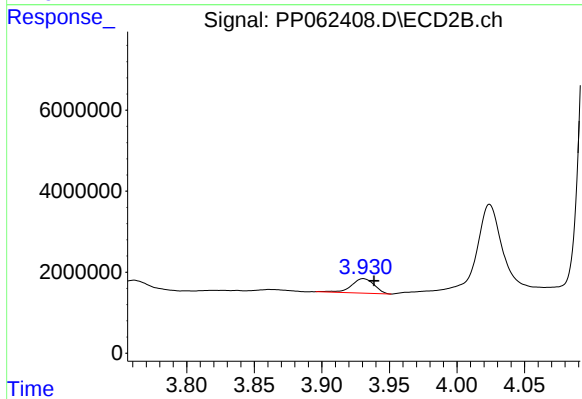

#8 AR-1221-1


R.T.: 3.931 min
Delta R.T.: -0.008 min
Response: 4210182
Conc: 113.75 ng/ml

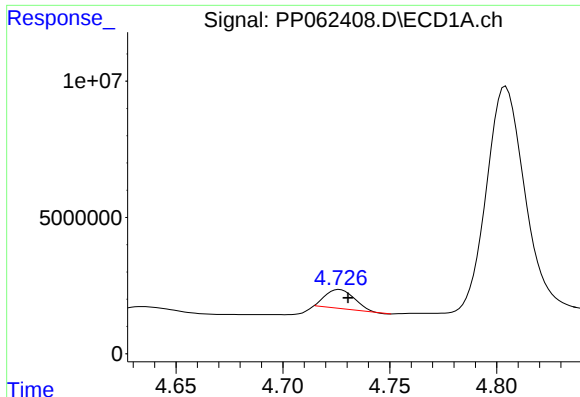

#9 AR-1221-2


R.T.: 4.726 min
Delta R.T.: -0.004 min
Response: 6480973
Conc: 567.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

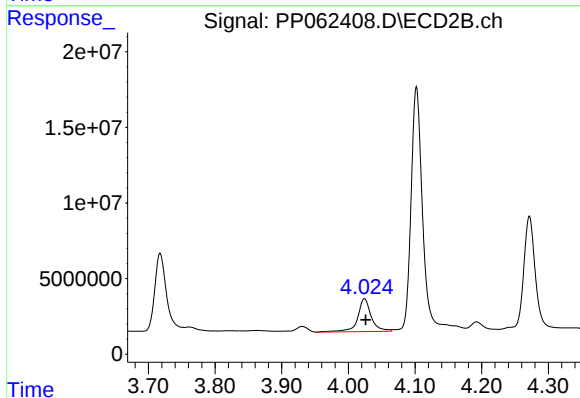


#9 AR-1221-2

R.T.: 4.024 min
Delta R.T.: -0.002 min
Response: 30734129
Conc: 1079.42 ng/ml

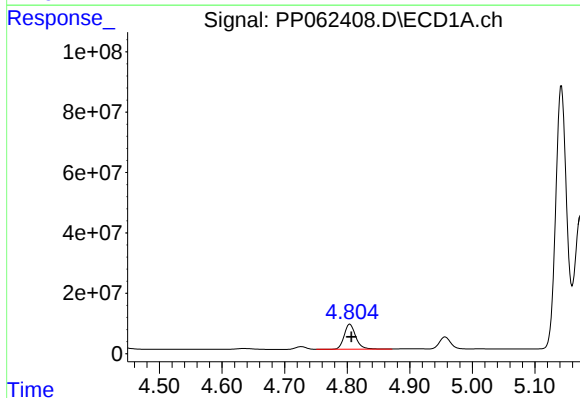


#10 AR-1221-3

R.T.: 4.804 min
Delta R.T.: -0.003 min
Response: 107959835
Conc: 2462.31 ng/ml

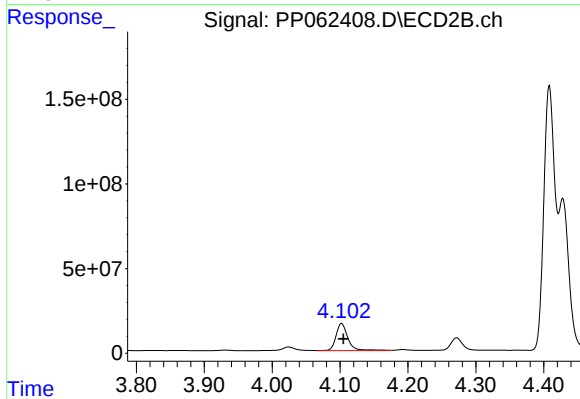

#10 AR-1221-3


R.T.: 4.102 min
Delta R.T.: -0.003 min
Response: 195943459
Conc: 2397.44 ng/ml

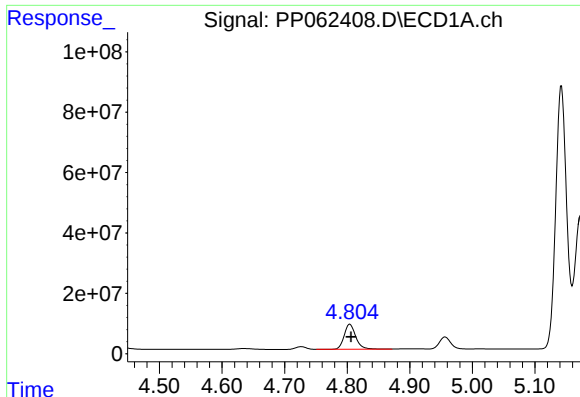

#11 AR-1232-1


R.T.: 4.804 min
Delta R.T.: -0.002 min
Response: 107959835
Conc: 3000.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

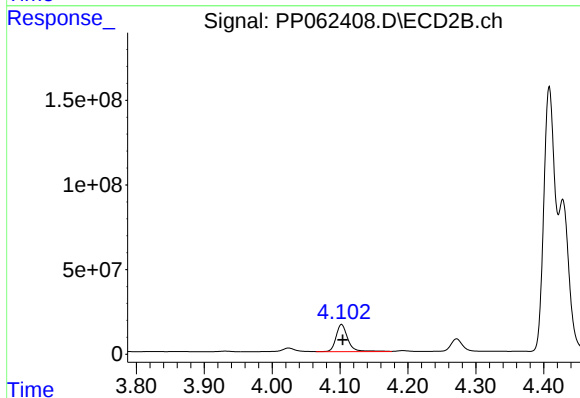


#11 AR-1232-1

R.T.: 4.102 min
Delta R.T.: -0.002 min
Response: 195943459
Conc: 3064.06 ng/ml

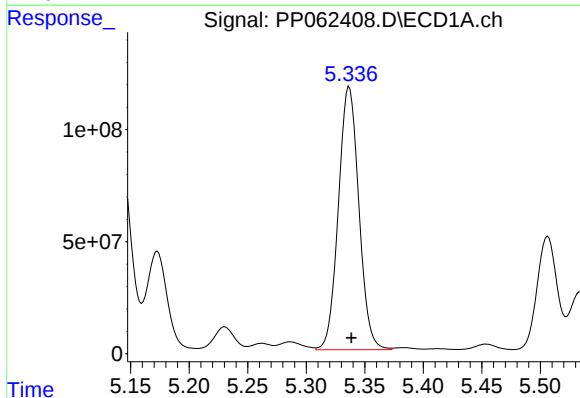


#12 AR-1232-2

R.T.: 5.337 min
Delta R.T.: -0.002 min
Response: 1428404568
Conc: 68514.60 ng/ml

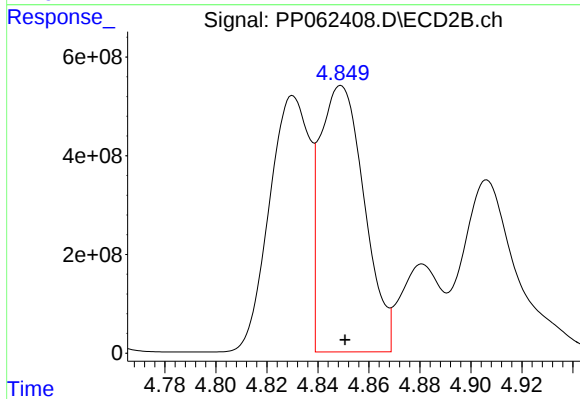

#12 AR-1232-2


R.T.: 4.849 min
Delta R.T.: -0.002 min
Response: 6511516569
Conc: 112465.83 ng/ml

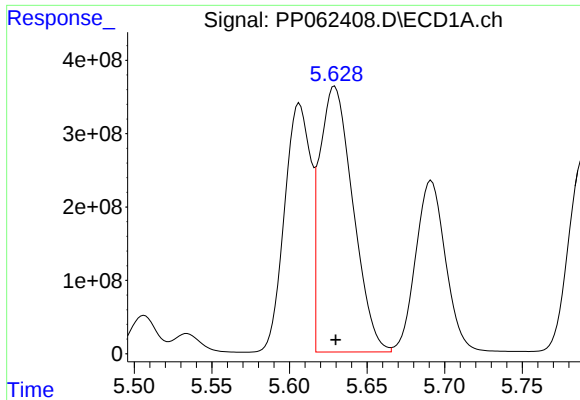

#13 AR-1232-3


R.T.: 5.629 min
Delta R.T.: 0.000 min
Response: 5420958340
Conc: 159866.24 ng

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

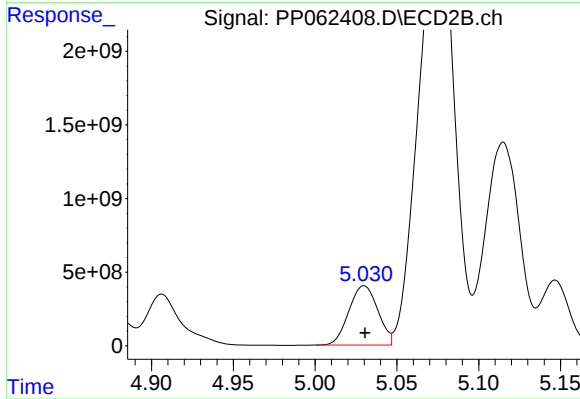


#13 AR-1232-3

R.T.: 5.030 min
Delta R.T.: 0.000 min
Response: 4965619138
Conc: 157603.97 ng/ml

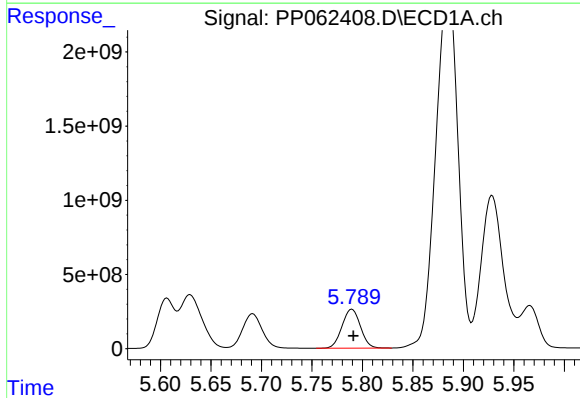


#14 AR-1232-4

R.T.: 5.790 min
Delta R.T.: -0.002 min
Response: 3353334328
Conc: 185170.41 ng/ml

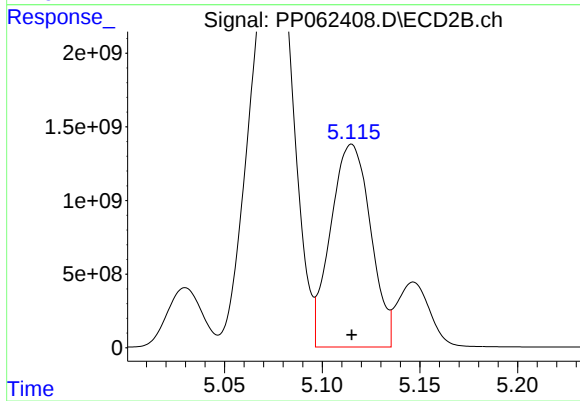

#14 AR-1232-4


R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 19687753027
Conc: 625382.53 ng/ml

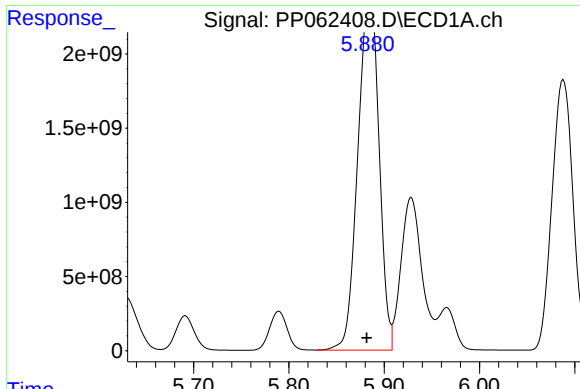

#15 AR-1232-5


R.T.: 5.882 min
Delta R.T.: 0.000 min
Response: 30468292077
Conc: 2034543.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

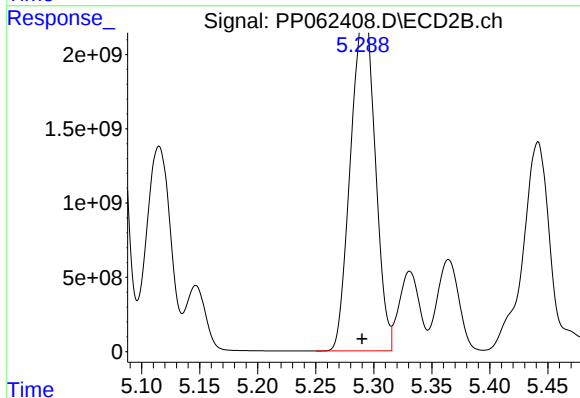


#15 AR-1232-5

R.T.: 5.292 min
Delta R.T.: 0.002 min
Response: 33143544764
Conc: 980431.00 ng/ml

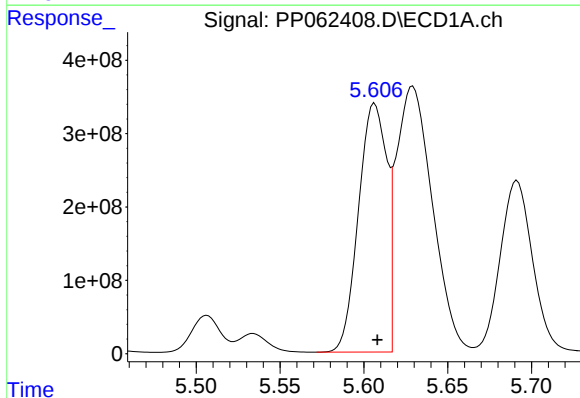


#16 AR-1242-1

R.T.: 5.606 min
Delta R.T.: -0.002 min
Response: 3980226777
Conc: 96589.82 ng/ml

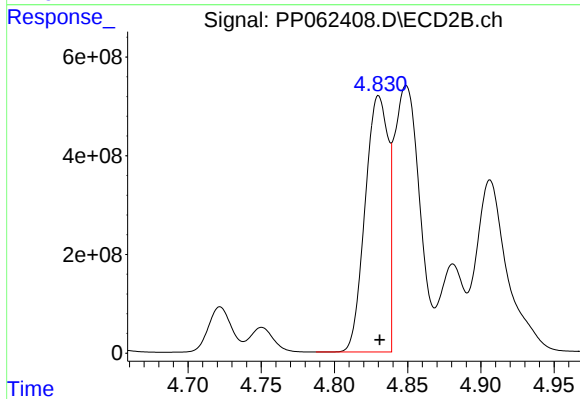

#16 AR-1242-1


R.T.: 4.830 min
Delta R.T.: 0.000 min
Response: 5669918168
Conc: 75551.65 ng/ml

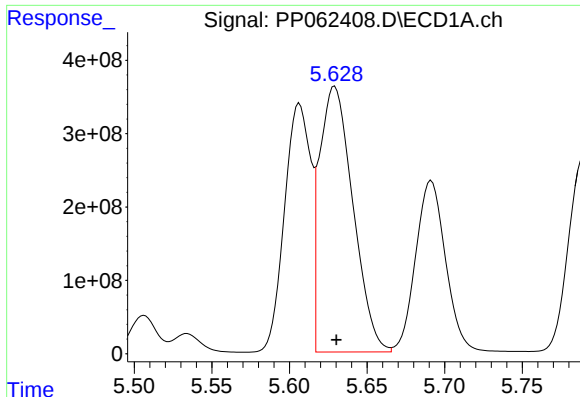

#17 AR-1242-2


R.T.: 5.629 min
Delta R.T.: -0.001 min
Response: 5420958340
Conc: 87146.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

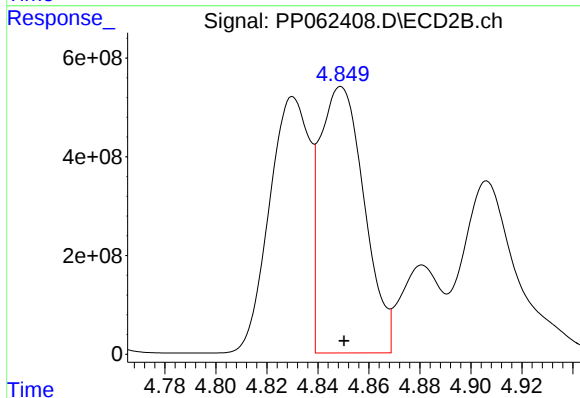


#17 AR-1242-2

R.T.: 4.849 min
Delta R.T.: -0.001 min
Response: 6511516569
Conc: 60988.74 ng/ml

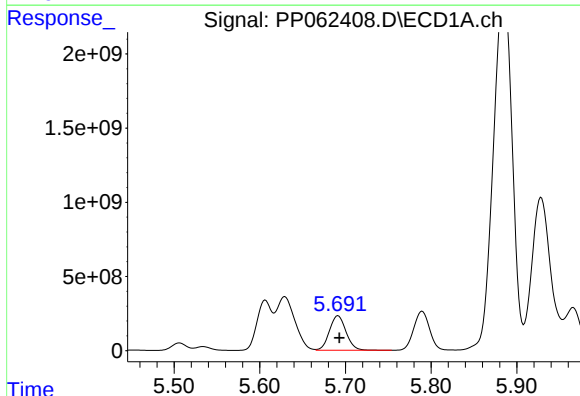


#18 AR-1242-3

R.T.: 5.691 min
Delta R.T.: -0.002 min
Response: 3135460171
Conc: 77349.71 ng/ml

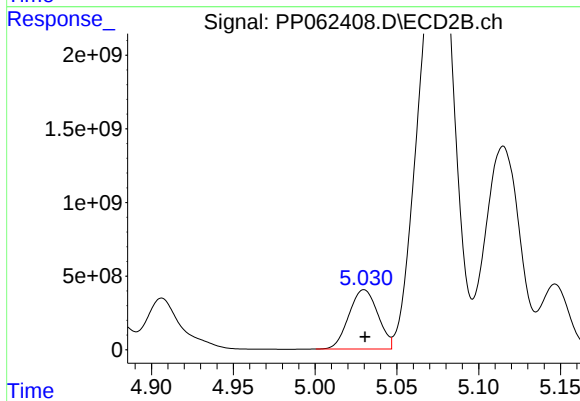

#18 AR-1242-3


R.T.: 5.030 min
Delta R.T.: 0.000 min
Response: 4965619138
Conc: 85239.45 ng/ml

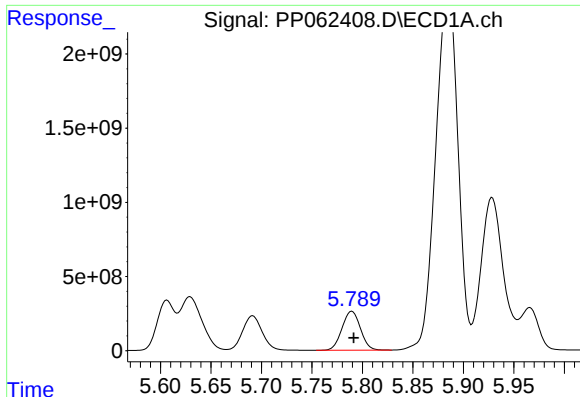

#19 AR-1242-4


R.T.: 5.790 min
Delta R.T.: -0.002 min
Response: 3353334328
Conc: 99402.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

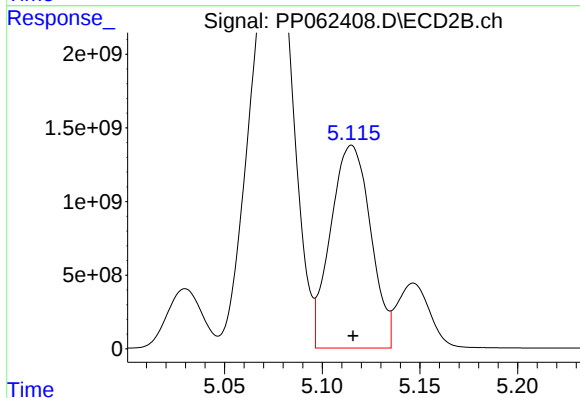


#19 AR-1242-4

R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 19687753027
Conc: 309018.83 ng/ml

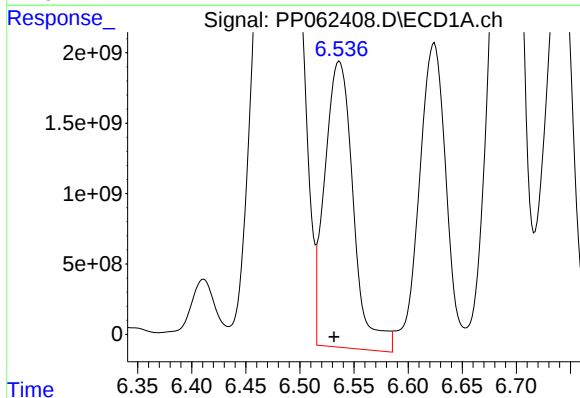


#20 AR-1242-5

R.T.: 6.539 min
Delta R.T.: 0.007 min
Response: 31976113702
Conc: 898897.84 ng/ml

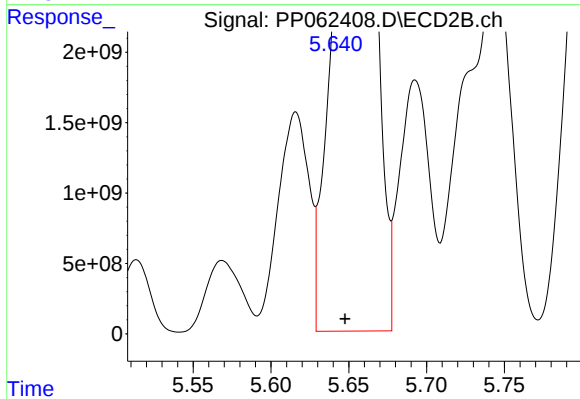

#20 AR-1242-5


R.T.: 5.666 min
Delta R.T.: 0.018 min
Response: 52626956959
Conc: 754754.92 ng/ml

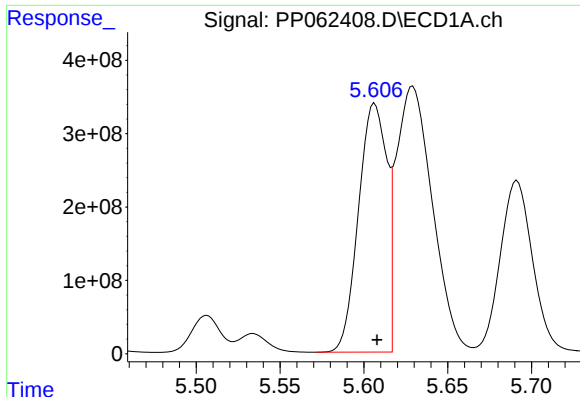

#21 AR-1248-1


R.T.: 5.606 min
Delta R.T.: -0.001 min
Response: 3980226777
Conc: 128622.02 ng

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

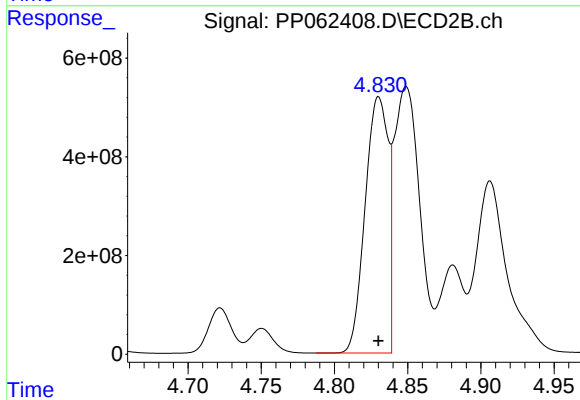


#21 AR-1248-1

R.T.: 4.830 min
Delta R.T.: 0.000 min
Response: 5669918168
Conc: 102161.41 ng/ml

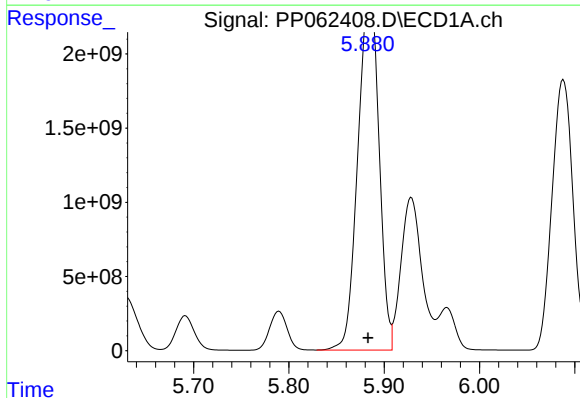


#22 AR-1248-2

R.T.: 5.882 min
Delta R.T.: -0.001 min
Response: 30468292077
Conc: 578692.02 ng/ml

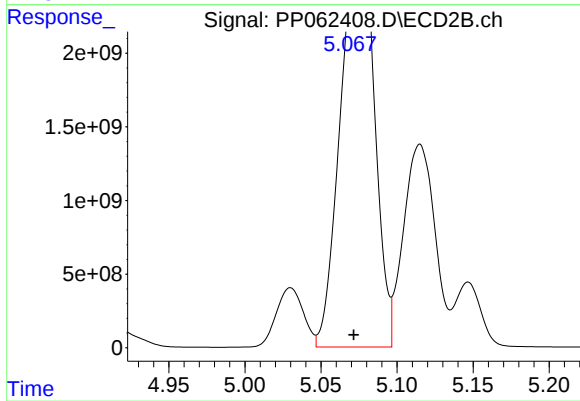

#22 AR-1248-2


R.T.: 5.079 min
Delta R.T.: 0.008 min
Response: 38633103931
Conc: 434254.68 ng/ml

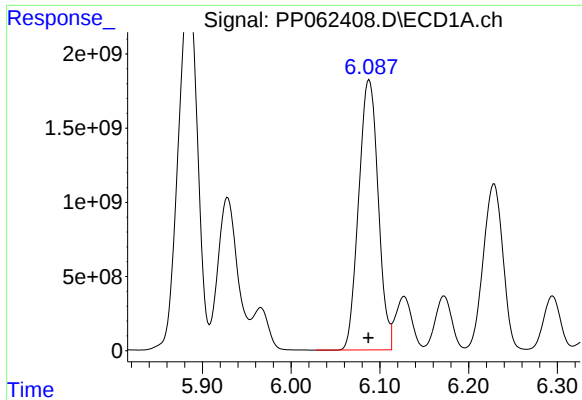

#23 AR-1248-3


R.T.: 6.085 min
Delta R.T.: -0.002 min
Response: 22465802572
Conc: 395086.81 ng

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

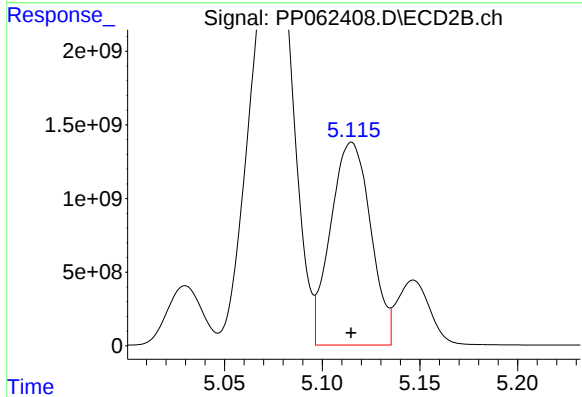


#23 AR-1248-3

R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 19687753027
Conc: 211892.68 ng/ml

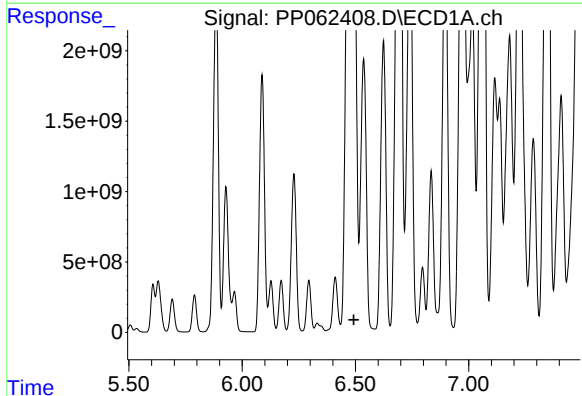


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 6.493 min
Response: 0
Conc: N.D.

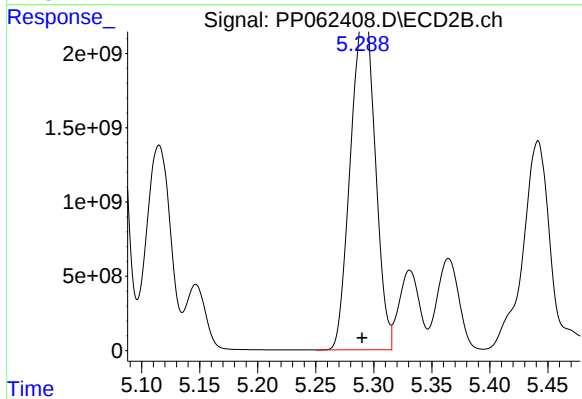

#24 AR-1248-4


R.T.: 5.292 min
Delta R.T.: 0.002 min
Response: 33143544764
Conc: 304277.74 ng/ml

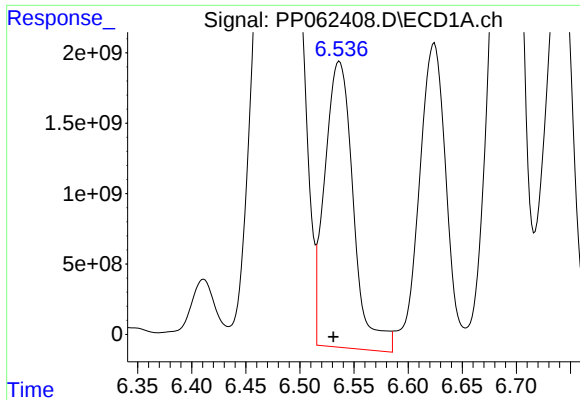

#25 AR-1248-5


R.T.: 6.539 min
Delta R.T.: 0.008 min
Response: 31976113702
Conc: 532595.68 ng

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

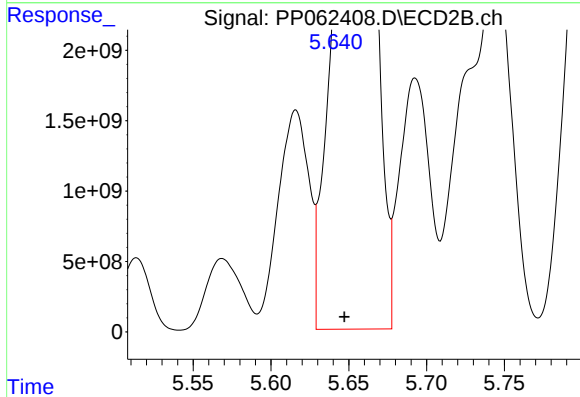


#25 AR-1248-5

R.T.: 5.666 min
Delta R.T.: 0.019 min
Response: 52626956959
Conc: 379430.51 ng/ml

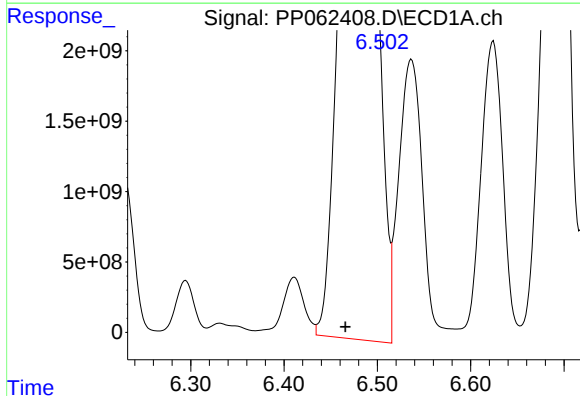


#26 AR-1254-1

R.T.: 6.459 min
Delta R.T.: -0.007 min
Response: 66912086995
Conc: 986881.34 ng/ml

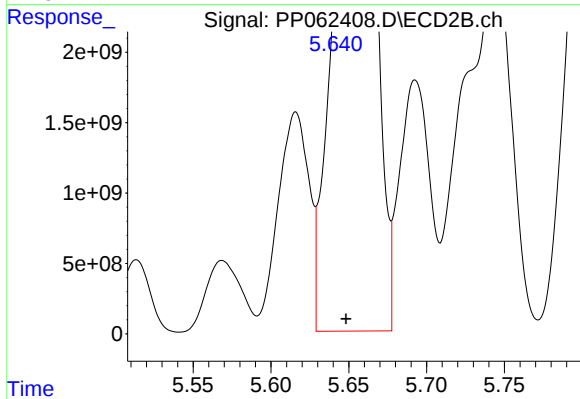

#26 AR-1254-1


R.T.: 5.666 min
Delta R.T.: 0.018 min
Response: 52626956959
Conc: 329990.06 ng/ml

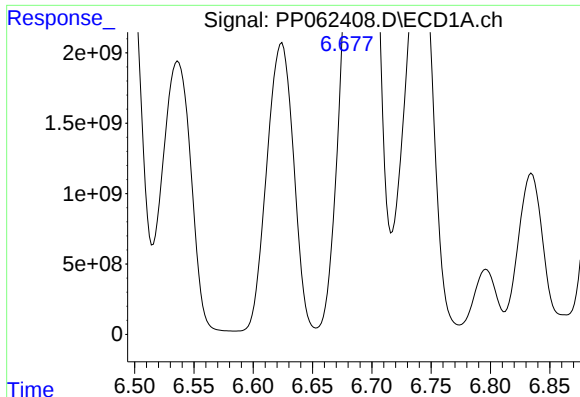

#27 AR-1254-2


R.T.: 6.679 min
Delta R.T.: -0.007 min
Response: 55281977323
Conc: 524450.16 ng

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

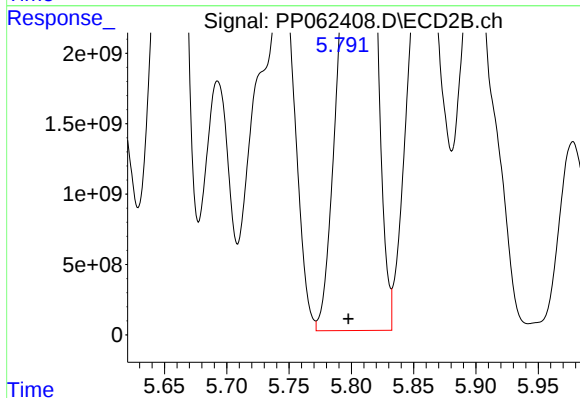


#27 AR-1254-2

R.T.: 5.817 min
Delta R.T.: 0.020 min
Response: 53406747109
Conc: 377468.77 ng/ml

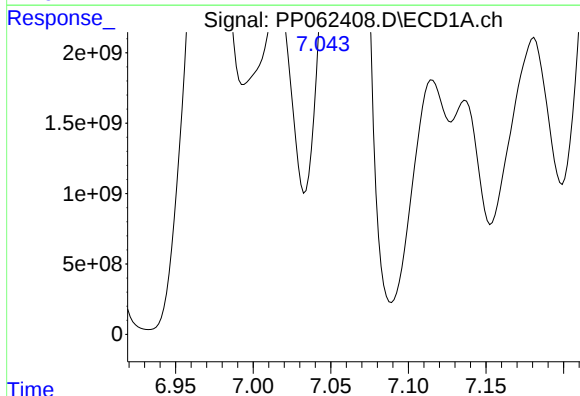


#28 AR-1254-3

R.T.: 7.075 min
Delta R.T.: 0.021 min
Response: 56367944415
Conc: 520651.07 ng/ml

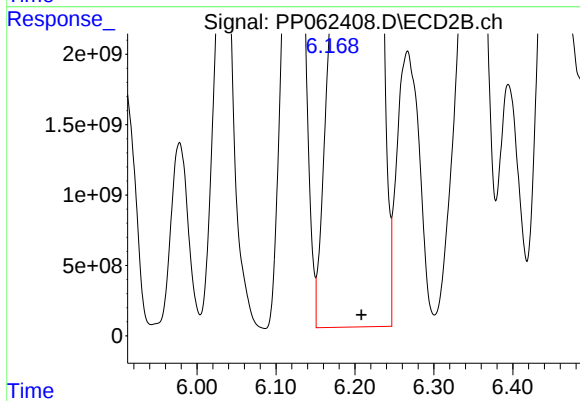

#28 AR-1254-3


R.T.: 6.231 min
Delta R.T.: 0.023 min
Response: 1.04674e+011
Conc: 472247.78 ng/ml

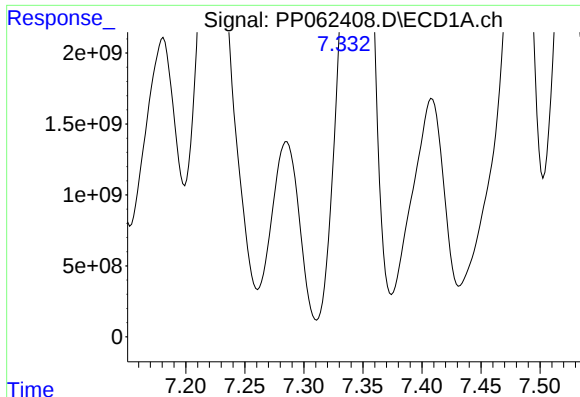

#29 AR-1254-4


R.T.: 7.337 min
Delta R.T.: -0.003 min
Response: 56990950797
Conc: 887626.17 ng

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

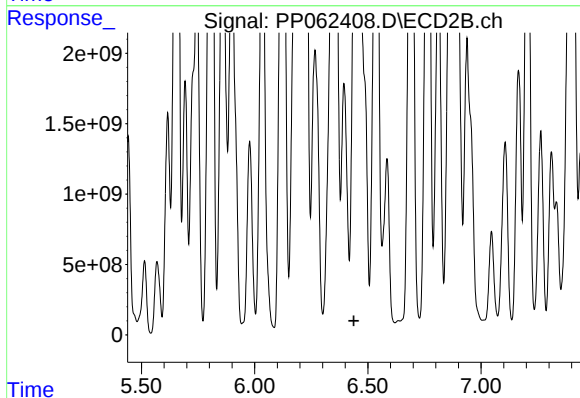


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.439 min
Response: 0
Conc: N.D.

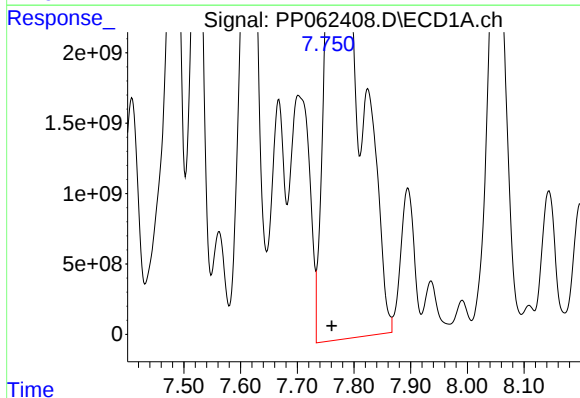


#30 AR-1254-5

R.T.: 7.761 min
Delta R.T.: 0.000 min
Response: 1.0155e+011
Conc: 1385203.31 ng/ml

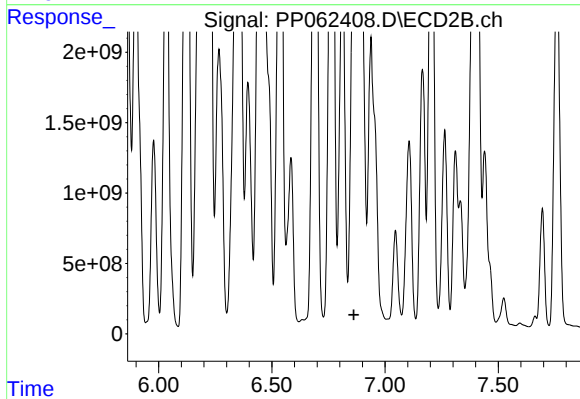

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.862 min
Response: 0
Conc: N.D.

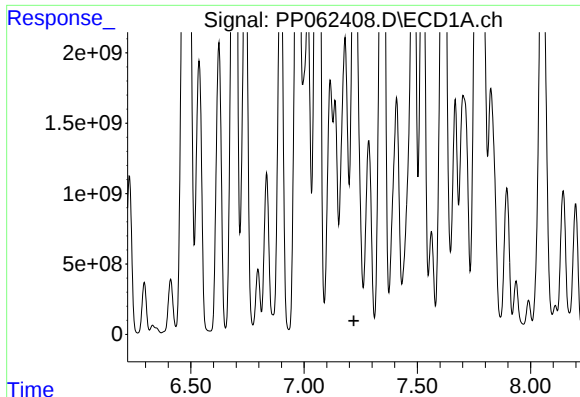

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

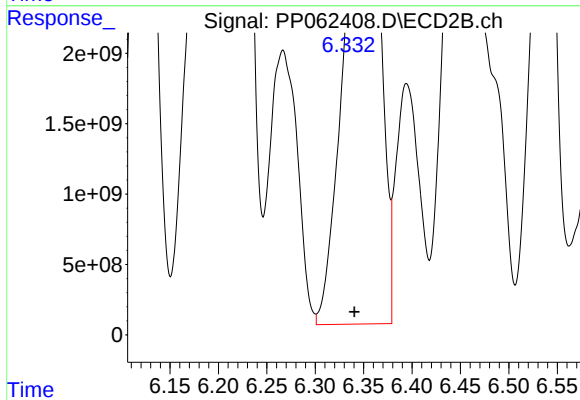


#31 AR-1260-1

R.T.: 6.359 min
Delta R.T.: 0.019 min
Response: 68834275045
Conc: 425401.47 ng/ml

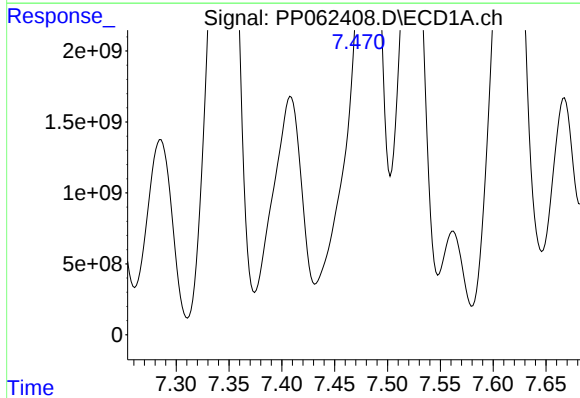


#32 AR-1260-2

R.T.: 7.476 min
Delta R.T.: -0.002 min
Response: 61276221409
Conc: 716275.72 ng/ml

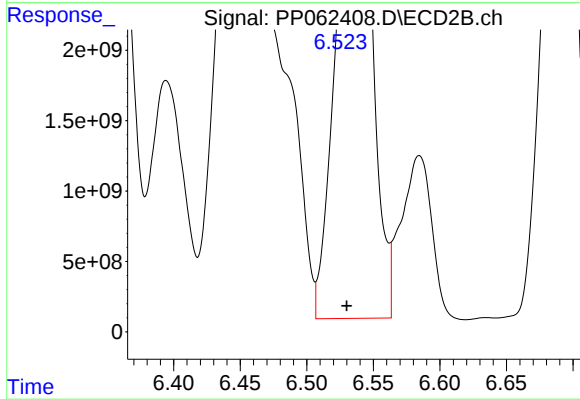

#32 AR-1260-2


R.T.: 6.542 min
Delta R.T.: 0.012 min
Response: 50048843113
Conc: 274719.76 ng/ml

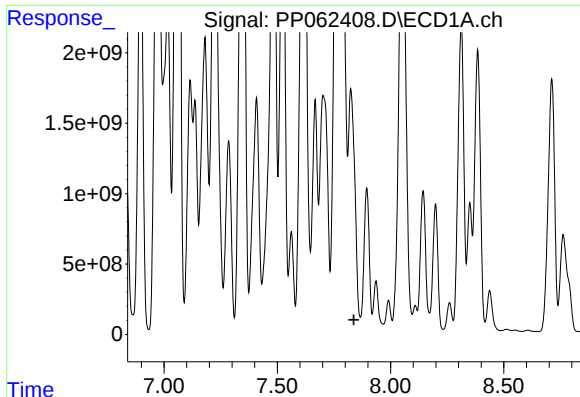

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.838 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

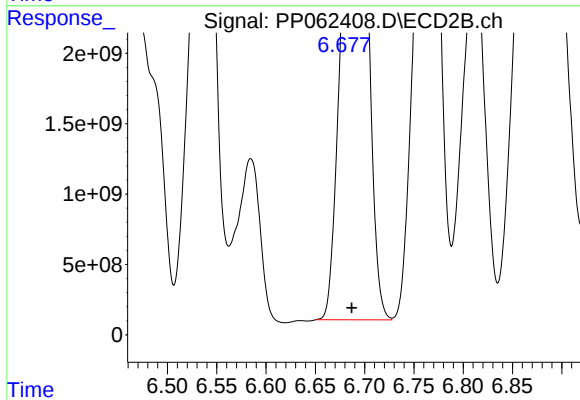


#33 AR-1260-3

R.T.: 6.696 min
Delta R.T.: 0.009 min
Response: 49312105419
Conc: 273989.70 ng/ml

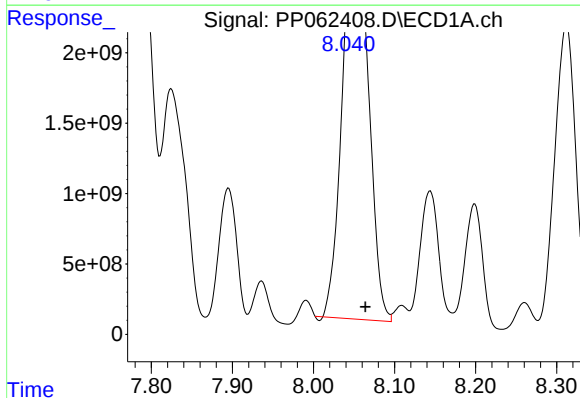


#34 AR-1260-4

R.T.: 8.046 min
Delta R.T.: -0.019 min
Response: 44035595652
Conc: 599202.51 ng/ml

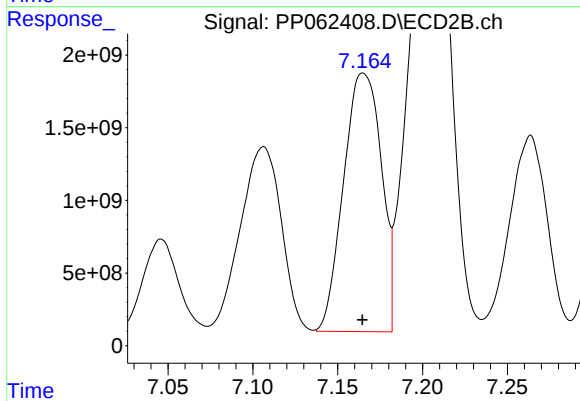

#34 AR-1260-4


R.T.: 7.165 min
Delta R.T.: 0.000 min
Response: 27489743814
Conc: 188125.90 ng/ml

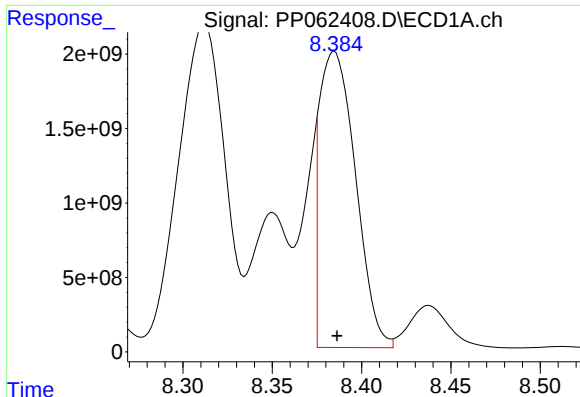

#35 AR-1260-5


R.T.: 8.386 min
Delta R.T.: 0.000 min
Response: 22814106460
Conc: 193910.67 ng

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

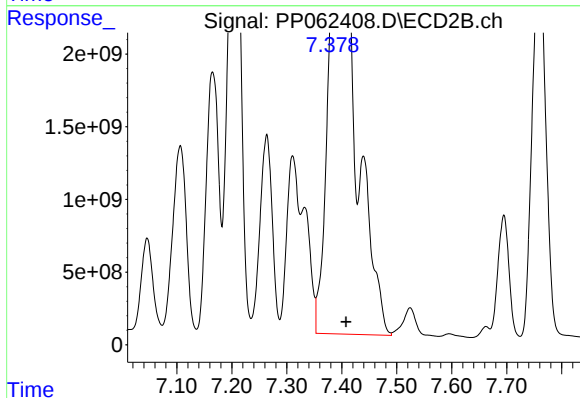


#35 AR-1260-5

R.T.: 7.409 min
Delta R.T.: 0.001 min
Response: 91051074323
Conc: 314773.06 ng/ml

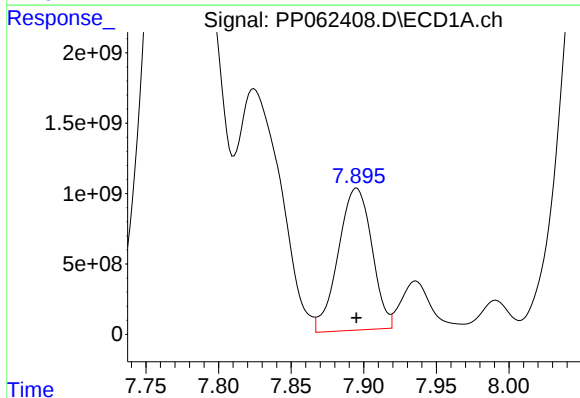


#36 AR-1262-1

R.T.: 7.895 min
Delta R.T.: 0.000 min
Response: 16287090579
Conc: 404670.49 ng/ml

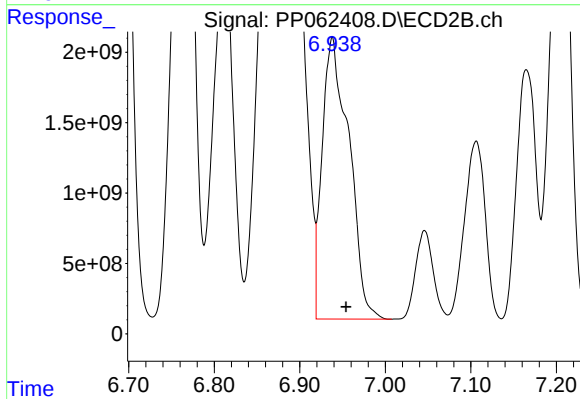

#36 AR-1262-1


R.T.: 6.938 min
Delta R.T.: -0.016 min
Response: 43603206042
Conc: 495970.05 ng/ml

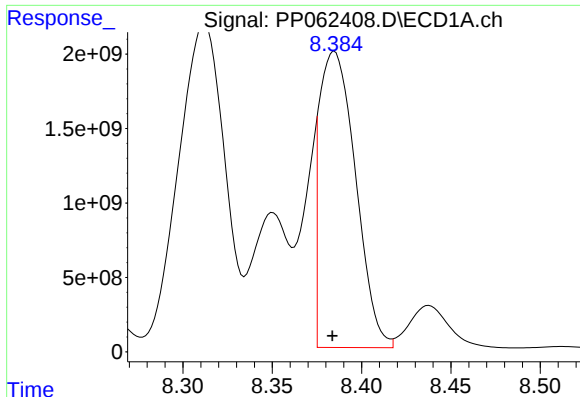

#37 AR-1262-2


R.T.: 8.386 min
Delta R.T.: 0.002 min
Response: 22814106460
Conc: 174772.75 ng

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

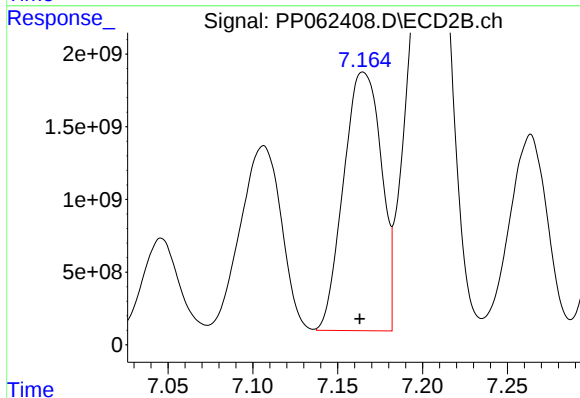


#37 AR-1262-2

R.T.: 7.165 min
Delta R.T.: 0.002 min
Response: 27489743814
Conc: 152096.47 ng/ml

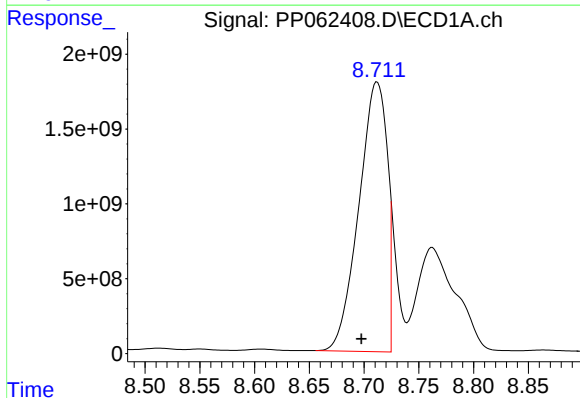


#38 AR-1262-3

R.T.: 8.712 min
Delta R.T.: 0.015 min
Response: 25589385401
Conc: 291949.54 ng/ml

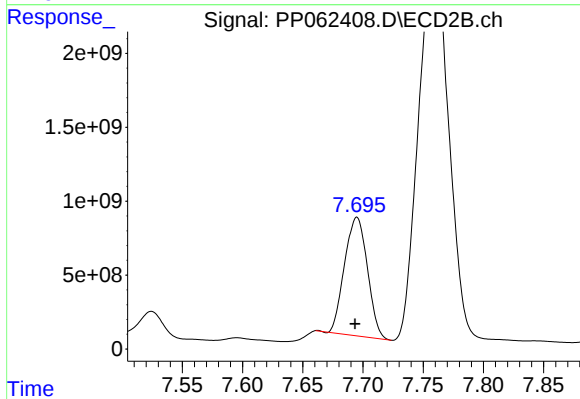

#38 AR-1262-3


R.T.: 7.695 min
Delta R.T.: 0.001 min
Response: 10634406213
Conc: 84892.08 ng/ml

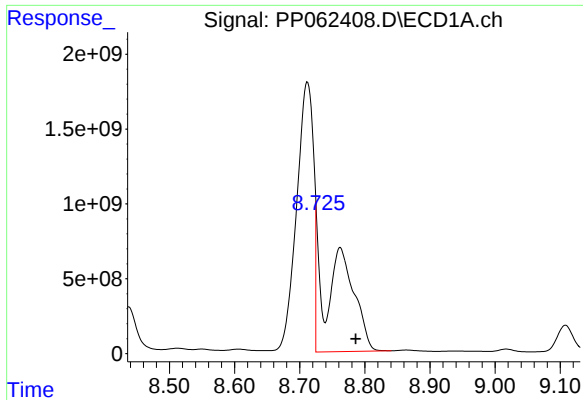

#39 AR-1262-4


R.T.: 8.762 min
Delta R.T.: -0.023 min
Response: 20535536741
Conc: 303000.65 ng

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

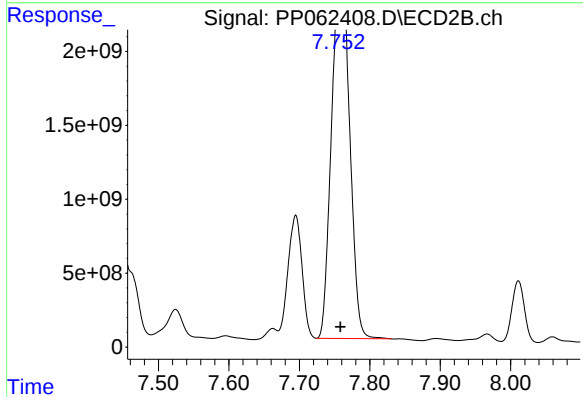


#39 AR-1262-4

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 41801975647
Conc: 177473.85 ng/ml

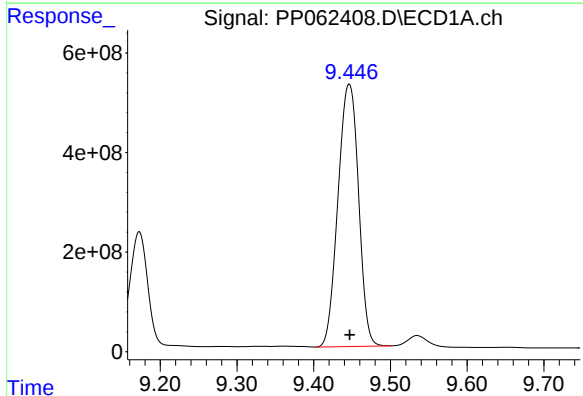


#40 AR-1262-5

R.T.: 9.446 min
Delta R.T.: 0.000 min
Response: 9842874154
Conc: 241784.38 ng/ml

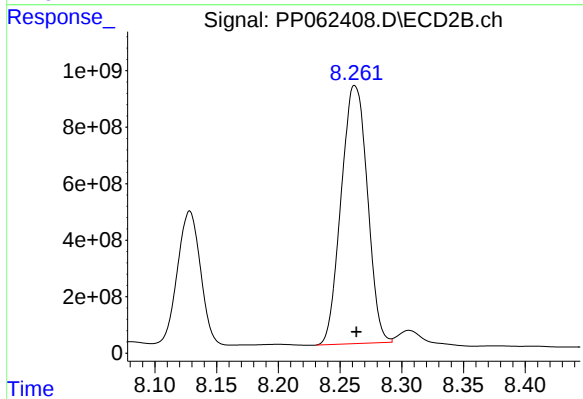

#40 AR-1262-5


R.T.: 8.262 min
Delta R.T.: -0.001 min
Response: 13503798512
Conc: 146070.91 ng/ml

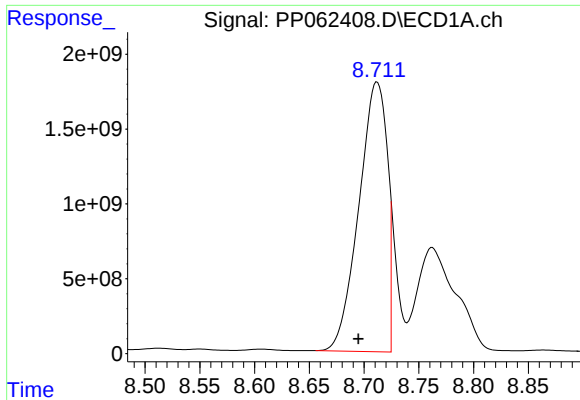

#41 AR-1268-1


R.T.: 8.712 min
Delta R.T.: 0.017 min
Response: 25589385401
Conc: 154736.29 ng

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

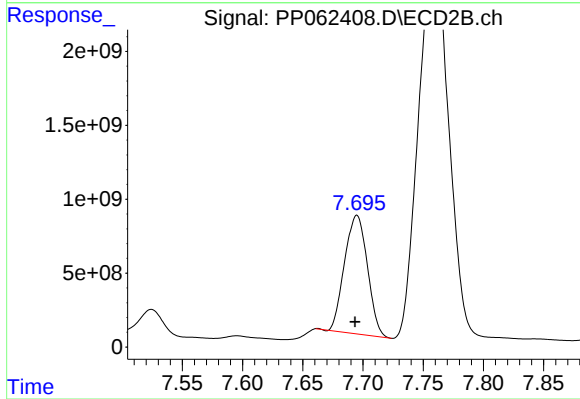


#41 AR-1268-1

R.T.: 7.695 min
Delta R.T.: 0.001 min
Response: 10634406213
Conc: 27076.66 ng/ml

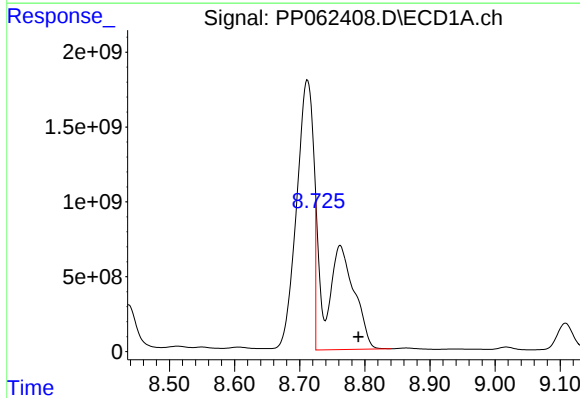


#42 AR-1268-2

R.T.: 8.762 min
Delta R.T.: -0.028 min
Response: 20535536741
Conc: 144198.81 ng/ml

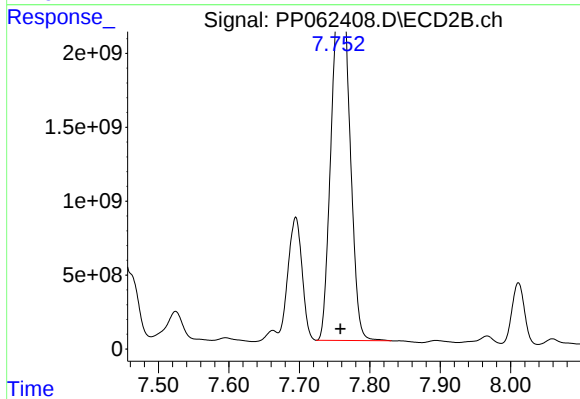

#42 AR-1268-2


R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 41801975647
Conc: 117480.77 ng/ml

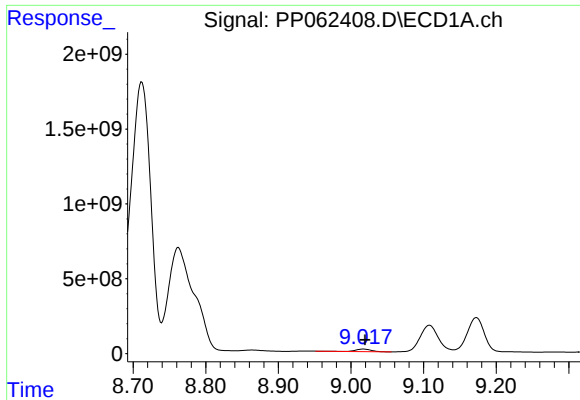

#43 AR-1268-3


R.T.: 9.017 min
Delta R.T.: -0.002 min
Response: 252350596
Conc: 1936.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

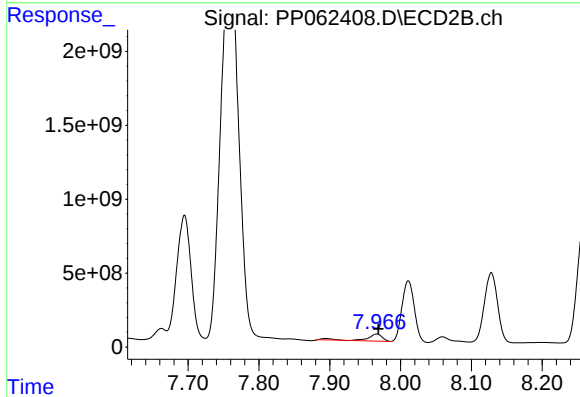


#43 AR-1268-3

R.T.: 7.966 min
Delta R.T.: -0.003 min
Response: 674593974
Conc: 2022.70 ng/ml

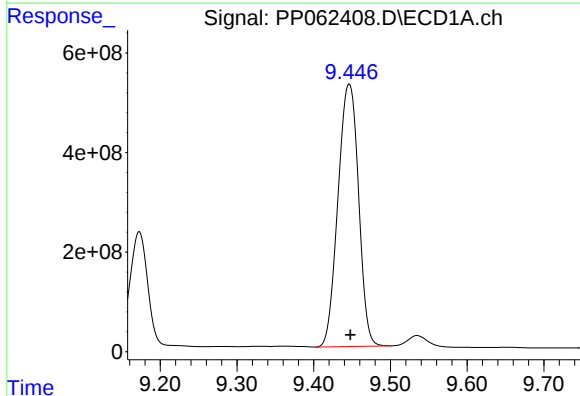


#44 AR-1268-4

R.T.: 9.446 min
Delta R.T.: -0.002 min
Response: 9842874154
Conc: 213909.78 ng/ml

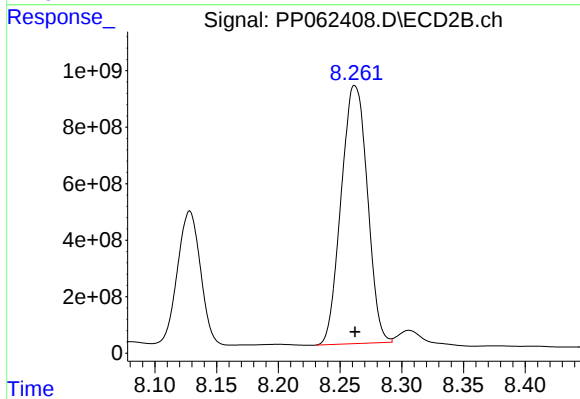

#44 AR-1268-4


R.T.: 8.262 min
Delta R.T.: 0.000 min
Response: 13503798512
Conc: 122455.48 ng/ml

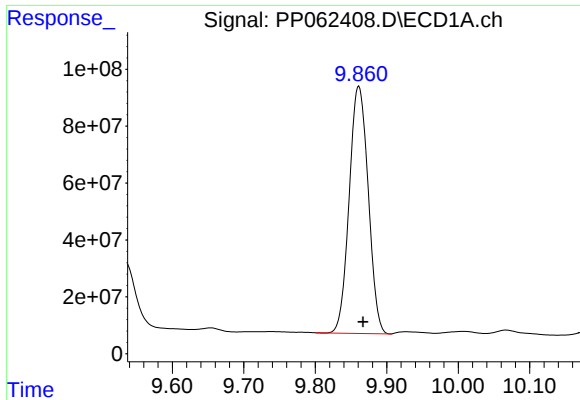

#45 AR-1268-5

R.T.: 9.861 min
Delta R.T.: -0.006 min
Response: 1605896337
Conc: 4109.61 ng/m

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02

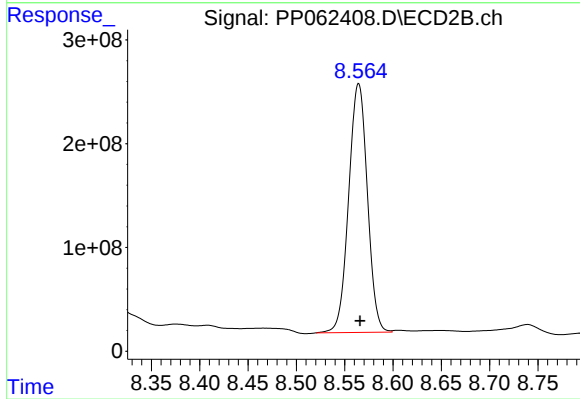

#45 AR-1268-5

R.T.: 8.564 min
Delta R.T.: -0.002 min
Response: 3232824013
Conc: 3758.09 ng/ml