

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121223\
 Data File : PP062435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2023 01:11
 Operator : YP\AJ
 Sample : 05765-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RT-SB-01-10-11

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/13/2023
 Supervised By :Ankita Jodhani 12/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 02:00:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 12 05:13:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.432	3.718	37219255	60869640	22.187	19.835
2) SA Decachlor...	10.202	8.832	25839889	50452300	24.727m	21.907

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121223\
Data File : PP062435.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2023 01:11
Operator : YP\AJ
Sample : 05765-01
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
RT-SB-01-10-11


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/13/2023
Supervised By :Ankita Jodhani 12/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 02:00:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 12 05:13:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

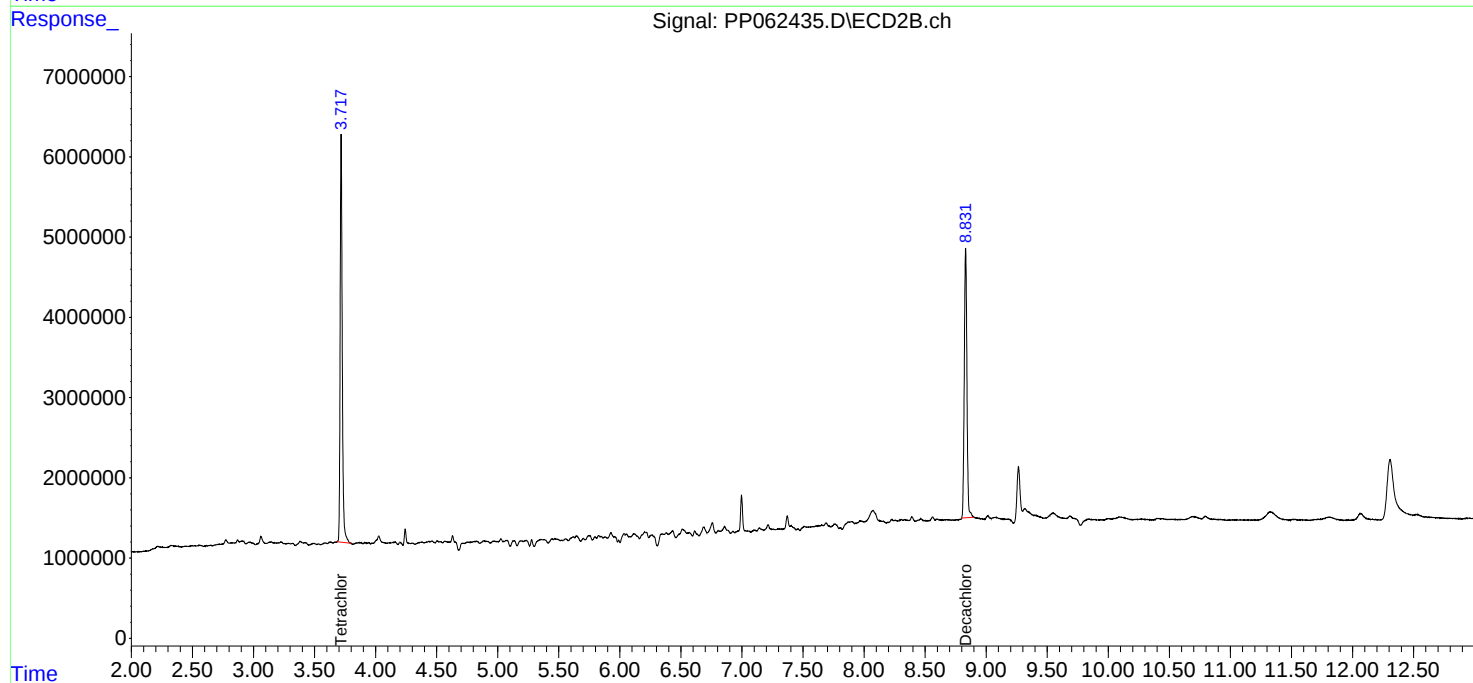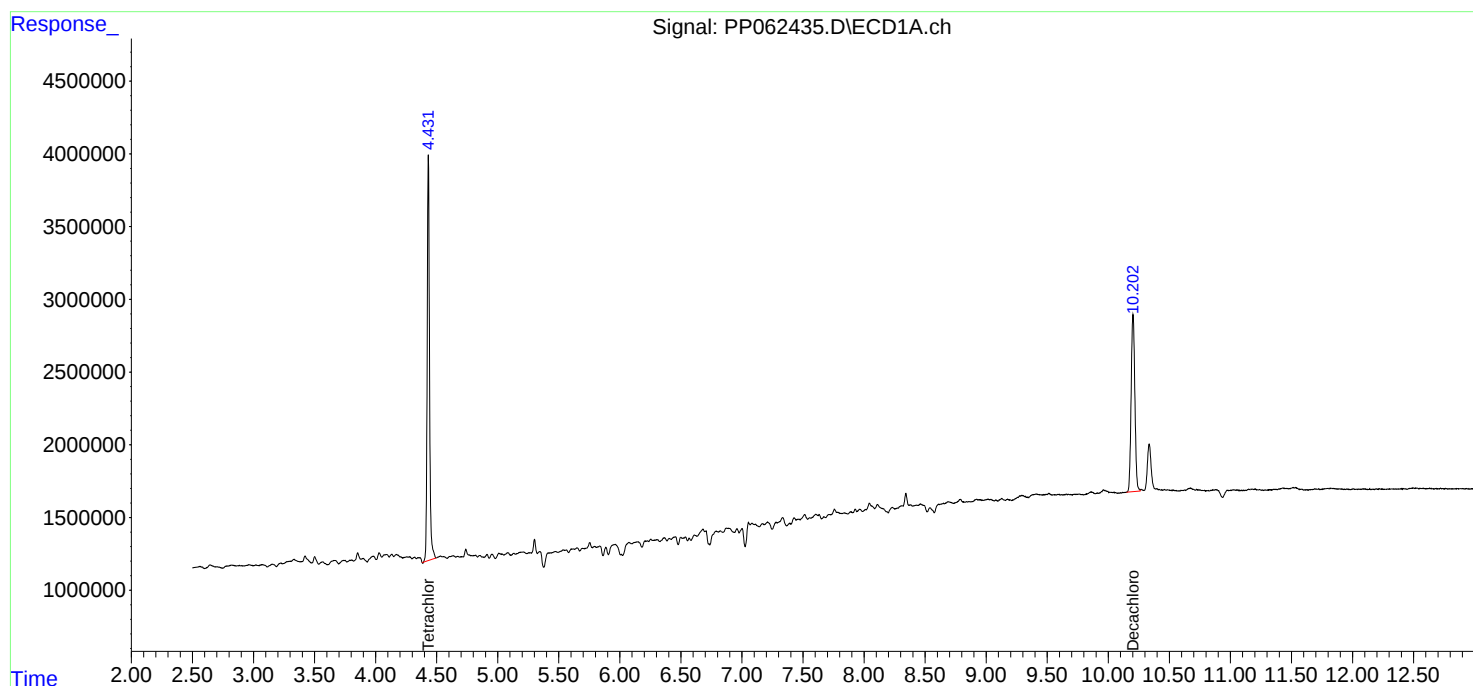

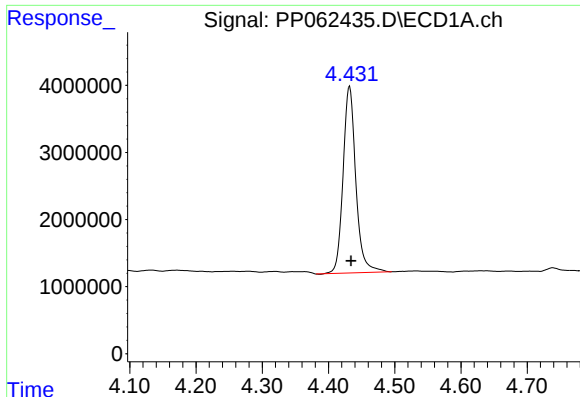


#1 Tetrachloro-m-xylene

R.T.: 4.432 min
Delta R.T.: -0.002 min
Response: 37219255
Conc: 22.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
RT-SB-01-10-11


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/13/2023
Supervised By :Ankita Jodhani 12/13/2023

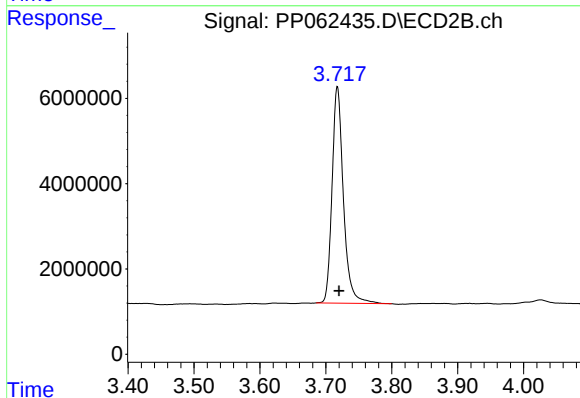


#1 Tetrachloro-m-xylene

R.T.: 3.718 min
Delta R.T.: -0.002 min
Response: 60869640
Conc: 19.84 ng/ml

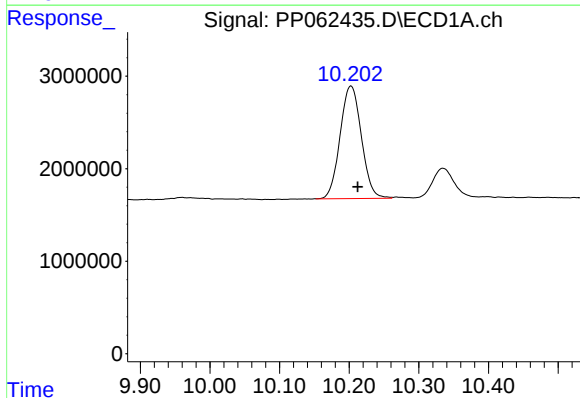

#2 Decachlorobiphenyl

R.T.: 10.202 min
Delta R.T.: -0.010 min
Response: 25839889
Conc: 24.73 ng/ml m

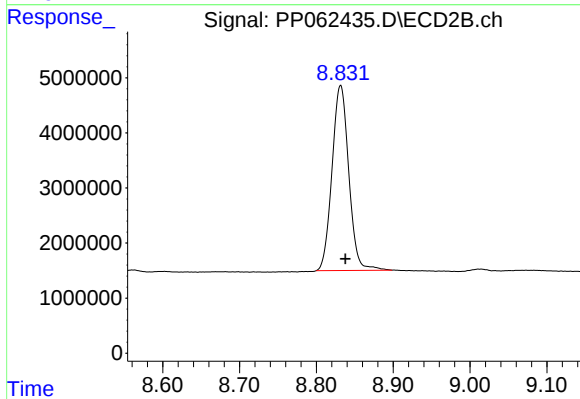

#2 Decachlorobiphenyl

R.T.: 8.832 min
Delta R.T.: -0.006 min
Response: 50452300
Conc: 21.91 ng/ml