

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121318\
Data File : PP028436.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Dec 2018 8:43
Operator : EI\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 14:06:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP120718.M
Quant Title : 8080.M
QLast Update : Fri Dec 07 14:01:32 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
15) T	Picloram	17.691	18.338	18377202	10486514	26.795 N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121318\
Data File : PP028436.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Dec 2018 8:43
Operator : EI\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 14:06:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP120718.M
Quant Title : 8080.M
QLast Update : Fri Dec 07 14:01:32 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

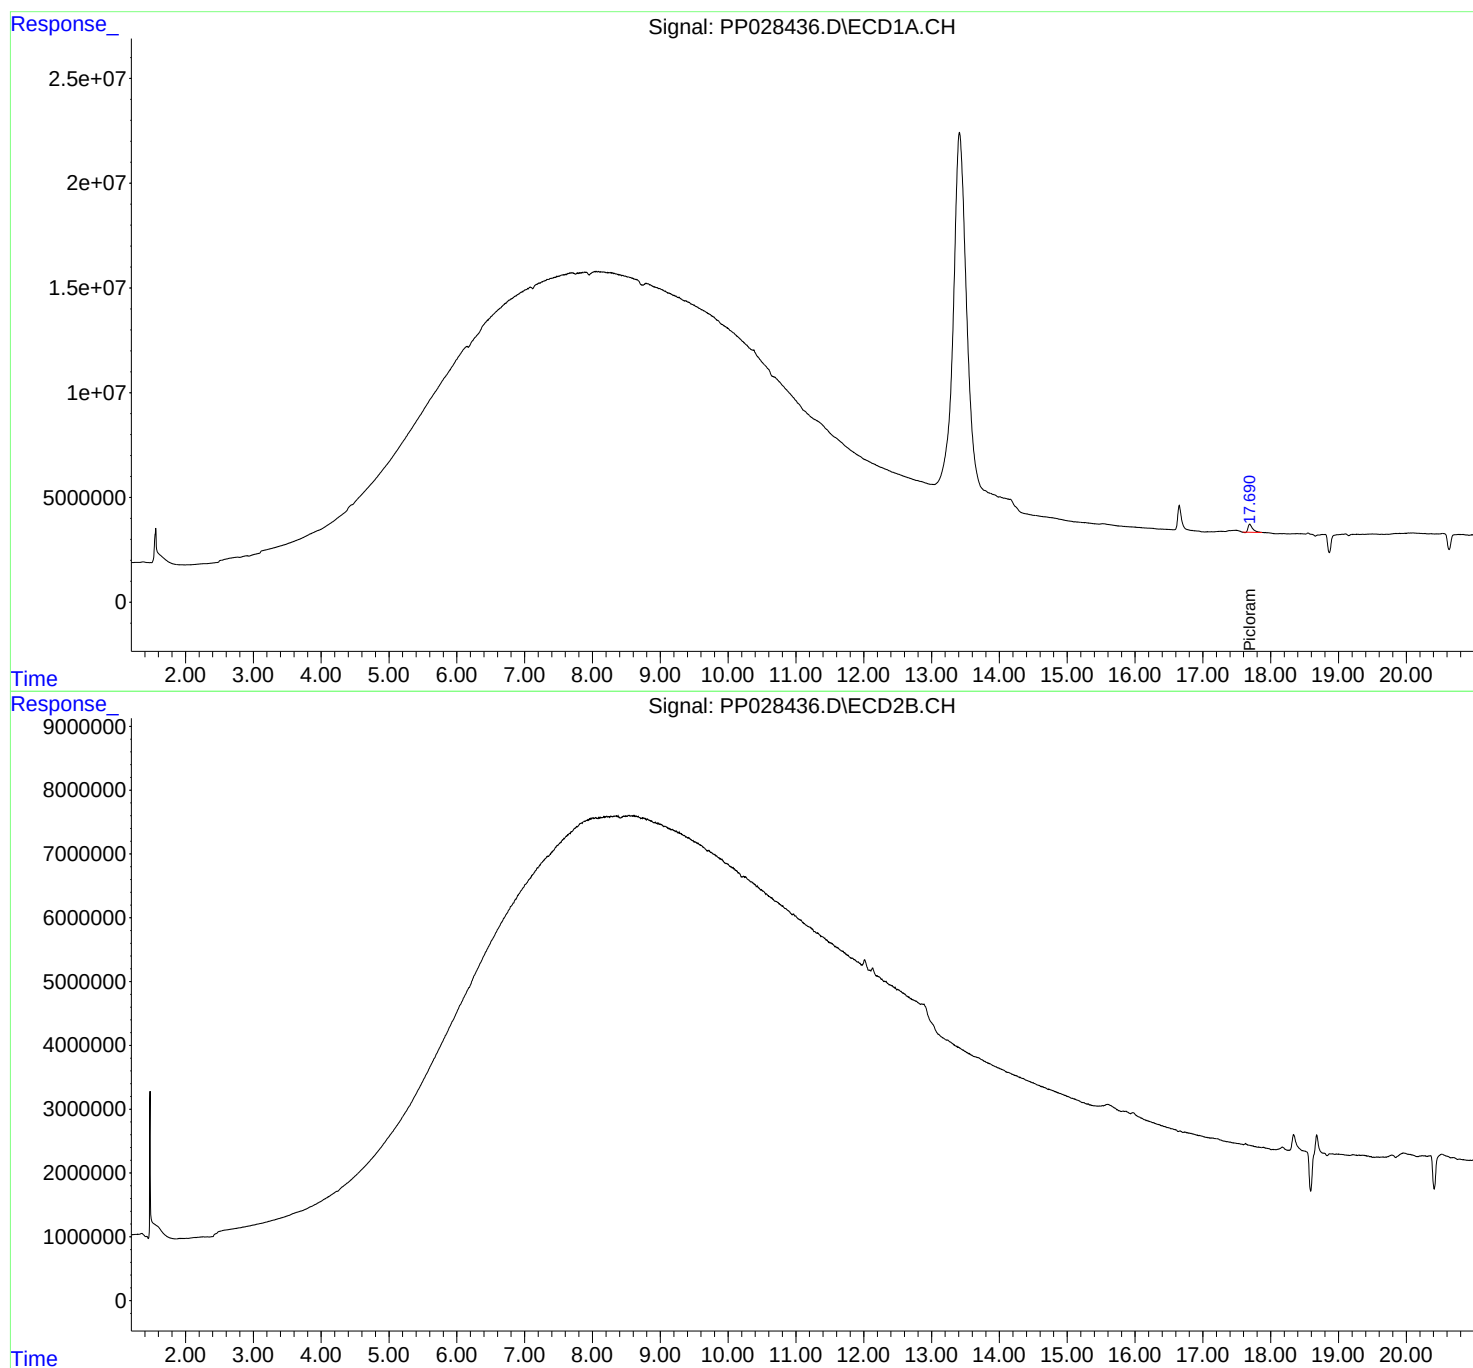


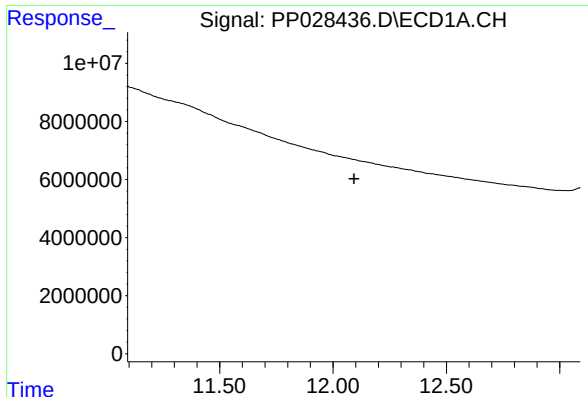

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 12.094 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

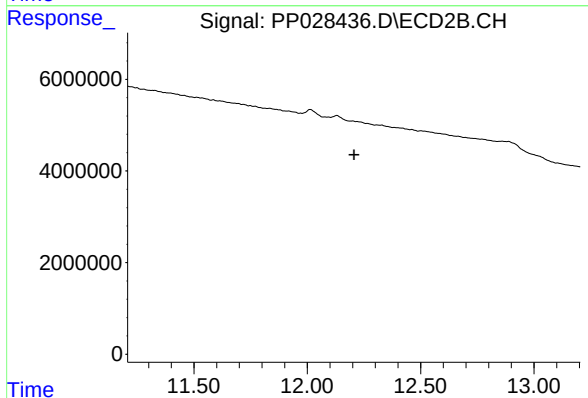


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 12.207 min
Response: 0
Conc: N.D.

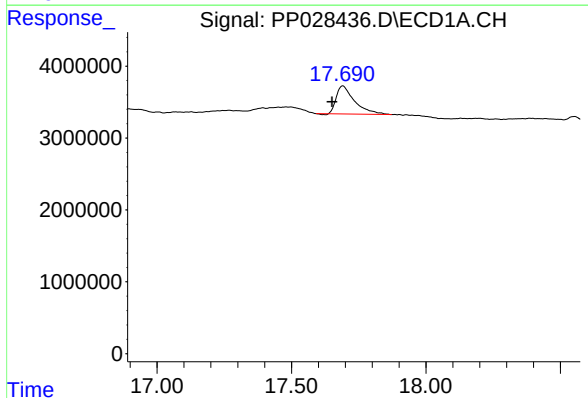

#15 Picloram

R.T.: 17.691 min
Delta R.T.: 0.040 min
Response: 18377202
Conc: 26.79 ng/ml

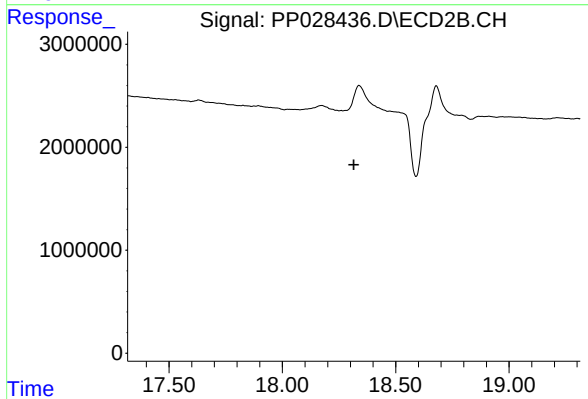

#15 Picloram

R.T.: 18.338 min
Delta R.T.: 0.023 min
Response: 10486514
Conc: N.D.