

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121323\
 Data File : PP062457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2023 11:18
 Operator : YP\AJ
 Sample : 05764-02DL 20000X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-120623-02DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 12:31:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 12 05:13:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

3)	L1	AR-1016-1	5.606	4.828	411794	691017	8.319	7.504
4)	L1	AR-1016-2	5.633	4.846	514995	549933	6.696	4.170 #
5)	L1	AR-1016-3	0.000	5.031	0	148674	N.D.	2.078 #
6)	L1	AR-1016-4	0.000	5.069	0	13497764	N.D.	213.988 #
7)	L1	AR-1016-5	6.084	5.287	5665060	10782036	136.614	130.445
8)	L2	AR-1221-1	0.000	3.936	0	445810	N.D.	12.045 #
9)	L2	AR-1221-2	0.000	4.026	0	284909	N.D.	10.006 #
10)	L2	AR-1221-3	0.000	4.100	0	225112	N.D.	2.754 #
11)	L3	AR-1232-1	0.000	4.100	0	225112	N.D.	3.520 #
12)	L3	AR-1232-2	0.000	4.846	0	549933	N.D.	9.498 #
13)	L3	AR-1232-3	5.633	5.031	514995	148674	15.187	4.719 #
14)	L3	AR-1232-4	0.000	5.111	0	2936506	N.D.	93.278 #
15)	L3	AR-1232-5	5.880	5.287	9780366	10782036	653.091	318.947 #
16)	L4	AR-1242-1	5.606	4.828	411794	691017	9.993	9.208
17)	L4	AR-1242-2	5.633	4.846	514995	549933	8.279	5.151 #
18)	L4	AR-1242-3	0.000	5.031	0	148674	N.D.	2.552 #
19)	L4	AR-1242-4	0.000	5.111	0	2936506	N.D.	46.091 #
20)	L4	AR-1242-5	6.532	5.645	6981522	53809032	196.261	771.708 #
21)	L5	AR-1248-1	5.606	4.828	411794	691017	13.307	12.451
22)	L5	AR-1248-2	5.880	5.069	9780366	13497764	185.761	151.721
23)	L5	AR-1248-3	6.084	5.111	5665060	2936506	99.627	31.605 #
24)	L5	AR-1248-4	6.489	5.287	9583339	10782036	163.898	98.986 #
25)	L5	AR-1248-5	6.532	5.645	6981522	53809032	116.285	387.953 #
26)	L6	AR-1254-1	6.463	5.645	25610252	53809032	377.724	337.402
27)	L6	AR-1254-2	6.683	5.794	42753749	67021780	405.597	473.697
28)	L6	AR-1254-3	7.050	6.204	46525295	88891835	429.738	401.044
29)	L6	AR-1254-4	7.337	6.435	31321124	52382673	487.822	475.152
30)	L6	AR-1254-5	7.756	6.859	42309783	92155761	577.129	496.622
31)	L7	AR-1260-1	7.215	6.336	24614033	60989802	311.486	376.922
32)	L7	AR-1260-2	7.472	6.526	26548091	47656325	310.328	261.587
33)	L7	AR-1260-3	7.817f	6.681	7140730	42566444	107.862	236.509 #
34)	L7	AR-1260-4	8.046f	7.160	16003952	9370255	217.769	64.125 #
35)	L7	AR-1260-5	8.379	7.401	7288334	13359739	61.948	46.186 #
36)	L8	AR-1262-1	7.891	6.951	2210980	14371541	54.934	163.471 #
37)	L8	AR-1262-2	8.379	7.160	7288334	9370255	55.834	51.844
38)	L8	AR-1262-3	8.706	7.692	5681865	1700119	64.824	13.572 #
39)	L8	AR-1262-4	8.757f	7.752	1709705	15818860	25.227	67.160 #
40)	L8	AR-1262-5	9.441	0.000	897831	0	22.055	N.D. #
41)	L9	AR-1268-1	8.706	7.692	5681865	1700119	34.358	4.329 #
42)	L9	AR-1268-2	0.000	7.752	0	15818860	N.D.	44.458 #
43)	L9	AR-1268-3	0.000	7.967	0	16632305	N.D.	49.870 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121323\
 Data File : PP062457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2023 11:18
 Operator : YP\AJ
 Sample : 05764-02DL 20000X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-120623-02DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 12:31:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 12 05:13:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44)	L9 AR-1268-4	9.441	0.000	897831	0	19.512	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121323\
Data File : PP062457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2023 11:18
Operator : YP\AJ
Sample : 05764-02DL 20000X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 12:31:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 12 05:13:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

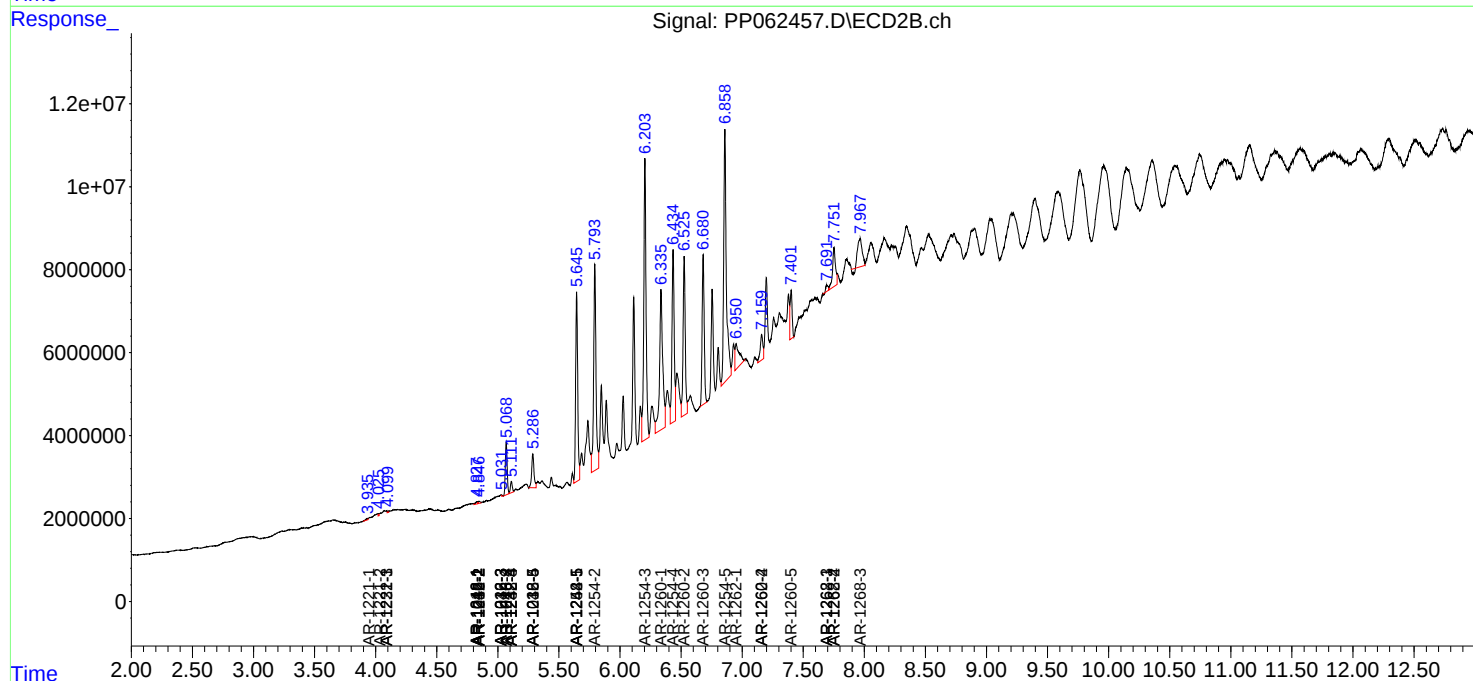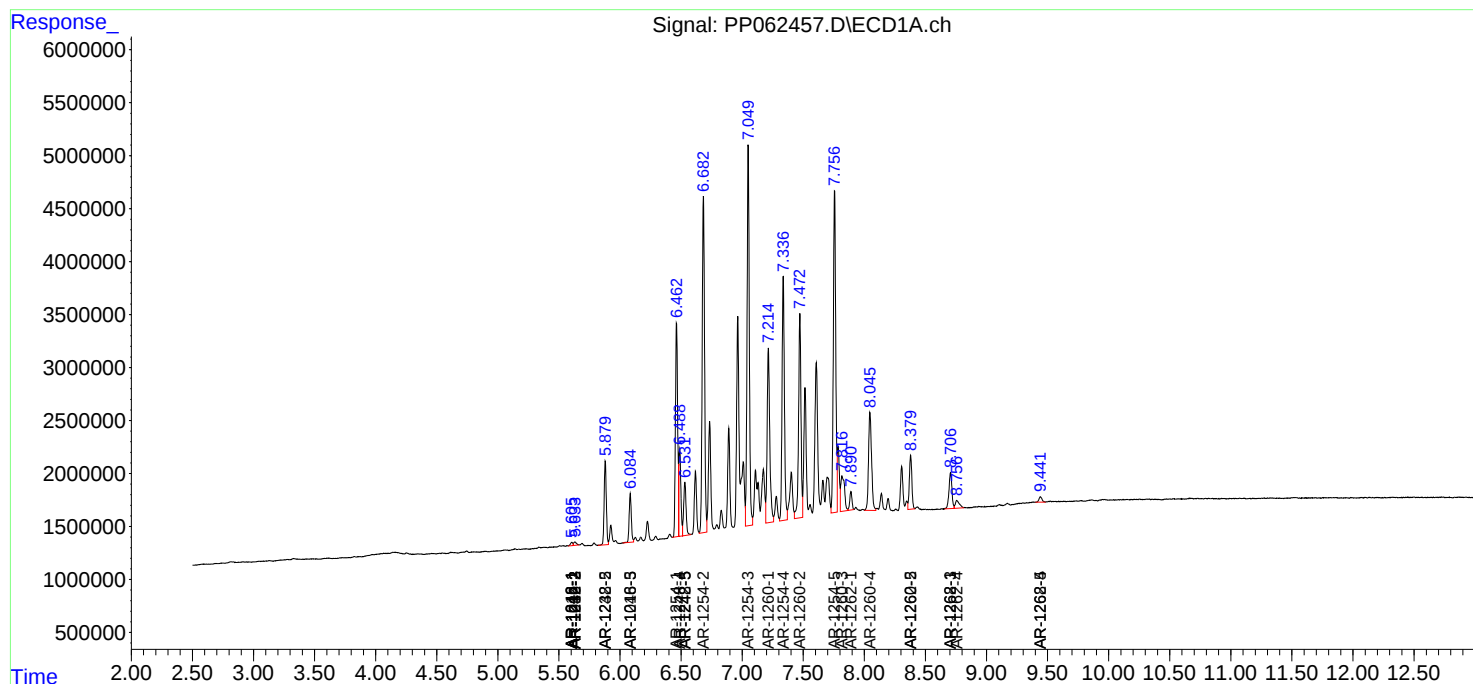


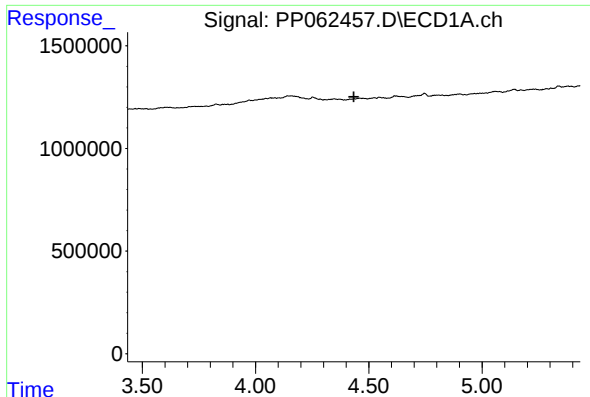

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

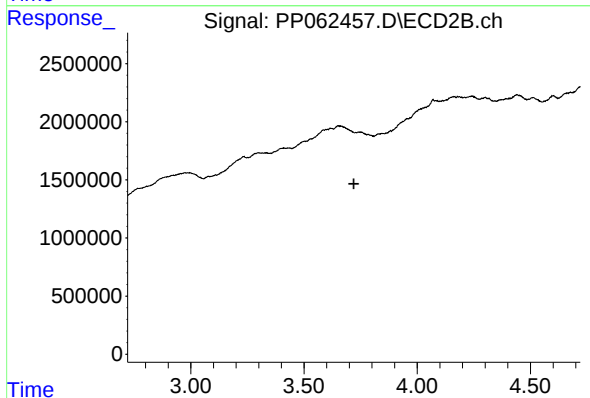


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.720 min
Response: 0
Conc: N.D.

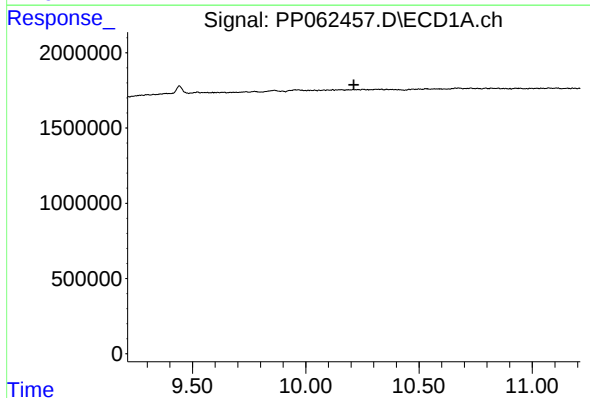


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.212 min
Response: 0
Conc: N.D.

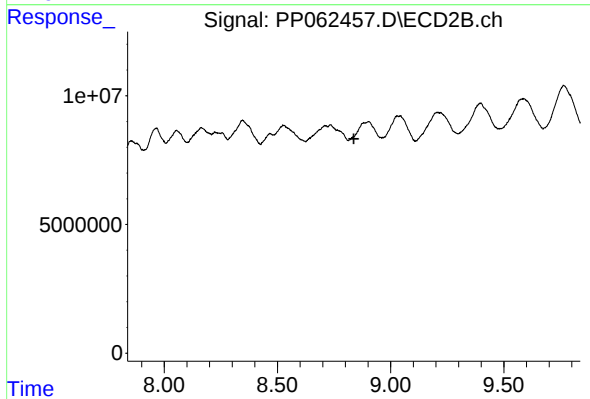

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.838 min
Response: 0
Conc: N.D.

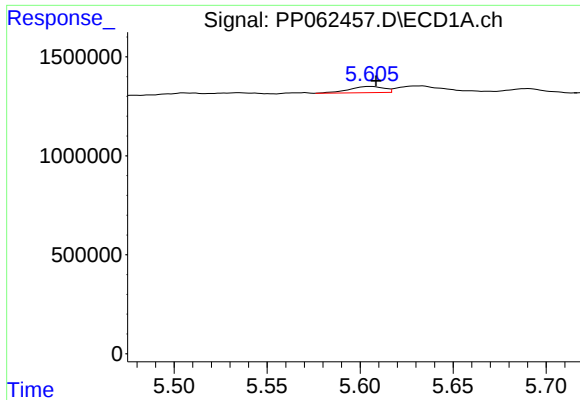

#3 AR-1016-1


R.T.: 5.606 min
Delta R.T.: -0.003 min
Response: 411794
Conc: 8.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

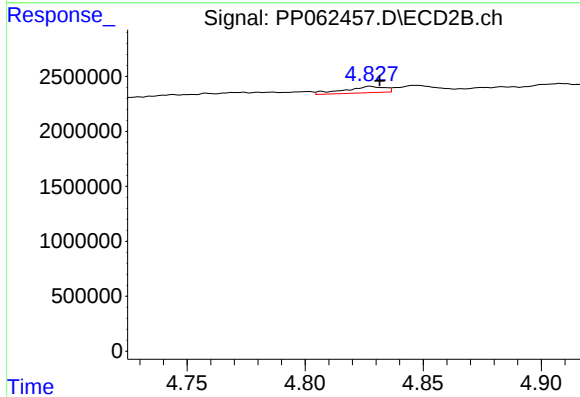


#3 AR-1016-1

R.T.: 4.828 min
Delta R.T.: -0.004 min
Response: 691017
Conc: 7.50 ng/ml

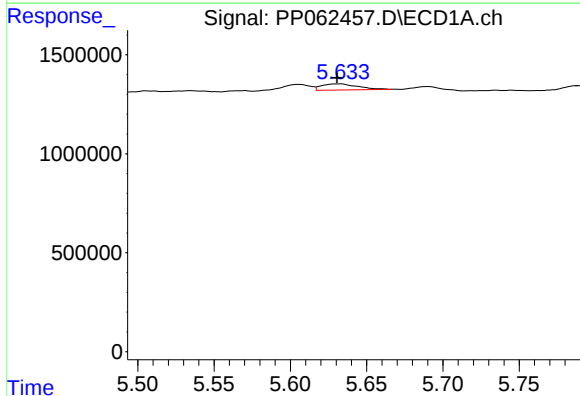


#4 AR-1016-2

R.T.: 5.633 min
Delta R.T.: 0.002 min
Response: 514995
Conc: 6.70 ng/ml

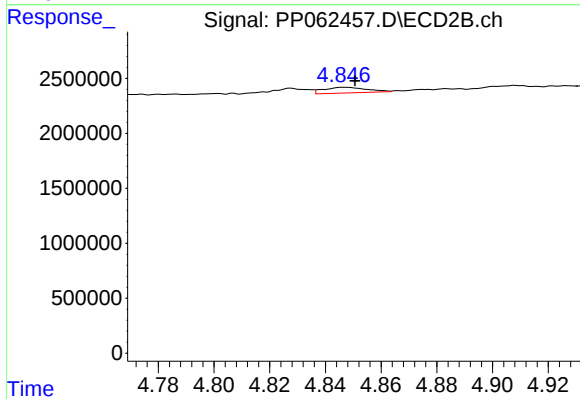

#4 AR-1016-2


R.T.: 4.846 min
Delta R.T.: -0.005 min
Response: 549933
Conc: 4.17 ng/ml

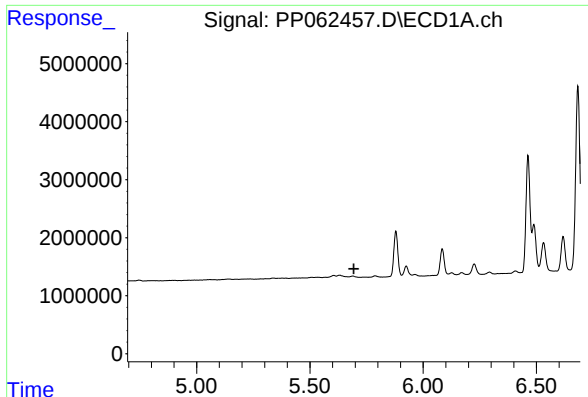

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T.: 5.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

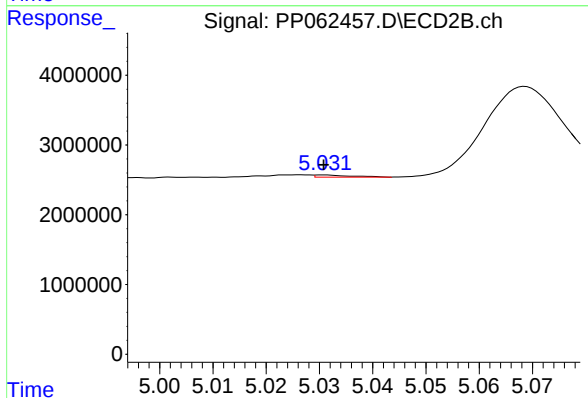


#5 AR-1016-3

R.T.: 5.031 min
Delta R.T.: 0.000 min
Response: 148674
Conc: 2.08 ng/ml

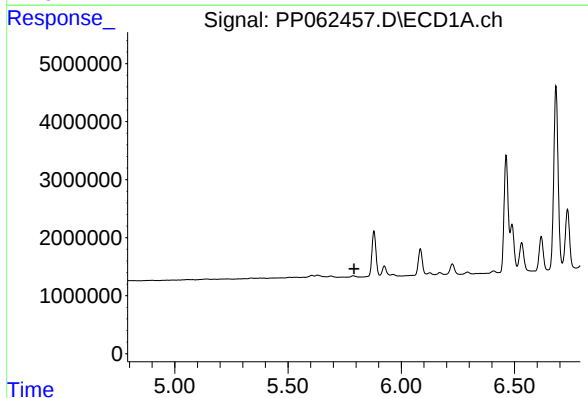


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T.: 5.791 min
Response: 0
Conc: N.D.

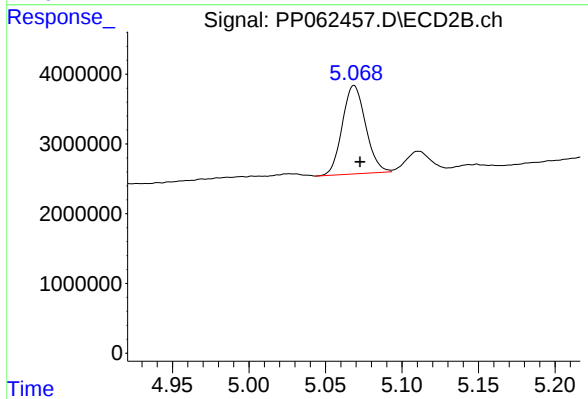

#6 AR-1016-4


R.T.: 5.069 min
Delta R.T.: -0.004 min
Response: 13497764
Conc: 213.99 ng/ml

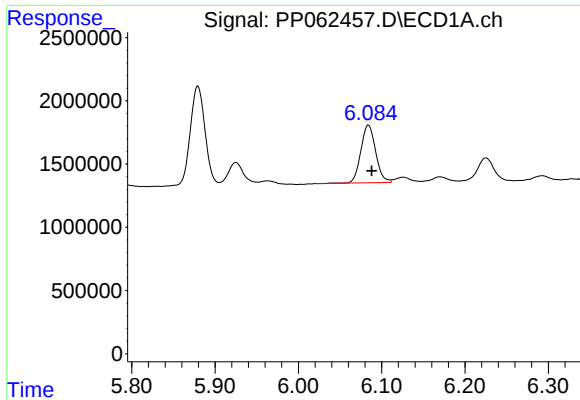

#7 AR-1016-5


R.T.: 6.084 min
Delta R.T.: -0.004 min
Response: 5665060
Conc: 136.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

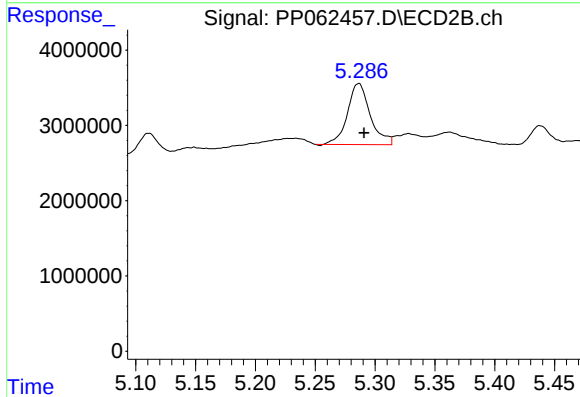


#7 AR-1016-5

R.T.: 5.287 min
Delta R.T.: -0.004 min
Response: 10782036
Conc: 130.45 ng/ml

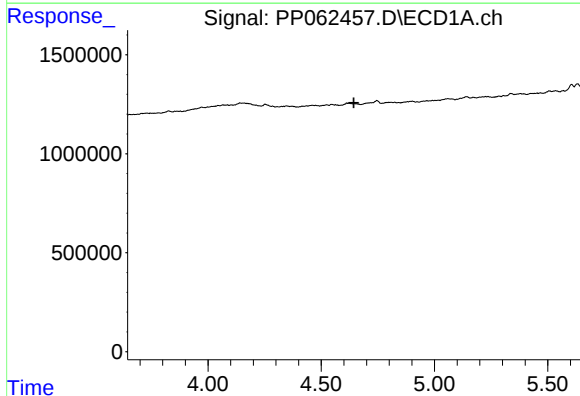


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.644 min
Response: 0
Conc: N.D.

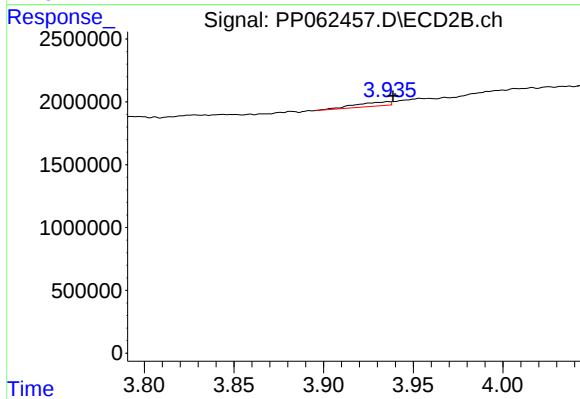

#8 AR-1221-1


R.T.: 3.936 min
Delta R.T.: -0.003 min
Response: 445810
Conc: 12.05 ng/ml

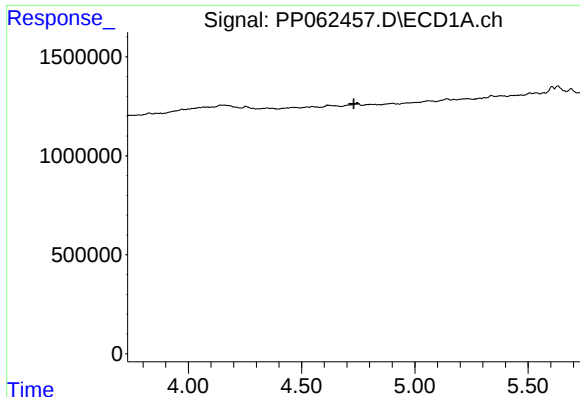

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 4.731 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

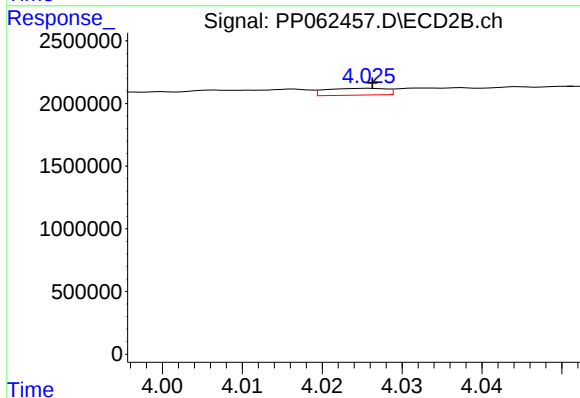


#9 AR-1221-2

R.T.: 4.026 min
Delta R.T.: 0.000 min
Response: 284909
Conc: 10.01 ng/ml

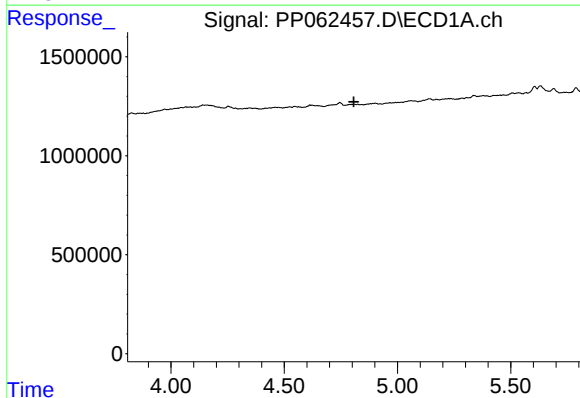


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T.: 4.807 min
Response: 0
Conc: N.D.

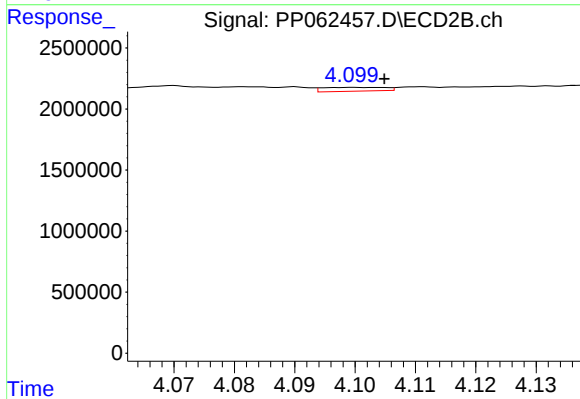

#10 AR-1221-3


R.T.: 4.100 min
Delta R.T.: -0.005 min
Response: 225112
Conc: 2.75 ng/ml

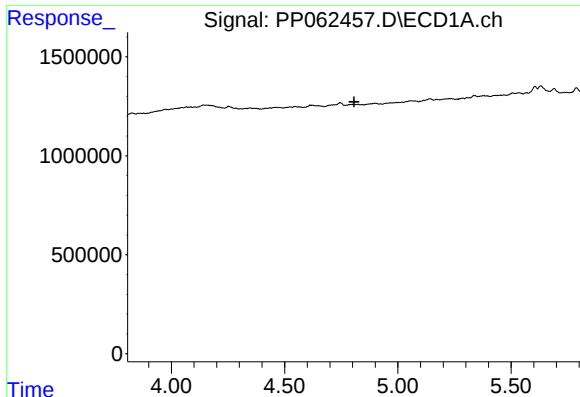

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

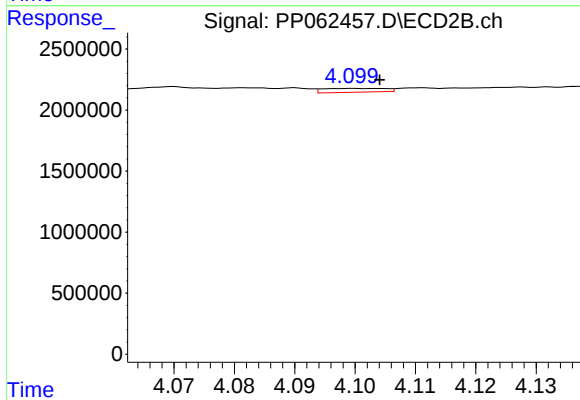


#11 AR-1232-1

R.T.: 4.100 min
Delta R.T.: -0.004 min
Response: 225112
Conc: 3.52 ng/ml

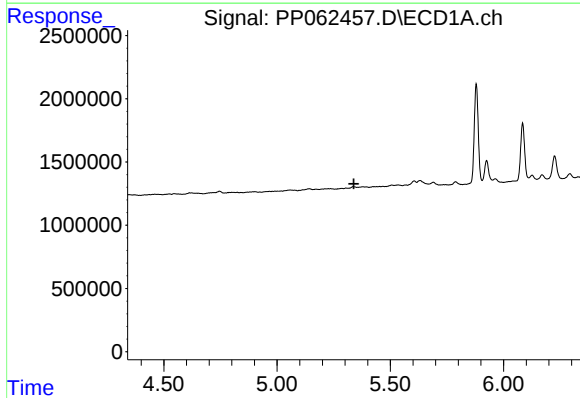


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T.: 5.338 min
Response: 0
Conc: N.D.

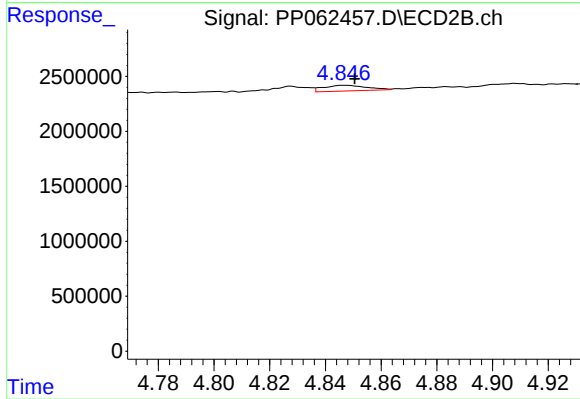

#12 AR-1232-2


R.T.: 4.846 min
Delta R.T.: -0.005 min
Response: 549933
Conc: 9.50 ng/ml

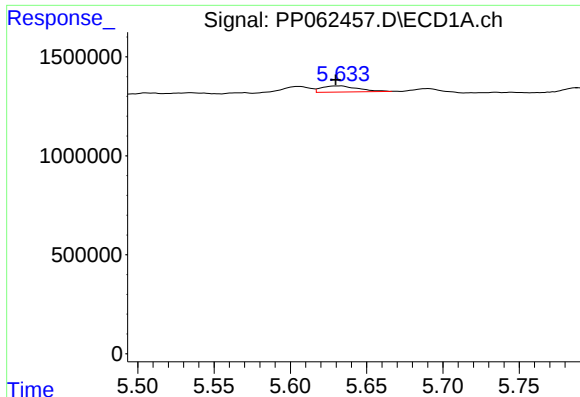

#13 AR-1232-3


R.T.: 5.633 min
Delta R.T.: 0.003 min
Response: 514995
Conc: 15.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

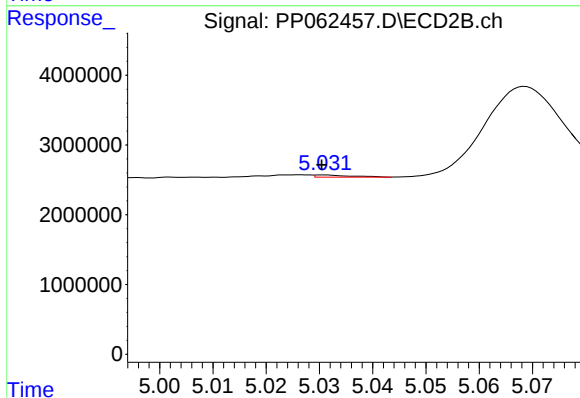


#13 AR-1232-3

R.T.: 5.031 min
Delta R.T.: 0.000 min
Response: 148674
Conc: 4.72 ng/ml

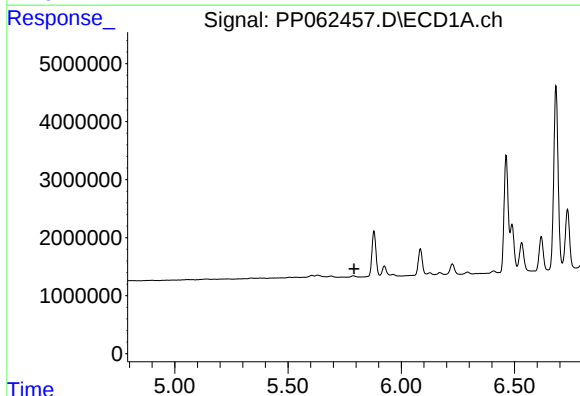


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.791 min
Response: 0
Conc: N.D.

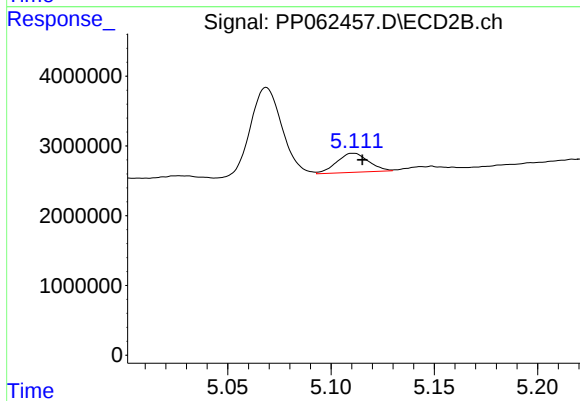

#14 AR-1232-4


R.T.: 5.111 min
Delta R.T.: -0.004 min
Response: 2936506
Conc: 93.28 ng/ml

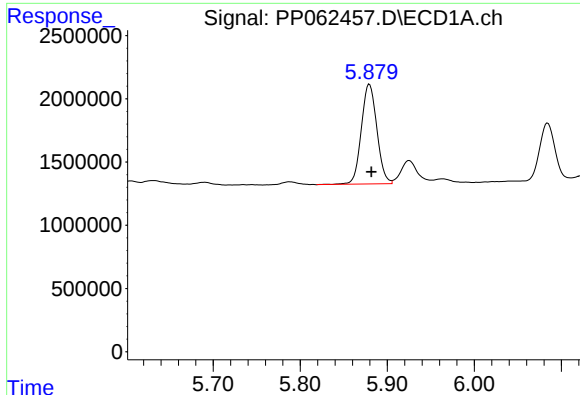

#15 AR-1232-5


R.T.: 5.880 min
Delta R.T.: -0.002 min
Response: 9780366
Conc: 653.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

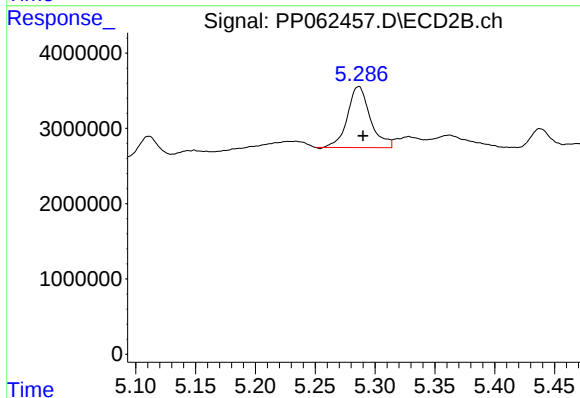


#15 AR-1232-5

R.T.: 5.287 min
Delta R.T.: -0.003 min
Response: 10782036
Conc: 318.95 ng/ml

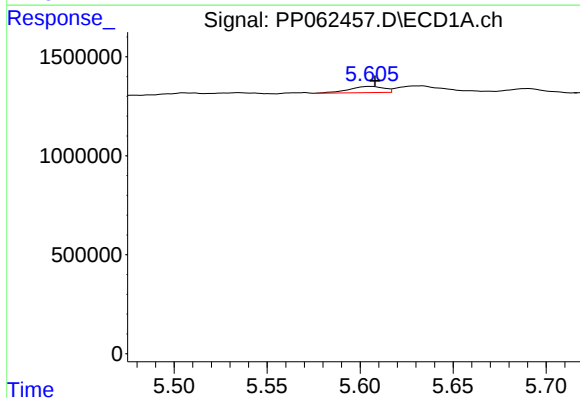


#16 AR-1242-1

R.T.: 5.606 min
Delta R.T.: -0.002 min
Response: 411794
Conc: 9.99 ng/ml

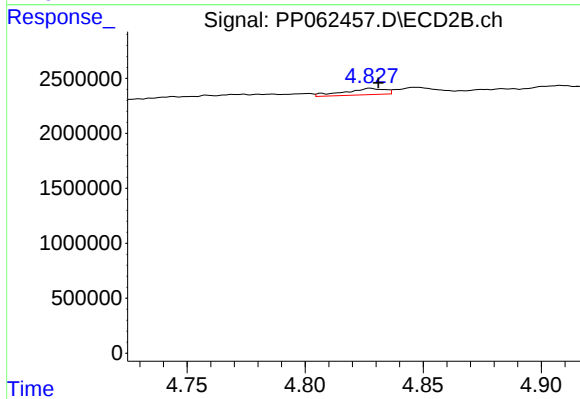

#16 AR-1242-1


R.T.: 4.828 min
Delta R.T.: -0.003 min
Response: 691017
Conc: 9.21 ng/ml

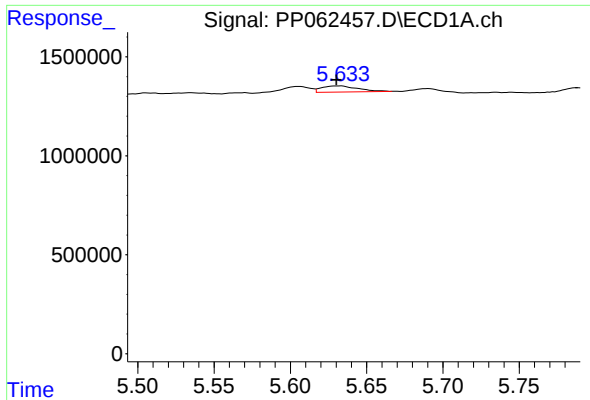

#17 AR-1242-2


R.T.: 5.633 min
Delta R.T.: 0.003 min
Response: 514995
Conc: 8.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

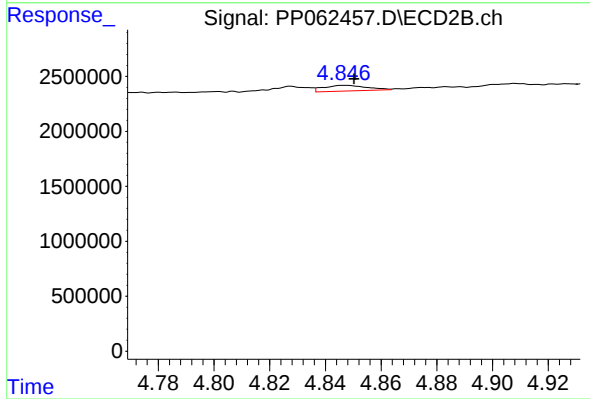


#17 AR-1242-2

R.T.: 4.846 min
Delta R.T.: -0.004 min
Response: 549933
Conc: 5.15 ng/ml

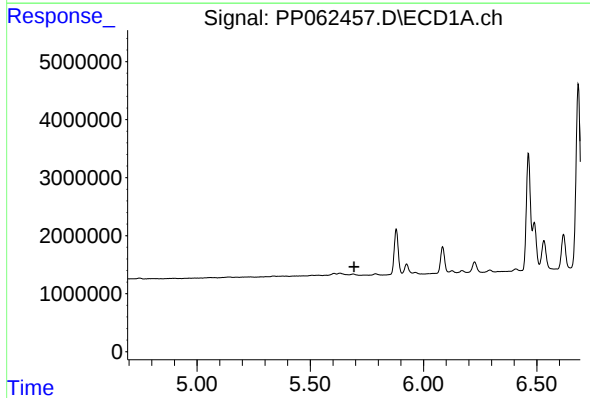


#18 AR-1242-3

R.T.: 0.000 min
Exp R.T. : 5.693 min
Response: 0
Conc: N.D.

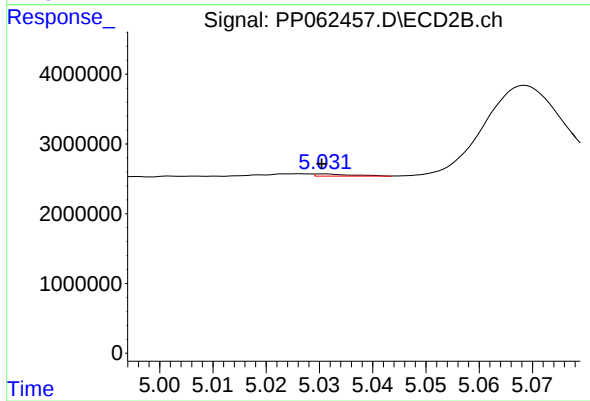

#18 AR-1242-3


R.T.: 5.031 min
Delta R.T.: 0.000 min
Response: 148674
Conc: 2.55 ng/ml

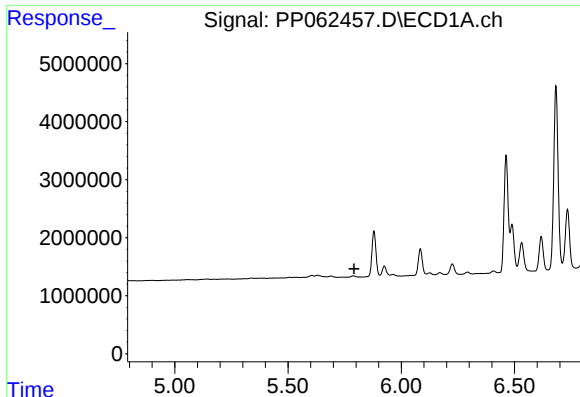

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.791 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

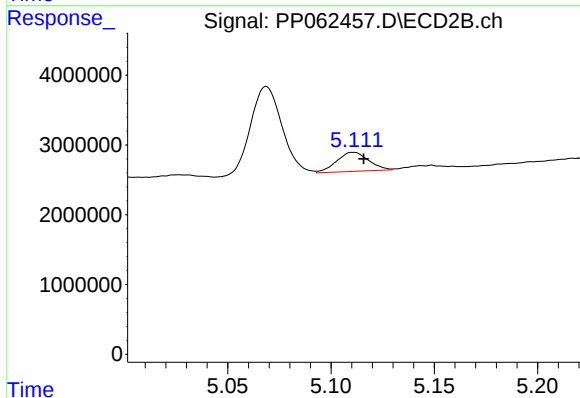


#19 AR-1242-4

R.T.: 5.111 min
Delta R.T.: -0.005 min
Response: 2936506
Conc: 46.09 ng/ml

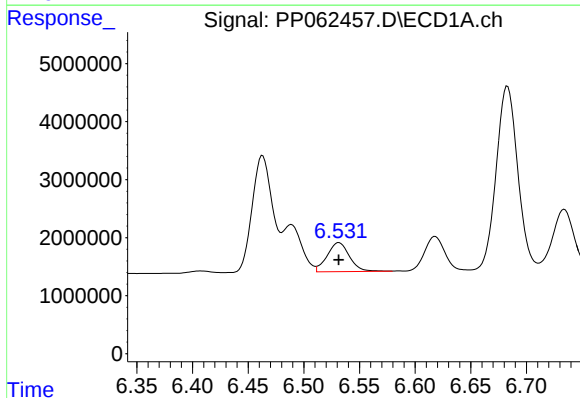


#20 AR-1242-5

R.T.: 6.532 min
Delta R.T.: 0.000 min
Response: 6981522
Conc: 196.26 ng/ml

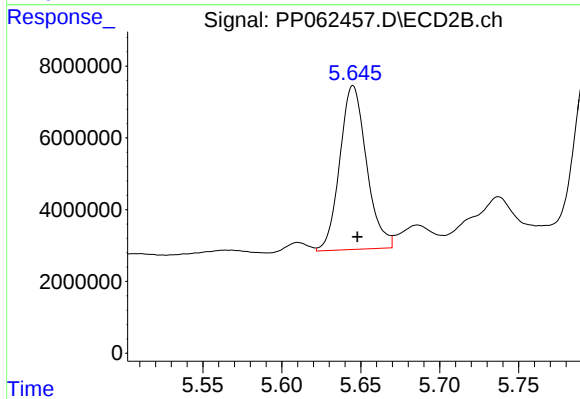

#20 AR-1242-5


R.T.: 5.645 min
Delta R.T.: -0.003 min
Response: 53809032
Conc: 771.71 ng/ml

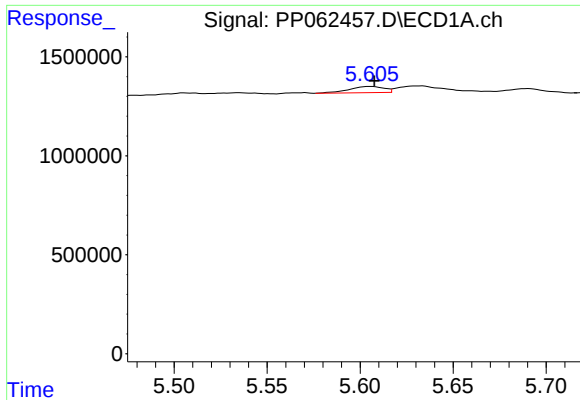

#21 AR-1248-1


R.T.: 5.606 min
Delta R.T.: -0.002 min
Response: 411794
Conc: 13.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

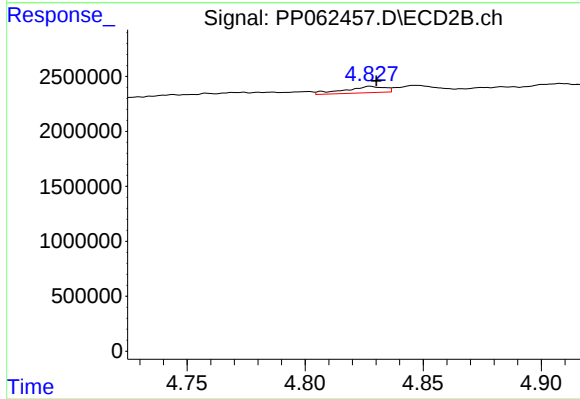


#21 AR-1248-1

R.T.: 4.828 min
Delta R.T.: -0.003 min
Response: 691017
Conc: 12.45 ng/ml

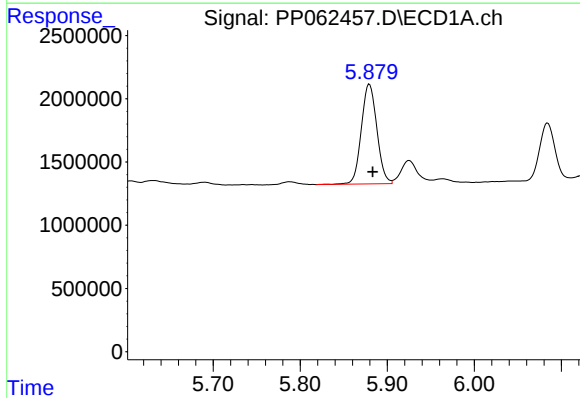


#22 AR-1248-2

R.T.: 5.880 min
Delta R.T.: -0.004 min
Response: 9780366
Conc: 185.76 ng/ml

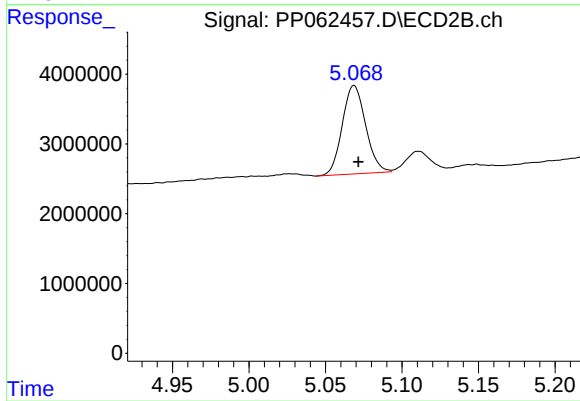

#22 AR-1248-2


R.T.: 5.069 min
Delta R.T.: -0.003 min
Response: 13497764
Conc: 151.72 ng/ml

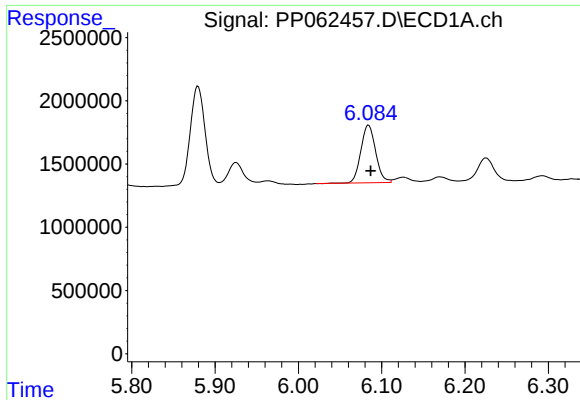

#23 AR-1248-3


R.T.: 6.084 min
Delta R.T.: -0.003 min
Response: 5665060
Conc: 99.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

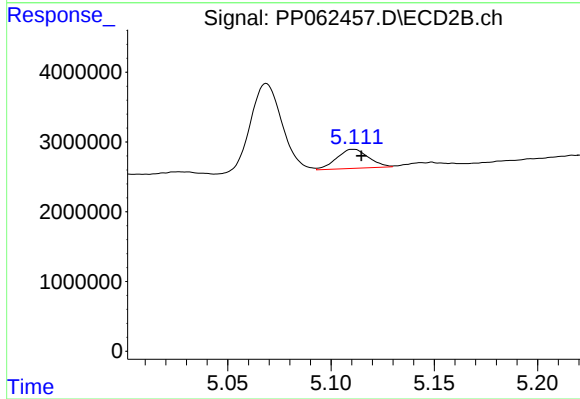


#23 AR-1248-3

R.T.: 5.111 min
Delta R.T.: -0.004 min
Response: 2936506
Conc: 31.60 ng/ml

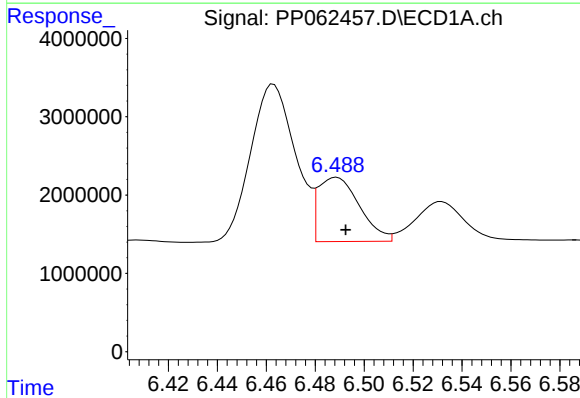


#24 AR-1248-4

R.T.: 6.489 min
Delta R.T.: -0.004 min
Response: 9583339
Conc: 163.90 ng/ml

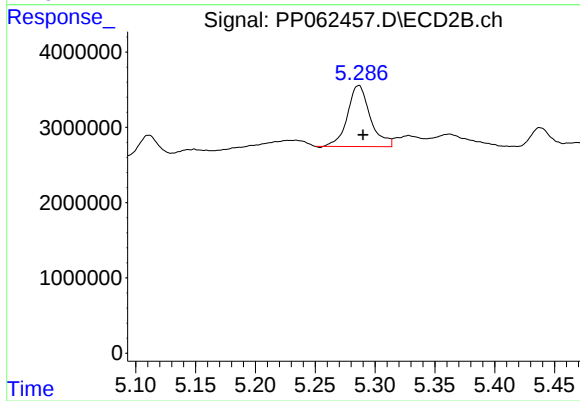

#24 AR-1248-4


R.T.: 5.287 min
Delta R.T.: -0.003 min
Response: 10782036
Conc: 98.99 ng/ml

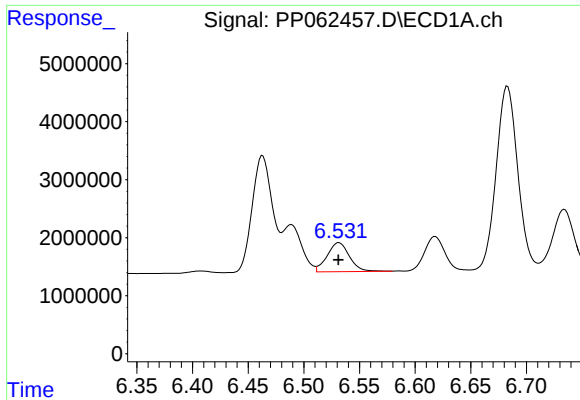

#25 AR-1248-5


R.T.: 6.532 min
Delta R.T.: 0.000 min
Response: 6981522
Conc: 116.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

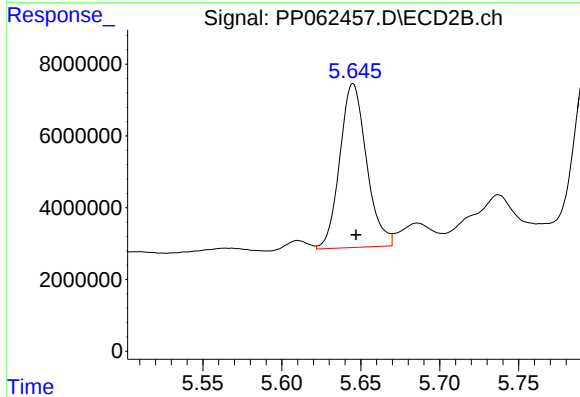


#25 AR-1248-5

R.T.: 5.645 min
Delta R.T.: -0.002 min
Response: 53809032
Conc: 387.95 ng/ml

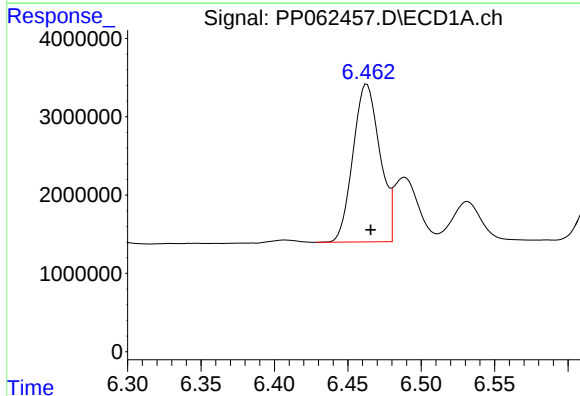


#26 AR-1254-1

R.T.: 6.463 min
Delta R.T.: -0.003 min
Response: 25610252
Conc: 377.72 ng/ml

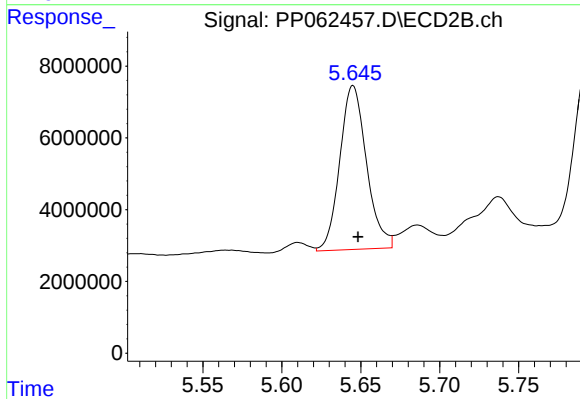

#26 AR-1254-1


R.T.: 5.645 min
Delta R.T.: -0.003 min
Response: 53809032
Conc: 337.40 ng/ml

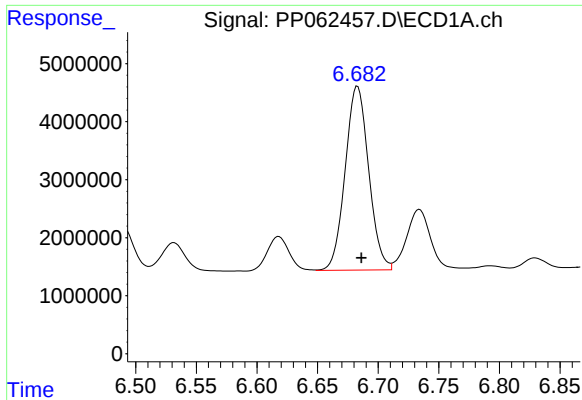

#27 AR-1254-2


R.T.: 6.683 min
Delta R.T.: -0.003 min
Response: 42753749
Conc: 405.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

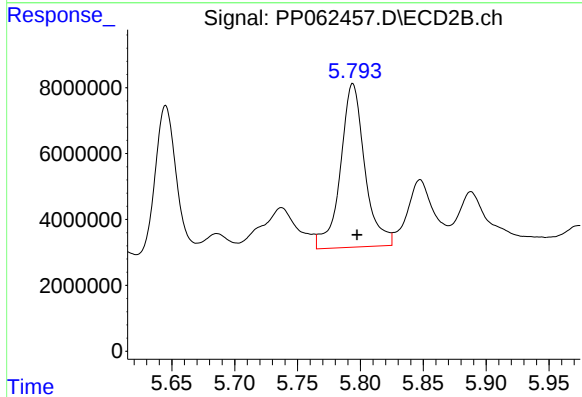


#27 AR-1254-2

R.T.: 5.794 min
Delta R.T.: -0.004 min
Response: 67021780
Conc: 473.70 ng/ml

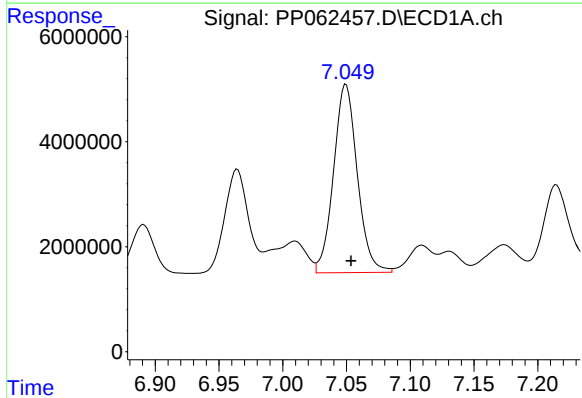


#28 AR-1254-3

R.T.: 7.050 min
Delta R.T.: -0.004 min
Response: 46525295
Conc: 429.74 ng/ml

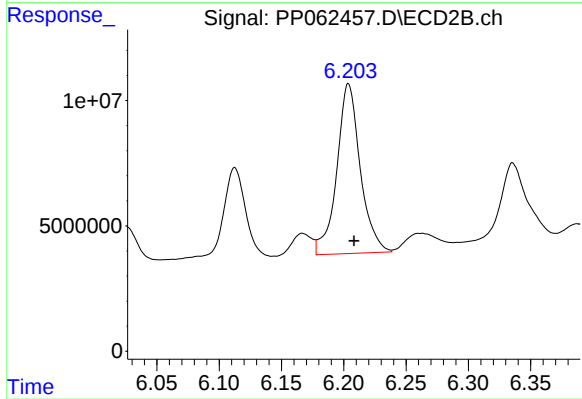

#28 AR-1254-3


R.T.: 6.204 min
Delta R.T.: -0.005 min
Response: 88891835
Conc: 401.04 ng/ml

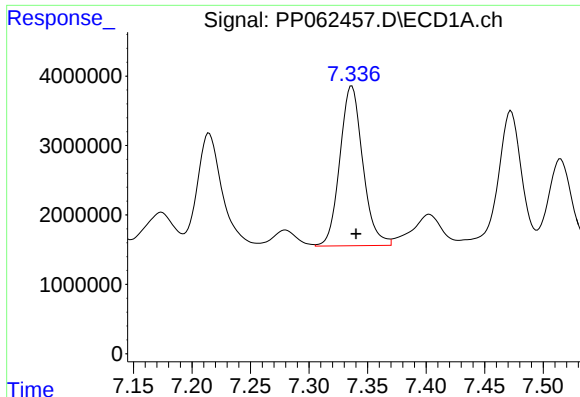

#29 AR-1254-4


R.T.: 7.337 min
Delta R.T.: -0.004 min
Response: 31321124
Conc: 487.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

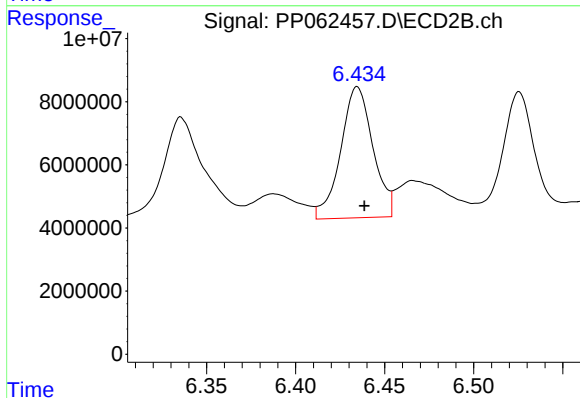


#29 AR-1254-4

R.T.: 6.435 min
Delta R.T.: -0.004 min
Response: 52382673
Conc: 475.15 ng/ml

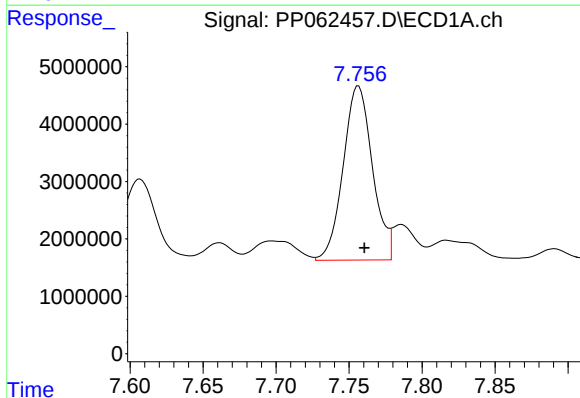


#30 AR-1254-5

R.T.: 7.756 min
Delta R.T.: -0.004 min
Response: 42309783
Conc: 577.13 ng/ml

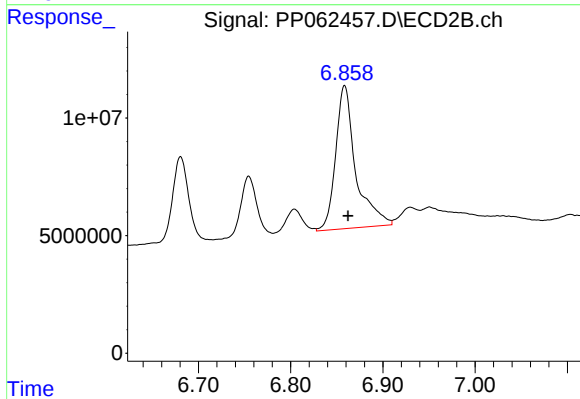

#30 AR-1254-5


R.T.: 6.859 min
Delta R.T.: -0.004 min
Response: 92155761
Conc: 496.62 ng/ml

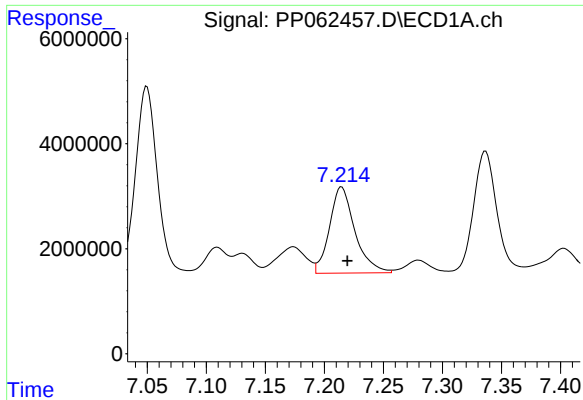

#31 AR-1260-1


R.T.: 7.215 min
Delta R.T.: -0.005 min
Response: 24614033
Conc: 311.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

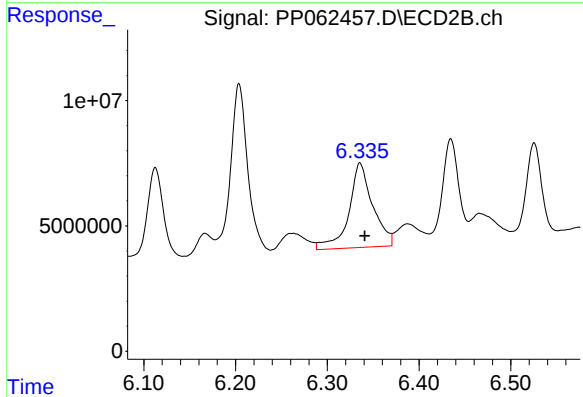


#31 AR-1260-1

R.T.: 6.336 min
Delta R.T.: -0.005 min
Response: 60989802
Conc: 376.92 ng/ml

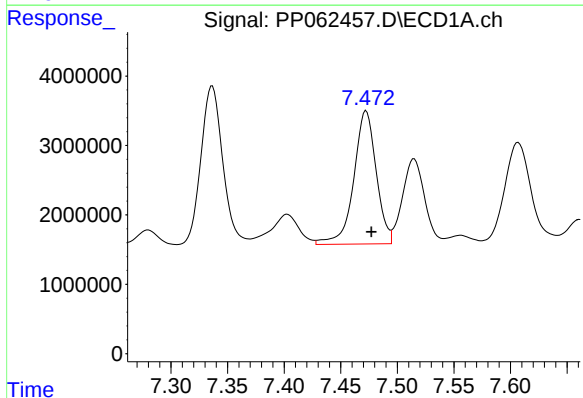


#32 AR-1260-2

R.T.: 7.472 min
Delta R.T.: -0.005 min
Response: 26548091
Conc: 310.33 ng/ml

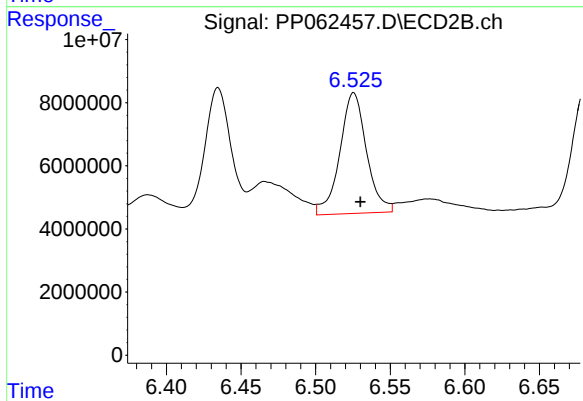

#32 AR-1260-2


R.T.: 6.526 min
Delta R.T.: -0.004 min
Response: 47656325
Conc: 261.59 ng/ml

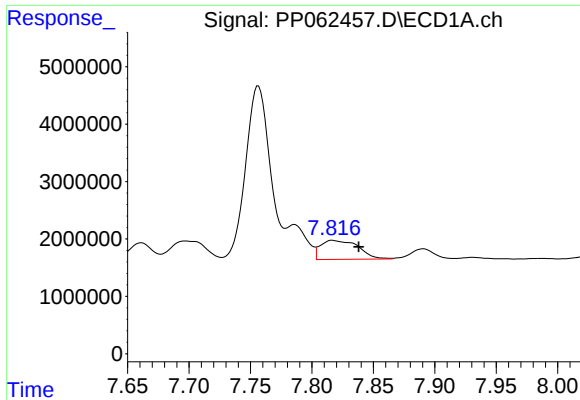

#33 AR-1260-3


R.T.: 7.817 min
Delta R.T.: -0.022 min
Response: 7140730
Conc: 107.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

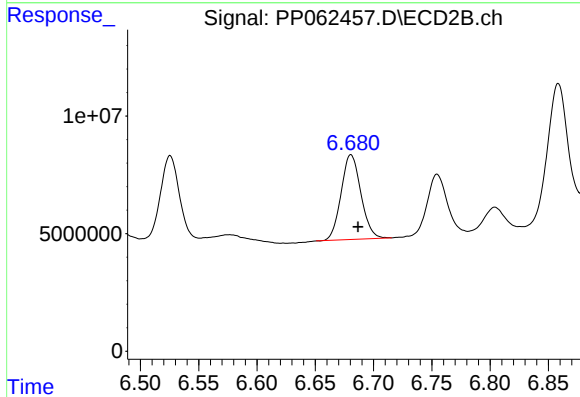


#33 AR-1260-3

R.T.: 6.681 min
Delta R.T.: -0.006 min
Response: 42566444
Conc: 236.51 ng/ml

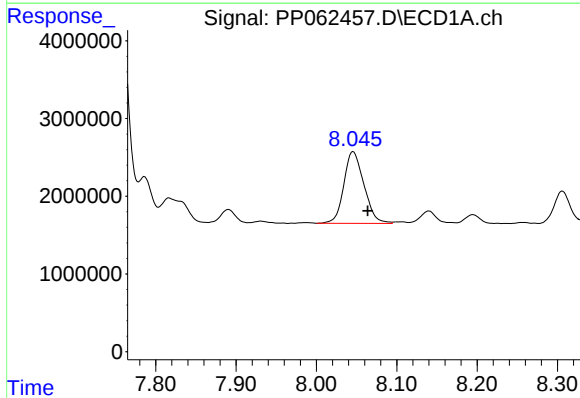


#34 AR-1260-4

R.T.: 8.046 min
Delta R.T.: -0.018 min
Response: 16003952
Conc: 217.77 ng/ml

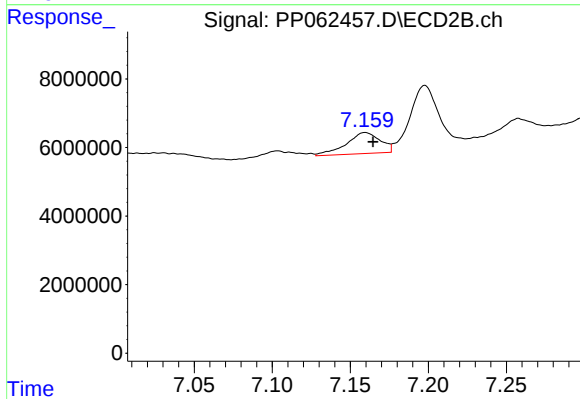

#34 AR-1260-4


R.T.: 7.160 min
Delta R.T.: -0.005 min
Response: 9370255
Conc: 64.13 ng/ml

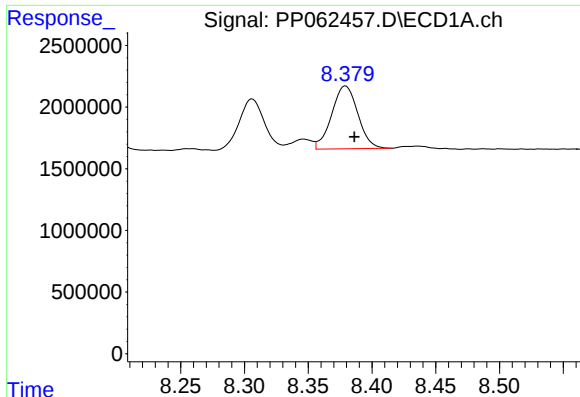

#35 AR-1260-5


R.T.: 8.379 min
Delta R.T.: -0.007 min
Response: 7288334
Conc: 61.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

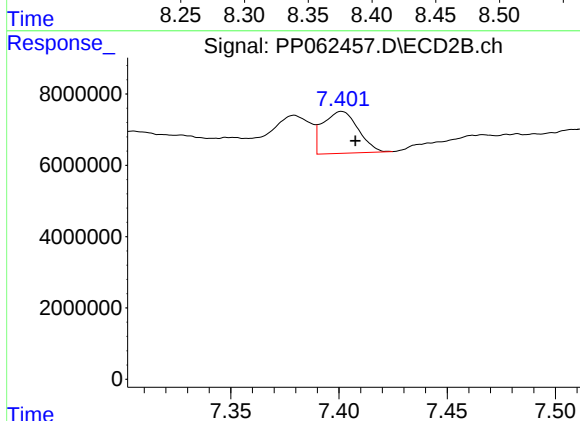


#35 AR-1260-5

R.T.: 7.401 min
Delta R.T.: -0.006 min
Response: 13359739
Conc: 46.19 ng/ml

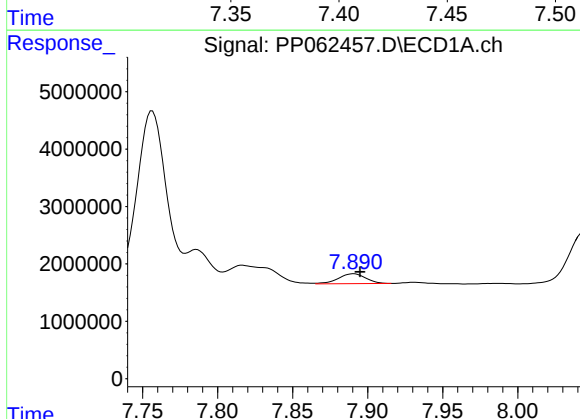


#36 AR-1262-1

R.T.: 7.891 min
Delta R.T.: -0.004 min
Response: 2210980
Conc: 54.93 ng/ml

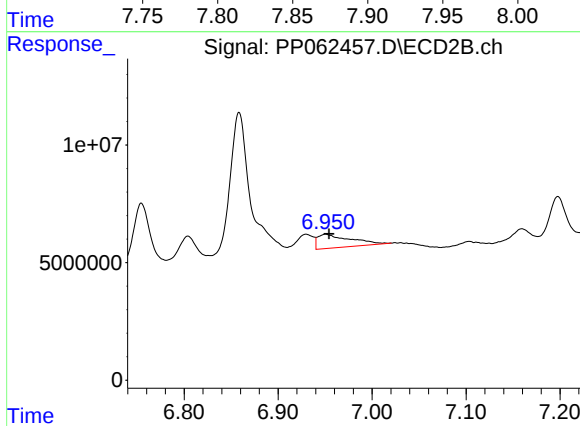

#36 AR-1262-1


R.T.: 6.951 min
Delta R.T.: -0.004 min
Response: 14371541
Conc: 163.47 ng/ml

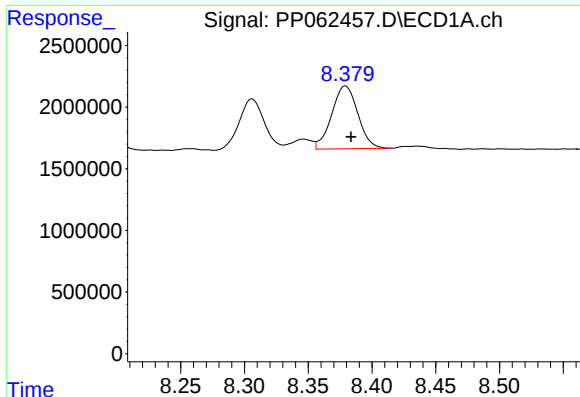

#37 AR-1262-2


R.T.: 8.379 min
Delta R.T.: -0.004 min
Response: 7288334
Conc: 55.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

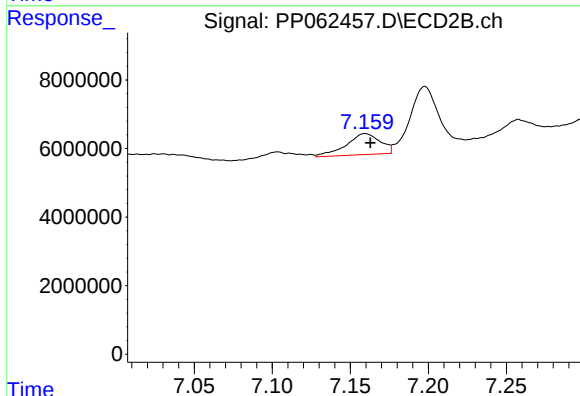


#37 AR-1262-2

R.T.: 7.160 min
Delta R.T.: -0.003 min
Response: 9370255
Conc: 51.84 ng/ml

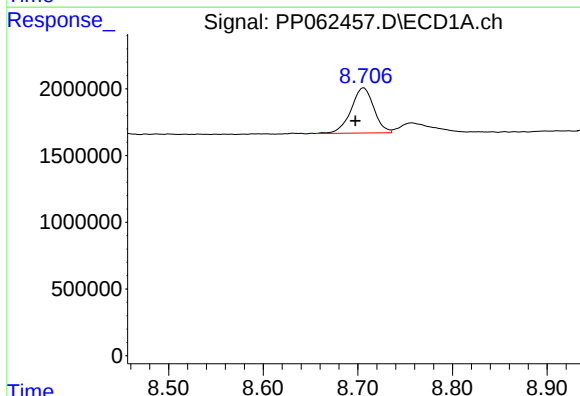


#38 AR-1262-3

R.T.: 8.706 min
Delta R.T.: 0.009 min
Response: 5681865
Conc: 64.82 ng/ml

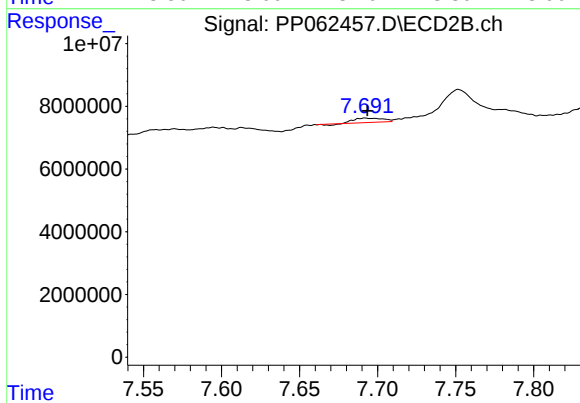

#38 AR-1262-3


R.T.: 7.692 min
Delta R.T.: -0.001 min
Response: 1700119
Conc: 13.57 ng/ml

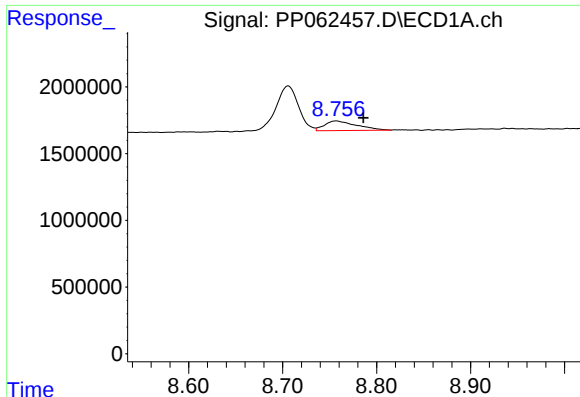

#39 AR-1262-4


R.T.: 8.757 min
Delta R.T.: -0.029 min
Response: 1709705
Conc: 25.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

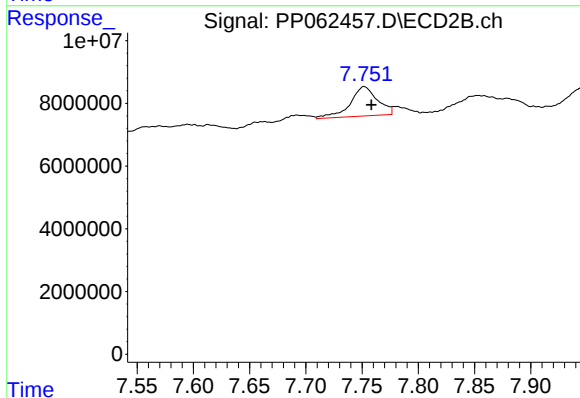


#39 AR-1262-4

R.T.: 7.752 min
Delta R.T.: -0.006 min
Response: 15818860
Conc: 67.16 ng/ml

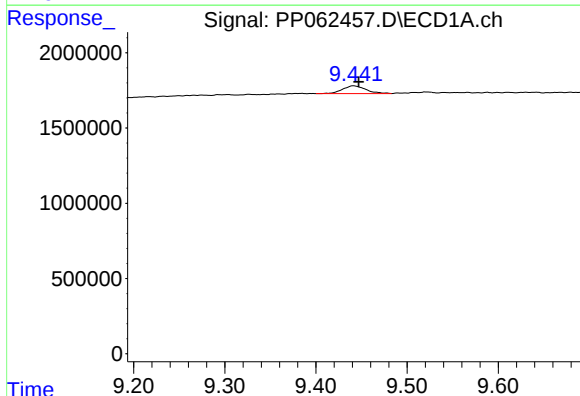


#40 AR-1262-5

R.T.: 9.441 min
Delta R.T.: -0.006 min
Response: 897831
Conc: 22.05 ng/ml

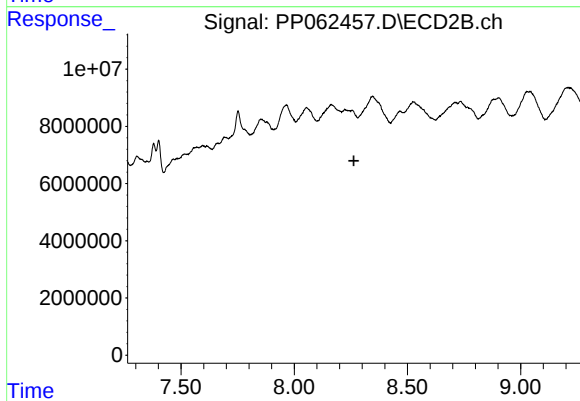

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 8.263 min
Response: 0
Conc: N.D.

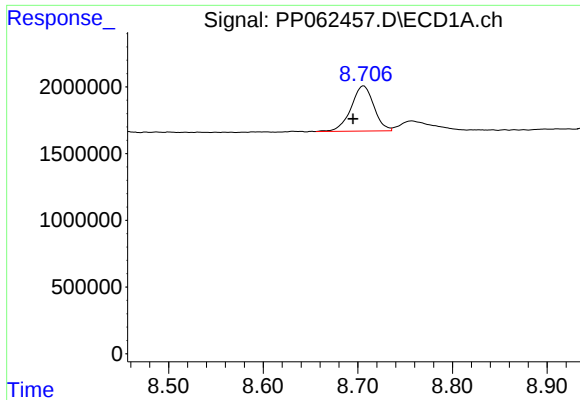

#41 AR-1268-1


R.T.: 8.706 min
Delta R.T.: 0.011 min
Response: 5681865
Conc: 34.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

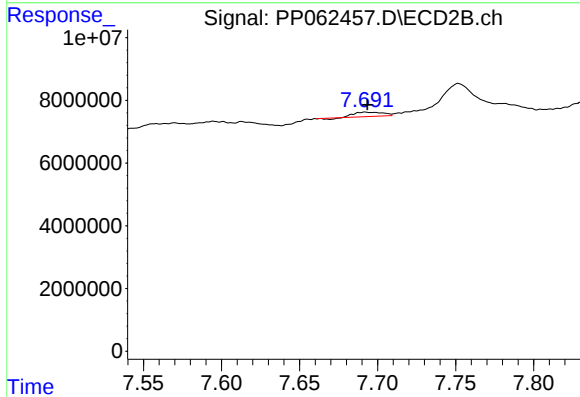


#41 AR-1268-1

R.T.: 7.692 min
Delta R.T.: -0.001 min
Response: 1700119
Conc: 4.33 ng/ml

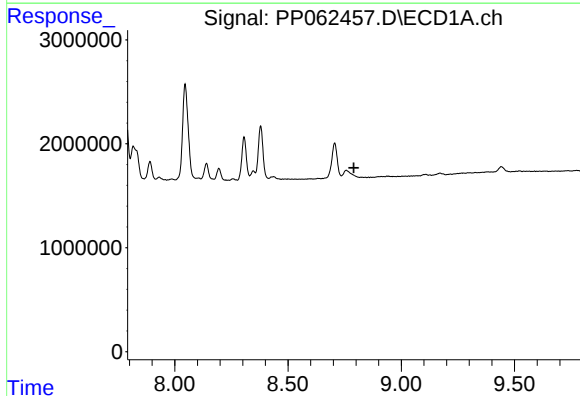


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.790 min
Response: 0
Conc: N.D.

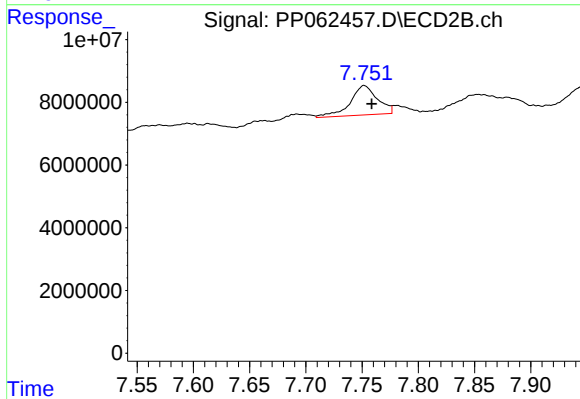

#42 AR-1268-2


R.T.: 7.752 min
Delta R.T.: -0.007 min
Response: 15818860
Conc: 44.46 ng/ml

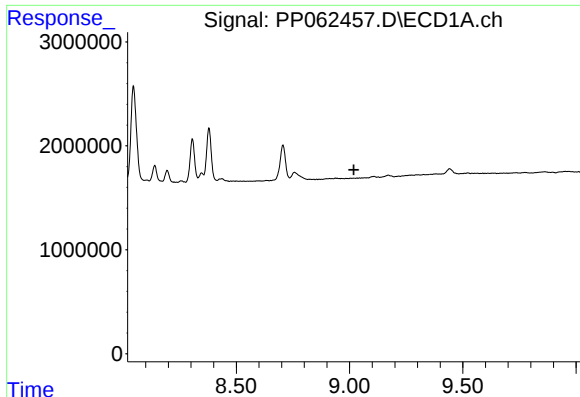

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.019 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-120623-02DL

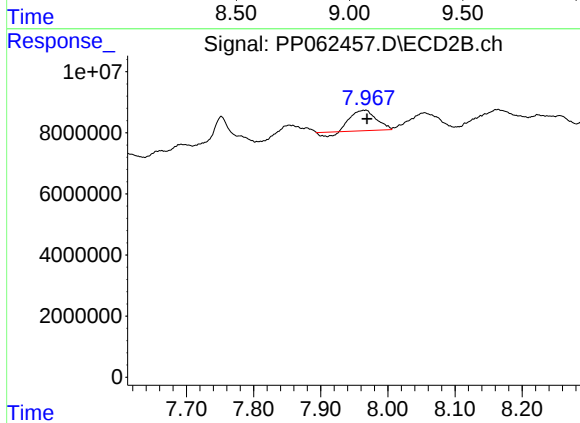


#43 AR-1268-3

R.T.: 7.967 min
Delta R.T.: -0.002 min
Response: 16632305
Conc: 49.87 ng/ml

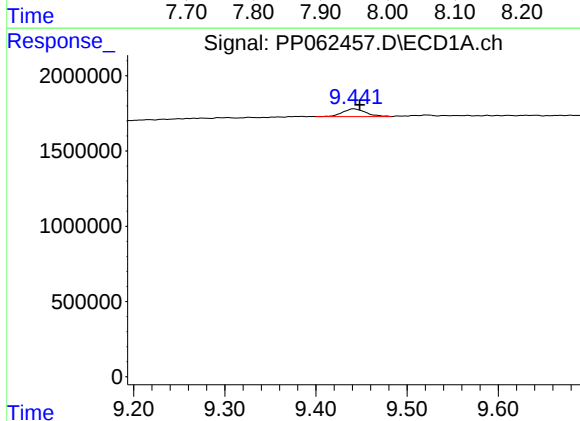

#44 AR-1268-4

R.T.: 9.441 min
Delta R.T.: -0.007 min
Response: 897831
Conc: 19.51 ng/ml

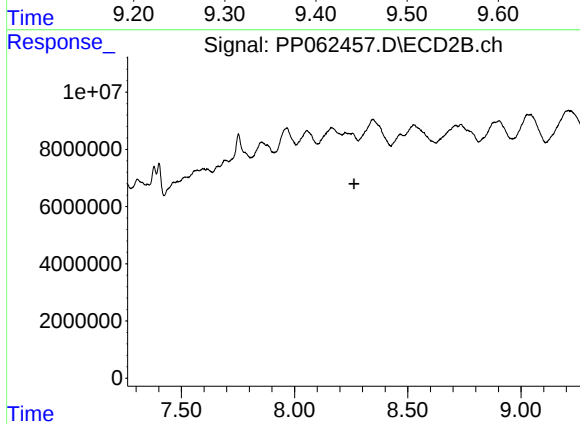

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 8.262 min
Response: 0
Conc: N.D.