

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121323\
 Data File : PP062462.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2023 14:17
 Operator : YP\AJ
 Sample : 05761-03 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FDA790B-END-1-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 16:16:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 12 05:13:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.431	3.717	3607034	5421900	2.150	1.767
2)	SA Decachlor...	10.204	8.832	2689099	4942793	2.573	2.146
Target Compounds							
27)	L6 AR-1254-2	6.681	5.794	675125	344747	6.405	2.437 #
28)	L6 AR-1254-3	7.049	6.205	873565	1903759	8.069	8.589
29)	L6 AR-1254-4	7.335	6.434	616078	895896	9.595	8.126
30)	L6 AR-1254-5	7.757	6.858	1254299	1865995	17.109	10.056 #
31)	L7 AR-1260-1	7.214	6.335	313826	837041	3.971	5.173 #
32)	L7 AR-1260-2	7.473	6.525	451595	1271929	5.279	6.982 #
33)	L7 AR-1260-3	7.833	6.684	539619	1437452	8.151	7.987
34)	L7 AR-1260-4	8.054	7.160	791420	764553	10.769	5.232 #
35)	L7 AR-1260-5	8.380	7.403	750391	1702456	6.378	5.886
36)	L8 AR-1262-1	0.000	6.951	0	379442	N.D.	4.316 #
37)	L8 AR-1262-2	8.380	7.160	750391	764553	5.749	4.230 #
38)	L8 AR-1262-3	8.693	7.690	760904	1316255	8.681	10.507
39)	L8 AR-1262-4	8.783	7.755	806445	2120362	11.899	9.002
40)	L8 AR-1262-5	0.000	8.258	0	820748	N.D.	8.878 #
41)	L9 AR-1268-1	8.693	7.690	760904	1316255	4.601	3.351 #
42)	L9 AR-1268-2	8.783	7.755	806445	2120362	5.663	5.959
43)	L9 AR-1268-3	0.000	7.966	0	574503	N.D.	1.723 #
44)	L9 AR-1268-4	0.000	8.258	0	820748	N.D.	7.443 #
45)	L9 AR-1268-5	9.863	8.563	694713	1492433	1.778	1.735



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121323\
Data File : PP062462.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2023 14:17
Operator : YP\AJ
Sample : 05761-03 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FDA790B-END-1-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 16:16:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 12 05:13:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

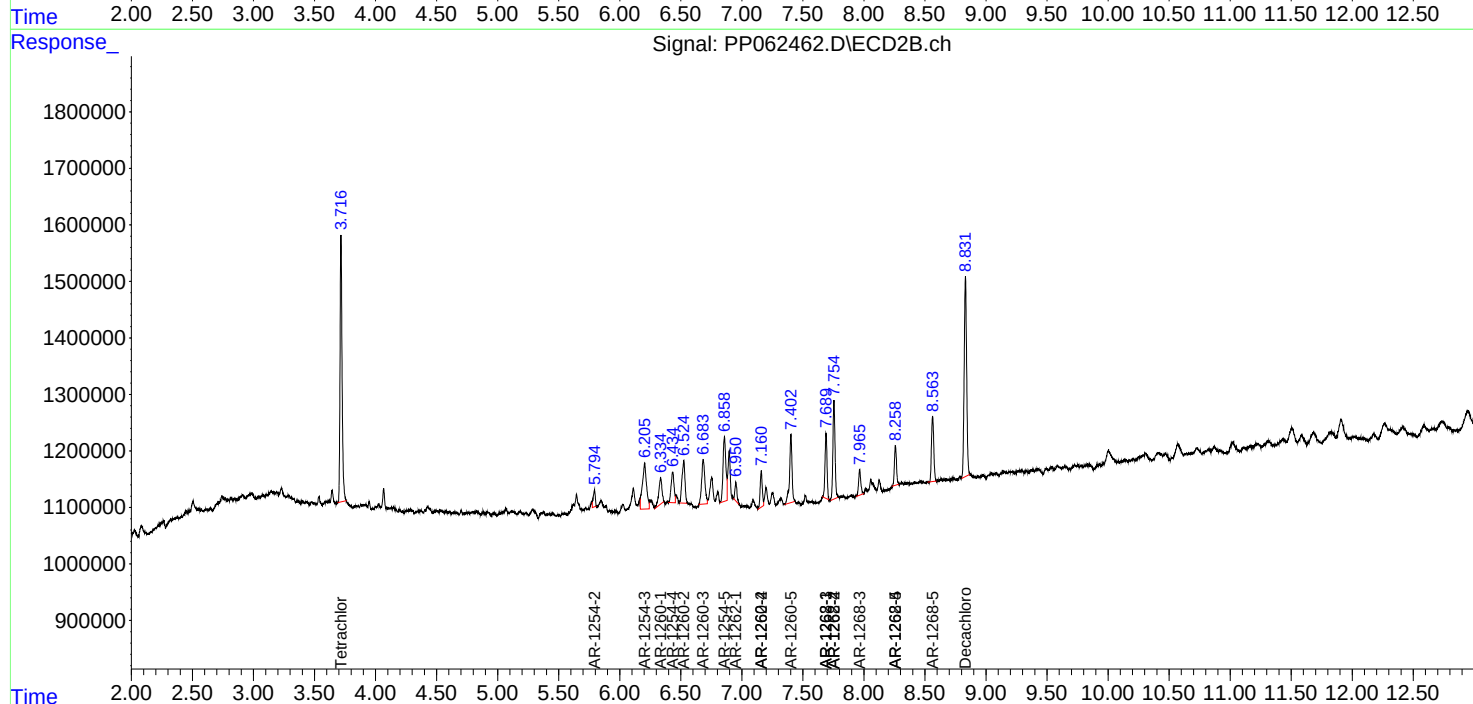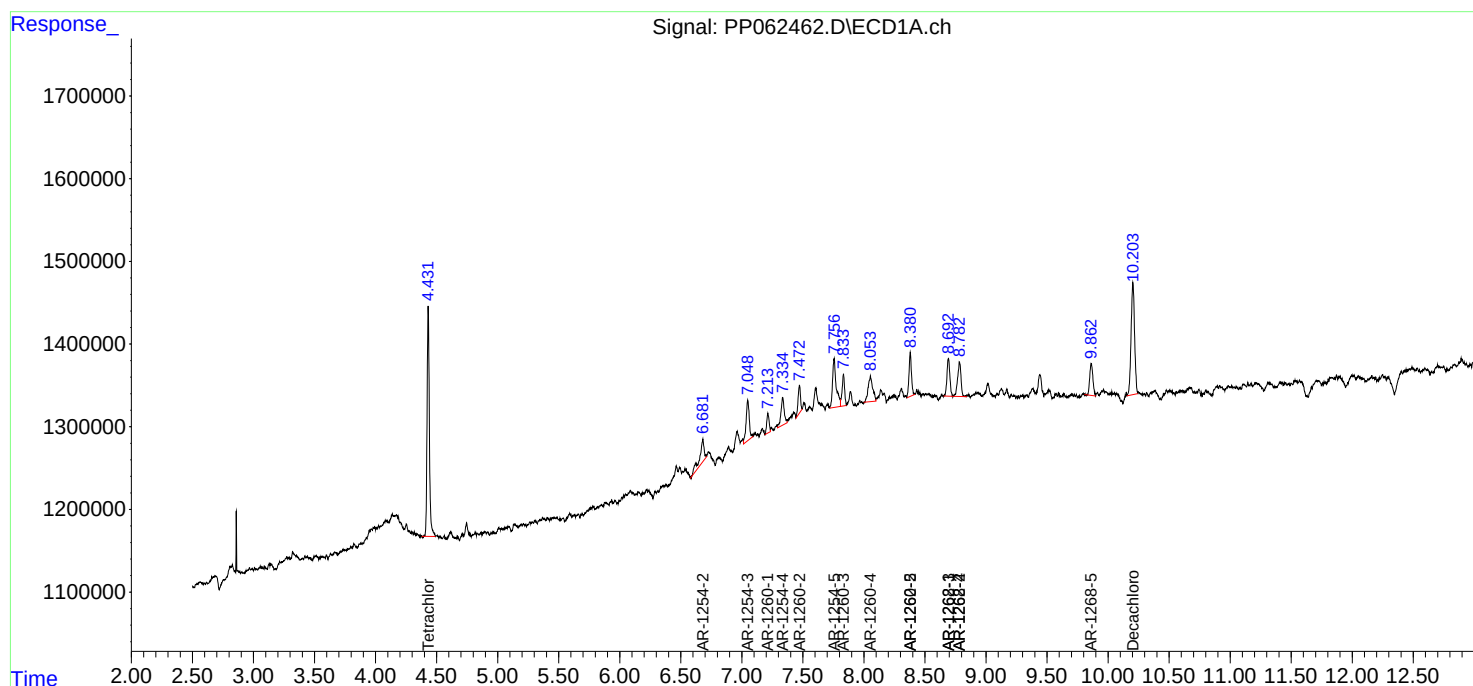


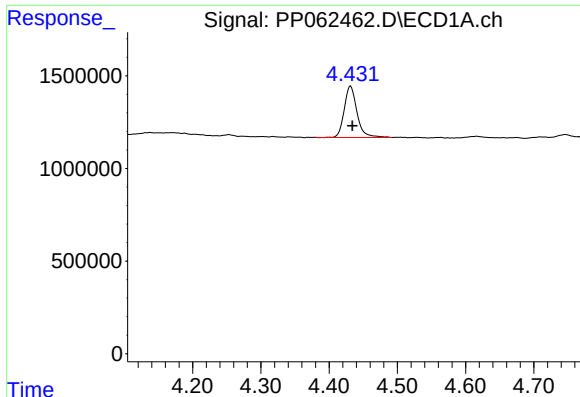

#1 Tetrachloro-m-xylene


R.T.: 4.431 min
Delta R.T.: -0.003 min
Response: 3607034
Conc: 2.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA790B-END-1-1

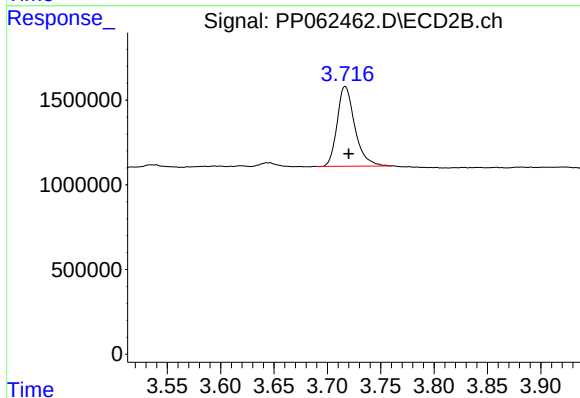


#1 Tetrachloro-m-xylene

R.T.: 3.717 min
Delta R.T.: -0.003 min
Response: 5421900
Conc: 1.77 ng/ml

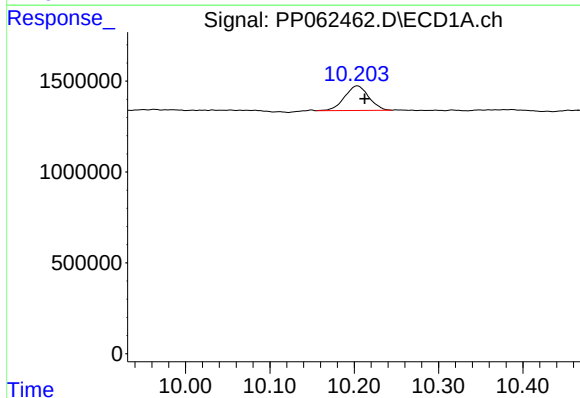


#2 Decachlorobiphenyl

R.T.: 10.204 min
Delta R.T.: -0.009 min
Response: 2689099
Conc: 2.57 ng/ml

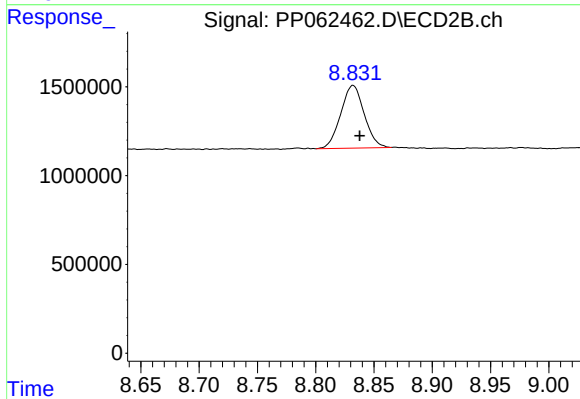

#2 Decachlorobiphenyl


R.T.: 8.832 min
Delta R.T.: -0.006 min
Response: 4942793
Conc: 2.15 ng/ml

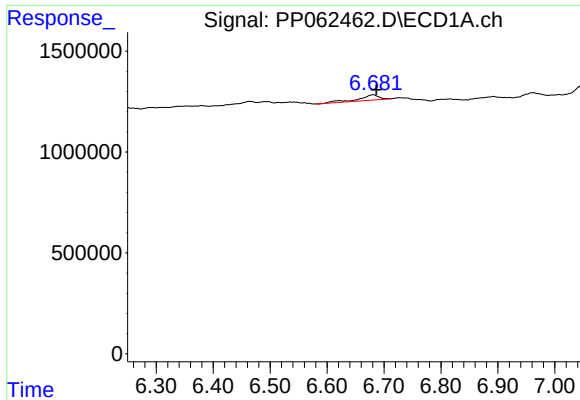

#27 AR-1254-2


R.T.: 6.681 min
Delta R.T.: -0.005 min
Response: 675125
Conc: 6.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA790B-END-1-1

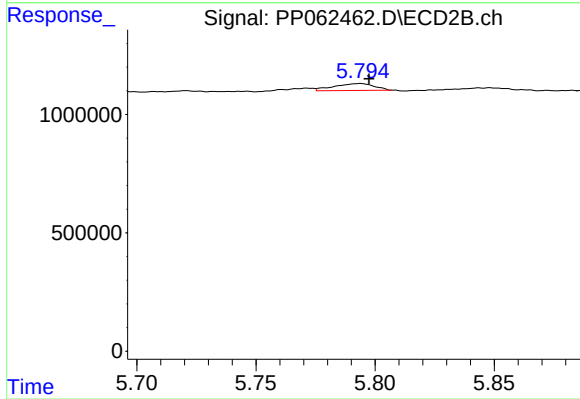


#27 AR-1254-2

R.T.: 5.794 min
Delta R.T.: -0.003 min
Response: 344747
Conc: 2.44 ng/ml

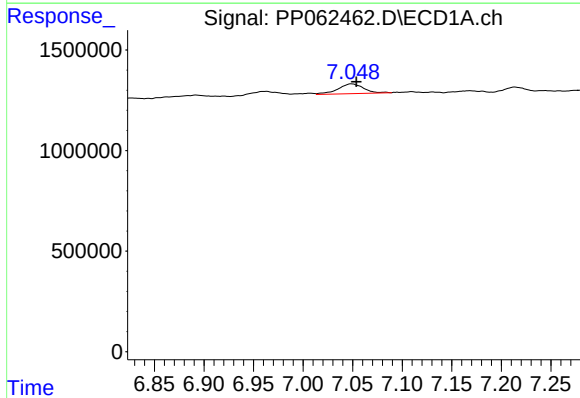


#28 AR-1254-3

R.T.: 7.049 min
Delta R.T.: -0.005 min
Response: 873565
Conc: 8.07 ng/ml

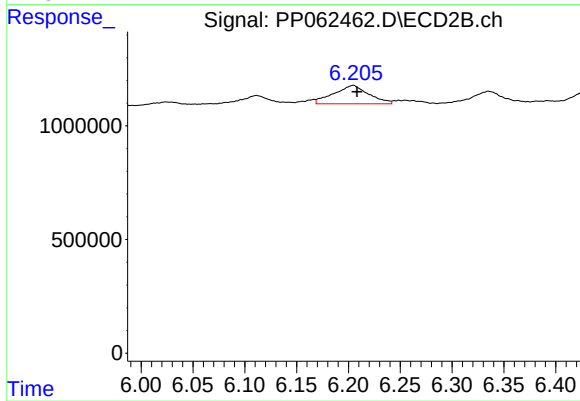

#28 AR-1254-3


R.T.: 6.205 min
Delta R.T.: -0.003 min
Response: 1903759
Conc: 8.59 ng/ml

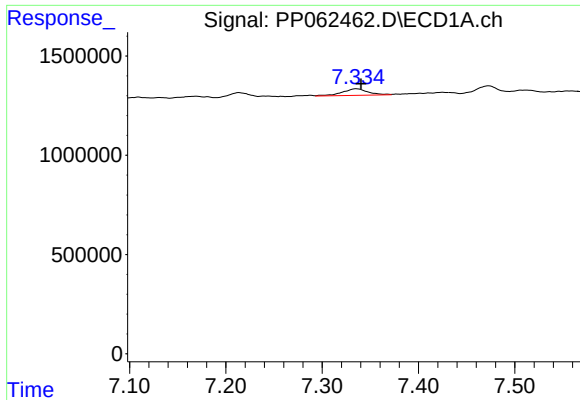

#29 AR-1254-4


R.T.: 7.335 min
Delta R.T.: -0.005 min
Response: 616078
Conc: 9.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA790B-END-1-1

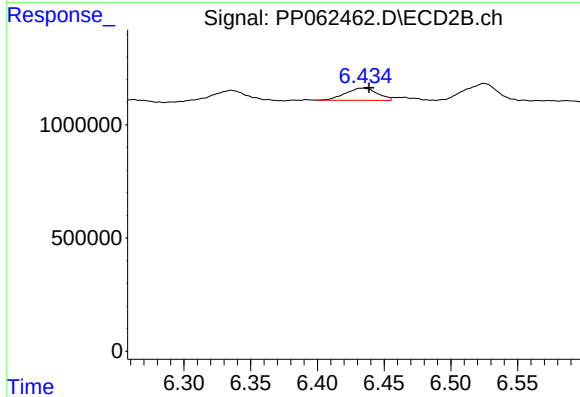


#29 AR-1254-4

R.T.: 6.434 min
Delta R.T.: -0.004 min
Response: 895896
Conc: 8.13 ng/ml

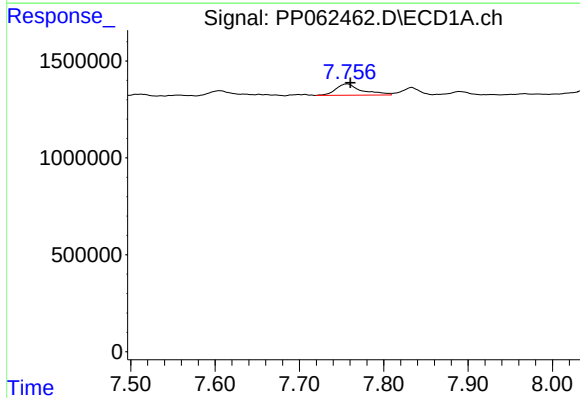


#30 AR-1254-5

R.T.: 7.757 min
Delta R.T.: -0.004 min
Response: 1254299
Conc: 17.11 ng/ml

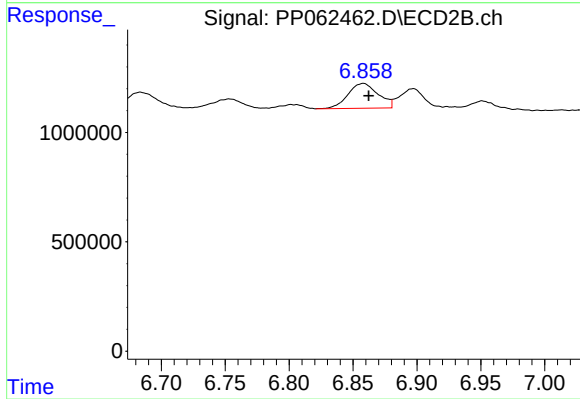

#30 AR-1254-5


R.T.: 6.858 min
Delta R.T.: -0.004 min
Response: 1865995
Conc: 10.06 ng/ml

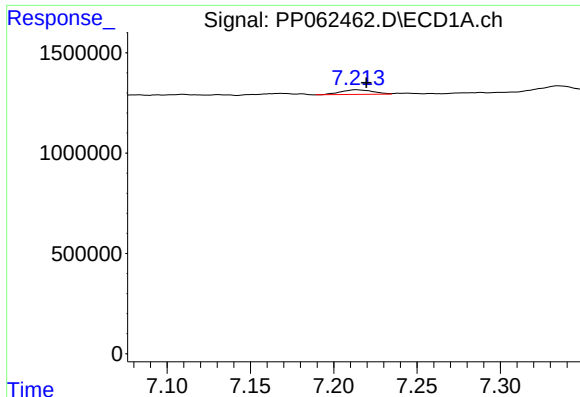

#31 AR-1260-1


R.T.: 7.214 min
Delta R.T.: -0.006 min
Response: 313826
Conc: 3.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA790B-END-1-1

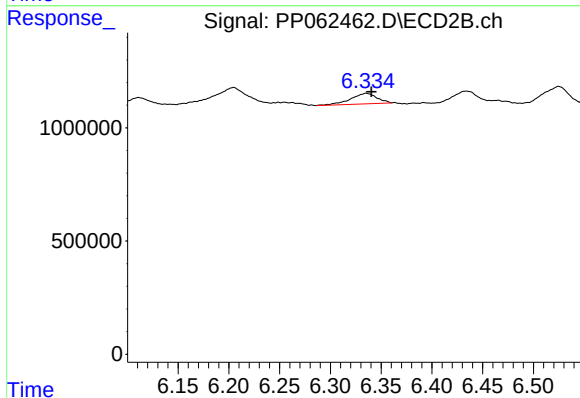


#31 AR-1260-1

R.T.: 6.335 min
Delta R.T.: -0.006 min
Response: 837041
Conc: 5.17 ng/ml

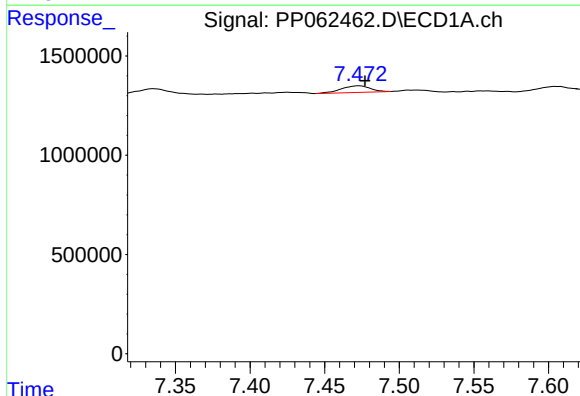


#32 AR-1260-2

R.T.: 7.473 min
Delta R.T.: -0.004 min
Response: 451595
Conc: 5.28 ng/ml

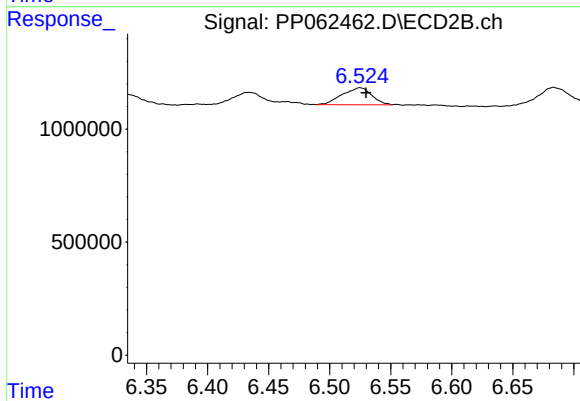

#32 AR-1260-2


R.T.: 6.525 min
Delta R.T.: -0.005 min
Response: 1271929
Conc: 6.98 ng/ml

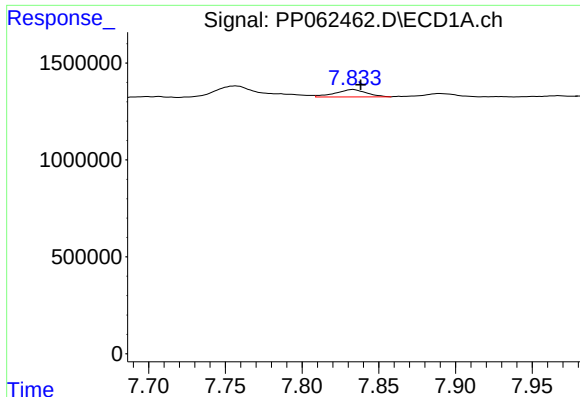

#33 AR-1260-3


R.T.: 7.833 min
Delta R.T.: -0.005 min
Response: 539619
Conc: 8.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA790B-END-1-1

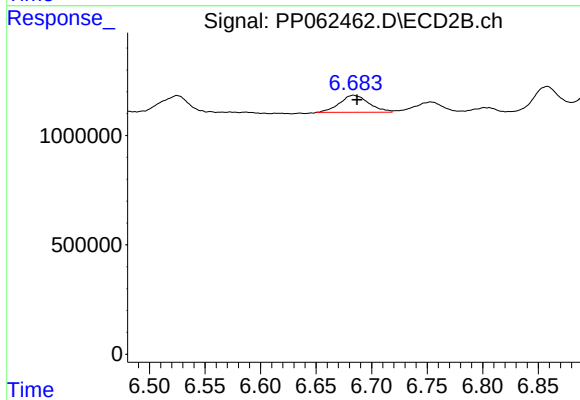


#33 AR-1260-3

R.T.: 6.684 min
Delta R.T.: -0.003 min
Response: 1437452
Conc: 7.99 ng/ml

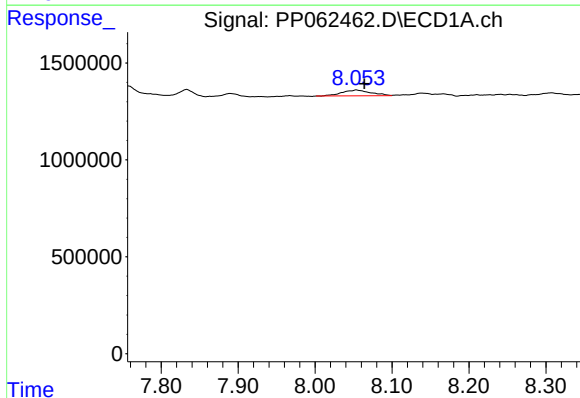


#34 AR-1260-4

R.T.: 8.054 min
Delta R.T.: -0.010 min
Response: 791420
Conc: 10.77 ng/ml

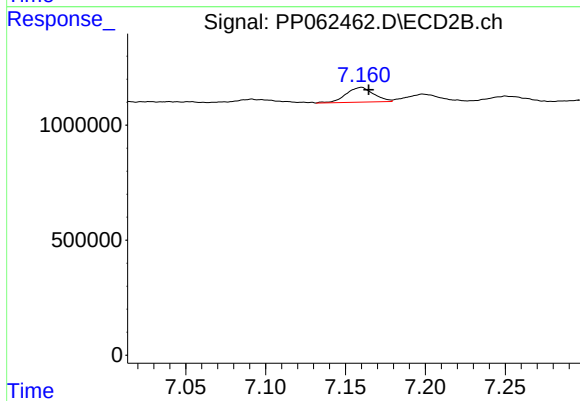

#34 AR-1260-4


R.T.: 7.160 min
Delta R.T.: -0.004 min
Response: 764553
Conc: 5.23 ng/ml

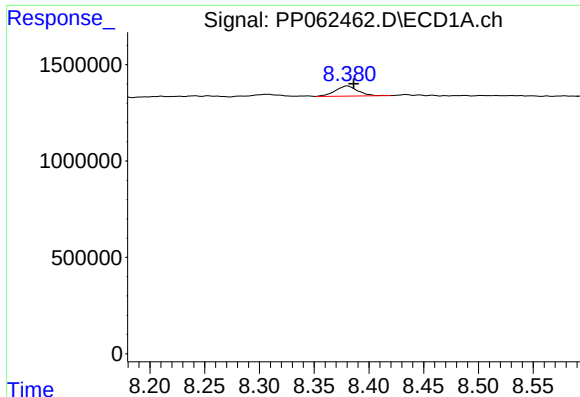

#35 AR-1260-5


R.T.: 8.380 min
Delta R.T.: -0.006 min
Response: 750391
Conc: 6.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA790B-END-1-1

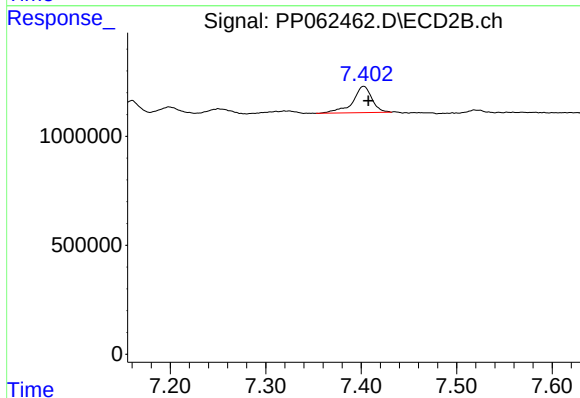


#35 AR-1260-5

R.T.: 7.403 min
Delta R.T.: -0.005 min
Response: 1702456
Conc: 5.89 ng/ml

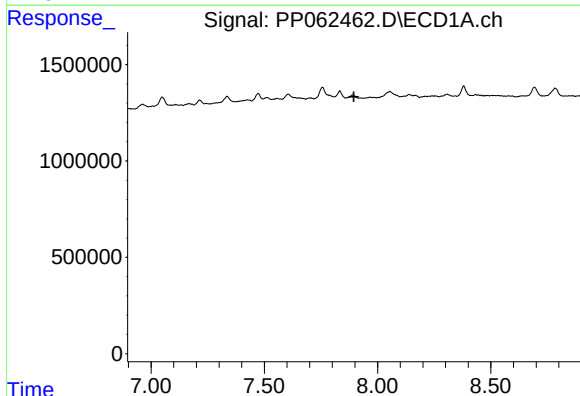


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.895 min
Response: 0
Conc: N.D.

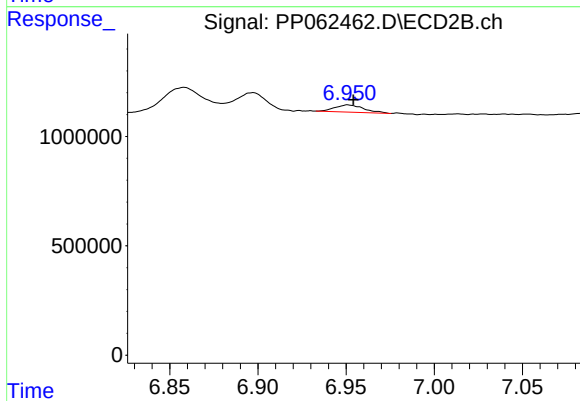

#36 AR-1262-1


R.T.: 6.951 min
Delta R.T.: -0.003 min
Response: 379442
Conc: 4.32 ng/ml

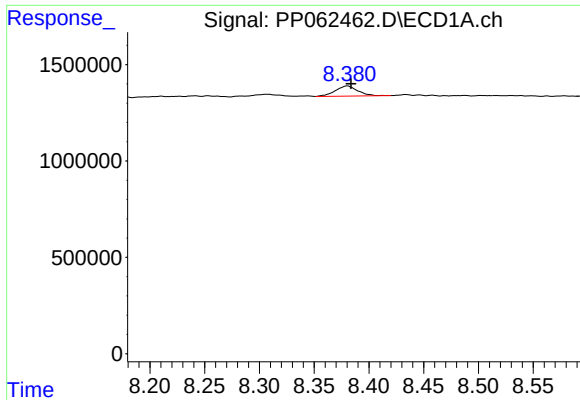

#37 AR-1262-2


R.T.: 8.380 min
Delta R.T.: -0.003 min
Response: 750391
Conc: 5.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA790B-END-1-1

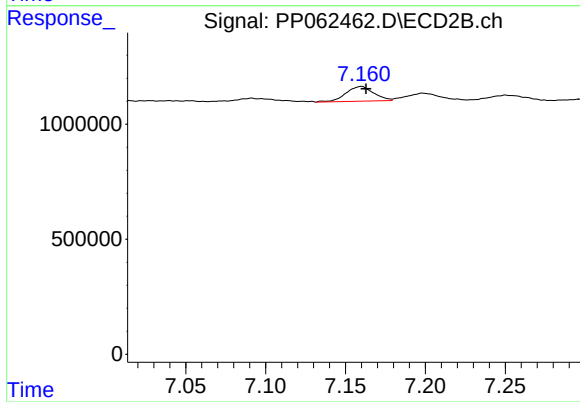


#37 AR-1262-2

R.T.: 7.160 min
Delta R.T.: -0.003 min
Response: 764553
Conc: 4.23 ng/ml

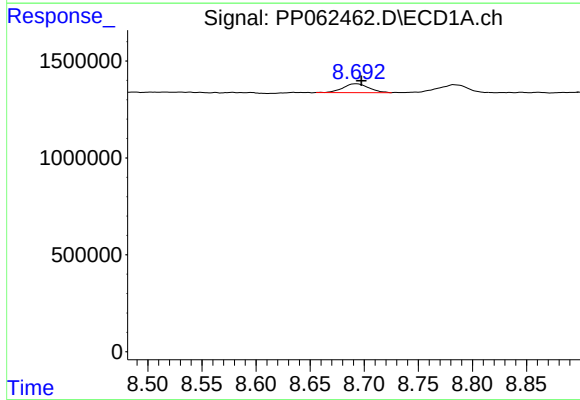


#38 AR-1262-3

R.T.: 8.693 min
Delta R.T.: -0.005 min
Response: 760904
Conc: 8.68 ng/ml

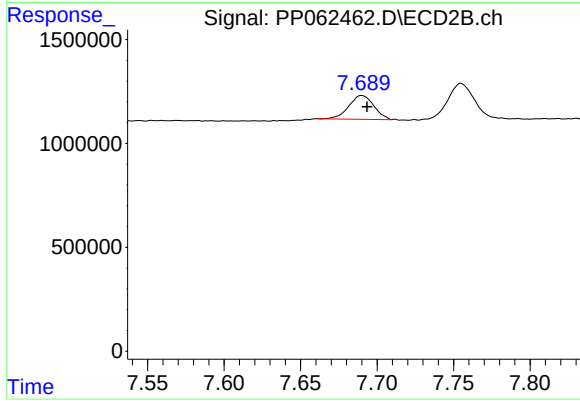

#38 AR-1262-3


R.T.: 7.690 min
Delta R.T.: -0.004 min
Response: 1316255
Conc: 10.51 ng/ml

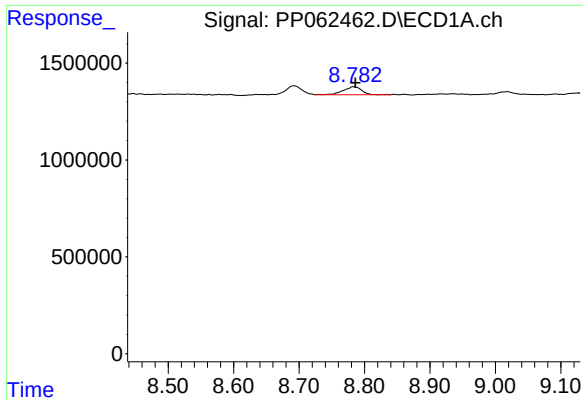

#39 AR-1262-4


R.T.: 8.783 min
Delta R.T.: -0.003 min
Response: 806445
Conc: 11.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA790B-END-1-1

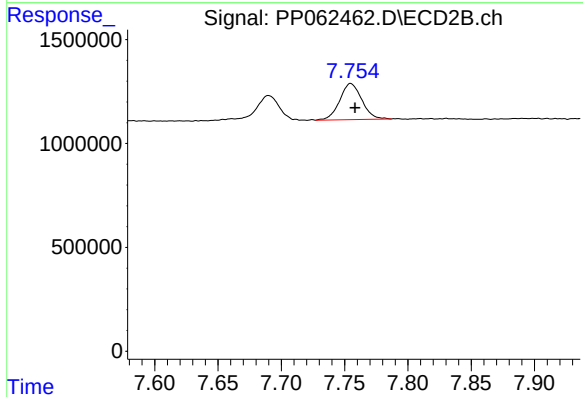


#39 AR-1262-4

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 2120362
Conc: 9.00 ng/ml

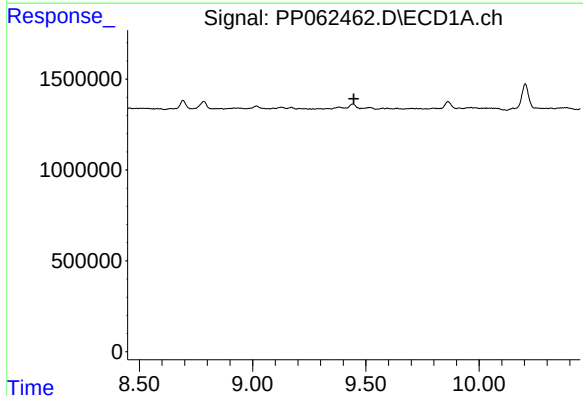


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.447 min
Response: 0
Conc: N.D.

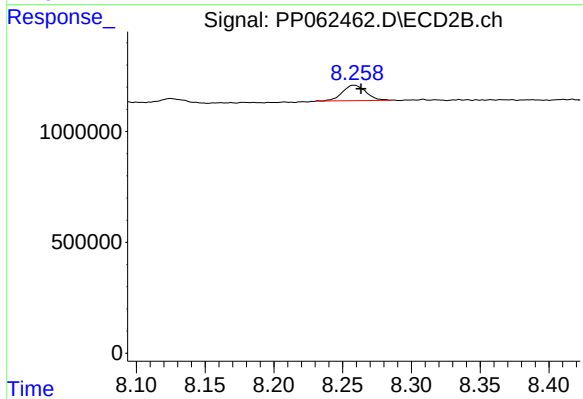

#40 AR-1262-5


R.T.: 8.258 min
Delta R.T.: -0.005 min
Response: 820748
Conc: 8.88 ng/ml

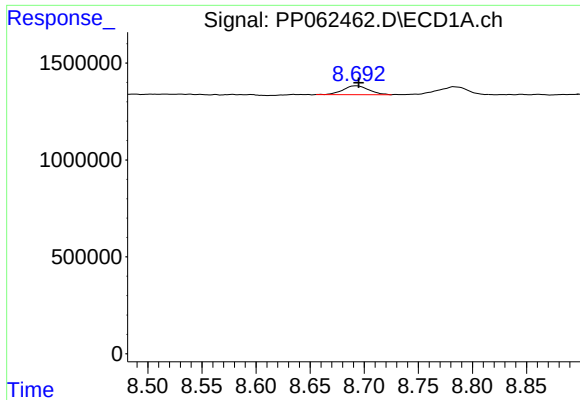

#41 AR-1268-1


R.T.: 8.693 min
Delta R.T.: -0.002 min
Response: 760904
Conc: 4.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA790B-END-1-1

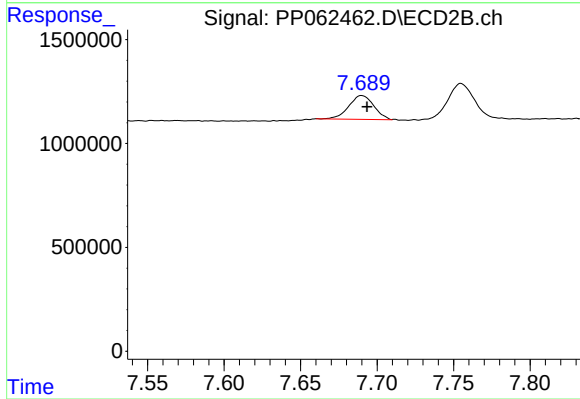


#41 AR-1268-1

R.T.: 7.690 min
Delta R.T.: -0.004 min
Response: 1316255
Conc: 3.35 ng/ml

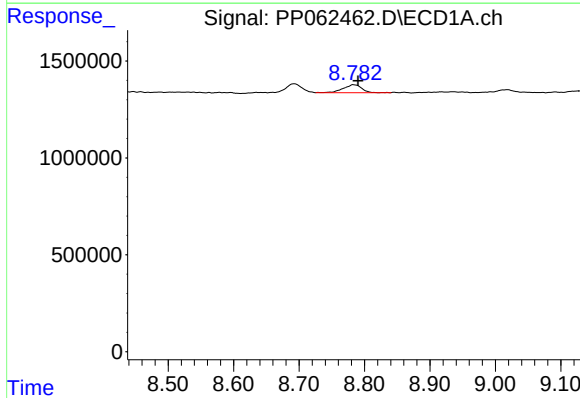


#42 AR-1268-2

R.T.: 8.783 min
Delta R.T.: -0.007 min
Response: 806445
Conc: 5.66 ng/ml

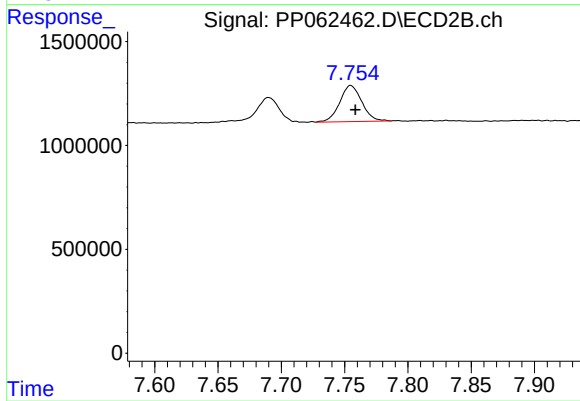

#42 AR-1268-2


R.T.: 7.755 min
Delta R.T.: -0.004 min
Response: 2120362
Conc: 5.96 ng/ml

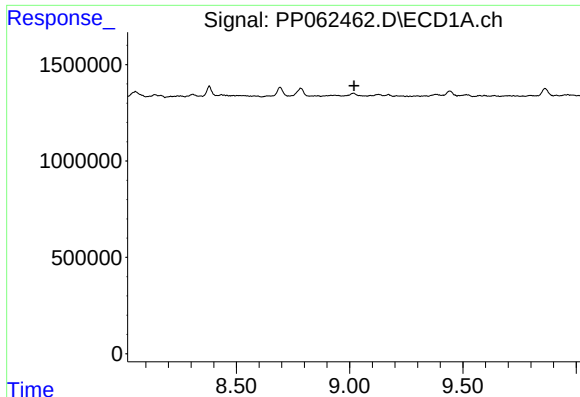

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.019 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FDA790B-END-1-1

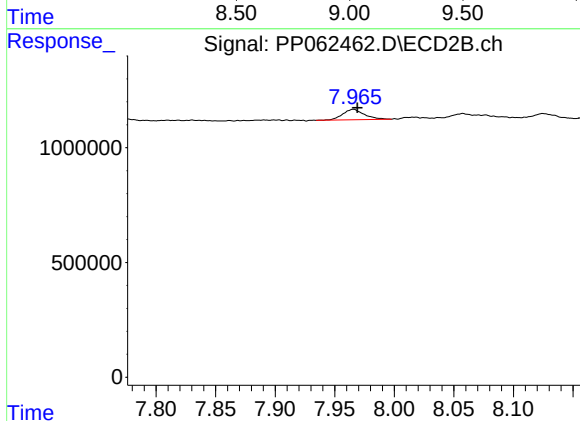


#43 AR-1268-3

R.T.: 7.966 min
Delta R.T.: -0.003 min
Response: 574503
Conc: 1.72 ng/ml

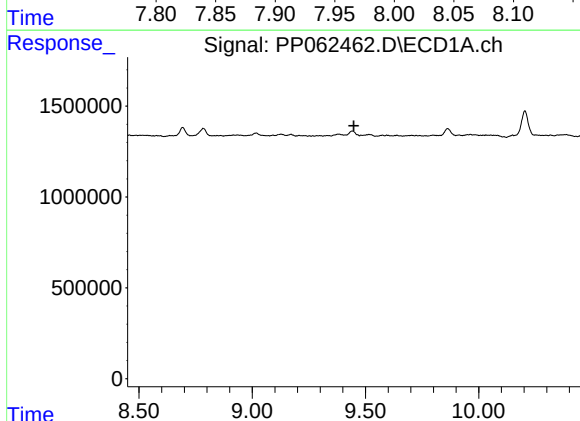


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.448 min
Response: 0
Conc: N.D.

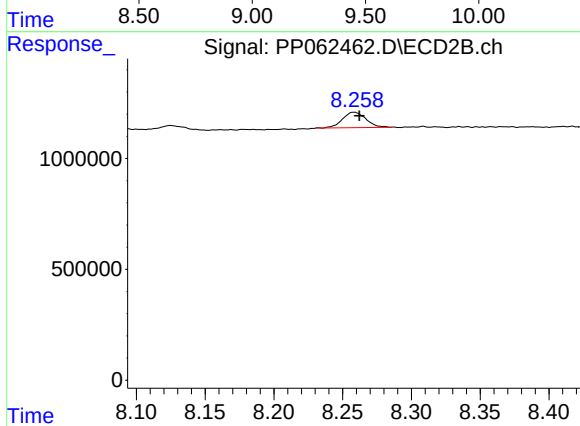

#44 AR-1268-4


R.T.: 8.258 min
Delta R.T.: -0.004 min
Response: 820748
Conc: 7.44 ng/ml

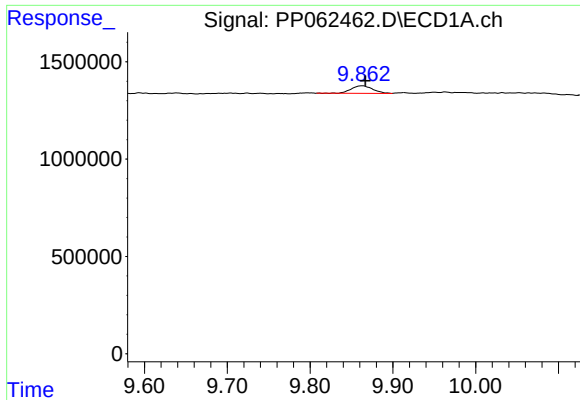

#45 AR-1268-5

R.T.: 9.863 min
Delta R.T.: -0.004 min
Response: 694713
Conc: 1.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
FDA790B-END-1-1

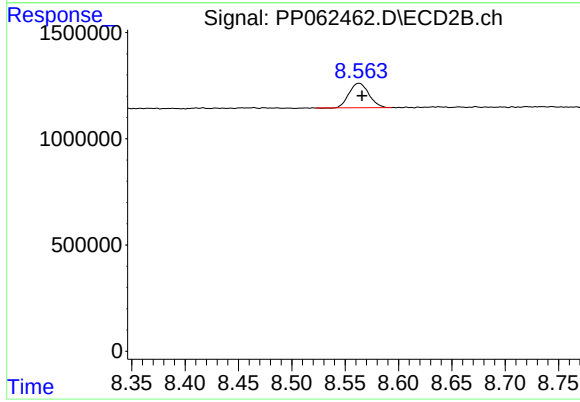

#45 AR-1268-5

R.T.: 8.563 min
Delta R.T.: -0.003 min
Response: 1492433
Conc: 1.73 ng/ml