

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121420\
 Data File : PP032097.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Dec 2020 11:48
 Operator : DD\AJ
 Sample : L5043-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KENS-SS1-121020-0-7

Manual Integrations
 APPROVED

Ankita
 12/15/2020 3:13:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 15 01:11:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.780	4.053	1111572	1014726	21.578	21.455
2) SA Decachlor...	10.645	9.345	664877	681423	21.202m	20.319

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121420\
Data File : PP032097.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Dec 2020 11:48
Operator : DD\AJ
Sample : L5043-02
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KENS-SS1-121020-0-7


Manual Integrations
APPROVED

Ankita
12/15/2020 3:13:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 01:11:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

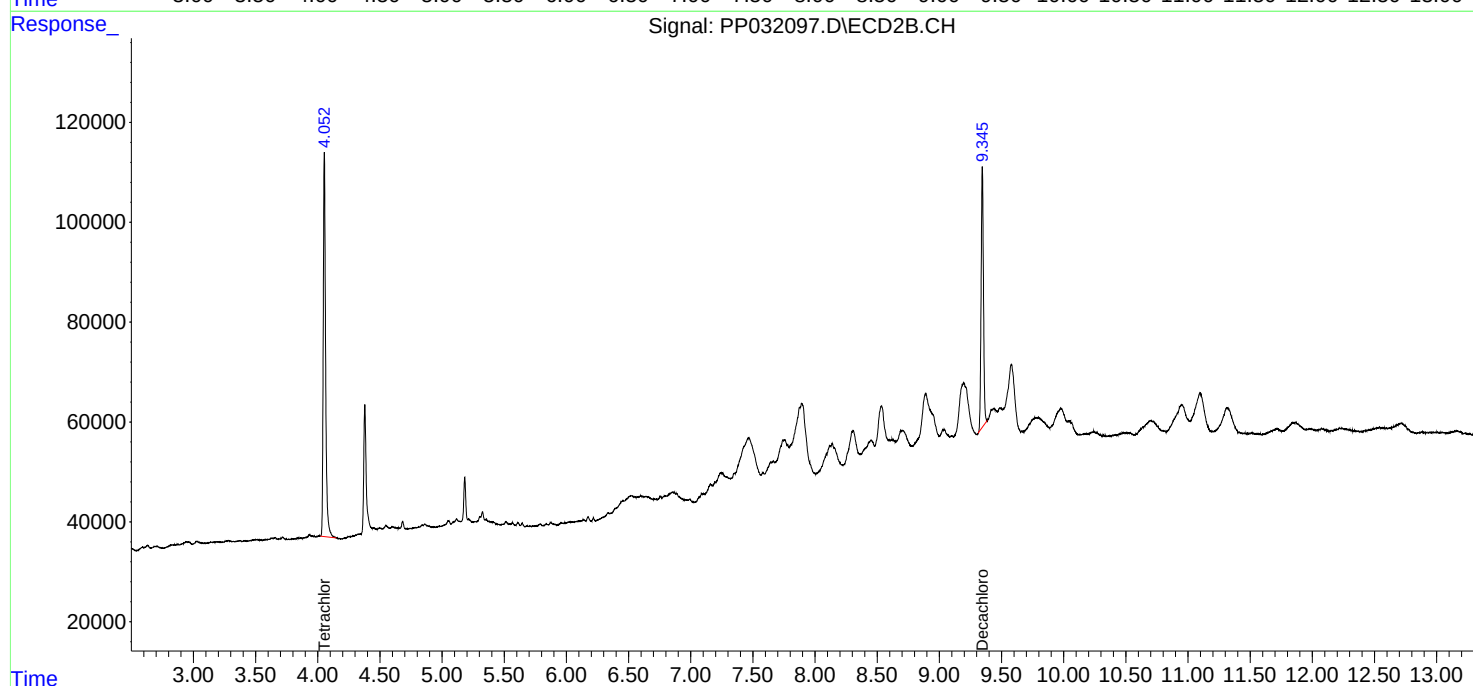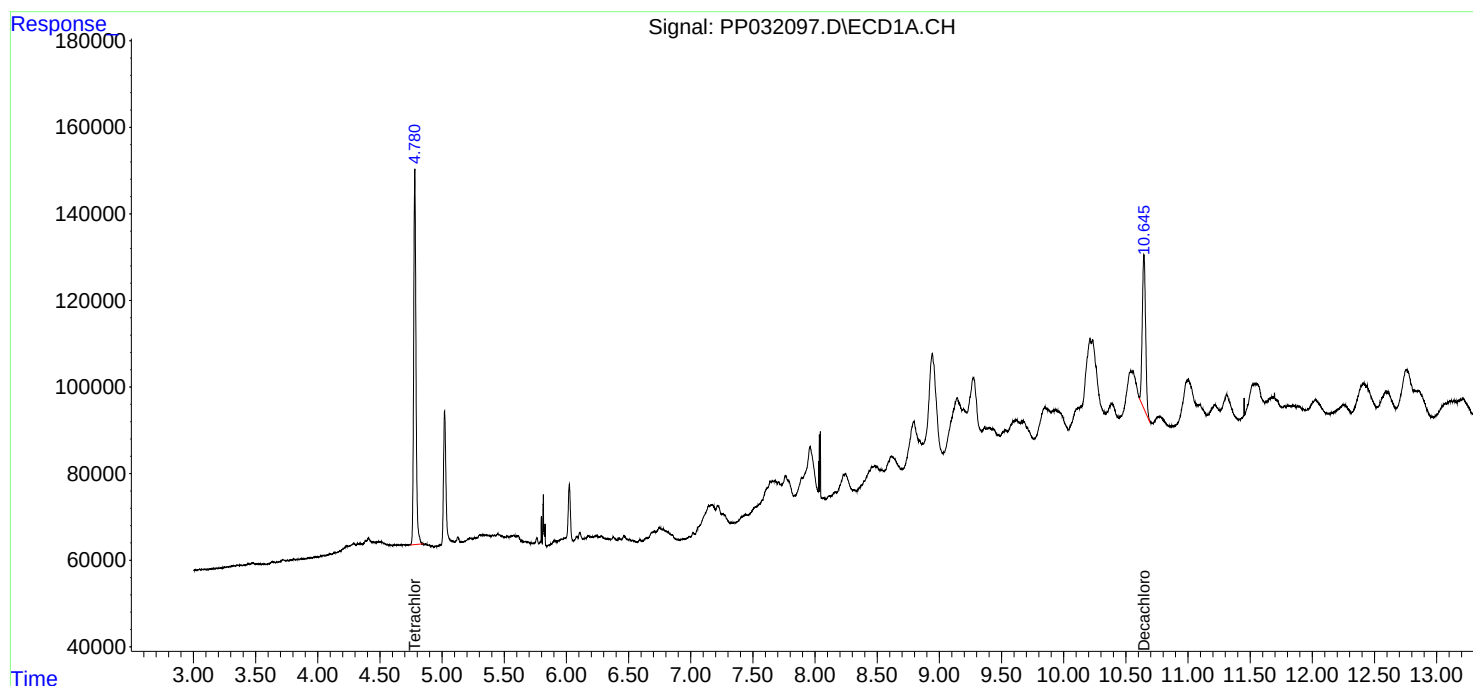

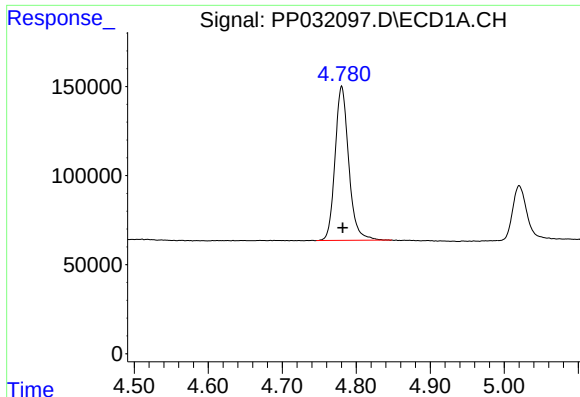


#1 Tetrachloro-m-xylene

R.T.: 4.780 min
Delta R.T.: -0.002 min
Response: 1111572
Conc: 21.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS1-121020-0-7


Manual Integrations
APPROVED

Ankita
12/15/2020 3:13:21 PM

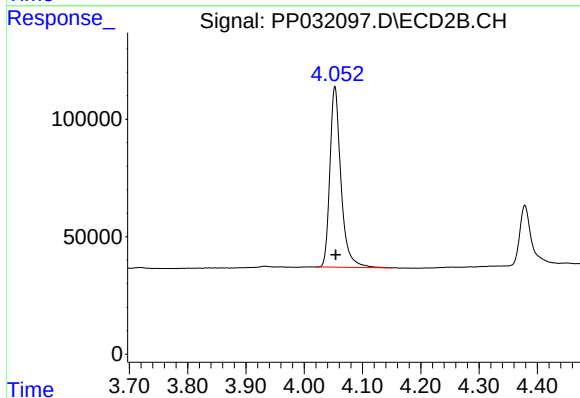


#1 Tetrachloro-m-xylene

R.T.: 4.053 min
Delta R.T.: -0.001 min
Response: 1014726
Conc: 21.45 ng/ml

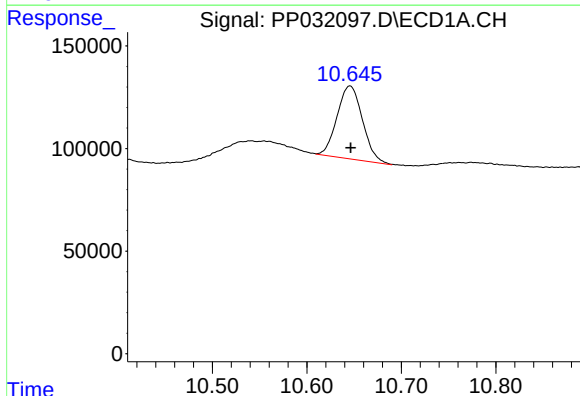

#2 Decachlorobiphenyl

R.T.: 10.645 min
Delta R.T.: -0.001 min
Response: 664877
Conc: 21.20 ng/ml m

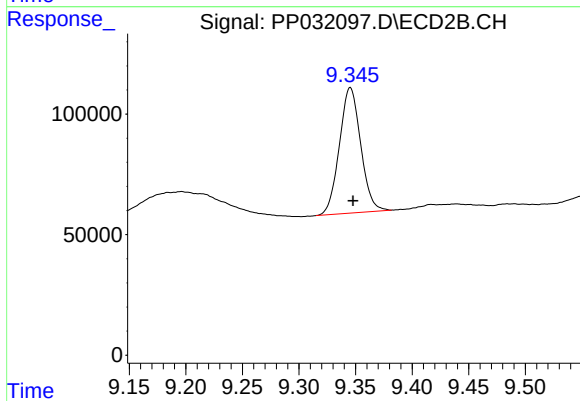

#2 Decachlorobiphenyl

R.T.: 9.345 min
Delta R.T.: -0.002 min
Response: 681423
Conc: 20.32 ng/ml