

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121420\
Data File : PP032101.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Dec 2020 12:55
Operator : DD\AJ
Sample : L5043-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
KENS-SS-121020-BD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 04:48:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.780	4.052	1237456	1111121	24.022	23.493
2) SA Decachlor...	10.645	9.345	746415	805031	23.802	24.005

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121420\
Data File : PP032101.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Dec 2020 12:55
Operator : DD\AJ
Sample : L5043-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
KENS-SS-121020-BD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 15 04:48:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

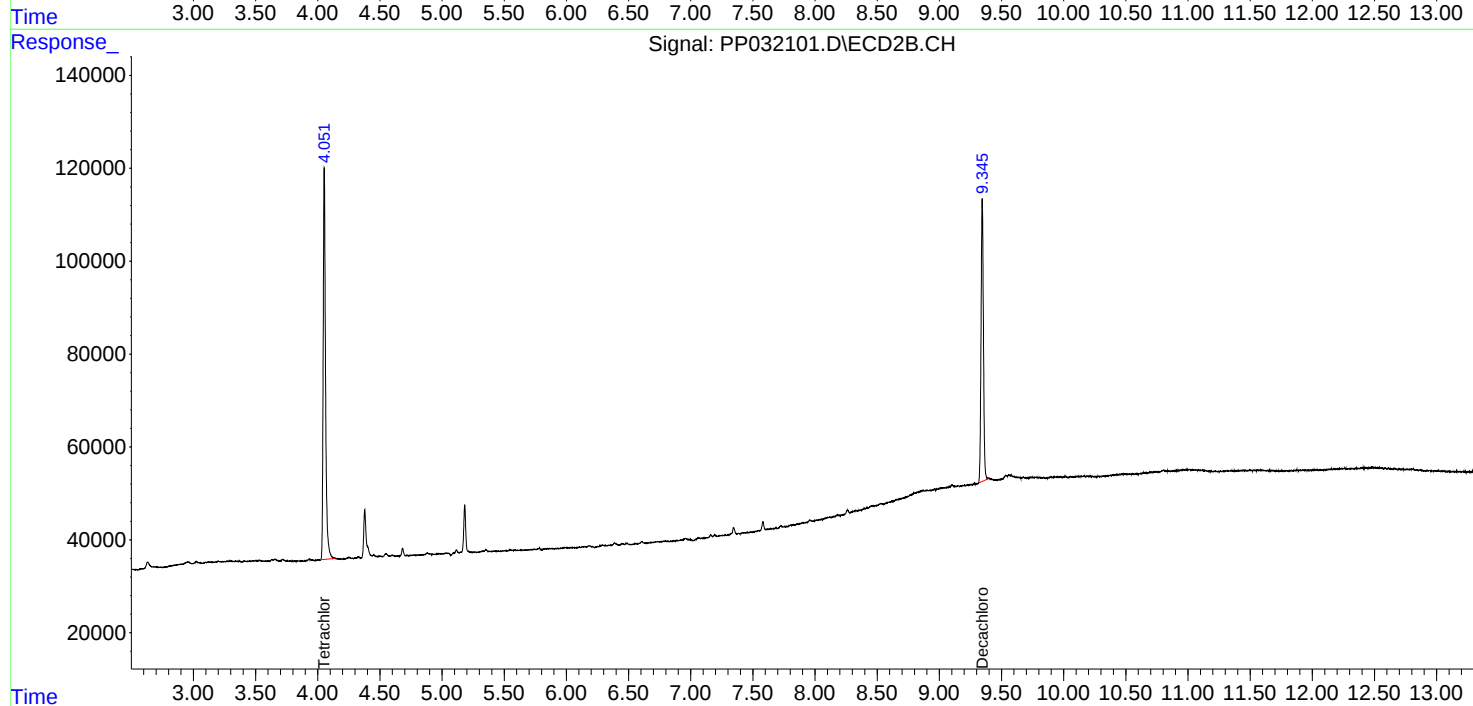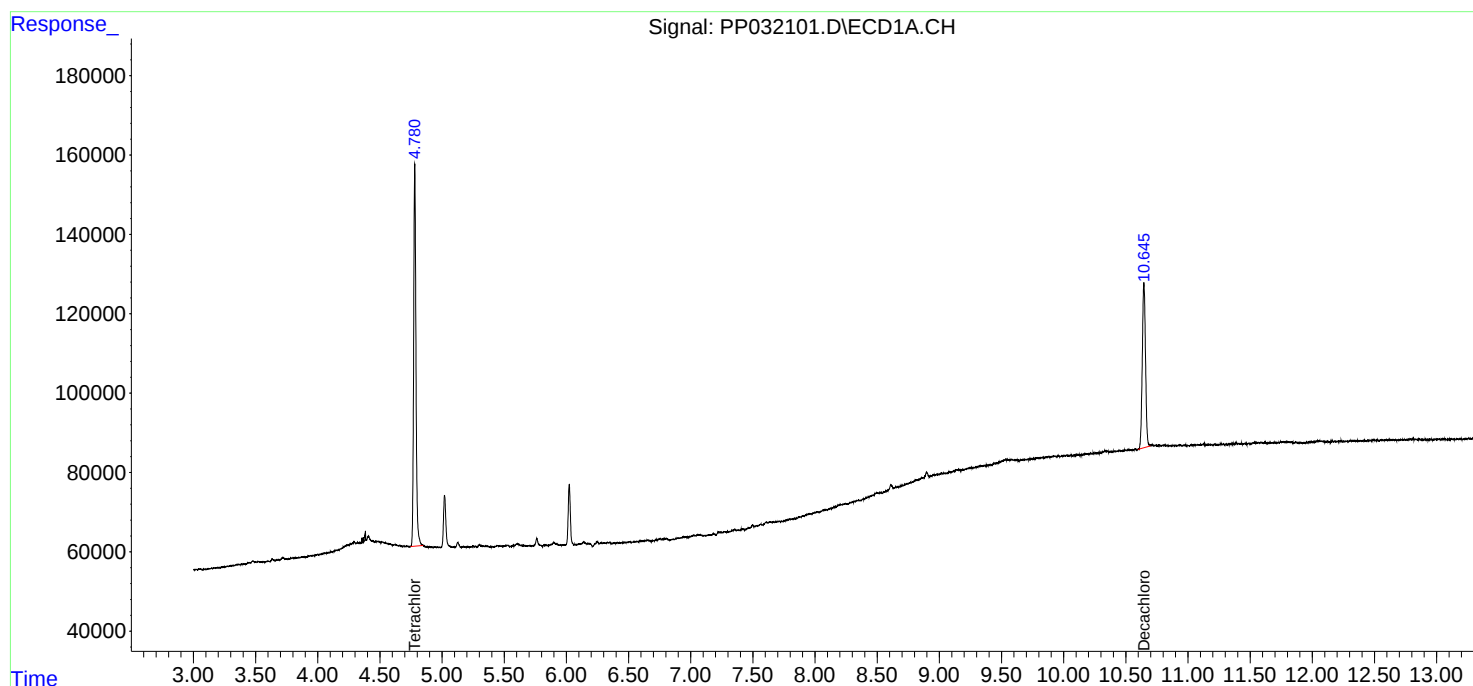


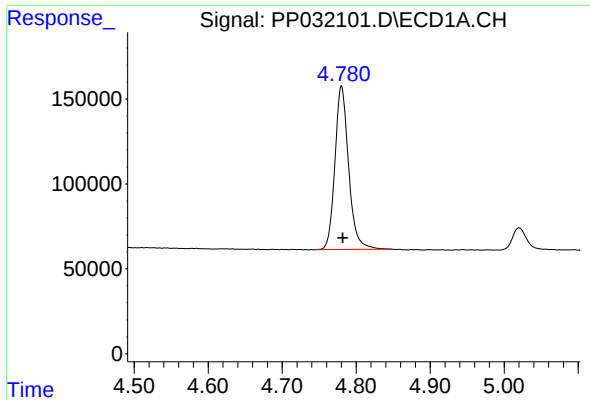

#1 Tetrachloro-m-xylene


R.T.: 4.780 min
Delta R.T.: -0.002 min
Response: 1237456
Conc: 24.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS-121020-BD

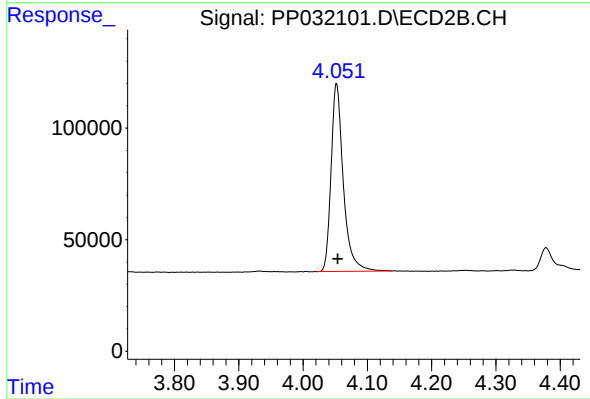


#1 Tetrachloro-m-xylene

R.T.: 4.052 min
Delta R.T.: -0.002 min
Response: 1111121
Conc: 23.49 ng/ml

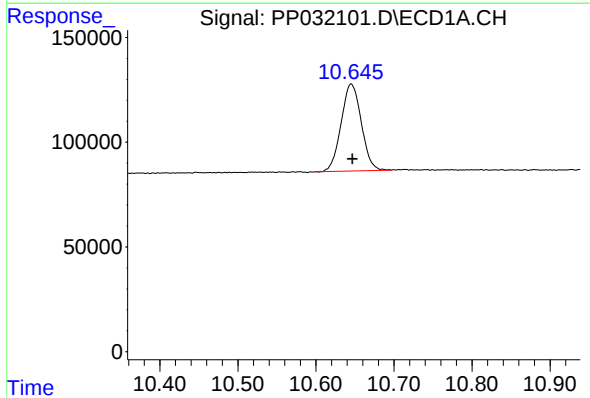

#2 Decachlorobiphenyl

R.T.: 10.645 min
Delta R.T.: -0.001 min
Response: 746415
Conc: 23.80 ng/ml

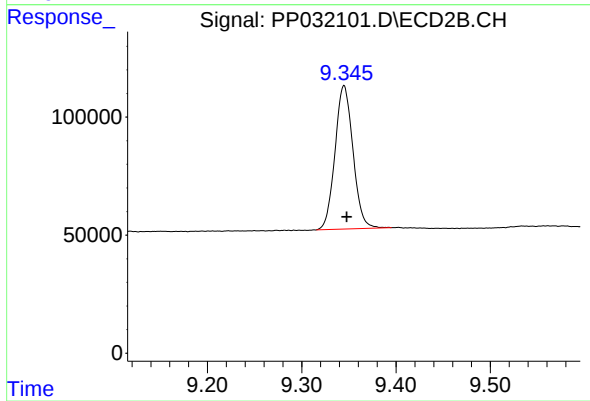

#2 Decachlorobiphenyl

R.T.: 9.345 min
Delta R.T.: -0.003 min
Response: 805031
Conc: 24.00 ng/ml