

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121520\
 Data File : PP032136.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Dec 2020 10:03
 Operator : DD\AJ
 Sample : L5043-08MSD
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KENS-SS2-121020-0-7MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 04:28:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.778	4.050	1266738	1068138	24.591	22.584
2)	SA Decachlor...	10.638	9.339	857443	905643	27.342	27.005
Target Compounds							
3)	L1 AR-1016-1	6.081	5.300	841075	744461	576.647	569.531
4)	L1 AR-1016-2	6.104	5.320	1258664	1127520	560.347	569.487
5)	L1 AR-1016-3	6.170	5.512	782158	614193	565.895	574.358
6)	L1 AR-1016-4	6.275	5.563	666317	455513	577.814	536.836
7)	L1 AR-1016-5	6.589	5.790	594496	264176	557.173	243.118 #
8)	L2 AR-1221-1	5.019	4.303	99091	80283	190.399	167.819
9)	L2 AR-1221-2	5.121	4.404	110752	94189	279.244	261.737
10)	L2 AR-1221-3	5.206	4.492	474481	423023	393.817	378.229
11)	L3 AR-1232-1	5.206	4.492	474481	423023	458.847	456.584
12)	L3 AR-1232-2	5.789	5.320	688540	1127520	1284.025	1314.069
13)	L3 AR-1232-3	6.104	5.512	1258664	614193	1309.087	1352.685
14)	L3 AR-1232-4	6.275	5.607	666317	554892	1392.434	1414.358
15)	L3 AR-1232-5	6.374	5.790	459628	264176	1510.001	610.767 #
16)	L4 AR-1242-1	6.081	5.300	841075	744461	734.064	718.735
17)	L4 AR-1242-2	6.104	5.320	1258664	1127520	714.600	729.446
18)	L4 AR-1242-3	6.170	5.512	782158	614193	704.814	729.463
19)	L4 AR-1242-4	6.275	5.607	666317	554892	732.186	684.116
20)	L4 AR-1242-5	7.054	6.170	184595	500892	212.819	563.224 #
21)	L5 AR-1248-1	6.081	5.300	841075	744461	966.333	951.423
22)	L5 AR-1248-2	6.374	5.563	459628	455513	388.026	394.269
23)	L5 AR-1248-3	6.589	5.607	594496	554892	407.494	454.267
24)	L5 AR-1248-4	7.015	5.790	180285	264176	126.021	180.158 #
25)	L5 AR-1248-5	7.054	6.213	184595	85144	124.400	67.864 #
26)	L6 AR-1254-1	6.988	6.170	281421	500892	181.183	242.325 #
27)	L6 AR-1254-2	7.213	6.328	455799	434741	198.149	242.503
28)	L6 AR-1254-3	7.598	6.766	817693	1010207	335.818	353.465
29)	L6 AR-1254-4	7.885	6.988	606514	176377	394.042	127.630 #
30)	L6 AR-1254-5	8.313	7.415	1748706	1605980	1020.331	675.061 #
31)	L7 AR-1260-1	7.760	6.884	1507067	1376385	869.582	725.998
32)	L7 AR-1260-2	8.025	7.081	1683706	1625251	819.484	747.113
33)	L7 AR-1260-3	8.390	7.235	1125009	1429544	644.720	672.831
34)	L7 AR-1260-4	8.618	7.718	1173632	945688	651.292	532.301
35)	L7 AR-1260-5	8.932	7.965	2079503	2218270	578.458	579.866
36)	L8 AR-1262-1	8.390	7.455	1125009	1033074	416.931	384.404
37)	L8 AR-1262-2	8.932	7.965	2079503	2218270	512.797	531.999
38)	L8 AR-1262-3	9.245	8.250	1265625	442226	441.678	244.093 #
39)	L8 AR-1262-4	9.314	8.312	311897	1630119	127.943	484.529 #
40)	L8 AR-1262-5	9.940	8.811	473888	509727	349.578	389.068
41)	L9 AR-1268-1	9.245	8.250	1265625	442226	243.565	87.749 #
42)	L9 AR-1268-2	9.314	8.312	311897	1630119	64.077	318.827 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121520\
 Data File : PP032136.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Dec 2020 10:03
 Operator : DD\AJ
 Sample : L5043-08MSD
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KENS-SS2-121020-0-7MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 04:28:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	8.521	0	43457	N.D.	9.856 #
44) L9	AR-1268-4	9.940	8.811	473888	509727	341.101	348.790
45) L9	AR-1268-5	10.326	9.094	162502	178395	13.492	14.107



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121520\
Data File : PP032136.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Dec 2020 10:03
Operator : DD\AJ
Sample : L5043-08MSD
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 04:28:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

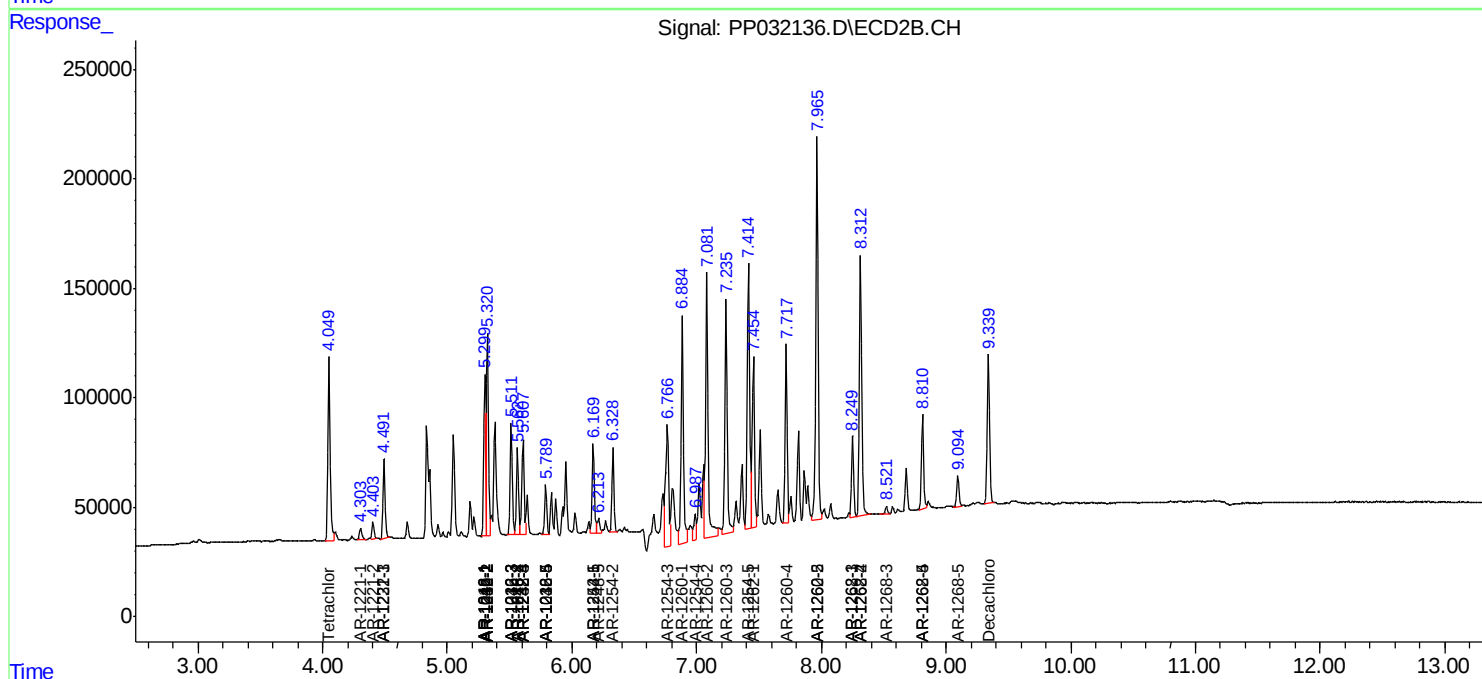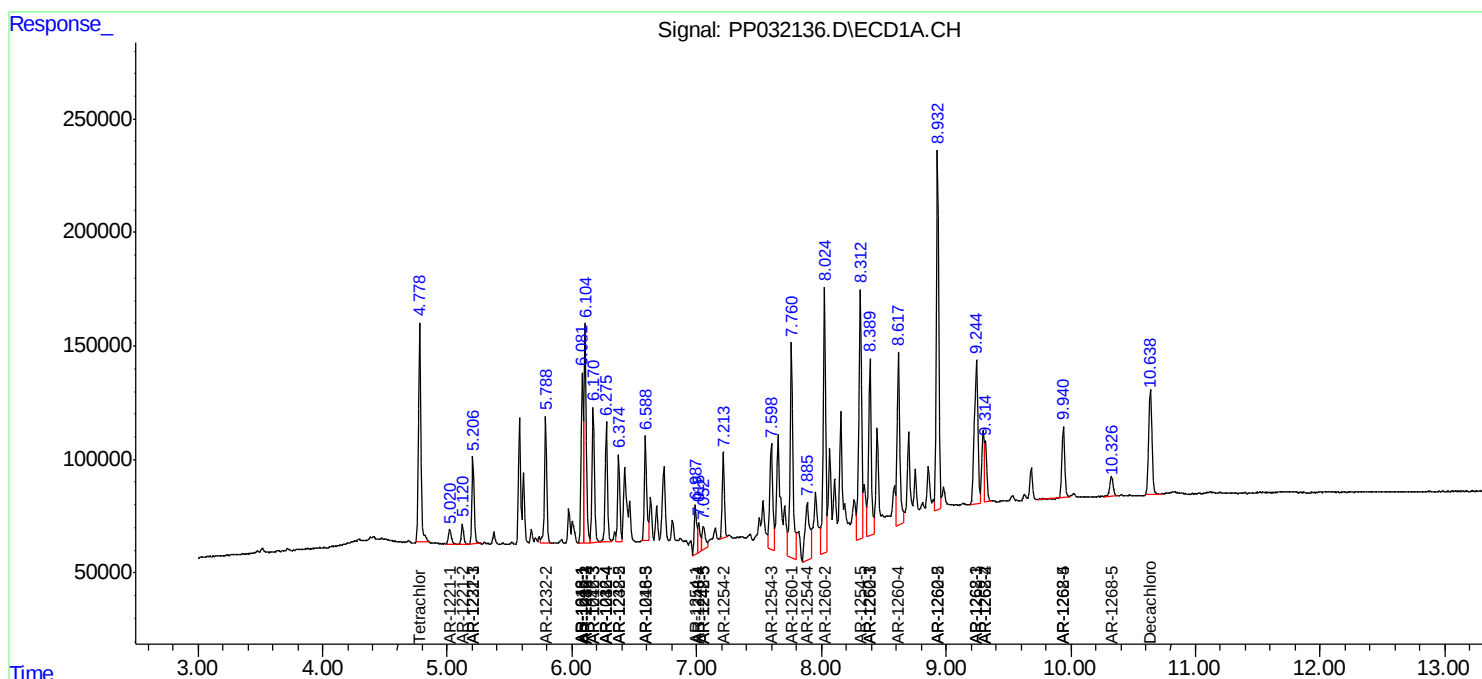




#1 Tetrachloro-m-xylene


R.T.: 4.778 min
Delta R.T.: -0.004 min
Response: 1266738
Conc: 24.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

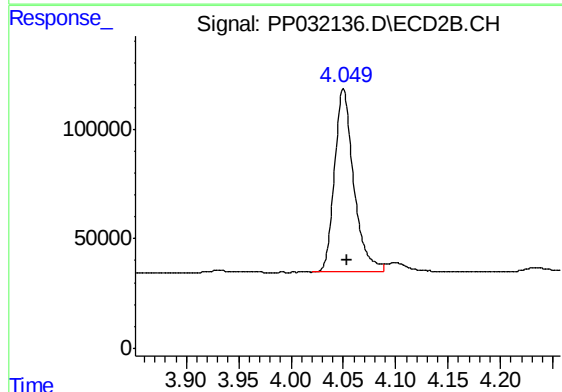


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.004 min
Response: 1068138
Conc: 22.58 ng/ml

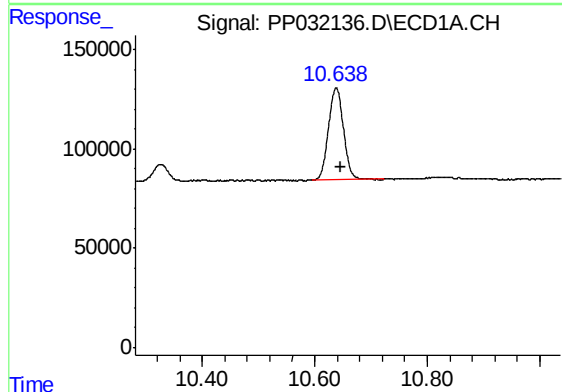


#2 Decachlorobiphenyl

R.T.: 10.638 min
Delta R.T.: -0.009 min
Response: 857443
Conc: 27.34 ng/ml

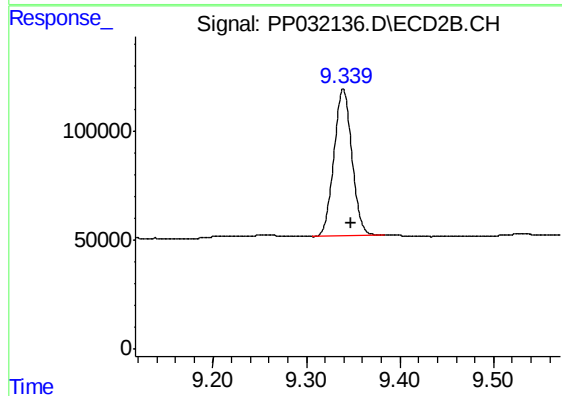

#2 Decachlorobiphenyl


R.T.: 9.339 min
Delta R.T.: -0.009 min
Response: 905643
Conc: 27.00 ng/ml

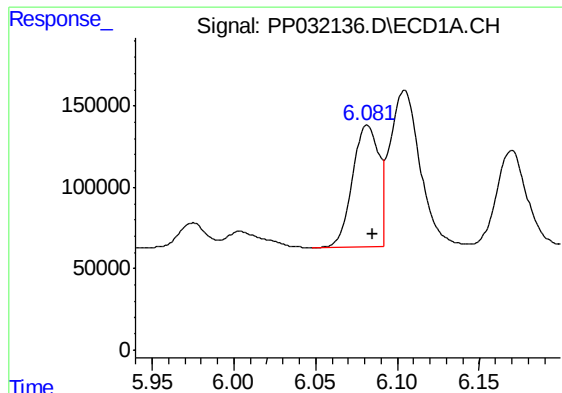

#3 AR-1016-1


R.T.: 6.081 min
Delta R.T.: -0.003 min
Response: 841075
Conc: 576.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

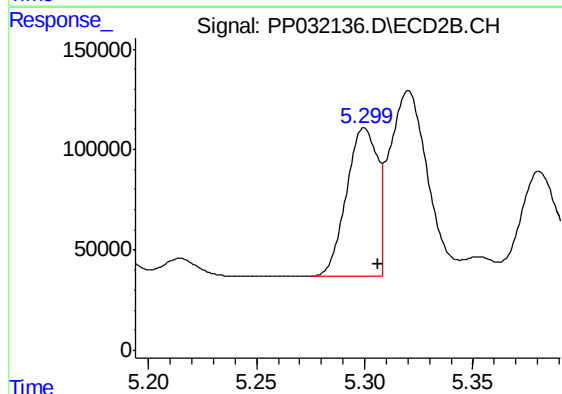


#3 AR-1016-1

R.T.: 5.300 min
Delta R.T.: -0.006 min
Response: 744461
Conc: 569.53 ng/ml




#4 AR-1016-2

R.T.: 6.104 min
Delta R.T.: -0.003 min
Response: 1258664
Conc: 560.35 ng/ml

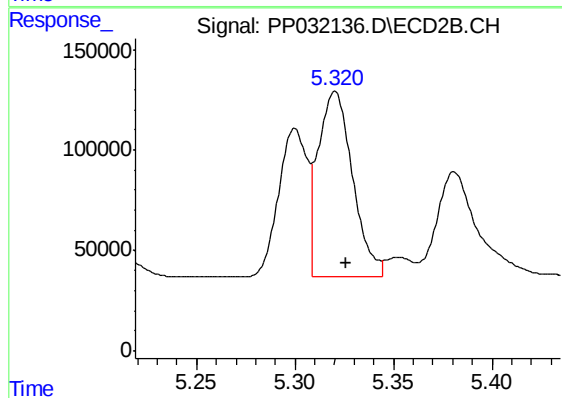

#4 AR-1016-2


R.T.: 5.320 min
Delta R.T.: -0.006 min
Response: 1127520
Conc: 569.49 ng/ml



#5 AR-1016-3


R.T.: 6.170 min
Delta R.T.: -0.004 min
Response: 782158
Conc: 565.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

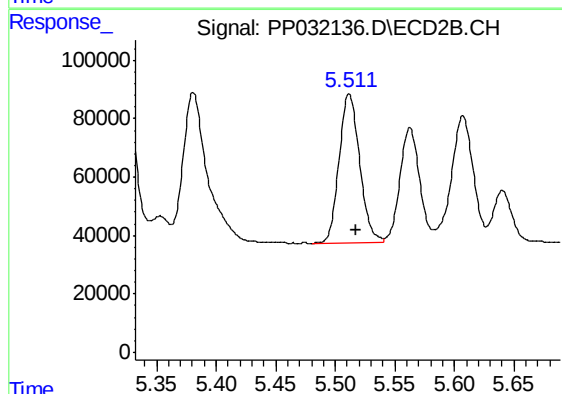


#5 AR-1016-3

R.T.: 5.512 min
Delta R.T.: -0.006 min
Response: 614193
Conc: 574.36 ng/ml

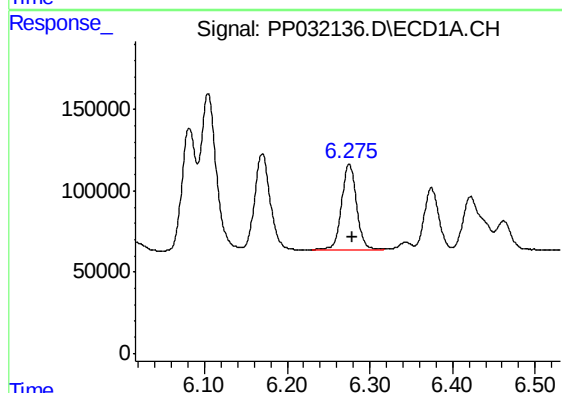


#6 AR-1016-4

R.T.: 6.275 min
Delta R.T.: -0.004 min
Response: 666317
Conc: 577.81 ng/ml

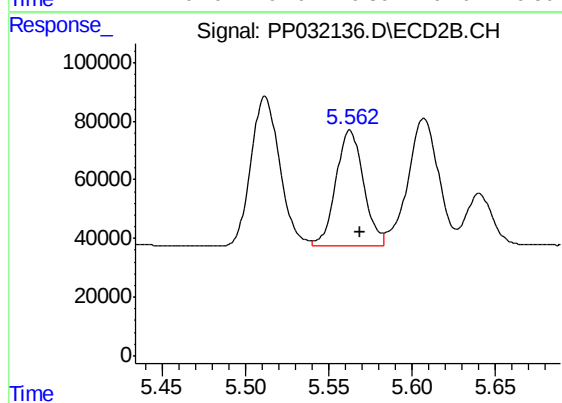

#6 AR-1016-4


R.T.: 5.563 min
Delta R.T.: -0.006 min
Response: 455513
Conc: 536.84 ng/ml



#7 AR-1016-5


R.T.: 6.589 min
Delta R.T.: -0.004 min
Response: 594496
Conc: 557.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

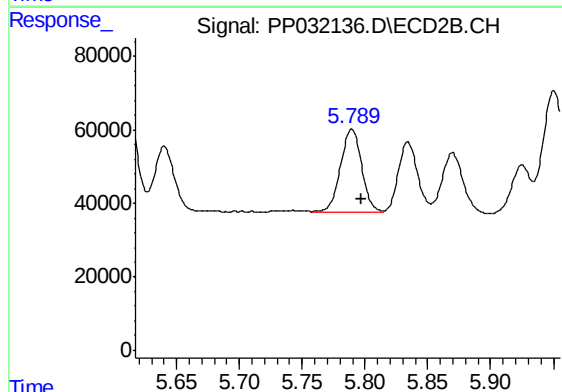


#7 AR-1016-5

R.T.: 5.790 min
Delta R.T.: -0.008 min
Response: 264176
Conc: 243.12 ng/ml




#8 AR-1221-1

R.T.: 5.019 min
Delta R.T.: -0.007 min
Response: 99091
Conc: 190.40 ng/ml

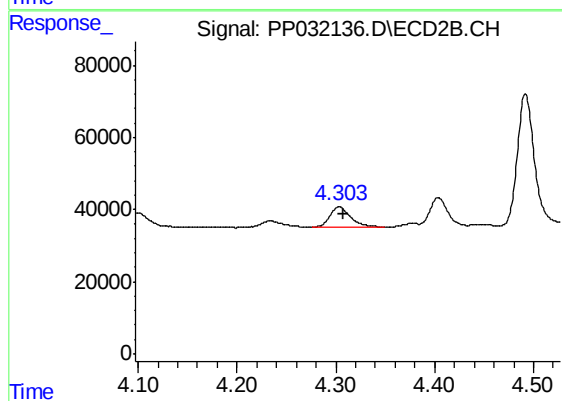

#8 AR-1221-1


R.T.: 4.303 min
Delta R.T.: -0.004 min
Response: 80283
Conc: 167.82 ng/ml

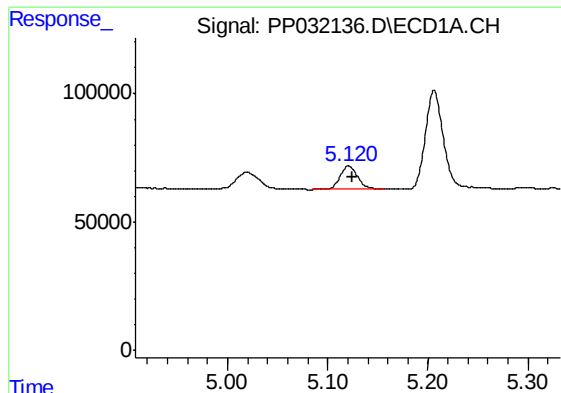

#9 AR-1221-2


R.T.: 5.121 min
Delta R.T.: -0.003 min
Response: 110752
Conc: 279.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

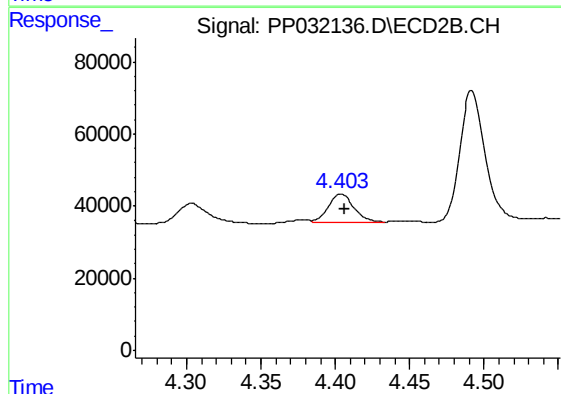


#9 AR-1221-2

R.T.: 4.404 min
Delta R.T.: -0.003 min
Response: 94189
Conc: 261.74 ng/ml

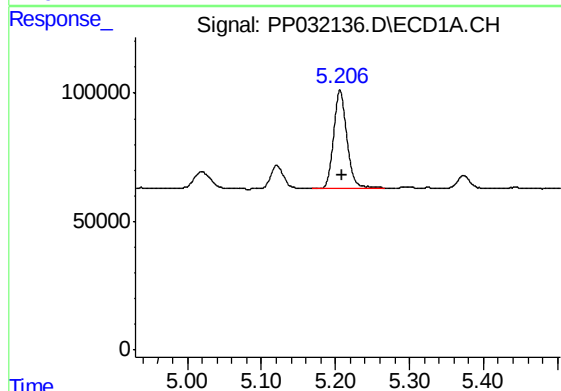


#10 AR-1221-3

R.T.: 5.206 min
Delta R.T.: -0.003 min
Response: 474481
Conc: 393.82 ng/ml

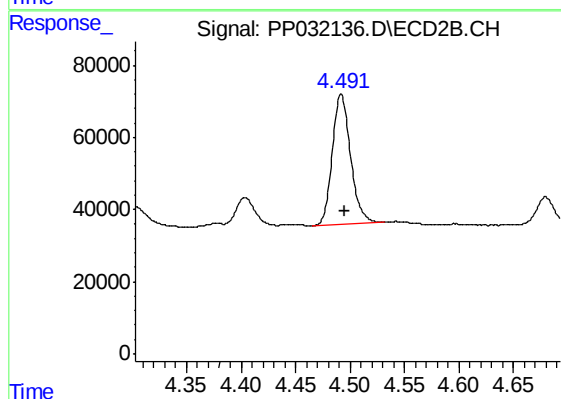

#10 AR-1221-3


R.T.: 4.492 min
Delta R.T.: -0.003 min
Response: 423023
Conc: 378.23 ng/ml

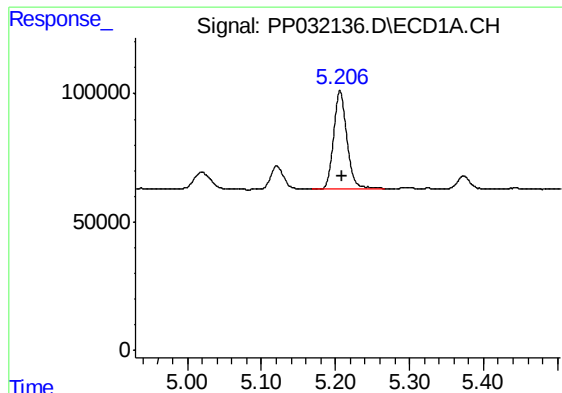

#11 AR-1232-1


R.T.: 5.206 min
Delta R.T.: -0.003 min
Response: 474481
Conc: 458.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

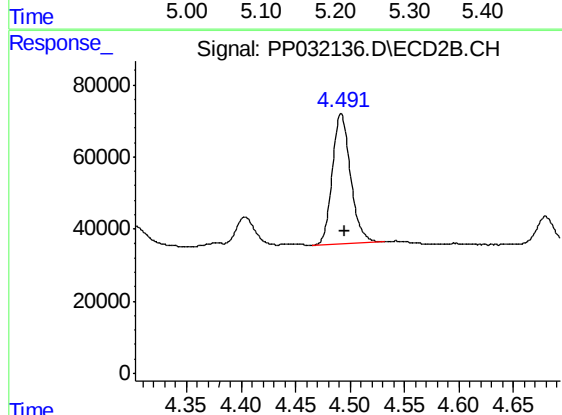


#11 AR-1232-1

R.T.: 4.492 min
Delta R.T.: -0.004 min
Response: 423023
Conc: 456.58 ng/ml

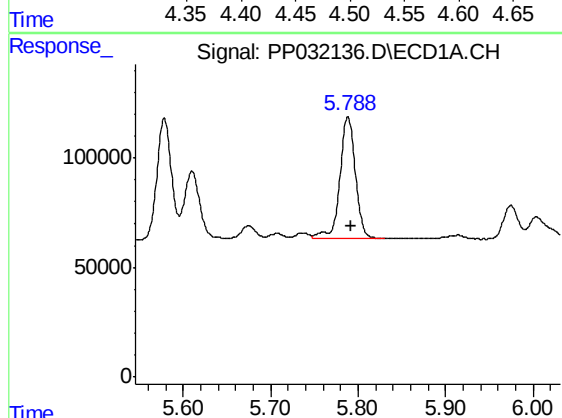


#12 AR-1232-2

R.T.: 5.789 min
Delta R.T.: -0.004 min
Response: 688540
Conc: 1284.02 ng/ml

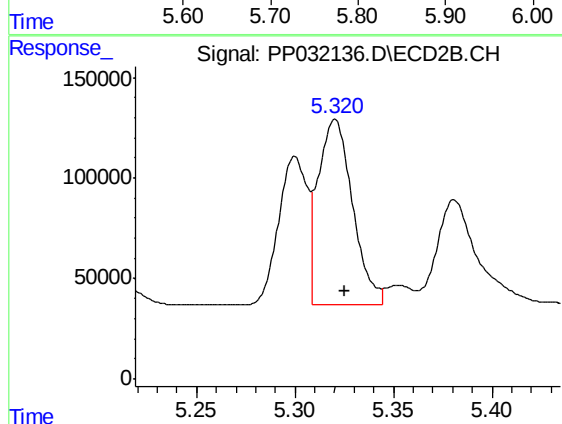

#12 AR-1232-2


R.T.: 5.320 min
Delta R.T.: -0.005 min
Response: 1127520
Conc: 1314.07 ng/ml



#13 AR-1232-3


R.T.: 6.104 min
Delta R.T.: -0.003 min
Response: 1258664
Conc: 1309.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

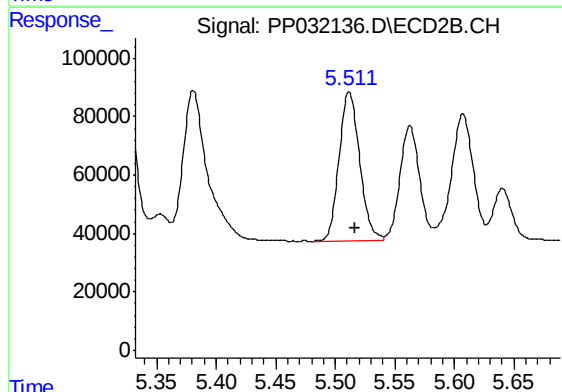


#13 AR-1232-3

R.T.: 5.512 min
Delta R.T.: -0.005 min
Response: 614193
Conc: 1352.68 ng/ml

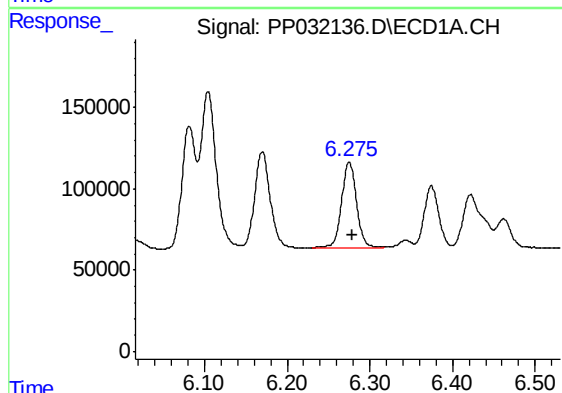


#14 AR-1232-4

R.T.: 6.275 min
Delta R.T.: -0.004 min
Response: 666317
Conc: 1392.43 ng/ml

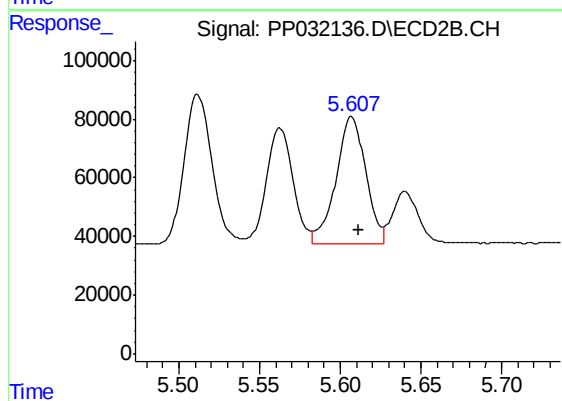

#14 AR-1232-4


R.T.: 5.607 min
Delta R.T.: -0.005 min
Response: 554892
Conc: 1414.36 ng/ml

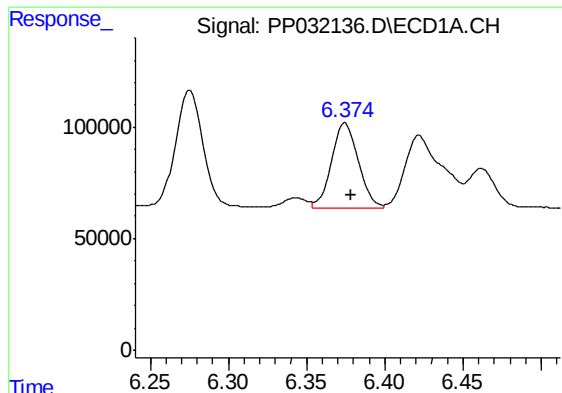

#15 AR-1232-5


R.T.: 6.374 min
Delta R.T.: -0.004 min
Response: 459628
Conc: 1510.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

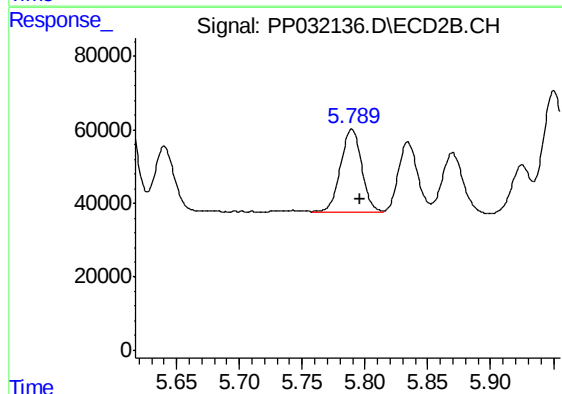


#15 AR-1232-5

R.T.: 5.790 min
Delta R.T.: -0.007 min
Response: 264176
Conc: 610.77 ng/ml

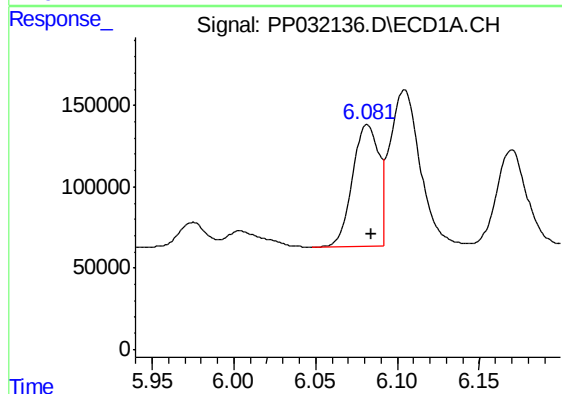


#16 AR-1242-1

R.T.: 6.081 min
Delta R.T.: -0.003 min
Response: 841075
Conc: 734.06 ng/ml

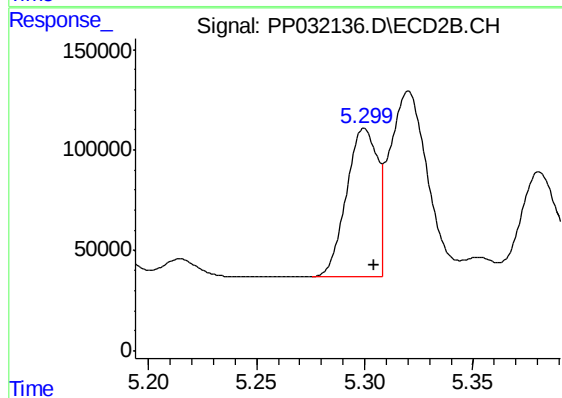

#16 AR-1242-1


R.T.: 5.300 min
Delta R.T.: -0.005 min
Response: 744461
Conc: 718.73 ng/ml



#17 AR-1242-2


R.T.: 6.104 min
Delta R.T.: -0.003 min
Response: 1258664
Conc: 714.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

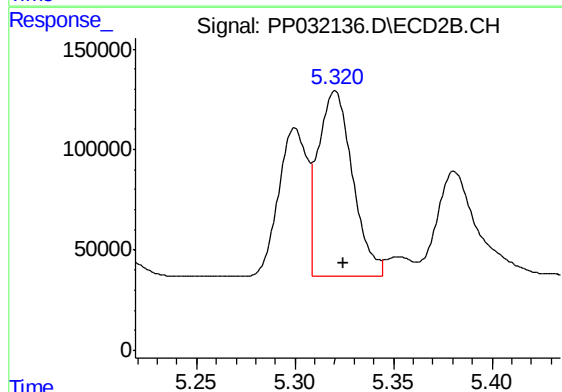


#17 AR-1242-2

R.T.: 5.320 min
Delta R.T.: -0.005 min
Response: 1127520
Conc: 729.45 ng/ml

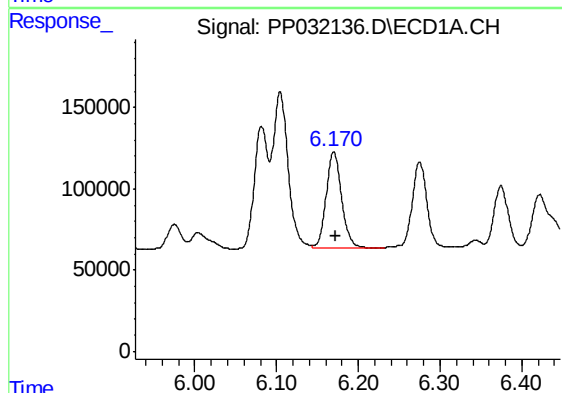


#18 AR-1242-3

R.T.: 6.170 min
Delta R.T.: -0.003 min
Response: 782158
Conc: 704.81 ng/ml

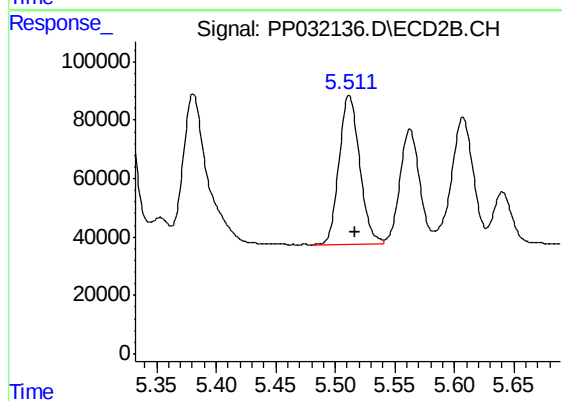

#18 AR-1242-3


R.T.: 5.512 min
Delta R.T.: -0.005 min
Response: 614193
Conc: 729.46 ng/ml



#19 AR-1242-4


R.T.: 6.275 min
Delta R.T.: -0.003 min
Response: 666317
Conc: 732.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

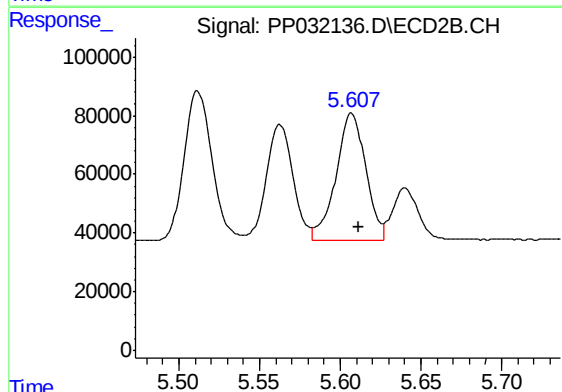


#19 AR-1242-4

R.T.: 5.607 min
Delta R.T.: -0.004 min
Response: 554892
Conc: 684.12 ng/ml




#20 AR-1242-5

R.T.: 7.054 min
Delta R.T.: -0.003 min
Response: 184595
Conc: 212.82 ng/ml

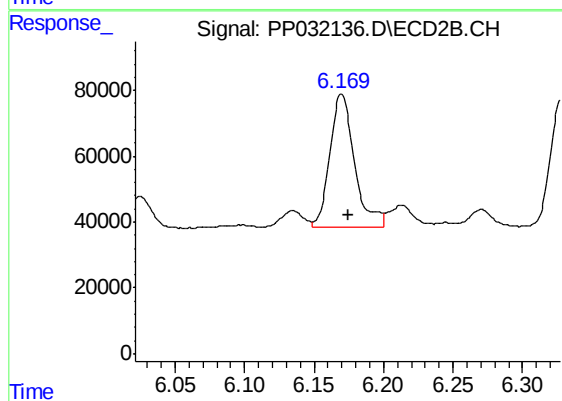

#20 AR-1242-5


R.T.: 6.170 min
Delta R.T.: -0.005 min
Response: 500892
Conc: 563.22 ng/ml

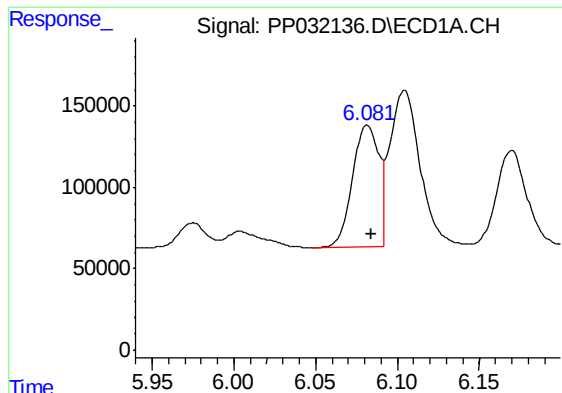

#21 AR-1248-1


R.T.: 6.081 min
Delta R.T.: -0.003 min
Response: 841075
Conc: 966.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

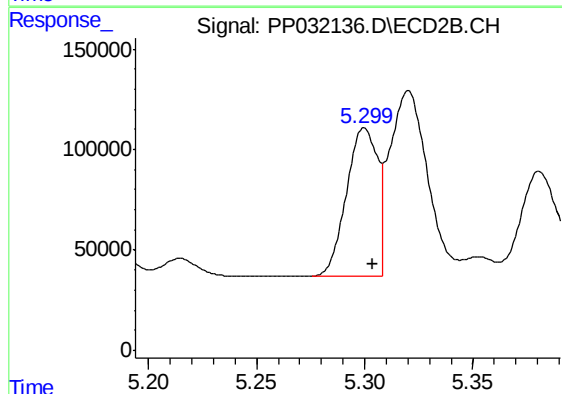


#21 AR-1248-1

R.T.: 5.300 min
Delta R.T.: -0.004 min
Response: 744461
Conc: 951.42 ng/ml

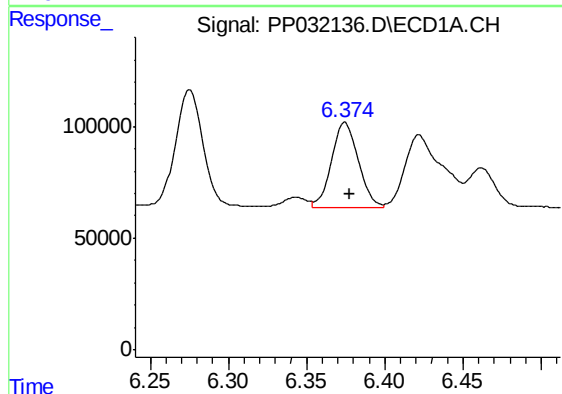


#22 AR-1248-2

R.T.: 6.374 min
Delta R.T.: -0.003 min
Response: 459628
Conc: 388.03 ng/ml

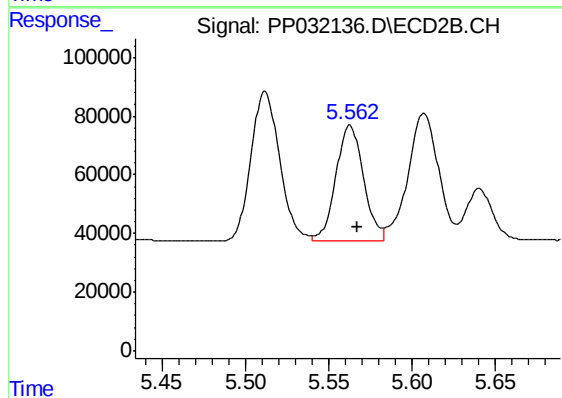

#22 AR-1248-2


R.T.: 5.563 min
Delta R.T.: -0.004 min
Response: 455513
Conc: 394.27 ng/ml



#23 AR-1248-3


R.T.: 6.589 min
Delta R.T.: -0.003 min
Response: 594496
Conc: 407.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

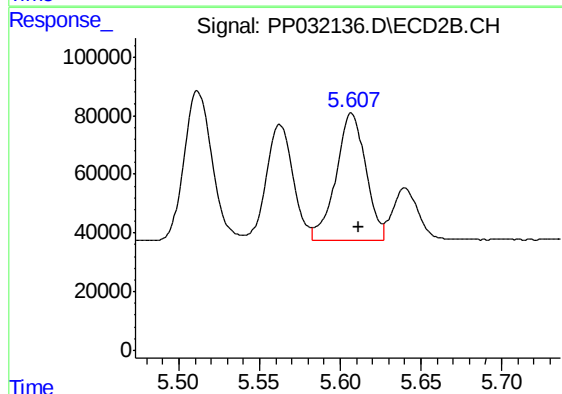


#23 AR-1248-3

R.T.: 5.607 min
Delta R.T.: -0.004 min
Response: 554892
Conc: 454.27 ng/ml




#24 AR-1248-4

R.T.: 7.015 min
Delta R.T.: -0.003 min
Response: 180285
Conc: 126.02 ng/ml

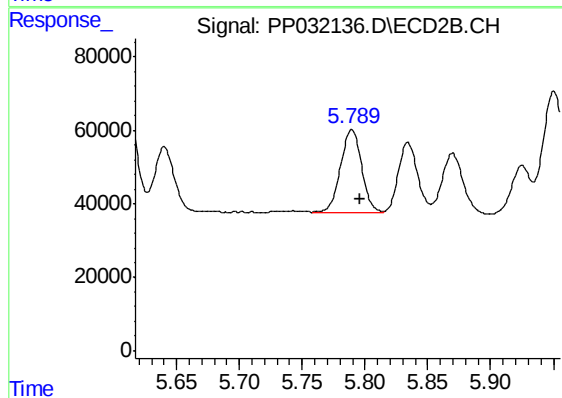

#24 AR-1248-4


R.T.: 5.790 min
Delta R.T.: -0.007 min
Response: 264176
Conc: 180.16 ng/ml

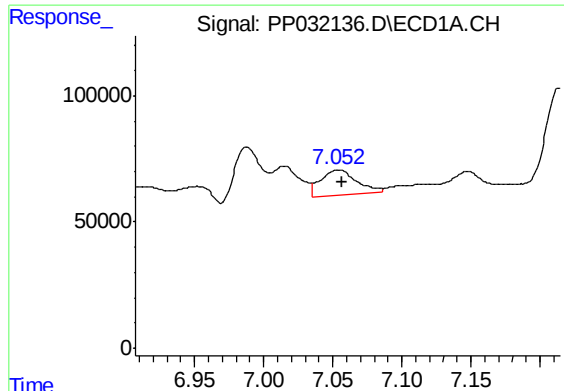

#25 AR-1248-5


R.T.: 7.054 min
Delta R.T.: -0.003 min
Response: 184595
Conc: 124.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

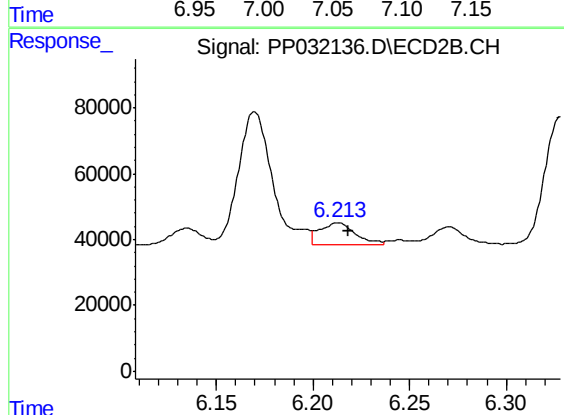


#25 AR-1248-5

R.T.: 6.213 min
Delta R.T.: -0.005 min
Response: 85144
Conc: 67.86 ng/ml

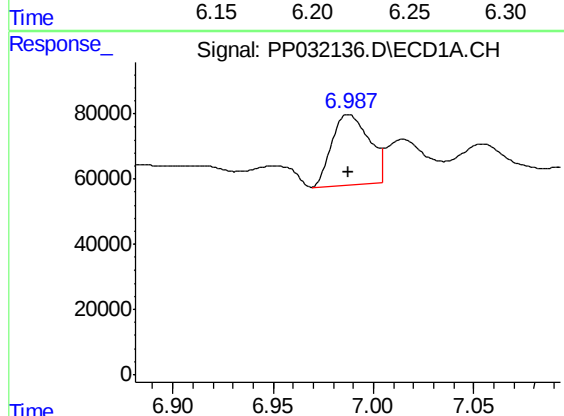


#26 AR-1254-1

R.T.: 6.988 min
Delta R.T.: 0.000 min
Response: 281421
Conc: 181.18 ng/ml

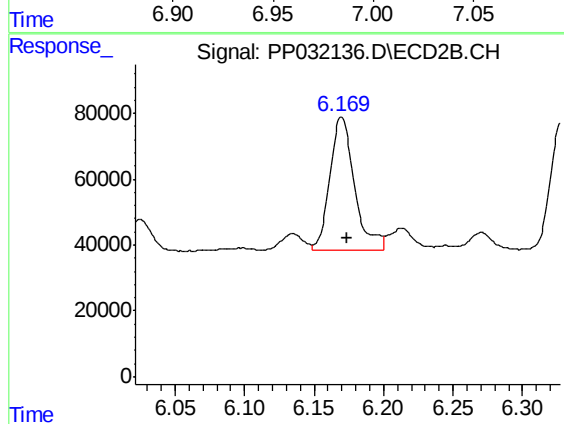

#26 AR-1254-1


R.T.: 6.170 min
Delta R.T.: -0.004 min
Response: 500892
Conc: 242.32 ng/ml

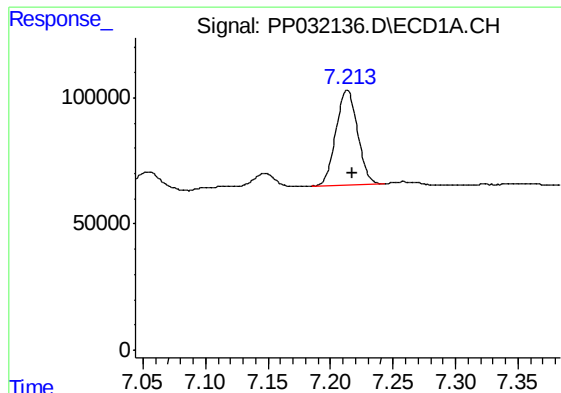

#27 AR-1254-2


R.T.: 7.213 min
Delta R.T.: -0.004 min
Response: 455799
Conc: 198.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

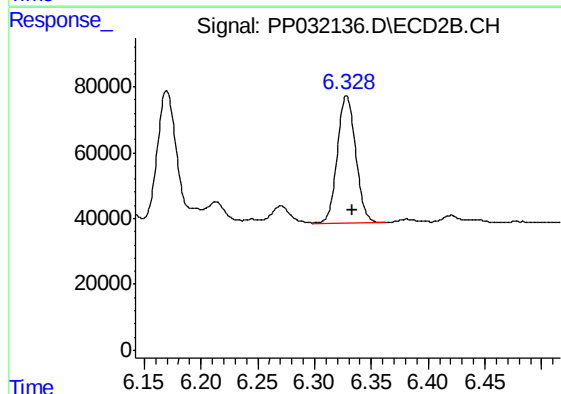


#27 AR-1254-2

R.T.: 6.328 min
Delta R.T.: -0.005 min
Response: 434741
Conc: 242.50 ng/ml

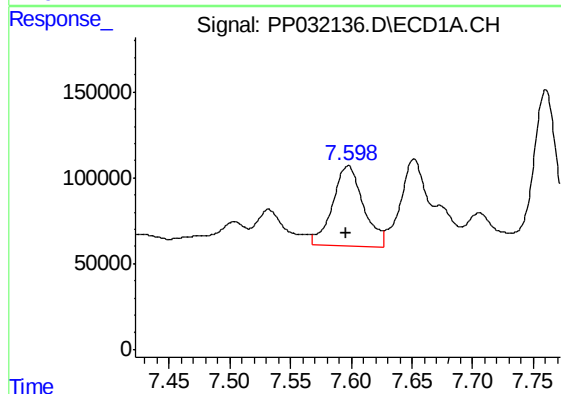


#28 AR-1254-3

R.T.: 7.598 min
Delta R.T.: 0.002 min
Response: 817693
Conc: 335.82 ng/ml

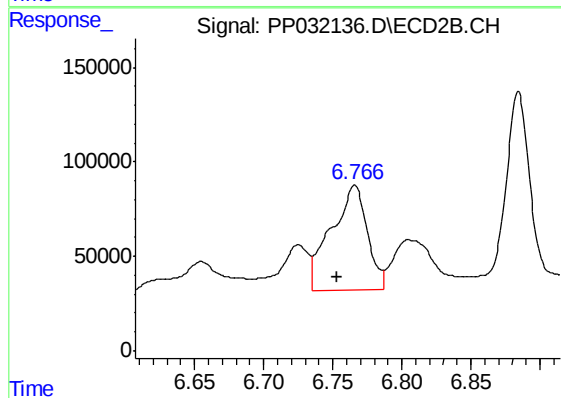

#28 AR-1254-3


R.T.: 6.766 min
Delta R.T.: 0.013 min
Response: 1010207
Conc: 353.47 ng/ml

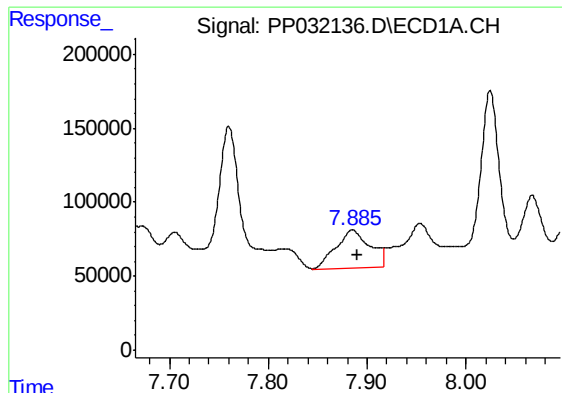

#29 AR-1254-4


R.T.: 7.885 min
Delta R.T.: -0.005 min
Response: 606514
Conc: 394.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

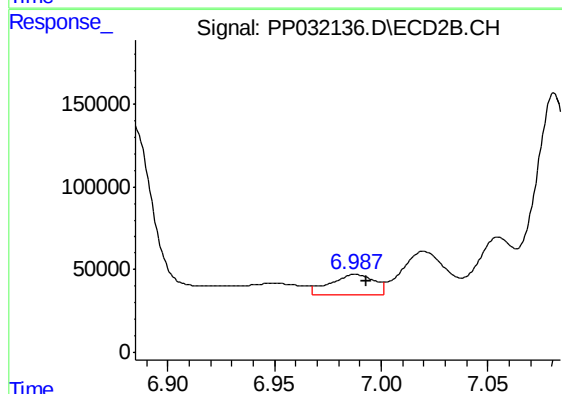


#29 AR-1254-4

R.T.: 6.988 min
Delta R.T.: -0.005 min
Response: 176377
Conc: 127.63 ng/ml

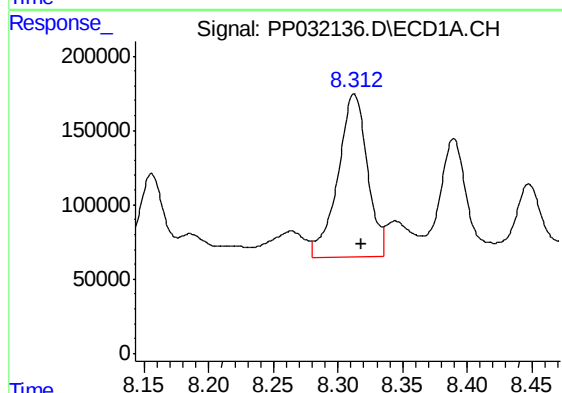


#30 AR-1254-5

R.T.: 8.313 min
Delta R.T.: -0.005 min
Response: 1748706
Conc: 1020.33 ng/ml

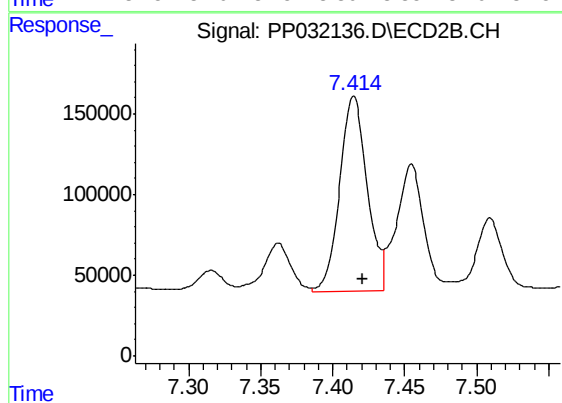

#30 AR-1254-5


R.T.: 7.415 min
Delta R.T.: -0.006 min
Response: 1605980
Conc: 675.06 ng/ml



#31 AR-1260-1


R.T.: 7.760 min
Delta R.T.: -0.004 min
Response: 1507067
Conc: 869.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

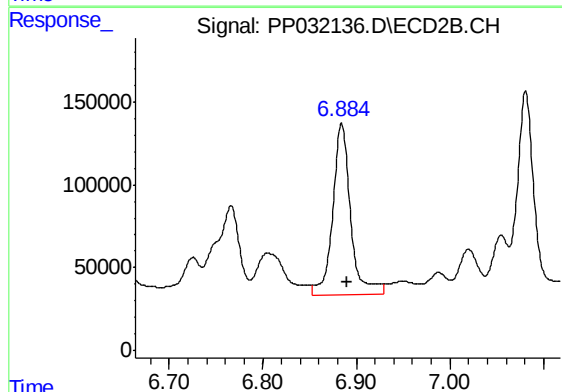


#31 AR-1260-1

R.T.: 6.884 min
Delta R.T.: -0.006 min
Response: 1376385
Conc: 726.00 ng/ml

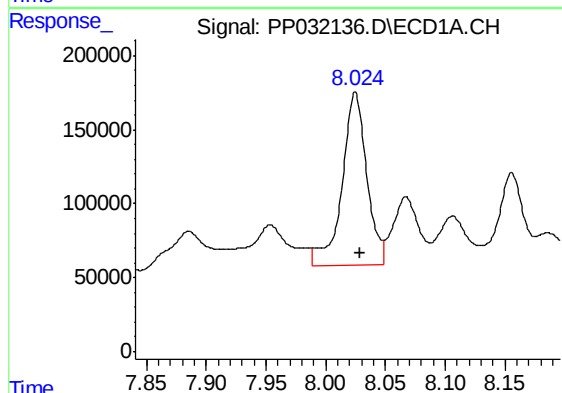


#32 AR-1260-2

R.T.: 8.025 min
Delta R.T.: -0.005 min
Response: 1683706
Conc: 819.48 ng/ml

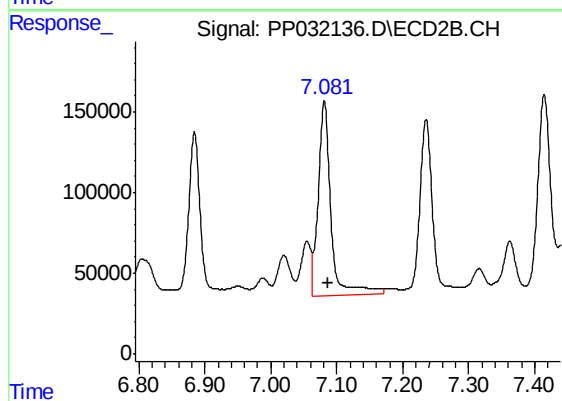

#32 AR-1260-2


R.T.: 7.081 min
Delta R.T.: -0.007 min
Response: 1625251
Conc: 747.11 ng/ml



#33 AR-1260-3


R.T.: 8.390 min
Delta R.T.: -0.005 min
Response: 1125009
Conc: 644.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

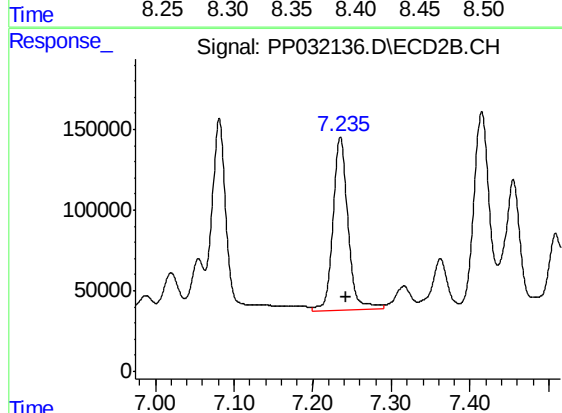


#33 AR-1260-3

R.T.: 7.235 min
Delta R.T.: -0.008 min
Response: 1429544
Conc: 672.83 ng/ml

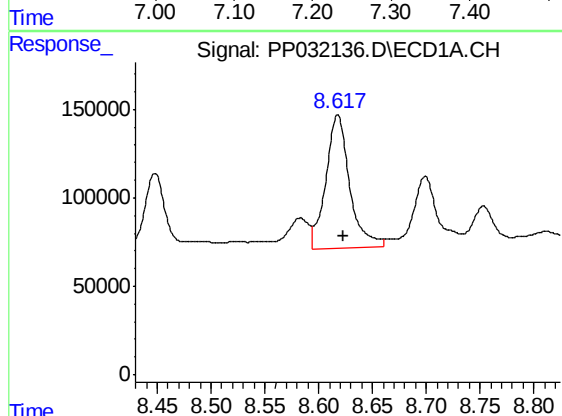


#34 AR-1260-4

R.T.: 8.618 min
Delta R.T.: -0.005 min
Response: 1173632
Conc: 651.29 ng/ml

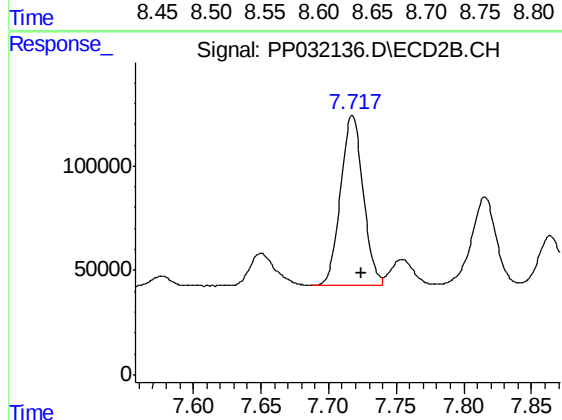

#34 AR-1260-4


R.T.: 7.718 min
Delta R.T.: -0.007 min
Response: 945688
Conc: 532.30 ng/ml



#35 AR-1260-5


R.T.: 8.932 min
Delta R.T.: -0.004 min
Response: 2079503
Conc: 578.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

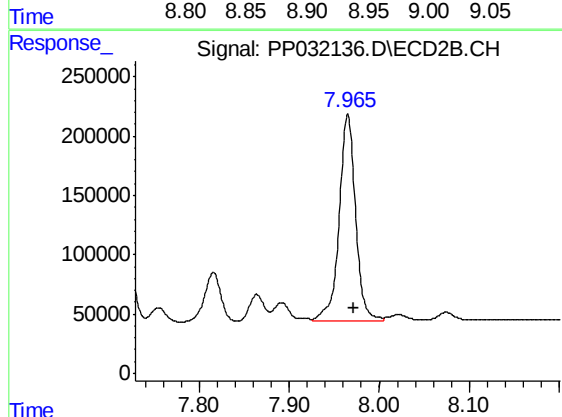


#35 AR-1260-5

R.T.: 7.965 min
Delta R.T.: -0.007 min
Response: 2218270
Conc: 579.87 ng/ml

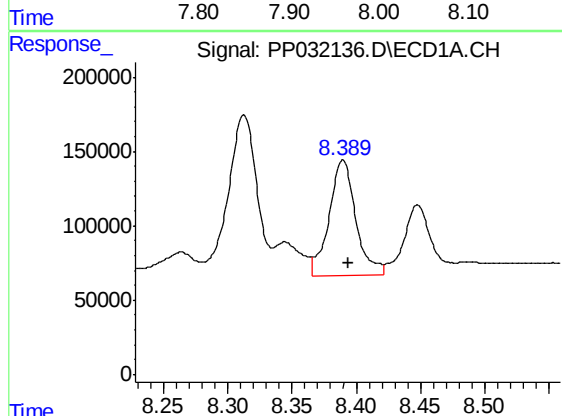


#36 AR-1262-1

R.T.: 8.390 min
Delta R.T.: -0.005 min
Response: 1125009
Conc: 416.93 ng/ml

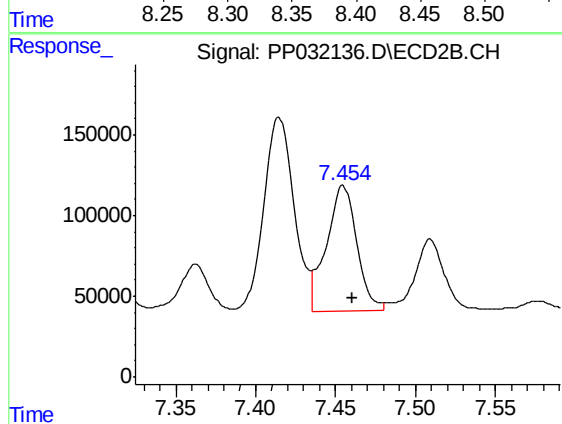

#36 AR-1262-1


R.T.: 7.455 min
Delta R.T.: -0.006 min
Response: 1033074
Conc: 384.40 ng/ml



#37 AR-1262-2


R.T.: 8.932 min
Delta R.T.: -0.004 min
Response: 2079503
Conc: 512.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

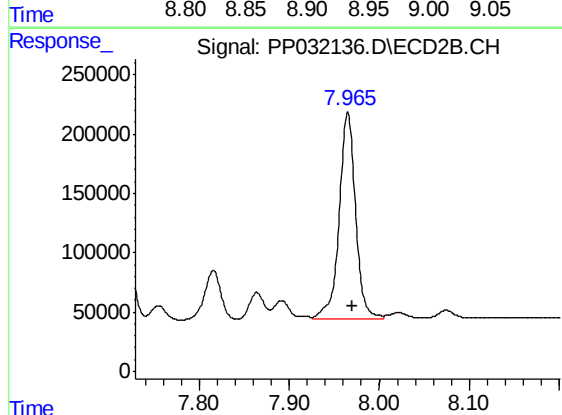


#37 AR-1262-2

R.T.: 7.965 min
Delta R.T.: -0.005 min
Response: 2218270
Conc: 532.00 ng/ml

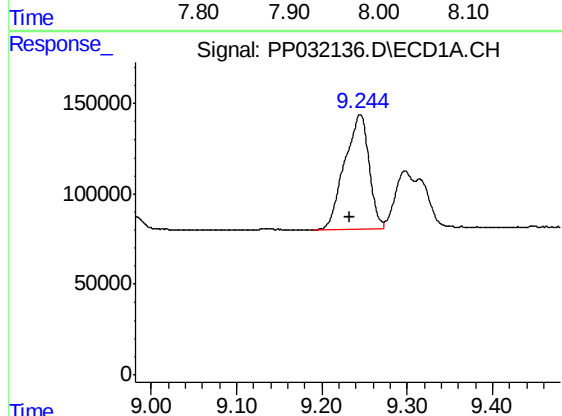


#38 AR-1262-3

R.T.: 9.245 min
Delta R.T.: 0.012 min
Response: 1265625
Conc: 441.68 ng/ml

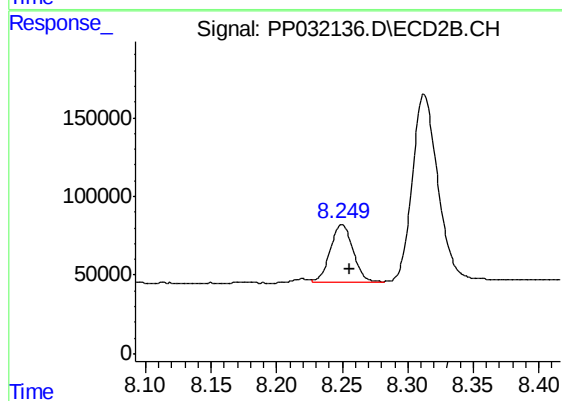

#38 AR-1262-3


R.T.: 8.250 min
Delta R.T.: -0.006 min
Response: 442226
Conc: 244.09 ng/ml

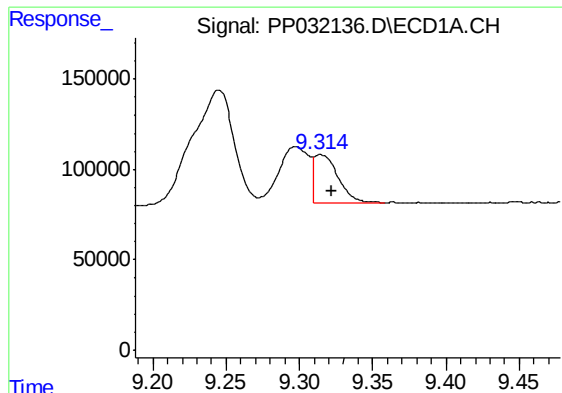

#39 AR-1262-4


R.T.: 9.314 min
Delta R.T.: -0.008 min
Response: 311897
Conc: 127.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

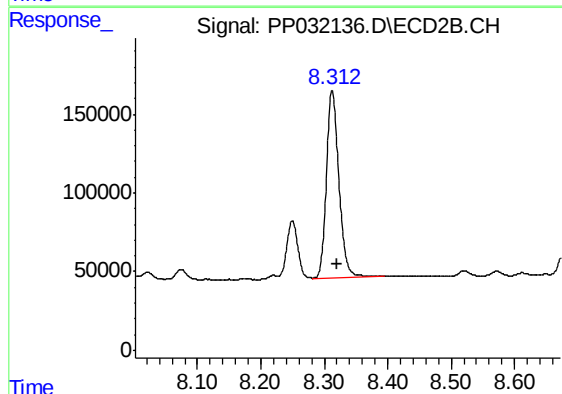


#39 AR-1262-4

R.T.: 8.312 min
Delta R.T.: -0.007 min
Response: 1630119
Conc: 484.53 ng/ml




#40 AR-1262-5

R.T.: 9.940 min
Delta R.T.: -0.006 min
Response: 473888
Conc: 349.58 ng/ml

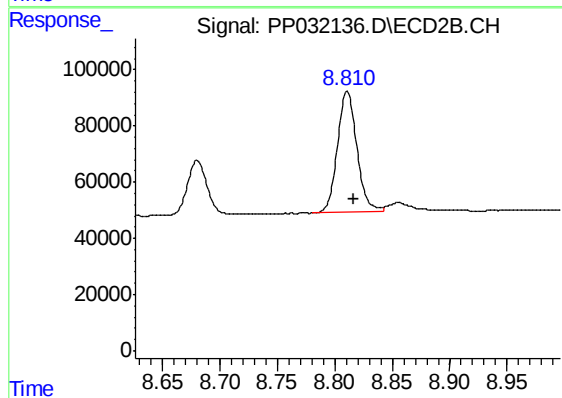

#40 AR-1262-5


R.T.: 8.811 min
Delta R.T.: -0.006 min
Response: 509727
Conc: 389.07 ng/ml



#41 AR-1268-1


R.T.: 9.245 min
Delta R.T.: 0.012 min
Response: 1265625
Conc: 243.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

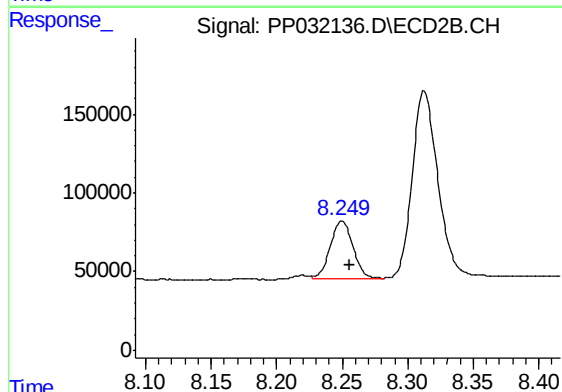


#41 AR-1268-1

R.T.: 8.250 min
Delta R.T.: -0.006 min
Response: 442226
Conc: 87.75 ng/ml




#42 AR-1268-2

R.T.: 9.314 min
Delta R.T.: -0.008 min
Response: 311897
Conc: 64.08 ng/ml

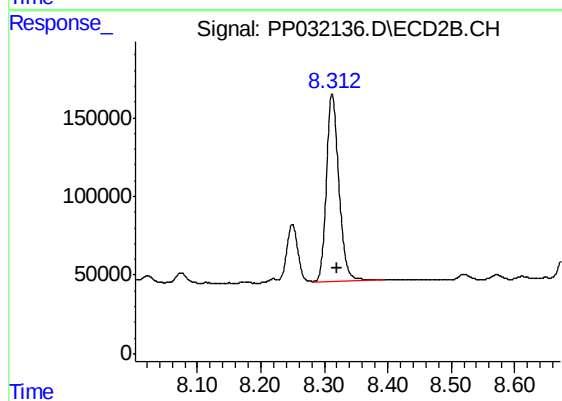

#42 AR-1268-2


R.T.: 8.312 min
Delta R.T.: -0.008 min
Response: 1630119
Conc: 318.83 ng/ml



#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.537 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

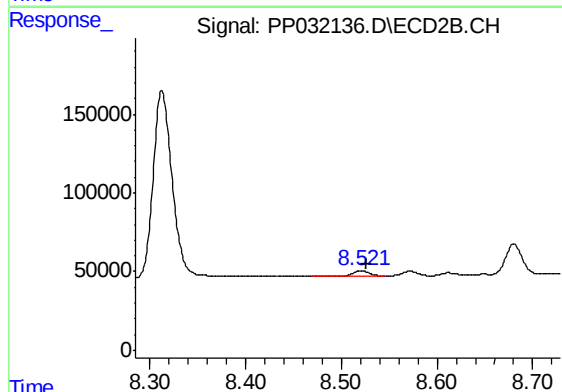


#43 AR-1268-3

R.T.: 8.521 min
Delta R.T.: -0.006 min
Response: 43457
Conc: 9.86 ng/ml




#44 AR-1268-4

R.T.: 9.940 min
Delta R.T.: -0.004 min
Response: 473888
Conc: 341.10 ng/ml

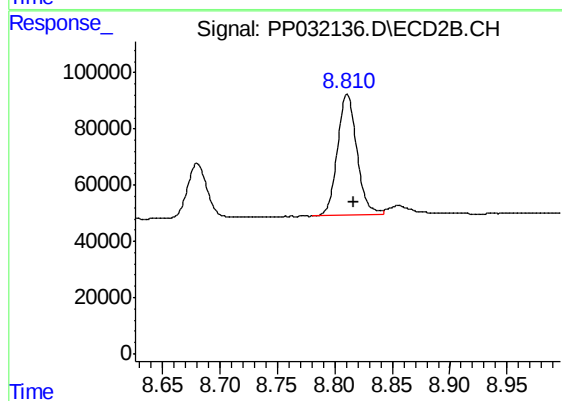

#44 AR-1268-4


R.T.: 8.811 min
Delta R.T.: -0.005 min
Response: 509727
Conc: 348.79 ng/ml

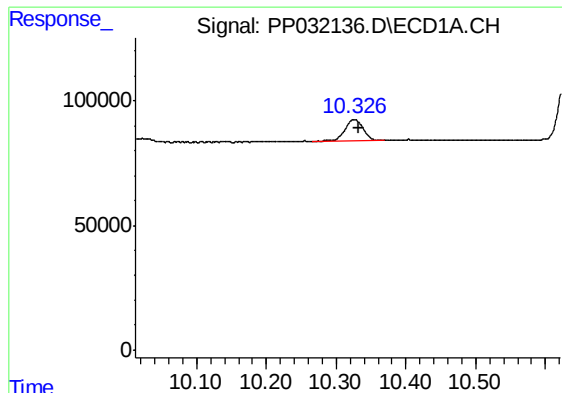

#45 AR-1268-5

R.T.: 10.326 min
Delta R.T.: -0.007 min
Response: 162502
Conc: 13.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
KENS-SS2-121020-0-7MSD

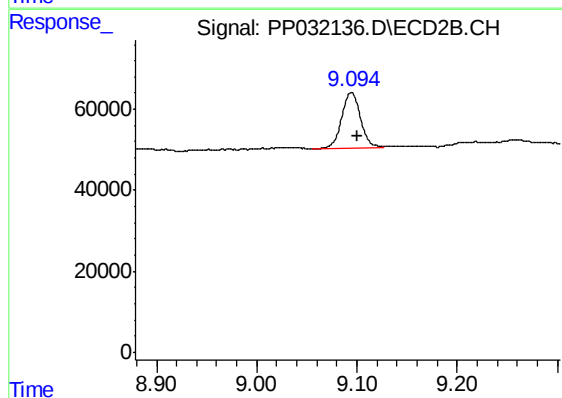

#45 AR-1268-5

R.T.: 9.094 min
Delta R.T.: -0.007 min
Response: 178395
Conc: 14.11 ng/ml