

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121520\
 Data File : PP032167.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Dec 2020 19:36
 Operator : DD\AJ
 Sample : L5090-05
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 GRAY-CHIPS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 04:50:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.777	4.049	1116405	987977	21.672	20.889
2)	SA Decachlor...	10.635	9.338	1317625	1453719	42.017	43.348
Target Compounds							
3)	L1 AR-1016-1	6.080	5.299	71245	43505	48.846	33.282 #
4)	L1 AR-1016-2	6.102	5.320	81877	100368	36.451	50.694 #
5)	L1 AR-1016-3	6.169	5.511	44260	58309	32.022	54.527 #
6)	L1 AR-1016-4	0.000	5.562	0	71280	N.D.	84.005 #
7)	L1 AR-1016-5	6.587	5.790	86154	52236	80.745	48.072 #
8)	L2 AR-1221-1	0.000	4.325f	0	27276	N.D.	57.016 #
10)	L2 AR-1221-3	0.000	4.492	0	32495	N.D.	29.054 #
11)	L3 AR-1232-1	0.000	4.492	0	32495	N.D.	35.073 #
12)	L3 AR-1232-2	0.000	5.320	0	100368	N.D.	116.975 #
13)	L3 AR-1232-3	6.102	5.511	81877	58309	85.157	128.418 #
14)	L3 AR-1232-4	0.000	5.605	0	35049	N.D.	89.336 #
15)	L3 AR-1232-5	6.374	5.790	81544	52236	267.893	120.768 #
16)	L4 AR-1242-1	6.080	5.299	71245	43505	62.180	42.002 #
17)	L4 AR-1242-2	6.102	5.320	81877	100368	46.485	64.933 #
18)	L4 AR-1242-3	6.169	5.511	44260	58309	39.883	69.252 #
19)	L4 AR-1242-4	0.000	5.605	0	35049	N.D.	43.211 #
20)	L4 AR-1242-5	7.054	6.168	167967	288056	193.648	323.902 #
21)	L5 AR-1248-1	6.080	5.299	71245	43505	81.855	55.600 #
22)	L5 AR-1248-2	6.374	5.562	81544	71280	68.841	61.696
23)	L5 AR-1248-3	6.587	5.605	86154	35049	59.054	28.693 #
24)	L5 AR-1248-4	7.013	5.790	131157	52236	91.681	35.623 #
25)	L5 AR-1248-5	7.054	6.212	167967	90105	113.194	71.818 #
26)	L6 AR-1254-1	6.984	6.168	156761	288056	100.925	139.357 #
27)	L6 AR-1254-2	7.213	6.327	336280	182831	146.191	101.985 #
28)	L6 AR-1254-3	7.592	6.748	387742	297425	159.241	104.067 #
29)	L6 AR-1254-4	7.886	6.986	213823	204009	138.917	147.625
30)	L6 AR-1254-5	8.313	7.414	235824	1486295	137.598	624.753 #
31)	L7 AR-1260-1	7.756	6.882	137734	247391	79.473	130.491 #
32)	L7 AR-1260-2	8.020	7.081	545396	386240	265.452	177.551 #
33)	L7 AR-1260-3	8.388	7.233	168253	237561	96.422	111.811
34)	L7 AR-1260-4	8.614	7.716	212280	153629	117.802	86.473 #
35)	L7 AR-1260-5	8.930	7.963	305138	799037	84.881	208.872 #
36)	L8 AR-1262-1	8.388	7.454	168253	241406	62.355	89.826 #
37)	L8 AR-1262-2	8.930	7.963	305138	799037	75.246	191.630 #
38)	L8 AR-1262-3	9.227	8.249	311816	234028	108.817	129.175
39)	L8 AR-1262-4	9.316	8.313	229640	319931	94.200	95.095
40)	L8 AR-1262-5	9.939	8.810	152051	153816	112.165	117.406
41)	L9 AR-1268-1	9.227	8.249	311816	234028	60.008	46.437
42)	L9 AR-1268-2	9.316	8.313	229640	319931	47.178	62.574 #
43)	L9 AR-1268-3	9.530	8.519	77030	101475	17.825	23.015 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121520\
 Data File : PP032167.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Dec 2020 19:36
 Operator : DD\AJ
 Sample : L5090-05
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 GRAY-CHIPS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 04:50:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	9.939	8.810	152051	153816	109.445	105.251
45) L9	AR-1268-5	10.324	9.093	440890	467460	36.605	36.966



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121520\
Data File : PP032167.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Dec 2020 19:36
Operator : DD\AJ
Sample : L5090-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
GRAY-CHIPS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 04:50:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

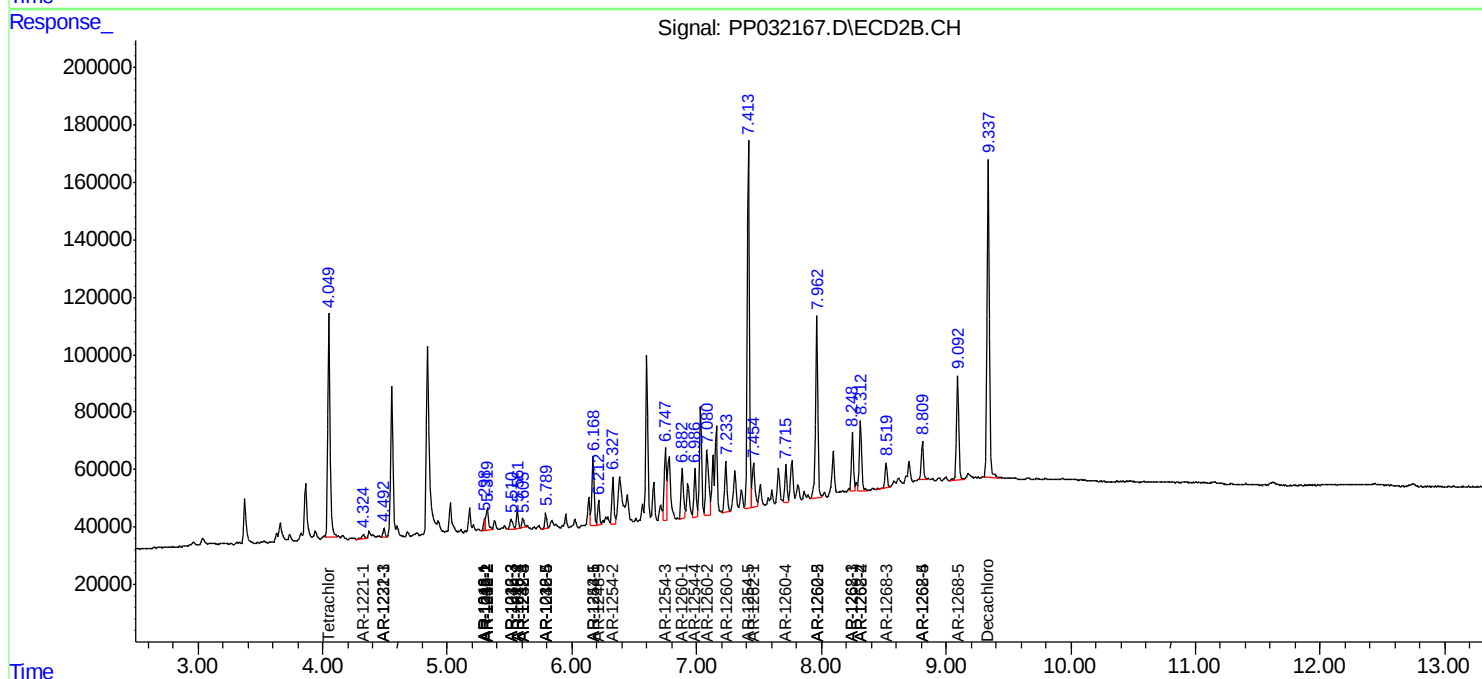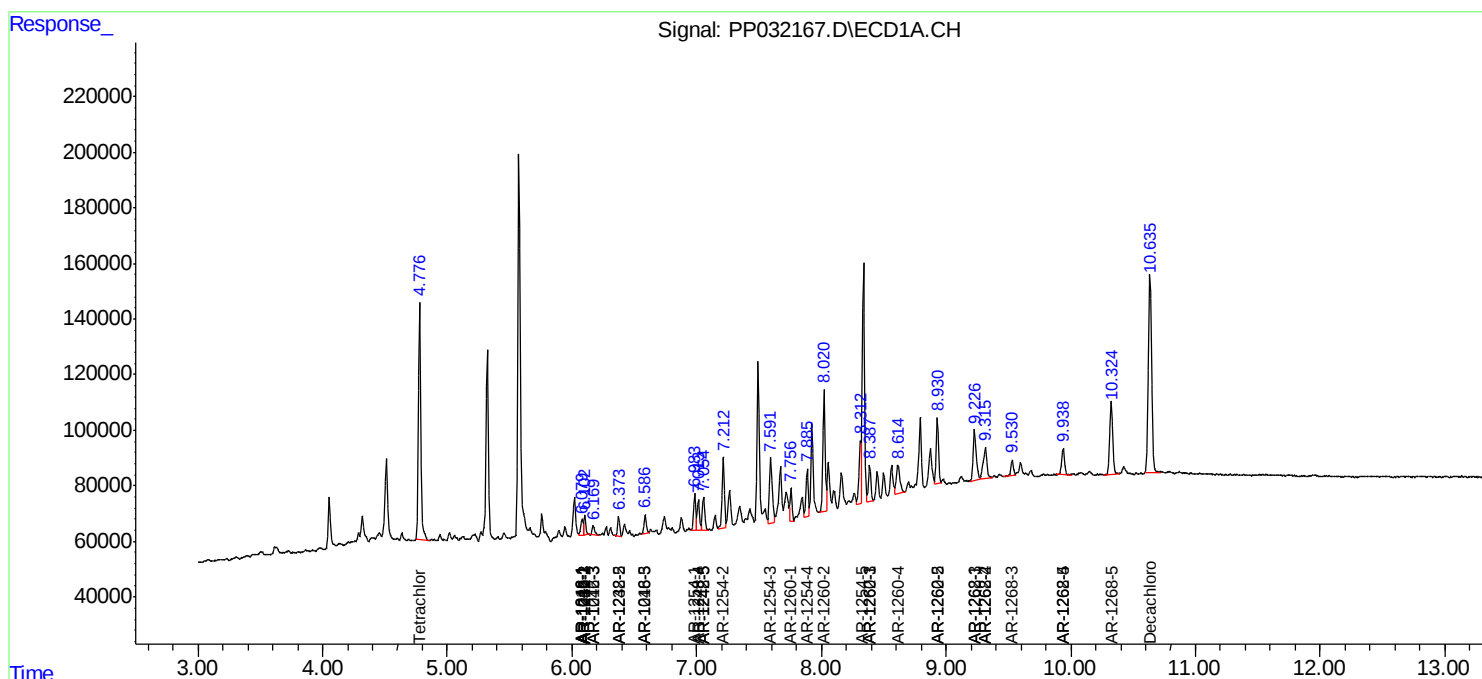


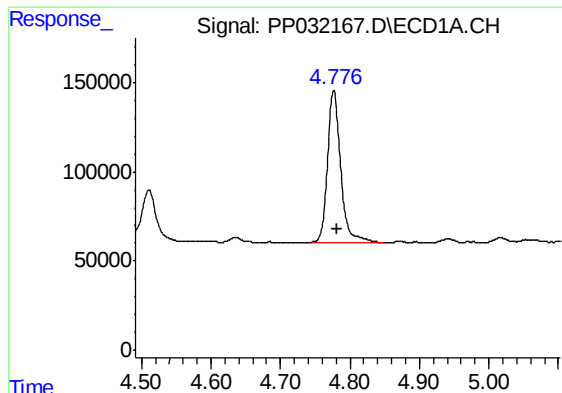

#1 Tetrachloro-m-xylene


R.T.: 4.777 min
Delta R.T.: -0.005 min
Response: 1116405
Conc: 21.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

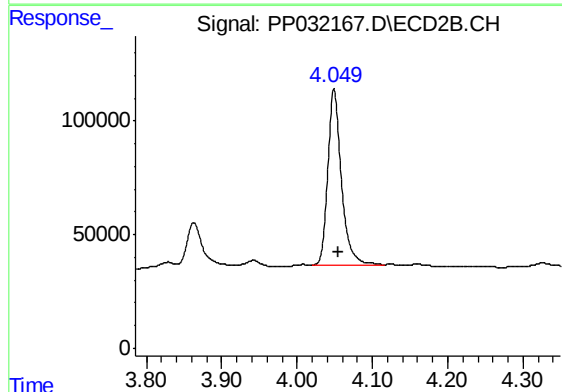


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.005 min
Response: 987977
Conc: 20.89 ng/ml

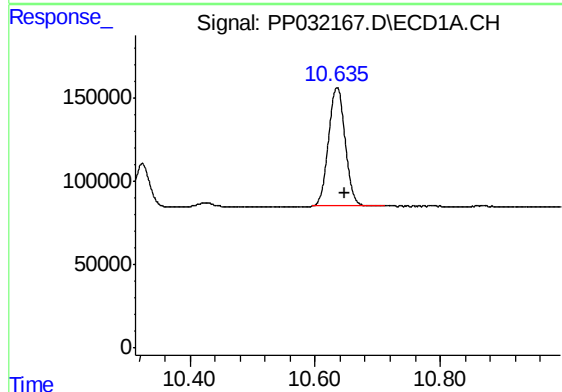


#2 Decachlorobiphenyl

R.T.: 10.635 min
Delta R.T.: -0.011 min
Response: 1317625
Conc: 42.02 ng/ml

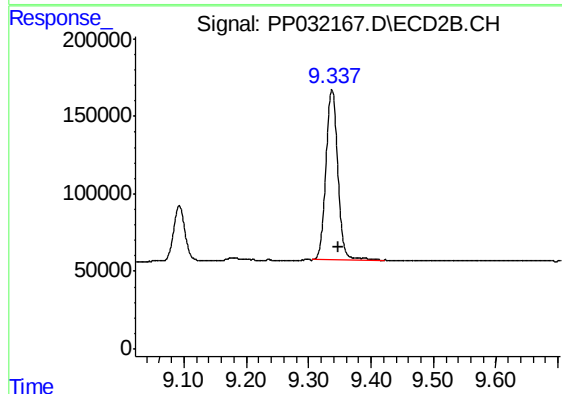

#2 Decachlorobiphenyl


R.T.: 9.338 min
Delta R.T.: -0.010 min
Response: 1453719
Conc: 43.35 ng/ml

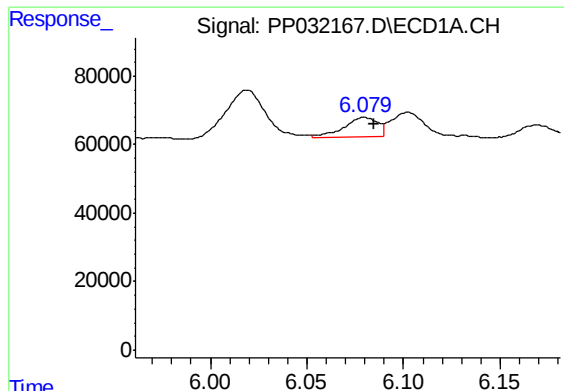

#3 AR-1016-1


R.T.: 6.080 min
Delta R.T.: -0.005 min
Response: 71245
Conc: 48.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

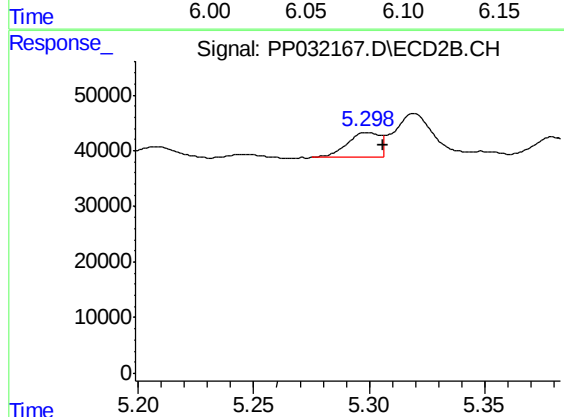


#3 AR-1016-1

R.T.: 5.299 min
Delta R.T.: -0.007 min
Response: 43505
Conc: 33.28 ng/ml

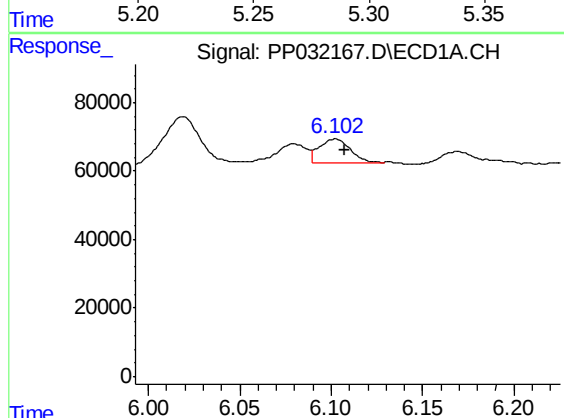


#4 AR-1016-2

R.T.: 6.102 min
Delta R.T.: -0.005 min
Response: 81877
Conc: 36.45 ng/ml

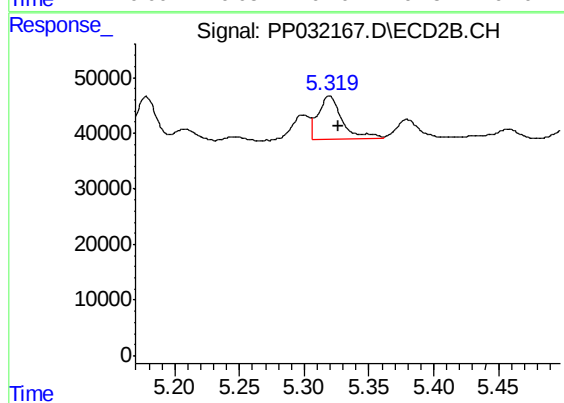

#4 AR-1016-2


R.T.: 5.320 min
Delta R.T.: -0.006 min
Response: 100368
Conc: 50.69 ng/ml

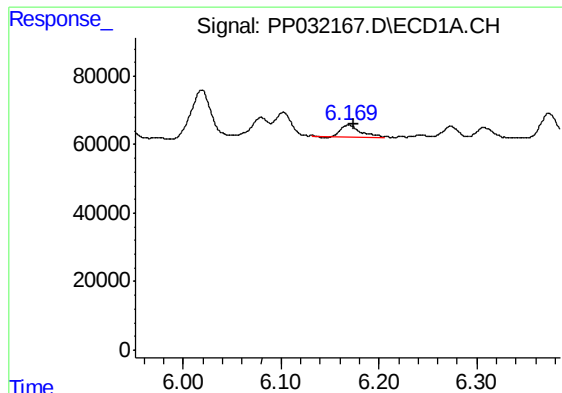

#5 AR-1016-3


R.T.: 6.169 min
Delta R.T.: -0.005 min
Response: 44260
Conc: 32.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

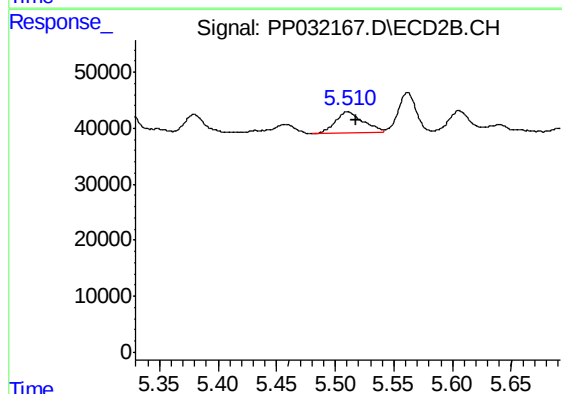


#5 AR-1016-3

R.T.: 5.511 min
Delta R.T.: -0.007 min
Response: 58309
Conc: 54.53 ng/ml

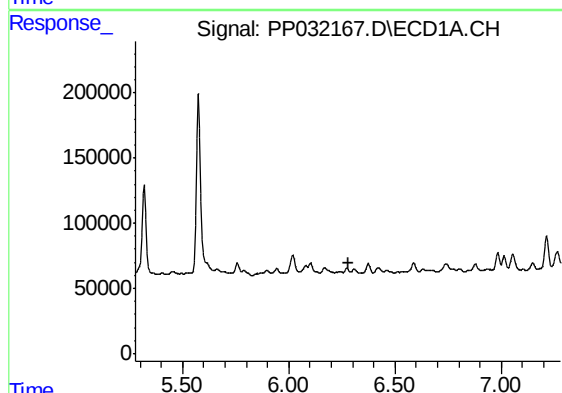


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 6.279 min
Response: 0
Conc: N.D.

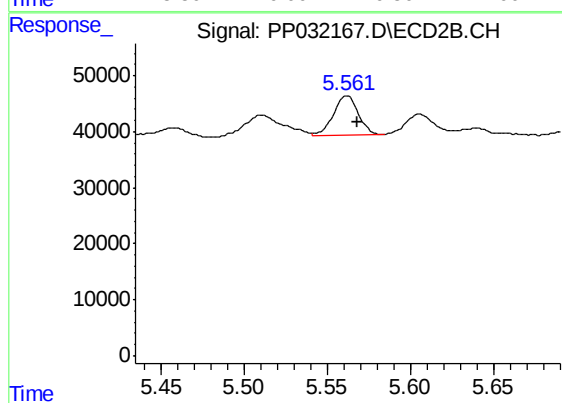

#6 AR-1016-4


R.T.: 5.562 min
Delta R.T.: -0.007 min
Response: 71280
Conc: 84.01 ng/ml

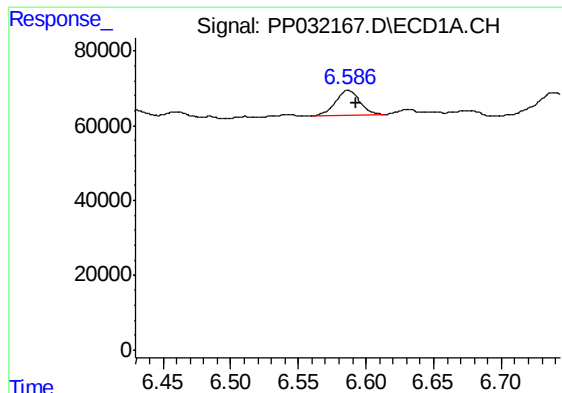

#7 AR-1016-5


R.T.: 6.587 min
Delta R.T.: -0.006 min
Response: 86154
Conc: 80.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

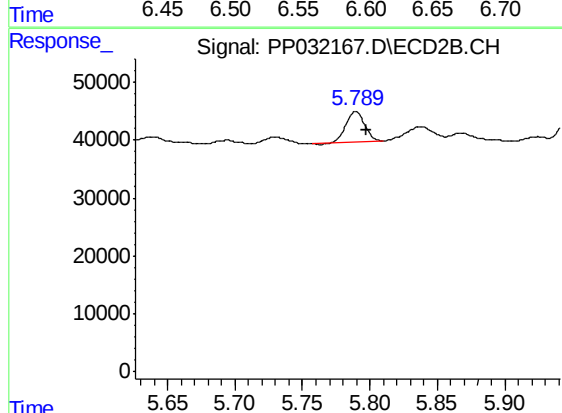


#7 AR-1016-5

R.T.: 5.790 min
Delta R.T.: -0.008 min
Response: 52236
Conc: 48.07 ng/ml

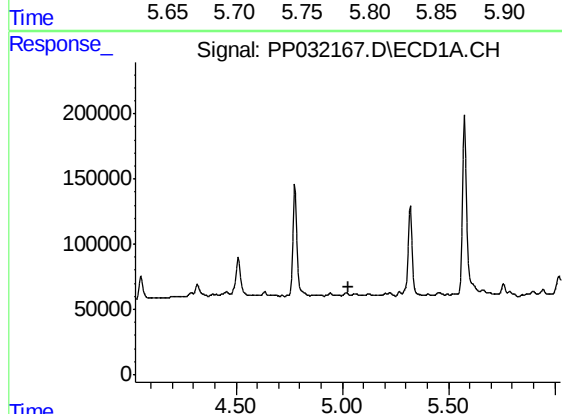


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 5.027 min
Response: 0
Conc: N.D.

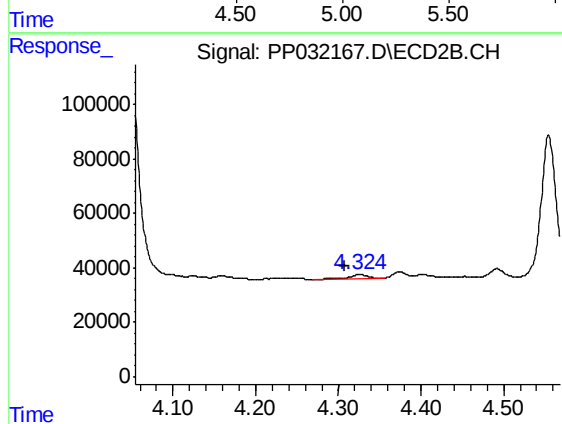

#8 AR-1221-1


R.T.: 4.325 min
Delta R.T.: 0.017 min
Response: 27276
Conc: 57.02 ng/ml



#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

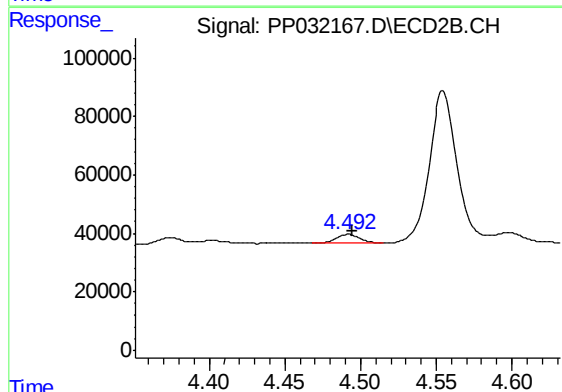


#10 AR-1221-3

R.T.: 4.492 min
Delta R.T.: -0.003 min
Response: 32495
Conc: 29.05 ng/ml




#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.210 min
Response: 0
Conc: N.D.

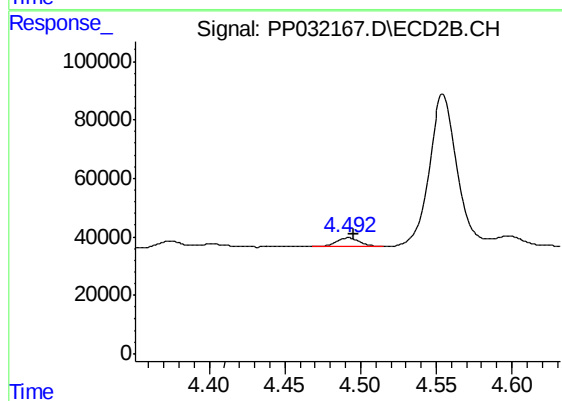

#11 AR-1232-1


R.T.: 4.492 min
Delta R.T.: -0.004 min
Response: 32495
Conc: 35.07 ng/ml

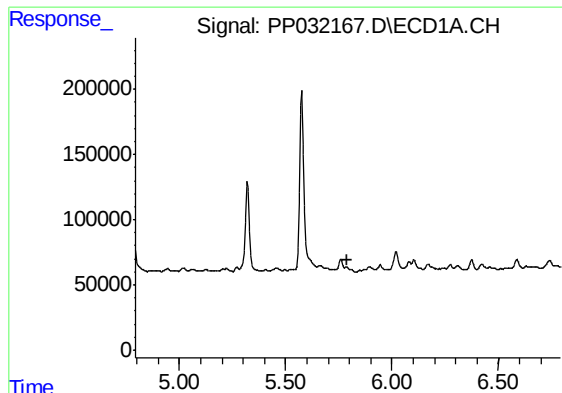

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 5.792 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

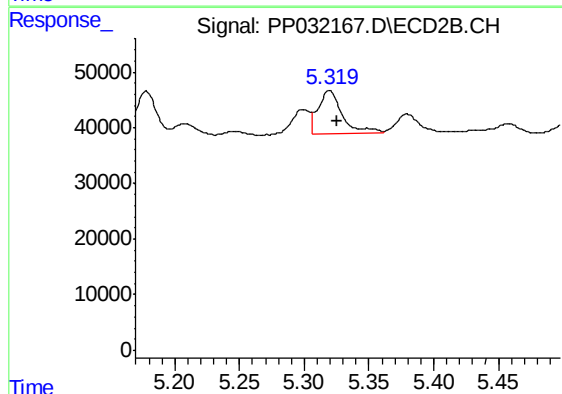


#12 AR-1232-2

R.T.: 5.320 min
Delta R.T.: -0.006 min
Response: 100368
Conc: 116.97 ng/ml

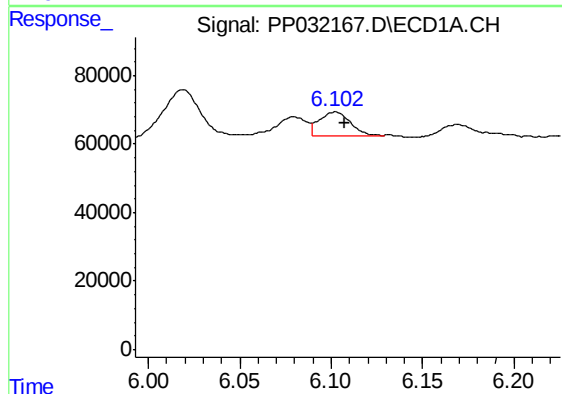


#13 AR-1232-3

R.T.: 6.102 min
Delta R.T.: -0.005 min
Response: 81877
Conc: 85.16 ng/ml

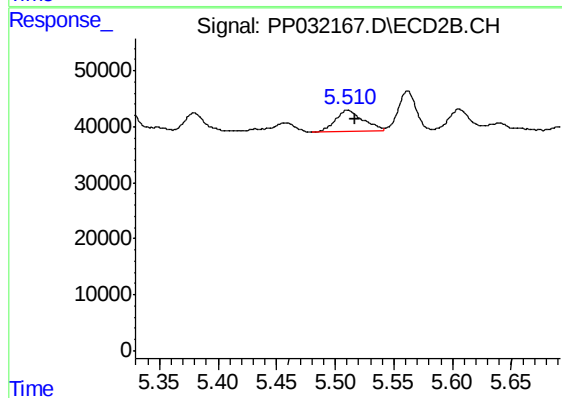

#13 AR-1232-3


R.T.: 5.511 min
Delta R.T.: -0.006 min
Response: 58309
Conc: 128.42 ng/ml

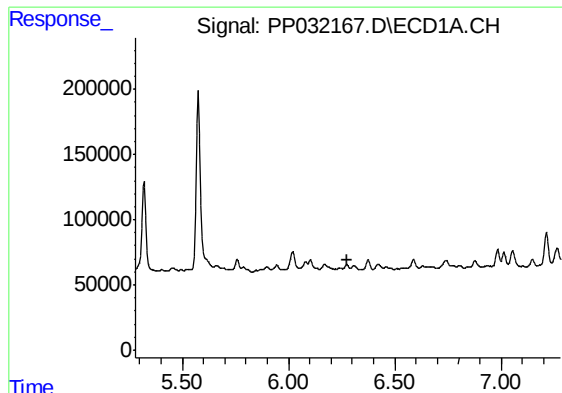

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T.: 6.279 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

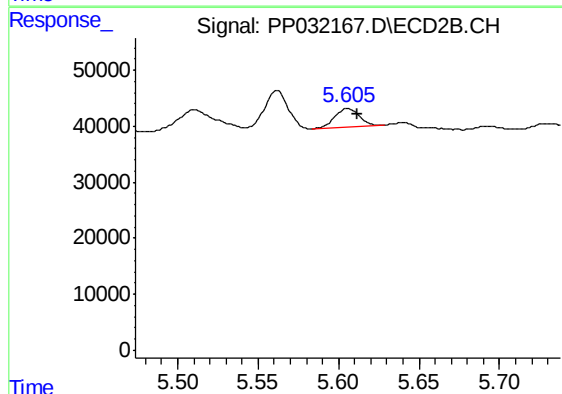


#14 AR-1232-4

R.T.: 5.605 min
Delta R.T.: -0.007 min
Response: 35049
Conc: 89.34 ng/ml

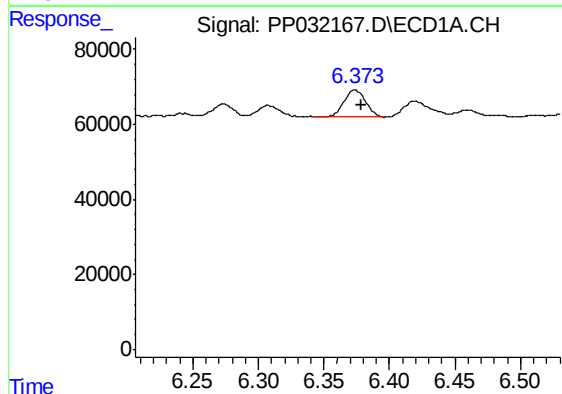


#15 AR-1232-5

R.T.: 6.374 min
Delta R.T.: -0.005 min
Response: 81544
Conc: 267.89 ng/ml

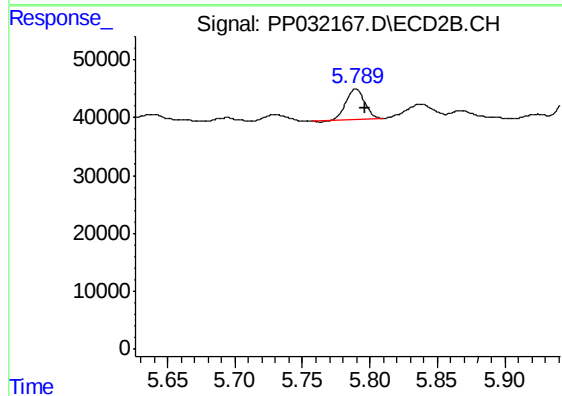

#15 AR-1232-5


R.T.: 5.790 min
Delta R.T.: -0.007 min
Response: 52236
Conc: 120.77 ng/ml

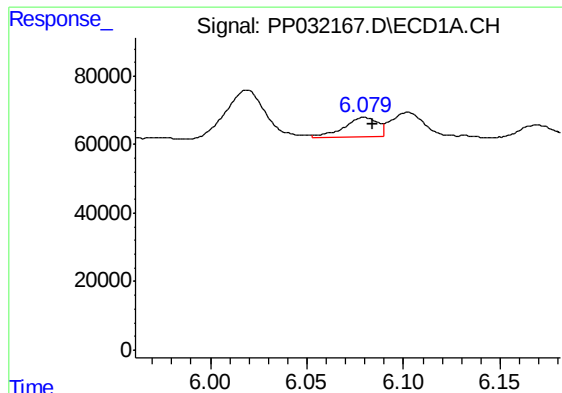

#16 AR-1242-1


R.T.: 6.080 min
Delta R.T.: -0.005 min
Response: 71245
Conc: 62.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

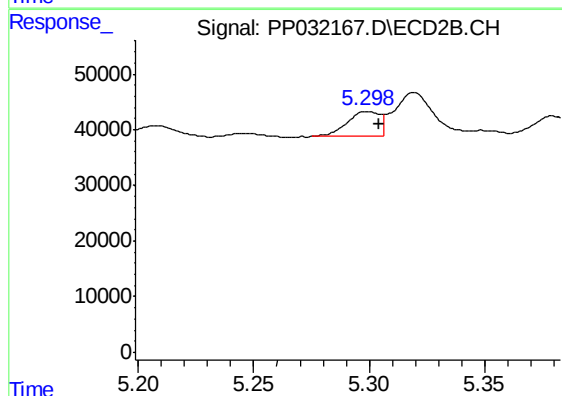


#16 AR-1242-1

R.T.: 5.299 min
Delta R.T.: -0.005 min
Response: 43505
Conc: 42.00 ng/ml

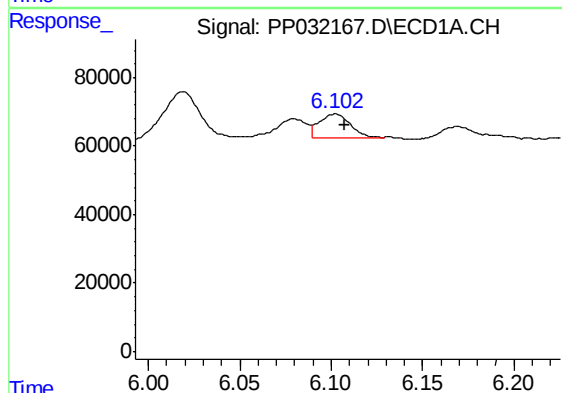


#17 AR-1242-2

R.T.: 6.102 min
Delta R.T.: -0.005 min
Response: 81877
Conc: 46.49 ng/ml

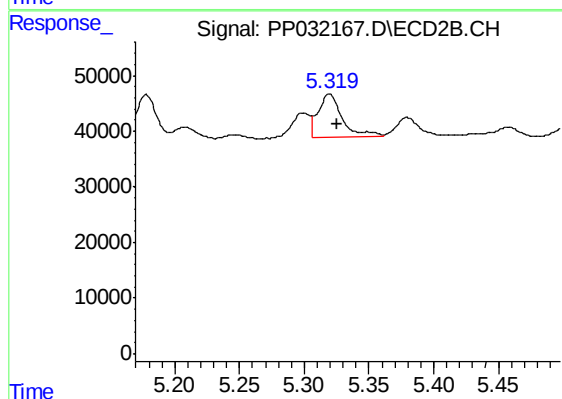

#17 AR-1242-2


R.T.: 5.320 min
Delta R.T.: -0.005 min
Response: 100368
Conc: 64.93 ng/ml



#18 AR-1242-3


R.T.: 6.169 min
Delta R.T.: -0.004 min
Response: 44260
Conc: 39.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

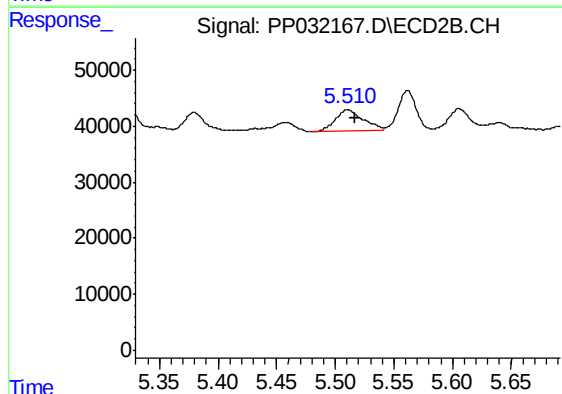


#18 AR-1242-3

R.T.: 5.511 min
Delta R.T.: -0.006 min
Response: 58309
Conc: 69.25 ng/ml




#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 6.278 min
Response: 0
Conc: N.D.

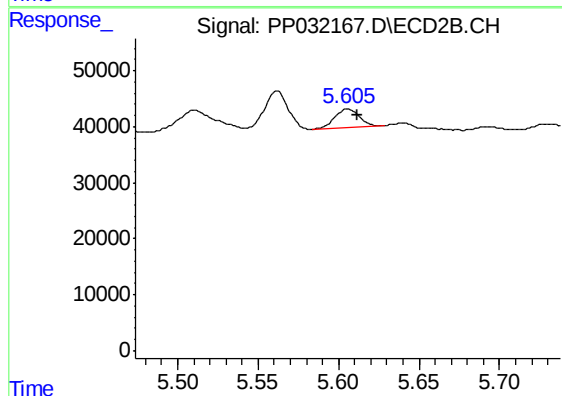

#19 AR-1242-4


R.T.: 5.605 min
Delta R.T.: -0.006 min
Response: 35049
Conc: 43.21 ng/ml



#20 AR-1242-5


R.T.: 7.054 min
Delta R.T.: -0.004 min
Response: 167967
Conc: 193.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

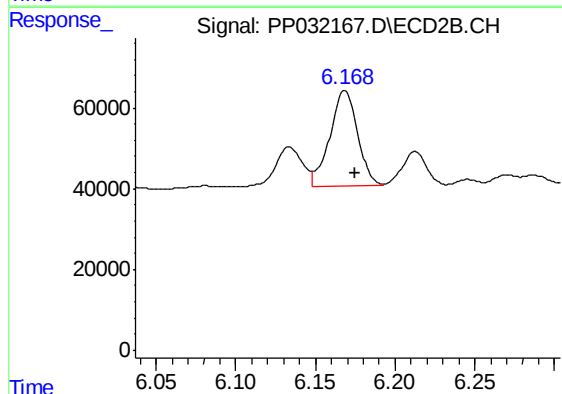


#20 AR-1242-5

R.T.: 6.168 min
Delta R.T.: -0.007 min
Response: 288056
Conc: 323.90 ng/ml




#21 AR-1248-1

R.T.: 6.080 min
Delta R.T.: -0.004 min
Response: 71245
Conc: 81.86 ng/ml

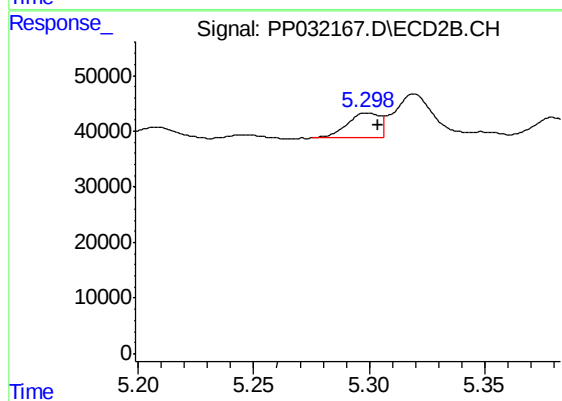

#21 AR-1248-1


R.T.: 5.299 min
Delta R.T.: -0.005 min
Response: 43505
Conc: 55.60 ng/ml

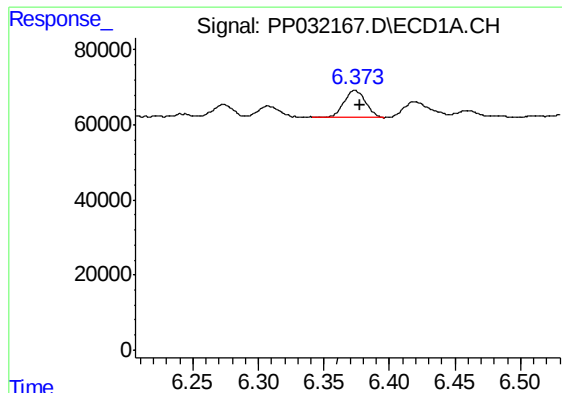

#22 AR-1248-2


R.T.: 6.374 min
Delta R.T.: -0.004 min
Response: 81544
Conc: 68.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

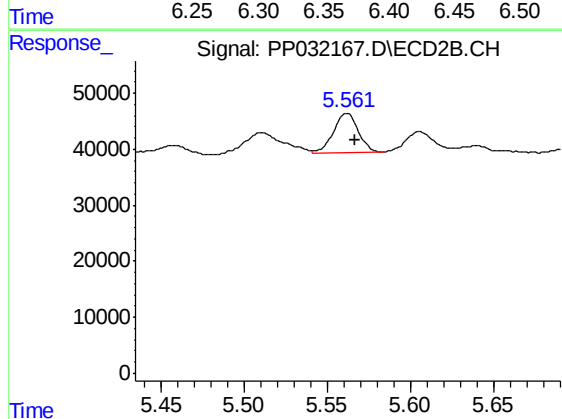


#22 AR-1248-2

R.T.: 5.562 min
Delta R.T.: -0.005 min
Response: 71280
Conc: 61.70 ng/ml

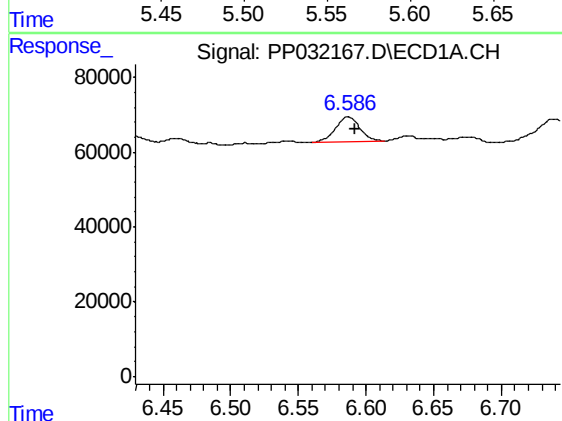


#23 AR-1248-3

R.T.: 6.587 min
Delta R.T.: -0.005 min
Response: 86154
Conc: 59.05 ng/ml

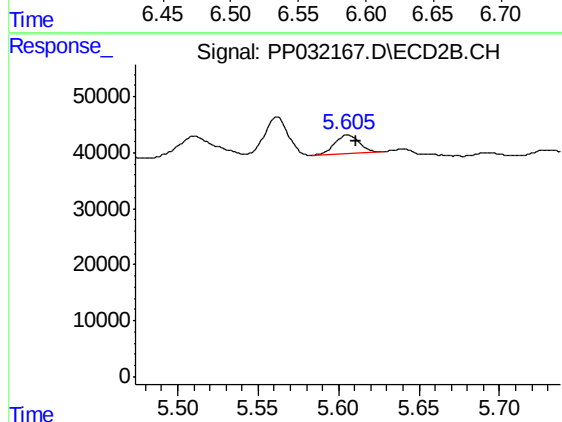

#23 AR-1248-3


R.T.: 5.605 min
Delta R.T.: -0.006 min
Response: 35049
Conc: 28.69 ng/ml



#24 AR-1248-4


R.T.: 7.013 min
Delta R.T.: -0.005 min
Response: 131157
Conc: 91.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

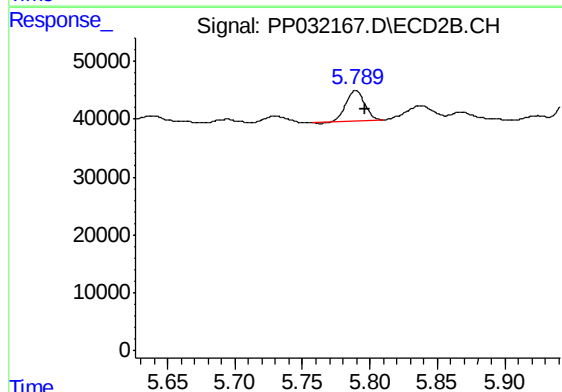


#24 AR-1248-4

R.T.: 5.790 min
Delta R.T.: -0.007 min
Response: 52236
Conc: 35.62 ng/ml

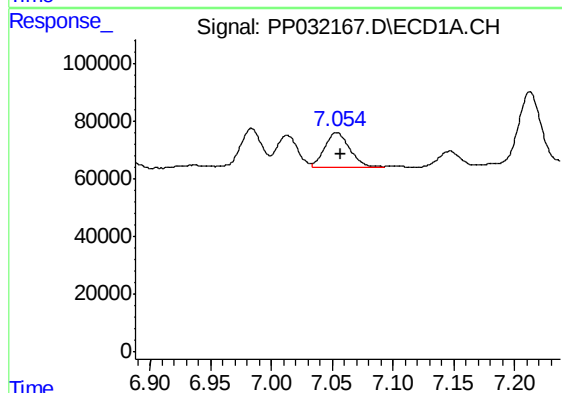


#25 AR-1248-5

R.T.: 7.054 min
Delta R.T.: -0.003 min
Response: 167967
Conc: 113.19 ng/ml

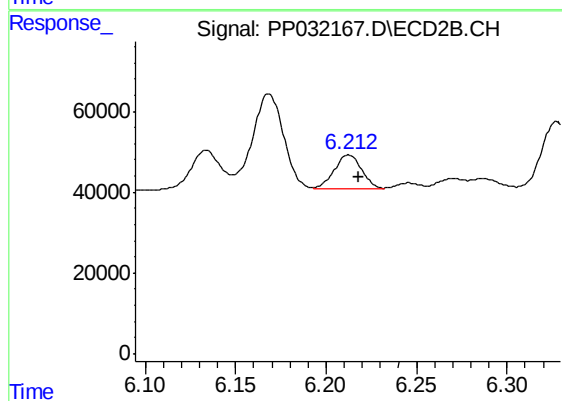

#25 AR-1248-5


R.T.: 6.212 min
Delta R.T.: -0.006 min
Response: 90105
Conc: 71.82 ng/ml



#26 AR-1254-1


R.T.: 6.984 min
Delta R.T.: -0.004 min
Response: 156761
Conc: 100.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

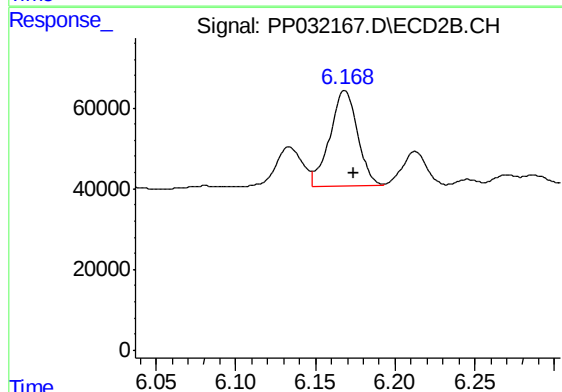


#26 AR-1254-1

R.T.: 6.168 min
Delta R.T.: -0.006 min
Response: 288056
Conc: 139.36 ng/ml

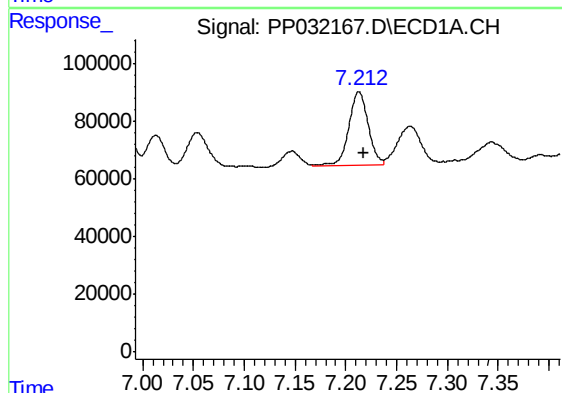


#27 AR-1254-2

R.T.: 7.213 min
Delta R.T.: -0.004 min
Response: 336280
Conc: 146.19 ng/ml

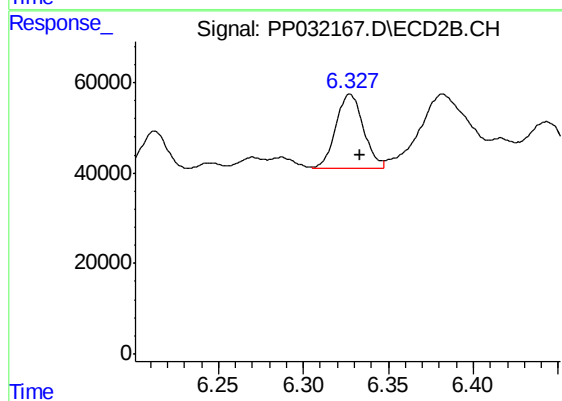

#27 AR-1254-2


R.T.: 6.327 min
Delta R.T.: -0.006 min
Response: 182831
Conc: 101.99 ng/ml

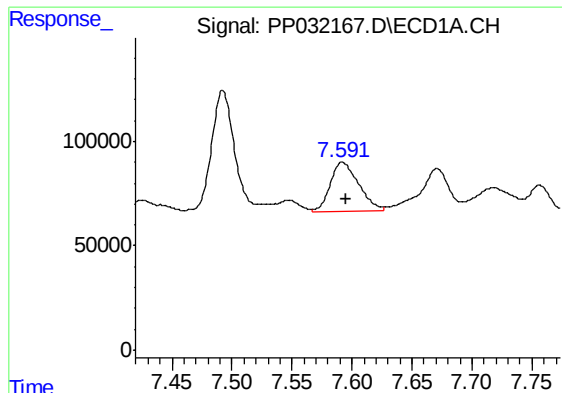

#28 AR-1254-3


R.T.: 7.592 min
Delta R.T.: -0.004 min
Response: 387742
Conc: 159.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

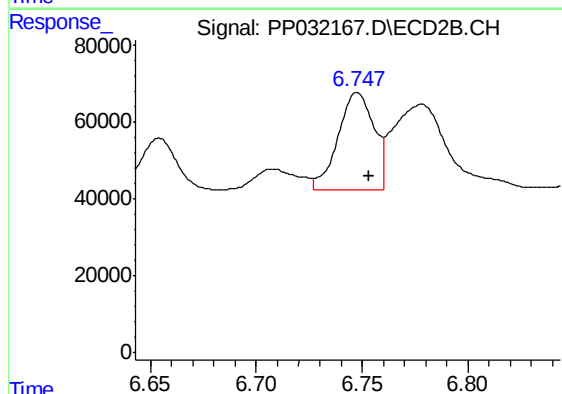


#28 AR-1254-3

R.T.: 6.748 min
Delta R.T.: -0.006 min
Response: 297425
Conc: 104.07 ng/ml

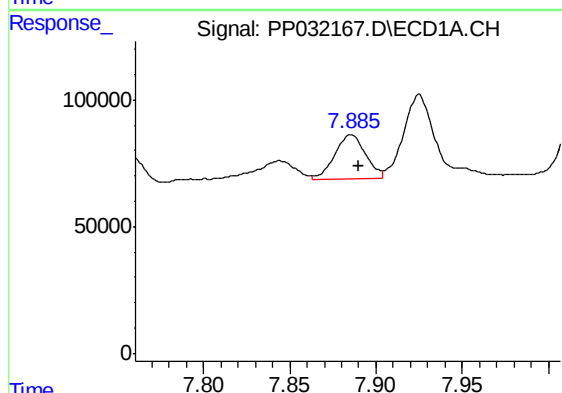


#29 AR-1254-4

R.T.: 7.886 min
Delta R.T.: -0.005 min
Response: 213823
Conc: 138.92 ng/ml

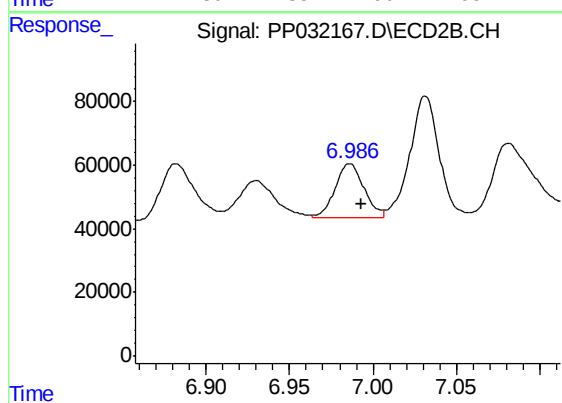

#29 AR-1254-4


R.T.: 6.986 min
Delta R.T.: -0.007 min
Response: 204009
Conc: 147.62 ng/ml

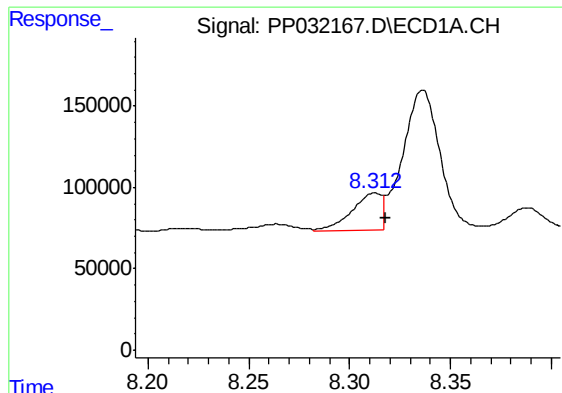

#30 AR-1254-5


R.T.: 8.313 min
Delta R.T.: -0.005 min
Response: 235824
Conc: 137.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

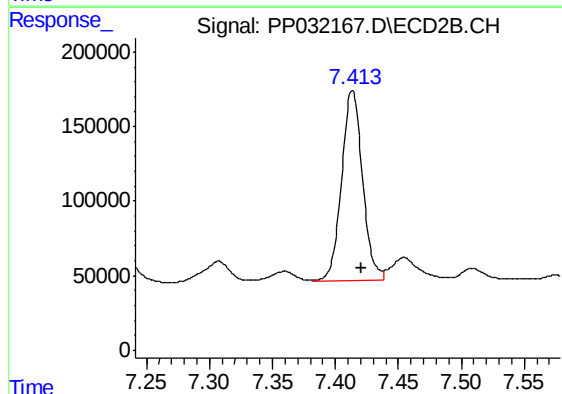


#30 AR-1254-5

R.T.: 7.414 min
Delta R.T.: -0.007 min
Response: 1486295
Conc: 624.75 ng/ml




#31 AR-1260-1

R.T.: 7.756 min
Delta R.T.: -0.008 min
Response: 137734
Conc: 79.47 ng/ml

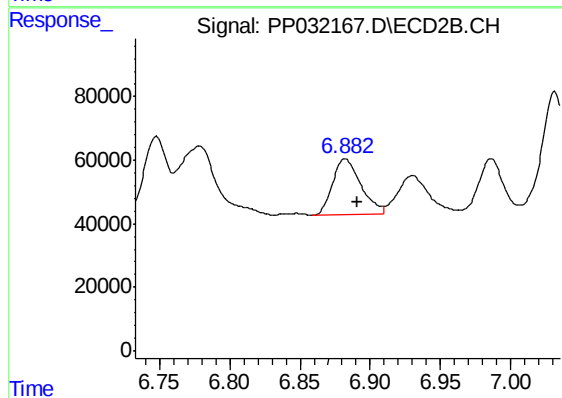

#31 AR-1260-1


R.T.: 6.882 min
Delta R.T.: -0.008 min
Response: 247391
Conc: 130.49 ng/ml

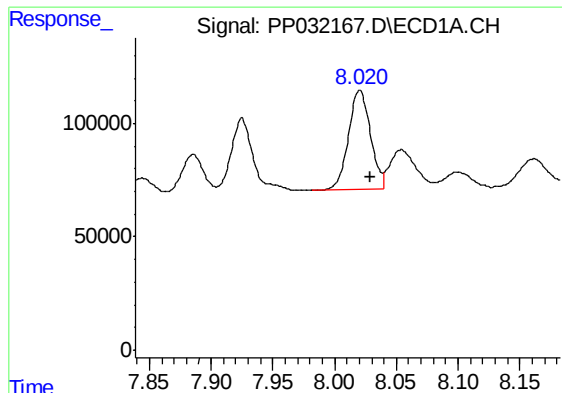

#32 AR-1260-2


R.T.: 8.020 min
Delta R.T.: -0.009 min
Response: 545396
Conc: 265.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

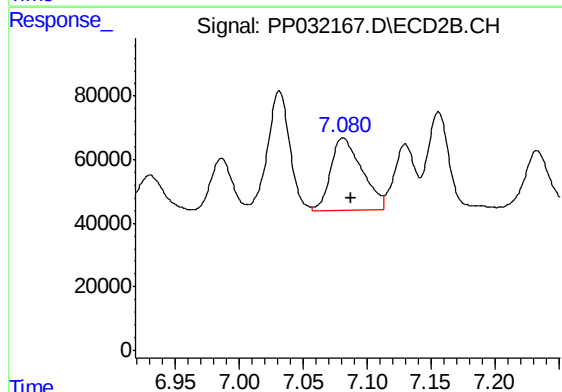


#32 AR-1260-2

R.T.: 7.081 min
Delta R.T.: -0.007 min
Response: 386240
Conc: 177.55 ng/ml

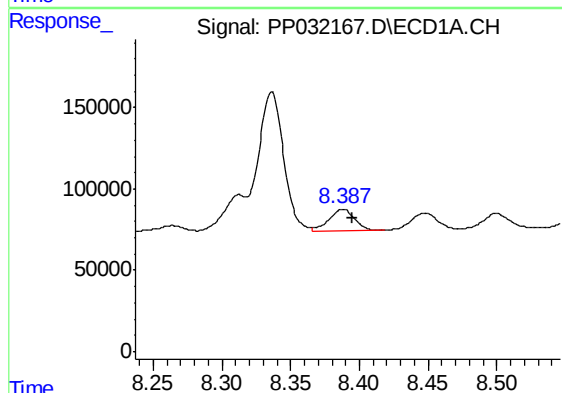


#33 AR-1260-3

R.T.: 8.388 min
Delta R.T.: -0.007 min
Response: 168253
Conc: 96.42 ng/ml

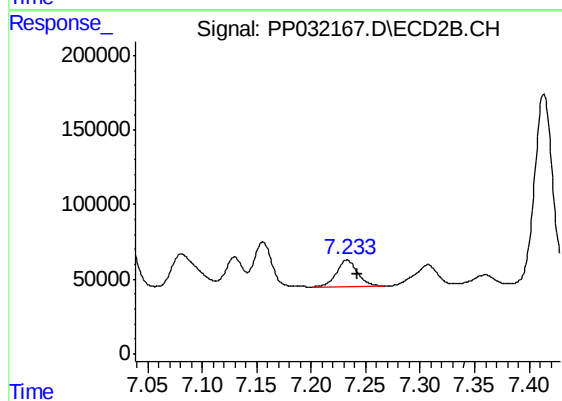

#33 AR-1260-3


R.T.: 7.233 min
Delta R.T.: -0.010 min
Response: 237561
Conc: 111.81 ng/ml

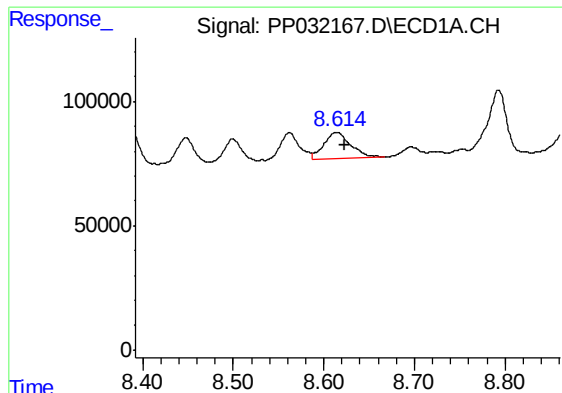

#34 AR-1260-4


R.T.: 8.614 min
Delta R.T.: -0.009 min
Response: 212280
Conc: 117.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

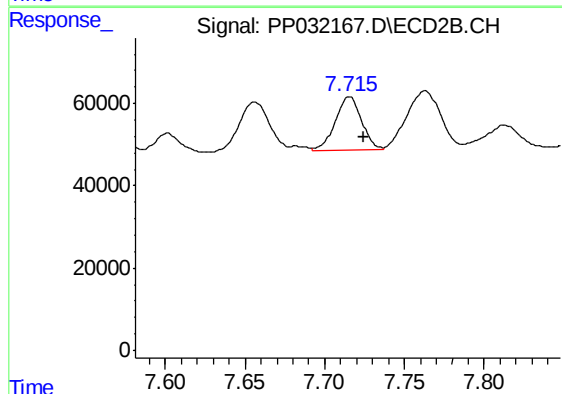


#34 AR-1260-4

R.T.: 7.716 min
Delta R.T.: -0.009 min
Response: 153629
Conc: 86.47 ng/ml

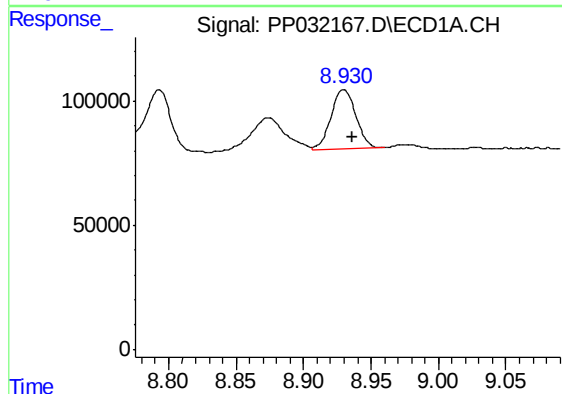


#35 AR-1260-5

R.T.: 8.930 min
Delta R.T.: -0.007 min
Response: 305138
Conc: 84.88 ng/ml

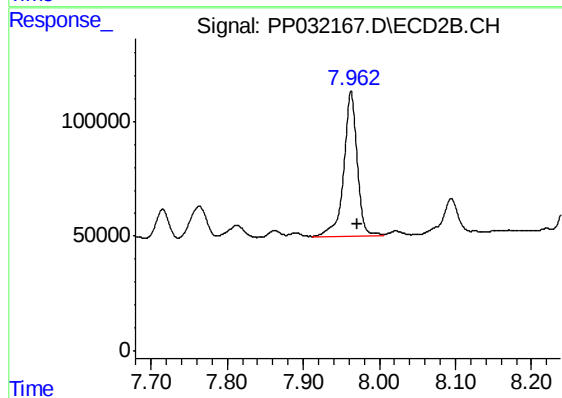

#35 AR-1260-5


R.T.: 7.963 min
Delta R.T.: -0.009 min
Response: 799037
Conc: 208.87 ng/ml



#36 AR-1262-1


R.T.: 8.388 min
Delta R.T.: -0.006 min
Response: 168253
Conc: 62.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

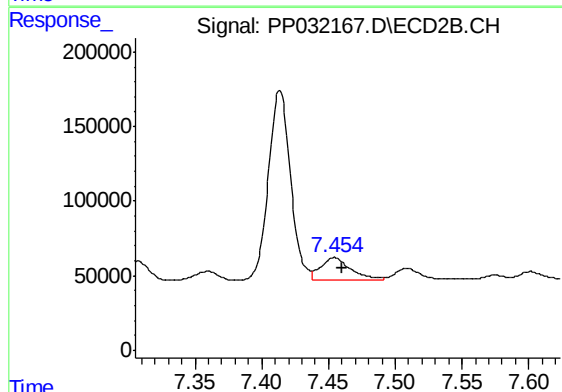


#36 AR-1262-1

R.T.: 7.454 min
Delta R.T.: -0.006 min
Response: 241406
Conc: 89.83 ng/ml

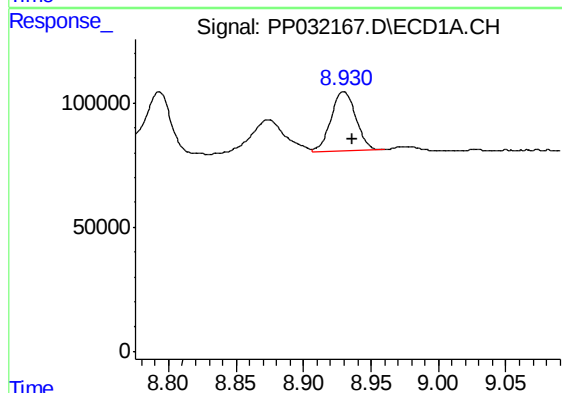


#37 AR-1262-2

R.T.: 8.930 min
Delta R.T.: -0.006 min
Response: 305138
Conc: 75.25 ng/ml

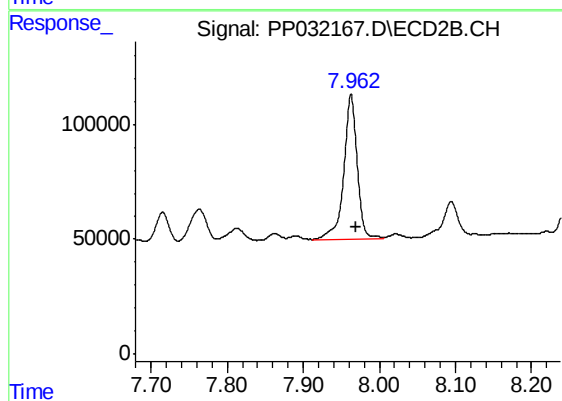

#37 AR-1262-2


R.T.: 7.963 min
Delta R.T.: -0.007 min
Response: 799037
Conc: 191.63 ng/ml

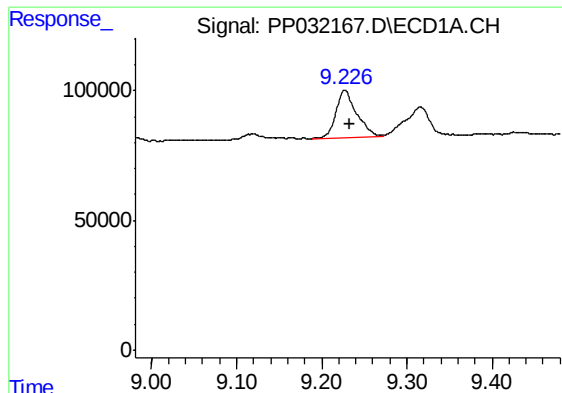

#38 AR-1262-3


R.T.: 9.227 min
Delta R.T.: -0.006 min
Response: 311816
Conc: 108.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

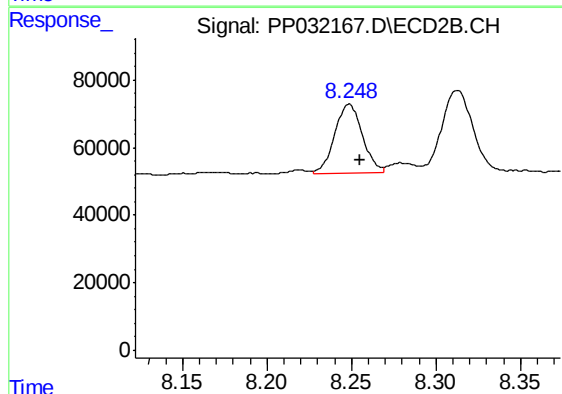


#38 AR-1262-3

R.T.: 8.249 min
Delta R.T.: -0.007 min
Response: 234028
Conc: 129.18 ng/ml




#39 AR-1262-4

R.T.: 9.316 min
Delta R.T.: -0.006 min
Response: 229640
Conc: 94.20 ng/ml

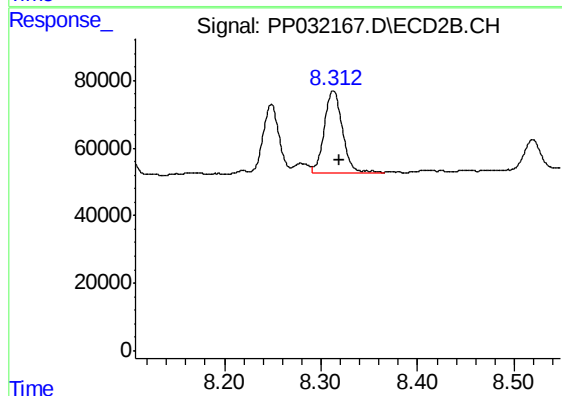

#39 AR-1262-4


R.T.: 8.313 min
Delta R.T.: -0.007 min
Response: 319931
Conc: 95.09 ng/ml



#40 AR-1262-5


R.T.: 9.939 min
Delta R.T.: -0.008 min
Response: 152051
Conc: 112.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

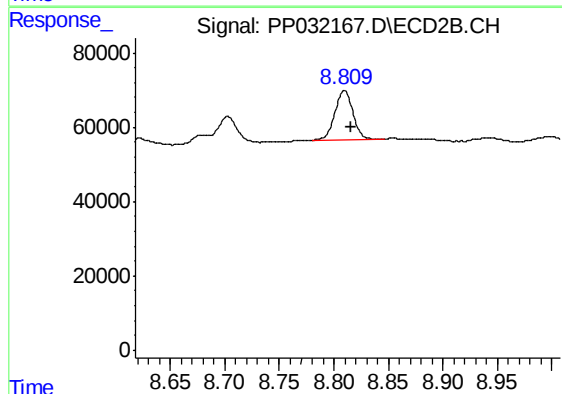


#40 AR-1262-5

R.T.: 8.810 min
Delta R.T.: -0.007 min
Response: 153816
Conc: 117.41 ng/ml




#41 AR-1268-1

R.T.: 9.227 min
Delta R.T.: -0.006 min
Response: 311816
Conc: 60.01 ng/ml

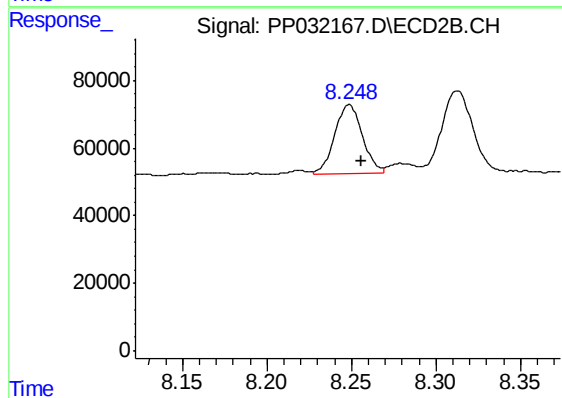

#41 AR-1268-1


R.T.: 8.249 min
Delta R.T.: -0.007 min
Response: 234028
Conc: 46.44 ng/ml

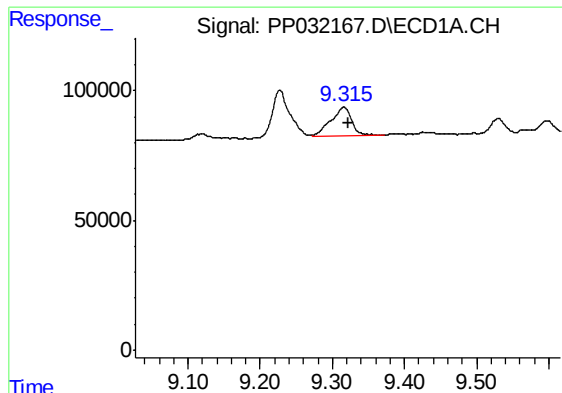

#42 AR-1268-2


R.T.: 9.316 min
Delta R.T.: -0.007 min
Response: 229640
Conc: 47.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

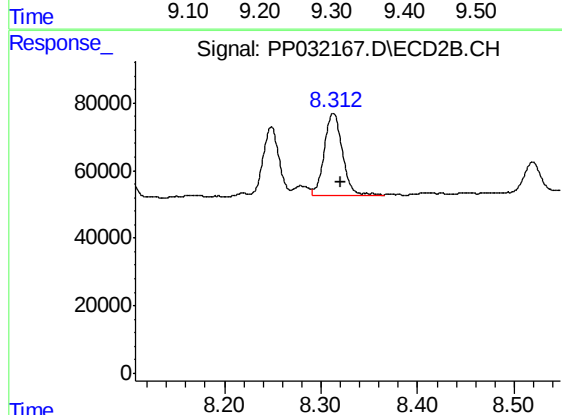


#42 AR-1268-2

R.T.: 8.313 min
Delta R.T.: -0.007 min
Response: 319931
Conc: 62.57 ng/ml

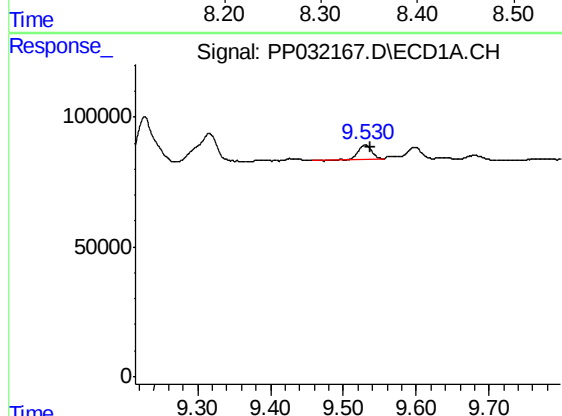


#43 AR-1268-3

R.T.: 9.530 min
Delta R.T.: -0.007 min
Response: 77030
Conc: 17.83 ng/ml

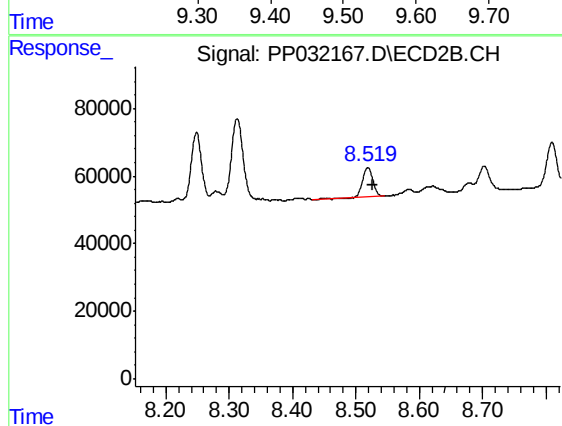

#43 AR-1268-3


R.T.: 8.519 min
Delta R.T.: -0.008 min
Response: 101475
Conc: 23.02 ng/ml

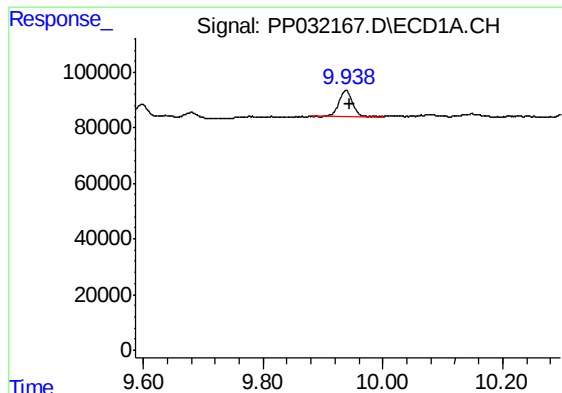

#44 AR-1268-4


R.T.: 9.939 min
Delta R.T.: -0.006 min
Response: 152051
Conc: 109.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
GRAY-CHIPS

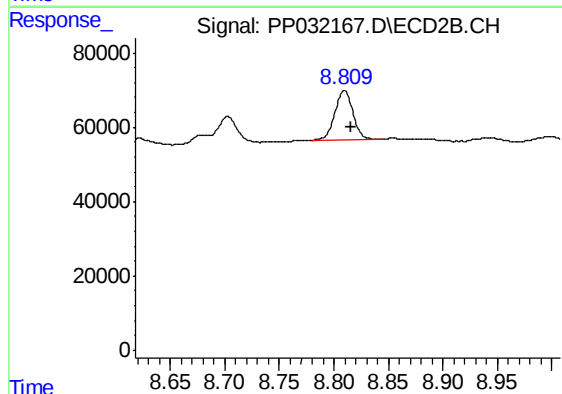


#44 AR-1268-4

R.T.: 8.810 min
Delta R.T.: -0.006 min
Response: 153816
Conc: 105.25 ng/ml

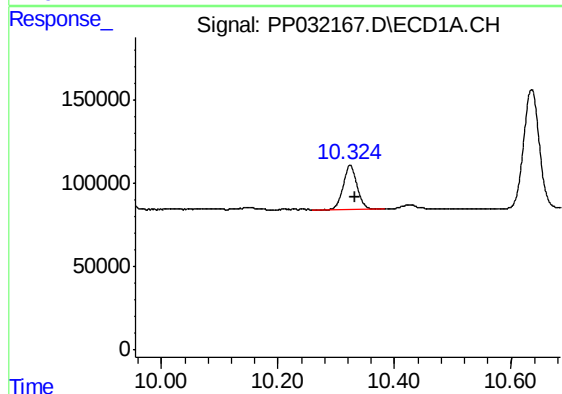

#45 AR-1268-5

R.T.: 10.324 min
Delta R.T.: -0.009 min
Response: 440890
Conc: 36.60 ng/ml

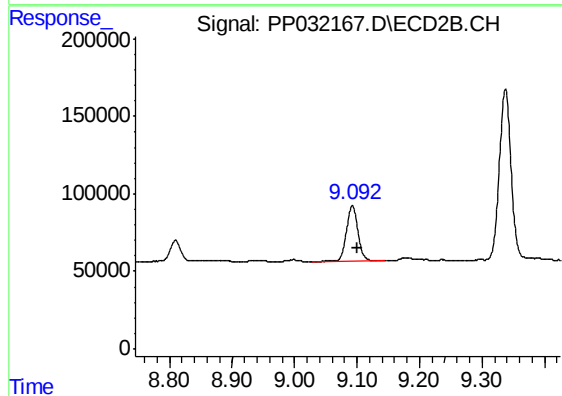

#45 AR-1268-5

R.T.: 9.093 min
Delta R.T.: -0.008 min
Response: 467460
Conc: 36.97 ng/ml