

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121520\
 Data File : PP032140.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Dec 2020 11:09
 Operator : DD\AJ
 Sample : L5081-19
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WOOSPK-035-0002

Manual Integrations
 APPROVED

Ankita
 12/16/2020 10:55:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 04:31:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.778	4.050	823600	850080	15.988m	17.973
2) SA Decachlor...	10.639	9.340	806050	743585	25.704	22.173

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121520\
Data File : PP032140.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Dec 2020 11:09
Operator : DD\AJ
Sample : L5081-19
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WOOSPK-035-0002


Manual Integrations
APPROVED

Ankita
12/16/2020 10:55:45 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 04:31:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

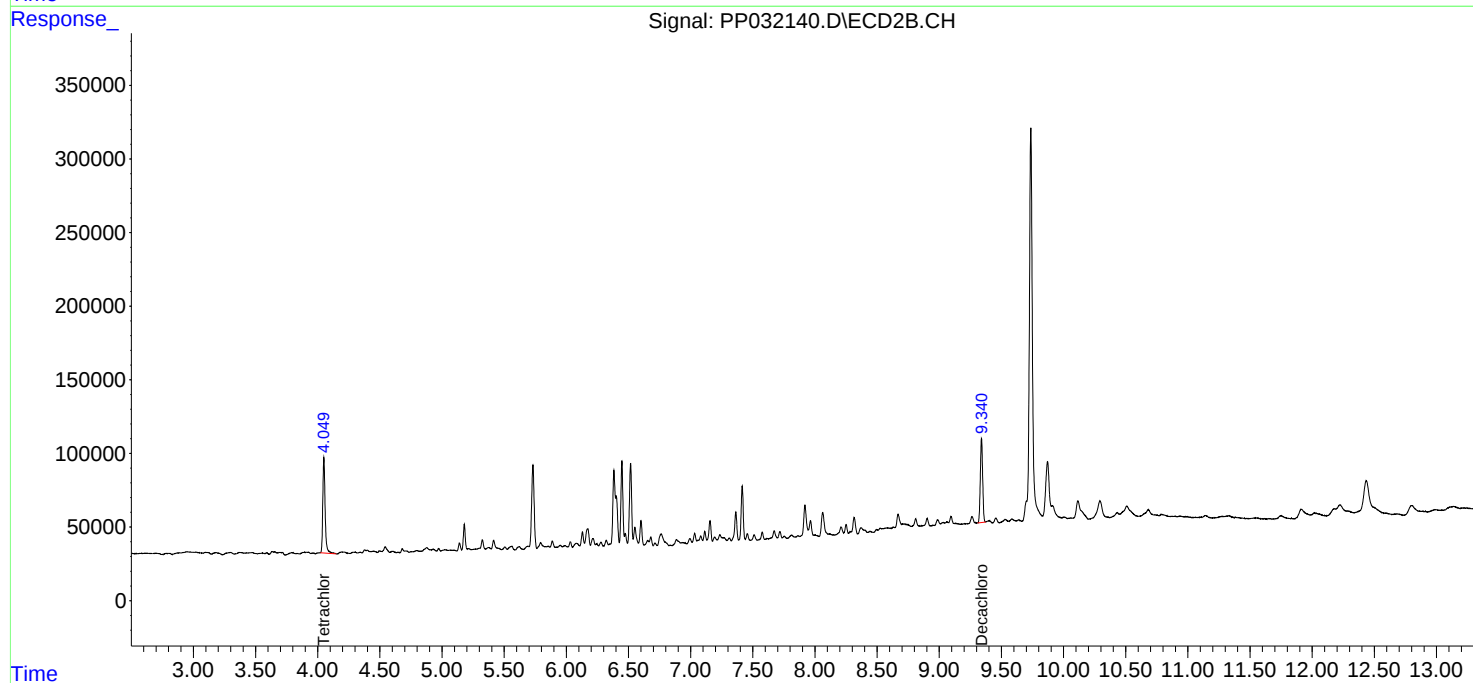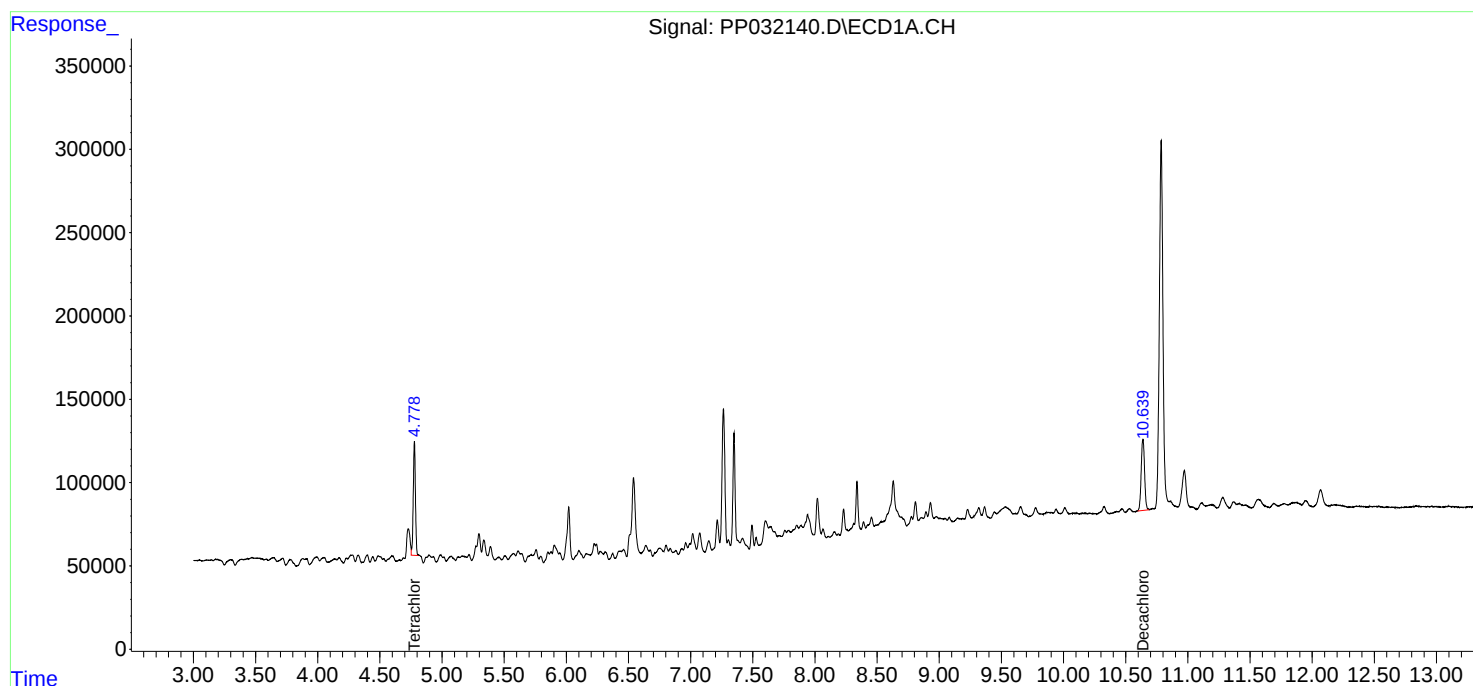

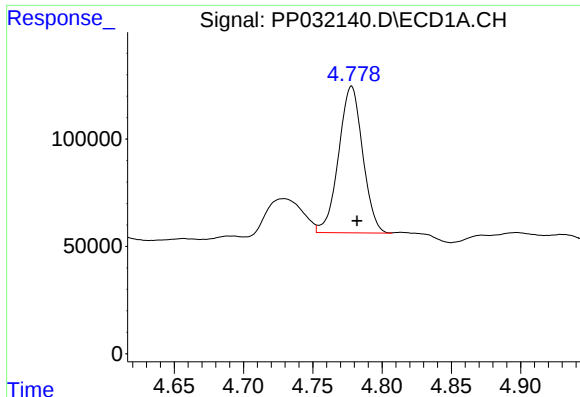


#1 Tetrachloro-m-xylene

R.T.: 4.778 min
Delta R.T.: -0.004 min
Response: 823600
Conc: 15.99 ng/ml m

Instrument :
ECD_P
ClientSampleId :
WOOSPK-035-0002


Manual Integrations
APPROVED

Ankita
12/16/2020 10:55:45 AM

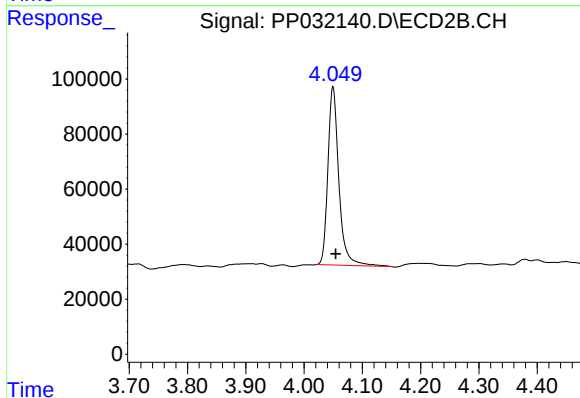


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.004 min
Response: 850080
Conc: 17.97 ng/ml

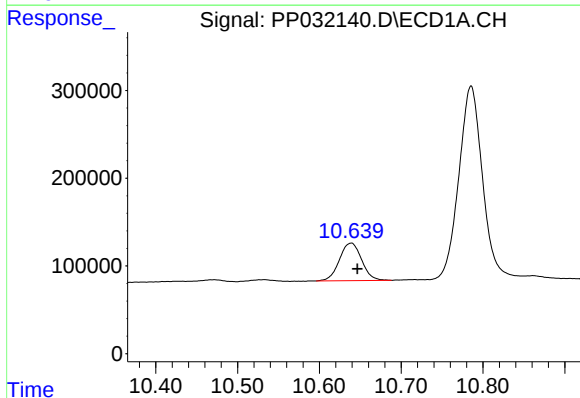

#2 Decachlorobiphenyl

R.T.: 10.639 min
Delta R.T.: -0.008 min
Response: 806050
Conc: 25.70 ng/ml

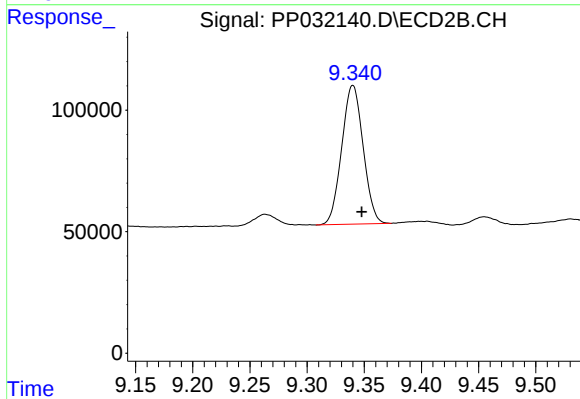

#2 Decachlorobiphenyl

R.T.: 9.340 min
Delta R.T.: -0.008 min
Response: 743585
Conc: 22.17 ng/ml