

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121525\
 Data File : PP077049.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Dec 2025 17:51
 Operator : YP\AJ
 Sample : Q3869-07 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 4-END-B

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 12/16/2025
 Supervised By :Yogesh Patel 12/16/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 00:32:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 21 22:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.611	3.766	2607795	2596157	1.421m	1.246
2) SA Decachlor...	10.358	8.757	2038136	2321572	1.360m	1.316

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121525\
Data File : PP077049.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Dec 2025 17:51
Operator : YP\AJ
Sample : Q3869-07 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
4-END-B


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/16/2025
Supervised By :Yogesh Patel 12/16/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 00:32:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP112125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 21 22:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

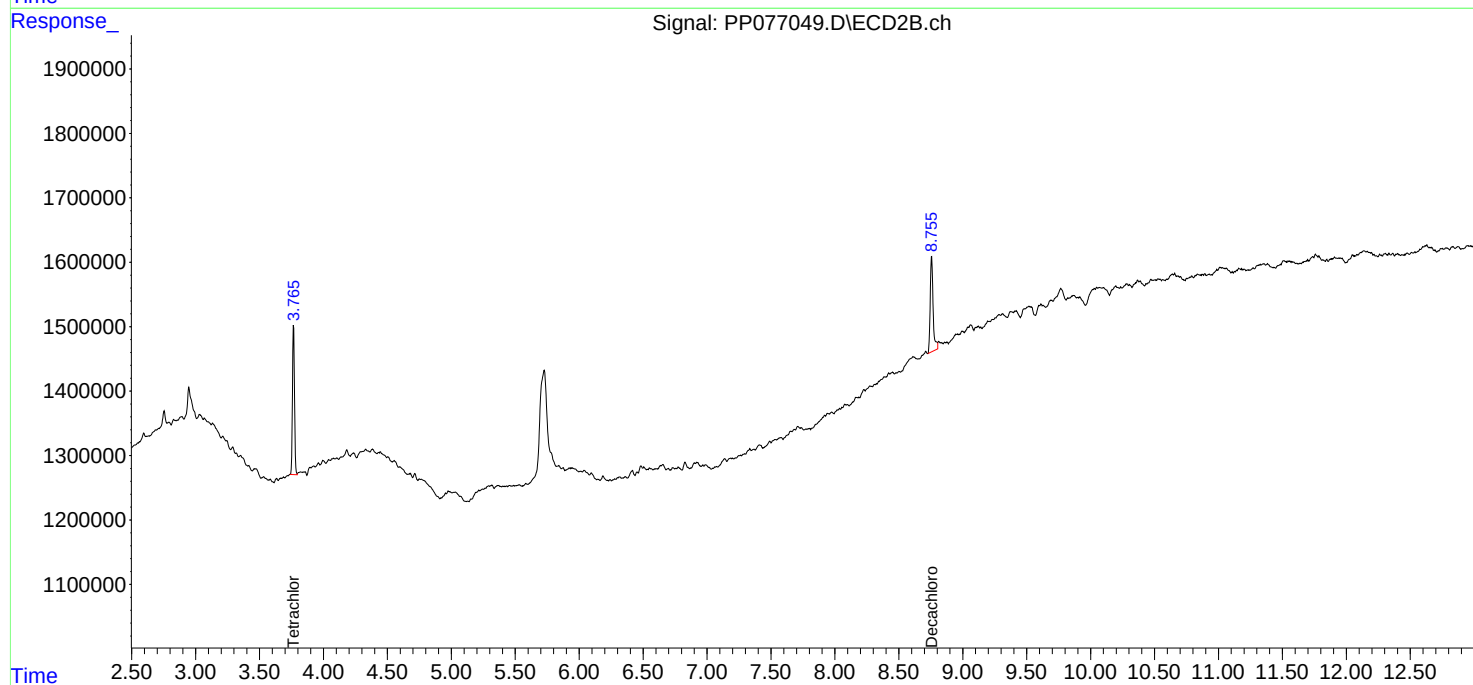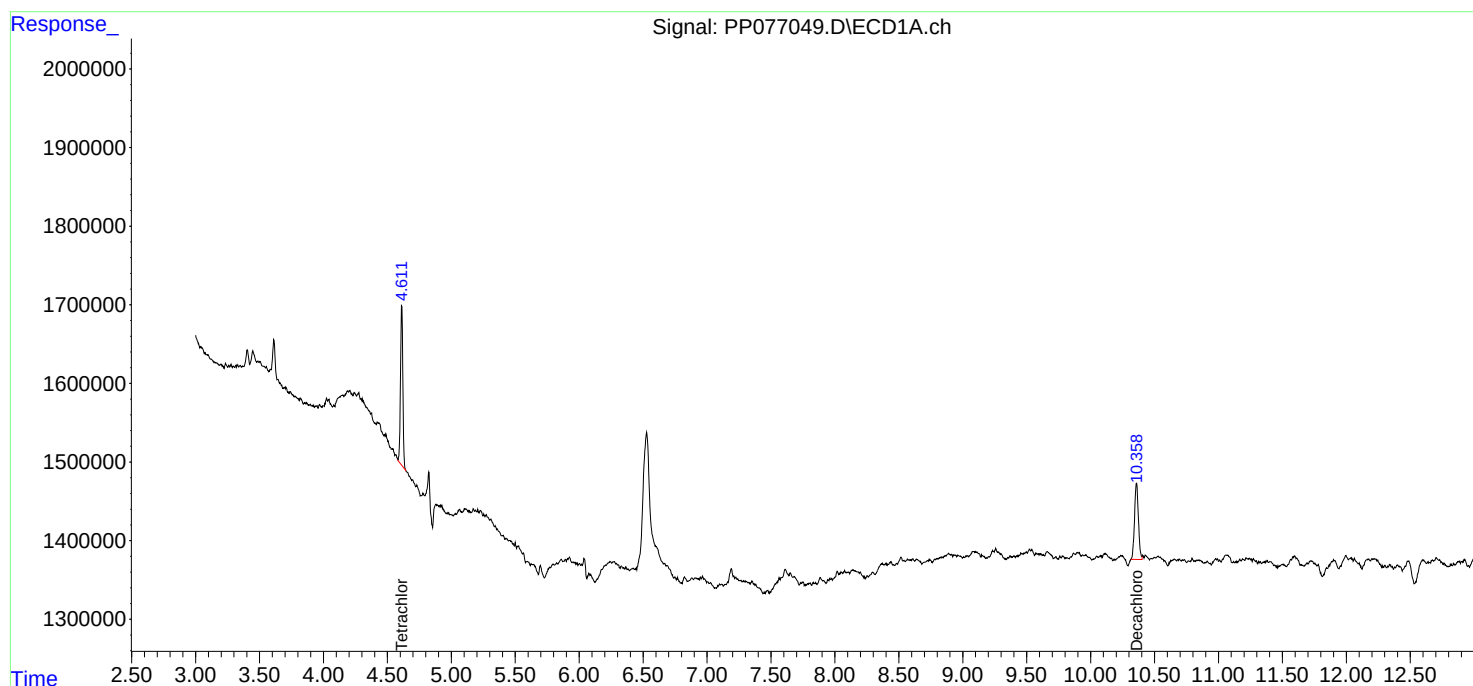

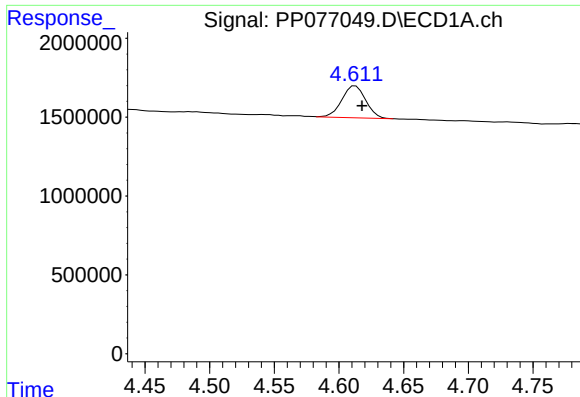


#1 Tetrachloro-m-xylene

R.T.: 4.611 min
Delta R.T.: -0.007 min
Response: 2607795
Conc: 1.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
4-END-B


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 12/16/2025
Supervised By :Yogesh Patel 12/16/2025

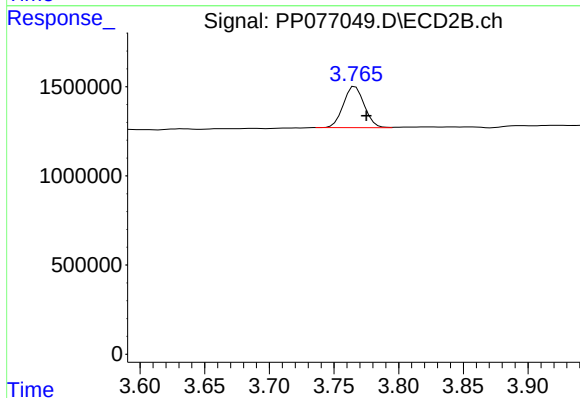


#1 Tetrachloro-m-xylene

R.T.: 3.766 min
Delta R.T.: -0.009 min
Response: 2596157
Conc: 1.25 ng/ml

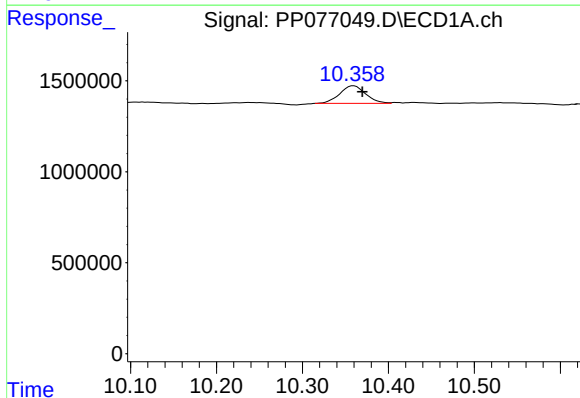

#2 Decachlorobiphenyl

R.T.: 10.358 min
Delta R.T.: -0.011 min
Response: 2038136
Conc: 1.36 ng/ml m

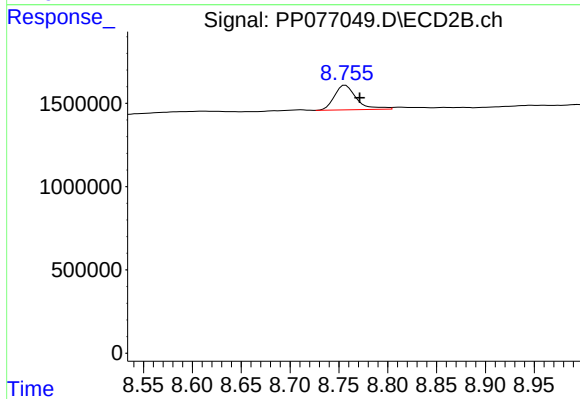

#2 Decachlorobiphenyl

R.T.: 8.757 min
Delta R.T.: -0.014 min
Response: 2321572
Conc: 1.32 ng/ml