

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121620\
 Data File : PP032214.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Dec 2020 23:23
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 01:19:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.778	4.050	960235	856081	18.641	18.100
2)	SA Decachlor...	10.643	9.341	672242	712877	21.437	21.257
Target Compounds							
20)	L4 AR-1242-5	0.000	6.195f	0	20580	N.D.	23.141 #
24)	L5 AR-1248-4	6.999f	0.000	43664	0	30.522	N.D. #
25)	L5 AR-1248-5	0.000	6.195f	0	20580	N.D.	16.403 #
26)	L6 AR-1254-1	6.999	6.195f	43664	20580	28.112	9.956 #
28)	L6 AR-1254-3	7.603	0.000	45691	0	18.765	N.D. #
36)	L8 AR-1262-1	0.000	7.459	0	45929	N.D.	17.090 #
38)	L8 AR-1262-3	0.000	8.241	0	30116	N.D.	16.623 #
41)	L9 AR-1268-1	0.000	8.241	0	30116	N.D.	5.976 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121620\
Data File : PP032214.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Dec 2020 23:23
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 01:19:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

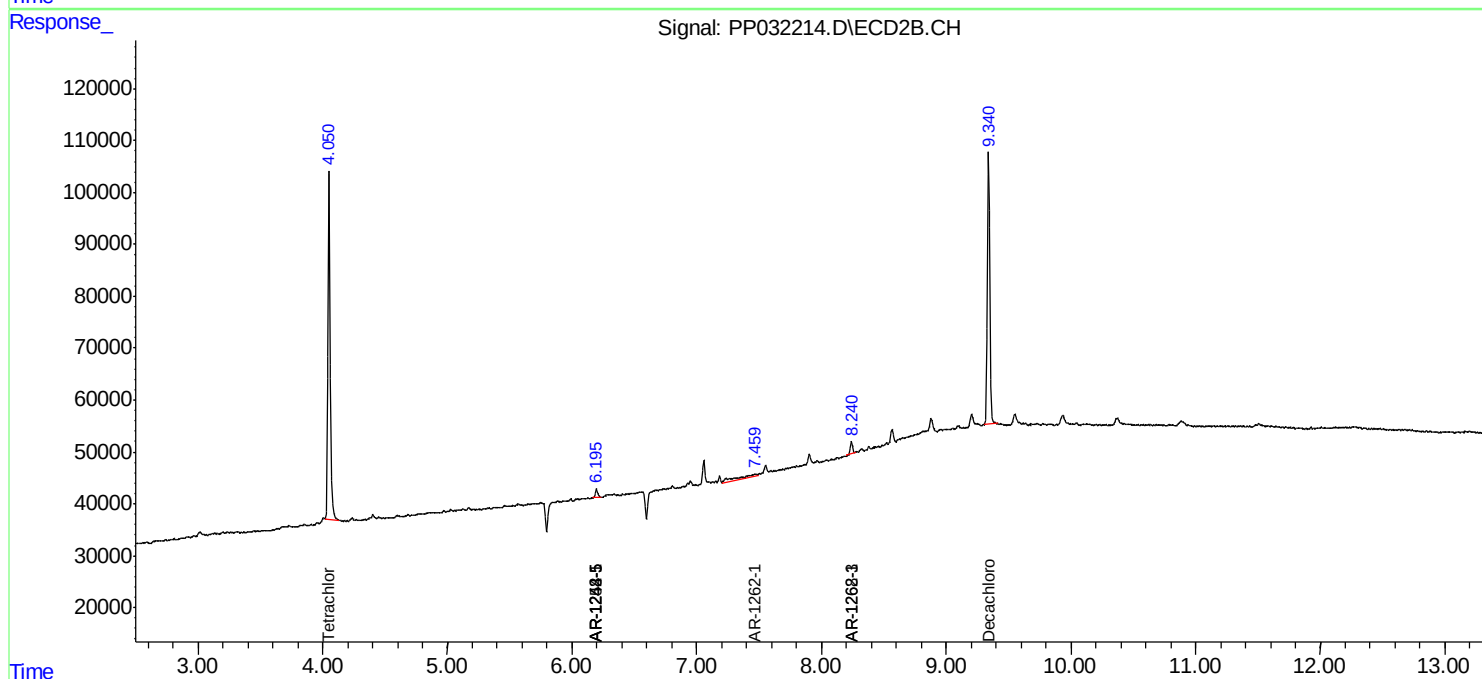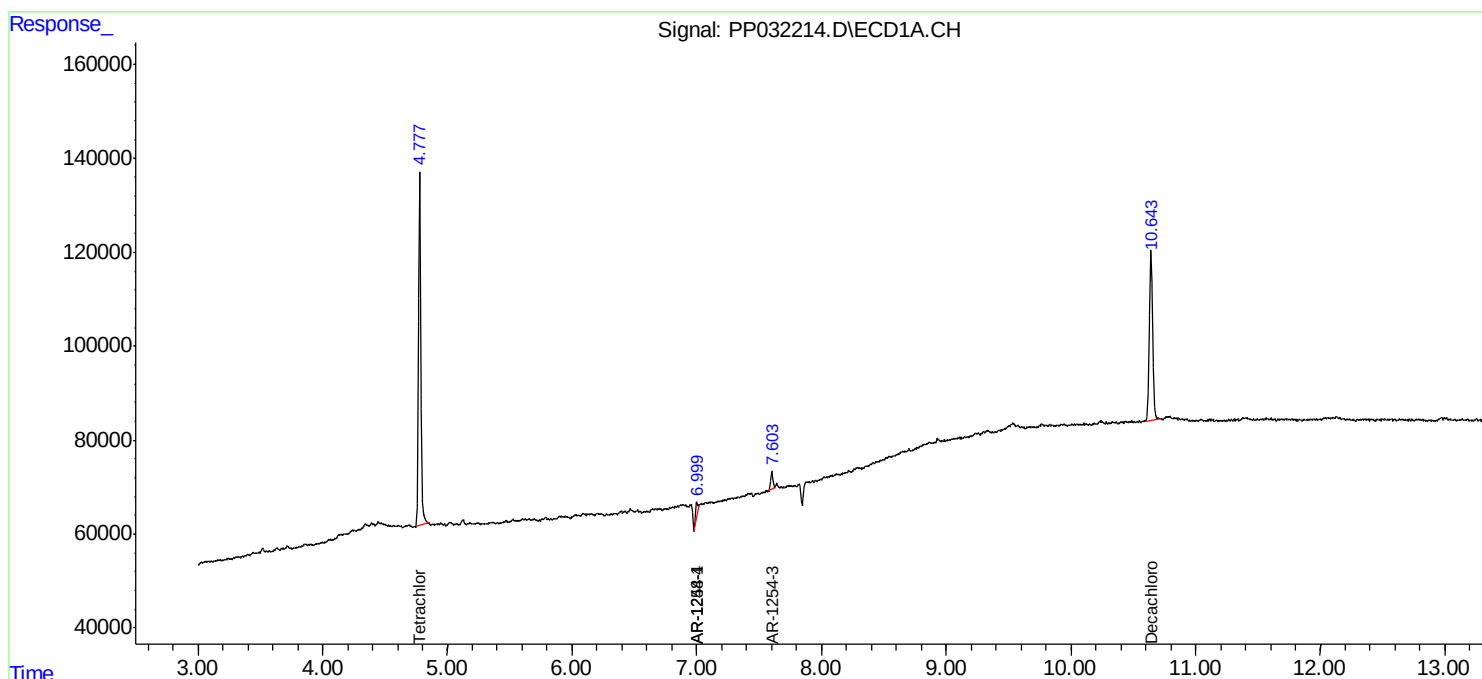


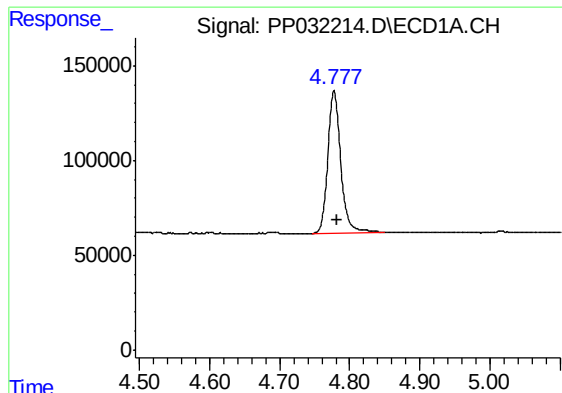

#1 Tetrachloro-m-xylene


R.T.: 4.778 min
Delta R.T.: -0.004 min
Response: 960235
Conc: 18.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

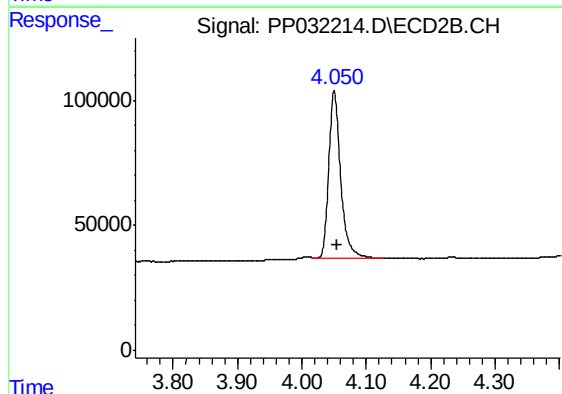


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.004 min
Response: 856081
Conc: 18.10 ng/ml

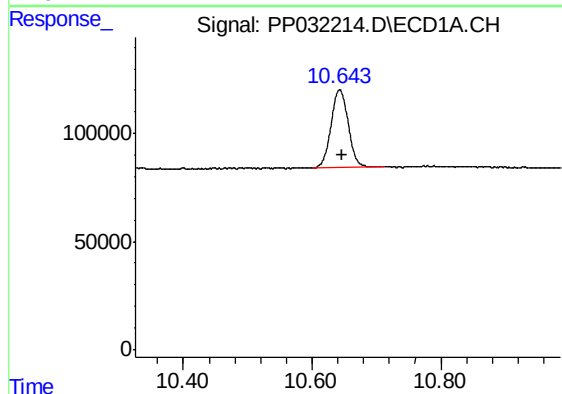


#2 Decachlorobiphenyl

R.T.: 10.643 min
Delta R.T.: -0.004 min
Response: 672242
Conc: 21.44 ng/ml

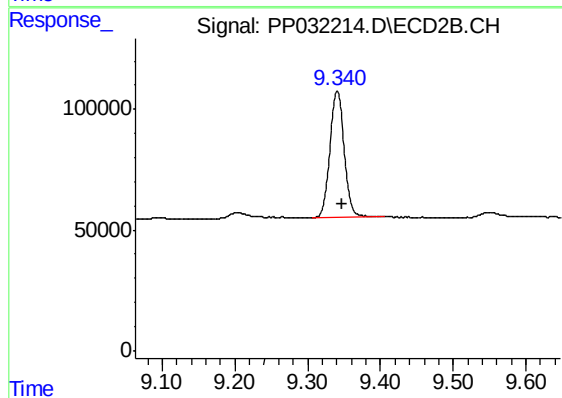

#2 Decachlorobiphenyl


R.T.: 9.341 min
Delta R.T.: -0.007 min
Response: 712877
Conc: 21.26 ng/ml

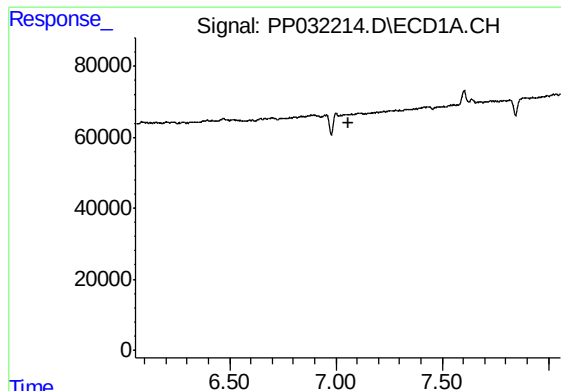

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 7.057 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

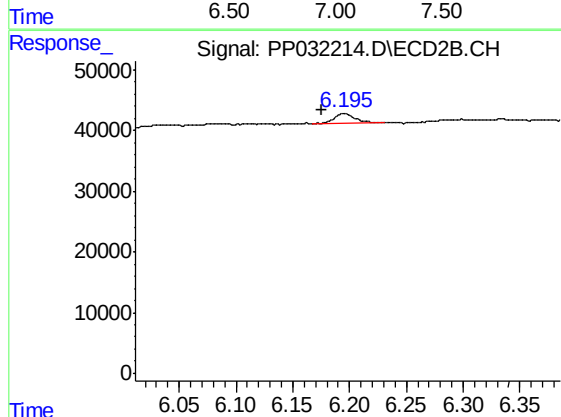


#20 AR-1242-5

R.T.: 6.195 min
Delta R.T.: 0.020 min
Response: 20580
Conc: 23.14 ng/ml

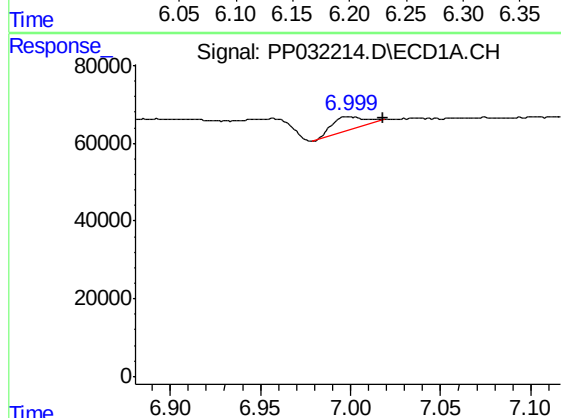


#24 AR-1248-4

R.T.: 6.999 min
Delta R.T.: -0.019 min
Response: 43664
Conc: 30.52 ng/ml

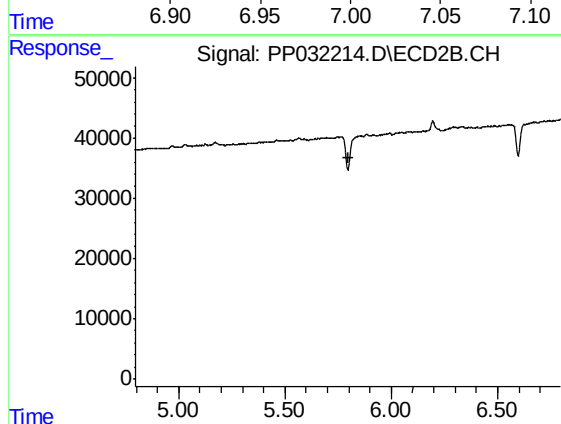

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.796 min
Response: 0
Conc: N.D.

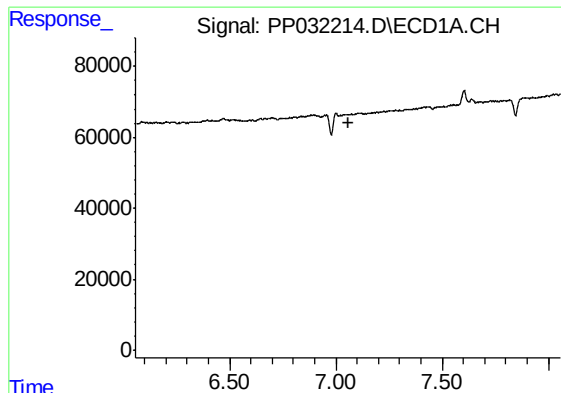

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.057 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

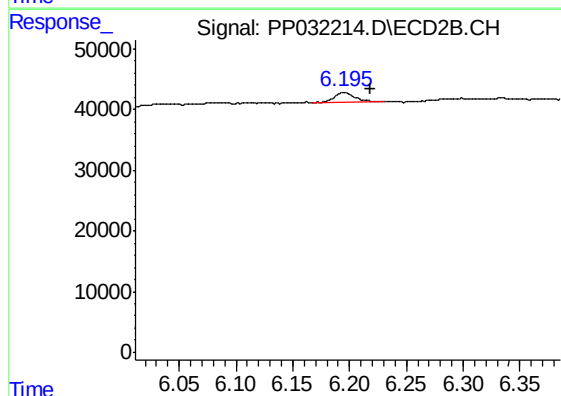


#25 AR-1248-5

R.T.: 6.195 min
Delta R.T.: -0.023 min
Response: 20580
Conc: 16.40 ng/ml

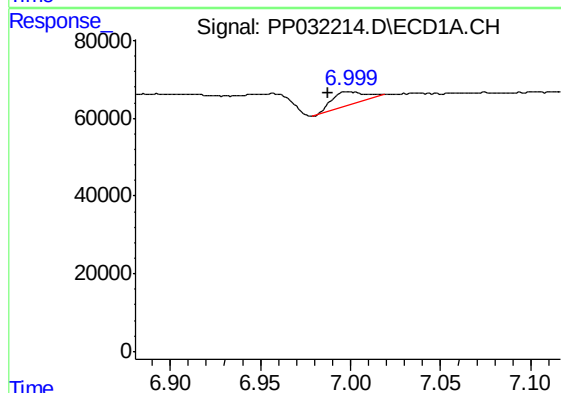


#26 AR-1254-1

R.T.: 6.999 min
Delta R.T.: 0.011 min
Response: 43664
Conc: 28.11 ng/ml

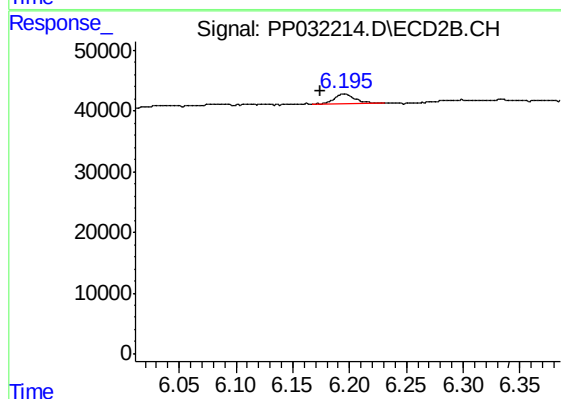

#26 AR-1254-1


R.T.: 6.195 min
Delta R.T.: 0.021 min
Response: 20580
Conc: 9.96 ng/ml

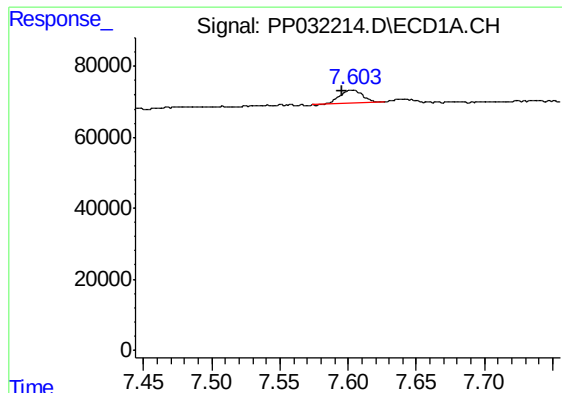

#28 AR-1254-3


R.T.: 7.603 min
Delta R.T.: 0.008 min
Response: 45691
Conc: 18.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

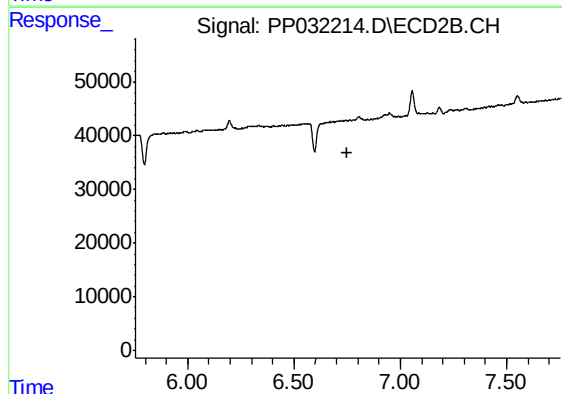


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.753 min
Response: 0
Conc: N.D.

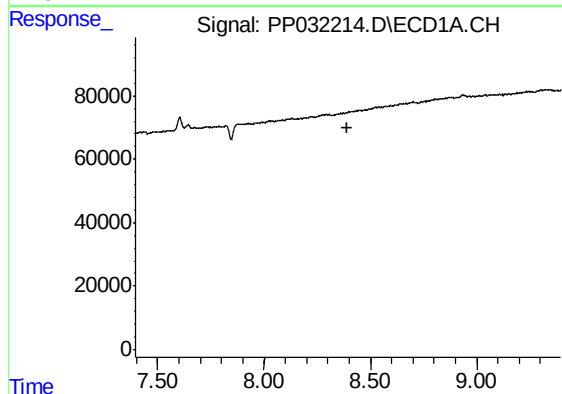


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.394 min
Response: 0
Conc: N.D.

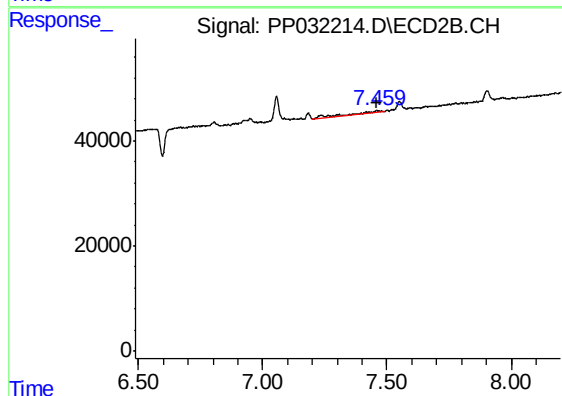

#36 AR-1262-1


R.T.: 7.459 min
Delta R.T.: -0.002 min
Response: 45929
Conc: 17.09 ng/ml

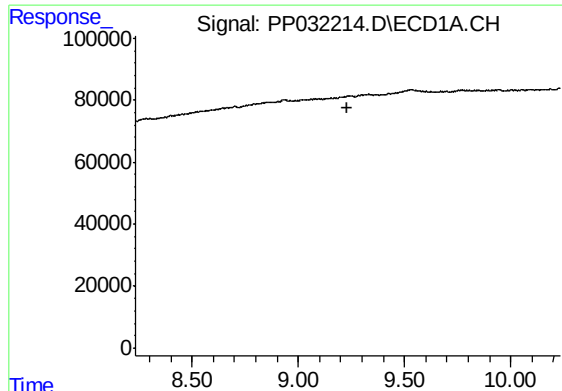

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.233 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

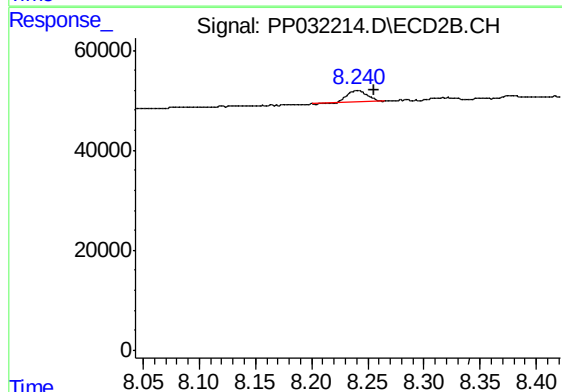


#38 AR-1262-3

R.T.: 8.241 min
Delta R.T.: -0.015 min
Response: 30116
Conc: 16.62 ng/ml

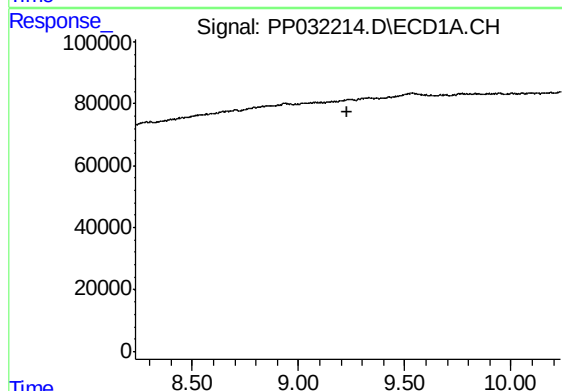

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.233 min
Response: 0
Conc: N.D.

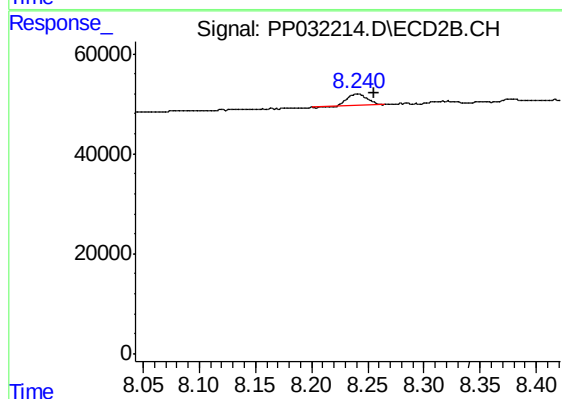

#41 AR-1268-1

R.T.: 8.241 min
Delta R.T.: -0.015 min
Response: 30116
Conc: 5.98 ng/ml