

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121620\
 Data File : PP032199.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Dec 2020 19:12
 Operator : DD\AJ
 Sample : L5036-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 B-2

Manual Integrations
 APPROVED

Ankita
 12/17/2020 12:42:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 17 01:11:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.777	4.048	1229348	1118431	23.865	23.647
2) SA Decachlor...	10.636	9.337	820290	917036	26.158	27.345m
Target Compounds						
31) L7 AR-1260-1	7.758	6.883	79481	167271	45.861m	88.230 #
32) L7 AR-1260-2	8.022	7.080	172429	132427	83.923	60.875 #
33) L7 AR-1260-3	8.389	7.234	89946	75240	51.546	35.412 #
34) L7 AR-1260-4	8.616	7.716	142246	72190	78.937	40.634 #
35) L7 AR-1260-5	8.931	7.963	138586	193927	38.551	50.693 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121620\
Data File : PP032199.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Dec 2020 19:12
Operator : DD\AJ
Sample : L5036-03
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
B-2


Manual Integrations
APPROVED

Ankita
12/17/2020 12:42:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 17 01:11:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

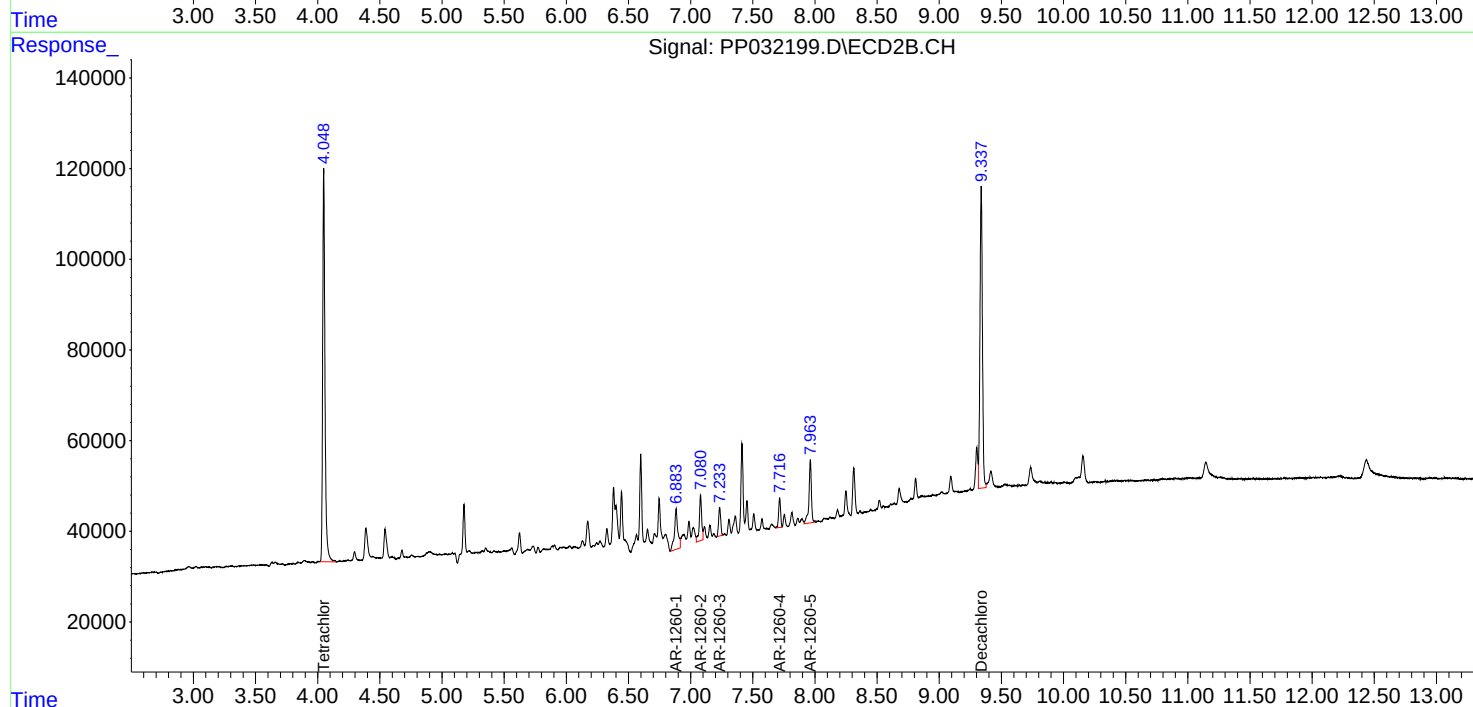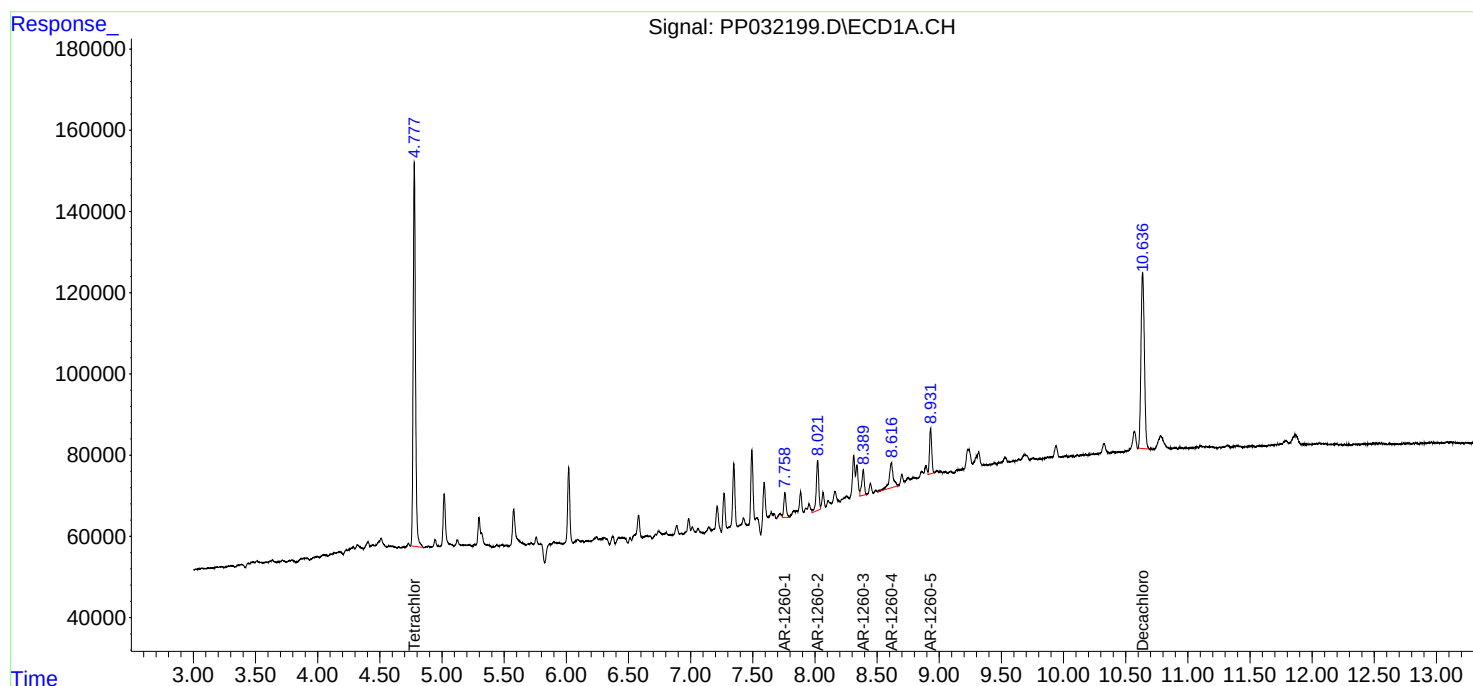

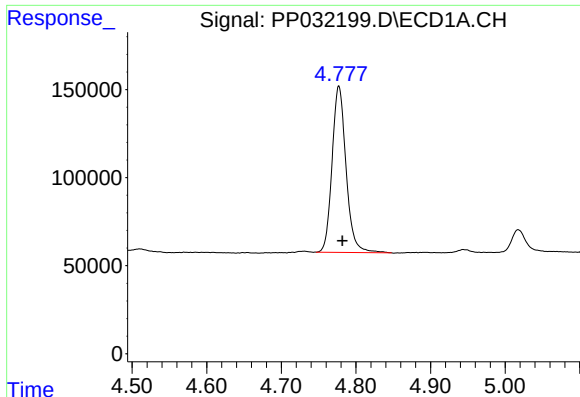


#1 Tetrachloro-m-xylene

R.T.: 4.777 min
Delta R.T.: -0.005 min
Response: 1229348
Conc: 23.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
B-2


Manual Integrations
APPROVED

Ankita
12/17/2020 12:42:15 PM

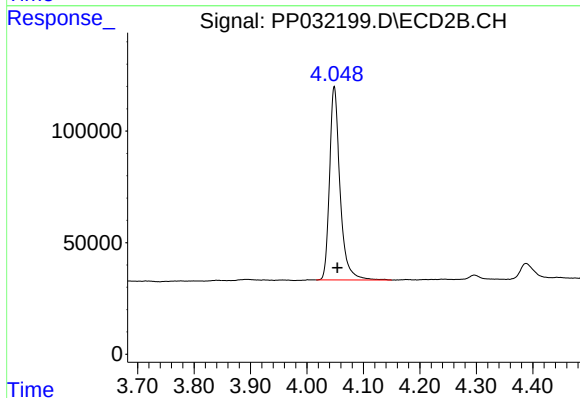


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: -0.006 min
Response: 1118431
Conc: 23.65 ng/ml

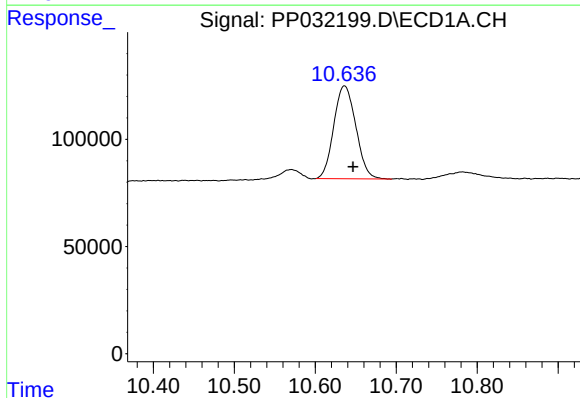


#2 Decachlorobiphenyl

R.T.: 10.636 min
Delta R.T.: -0.011 min
Response: 820290
Conc: 26.16 ng/ml

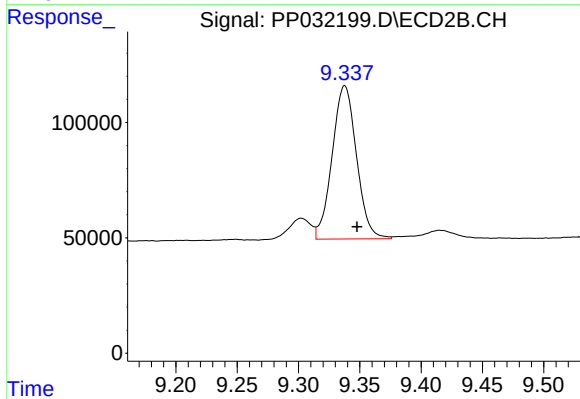

#2 Decachlorobiphenyl

R.T.: 9.337 min
Delta R.T.: -0.011 min
Response: 917036
Conc: 27.34 ng/ml m

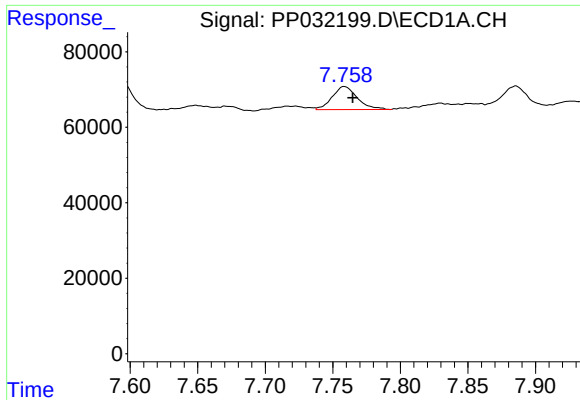


#31 AR-1260-1

R.T.: 7.758 min
Delta R.T.: -0.007 min
Response: 79481
Conc: 45.86 ng/ml m

Instrument :
ECD_P
ClientSampleId :
B-2


Manual Integrations
APPROVED

Ankita
12/17/2020 12:42:15 PM

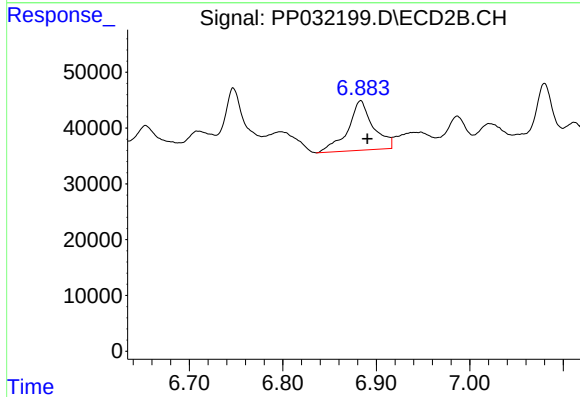


#31 AR-1260-1

R.T.: 6.883 min
Delta R.T.: -0.007 min
Response: 167271
Conc: 88.23 ng/ml

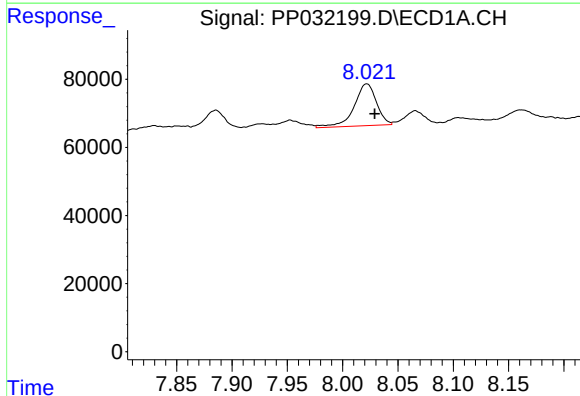


#32 AR-1260-2

R.T.: 8.022 min
Delta R.T.: -0.007 min
Response: 172429
Conc: 83.92 ng/ml

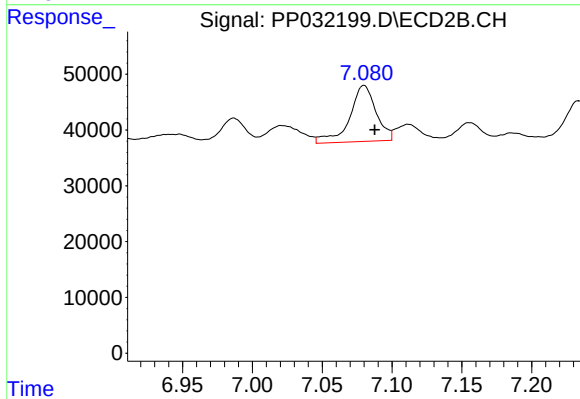

#32 AR-1260-2

R.T.: 7.080 min
Delta R.T.: -0.008 min
Response: 132427
Conc: 60.88 ng/ml

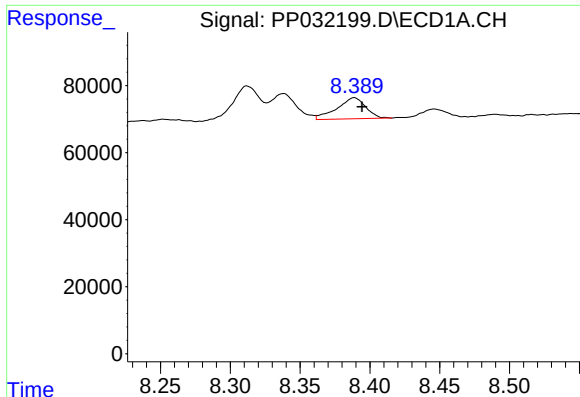


#33 AR-1260-3

R.T.: 8.389 min
Delta R.T.: -0.006 min
Response: 89946
Conc: 51.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
B-2


Manual Integrations
APPROVED

Ankita
12/17/2020 12:42:15 PM

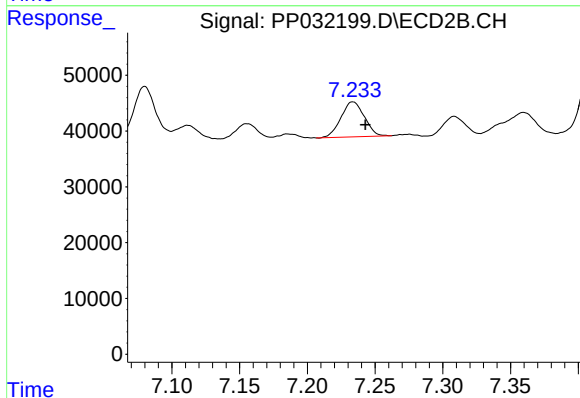


#33 AR-1260-3

R.T.: 7.234 min
Delta R.T.: -0.009 min
Response: 75240
Conc: 35.41 ng/ml

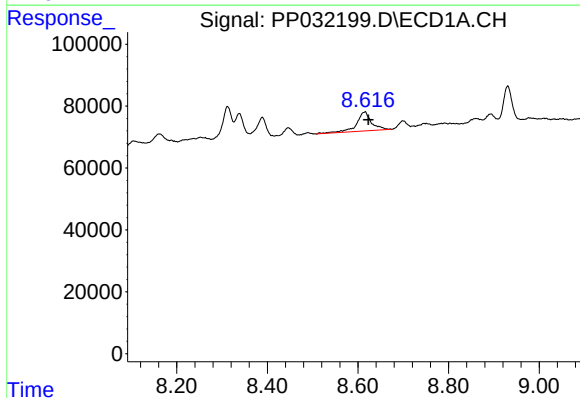


#34 AR-1260-4

R.T.: 8.616 min
Delta R.T.: -0.007 min
Response: 142246
Conc: 78.94 ng/ml

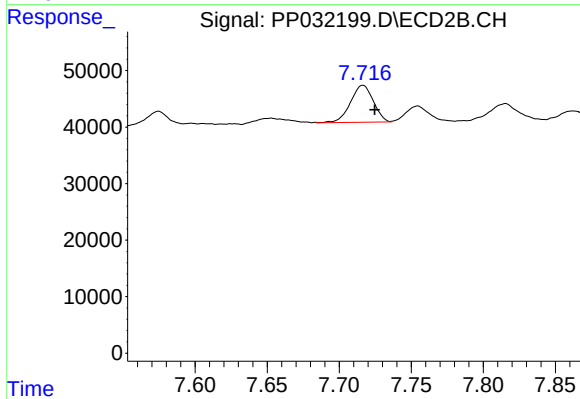

#34 AR-1260-4

R.T.: 7.716 min
Delta R.T.: -0.008 min
Response: 72190
Conc: 40.63 ng/ml

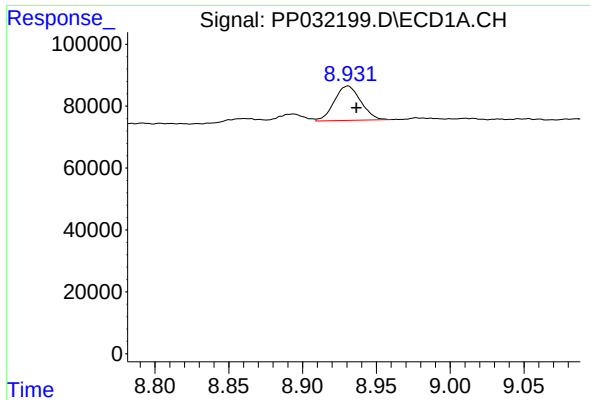


#35 AR-1260-5

R.T.: 8.931 min
Delta R.T.: -0.006 min
Response: 138586
Conc: 38.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
B-2

Manual Integrations
APPROVED

Ankita
12/17/2020 12:42:15 PM

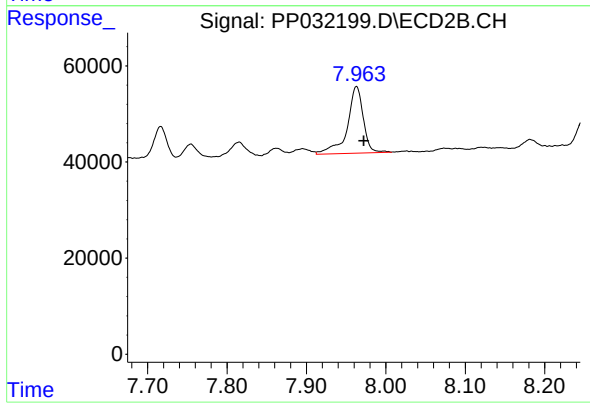

#35 AR-1260-5

R.T.: 7.963 min
Delta R.T.: -0.009 min
Response: 193927
Conc: 50.69 ng/ml