

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121621\
 Data File : PP042019.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Dec 2021 8:47
 Operator : AJ\MA
 Sample : M5074-06
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CS-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 12:47:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 06:21:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.927	4.068	327942	566808	25.417	23.105
2)	SA Decachlor...	10.917	9.427	363792	533611	27.606	26.540

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121621\
Data File : PP042019.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Dec 2021 8:47
Operator : AJ\MA
Sample : M5074-06
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CS-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 12:47:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 06:21:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

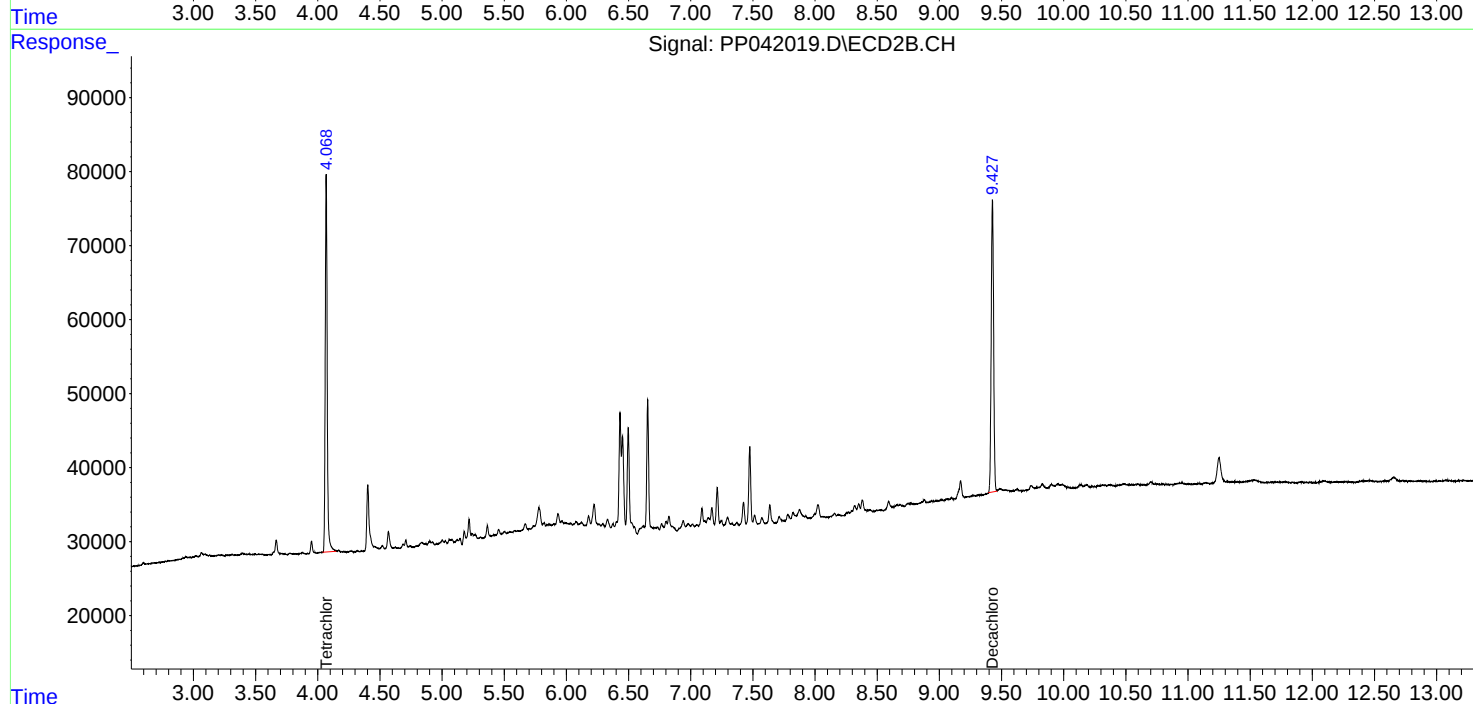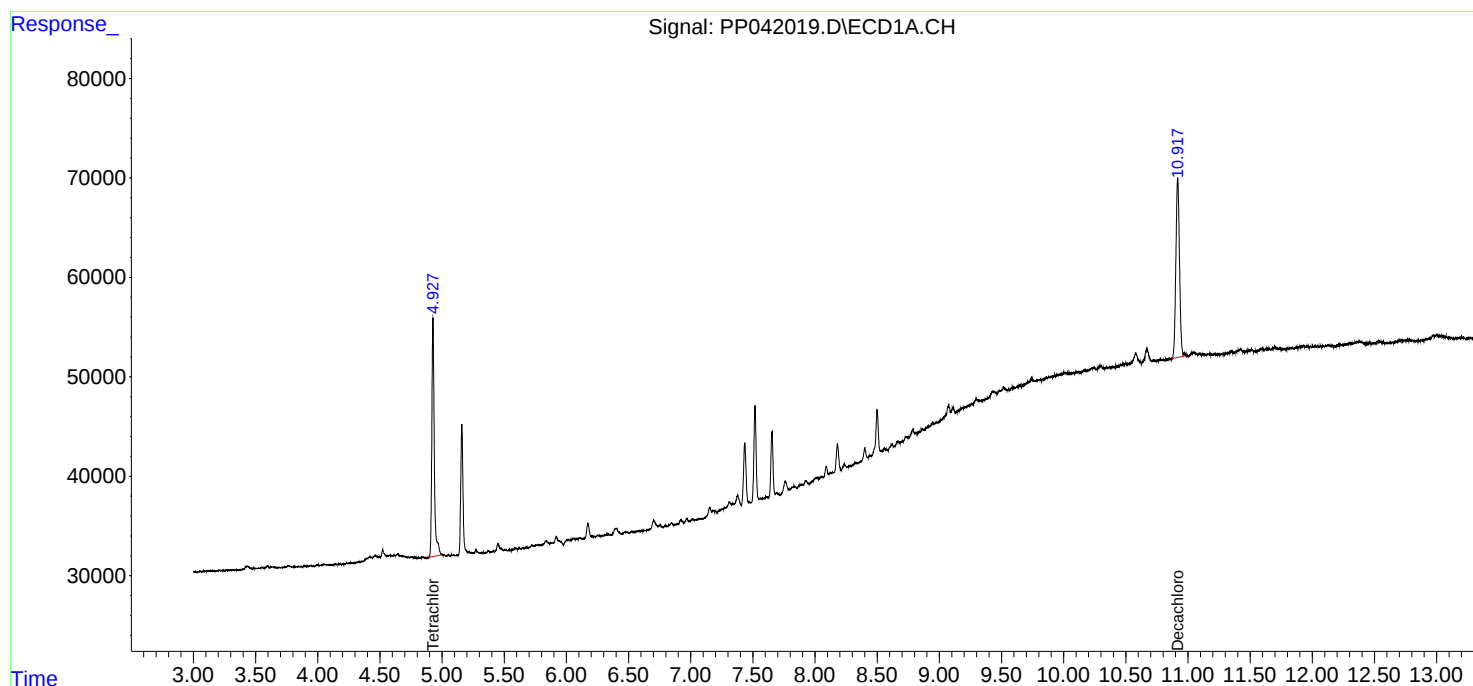


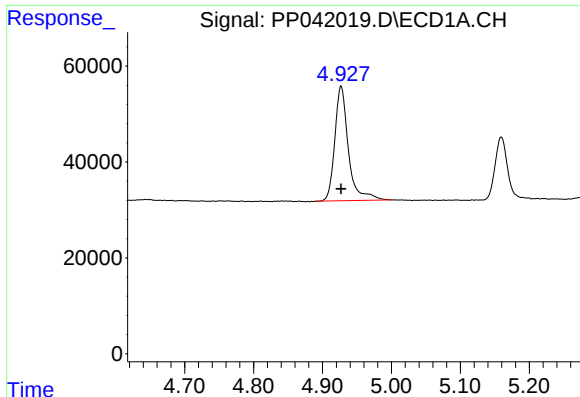

#1 Tetrachloro-m-xylene


R.T.: 4.927 min
Delta R.T.: 0.000 min
Response: 327942
Conc: 25.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
CS-3

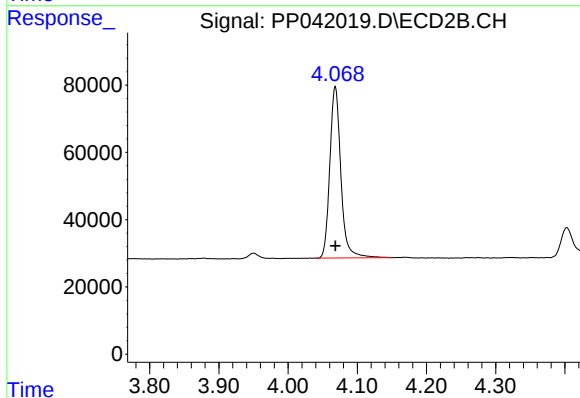


#1 Tetrachloro-m-xylene

R.T.: 4.068 min
Delta R.T.: 0.000 min
Response: 566808
Conc: 23.10 ng/ml

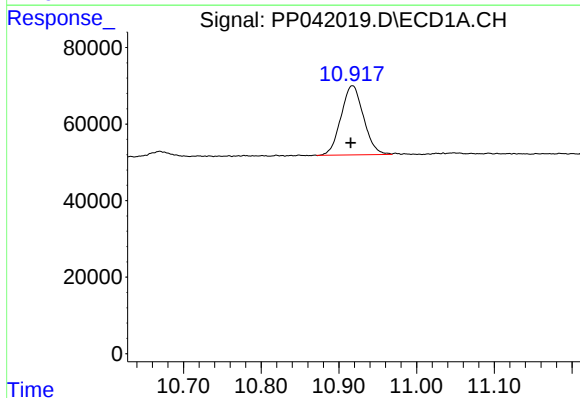

#2 Decachlorobiphenyl

R.T.: 10.917 min
Delta R.T.: 0.002 min
Response: 363792
Conc: 27.61 ng/ml

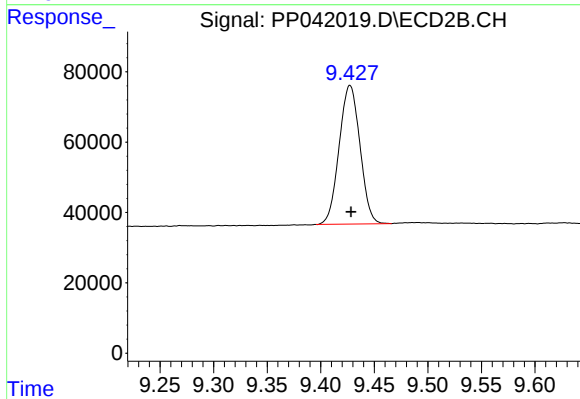

#2 Decachlorobiphenyl

R.T.: 9.427 min
Delta R.T.: -0.001 min
Response: 533611
Conc: 26.54 ng/ml