

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121621\
 Data File : PP042023.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Dec 2021 9:54
 Operator : AJ\MA
 Sample : M5078-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VNJ-229

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 12/17/2021
 Supervised By :mohammad ahmed 12/17/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 16 12:49:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 16 06:21:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.927	4.068	288408	501079	22.353	20.425
2) SA Decachlor...	10.918	9.428	203312	291683	15.428	14.507m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121621\
Data File : PP042023.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Dec 2021 9:54
Operator : AJ\MA
Sample : M5078-01
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
VNJ-229


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/17/2021
Supervised By :mohammad ahmed 12/17/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 16 12:49:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121621.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 16 06:21:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

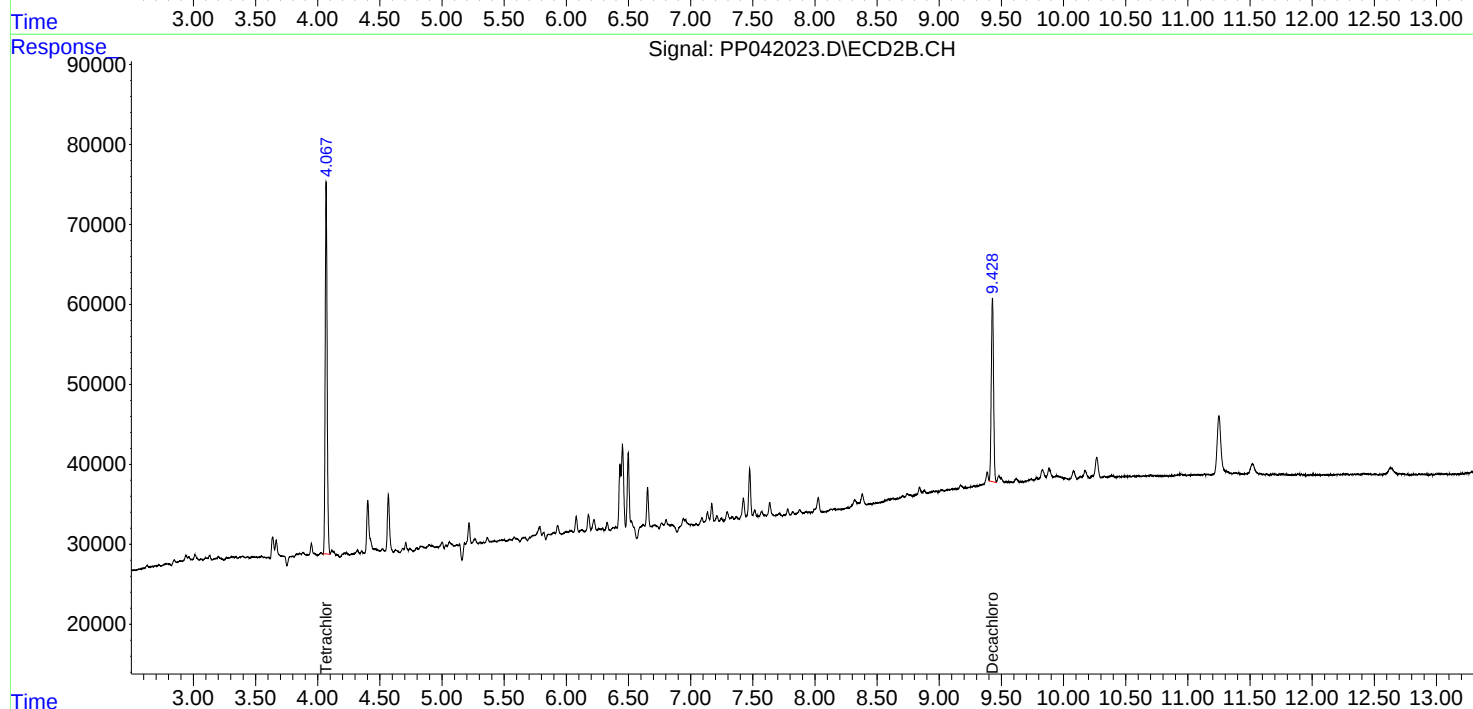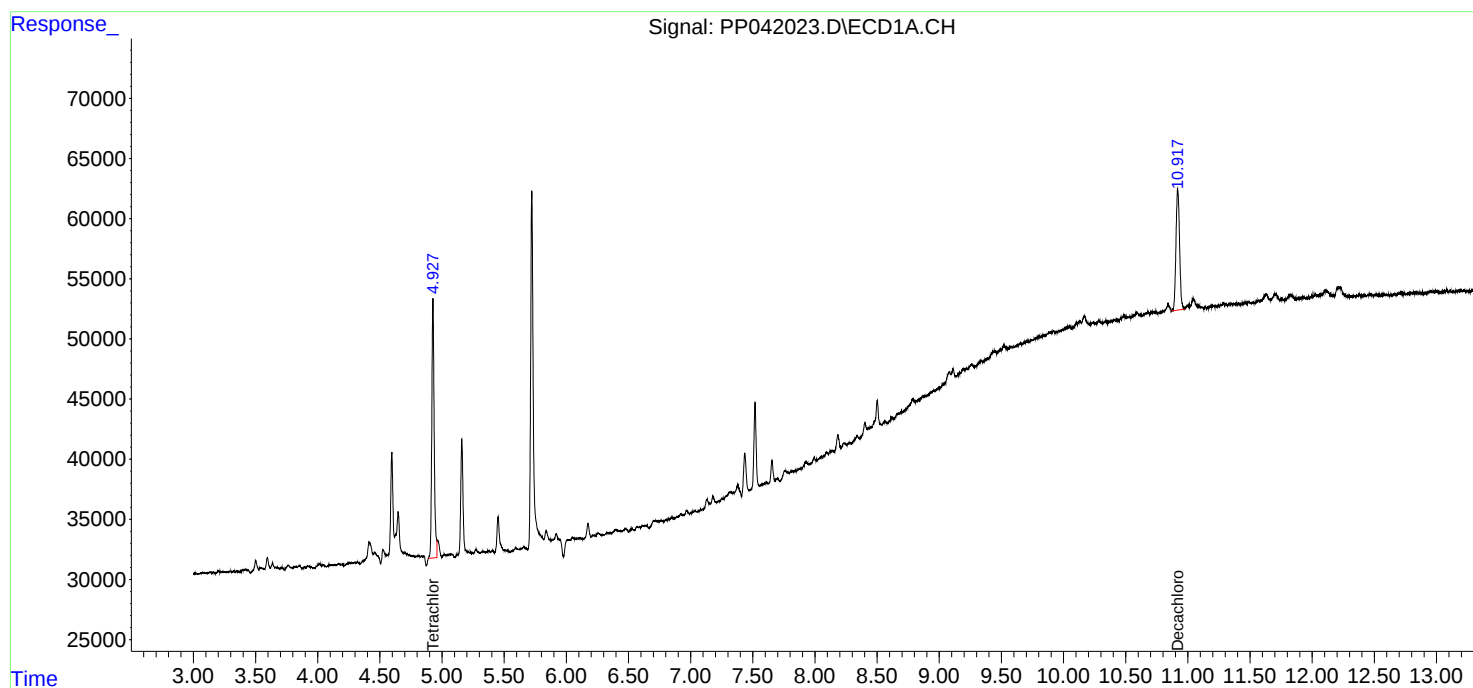

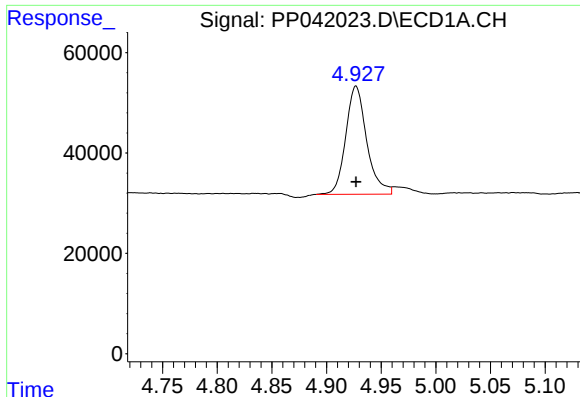


#1 Tetrachloro-m-xylene

R.T.: 4.927 min
Delta R.T.: 0.000 min
Response: 288408
Conc: 22.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
VNJ-229


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 12/17/2021
Supervised By :mohammad ahmed 12/17/2021

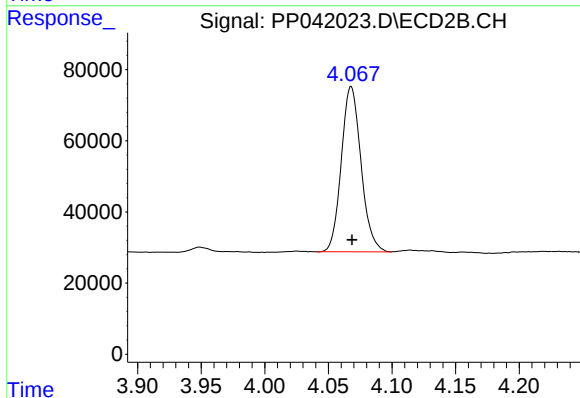


#1 Tetrachloro-m-xylene

R.T.: 4.068 min
Delta R.T.: 0.000 min
Response: 501079
Conc: 20.43 ng/ml

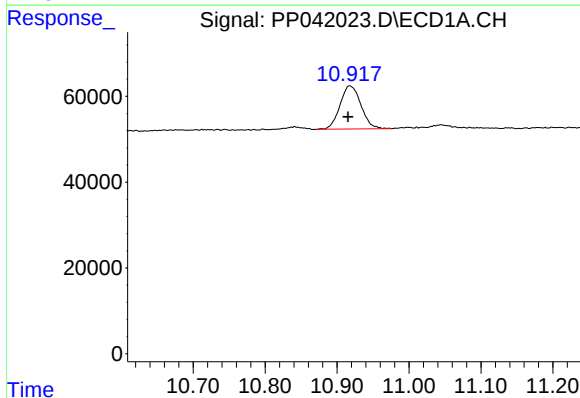

#2 Decachlorobiphenyl

R.T.: 10.918 min
Delta R.T.: 0.002 min
Response: 203312
Conc: 15.43 ng/ml

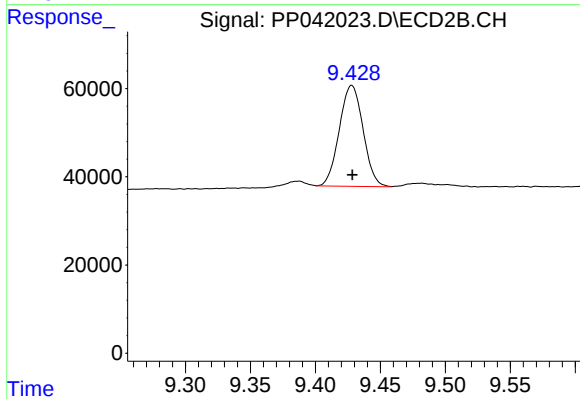

#2 Decachlorobiphenyl

R.T.: 9.428 min
Delta R.T.: 0.000 min
Response: 291683
Conc: 14.51 ng/ml m