

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121720\
 Data File : PP032225.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Dec 2020 13:43
 Operator : DD\AJ
 Sample : 500 PPB SPIKE TEST
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 500 PPB SPIKE TEST

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 18 03:54:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 12 05:15:55 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
3)	L1	AR-1016-1	6.093	5.301	740261	637789	507.528 487.925
4)	L1	AR-1016-2	6.116	5.321	1128494	954183	502.397 481.938
5)	L1	AR-1016-3	6.181	5.513	708679	525538	512.732 491.453
6)	L1	AR-1016-4	6.287	5.564	585225	404767	507.493 477.030
7)	L1	AR-1016-5	6.600	5.793	544540	532678	510.353 490.217
31)	L7	AR-1260-1	7.772	6.886	948678	1009589	547.390 532.525
32)	L7	AR-1260-2	8.037	7.083	1175801	1170811	572.279 538.211
33)	L7	AR-1260-3	8.402	7.237	843001	1162122	483.106 546.965
34)	L7	AR-1260-4	8.630	7.719	890446	857044	494.142 482.406
35)	L7	AR-1260-5	8.944	7.967	1843661	1967856	512.853 514.407



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP121720\
Data File : PP032225.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Dec 2020 13:43
Operator : DD\AJ
Sample : 500 PPB SPIKE TEST
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
500 PPB SPIKE TEST

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 18 03:54:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP121120.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 12 05:15:55 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

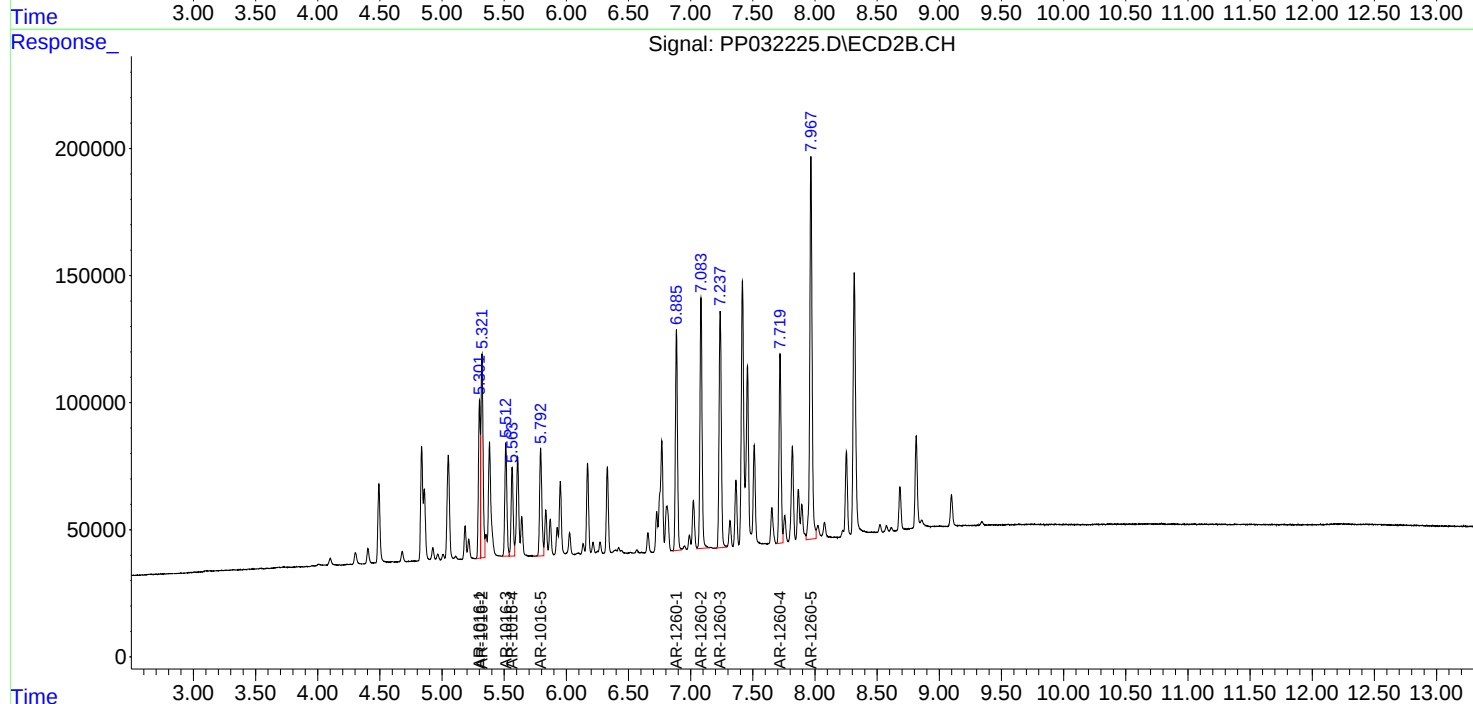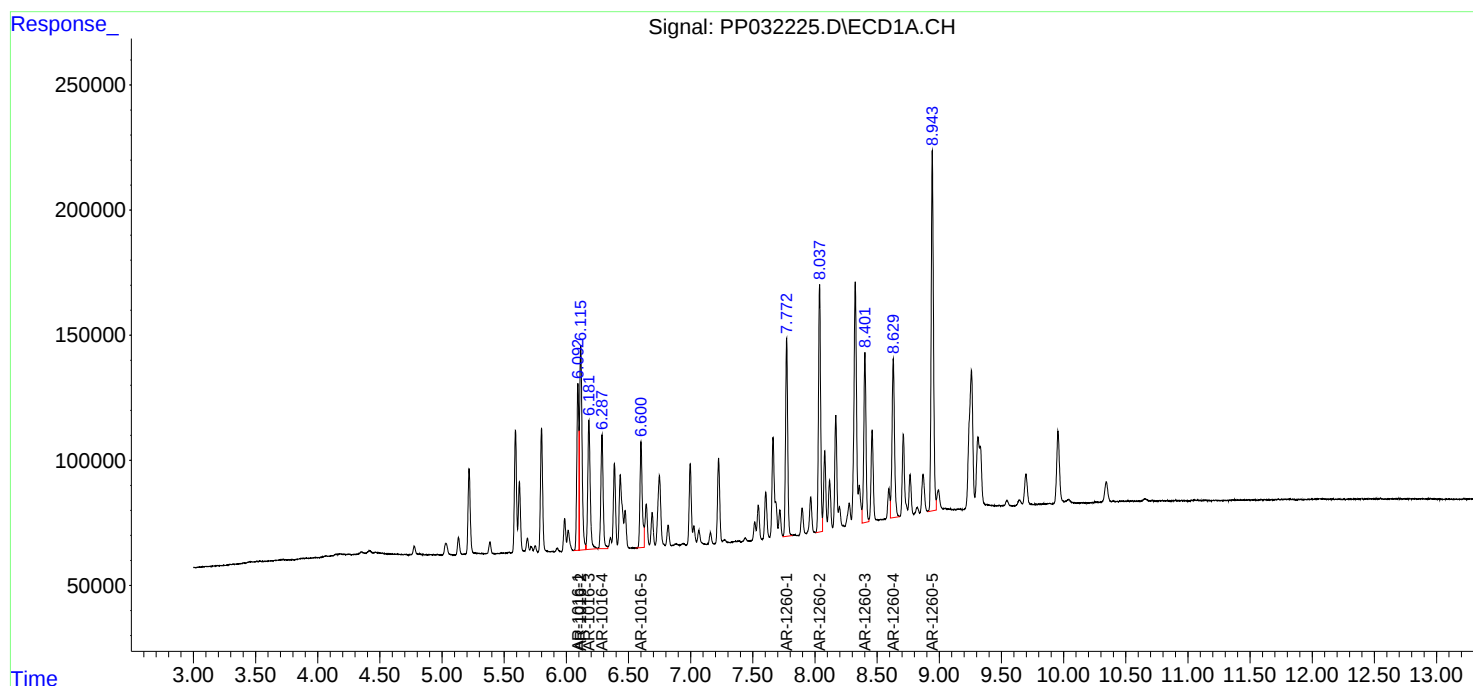


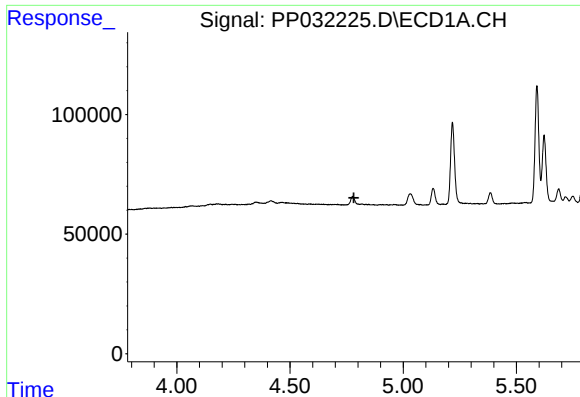

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.782 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
500 PPB SPIKE TEST

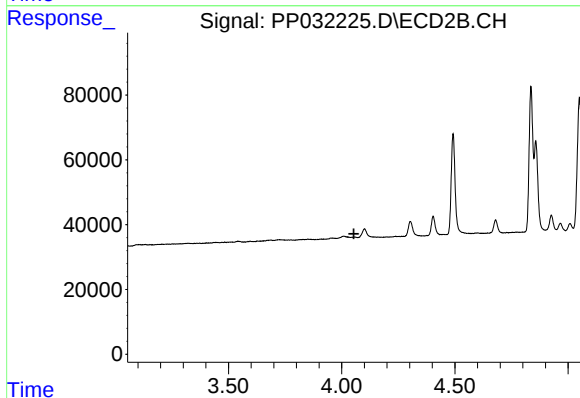


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.054 min
Response: 0
Conc: N.D.

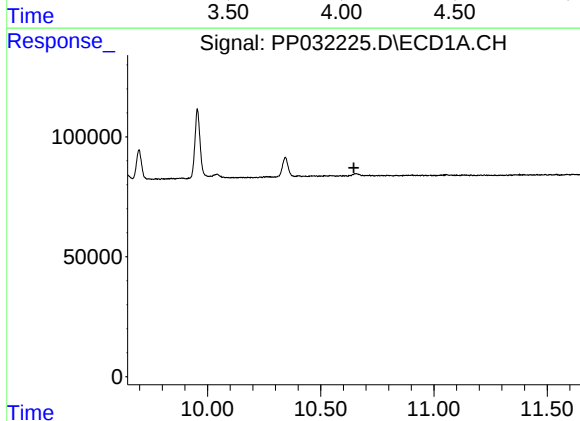


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.647 min
Response: 0
Conc: N.D.

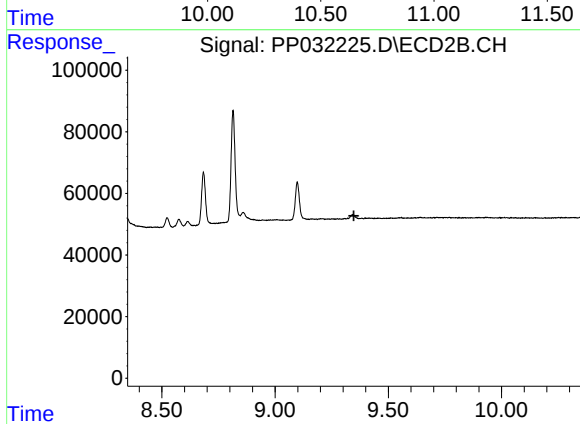

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.348 min
Response: 0
Conc: N.D.

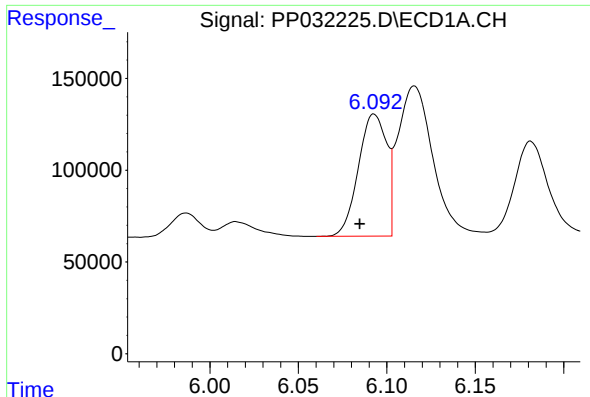

#3 AR-1016-1


R.T.: 6.093 min
Delta R.T.: 0.008 min
Response: 740261
Conc: 507.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
500 PPB SPIKE TEST

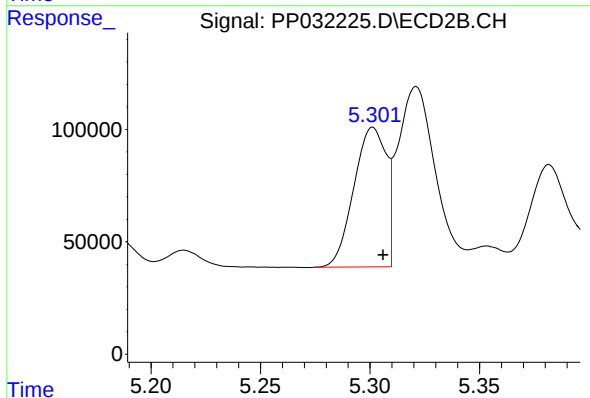


#3 AR-1016-1

R.T.: 5.301 min
Delta R.T.: -0.005 min
Response: 637789
Conc: 487.92 ng/ml

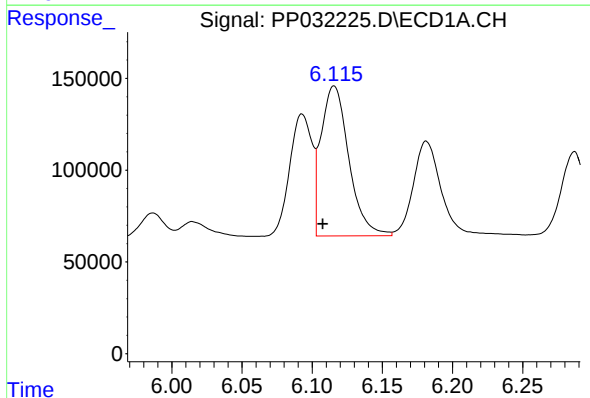


#4 AR-1016-2

R.T.: 6.116 min
Delta R.T.: 0.008 min
Response: 1128494
Conc: 502.40 ng/ml

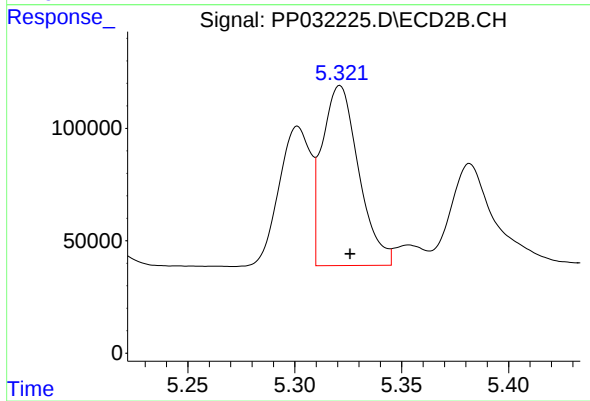

#4 AR-1016-2


R.T.: 5.321 min
Delta R.T.: -0.005 min
Response: 954183
Conc: 481.94 ng/ml

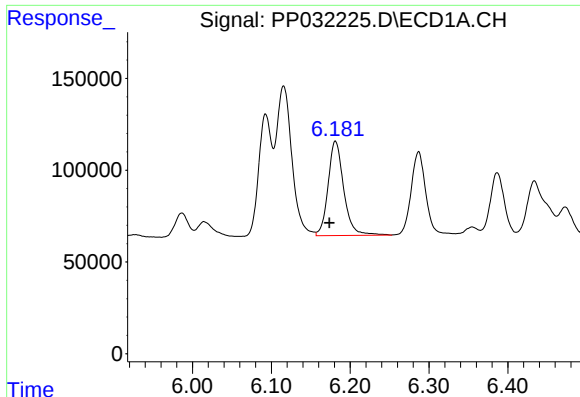

#5 AR-1016-3


R.T.: 6.181 min
Delta R.T.: 0.008 min
Response: 708679
Conc: 512.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
500 PPB SPIKE TEST

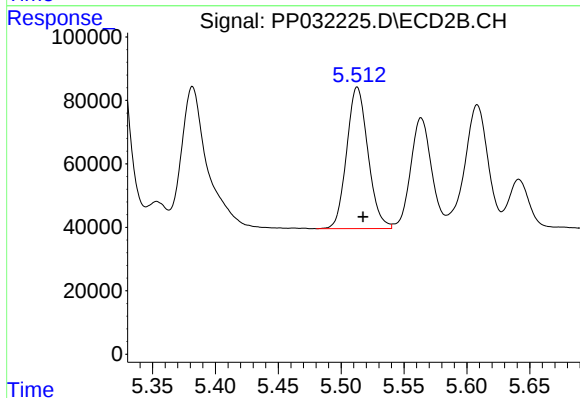


#5 AR-1016-3

R.T.: 5.513 min
Delta R.T.: -0.005 min
Response: 525538
Conc: 491.45 ng/ml

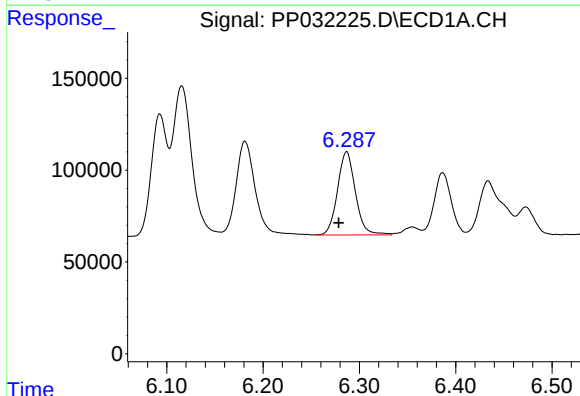


#6 AR-1016-4

R.T.: 6.287 min
Delta R.T.: 0.008 min
Response: 585225
Conc: 507.49 ng/ml

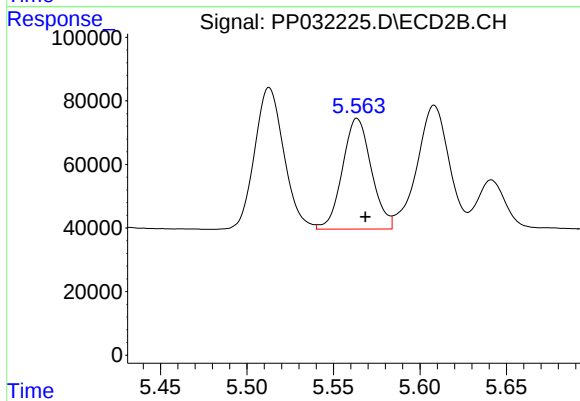

#6 AR-1016-4


R.T.: 5.564 min
Delta R.T.: -0.005 min
Response: 404767
Conc: 477.03 ng/ml

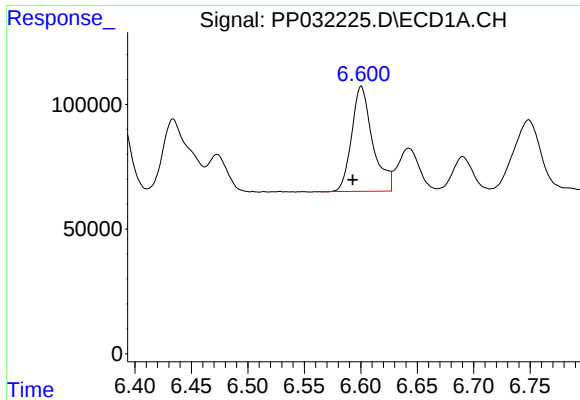

#7 AR-1016-5


R.T.: 6.600 min
Delta R.T.: 0.007 min
Response: 544540
Conc: 510.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
500 PPB SPIKE TEST

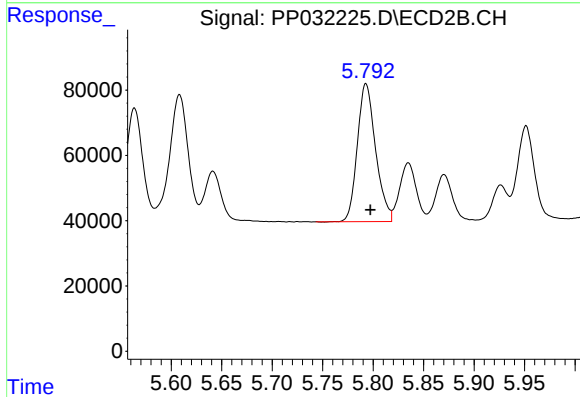


#7 AR-1016-5

R.T.: 5.793 min
Delta R.T.: -0.005 min
Response: 532678
Conc: 490.22 ng/ml

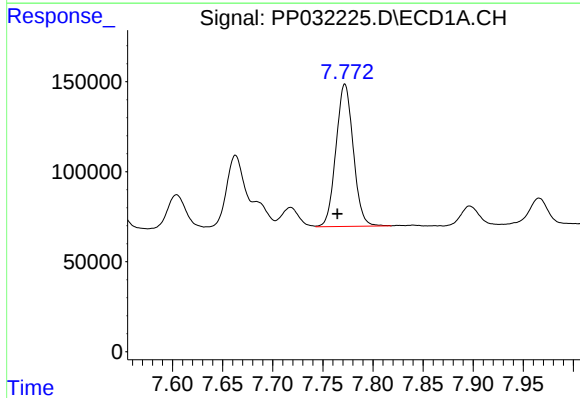


#31 AR-1260-1

R.T.: 7.772 min
Delta R.T.: 0.007 min
Response: 948678
Conc: 547.39 ng/ml

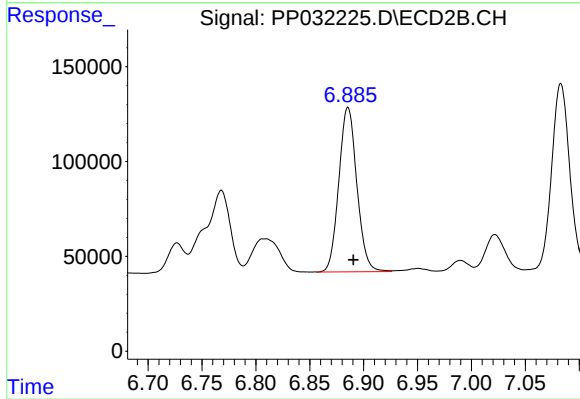

#31 AR-1260-1


R.T.: 6.886 min
Delta R.T.: -0.005 min
Response: 1009589
Conc: 532.53 ng/ml

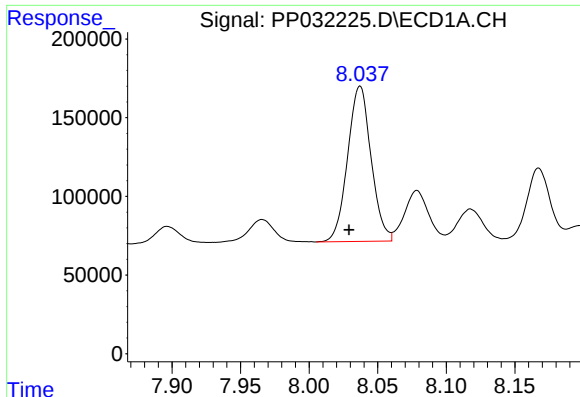

#32 AR-1260-2


R.T.: 8.037 min
Delta R.T.: 0.008 min
Response: 1175801
Conc: 572.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
500 PPB SPIKE TEST

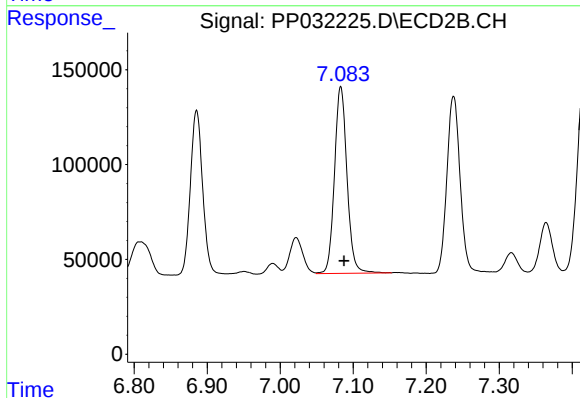


#32 AR-1260-2

R.T.: 7.083 min
Delta R.T.: -0.005 min
Response: 1170811
Conc: 538.21 ng/ml

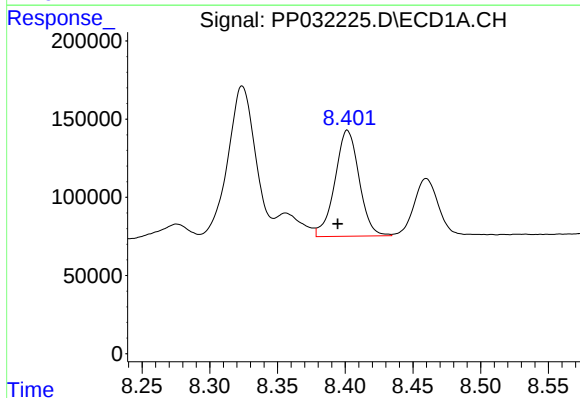


#33 AR-1260-3

R.T.: 8.402 min
Delta R.T.: 0.007 min
Response: 843001
Conc: 483.11 ng/ml

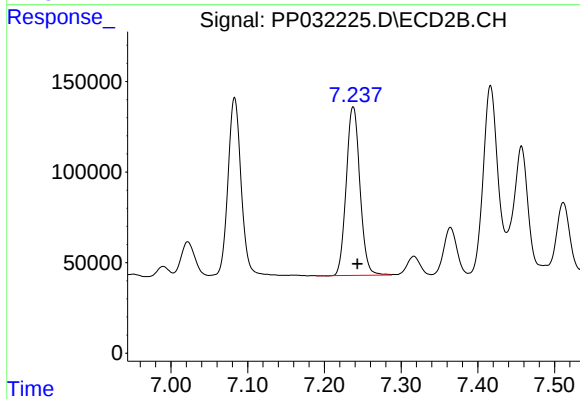

#33 AR-1260-3


R.T.: 7.237 min
Delta R.T.: -0.006 min
Response: 1162122
Conc: 546.97 ng/ml

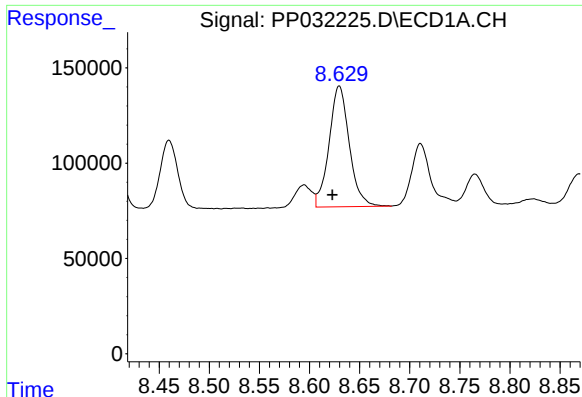

#34 AR-1260-4


R.T.: 8.630 min
Delta R.T.: 0.007 min
Response: 890446
Conc: 494.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
500 PPB SPIKE TEST

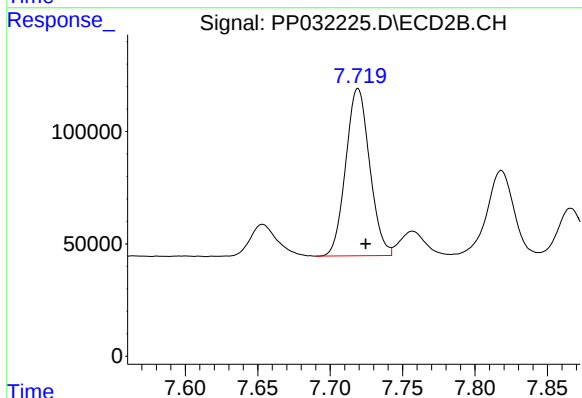


#34 AR-1260-4

R.T.: 7.719 min
Delta R.T.: -0.005 min
Response: 857044
Conc: 482.41 ng/ml

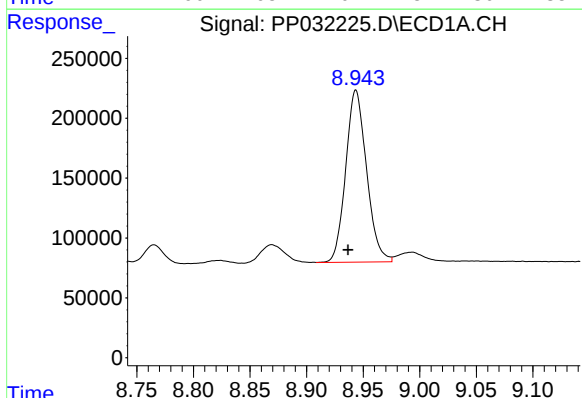

#35 AR-1260-5

R.T.: 8.944 min
Delta R.T.: 0.007 min
Response: 1843661
Conc: 512.85 ng/ml

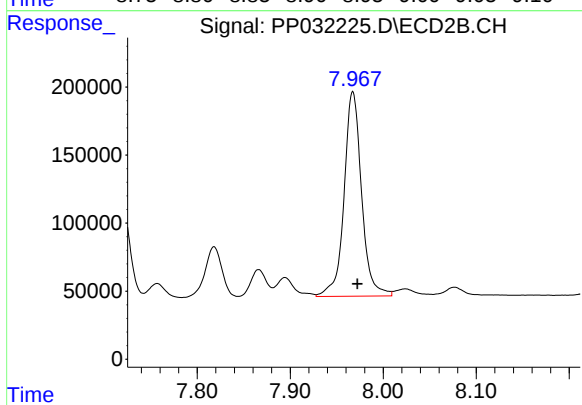

#35 AR-1260-5

R.T.: 7.967 min
Delta R.T.: -0.005 min
Response: 1967856
Conc: 514.41 ng/ml